


Data Path : Z:\HPCHEM1\BNA_G\Data\BG080915\
Data File : BG018340.D
Acq On : 9 Aug 2015 22:18
Operator : UM/TP
Sample : G3136-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 10 08:06:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 07:50:23 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
C01T5

Manual Integrations
APPROVED
MMDadoda
8/10/2015 7:26:05 PM

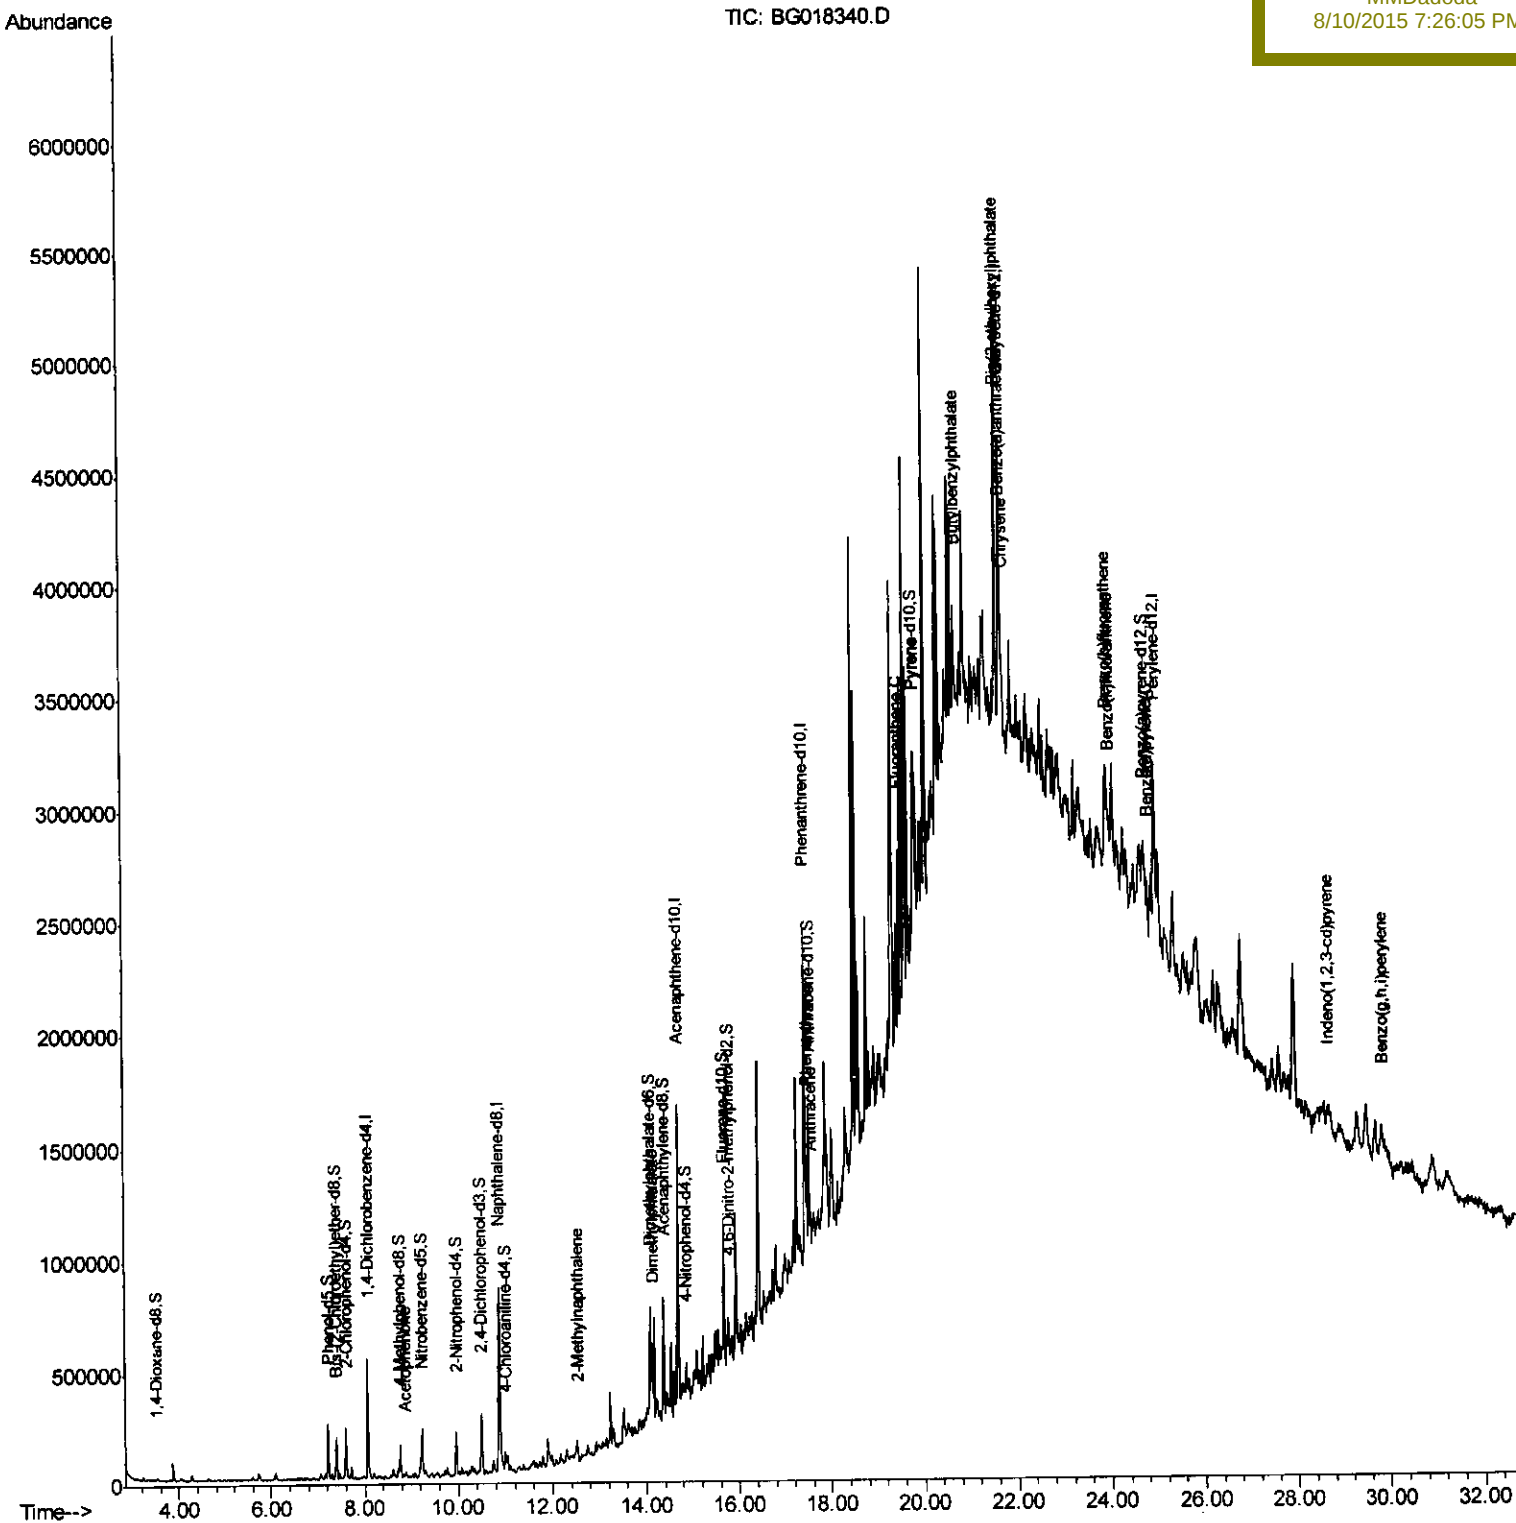

Instrument :
BNA_G
ClientSampleId :
C01T5

MMDadoda
8/10/2015 7:26:05 PM

Ion 178.00 (177.70 to 178.70): BG018340.D

8/10/2015 7:26:05 PM

abundance

250000

200000

150000

100000

50000

0

m/z-->

16.50 16.60 16.70 16.80 16.90 17.00 17.10 17.20 17.30 17.40 17.50 17.60 17.70 17.80 17.90 18.00 18.10 18.20 18.30 18.40

1

17.47

9d



4d

2d

3d

6d

7d

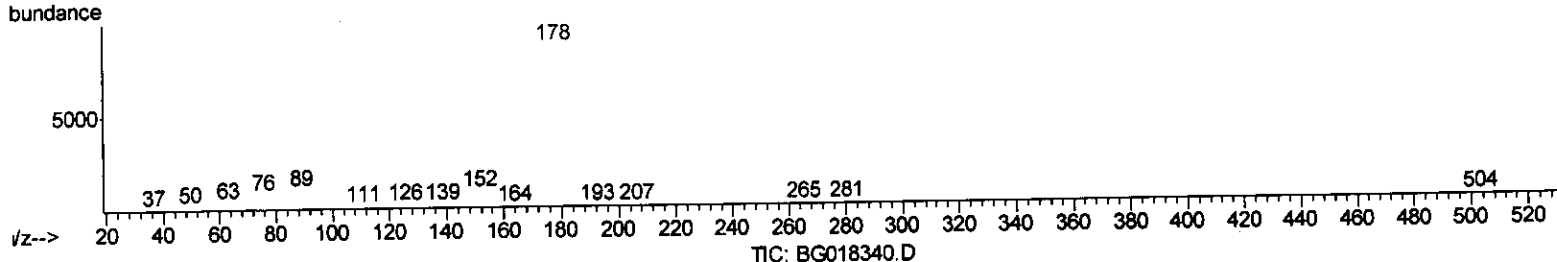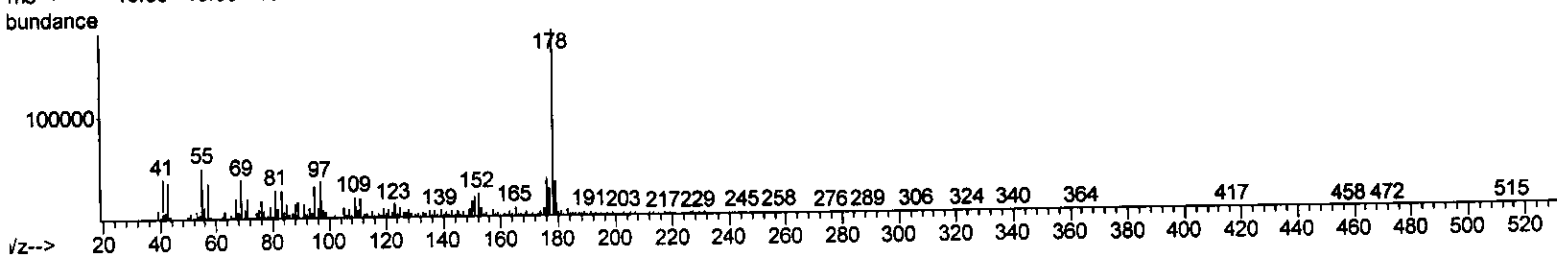

Ion	Exp%	Act%
178.00	100	100
179.00	16.20	18.34
176.00	20.00	20.63
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_G\Data\BG080915\
Data File : BG018340.D
Acq On : 9 Aug 2015 22:18
Operator : UM/TP
Sample : G3136-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 10 07:51:55 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 07:50:23 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
C01T5

Manual Integrations
APPROVED

MMDadoda
8/10/2015 7:26:05 PM

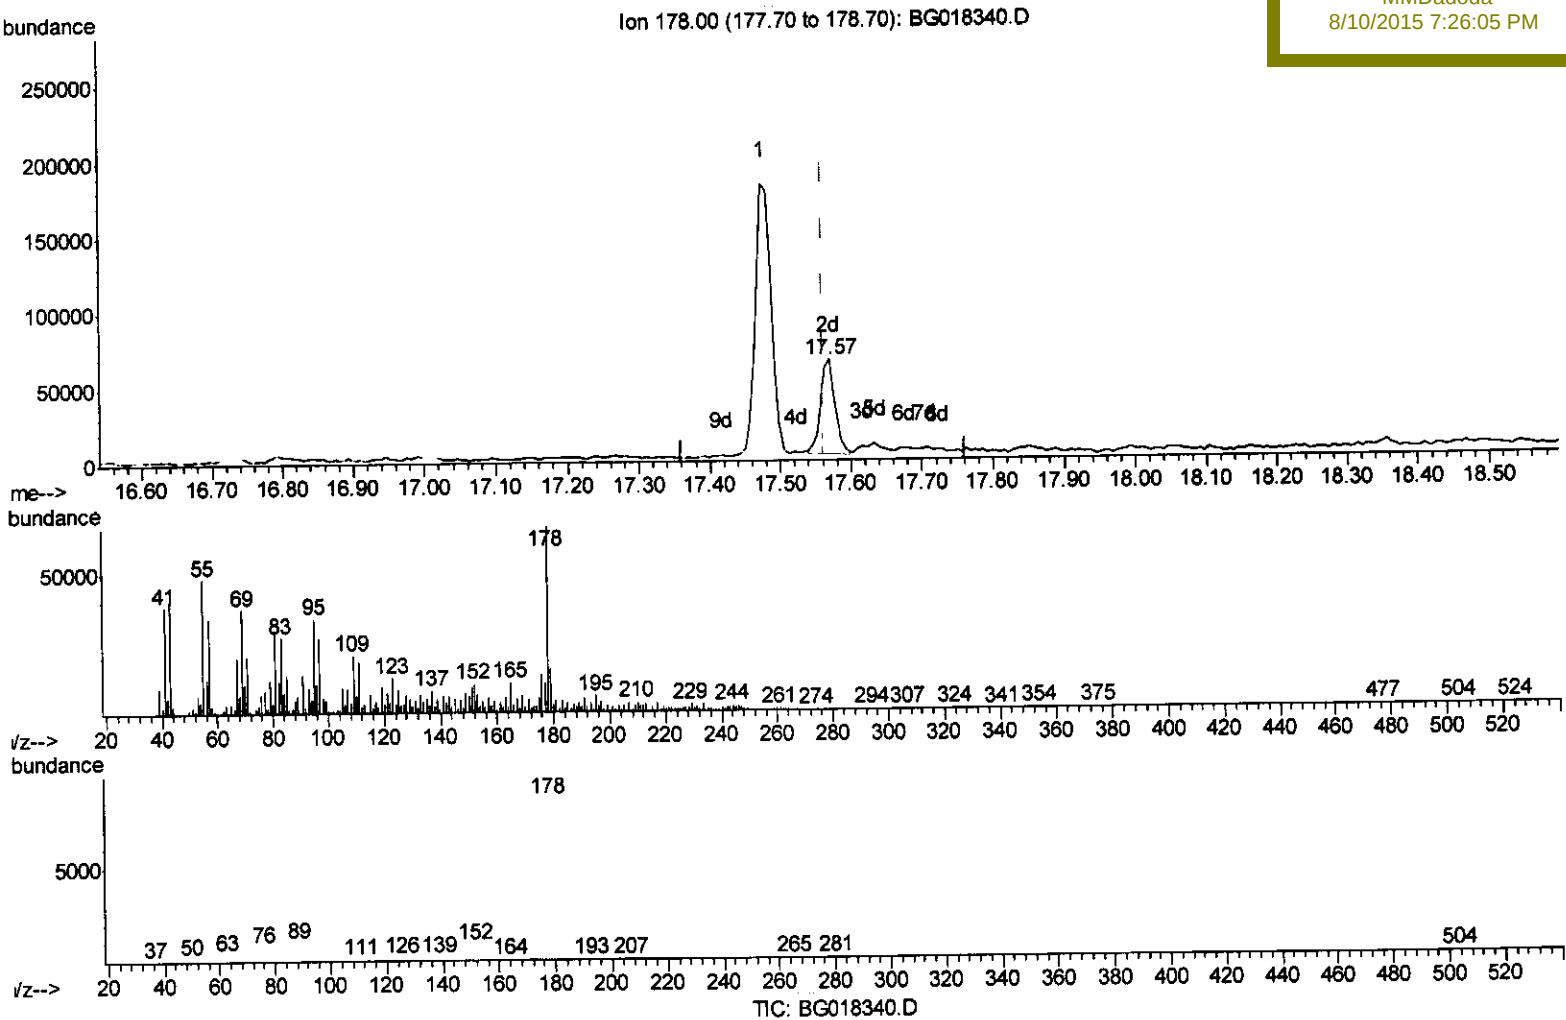

(72) Anthracene

17.569min (+0.008) 1.93ng/ul m

response 87011

Ion	Exp%	Act%
178.00	100	100
179.00	16.20	23.82#
176.00	20.00	20.98
0.00	0.00	0.00

U.M
08/11/15




Data Path : Z:\HPCHEM1\BNA_G\Data\BG080915\
Data File : BG018340.D
Acq On : 9 Aug 2015 22:18
Operator : UM/TP
Sample : G3136-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 10 07:51:55 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 07:50:23 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
C01T5

Manual Integrations
APPROVED

MMDadoda
8/10/2015 7:26:05 PM

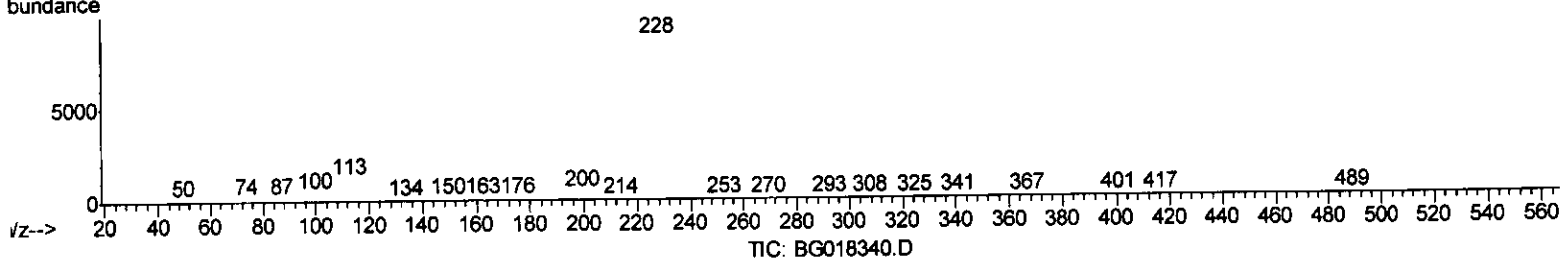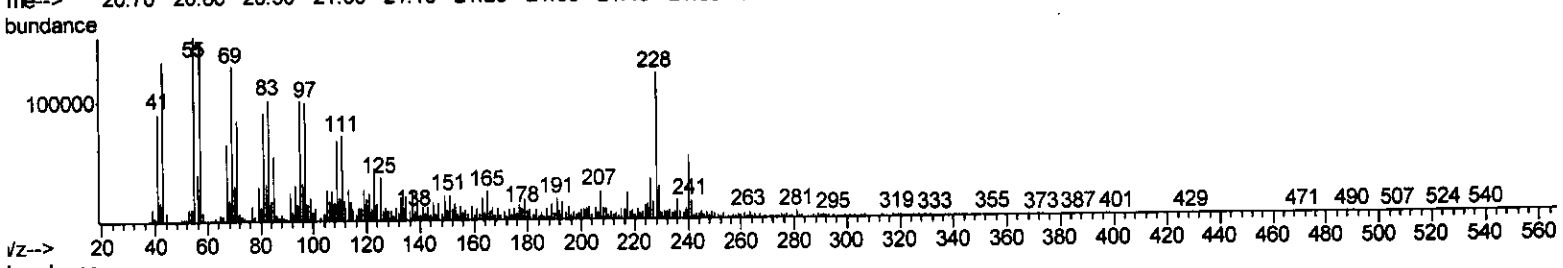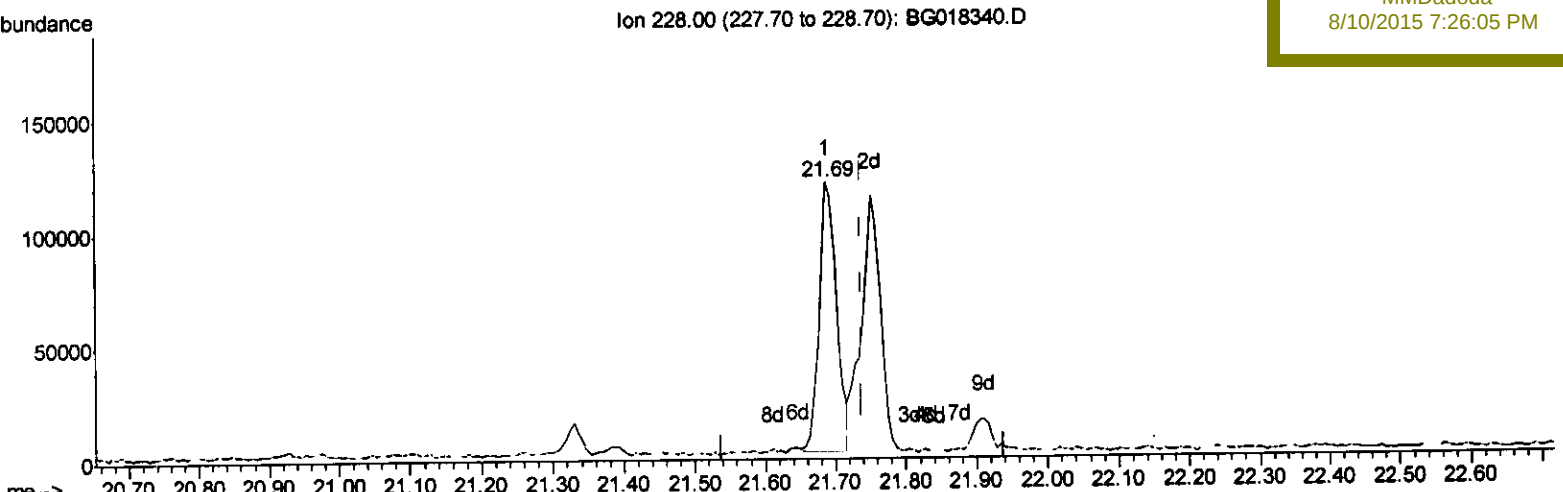

(85) Chrysene

21.688min (-0.051) 5.19ng/ul

response 204334




Ion	Exp%	Act%
228.00	100	100
226.00	33.10	28.34
229.00	21.10	22.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG080915\
Data File : BG018340.D
Acq On : 9 Aug 2015 22:18
Operator : UM/TP
Sample : G3136-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 10 07:51:55 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 07:50:23 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
C01T5

Manual Integrations
APPROVED
MMDadoda
8/10/2015 7:26:05 PM

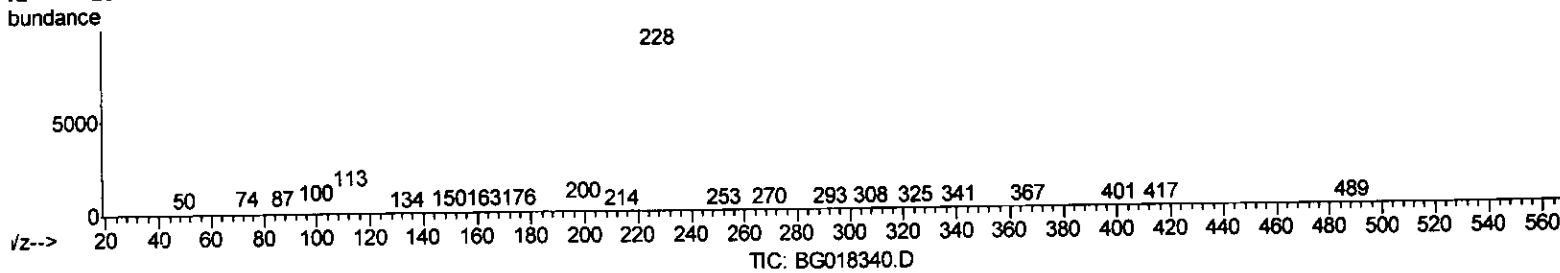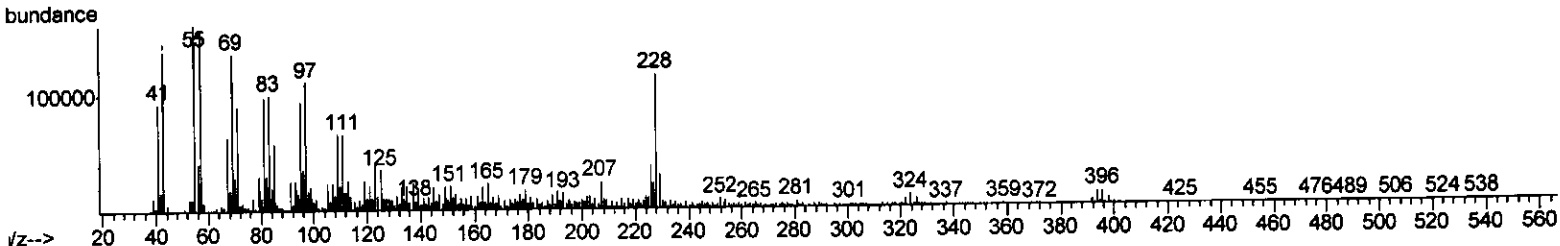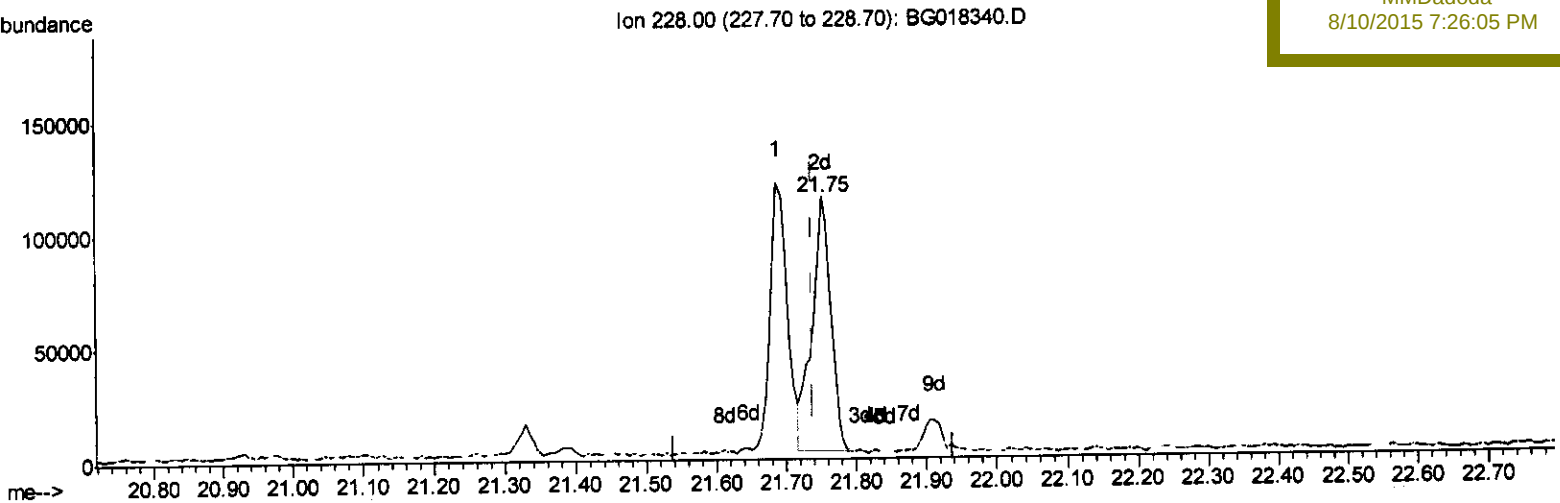

(85) Chrysene

21.752min (+0.014) 5.28ng/ul m

response 207019

Ion	Exp%	Act%
228.00	100	100
226.00	33.10	32.83
229.00	21.10	25.43#
0.00	0.00	0.00

> U.M
08/11/15




Data Path : Z:\HPCHEM1\BNA_G\Data\BG080915\
 Data File : BG018340.D
 Acq On : 9 Aug 2015 22:18
 Operator : UM/TP
 Sample : G3136-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 10 07:51:55 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 10 07:50:23 2015
 Response via : Initial Calibration

Instrument :
 BNA_G
 ClientSampleId :
 C01T5

Manual Integrations
 APPROVED

MMDadoda
 8/10/2015 7:26:05 PM

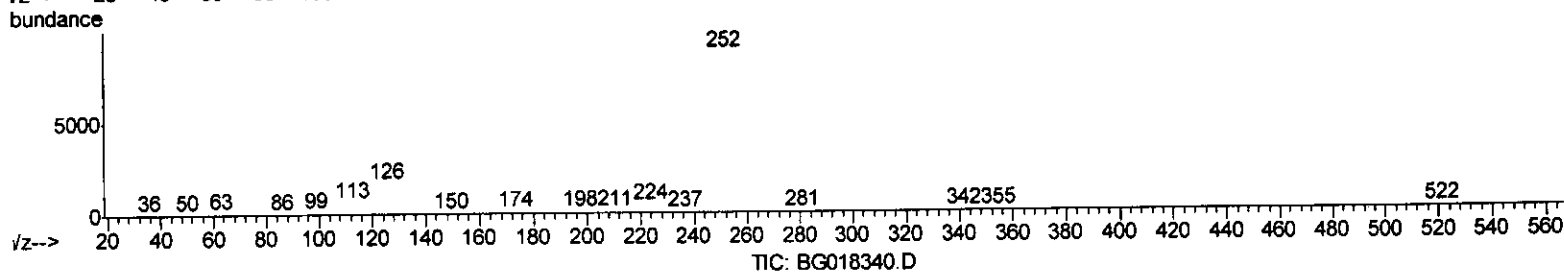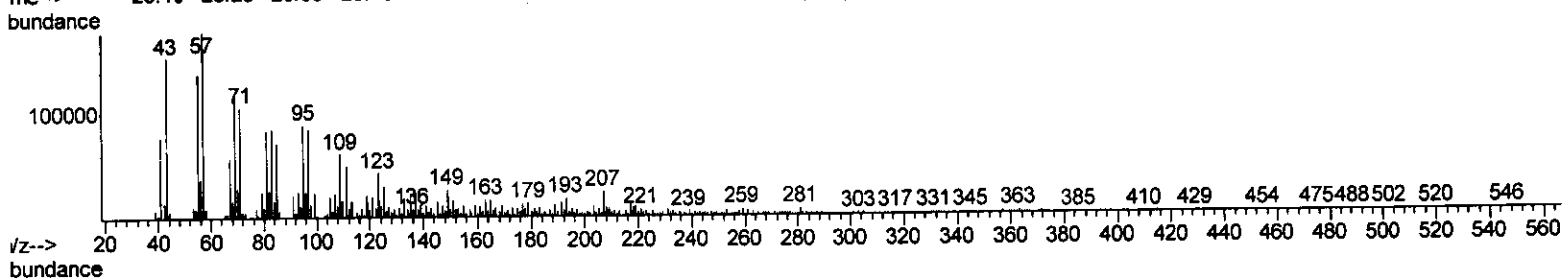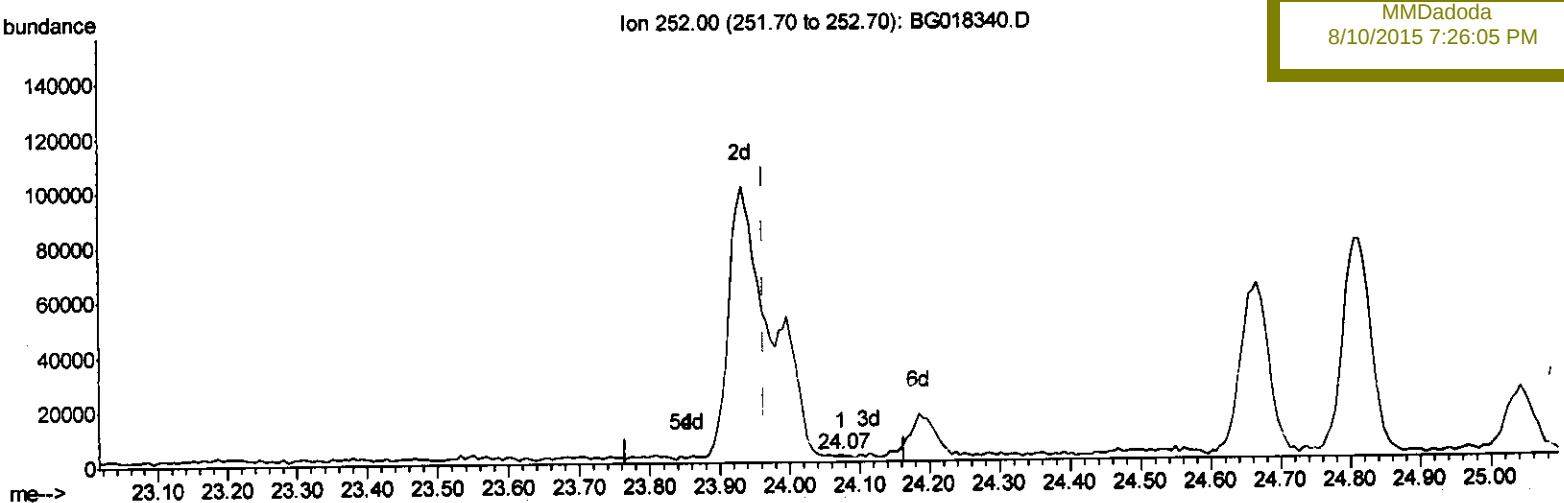

(89) Benzo(k)fluoranthene
 24.073min (+0.108) 0.02ng/ul
 response 829

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	168.03#
125.00	11.20	1047.71#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\Data\BG080915\
 Data File : BG018340.D
 Acq On : 9 Aug 2015 22:18
 Operator : UM/TP
 Sample : G3136-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 10 07:51:55 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 10 07:50:23 2015
 Response via : Initial Calibration

Instrument :
 BNA_G
 ClientSampleId :
 C01T5

Manual Integrations
 APPROVED

MMDadoda
 8/10/2015 7:26:05 PM

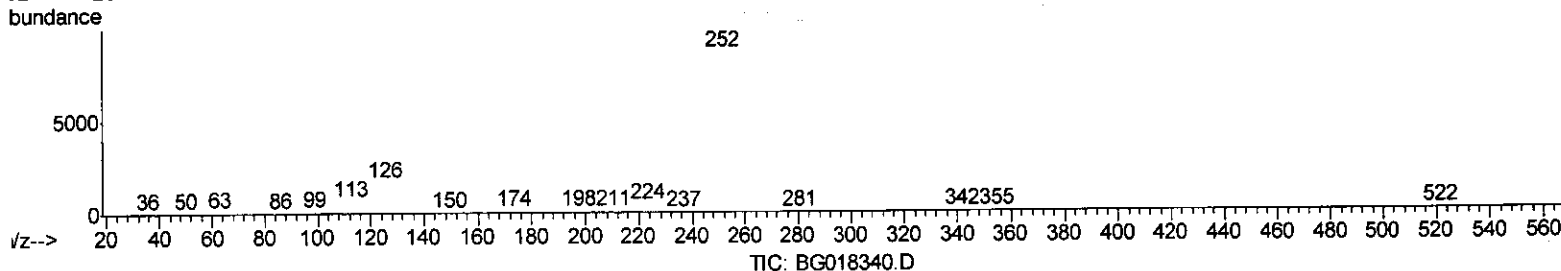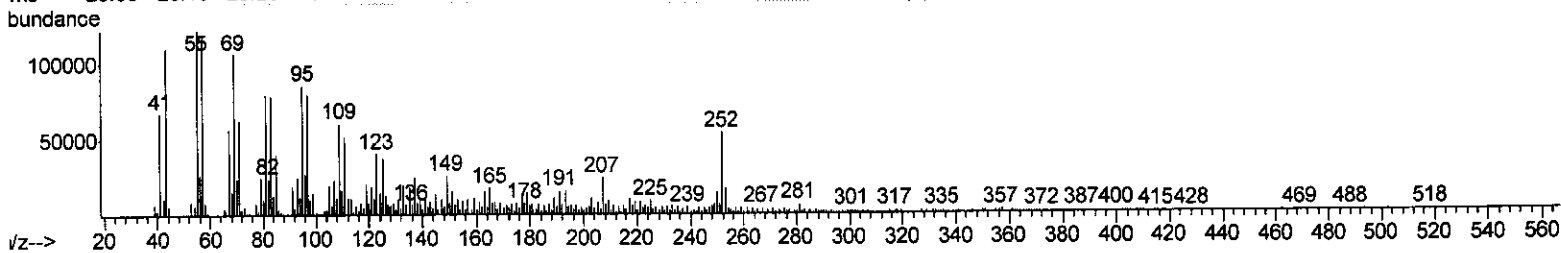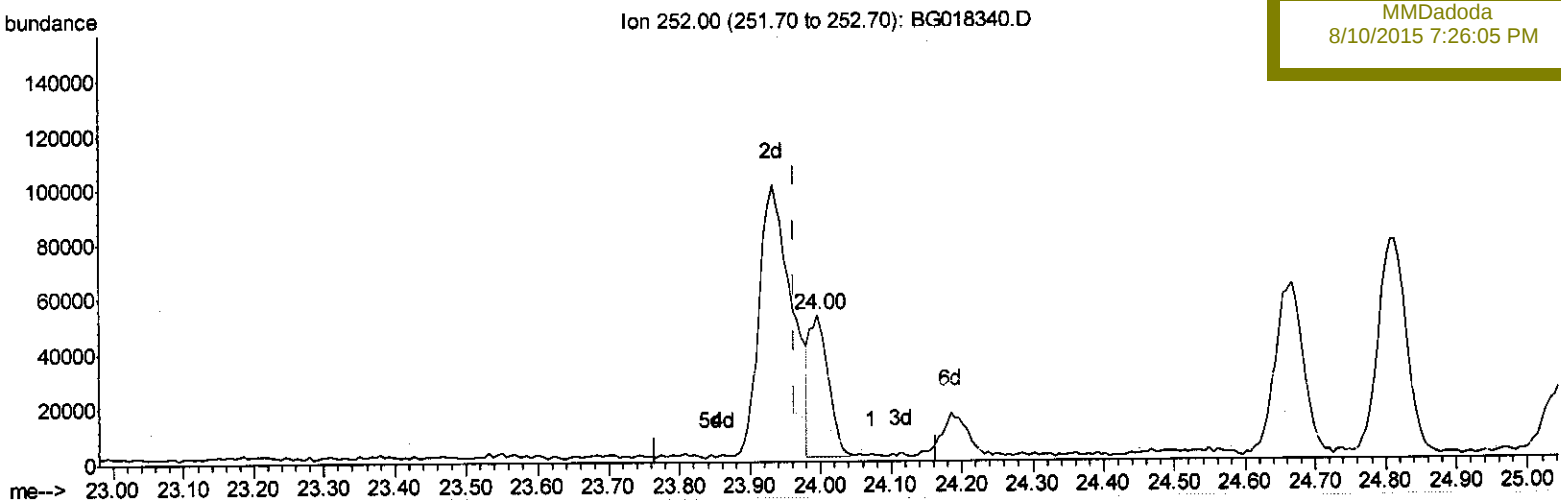

(89) Benzo(k)fluoranthene

23.997min (+0.031) 2.36ng/ul m

response 95944

U.M
 06/11/15

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	31.97#
125.00	11.20	68.95#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG080915\
Data File : BG018340.D
Acq On : 9 Aug 2015 22:18
Operator : UM/TP
Sample : G3136-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 10 08:06:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 07:50:23 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
C01T5

Manual Integrations
APPROVED

MMDadoda
8/10/2015 7:26:05 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	144706	20.00	ng/ul	0.00
18) Naphthalene-d8	10.88	136	683857	20.00	ng/ul	0.01
36) Acenaphthene-d10	14.70	164	413240	20.00	ng/ul	0.01
62) Phenanthrene-d10	17.43	188	816097	20.00	ng/ul	0.00
78) Chrysene-d12	21.71	240	679344	20.00	ng/ul	0.02
86) Perylene-d12	24.97	264	672705	20.00	ng/ul	0.05

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	5213	1.59	ng/uL	0.00
5) Phenol-d5	7.22	99	124036	9.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	84993	10.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	101970	10.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.76	113	55770	5.05	ng/ul	0.00
19) Nitrobenzene-d5	9.23	128	54005	10.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.95	143	58338	10.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.49	165	100454	8.72	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	45645	3.51	ng/ul	0.00
44) Dimethylphthalate-d6	14.10	166	331610	9.54	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	365772	8.35	ng/ul	0.00
52) 4-Nitrophenol-d4	14.86	143	27947	4.47	ng/ul	0.00
58) Fluorene-d10	15.68	176	236333	7.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.79	200	19293	4.81	ng/ul	0.00
71) Anthracene-d10	17.53	188	310071	7.94	ng/ul	0.00
79) Pyrene-d10	19.82	212	291499	8.27	ng/ul	0.01
90) Benzo(a)pyrene-d12	24.74	264	283625	7.94	ng/ul	0.03

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
14) Acetophenone	8.88	105	16553	1.04	ng/ul#	68
34) 2-Methylnaphthalene	12.53	142	30147	1.15	ng/ul	85
45) Dimethylphthalate	14.14	163	162601	4.74	ng/ul#	97
70) Phenanthrene	17.47	178	278685	6.29	ng/ul	99
72) Anthracene	17.57	178	87011m	1.93	ng/ul	
77) Fluoranthene	19.48	202	452083	9.56	ng/ul	99
80) Pyrene	19.85	202	440487	9.59	ng/ul	100
81) Butylbenzylphthalate	20.73	149	110045	5.66	ng/ul#	81
83) Benzo(a)anthracene	21.69	228	206191	4.90	ng/ul	96
84) Bis(2-ethylhexyl)phthalate	21.61	149	728648	26.54	ng/ul#	98
85) Chrysene	21.75	228	207019m	5.26	ng/ul	
88) Benzo(b)fluoranthene	23.93	252	313296	7.41	ng/ul#	79
89) Benzo(k)fluoranthene	24.00	252	95944m	2.36	ng/ul	
91) Benzo(a)pyrene	24.81	252	215618	5.37	ng/ul#	69
92) Indeno(1,2,3-cd)pyrene	28.67	276	167571	3.60	ng/ul#	81
94) Benzo(g,h,i)perylene	29.83	276	157176	4.03	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M
08/11/15