

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080915\
 Data File : BG018334.D
 Acq On : 9 Aug 2015 18:30
 Operator : UM/TP
 Sample : G3136-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C02D2

Quant Time: Aug 10 07:39:26 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 10 07:38:18 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	142479	20.00	ng/ul	0.00
18) Naphthalene-d8	10.87	136	647894	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	405054	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	989869	20.00	ng/ul	0.00
78) Chrysene-d12	21.69	240	942533	20.00	ng/ul	0.00
86) Perylene-d12	24.92	264	896340	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	7844	2.43	ng/uL	0.00
5) Phenol-d5	7.22	99	181042	14.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	115755	14.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	138233	13.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.76	113	149642	13.77	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	71374	14.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.95	143	72677	14.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	144329	13.22	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	201405	16.32	ng/ul	0.00
44) Dimethylphthalate-d6	14.09	166	479693	14.08	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	581139	13.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.85	143	83618	13.64	ng/ul	0.00
58) Fluorene-d10	15.68	176	417165	14.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.78	200	55398	11.38	ng/ul	0.00
71) Anthracene-d10	17.52	188	648688	13.70	ng/ul	0.00
79) Pyrene-d10	19.80	212	712996	14.58	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.70	264	738288	15.52	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.14	163	242435	7.21	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080915\
Data File : BG018334.D
Acq On : 9 Aug 2015 18:30
Operator : UM/TP
Sample : G3136-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C02D2

Quant Time: Aug 10 07:39:26 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 07:38:18 2015
Response via : Initial Calibration

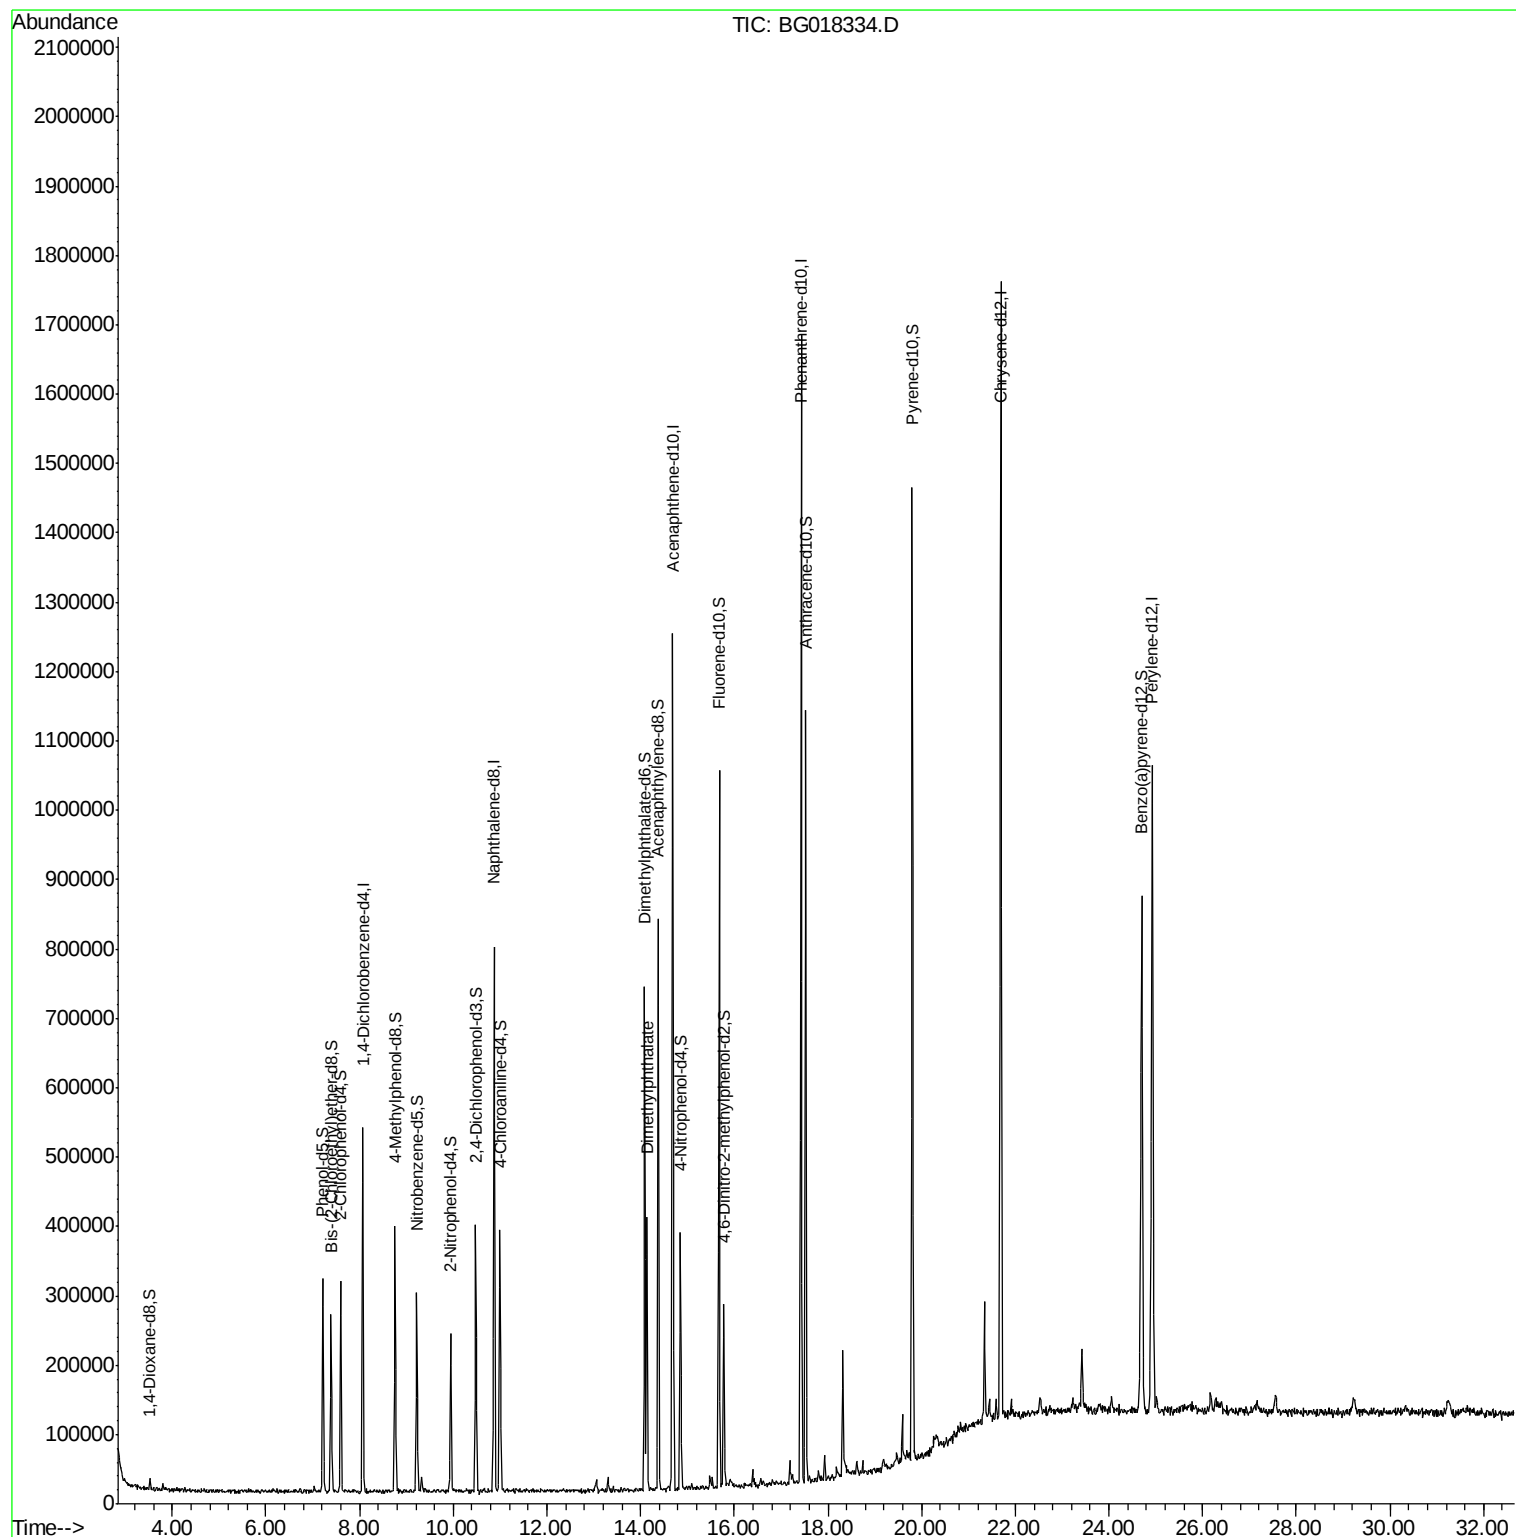

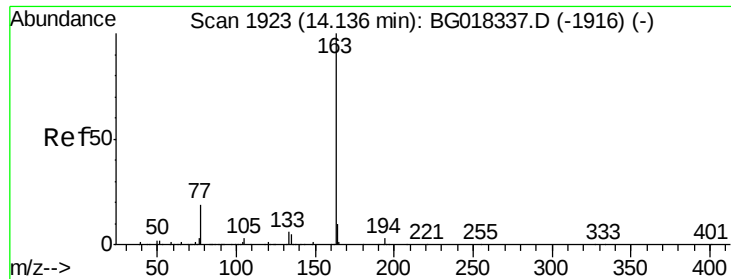

#45

Dimethylphthalate

Concen: 7.21 ng/ul

RT: 14.14 min Scan# 1923

Delta R.T. -0.00 min

Lab File: BG018334.D

Acq: 9 Aug 2015 18:30

Instrument :

BNA_G

ClientSampleId :

C02D2


Tot Ion:163 Resp: 242435

Ion Ratio Lower Upper

163 100

194 4.0 2.9 4.3

164 9.7 7.7 11.5

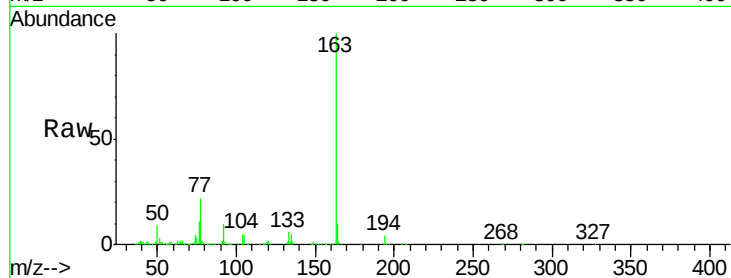

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

