

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080916\
 Data File : BG023558.D
 Acq On : 9 Aug 2016 16:09
 Operator : UM/SJ
 Sample : H4362-04MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS005-0002-01MS

Manual Integrations
 APPROVED

sohil
 8/10/2016 6:49:27 PM

Quant Time: Aug 10 05:21:41 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 10 05:01:49 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	130069	20.00	ng/ul	-0.03
18) Naphthalene-d8	10.95	136	625497	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.78	164	478952	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1179182	20.00	ng/ul	0.00
75) Chrysene-d12	21.87	240	1189572	20.00	ng/ul	0.00
83) Perylene-d12	25.26	264	1159702	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	6278	2.05	ng/uL	0.00
5) Phenol-d5	7.26	99	293795	22.42	ng/ul	-0.03
7) Bis-(2-Chloroethyl)ether-d	7.42	67	207631	24.73	ng/ul	-0.03
9) 2-Chlorophenol-d4	7.63	132	208398	23.31	ng/ul	-0.03
13) 4-Methylphenol-d8	8.83	113	211666	20.69	ng/ul	-0.02
19) Nitrobenzene-d5	9.29	128	112231	22.76	ng/ul	-0.03
22) 2-Nitrophenol-d4	10.02	143	131634	23.25	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.57	165	233839	21.89	ng/ul	-0.02
29) 4-Chloroaniline-d4	11.08	131	288642	23.03	ng/ul	-0.02
43) Dimethylphthalate-d6	14.18	166	899872	22.95	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	1021569	23.15	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	139666	20.86	ng/ul	0.00
57) Fluorene-d10	15.78	176	826348	22.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	162273	21.45	ng/ul	0.00
70) Anthracene-d10	17.64	188	1267108	23.85	ng/ul	0.00
76) Pyrene-d10	19.94	212	1419434	23.57	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.02	264	1267283	24.14	ng/ul	0.00

Target Compounds

						Qvalue
6) Phenol	7.29	94	303323m	22.23	ng/ul	
10) 2-Chlorophenol	7.67	128	198772	21.83	ng/ul#	83
15) N-Nitroso-di-n-propylamine	8.92	70	240927	24.41	ng/ul#	90
33) 4-Chloro-3-methylphenol	12.23	107	327897	23.65	ng/ul	84
44) Dimethylphthalate	14.23	163	497258	12.81	ng/ul	99
49) Acenaphthene	14.85	153	720744	22.92	ng/ul	95
52) 4-Nitrophenol	15.01	109	143300	21.37	ng/ul#	75
54) 2,4-Dinitrotoluene	15.15	165	293055	22.97	ng/ul#	67
68) Pentachlorophenol	17.20	266	187890	23.64	ng/ul	98
69) Phenanthrene	17.59	178	101990	1.67	ng/ul#	92
74) Fluoranthene	19.61	202	200995	3.21	ng/ul#	89
77) Pyrene	19.97	202	1834864	24.95	ng/ul	95
80) Benzo(a)anthracene	21.84	228	77838	1.16	ng/ul	94
81) Bis(2-ethylhexyl)phthalate	21.73	149	38265	1.02	ng/ul	99
82) Chrysene	21.92	228	97486	1.60	ng/ul	96
85) Benzo(b)fluoranthene	24.19	252	118470m	1.80	ng/ul	
88) Benzo(a)pyrene	25.09	252	83810	1.32	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080916\
Data File : BG023558.D
Acq On : 9 Aug 2016 16:09
Operator : UM/SJ
Sample : H4362-04MS
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
PR001-SS005-0002-01MS

Manual Integrations
APPROVED

sohil
8/10/2016 6:49:27 PM

Quant Time: Aug 10 05:21:41 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 10 05:01:49 2016
Response via : Initial Calibration

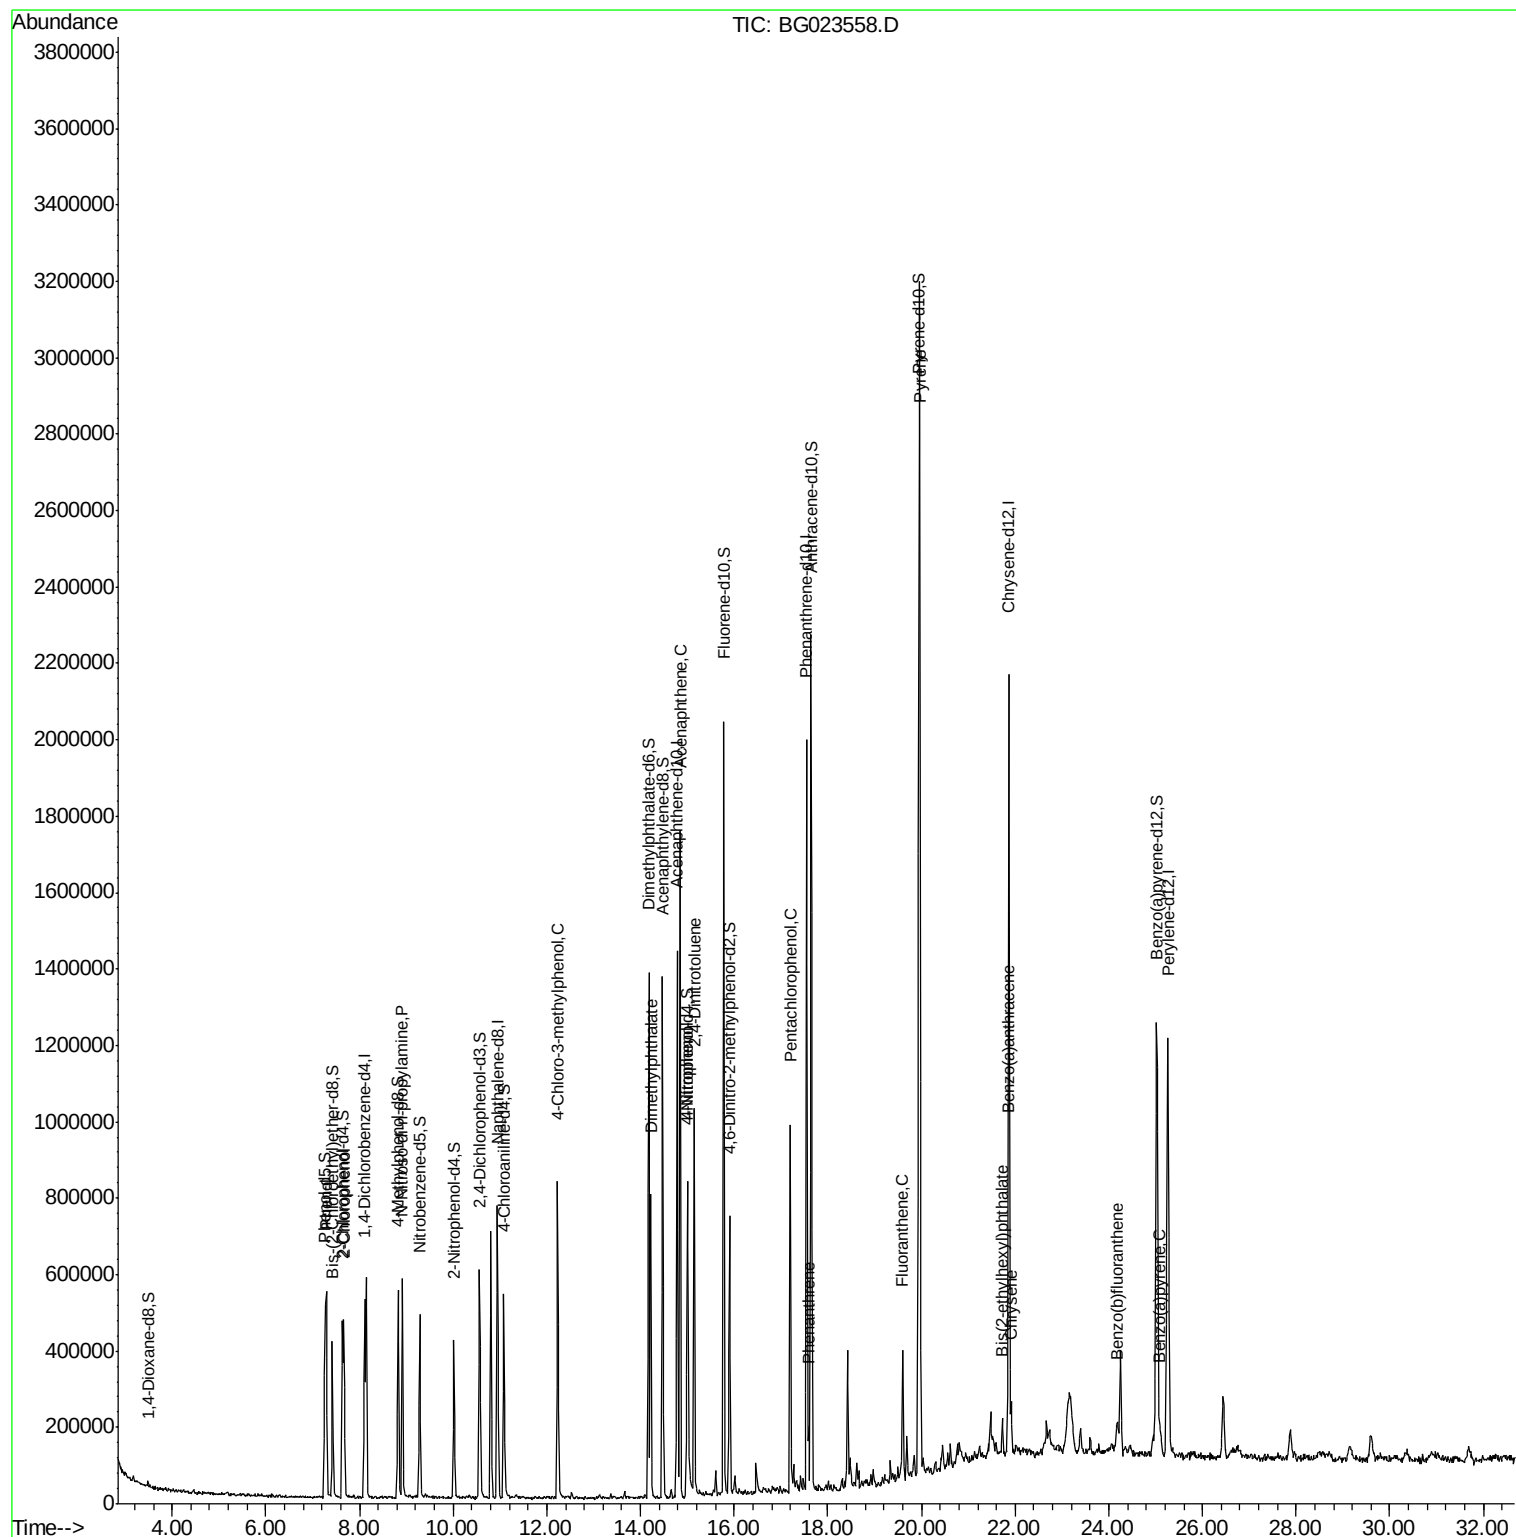

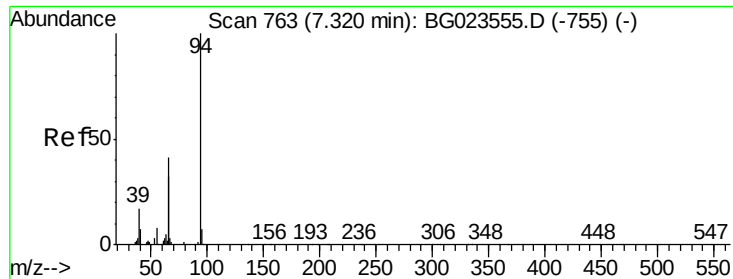

#6

Phenol

Concen: 22.23 ng/ul m

RT: 7.29 min Scan# 757

Delta R.T. -0.03 min

Lab File: BG023558.D

Acq: 9 Aug 2016 16:09

Instrument :

BNA_G

ClientSampleId :

PR001-SS005-0002-01MS

Tgt Ion: 94 Resp: 303323

Ion Ratio Lower Upper

94 100





65 32.0 16.8 25.2#

66 41.9 22.6 33.8#

Manual Integrations
APPROVED

sohil

8/10/2016 6:49:27 PM

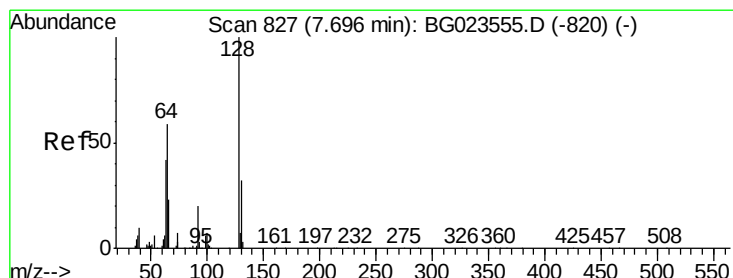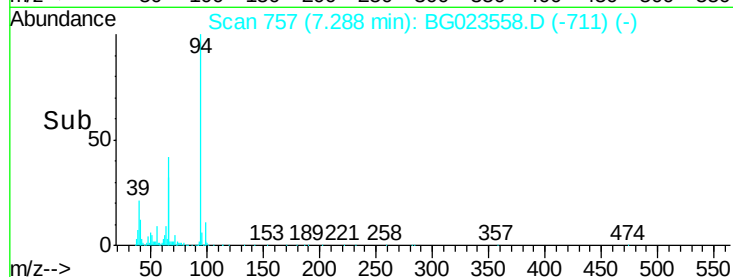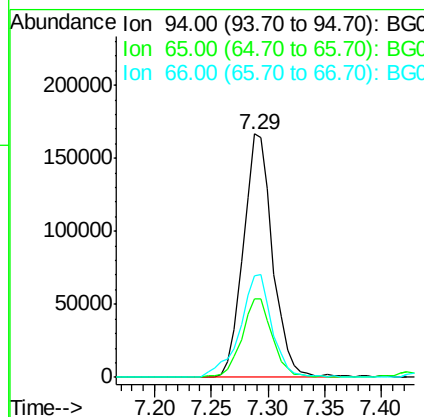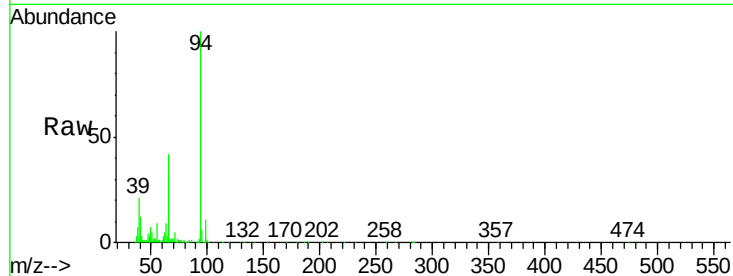

#10

2-Chlorophenol

Concen: 21.83 ng/ul

RT: 7.67 min Scan# 822

Delta R.T. -0.03 min

Lab File: BG023558.D

Acq: 9 Aug 2016 16:09




Tgt Ion: 128 Resp: 198772




Ion Ratio Lower Upper

128 100

64 60.6 34.2 51.4#

130 31.8 27.0 40.4

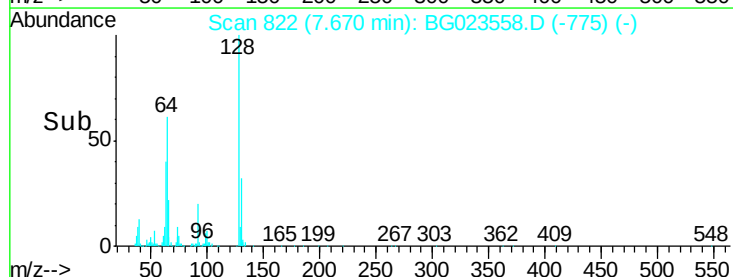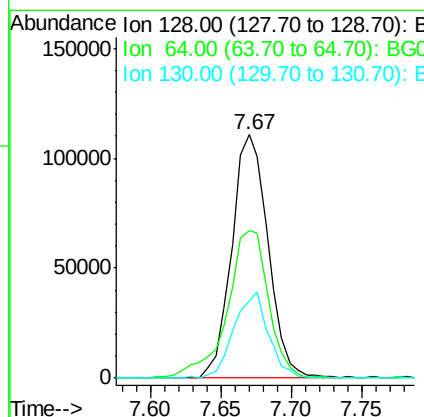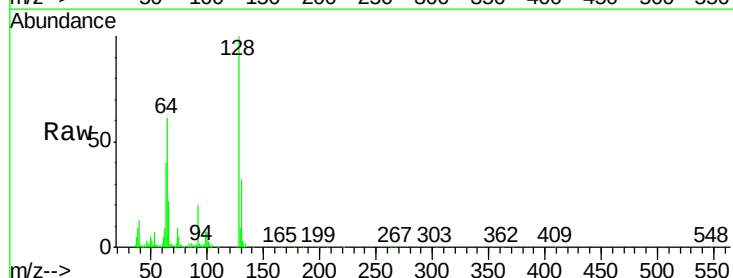

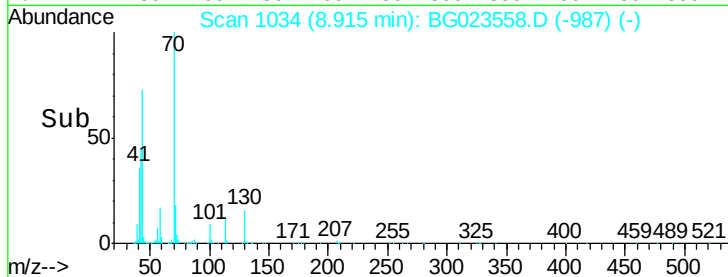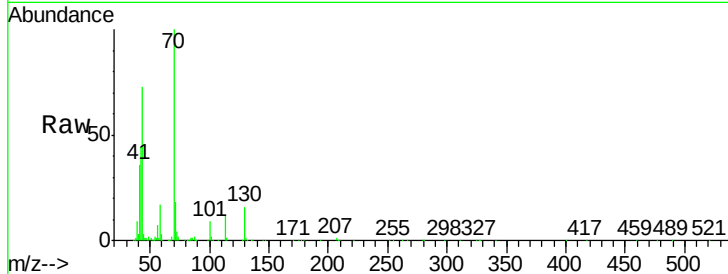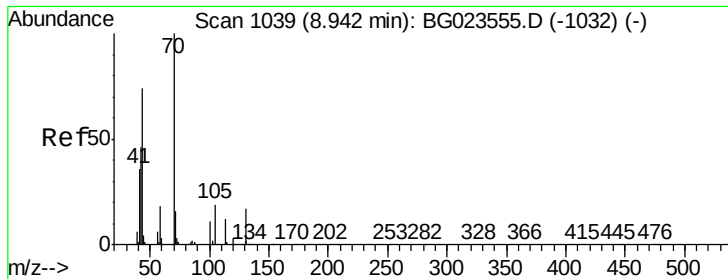





#15
N-Nitroso-di-n-propylamine
Concen: 24.41 ng/ul
RT: 8.92 min Scan# 1034
Delta R.T. -0.03 min
Lab File: BG023558.D
Acq: 9 Aug 2016 16:09

Instrument :
BNA_G
ClientSampleId :
PR001-SS005-0002-01MS

Tgt Ion	Ratio	Lower	Upper
70	100		
42	44.1	31.4	47.2
101	8.8	8.6	13.0
130	16.0	19.0	28.4


Manual Integrations
APPROVED


sohil
8/10/2016 6:49:27 PM

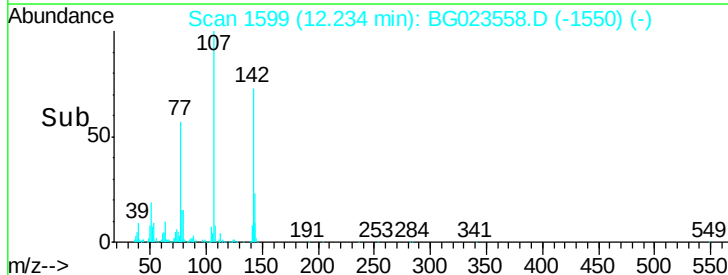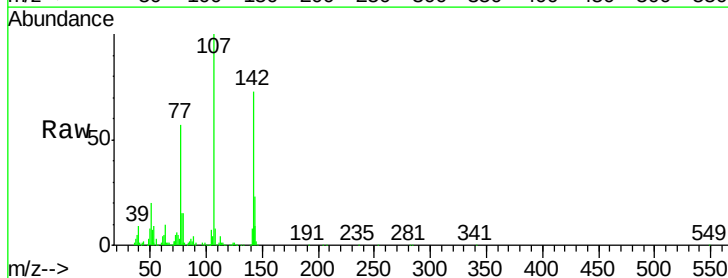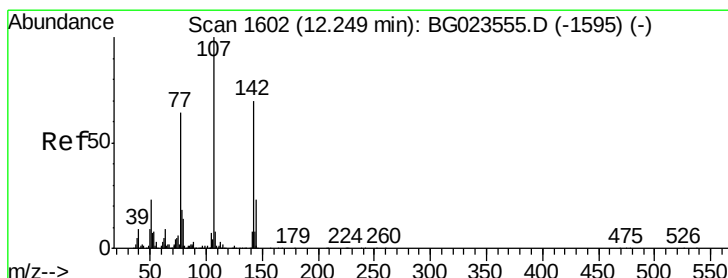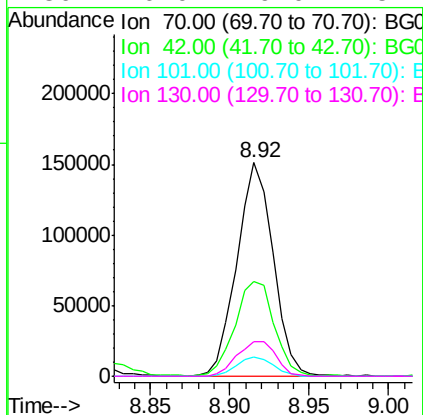

#33
4-Chloro-3-methylphenol
Concen: 23.65 ng/ul
RT: 12.23 min Scan# 1599
Delta R.T. -0.01 min
Lab File: BG023558.D
Acq: 9 Aug 2016 16:09

Tgt Ion	Ratio	Lower	Upper
107	100		
144	23.0	22.7	34.1
142	72.6	71.6	107.4

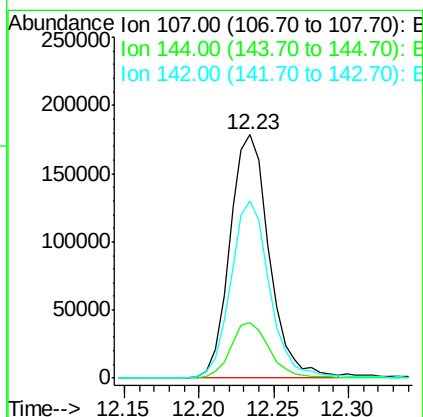

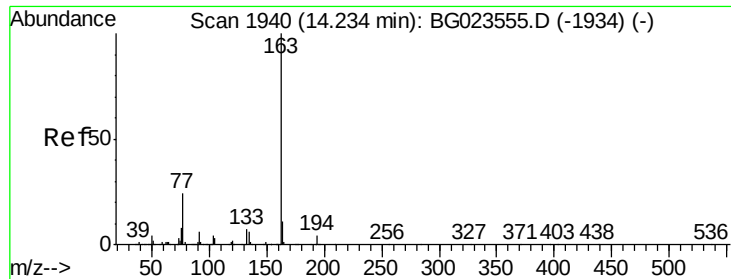





#44
Dimethylphthalate
Concen: 12.81 ng/ul
RT: 14.23 min Scan# 1938
Delta R.T. -0.01 min
Lab File: BG023558.D
Acq: 9 Aug 2016 16:09

Instrument :
BNA_G
ClientSampleId :
PR001-SS005-0002-01MS

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.4	5.2
164	10.6	8.8	13.2




Manual Integrations
APPROVED


sohil
8/10/2016 6:49:27 PM

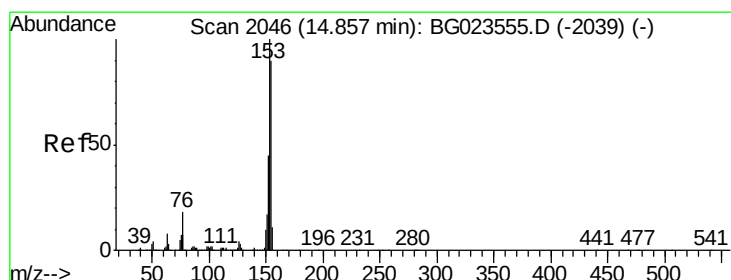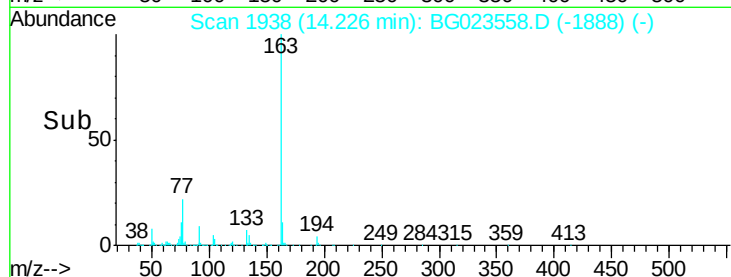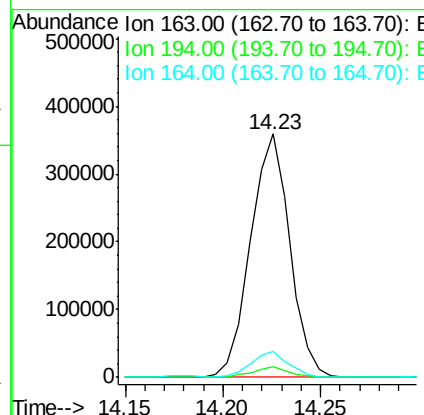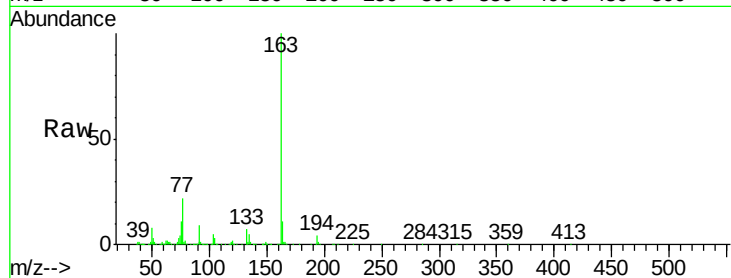

#49
Acenaphthene
Concen: 22.92 ng/ul
RT: 14.85 min Scan# 2044
Delta R.T. -0.01 min
Lab File: BG023558.D
Acq: 9 Aug 2016 16:09

Tgt Ion	Ratio	Lower	Upper
153	100		
152	49.1	37.3	55.9
154	90.6	68.2	102.2

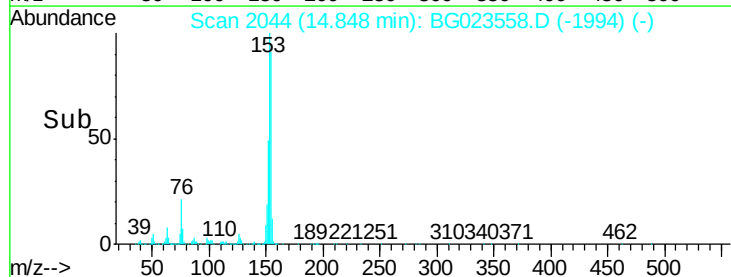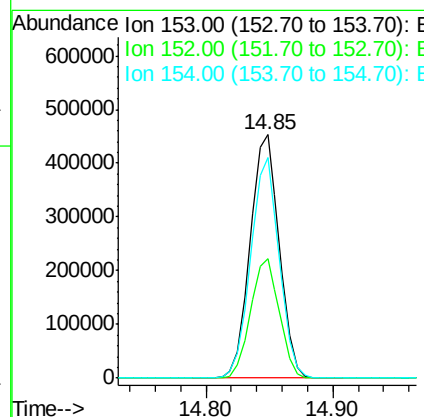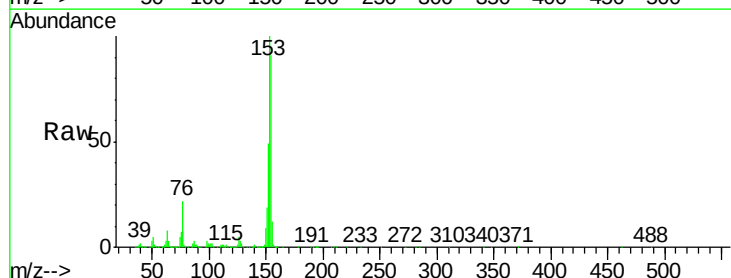

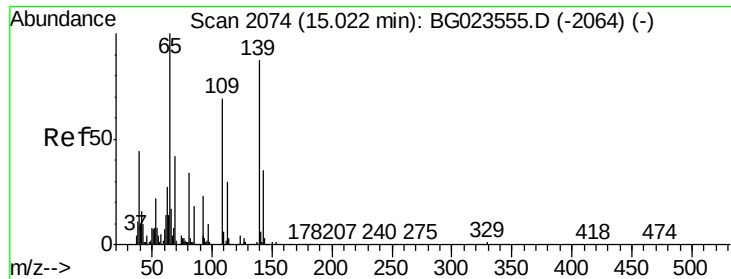





#52
4-Nitrophenol
Concen: 21.37 ng/ul
RT: 15.01 min Scan# 2071
Delta R.T. -0.01 min
Lab File: BG023558.D
Acq: 9 Aug 2016 16:09

Instrument :
BNA_G
ClientSampleId :
PR001-SS005-0002-01MS

Tgt Ion	Ratio	Resp	Lower	Upper
109	100	143300		
139	114.5	136.1	204.1#	
65	138.3	106.0	159.0	




Manual Integrations
APPROVED


sohil
8/10/2016 6:49:27 PM

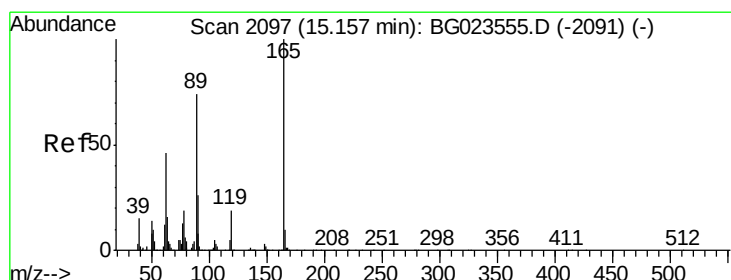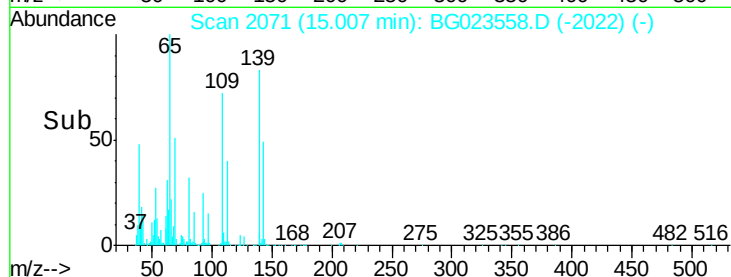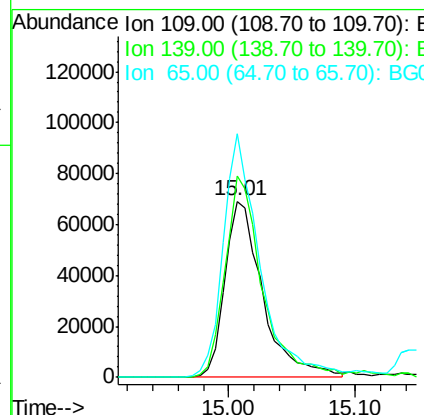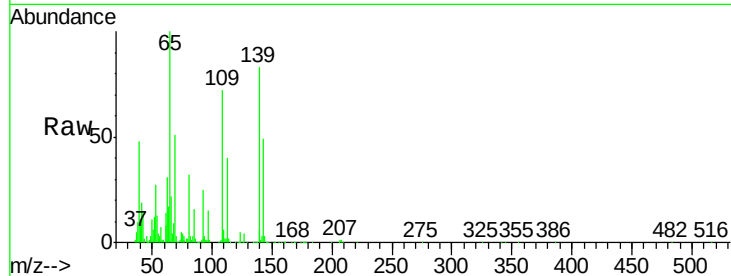

#54
2,4-Dinitrotoluene
Concen: 22.97 ng/ul
RT: 15.15 min Scan# 2095
Delta R.T. -0.01 min
Lab File: BG023558.D
Acq: 9 Aug 2016 16:09

Tgt Ion	Ratio	Resp	Lower	Upper
165	100	293055		
63	51.9	25.7	38.5#	
182	2.0	2.1	3.1#	

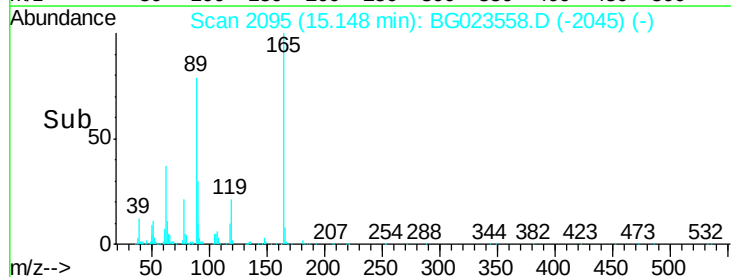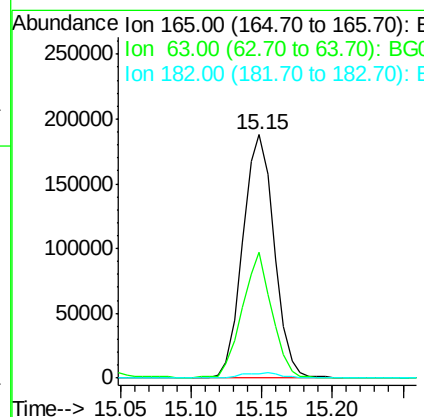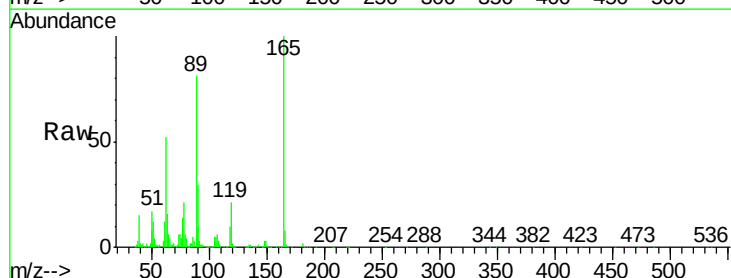

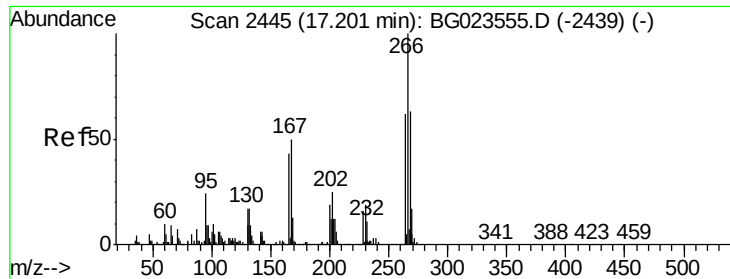

#68

Pentachlorophenol

Concen: 23.64 ng/ul

RT: 17.20 min Scan# 2444

Delta R.T. -0.00 min

Lab File: BG023558.D

Acq: 9 Aug 2016 16:09

Instrument :

BNA_G


ClientSampleId :

PR001-SS005-0002-01MS




Tgt Ion:	266	Resp:	187890
Ion Ratio	Lower	Upper	
266	100		
264	66.7	54.7	82.1
268	70.4	57.8	86.8

Manual Integrations
APPROVED

sohil
8/10/2016 6:49:27 PM

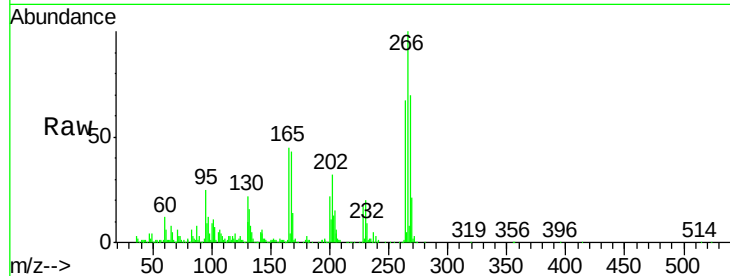

Abundance Ion 265.70 (265.40 to 266.40): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E

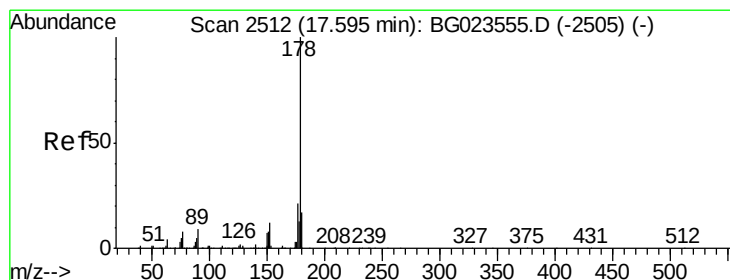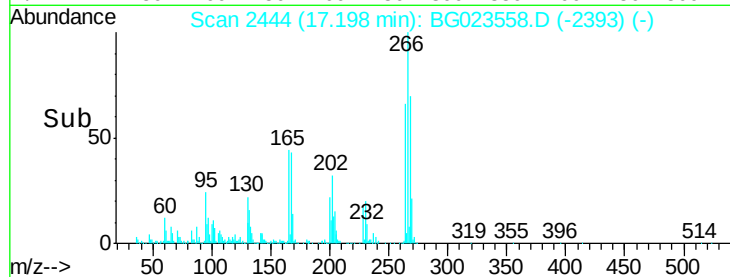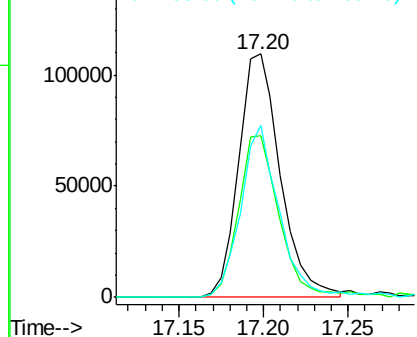

#69

Phenanthrene

Concen: 1.67 ng/ul


RT: 17.59 min Scan# 2511

Delta R.T. -0.00 min



Lab File: BG023558.D


Acq: 9 Aug 2016 16:09

Tgt Ion:	178	Resp:	101990
Ion Ratio	Lower	Upper	
178	100		
179	12.6	12.9	19.3#
176	16.2	15.8	23.8

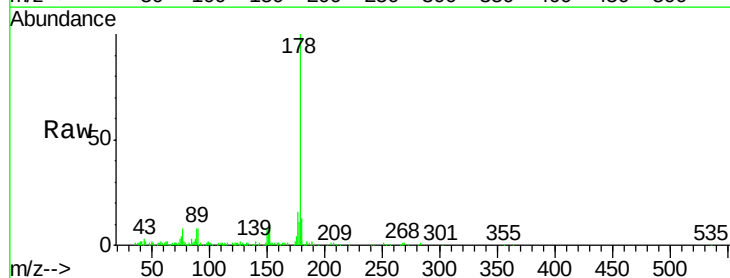

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

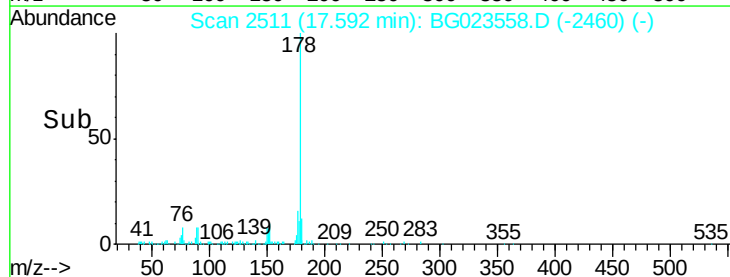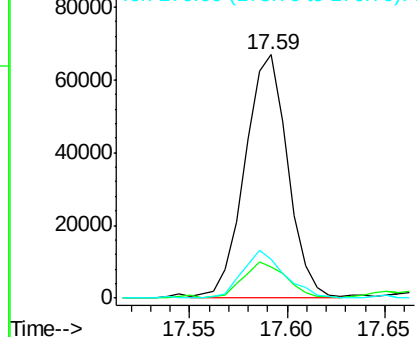

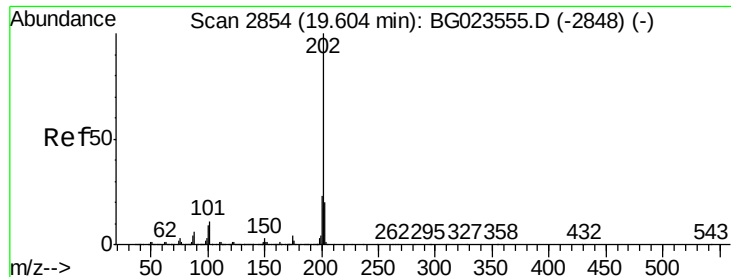

#74

Fluoranthene

Concen: 3.21 ng/ul

RT: 19.61 min Scan# 2854

Delta R.T. 0.00 min

Lab File: BG023558.D

Acq: 9 Aug 2016 16:09

Instrument :

BNA_G


ClientSampleId :

PR001-SS005-0002-01MS


Tgt Ion	Ratio	Resp Lower	Upper
202	100		
101	7.6	10.6	16.0#
100	8.2	8.7	13.1#

Manual Integrations
APPROVED



sohil
8/10/2016 6:49:27 PM

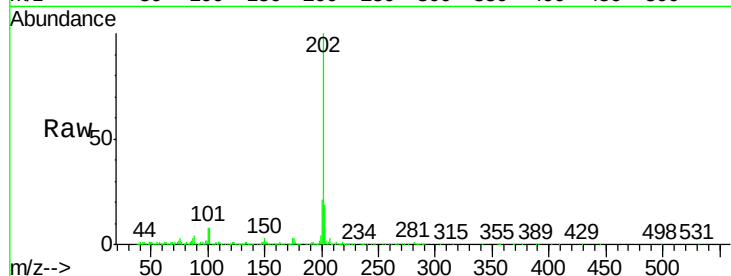

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

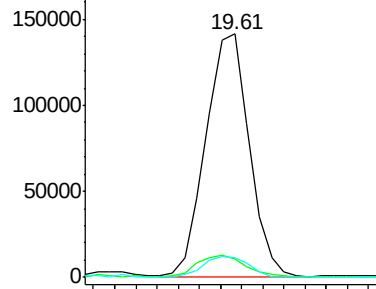

Time-->

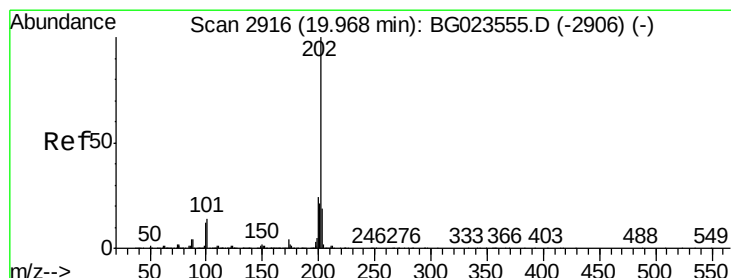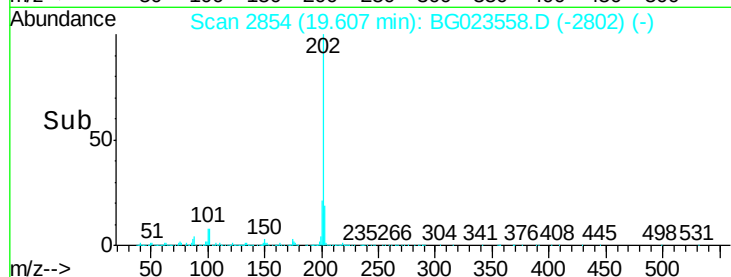

#77

Pyrene

Concen: 24.95 ng/ul


RT: 19.97 min Scan# 2916

Delta R.T. 0.00 min


Lab File: BG023558.D

Acq: 9 Aug 2016 16:09


Tgt Ion	Ratio	Resp Lower	Upper
202	100		
101	13.8	12.5	18.7
100	10.8	10.2	15.4

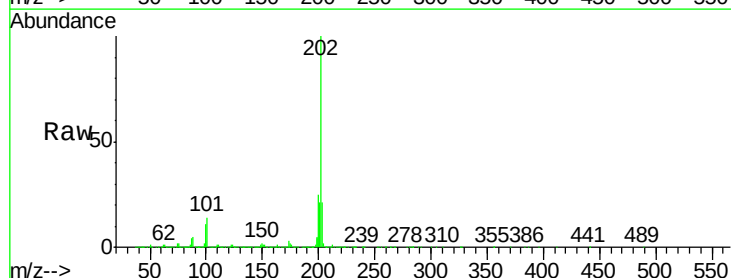


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

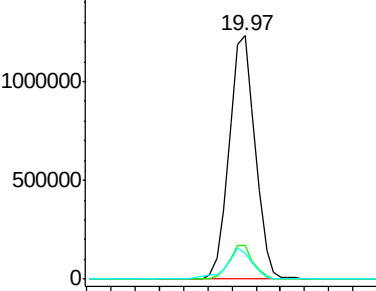

Time-->

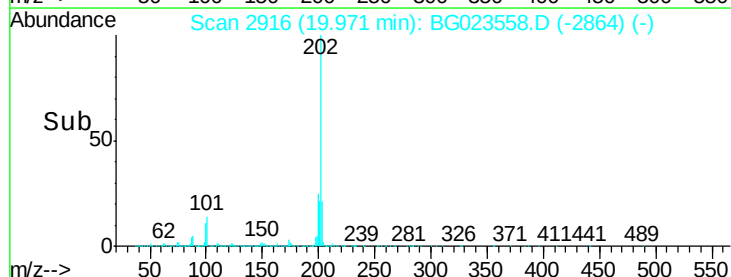

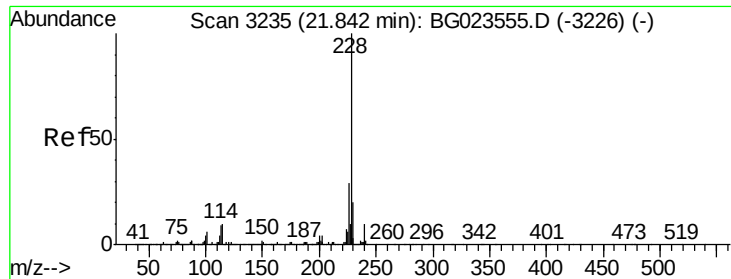

#80

Benzo(a)anthracene

Concen: 1.16 ng/ul

RT: 21.84 min Scan# 3235

Delta R.T. 0.00 min

Lab File: BG023558.D

Acq: 9 Aug 2016 16:09

Instrument :

BNA_G





ClientSampleId :

PR001-SS005-0002-01MS

Tgt Ion:	228	Resp:	77838
Ion Ratio	Lower	Upper	
228	100		
229	21.7	15.4	23.2
226	31.6	22.8	34.2

Manual Integrations
APPROVED

sohil
8/10/2016 6:49:27 PM

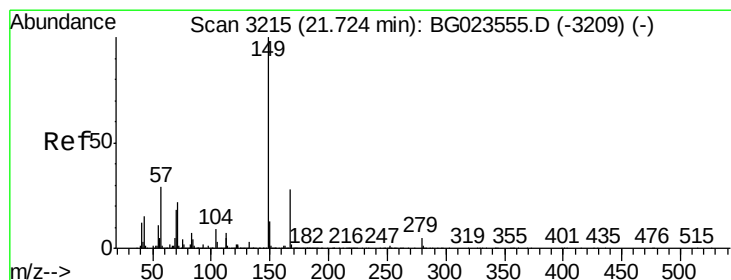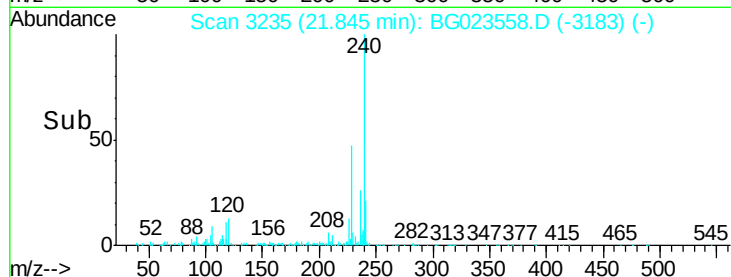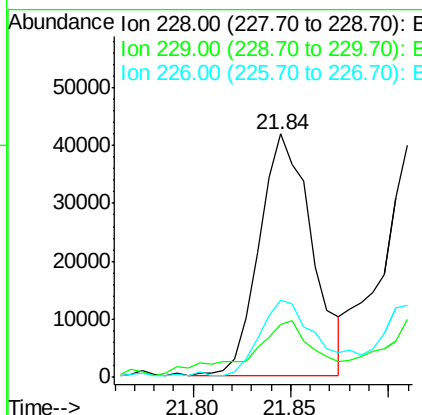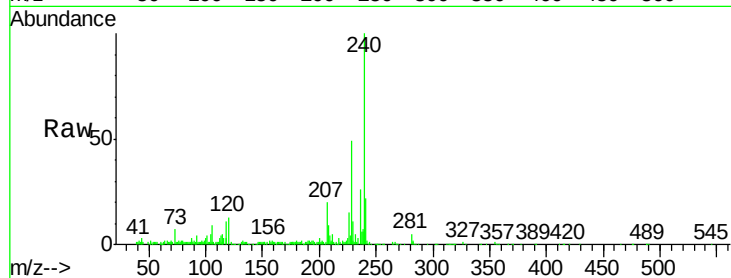

#81

Bis(2-ethylhexyl)phthalate

Concen: 1.02 ng/ul




RT: 21.73 min Scan# 3215


Delta R.T. 0.00 min

Lab File: BG023558.D

Acq: 9 Aug 2016 16:09

Tgt Ion:	149	Resp:	38265
Ion Ratio	Lower	Upper	
149	100		
167	27.0	21.9	32.9
279	3.6	2.9	4.3

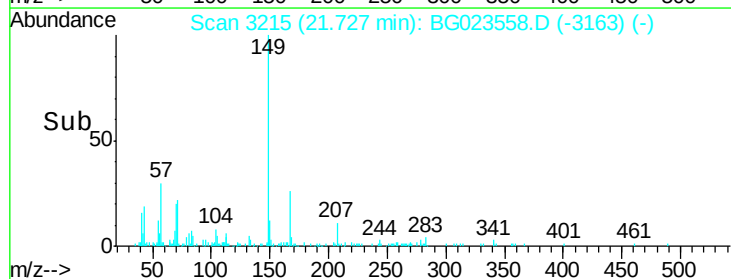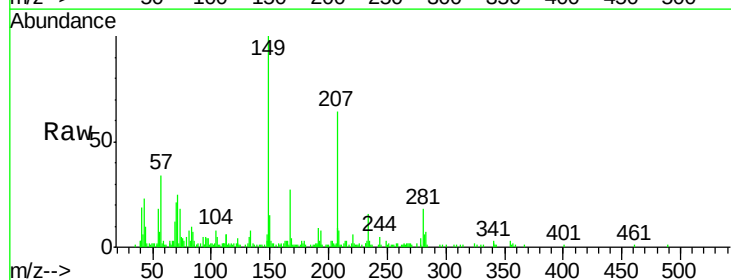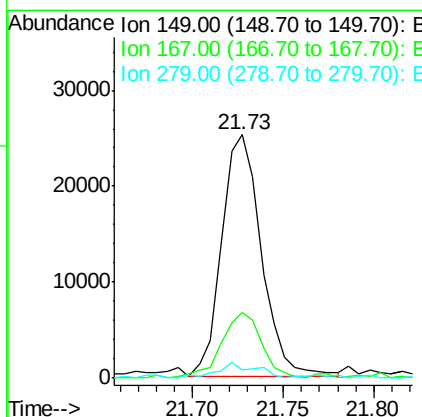

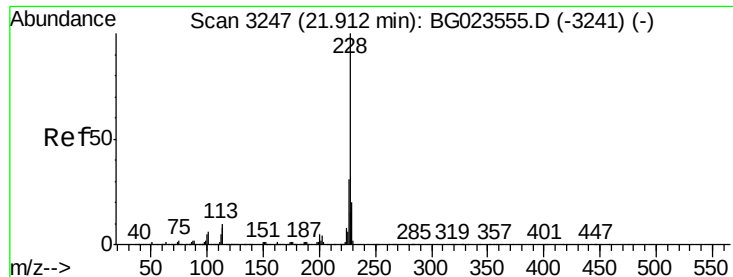





#82
Chrysene
 Concen: 1.60 ng/ul
 RT: 21.92 min Scan# 3247
 Delta R.T. 0.00 min
 Lab File: BG023558.D
 Acq: 9 Aug 2016 16:09

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS005-0002-01MS

Tgt Ion:	228	Resp:	97486
Ion Ratio	Lower	Upper	
228	100		
226	29.4	24.2	36.4
229	21.8	15.0	22.6




Manual Integrations
 APPROVED




sohil
 8/10/2016 6:49:27 PM

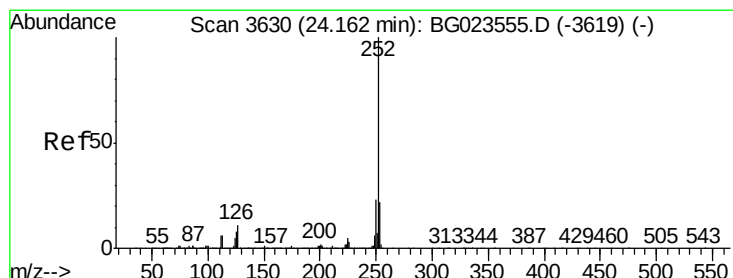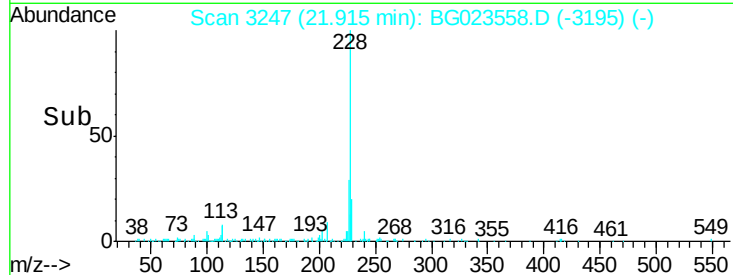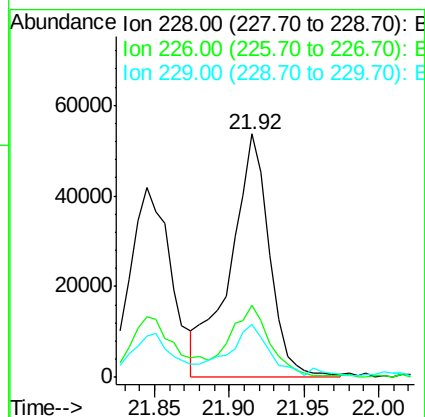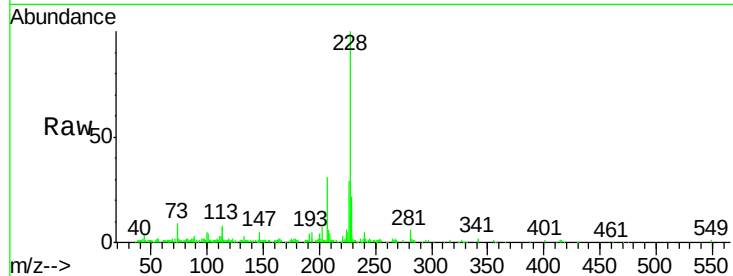

#85
Benzo(b)fluoranthene
 Concen: 1.80 ng/ul m
 RT: 24.19 min Scan# 3634
 Delta R.T. 0.03 min
 Lab File: BG023558.D
 Acq: 9 Aug 2016 16:09

Tgt Ion:	252	Resp:	118470
Ion Ratio	Lower	Upper	
252	100		
253	18.7	18.2	27.2
125	6.2	10.8	16.2#

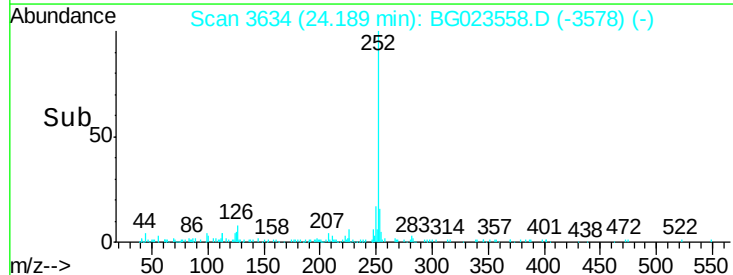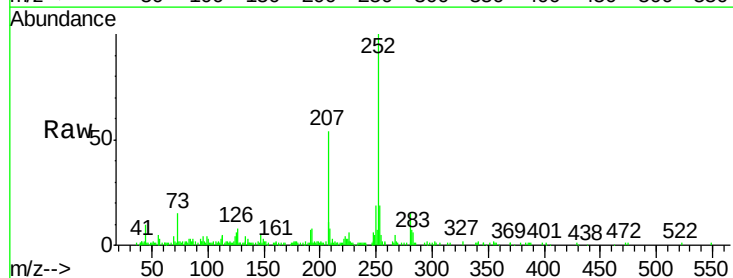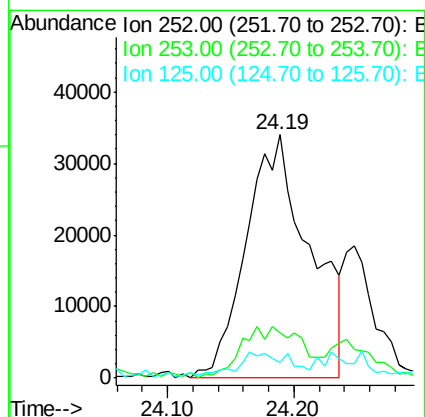

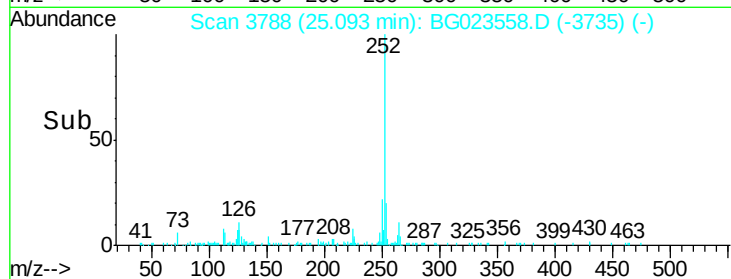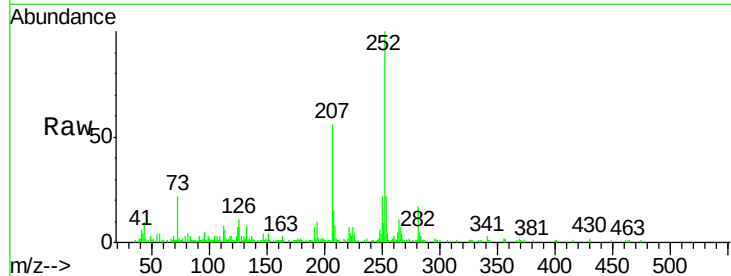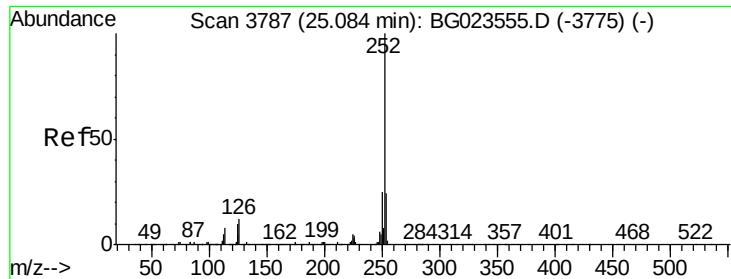

#88

Benzo(a)pyrene

Concen: 1.32 ng/ul

RT: 25.09 min Scan# 3788

Delta R.T. 0.01 min

Lab File: BG023558.D

Acq: 9 Aug 2016 16:09

Instrument :

BNA_G

ClientSampleId :

PR001-SS005-0002-01MS

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.0	19.0	28.4
125	6.7	12.0	18.0

Manual Integrations
APPROVED

sohil
8/10/2016 6:49:27 PM

