

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080916\
 Data File : BG023573.D
 Acq On : 10 Aug 2016 1:36
 Operator : UM/SJ
 Sample : H4392-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.710	145	148	151	rBV3	6933	10003	0.12%	0.019%
2	4.245	235	239	242	rBV4	8255	14909	0.18%	0.028%
3	4.527	283	287	290	rVB5	7090	10304	0.13%	0.020%
4	4.644	304	307	309	rVB5	7907	8962	0.11%	0.017%
5	5.367	425	430	432	rBV5	8947	13214	0.16%	0.025%
6	6.089	551	553	558	rVB5	12523	17248	0.21%	0.033%
7	6.988	701	706	709	rBV4	6079	11944	0.15%	0.023%
8	7.264	748	753	760	rBV	119063	207480	2.56%	0.394%
9	7.423	774	780	791	rVB	409734	703619	8.69%	1.336%
10	7.640	808	817	826	rBV	404482	717311	8.86%	1.362%
11	8.110	889	897	907	rBV	507704	899299	11.11%	1.708%
12	8.774	1005	1010	1013	rBV6	4721	9014	0.11%	0.017%
13	8.827	1013	1019	1032	rVV	335308	612512	7.57%	1.163%
14	9.285	1091	1097	1106	rBV	524829	955543	11.80%	1.815%
15	9.549	1141	1142	1147	rBV4	6174	10922	0.13%	0.021%
16	9.796	1181	1184	1189	rVB5	6007	8624	0.11%	0.016%
17	10.019	1215	1222	1231	rBV	462388	831266	10.27%	1.579%
18	10.471	1297	1299	1305	rBV5	6131	11102	0.14%	0.021%
19	10.565	1307	1315	1329	rVV	561101	1179484	14.57%	2.240%
20	10.947	1371	1380	1391	rVV	802683	1470452	18.16%	2.793%
21	11.094	1402	1405	1410	rBV5	9421	18281	0.23%	0.035%
22	11.617	1486	1494	1501	rBV4	21726	42848	0.53%	0.081%
23	12.339	1612	1617	1622	rVB6	5022	10402	0.13%	0.020%
24	12.422	1626	1631	1633	rBV4	11881	16713	0.21%	0.032%
25	12.545	1646	1652	1654	rBV5	10008	16698	0.21%	0.032%
26	13.297	1776	1780	1782	rBV4	7911	12308	0.15%	0.023%
27	13.650	1834	1840	1845	rVV7	11818	24689	0.30%	0.047%
28	14.178	1923	1930	1936	rBV	1536819	2306561	28.49%	4.381%
29	14.478	1973	1981	1990	rBV	1580951	2594085	32.04%	4.927%
30	14.766	2020	2030	2043	rBV2	4635719	8096473	100.00%	15.378%
31	15.018	2066	2073	2091	rBV4	79404	252473	3.12%	0.480%
32	15.130	2091	2092	2098	rVB5	6310	9435	0.12%	0.018%
33	15.300	2119	2121	2127	rVB6	5434	8115	0.10%	0.015%
34	15.559	2162	2165	2170	rVV5	9432	17999	0.22%	0.034%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080916\
 Data File : BG023573.D
 Acq On : 10 Aug 2016 1:36
 Operator : UM/SJ
 Sample : H4392-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Title : SVOA CALIBRATION

35	15.723	2191	2193	2196	rVV4	9827	12814	0.16%	0.024%
36	15.782	2196	2203	2211	rVB	2267857	3599965	44.46%	6.838%
37	15.899	2217	2223	2233	rBV	791604	1257670	15.53%	2.389%
38	16.023	2238	2244	2250	rVB4	34595	66798	0.83%	0.127%
39	16.510	2323	2327	2331	rBV6	6619	13719	0.17%	0.026%
40	16.728	2363	2364	2369	rVB5	7789	8110	0.10%	0.015%
41	16.980	2403	2407	2411	rVB4	12087	19097	0.24%	0.036%
42	17.121	2428	2431	2439	rVB6	11921	18596	0.23%	0.035%
43	17.327	2462	2466	2472	rVV3	13121	19854	0.25%	0.038%
44	17.421	2479	2482	2485	rBV4	5485	8312	0.10%	0.016%
45	17.485	2489	2493	2497	rVV7	13342	23910	0.30%	0.045%
46	17.544	2497	2503	2511	rVV2	2261500	3457981	42.71%	6.568%
47	17.644	2514	2520	2536	rVB	2619112	4213853	52.05%	8.004%
48	17.914	2564	2566	2568	rBV3	11623	10256	0.13%	0.019%
49	18.049	2583	2589	2590	rBV6	11803	15898	0.20%	0.030%
50	18.102	2595	2598	2599	rBV3	8053	8591	0.11%	0.016%
51	18.202	2610	2615	2621	rBV8	23192	37414	0.46%	0.071%
52	18.320	2632	2635	2640	rVB5	8643	12550	0.16%	0.024%
53	18.396	2642	2648	2651	rBV4	7745	15032	0.19%	0.029%
54	18.455	2654	2658	2661	rVB5	15440	23232	0.29%	0.044%
55	18.637	2684	2689	2697	rBV	92847	167454	2.07%	0.318%
56	18.948	2736	2742	2746	rBV7	19358	39084	0.48%	0.074%
57	19.007	2748	2752	2757	rVV7	15915	33788	0.42%	0.064%
58	19.066	2759	2762	2765	rBV5	9437	12675	0.16%	0.024%
59	19.160	2772	2778	2780	rBV6	7586	14546	0.18%	0.028%
60	19.201	2782	2785	2787	rBV4	13721	16487	0.20%	0.031%
61	19.289	2796	2800	2803	rBV5	19674	29488	0.36%	0.056%
62	19.571	2841	2848	2853	rBV2	35847	65323	0.81%	0.124%
63	19.688	2865	2868	2870	rVV3	14144	16167	0.20%	0.031%
64	19.741	2874	2877	2880	rBV4	8471	13525	0.17%	0.026%
65	19.794	2882	2886	2888	rVV5	6678	10544	0.13%	0.020%
66	19.829	2888	2892	2896	rVB2	38636	51009	0.63%	0.097%
67	19.941	2904	2911	2922	rBV	3242262	4841377	59.80%	9.196%
68	20.158	2946	2948	2952	rVB5	14942	14314	0.18%	0.027%
69	20.288	2966	2970	2973	rBV6	11283	18992	0.23%	0.036%
70	20.346	2979	2980	2983	rBV3	9483	10536	0.13%	0.020%
71	20.810	3057	3059	3061	rBV3	9498	9262	0.11%	0.018%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080916\
 Data File : BG023573.D
 Acq On : 10 Aug 2016 1:36
 Operator : UM/SJ
 Sample : H4392-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Title : SVOA CALIBRATION

72	20.992	3088	3090	3093	rVB4	16018	11722	0.14%	0.022%
73	21.533	3180	3182	3184	rBV3	12190	10030	0.12%	0.019%
74	21.721	3211	3214	3218	rVB5	28823	44645	0.55%	0.085%
75	21.780	3218	3224	3229	rBV5	59211	104313	1.29%	0.198%
76	21.868	3232	3239	3248	rVB	2285292	3853227	47.59%	7.319%
77	22.026	3264	3266	3268	rBV4	16435	18287	0.23%	0.035%
78	22.673	3374	3376	3380	rVB5	21519	19793	0.24%	0.038%
79	23.131	3452	3454	3455	rBV	14246	9044	0.11%	0.017%
80	23.730	3554	3556	3558	rBV3	11420	10578	0.13%	0.020%
81	24.247	3640	3644	3654	rVB4	77919	177655	2.19%	0.337%
82	25.028	3764	3777	3793	rBV2	1410736	4273652	52.78%	8.117%
83	25.263	3805	3817	3829	rBV2	1232920	3777603	46.66%	7.175%
84	25.422	3842	3844	3845	rBV2	14594	12361	0.15%	0.023%
85	25.698	3889	3891	3899	rBV9	14131	22646	0.28%	0.043%
86	26.450	4011	4019	4031	rVB5	99198	321186	3.97%	0.610%
87	27.813	4249	4251	4252	rBV2	16530	11269	0.14%	0.021%
88	27.877	4252	4262	4273	rVB4	106549	377577	4.66%	0.717%
89	29.551	4545	4547	4548	rBV2	16892	11450	0.14%	0.022%
90	29.593	4550	4554	4566	rVB7	64984	222255	2.75%	0.422%
91	31.625	4898	4900	4901	rBV2	14504	12396	0.15%	0.024%
92	31.890	4943	4945	4946	rBV2	12102	9115	0.11%	0.017%


Sum of corrected areas: 52649319

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080916\
Data File : BG023573.D
Acq On : 10 Aug 2016 1:36
Operator : UM/SJ
Sample : H4392-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDJW3

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

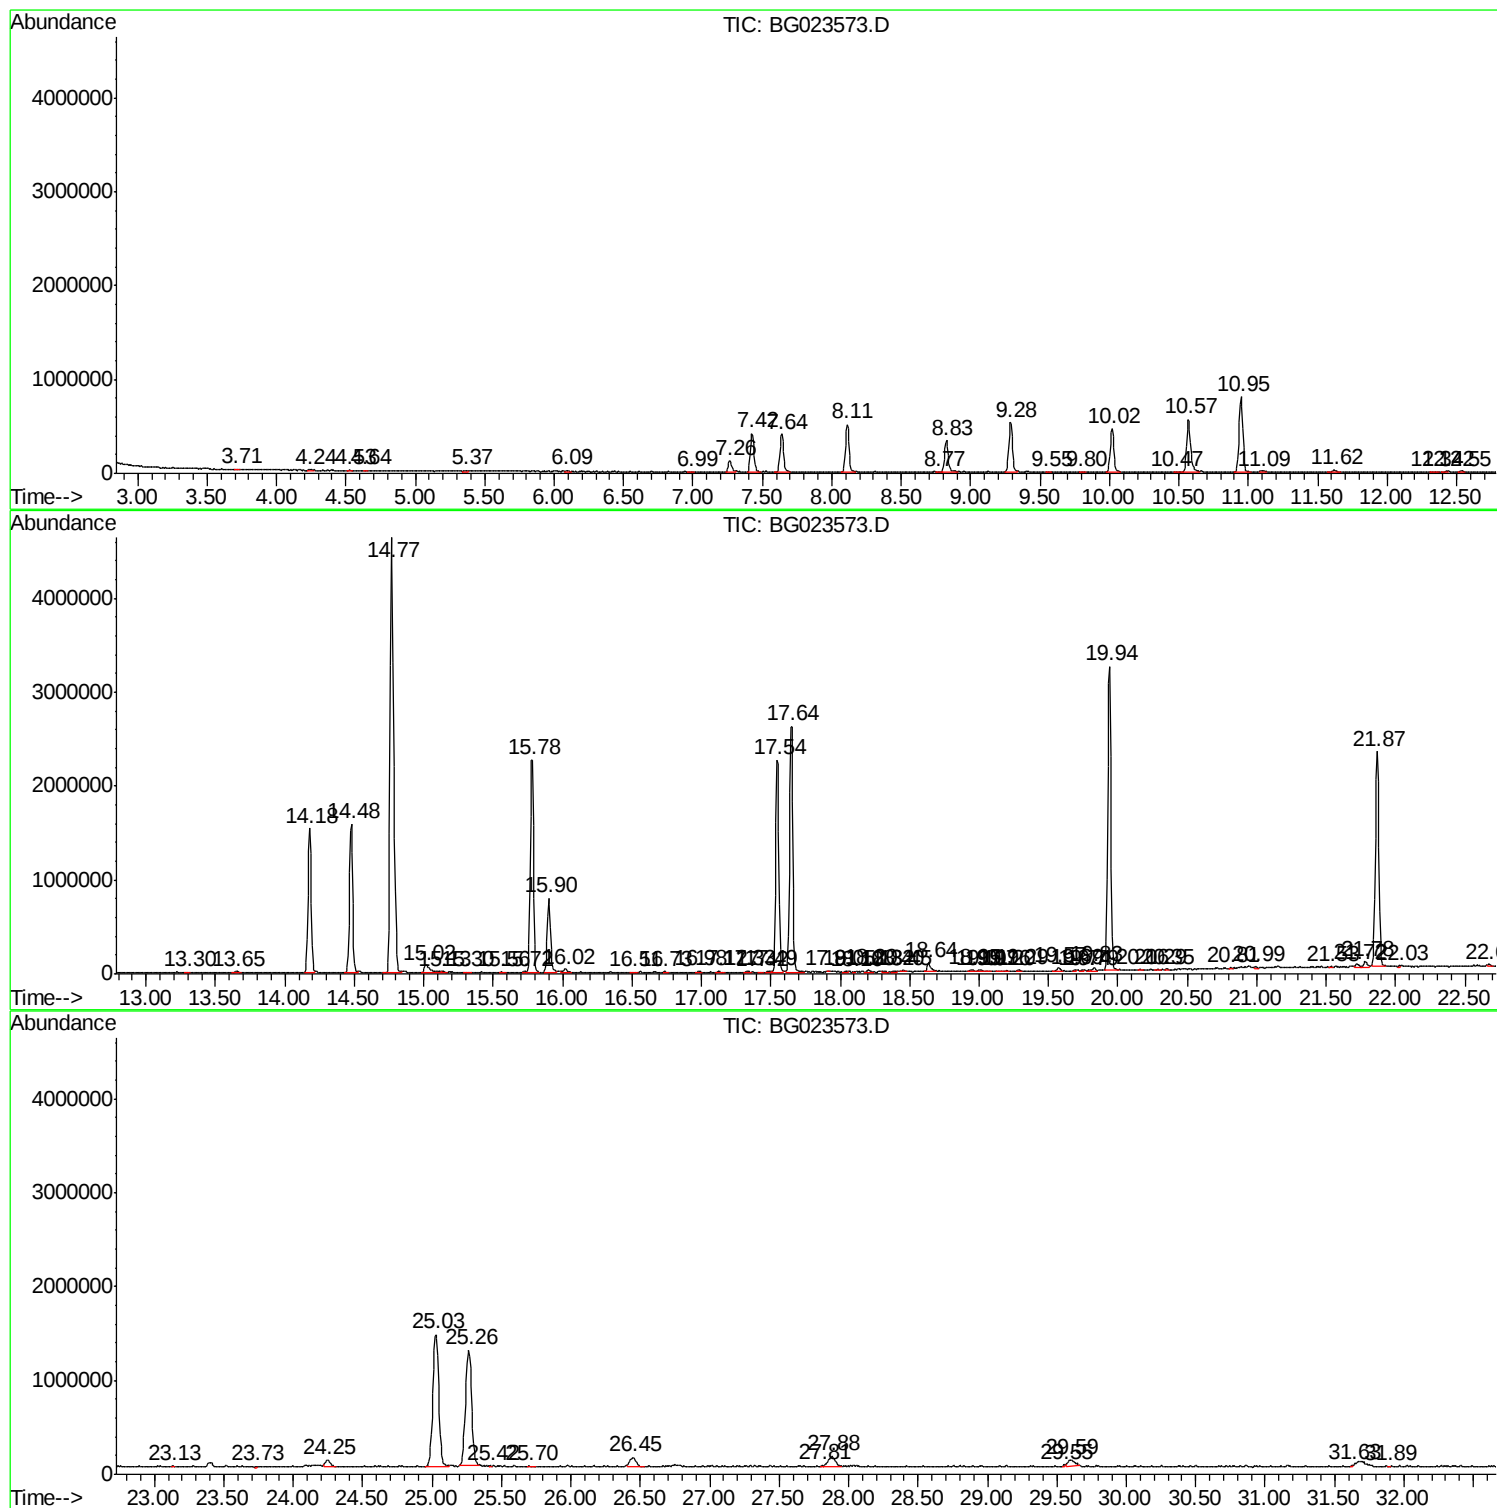

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080916\
Data File : BG023573.D
Acq On : 10 Aug 2016 1:36
Operator : UM/SJ
Sample : H4392-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDJW3

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080916\
Data File : BG023573.D
Acq On : 10 Aug 2016 1:36
Operator : UM/SJ
Sample : H4392-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDJW3

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc