

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080917\
 Data File : BG028221.D
 Acq On : 9 Aug 2017 11:54
 Operator : SJ/JU
 Sample : PB101334BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK34

Quant Time: Aug 10 02:05:57 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 10 01:59:02 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	29180	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	136251	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	107996	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.71	188	322132	20.00	ng/ul	0.00
75) Chrysene-d12	22.04	240	356622	20.00	ng/ul	0.00
83) Perylene-d12	25.54	264	339380	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.84	96	4697	7.50	ng/uL	0.00
5) Phenol-d5	7.50	99	93570	29.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.67	67	66571	32.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.89	132	67918	33.59	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	76219	28.46	ng/ul	0.00
19) Nitrobenzene-d5	9.52	128	36263	34.04	ng/ul	0.00
22) 2-Nitrophenol-d4	10.25	143	43771	37.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	76715	31.74	ng/ul	0.00
29) 4-Chloroaniline-d4	11.30	131	106944	39.75	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	365996	38.10	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	369361	34.11	ng/ul	0.00
51) 4-Nitrophenol-d4	15.14	143	52170	34.16	ng/ul	0.00
57) Fluorene-d10	15.95	176	299522	34.76	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	70488	33.68	ng/ul	0.00
70) Anthracene-d10	17.81	188	571048	36.97	ng/ul	0.00
76) Pyrene-d10	20.08	212	653939	35.76	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.30	264	580462	36.53	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	9.05	70	2368	1.091	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080917\
Data File : BG028221.D
Acq On : 9 Aug 2017 11:54
Operator : SJ/JU
Sample : PB101334BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK34

Quant Time: Aug 10 02:05:57 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 10 01:59:02 2017
Response via : Initial Calibration

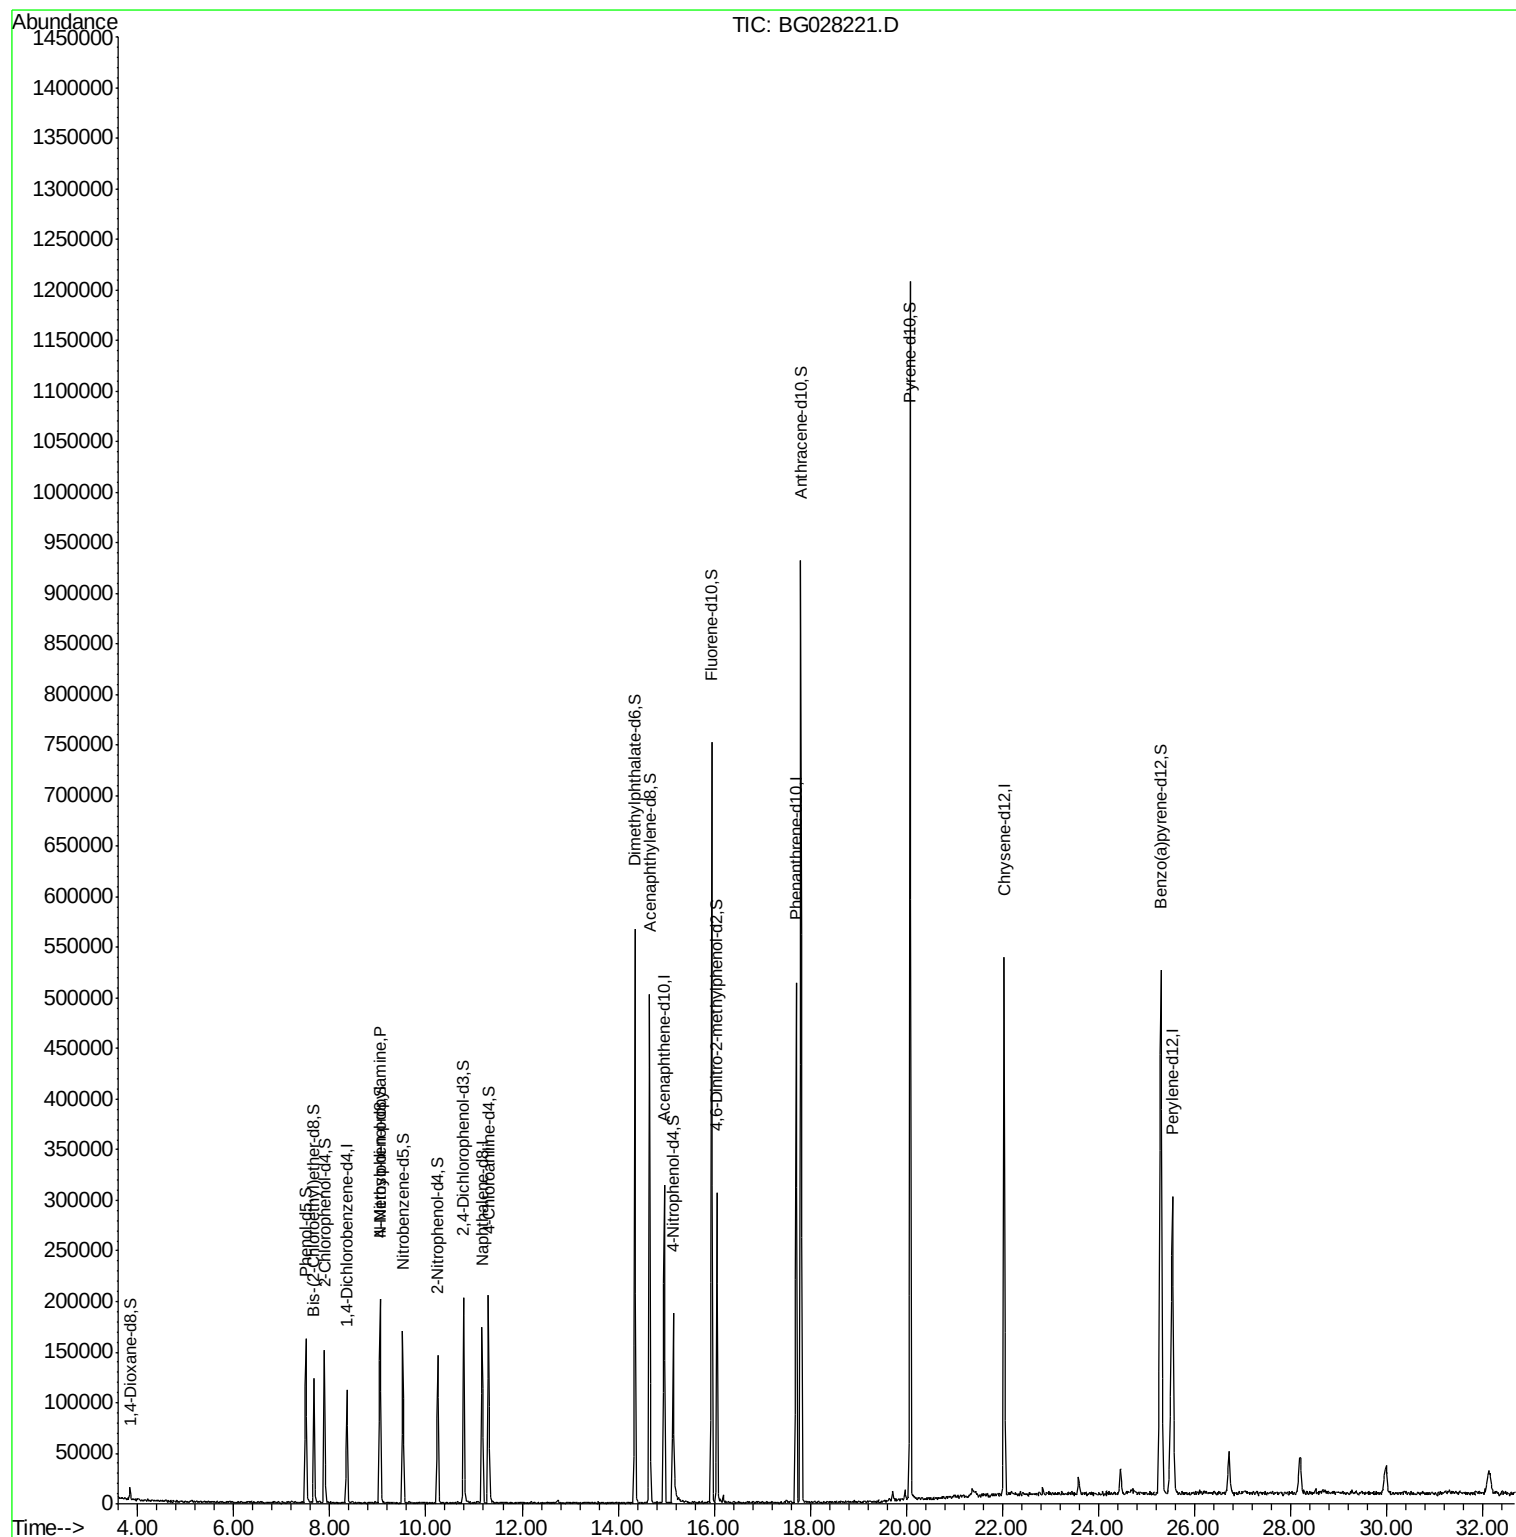

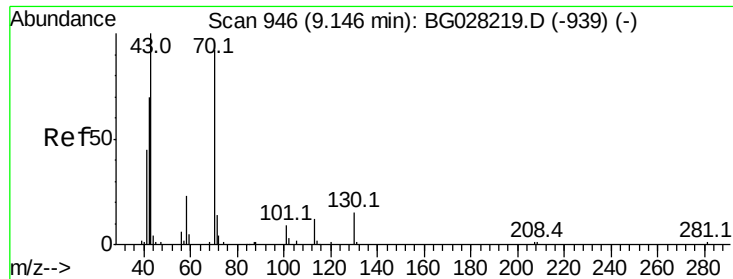

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.091 ng/ul
 RT: 9.05 min Scan# 929
 Delta R.T. -0.10 min
 Lab File: BG028221.D
 Acq: 9 Aug 2017 11:54

Instrument :
 BNA_G
 ClientSampleId :
 SBLK34

Tot Ion: 70 Resp: 2368
 Ion Ratio Lower Upper
 70 100
 42 309.6 59.0 88.6#
 101 0.0 6.6 9.8#
 130 0.0 15.6 23.4#

