
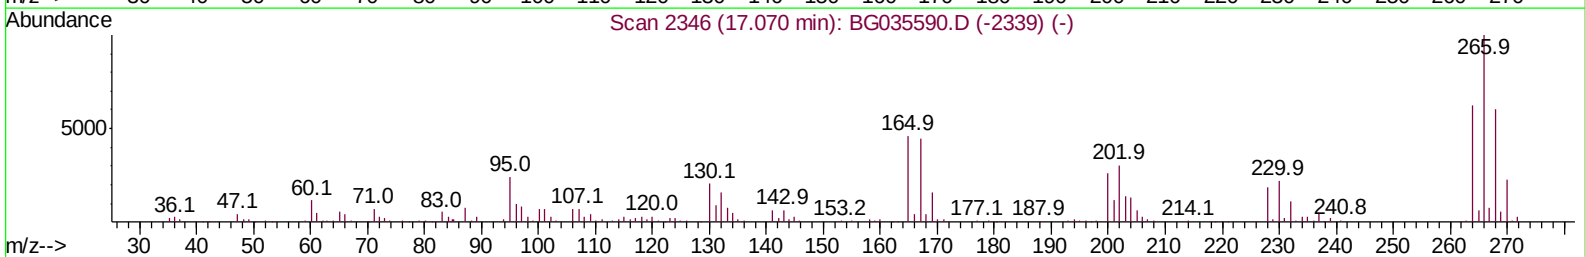
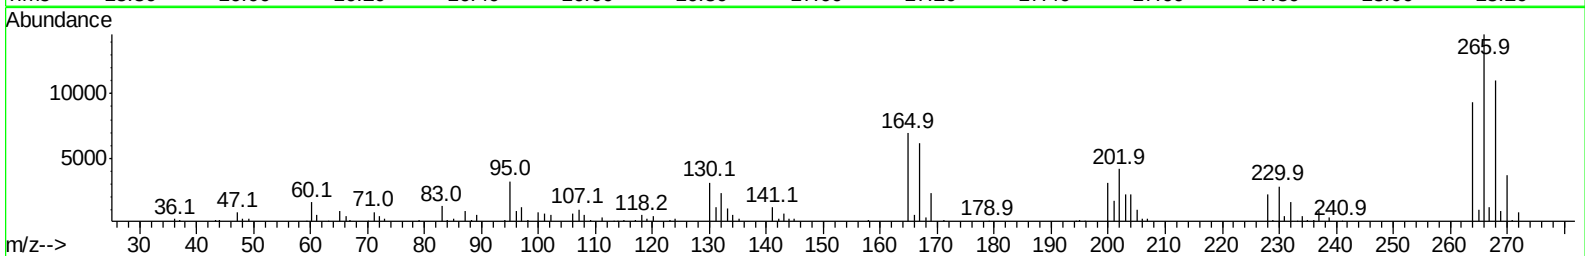


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080918\
Data File : BG036233.D
Acq On : 9 Aug 2018 15:01
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:39:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

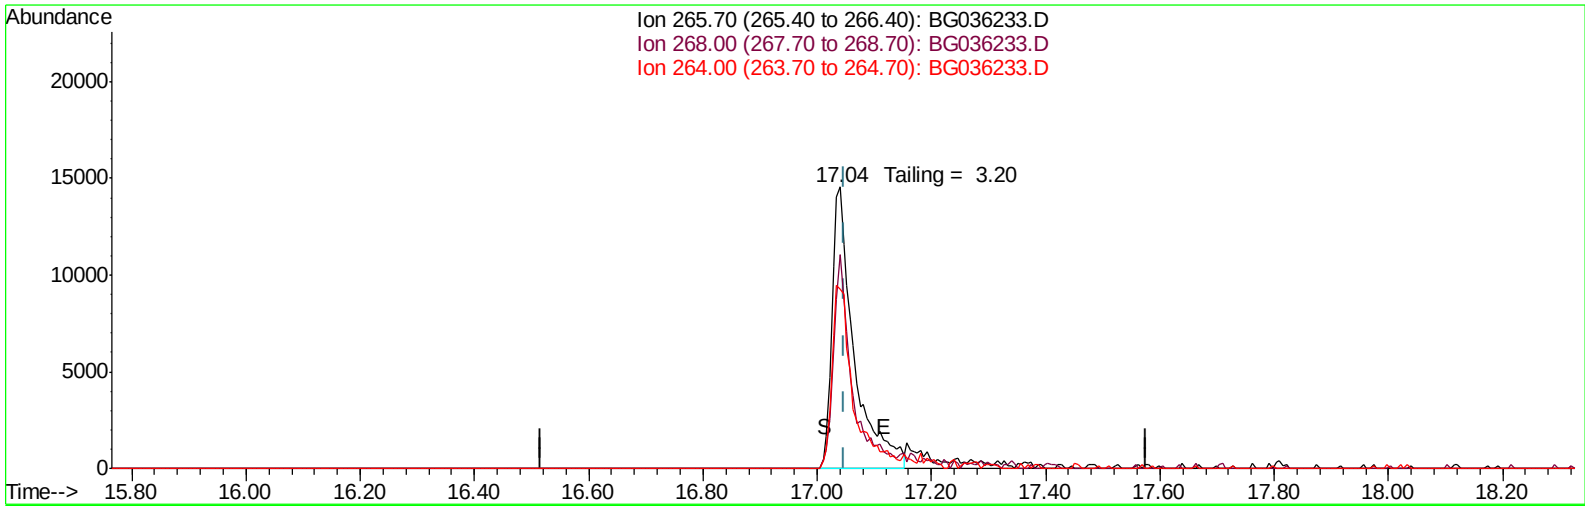

TIC: BG036233.D

(69) Pentachlorophenol (C)




17.040min (-0.008) 87639.73ng

response 38904

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	75.81
264.00	62.00	63.79
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080918\
Data File : BG036233.D
Acq On : 9 Aug 2018 15:01
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:39:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

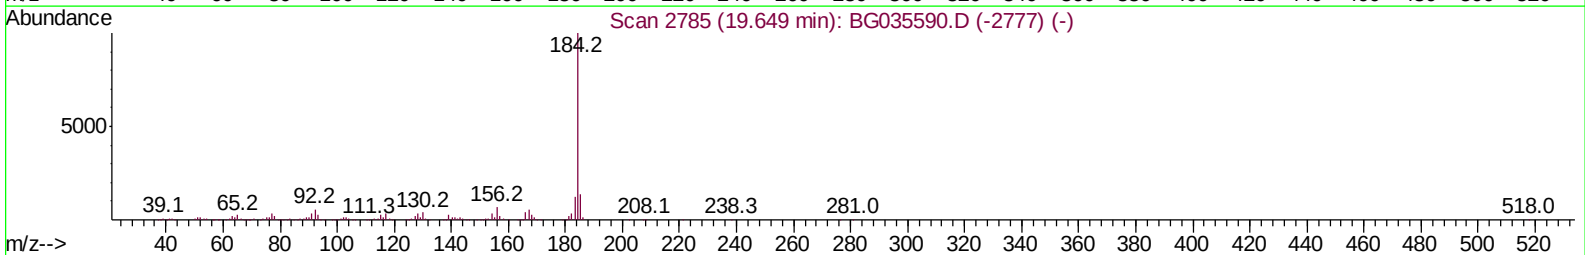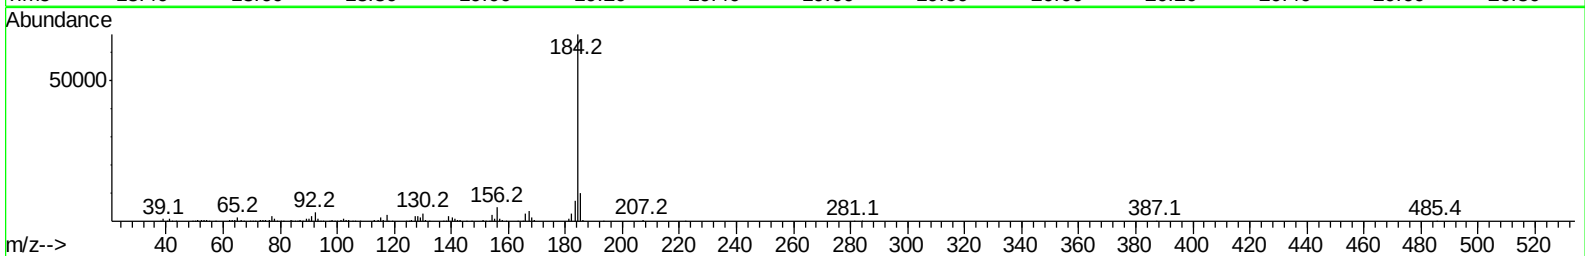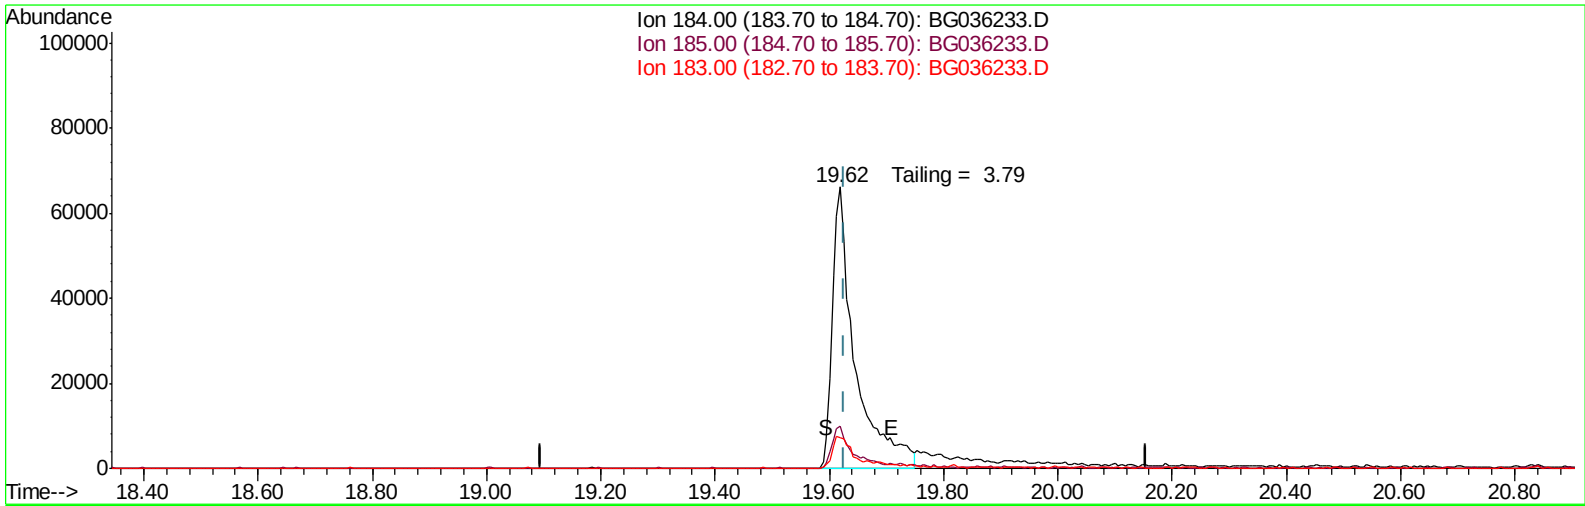

TIC: BG036233.D

(76) Benzidine

19.619min (-0.008) 87396.77ng

response 181517

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.15
183.00	13.30	11.14
0.00	0.00	0.00