
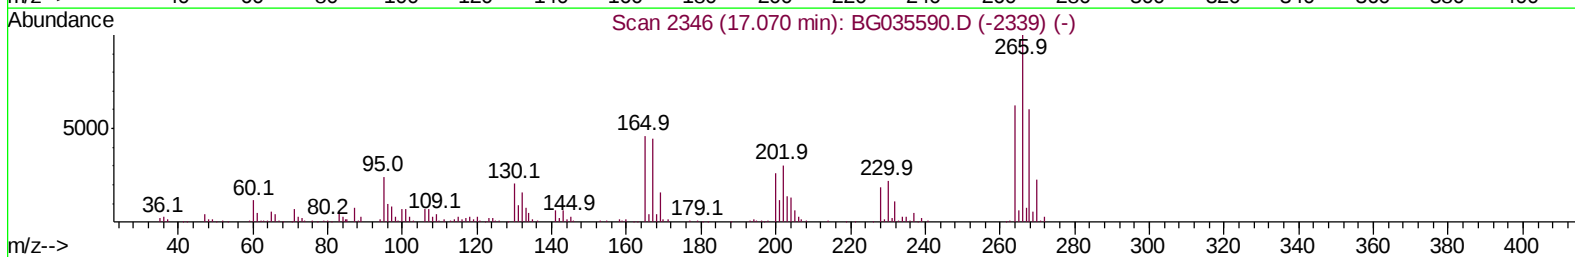
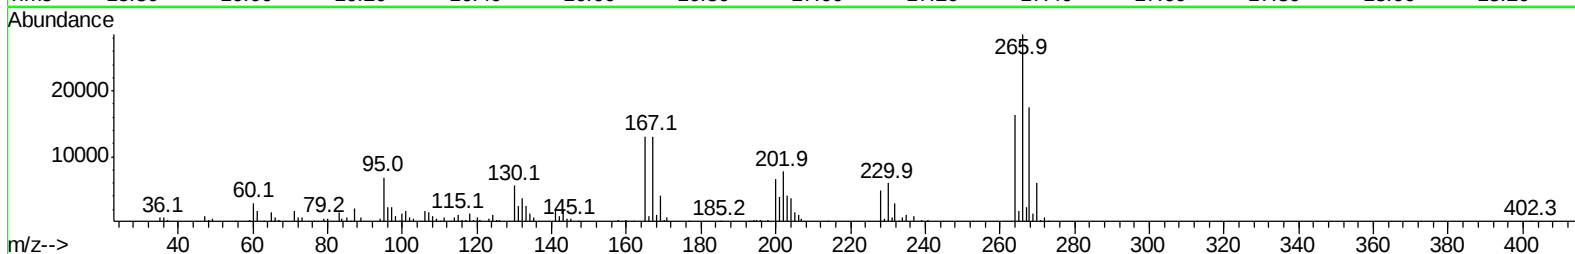


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080918\
Data File : BG036252.D
Acq On : 10 Aug 2018 4:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:49:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

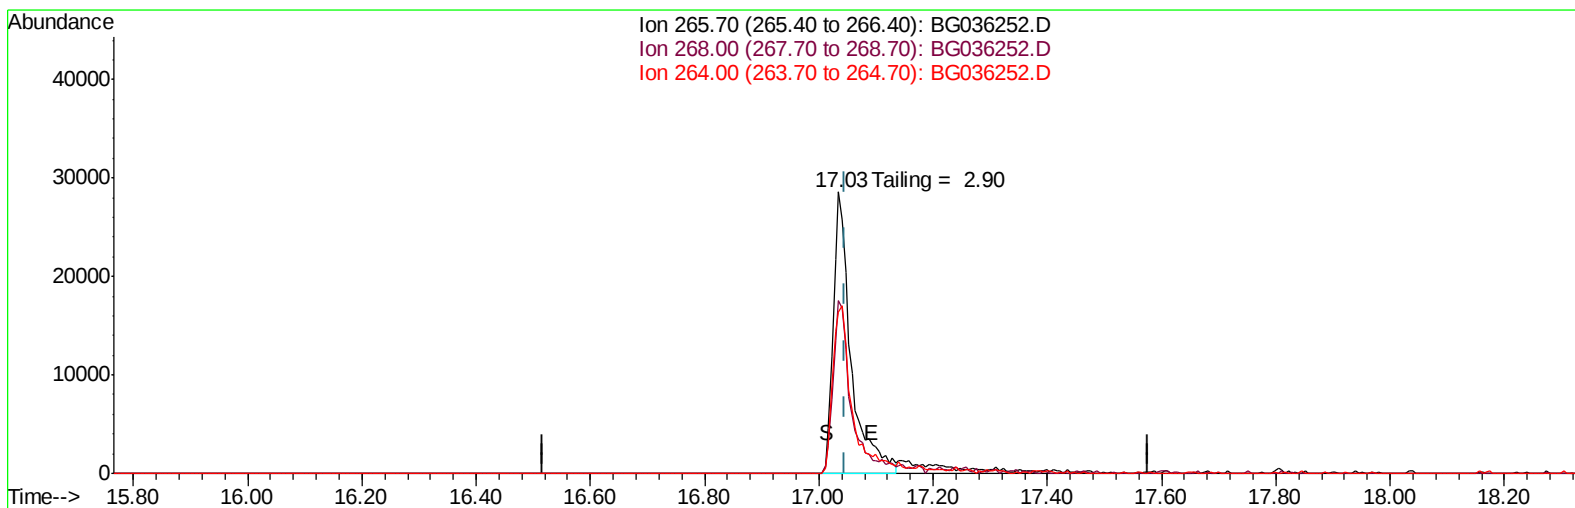

TIC: BG036252.D

(69) Pentachlorophenol (C)




17.035min (-0.013) 43107.89ng

response 61486

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.45
264.00	62.00	57.10
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080918\
 Data File : BG036252.D
 Acq On : 10 Aug 2018 4:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:49:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 31 12:30:06 2018
 Response via : Initial Calibration

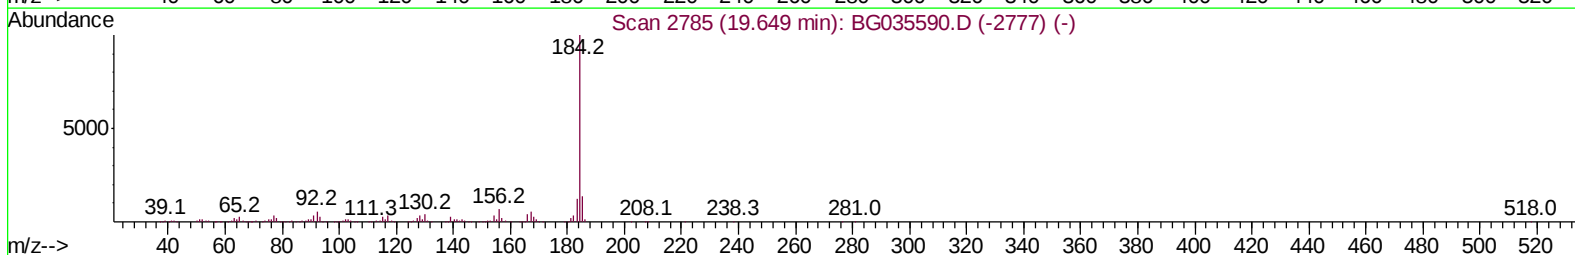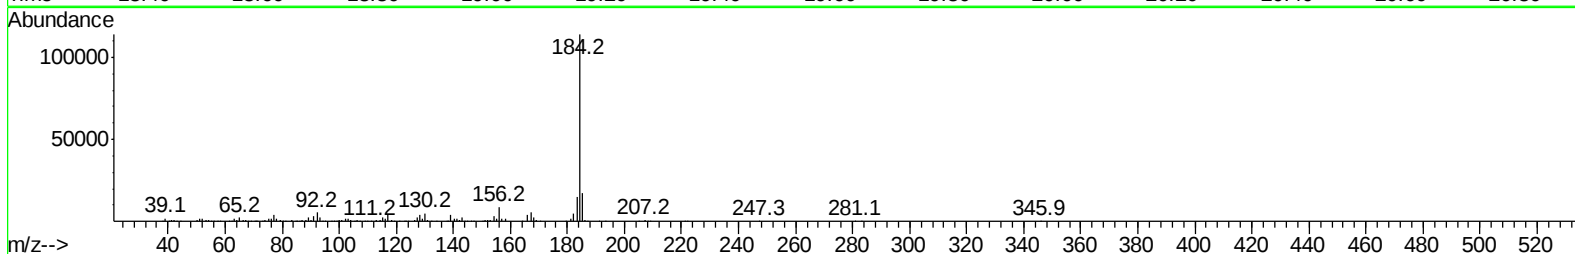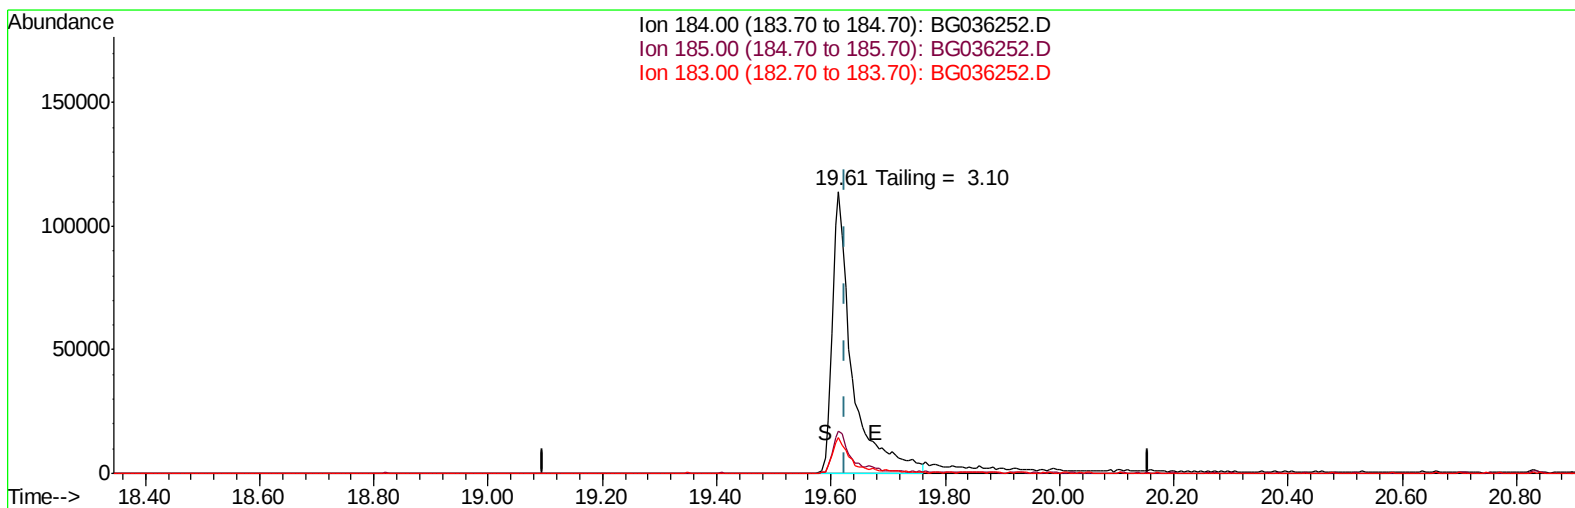

TIC: BG036252.D

(76) Benzidine

19.613min (-0.013) 52964.75ng

response 274314

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.97
183.00	13.30	12.89
0.00	0.00	0.00