


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080918\
 Data File : BG036233.D
 Acq On : 9 Aug 2018 15:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

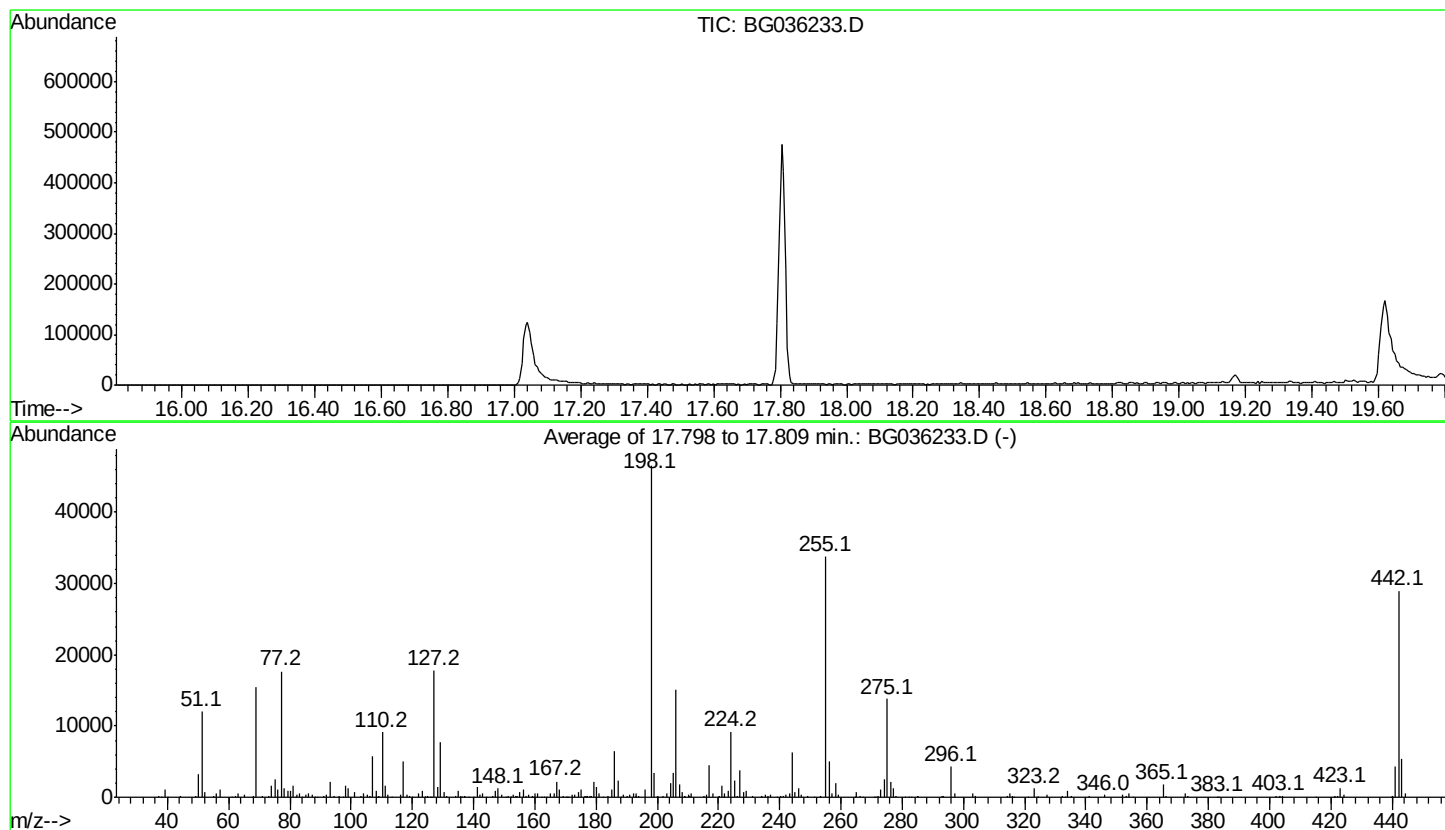

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	11960	PASS
68	69	0.00	2	1.3	209	PASS
69	198	0.00	100	33.4	15551	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.1	17731	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46562	PASS
199	198	5	9	7.3	3384	PASS
275	198	10	60	29.7	13827	PASS
365	198	1	100	3.8	1781	PASS
441	198	0.01	100	9.5	4407	PASS
442	198	50	100	62.3	29026	PASS
443	442	15	24	18.9	5475	PASS