


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080918\
 Data File : BG036252.D
 Acq On : 10 Aug 2018 4:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

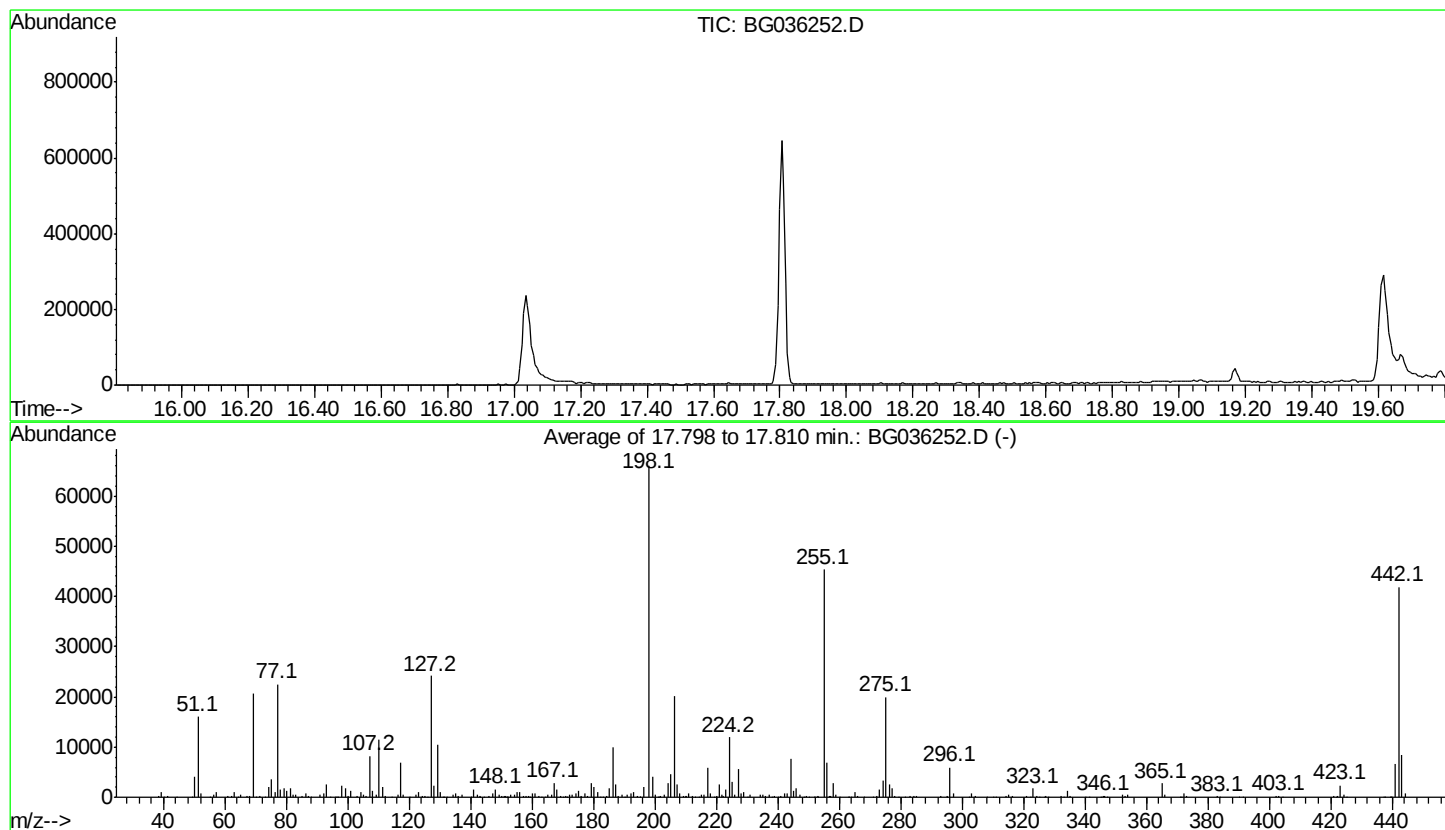

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	16006	PASS
68	69	0.00	2	1.5	315	PASS
69	198	0.00	100	31.3	20680	PASS
70	69	0.00	2	0.6	125	PASS
127	198	10	80	36.7	24224	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66064	PASS
199	198	5	9	6.4	4203	PASS
275	198	10	60	30.2	19942	PASS
365	198	1	100	4.1	2710	PASS
441	198	0.01	100	9.9	6565	PASS
442	198	50	100	63.4	41901	PASS
443	442	15	24	20.1	8418	PASS