
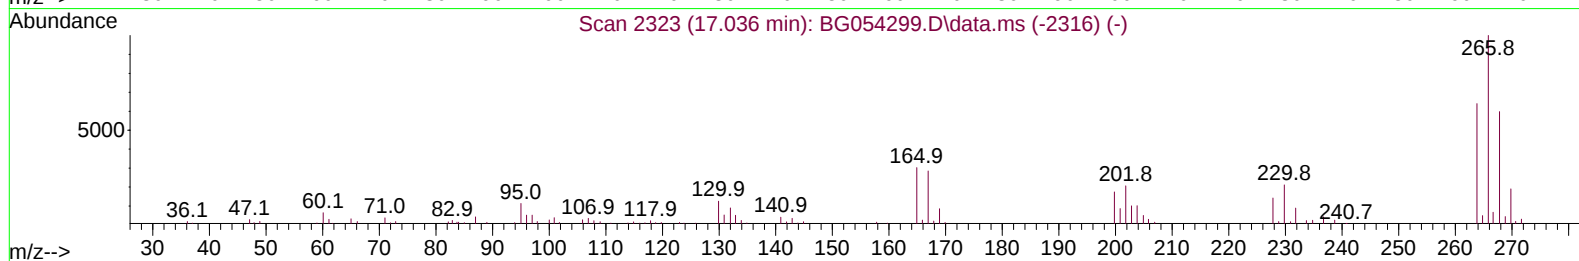
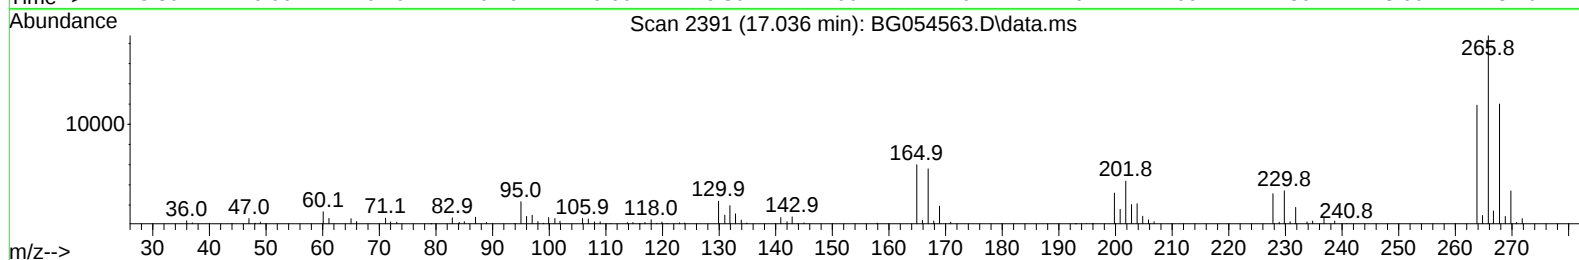


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080922\
Data File : BG054563.D
Acq On : 9 Aug 2022 9:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 09 17:08:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

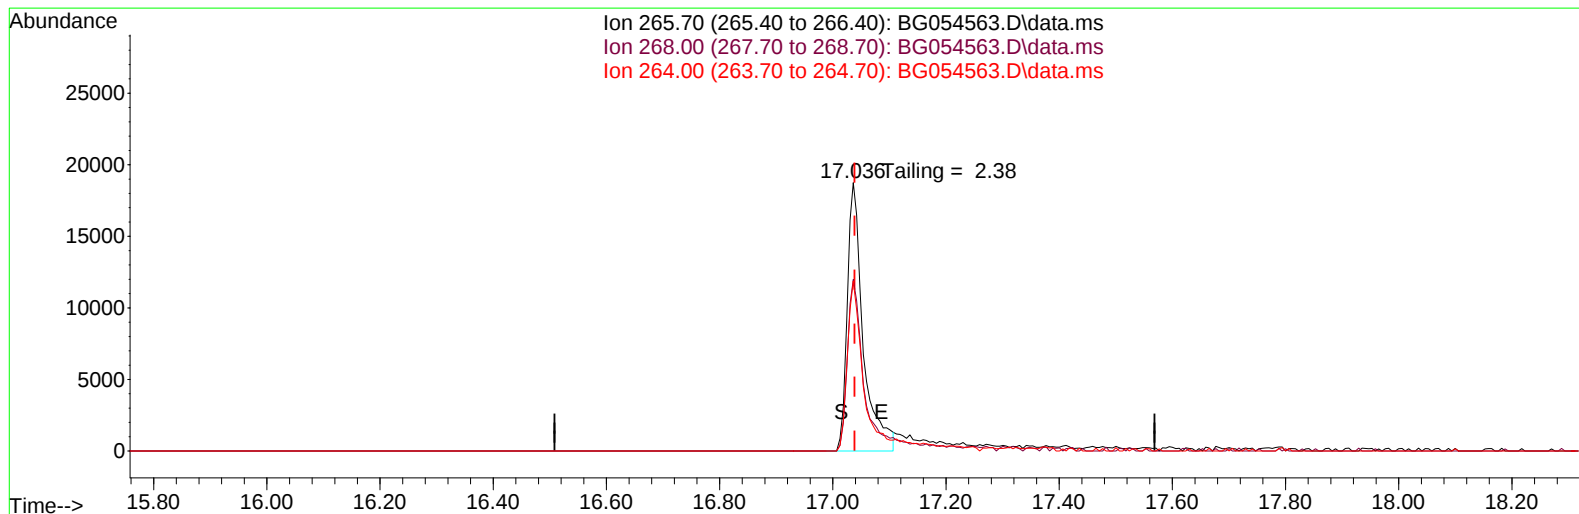

TIC: BG054563.D\data.ms

(70) Pentachlorophenol (C)

17.036min (-0.002) 19617.09 ng




response 39438

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.92
264.00	66.20	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080922\
 Data File : BG054563.D
 Acq On : 9 Aug 2022 9:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 09 17:08:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 14:48:51 2022
 Response via : Initial Calibration

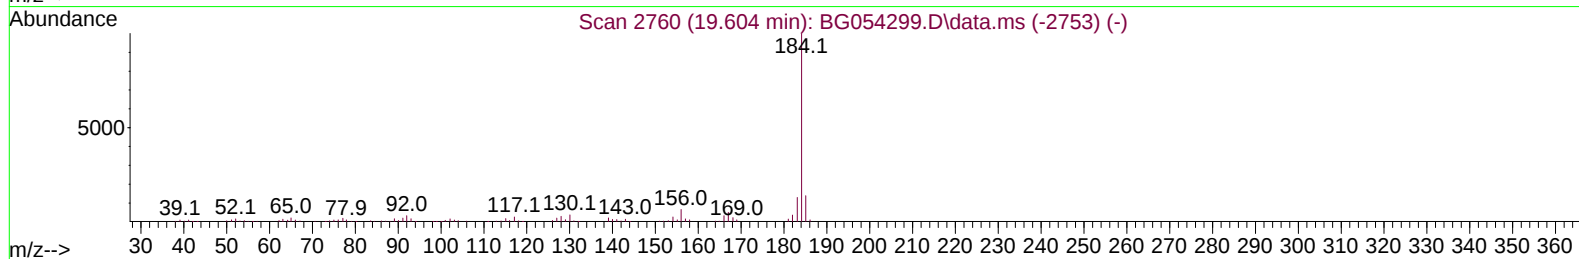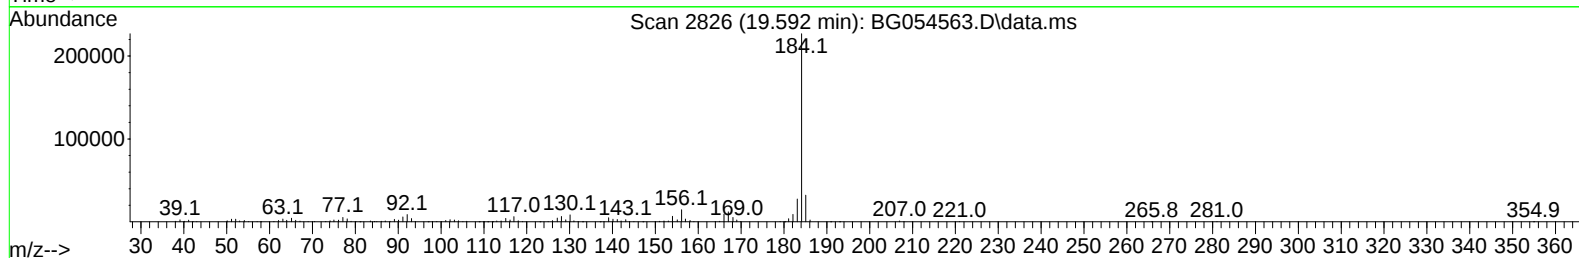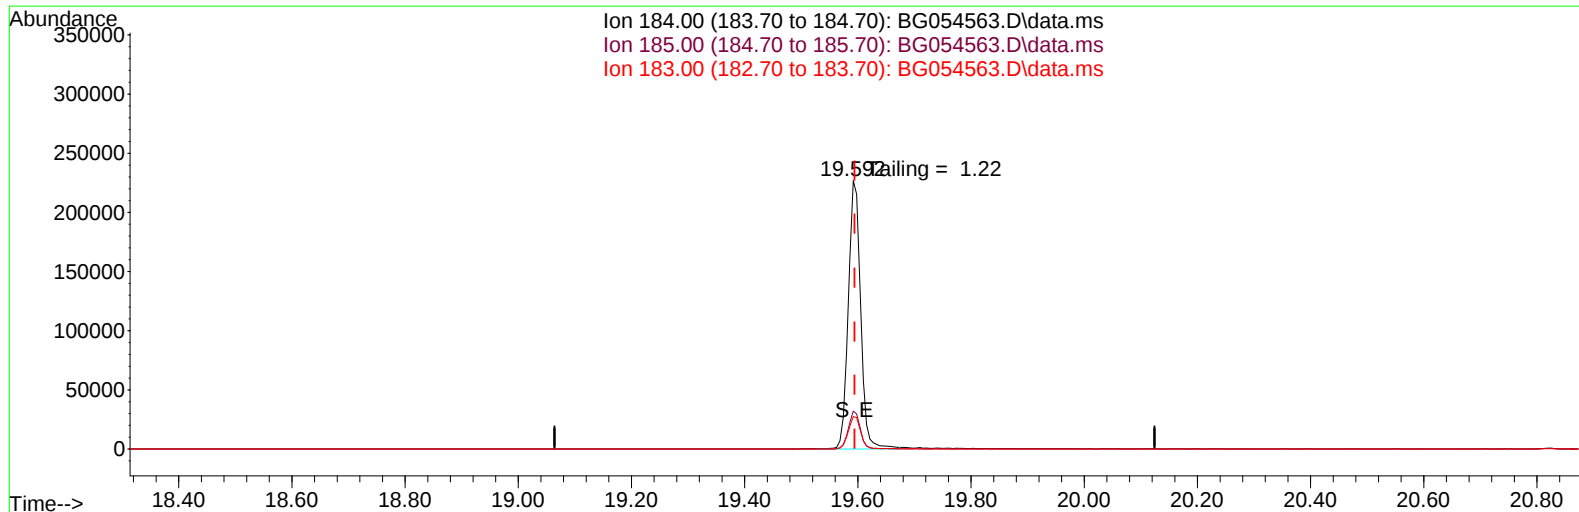

TIC: BG054563.D\data.ms

(77) Benzidine

19.592min (-0.002) 0.00 ng

response 344746


Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.15
183.00	11.10	12.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080922\
Data File : BG054563.D
Acq On : 9 Aug 2022 9:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 08 14:48:51 2022

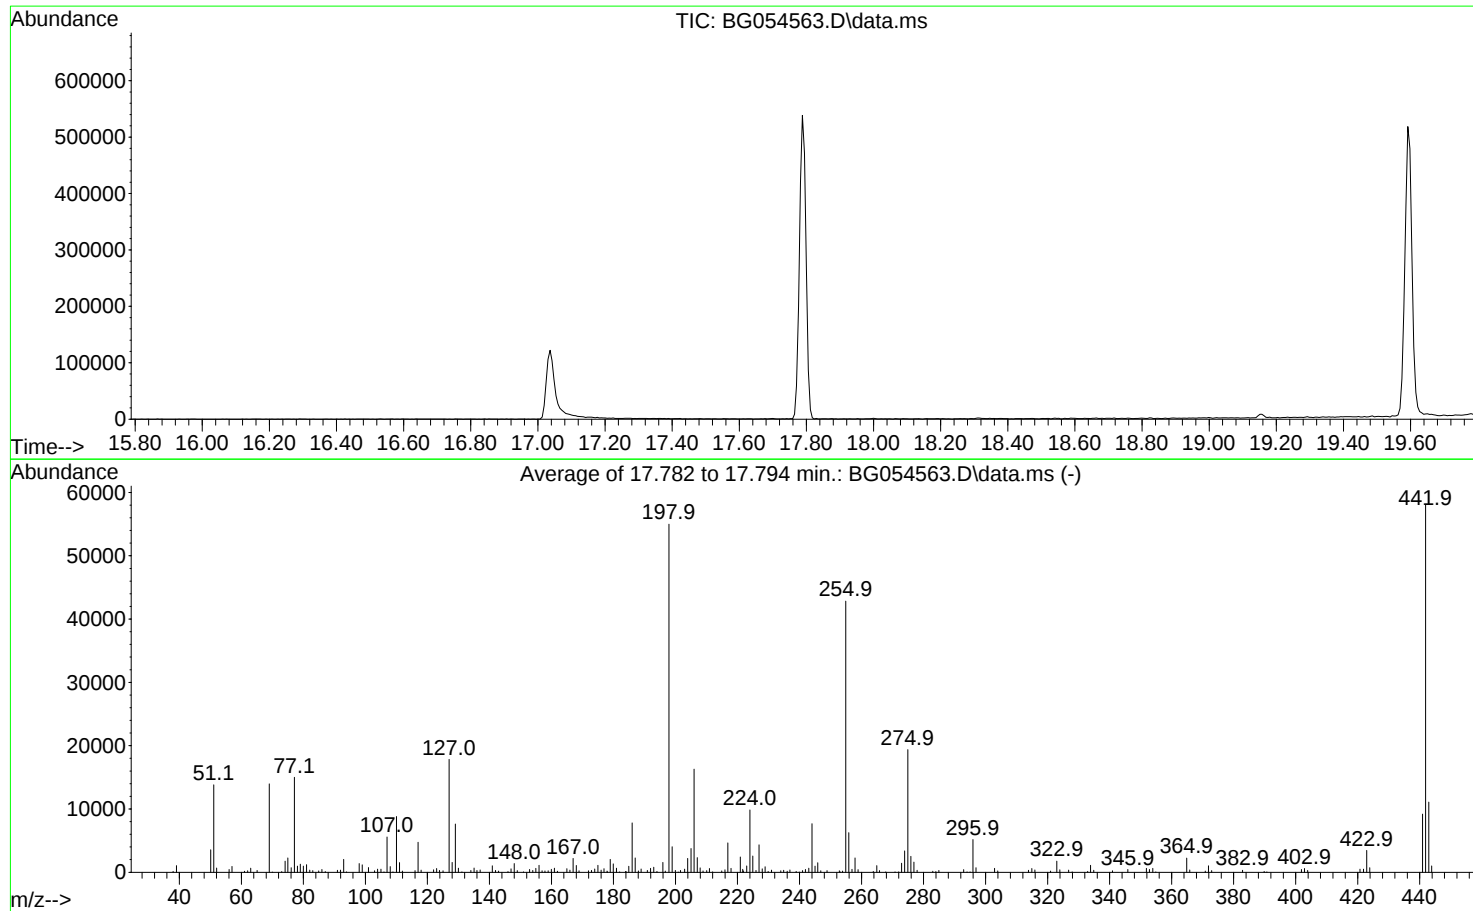

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	13816	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	25.4	13974	PASS
70	69	0.00	2	0.4	50	PASS
127	198	10	80	32.4	17840	PASS
197	198	0.00	2	0.4	201	PASS
198	198	100	100	100.0	54984	PASS
199	198	5	9	7.3	4023	PASS
275	198	10	60	35.2	19376	PASS
365	198	1	100	4.1	2237	PASS
441	198	0.01	100	16.7	9185	PASS
442	442	50	100	100.0	58112	PASS
443	442	15	24	19.1	11080	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2022	BNA_G	BG054563.D
Compound Name	Response	Retention Time
DDT	191931	20.82
DDD	9331	20.38
DDE	369	19.87
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9700	201631	4.81

Instrument :
BNA_G
ClientSampleId :
DFTPP