

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081015\
 Data File : BG018361.D
 Acq On : 10 Aug 2015 19:39
 Operator : UM/MA
 Sample : G3154-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01Z2

Quant Time: Aug 11 01:42:45 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 11 01:39:57 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	90142	20.00	ng/ul	0.00
18) Naphthalene-d8	10.83	136	433550	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.65	164	294620	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.40	188	748734	20.00	ng/ul	0.00
78) Chrysene-d12	21.66	240	733864	20.00	ng/ul	0.00
86) Perylene-d12	24.88	264	717892	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	9405	4.61	ng/uL	0.00
5) Phenol-d5	7.19	99	205815	25.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	134715	26.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.56	132	157437	25.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	181065	26.34	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	81502	24.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.91	143	85692	24.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.45	165	175023	23.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.96	131	220320	26.69	ng/ul	0.00
44) Dimethylphthalate-d6	14.06	166	632569	25.52	ng/ul	0.00
47) Acenaphthylene-d8	14.35	160	721364	23.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	113897	25.54	ng/ul	0.00
58) Fluorene-d10	15.65	176	526044	24.36	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.75	200	67342	18.29	ng/ul	0.00
71) Anthracene-d10	17.50	188	874179	24.41	ng/ul	0.00
79) Pyrene-d10	19.78	212	911558	23.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.65	264	914891	24.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.11	163	141867	5.80	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081015\
Data File : BG018361.D
Acq On : 10 Aug 2015 19:39
Operator : UM/MA
Sample : G3154-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01Z2

Quant Time: Aug 11 01:42:45 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 11 01:39:57 2015
Response via : Initial Calibration

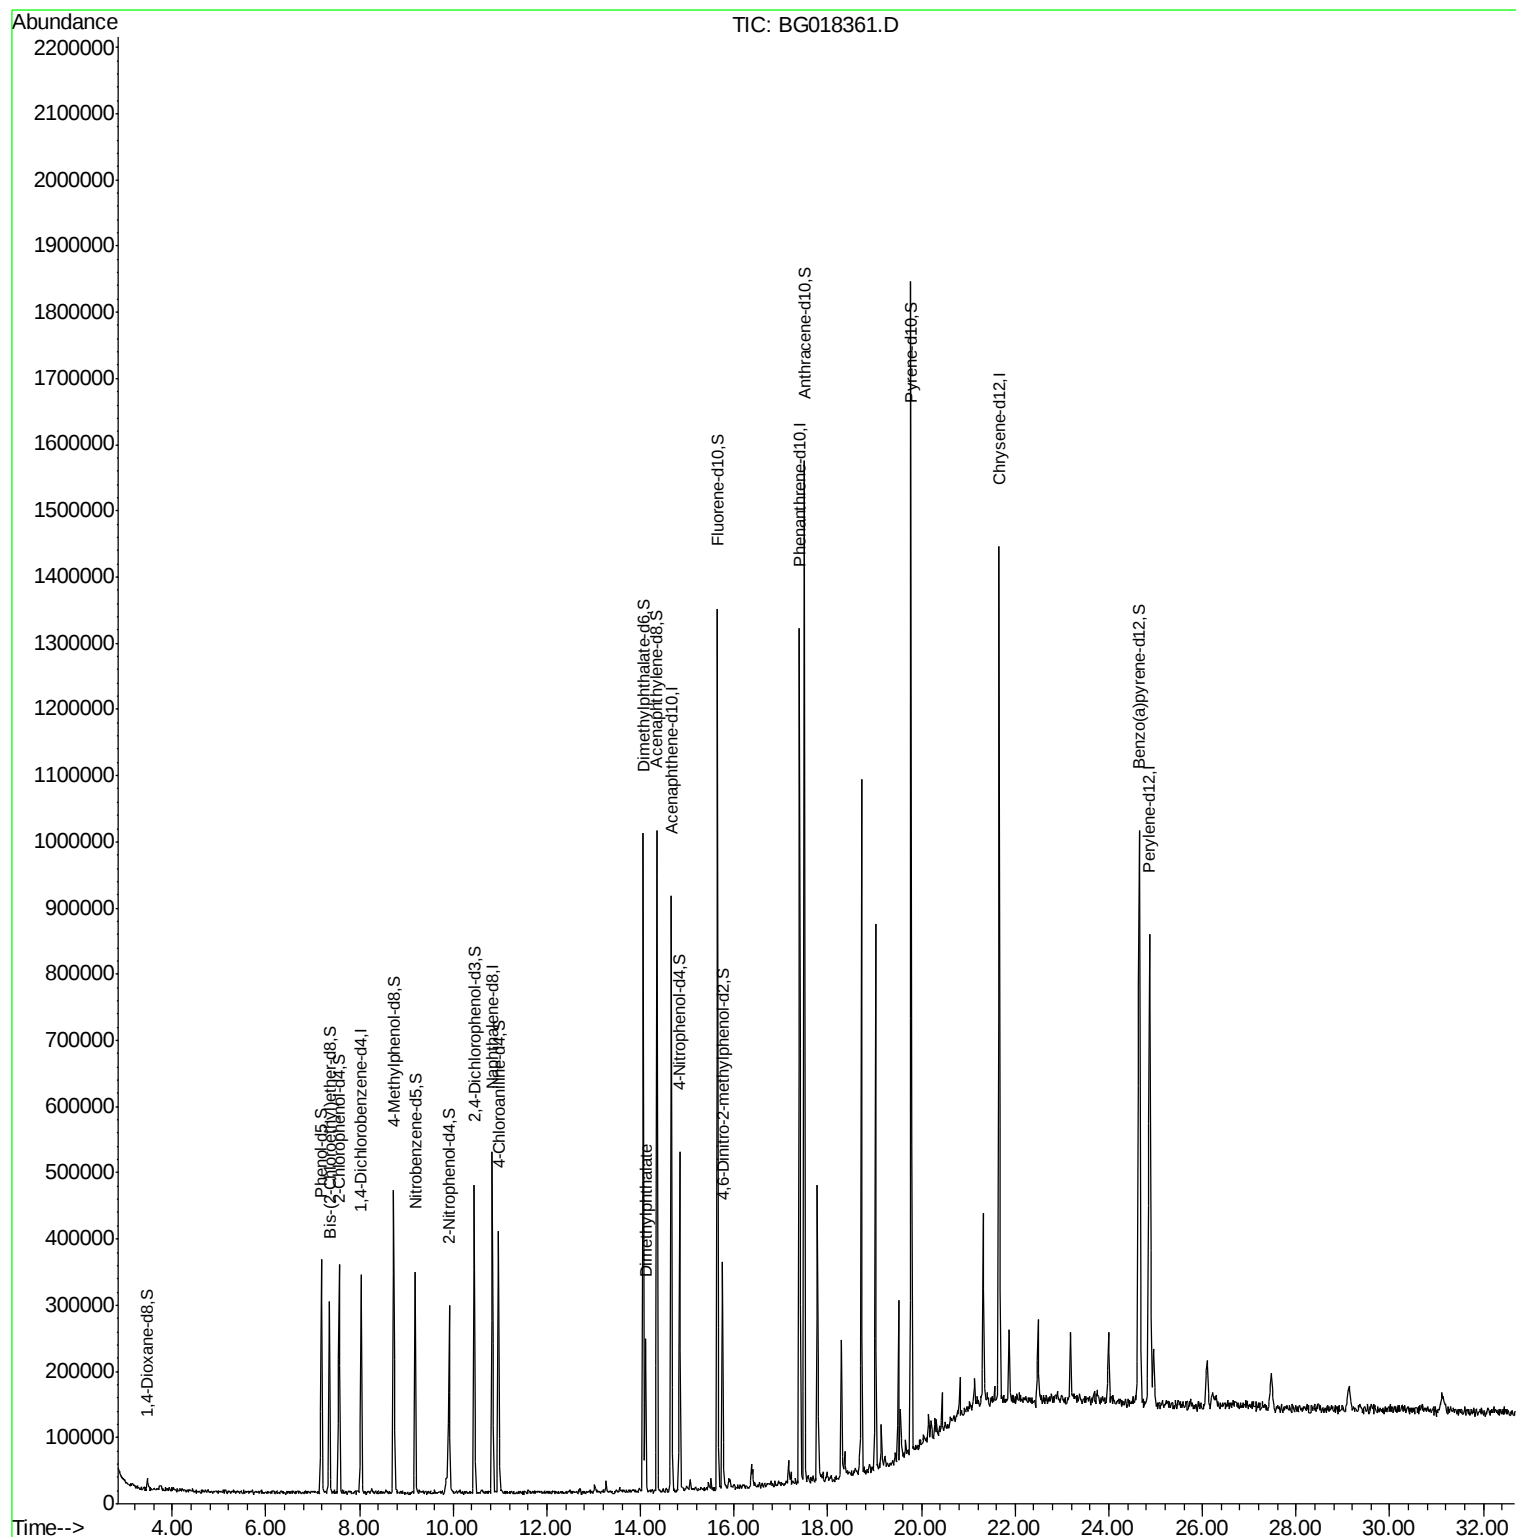

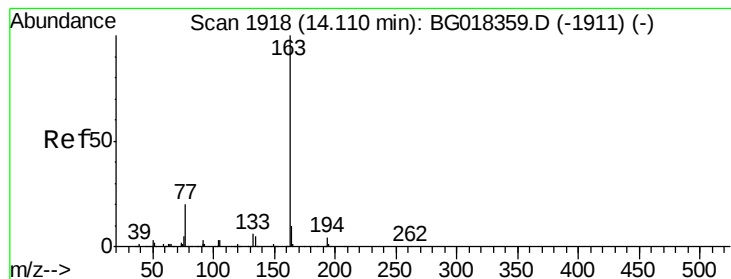

#45

Dimethylphthalate

Concen: 5.80 ng/ul

RT: 14.11 min Scan# 1918

Delta R.T. -0.00 min

Lab File: BG018361.D

Acq: 10 Aug 2015 19:39

Instrument :

BNA_G

ClientSampleId :

C01Z2


Tgt Ion:163 Resp: 141867

Ion Ratio Lower Upper

163 100

194 4.3 2.9 4.3

164 10.0 7.7 11.5

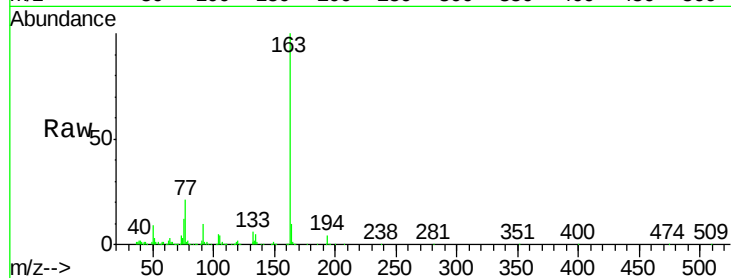

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

