

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081015\
 Data File : BG018372.D
 Acq On : 11 Aug 2015 2:38
 Operator : UM/MA
 Sample : G3136-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C02C8

Quant Time: Aug 11 04:20:41 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 11 01:39:57 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	162932	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	744999	20.00	ng/ul	0.01
36) Acenaphthene-d10	14.67	164	478170	20.00	ng/ul	0.01
62) Phenanthrene-d10	17.41	188	1013231	20.00	ng/ul	0.01
78) Chrysene-d12	21.68	240	859032	20.00	ng/ul	0.02
86) Perylene-d12	24.91	264	855072	20.00	ng/ul	0.04

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	9542	2.59	ng/uL	0.00
5) Phenol-d5	7.20	99	240306	16.25	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.37	67	151202	16.50	ng/ul	0.01
9) 2-Chlorophenol-d4	7.58	132	186141	16.44	ng/ul	0.02
13) 4-Methylphenol-d8	8.75	113	204043	16.42	ng/ul	0.01
19) Nitrobenzene-d5	9.20	128	92942	16.00	ng/ul	0.01
22) 2-Nitrophenol-d4	9.93	143	90494	15.30	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.47	165	200973	16.01	ng/ul	0.01
29) 4-Chloroaniline-d4	10.98	131	253217	17.85	ng/ul	0.01
44) Dimethylphthalate-d6	14.07	166	592959	14.74	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	649841	12.83	ng/ul	0.01
52) 4-Nitrophenol-d4	14.86	143	87647	12.11	ng/ul	0.02
58) Fluorene-d10	15.66	176	424875	12.12	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	15.77	200	19357	3.88	ng/ul	0.01
71) Anthracene-d10	17.51	188	596372	12.31	ng/ul	0.01
79) Pyrene-d10	19.79	212	546078	12.25	ng/ul	0.01
90) Benzo(a)pyrene-d12	24.69	264	554840	12.22	ng/ul	0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.12	163	342462	8.63	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081015\
Data File : BG018372.D
Acq On : 11 Aug 2015 2:38
Operator : UM/MA
Sample : G3136-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C02C8

Quant Time: Aug 11 04:20:41 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 11 01:39:57 2015
Response via : Initial Calibration

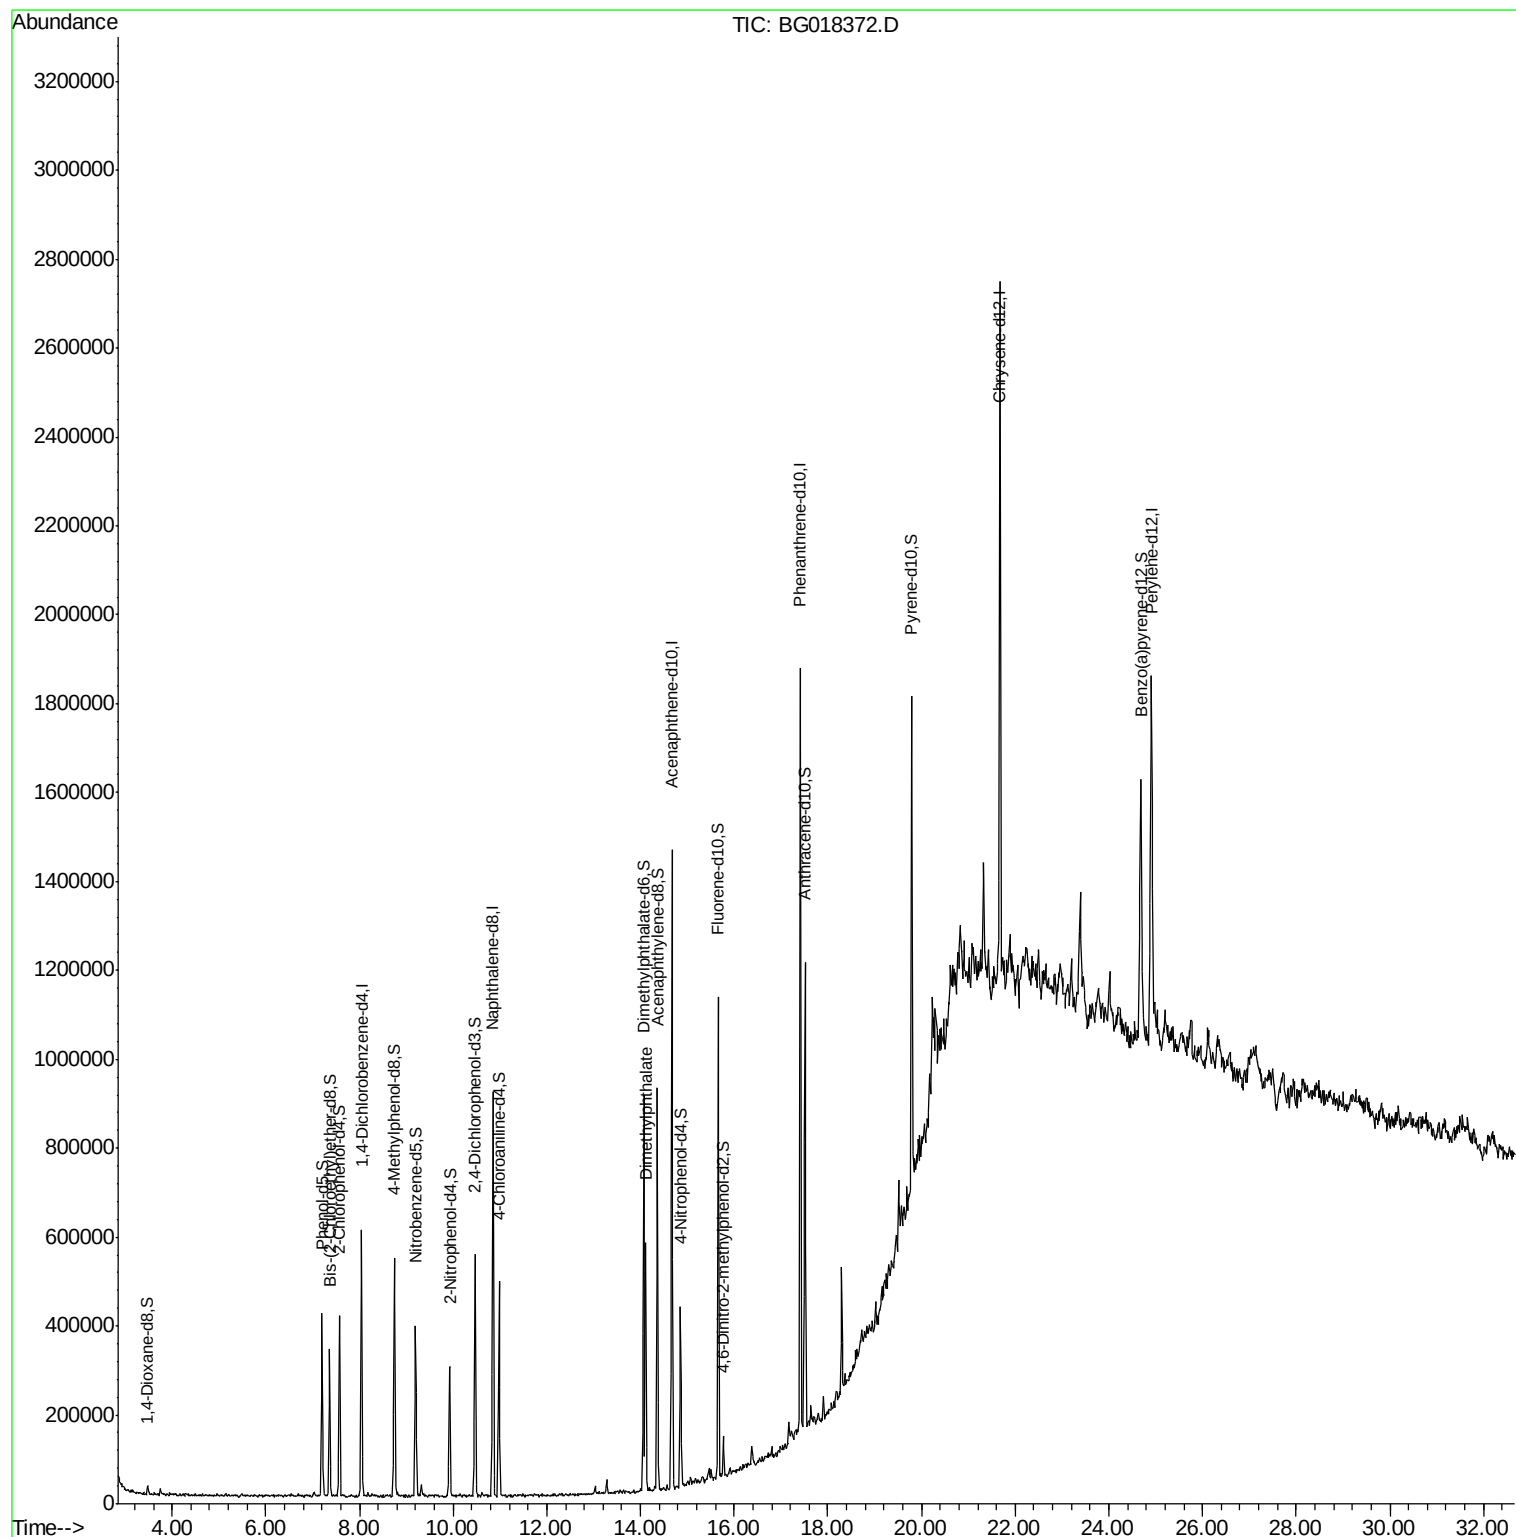

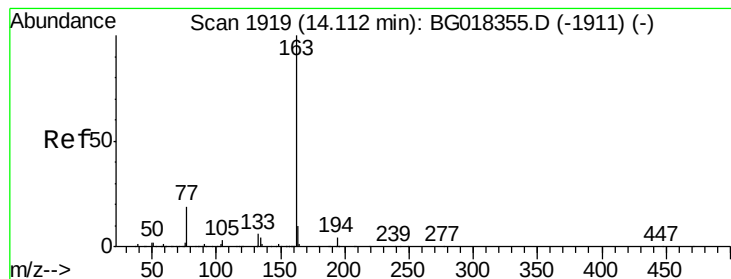

#45

Dimethylphthalate

Concen: 8.63 ng/ul

RT: 14.12 min Scan# 1919

Delta R.T. 0.01 min

Lab File: BG018372.D

Acq: 11 Aug 2015 2:38

Instrument :

BNA_G

ClientSampleId :

C02C8


Tgt Ion:163 Resp: 342462

Ion Ratio Lower Upper

163 100

194 4.3 2.9 4.3

164 10.0 7.7 11.5

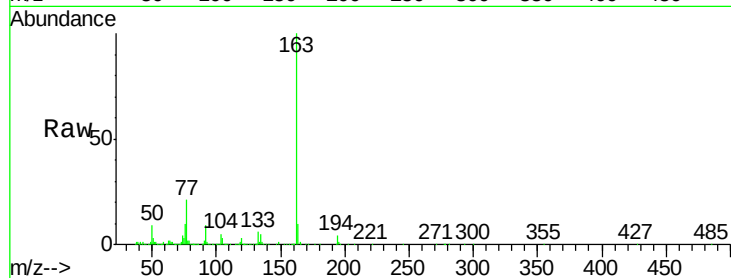

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

