

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
 Data File : BG023595.D
 Acq On : 10 Aug 2016 16:54
 Operator : UM/SJ
 Sample : H4360-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS002-0206-01

Quant Time: Aug 11 03:58:54 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 03:58:16 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	170058	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	762151	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	520153	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1246586	20.00	ng/ul	0.00
75) Chrysene-d12	21.87	240	1229665	20.00	ng/ul	0.00
83) Perylene-d12	25.27	264	1226075	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	6164	1.54	ng/uL	0.00
5) Phenol-d5	7.26	99	302351	17.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	209036	19.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	225101	19.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	216944	16.22	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	109858	18.29	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	133923	19.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	234408	18.01	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	604	0.04	ng/ul	0.17
43) Dimethylphthalate-d6	14.18	166	838341	19.68	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	967081	20.18	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	111269	15.30	ng/ul	0.01
57) Fluorene-d10	15.78	176	771642	19.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	137351	17.17	ng/ul	0.00
70) Anthracene-d10	17.65	188	1160032	20.65	ng/ul	0.00
76) Pyrene-d10	19.94	212	1264115	20.31	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.03	264	1142383	20.58	ng/ul	0.00

Target Compounds


						Qvalue
44) Dimethylphthalate	14.22	163	557394	13.22	ng/ul	100
69) Phenanthrene	17.59	178	398667	6.18	ng/ul	99
74) Fluoranthene	19.60	202	646563	9.78	ng/ul#	94
77) Pyrene	19.97	202	750468	9.87	ng/ul#	92
80) Benzo(a)anthracene	21.92	228	352290	5.09	ng/ul	92
81) Bis(2-ethylhexyl)phthalate	21.73	149	122243	3.15	ng/ul#	96
82) Chrysene	21.92	228	353050	5.61	ng/ul	94
86) Benzo(k)fluoranthene	24.24	252	110282	1.61	ng/ul#	93
89) Indeno(1,2,3-cd)pyrene	29.14	276	161858	2.05	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023595.D
Acq On : 10 Aug 2016 16:54
Operator : UM/SJ
Sample : H4360-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS002-0206-01

Quant Time: Aug 11 03:58:54 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

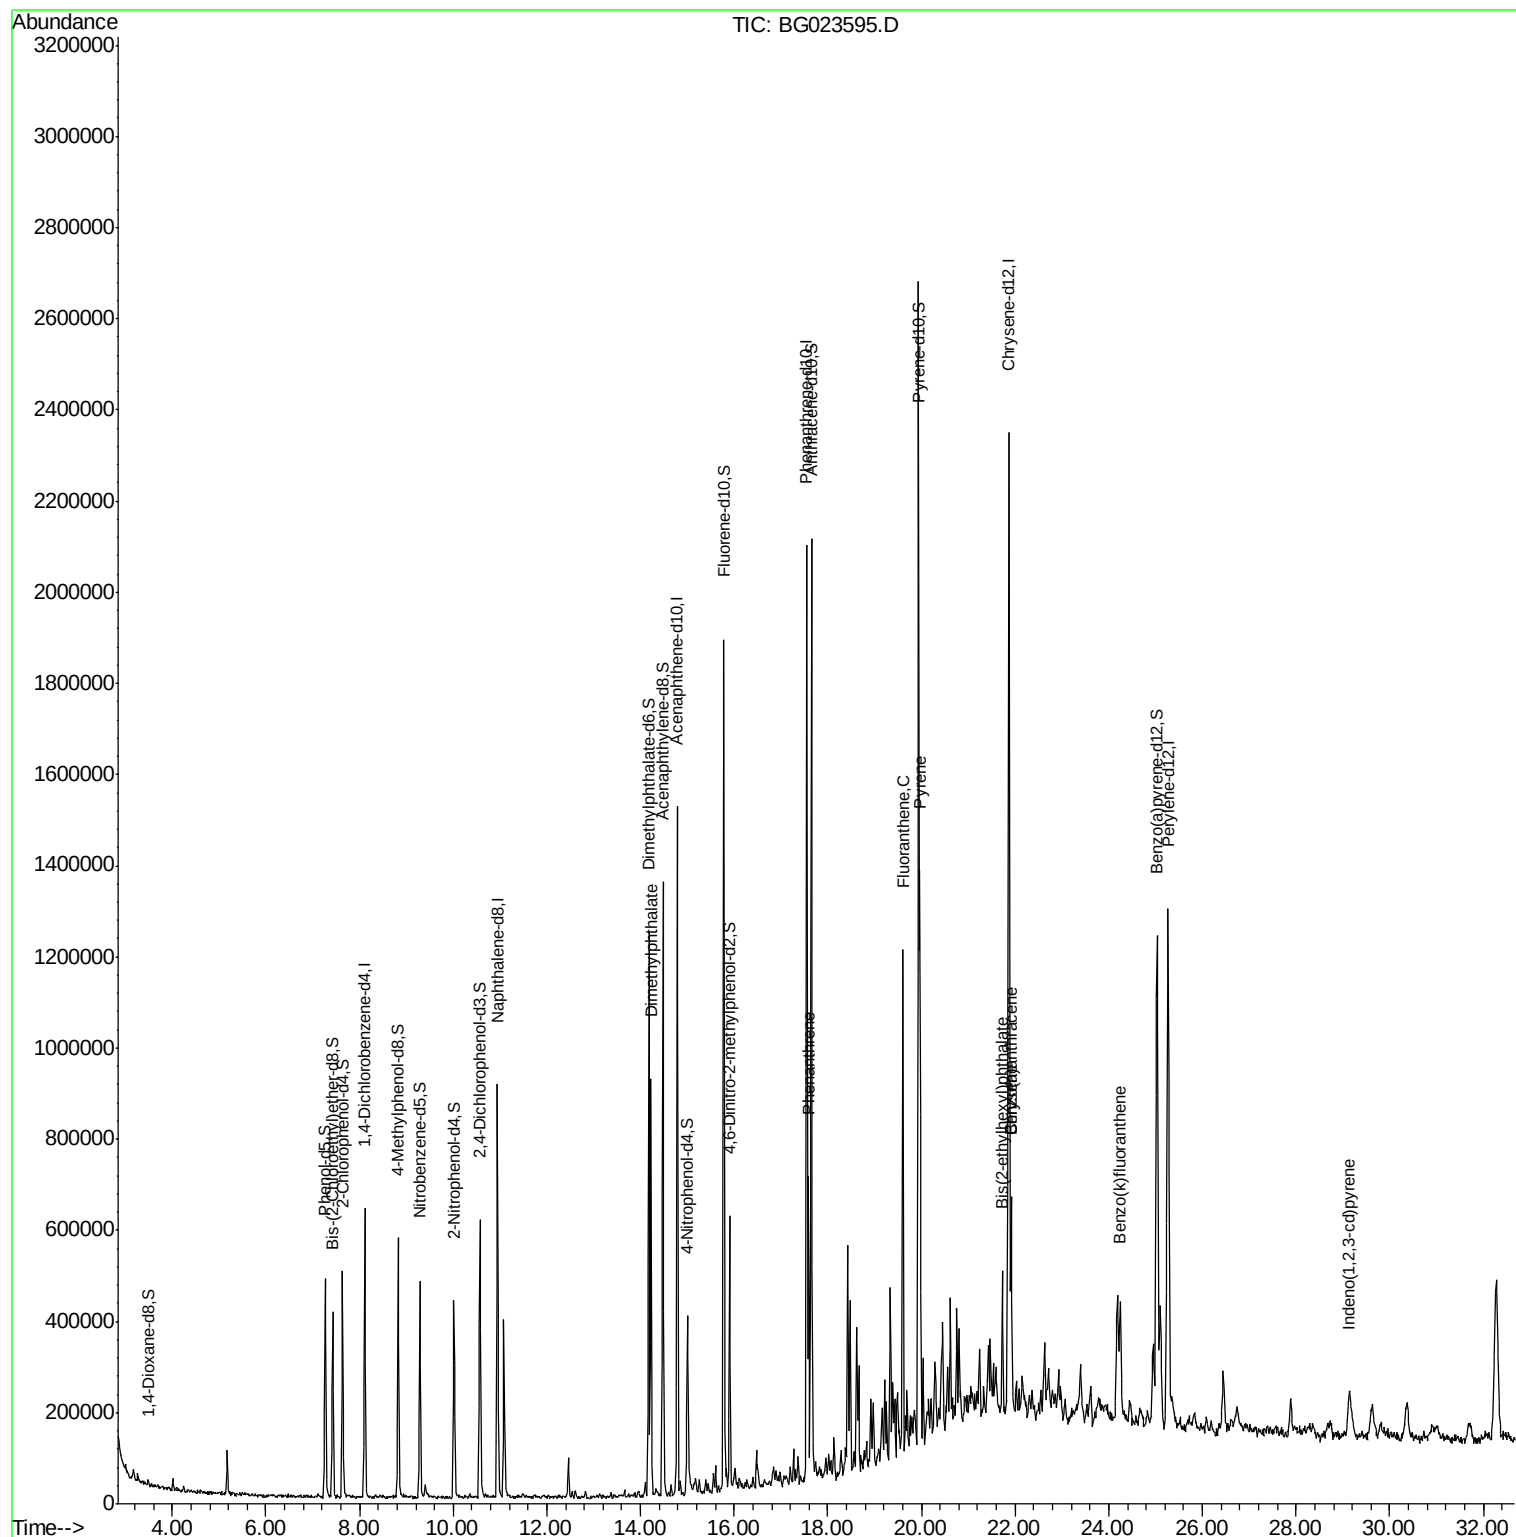

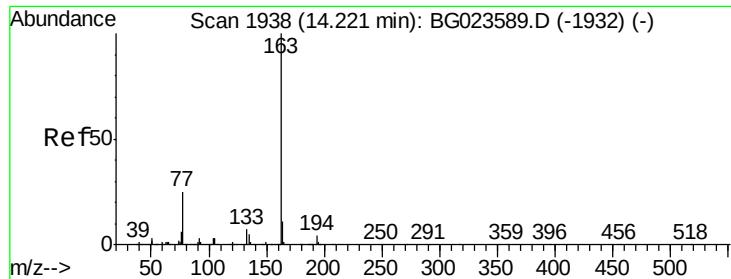

#44

Dimethylphthalate

Concen: 13.22 ng/ul

RT: 14.22 min Scan# 1938

Delta R.T. 0.00 min

Lab File: BG023595.D

Acq: 10 Aug 2016 16:54

Instrument :

BNA_G

ClientSampleId :

PR001-SS002-0206-01


Tgt Ion:163 Resp: 557394

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2




164 11.1 8.8 13.2

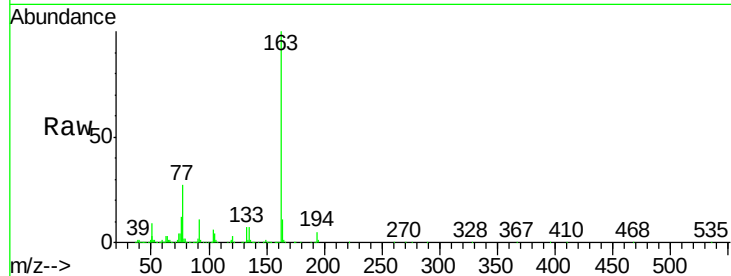

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

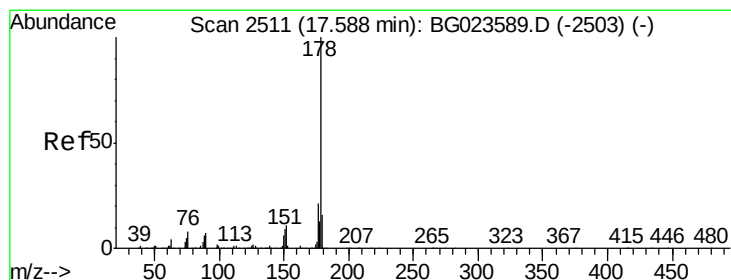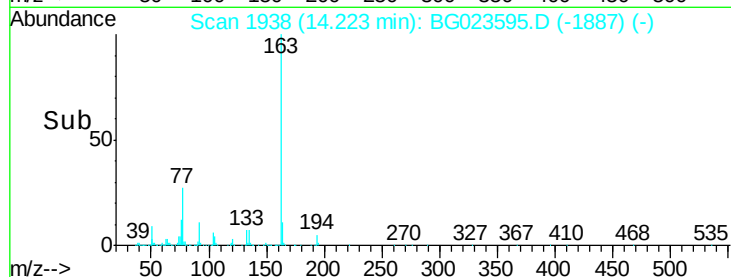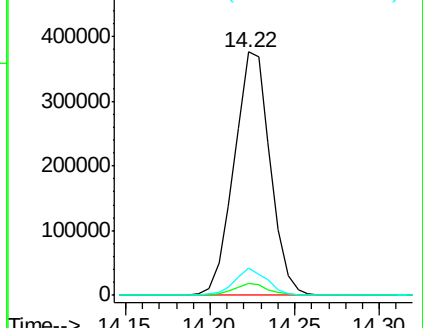

#69

Phenanthrene

Concen: 6.18 ng/ul

RT: 17.59 min Scan# 2511

Delta R.T. 0.00 min

Lab File: BG023595.D

Acq: 10 Aug 2016 16:54


Tgt Ion:178 Resp: 398667

Ion Ratio Lower Upper

178 100

179 15.8 12.9 19.3



176 20.4 15.8 23.8

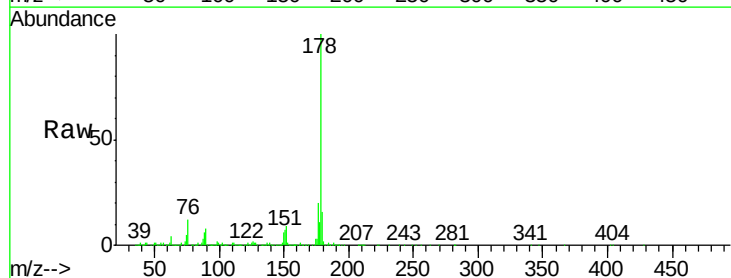


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

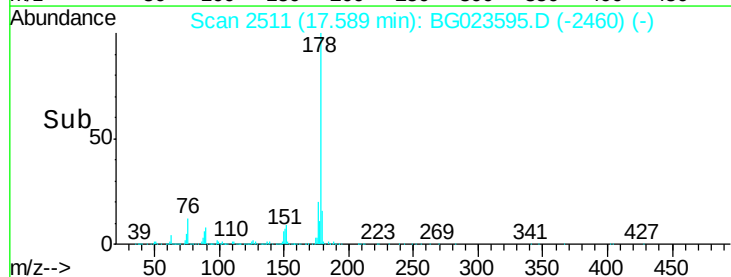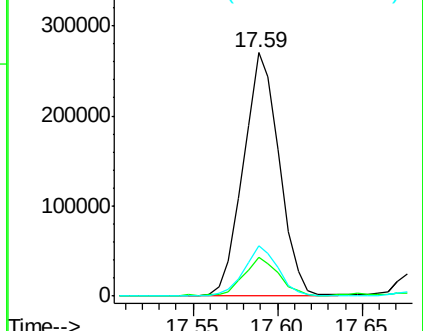

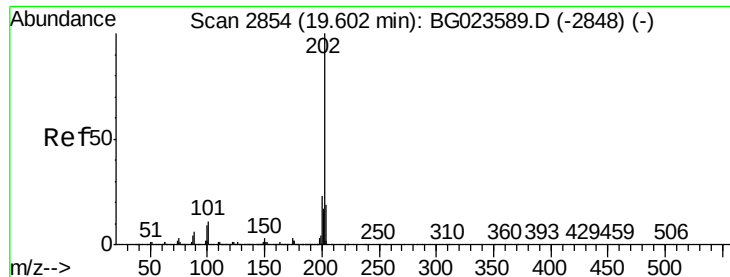

#74

Fluoranthene

Concen: 9.78 ng/ul

RT: 19.60 min Scan# 2854

Delta R.T. 0.00 min

Lab File: BG023595.D

Acq: 10 Aug 2016 16:54


Instrument :

BNA_G

ClientSampleId :

PR001-SS002-0206-01

Tgt Ion:	202	Resp:	646563
Ion Ratio	Lower	Upper	
202	100		
101	11.1	10.6	16.0
100	8.4	8.7	13.1#

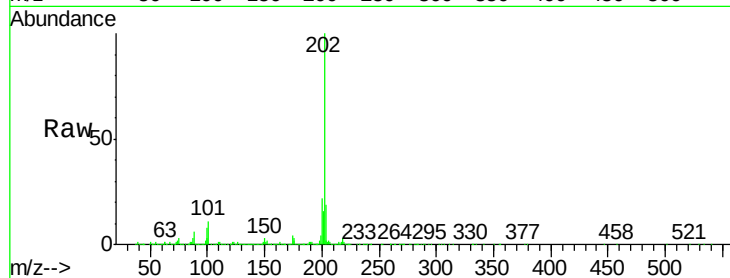



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

19.60

Time-->

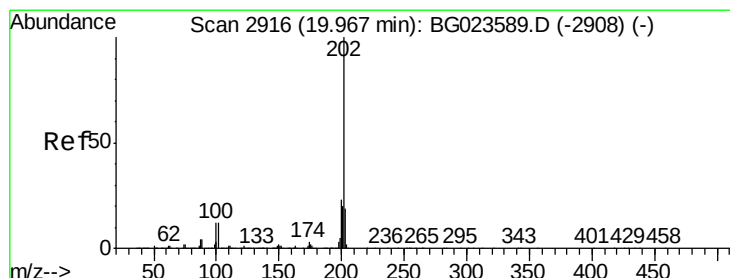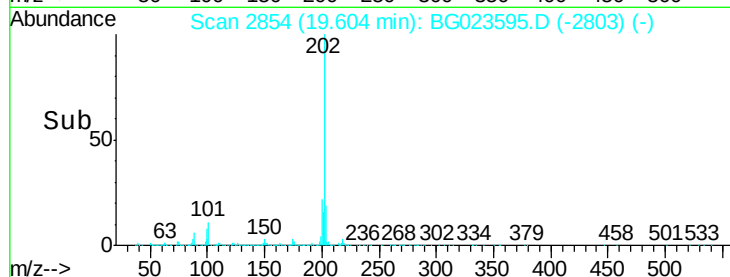

#77

Pyrene

Concen: 9.87 ng/ul


RT: 19.97 min Scan# 2916

Delta R.T. 0.00 min

Lab File: BG023595.D

Acq: 10 Aug 2016 16:54

Tgt Ion:	202	Resp:	750468
Ion Ratio	Lower	Upper	
202	100		
101	11.1	12.5	18.7#
100	11.0	10.2	15.4

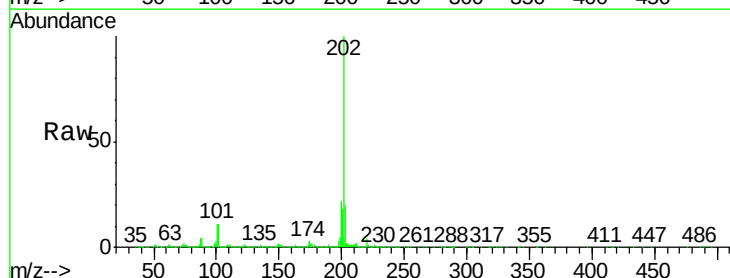


Abundance Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

19.97

Time-->

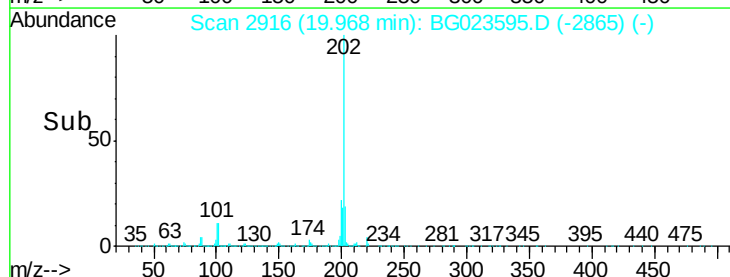

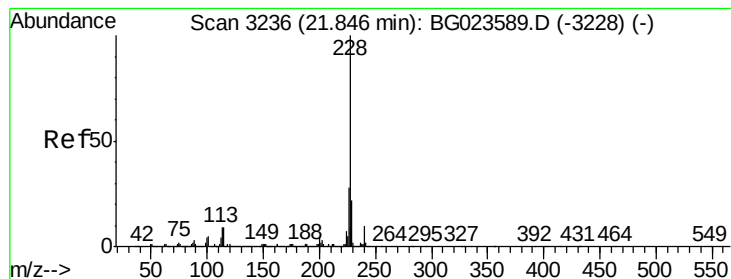

#80

Benzo(a)anthracene

Concen: 5.09 ng/ul

RT: 21.92 min Scan# 3248

Delta R.T. 0.07 min

Lab File: BG023595.D

Acq: 10 Aug 2016 16:54

Instrument :

BNA_G

ClientSampleId :

PR001-SS002-0206-01





Tgt Ion:228 Resp: 352290

Ion Ratio Lower Upper

228 100

229 21.9 15.4 23.2

226 33.5 22.8 34.2

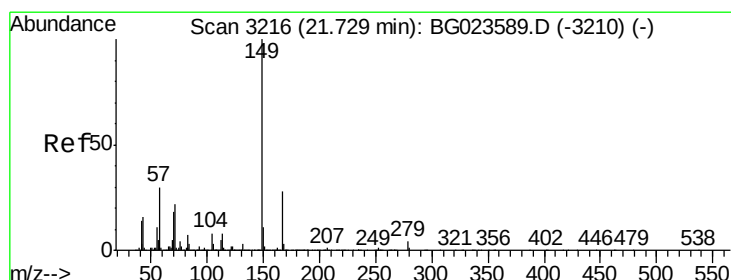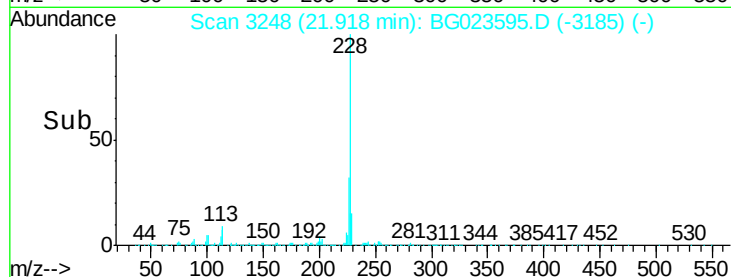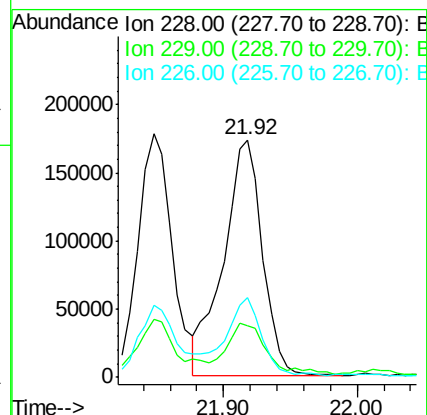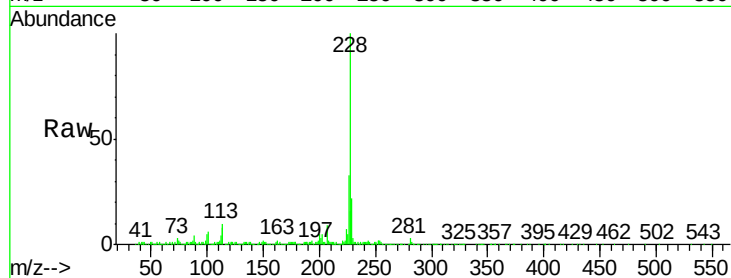

#81

Bis(2-ethylhexyl)phthalate

Concen: 3.15 ng/ul

RT: 21.73 min Scan# 3216

Delta R.T. 0.00 min

Lab File: BG023595.D

Acq: 10 Aug 2016 16:54




Tgt Ion:149 Resp: 122243


Ion Ratio Lower Upper

149 100

167 25.5 21.9 32.9

279 4.6 2.9 4.3#

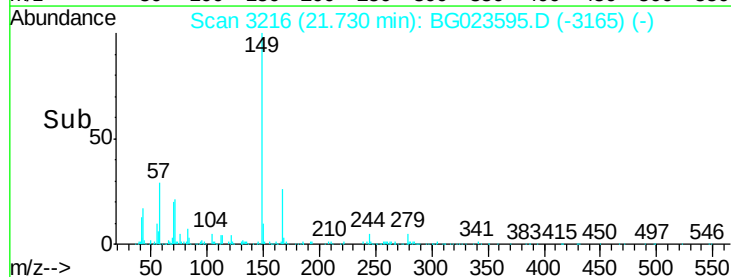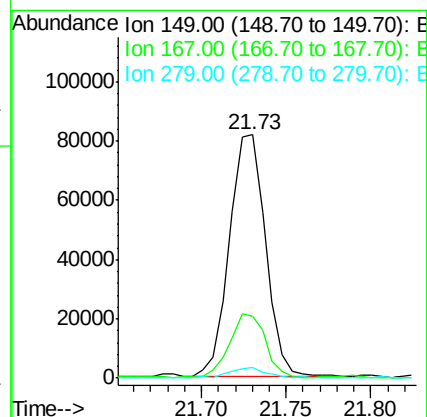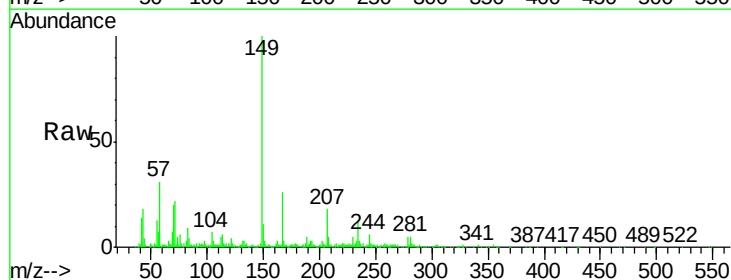

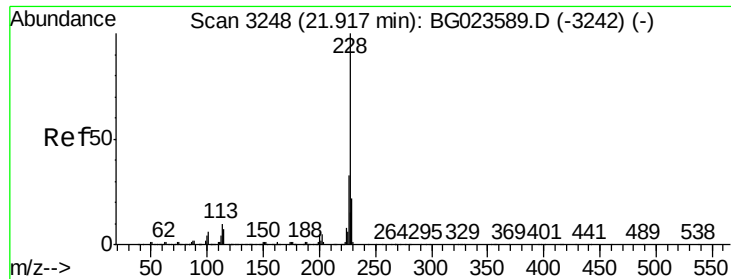

#82

Chrysene

Concen: 5.61 ng/ul

RT: 21.92 min Scan# 3248

Delta R.T. 0.00 min

Lab File: BG023595.D

Acq: 10 Aug 2016 16:54

Instrument :

BNA_G

ClientSampleId :

PR001-SS002-0206-01





Tgt Ion: 228 Resp: 353050

Ion Ratio Lower Upper

228 100

226 33.5 24.2 36.4

229 21.9 15.0 22.6

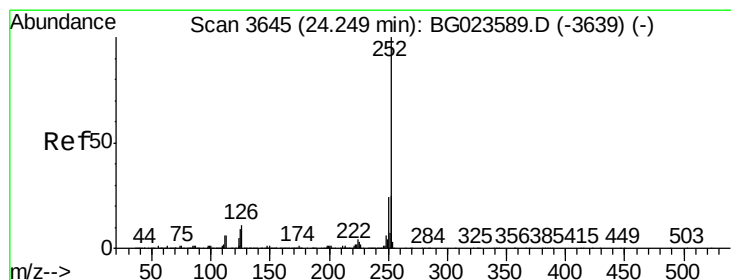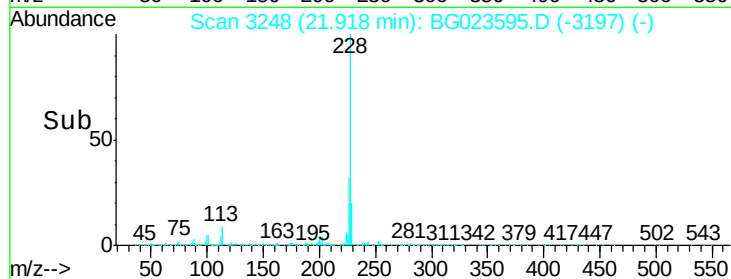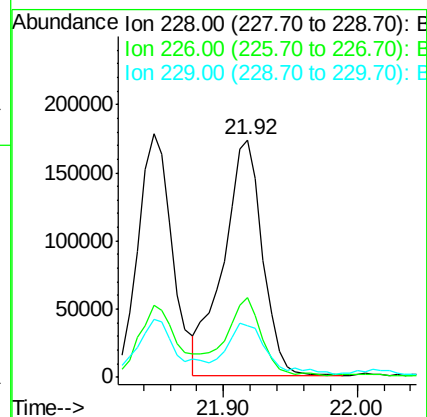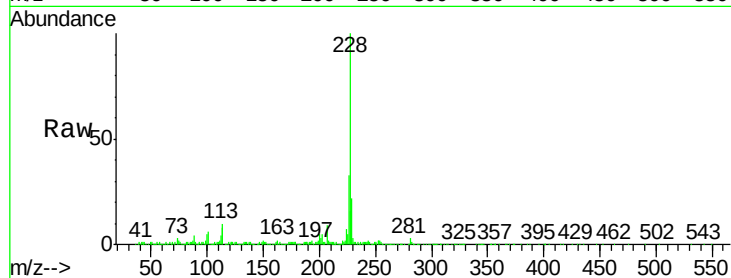

#86

Benzo(k)fluoranthene

Concen: 1.61 ng/ul

RT: 24.24 min Scan# 3643

Delta R.T. -0.01 min

Lab File: BG023595.D

Acq: 10 Aug 2016 16:54




Tgt Ion: 252 Resp: 110282


Ion Ratio Lower Upper

252 100

253 22.5 15.8 23.6

125 10.3 10.6 16.0#

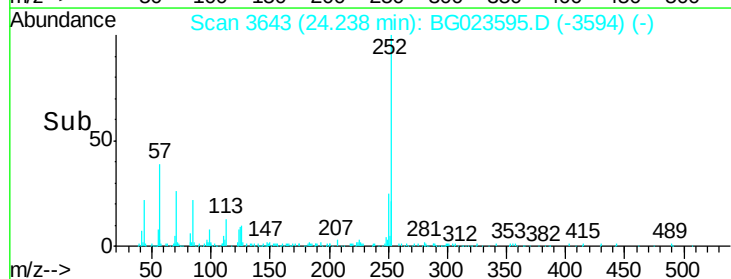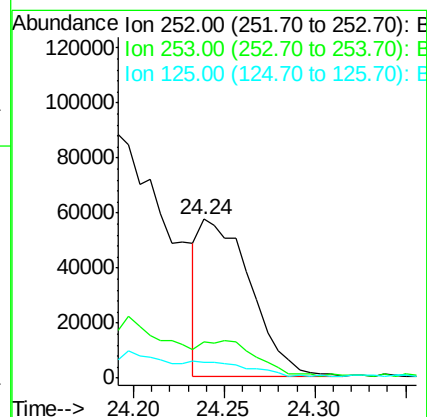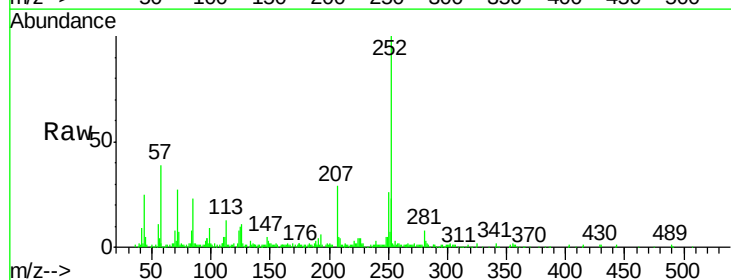

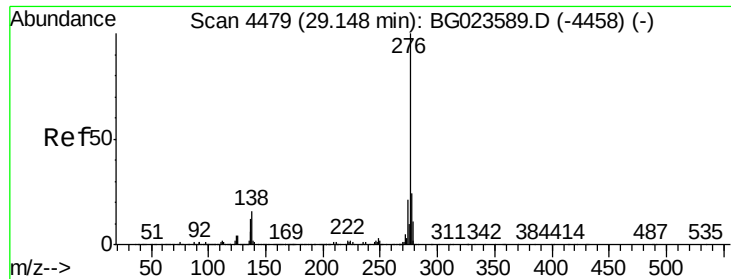

#89

Indeno(1,2,3-cd)pyrene

Concen: 2.05 ng/ul

RT: 29.14 min Scan# 4478

Delta R.T. -0.00 min

Lab File: BG023595.D


Acq: 10 Aug 2016 16:54

Instrument :

BNA_G

ClientSampleId :

PR001-SS002-0206-01

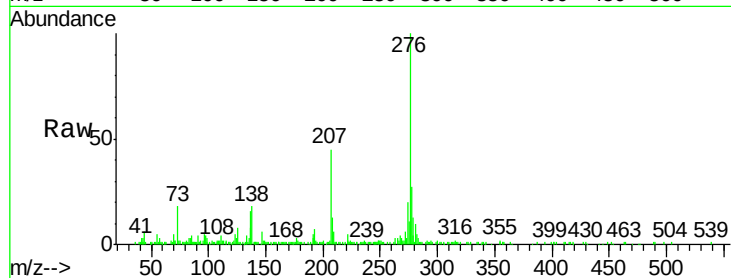


Tgt Ion: 276 Resp: 161858

Ion Ratio Lower Upper

276 100

138 18.1 20.8 31.2#

277 27.4 17.6 26.4#

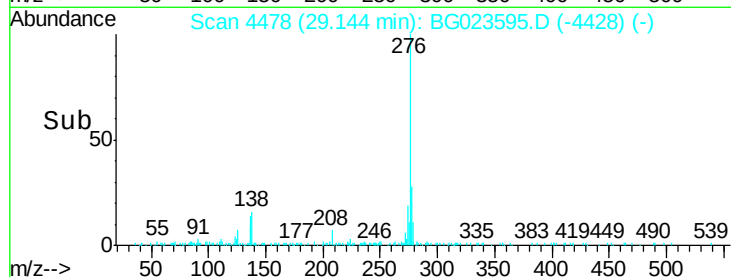

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

