

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
 Data File : BG023604.D
 Acq On : 10 Aug 2016 22:34
 Operator : UM/SJ
 Sample : H4384-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P001-SS002-2430-01

Quant Time: Aug 11 04:00:37 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 03:58:16 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	163006	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	721841	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	518454	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1294220	20.00	ng/ul	0.00
75) Chrysene-d12	21.87	240	1355280	20.00	ng/ul	0.00
83) Perylene-d12	25.27	264	1309048	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	11604	3.03	ng/uL	0.00
5) Phenol-d5	7.27	99	280384	17.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	207333	19.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	199951	17.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	214206	16.71	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	112415	19.76	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	130520	19.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	226322	18.36	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	311307	21.53	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	860778	20.28	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	972959	20.37	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	133920	18.48	ng/ul	0.01
57) Fluorene-d10	15.78	176	794468	20.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	143899	17.33	ng/ul	0.00
70) Anthracene-d10	17.65	188	1235210	21.18	ng/ul	0.00
76) Pyrene-d10	19.94	212	1391403	20.28	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.03	264	1226209	20.69	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.22	163	320991	7.64 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023604.D
Acq On : 10 Aug 2016 22:34
Operator : UM/SJ
Sample : H4384-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS002-2430-01

Quant Time: Aug 11 04:00:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

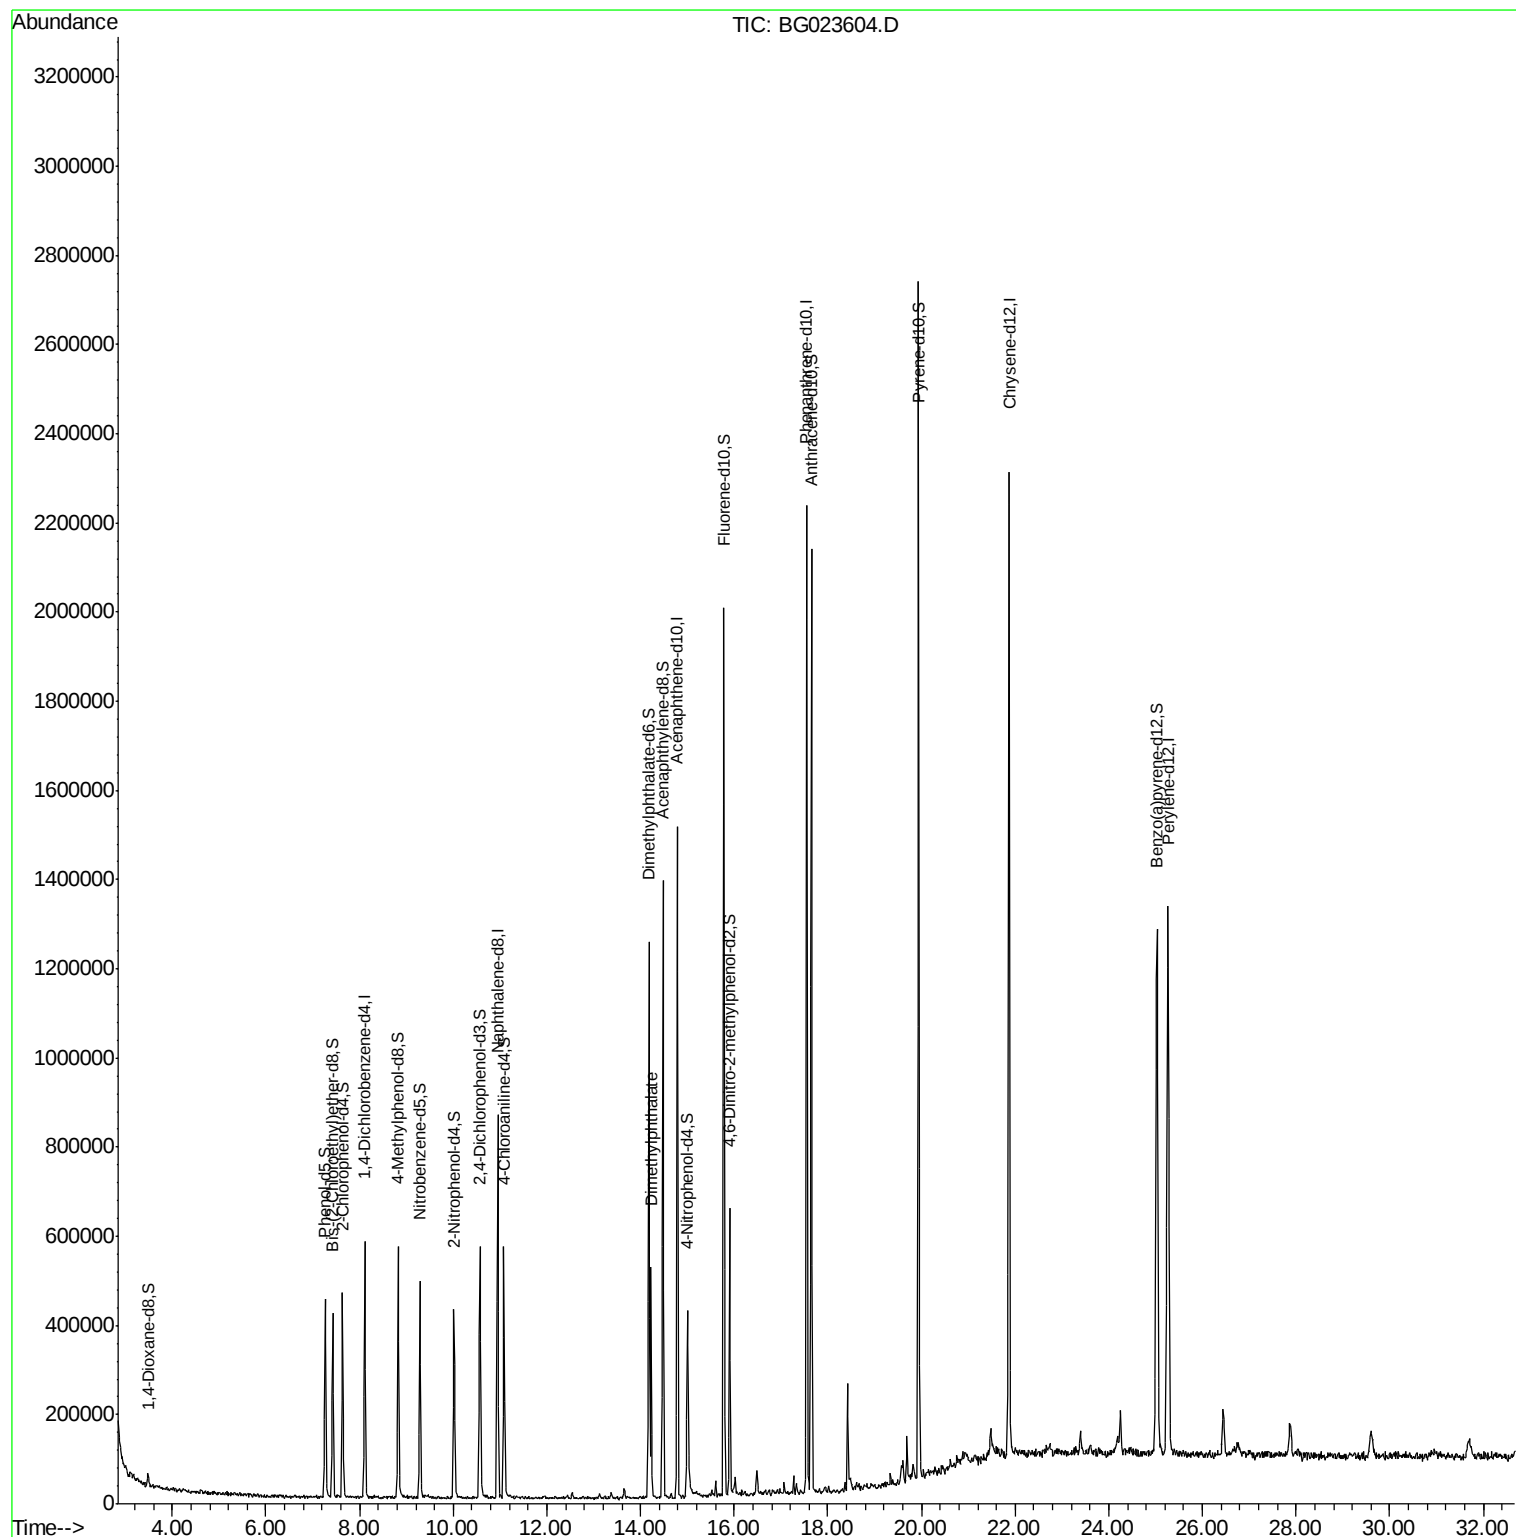

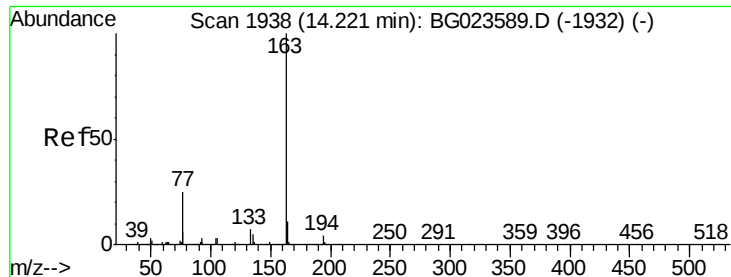

#44

Dimethylphthalate

Concen: 7.64 ng/ul

RT: 14.22 min Scan# 1938

Delta R.T. 0.00 min

Lab File: BG023604.D

Acq: 10 Aug 2016 22:34

Instrument :

BNA_G

ClientSampleId :

P001-SS002-2430-01

Tgt Ion:163 Resp: 320991

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.2

164 10.7 8.8 13.2

