




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
 Data File : BG023613.D
 Acq On : 11 Aug 2016 4:30
 Operator : UM/SJ
 Sample : H4384-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P001-SS001-0612-01

Manual Integrations
 APPROVED

sohil
 8/11/2016 6:14:31 PM

Quant Time: Aug 11 05:54:37 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 03:58:16 2016
 Response via : Initial Calibration

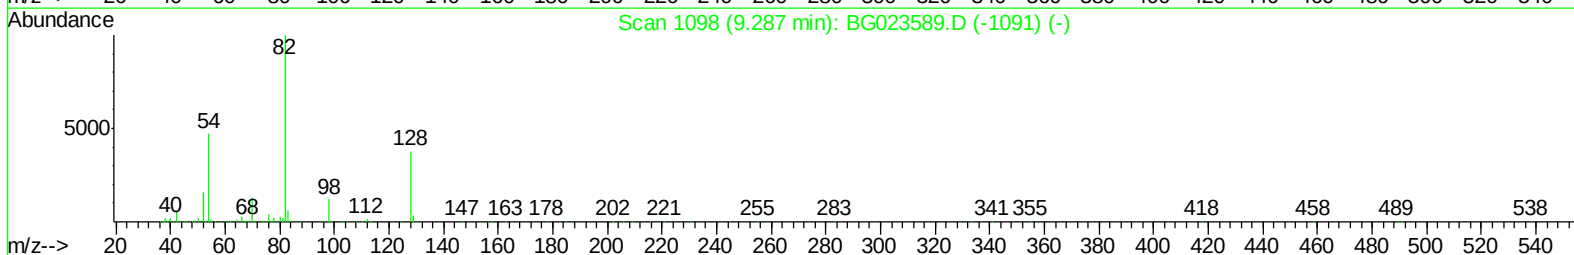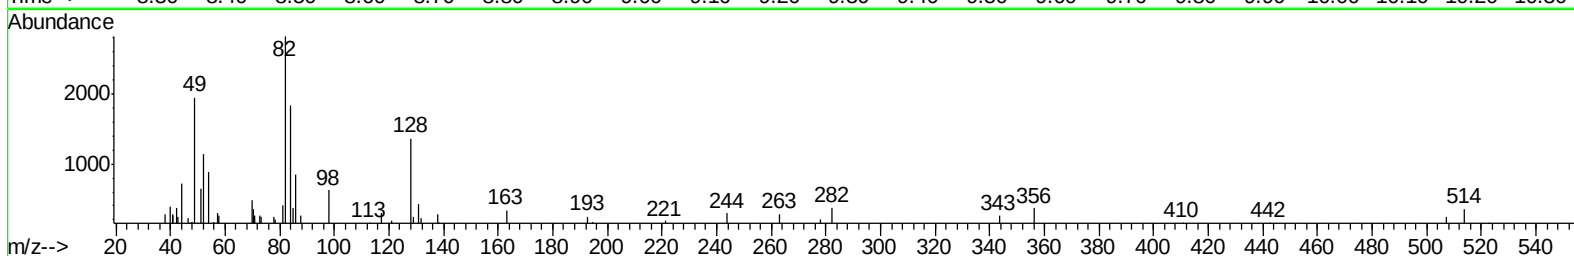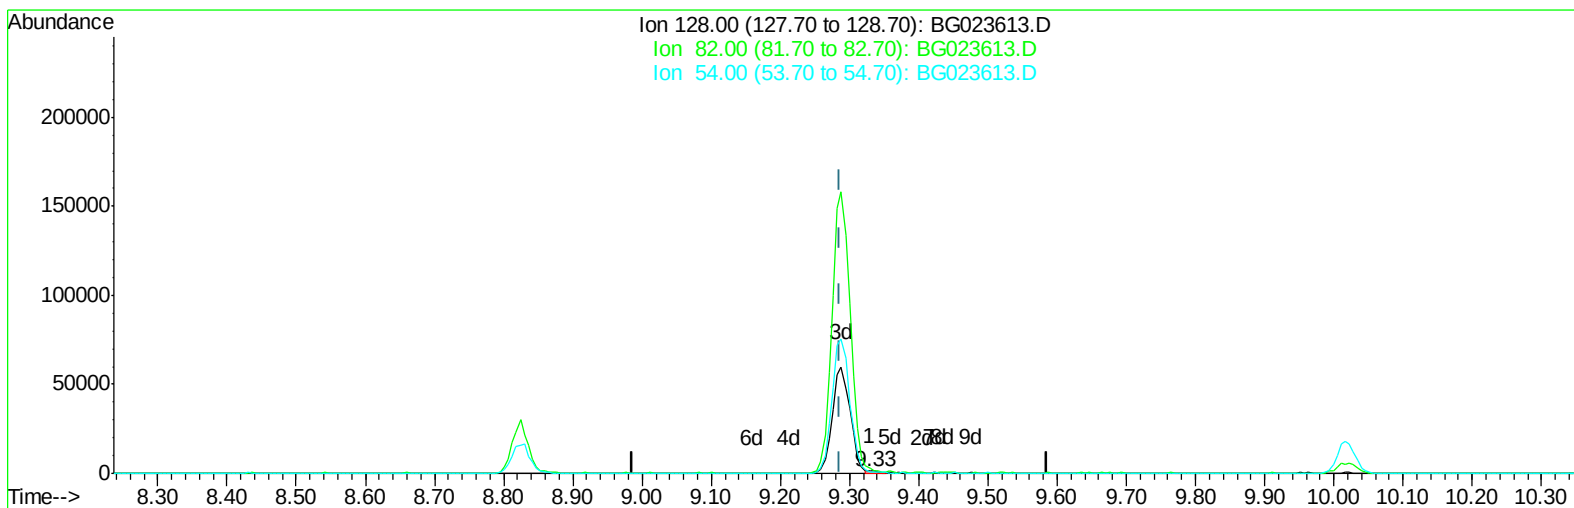

TIC: BG023613.D

(19) Nitrobenzene-d5 (S)

9.329min (+0.042) 0.23ng/ul

response 1253

Ion	Exp%	Act%
128.00	100	100
82.00	219.50	207.49
54.00	78.50	64.51
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

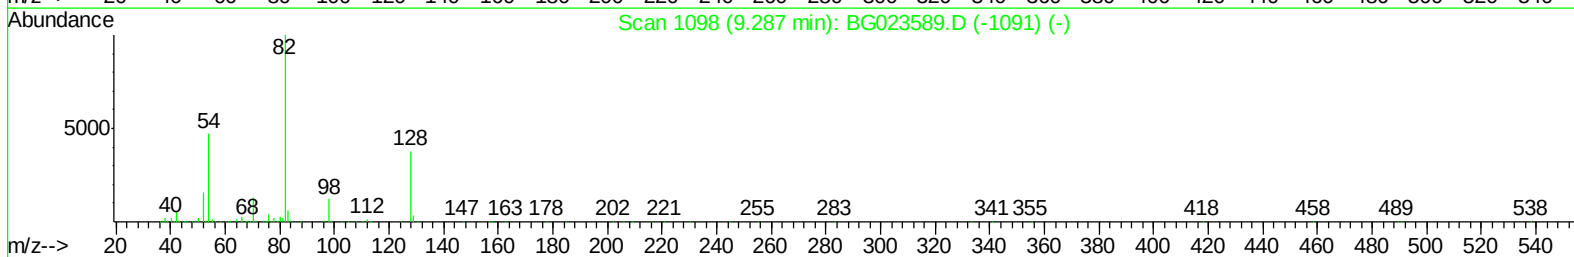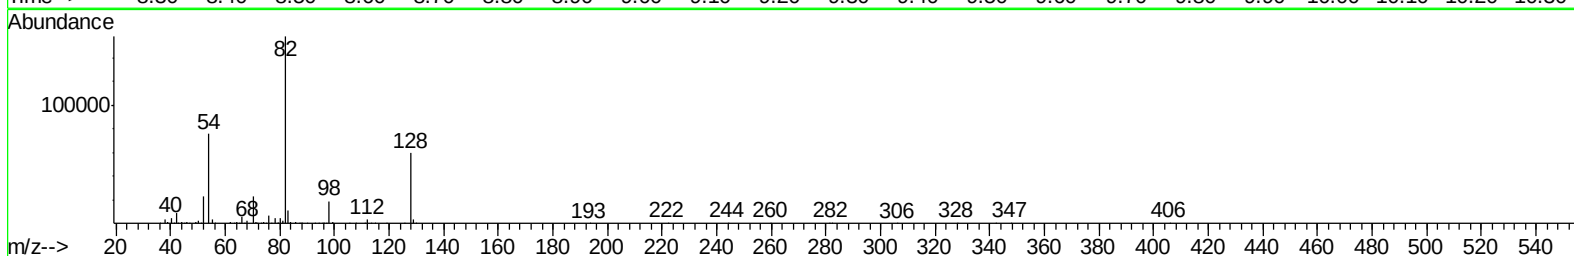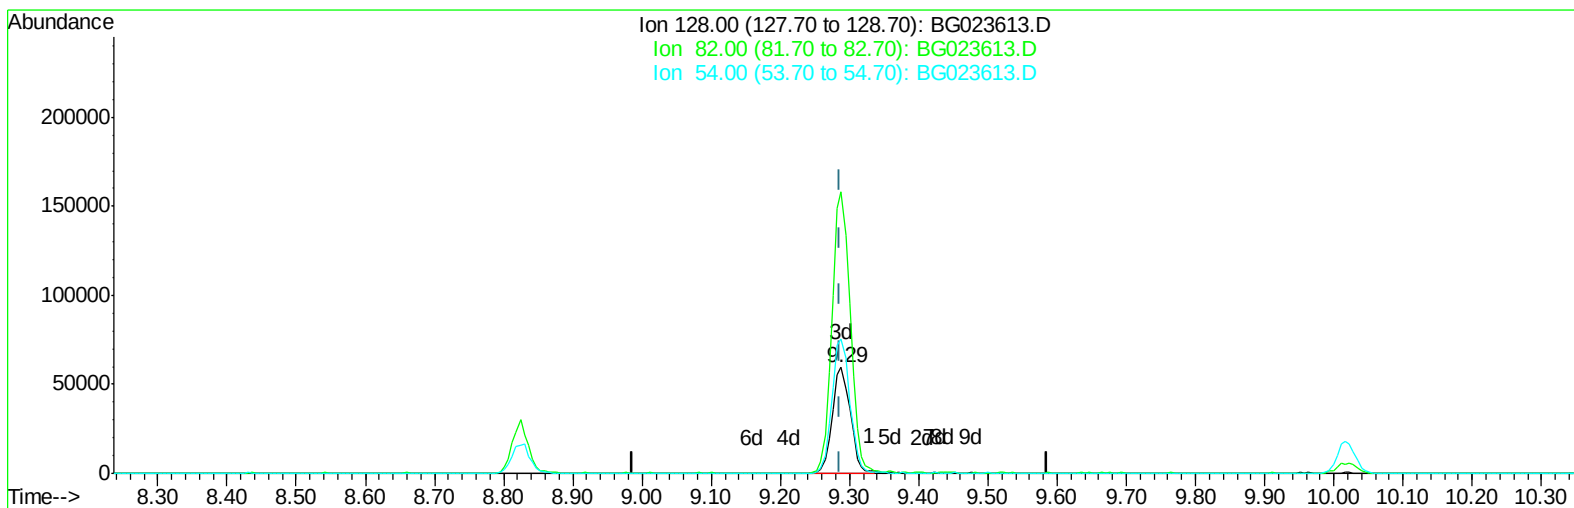

TIC: BG023613.D

(19) Nitrobenzene-d5 (S)

9.288min (+0.001) 19.51ng/ul m

response 106589

Ion	Exp%	Act%
128.00	100	100
82.00	219.50	265.24#
54.00	78.50	127.21#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

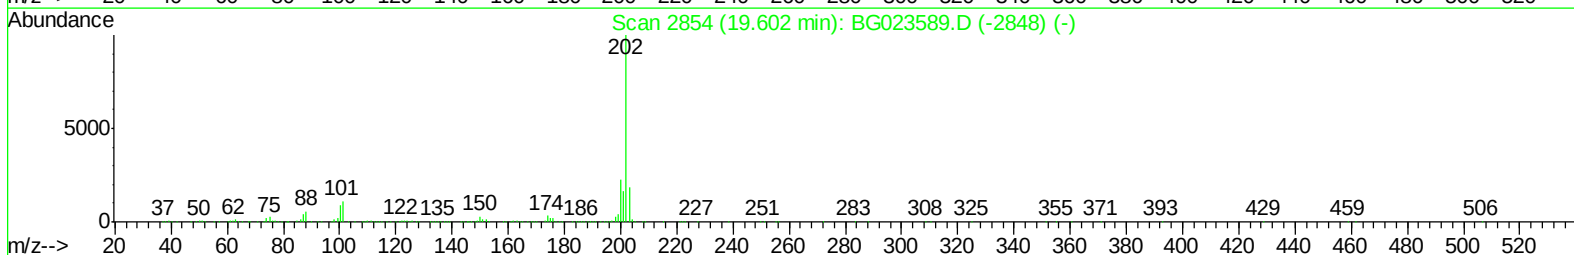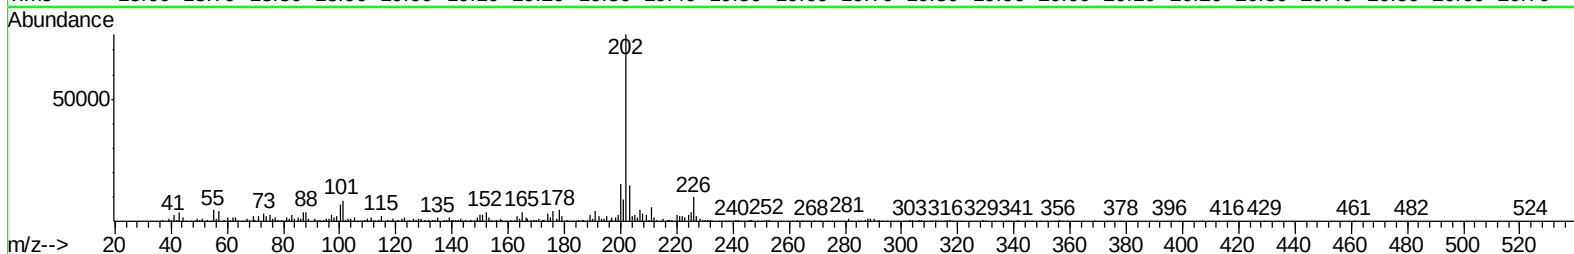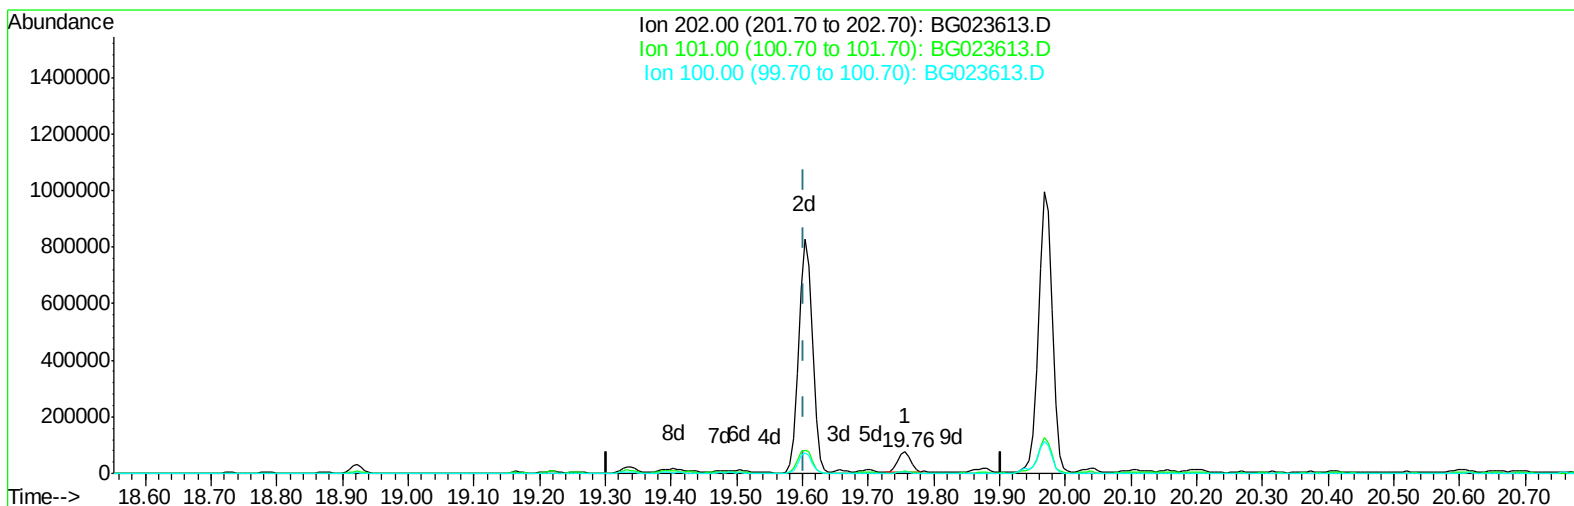

TIC: BG023613.D

(74) Fluoranthene (C)

19.756min (+0.154) 1.69ng/ul

response 102165

Ion	Exp%	Act%
202.00	100	100
101.00	13.30	11.22
100.00	10.90	8.91
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

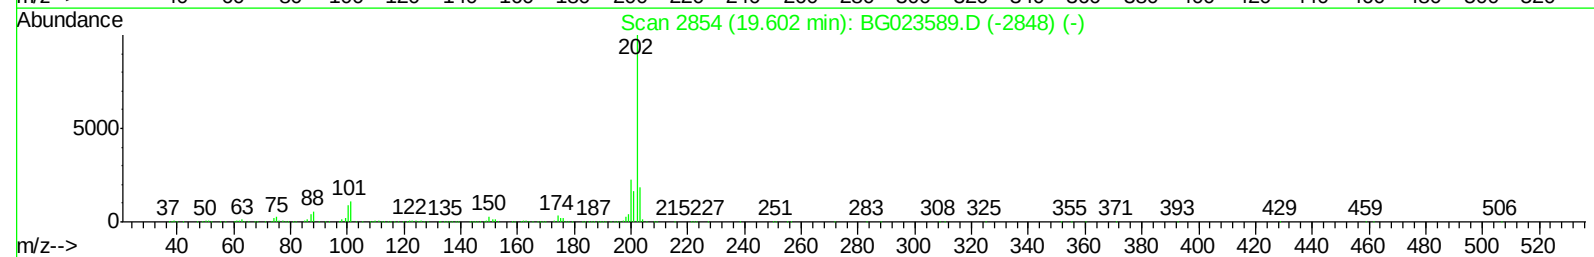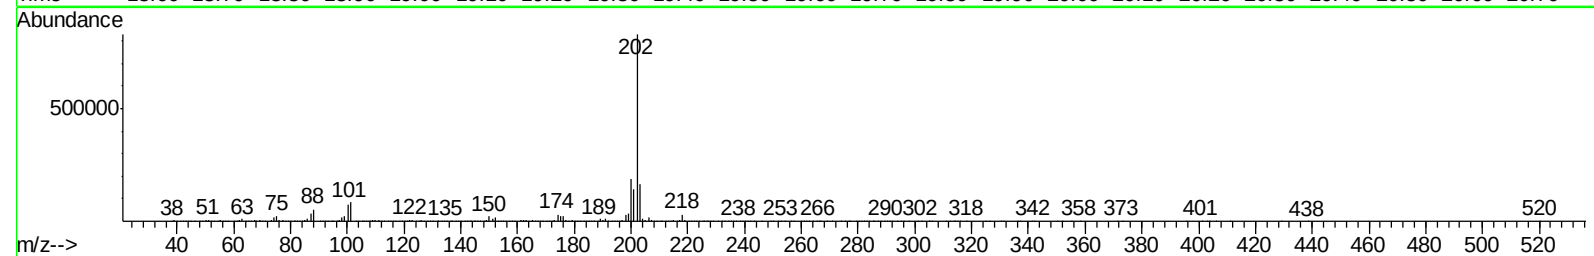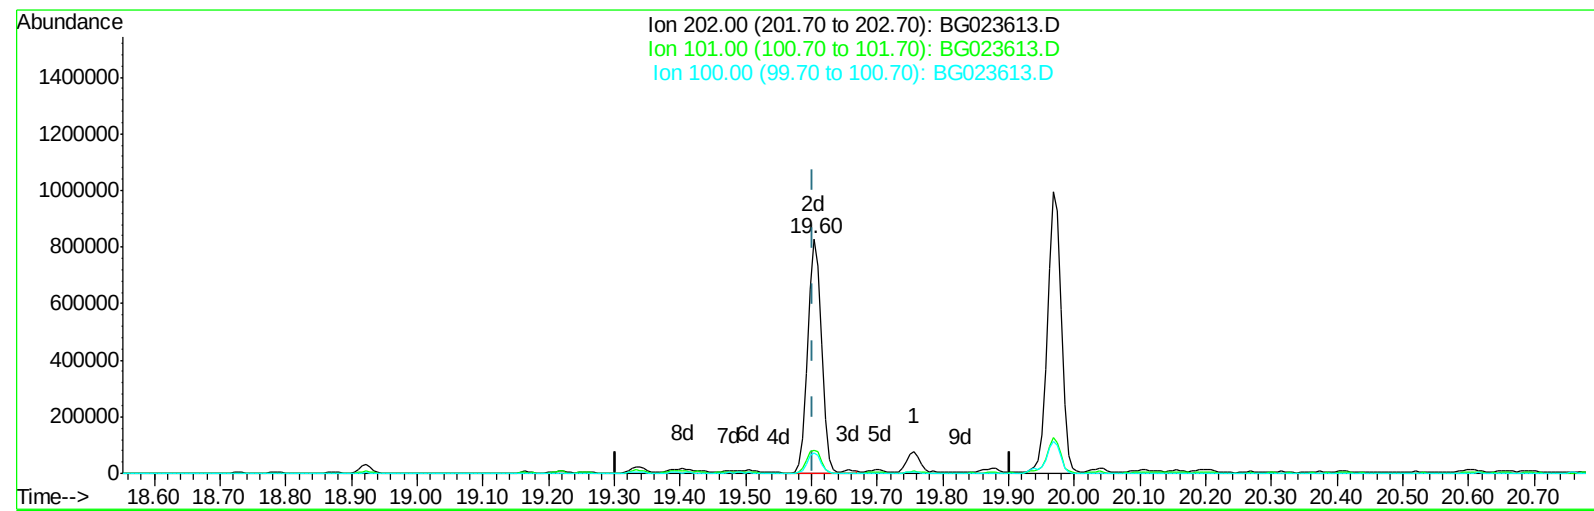

TIC: BG023613.D

(74) Fluoranthene (C)

19.603min (+0.001) 20.42ng/ul m

response 1232694

Ion	Exp%	Act%
202.00	100	100
101.00	13.30	10.06#
100.00	10.90	8.80
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

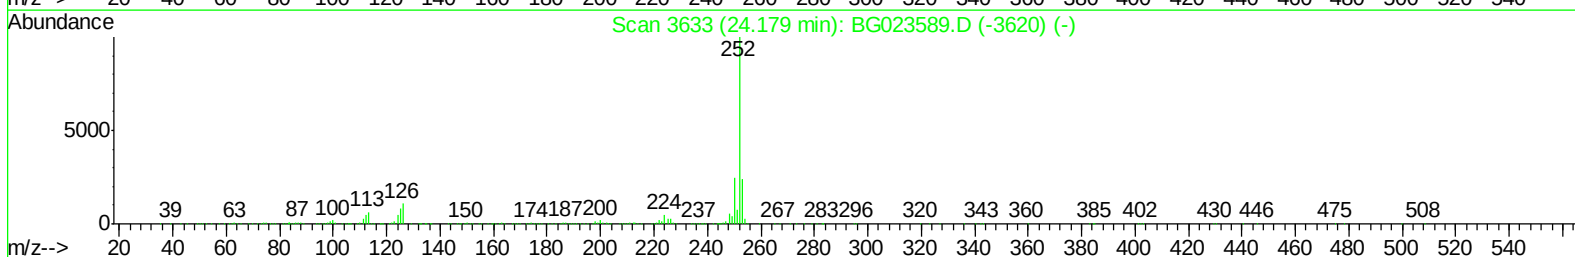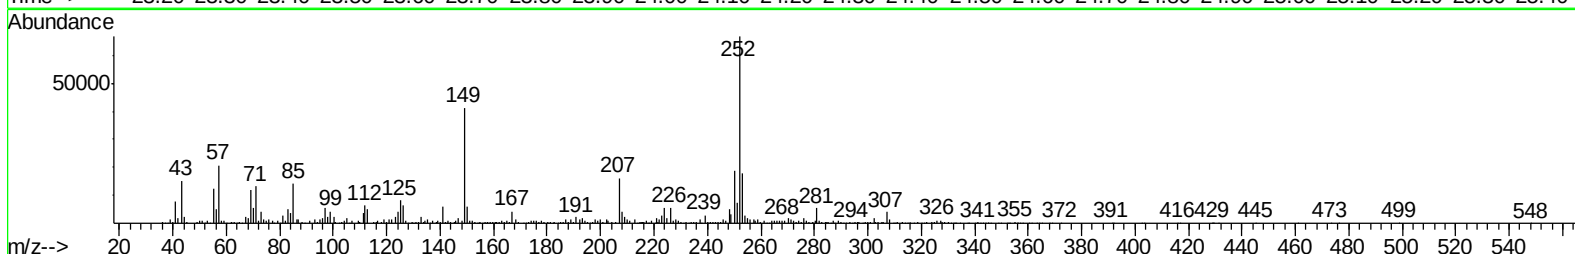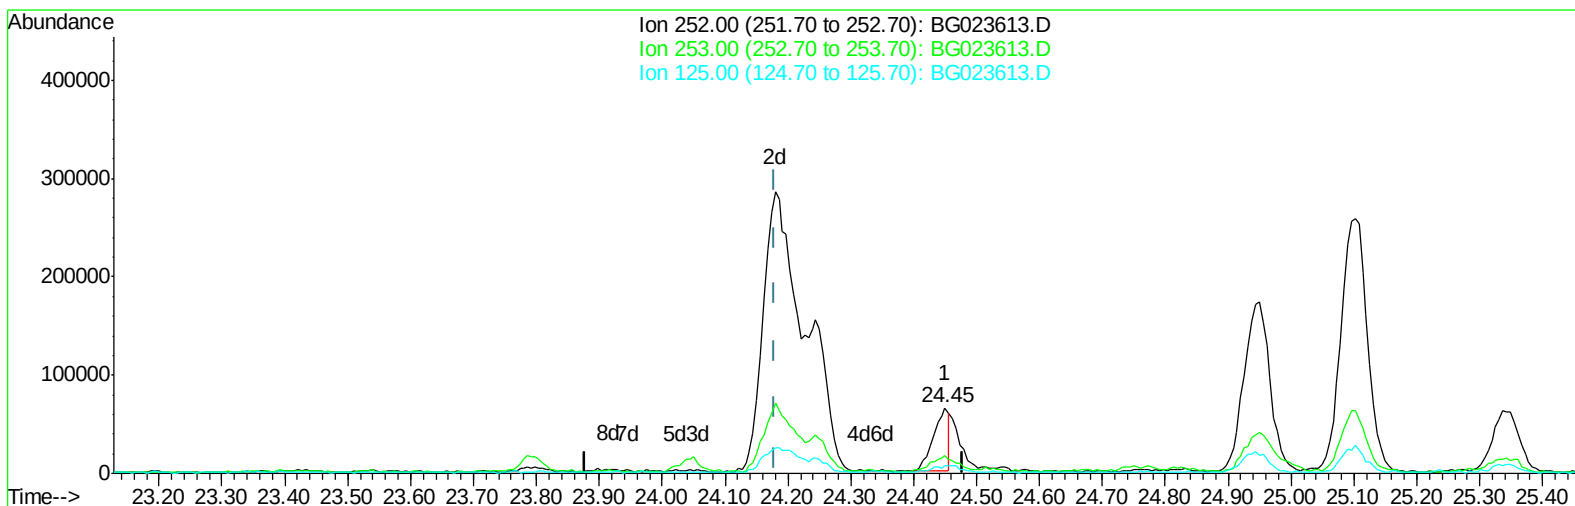

TIC: BG023613.D

(85) Benzo(b)fluoranthene

24.450min (+0.271) 1.78ng/ul

response 112467

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	26.81
125.00	13.50	12.41
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

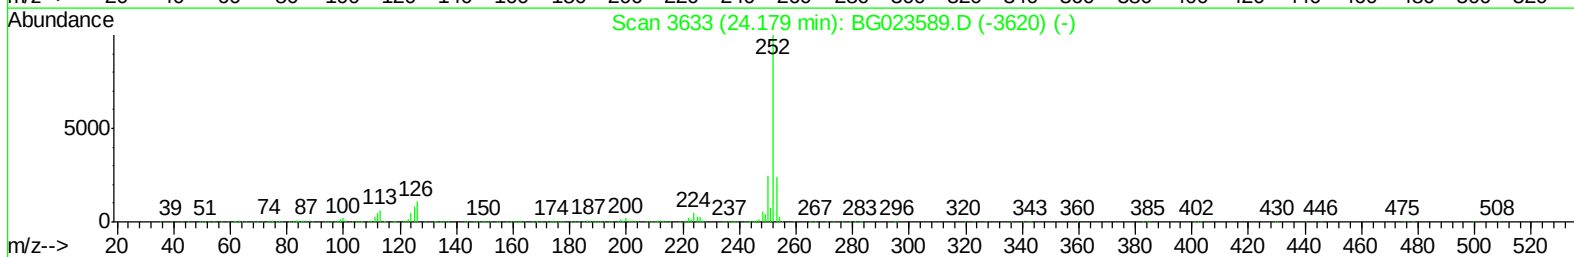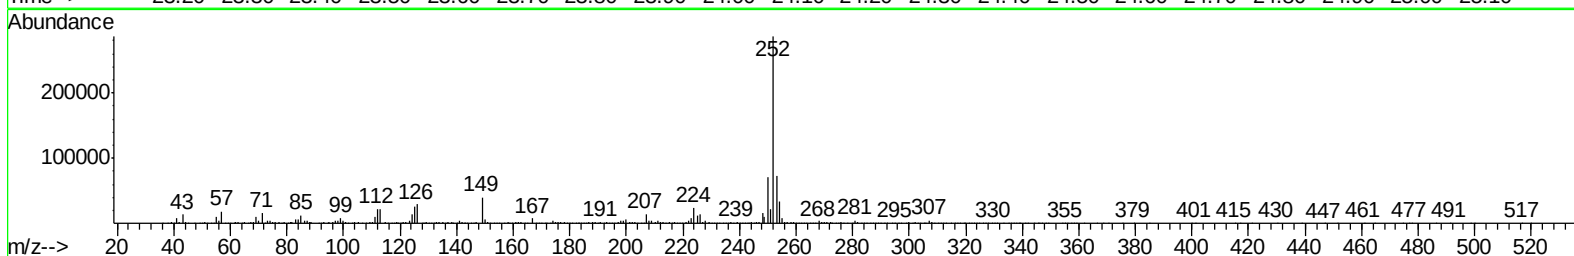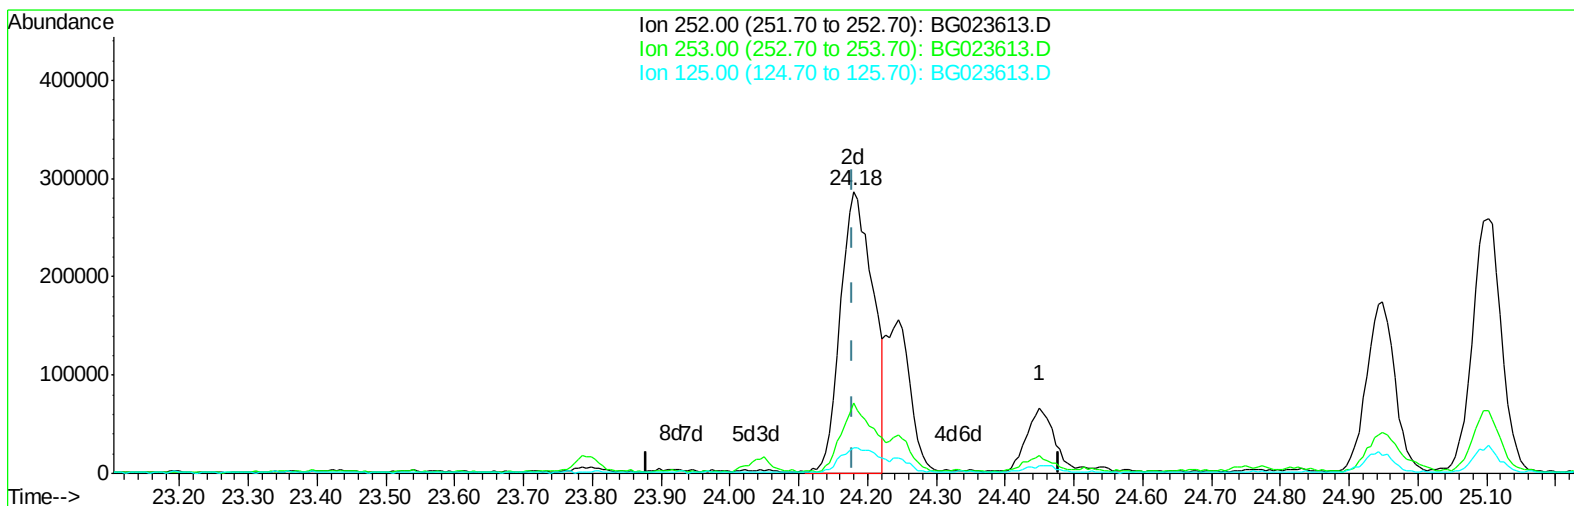

TIC: BG023613.D

(85) Benzo(b)fluoranthene

24.180min (+0.001) 15.03ng/ul m

response 948655

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	25.21
125.00	13.50	9.04#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

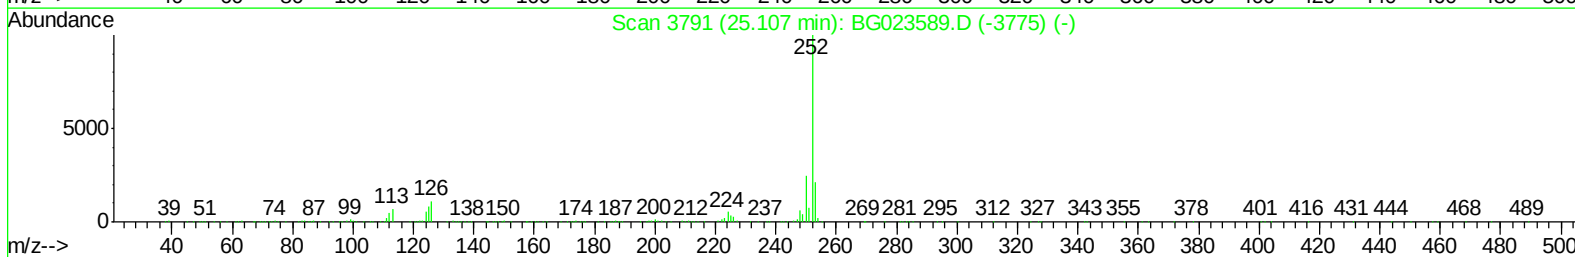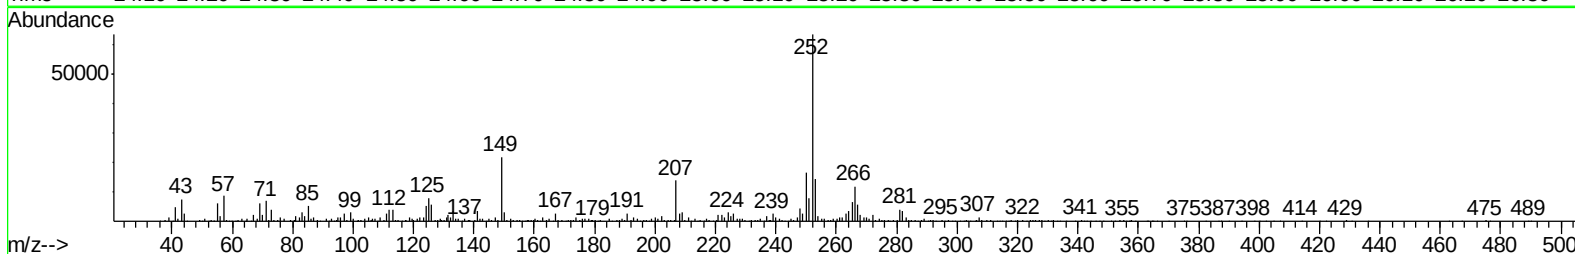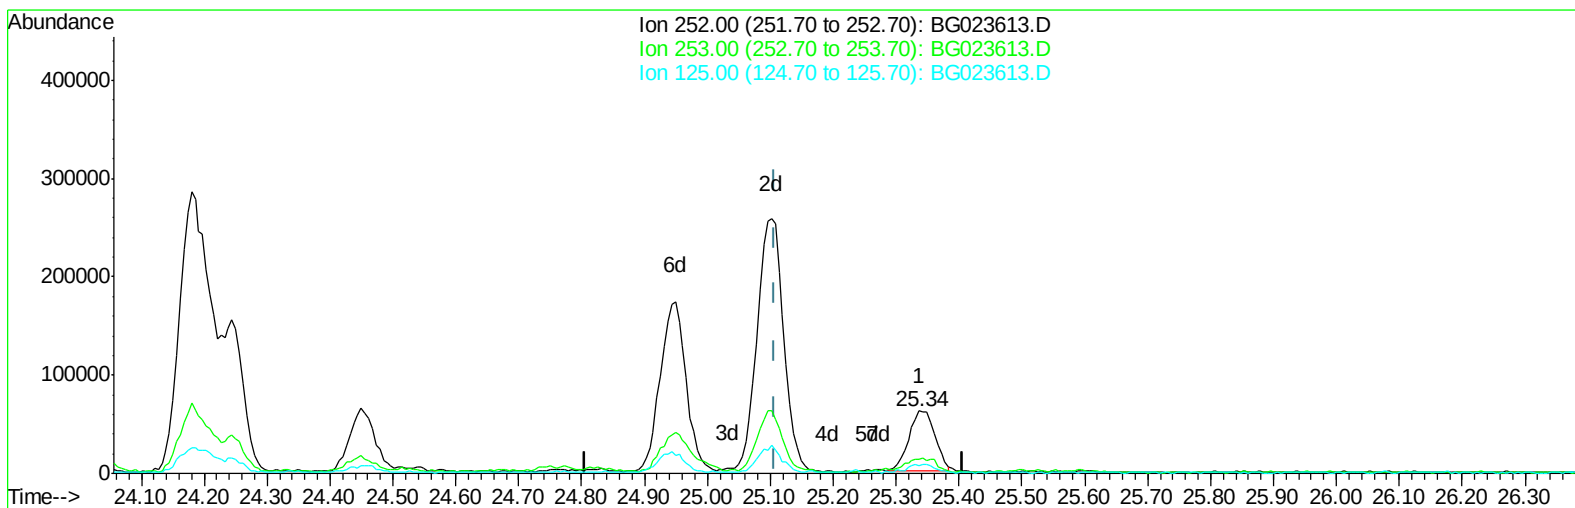

TIC: BG023613.D

(88) Benzo(a)pyrene (C)

25.337min (+0.230) 2.88ng/ul

response 175734

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	23.09
125.00	15.00	12.83
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

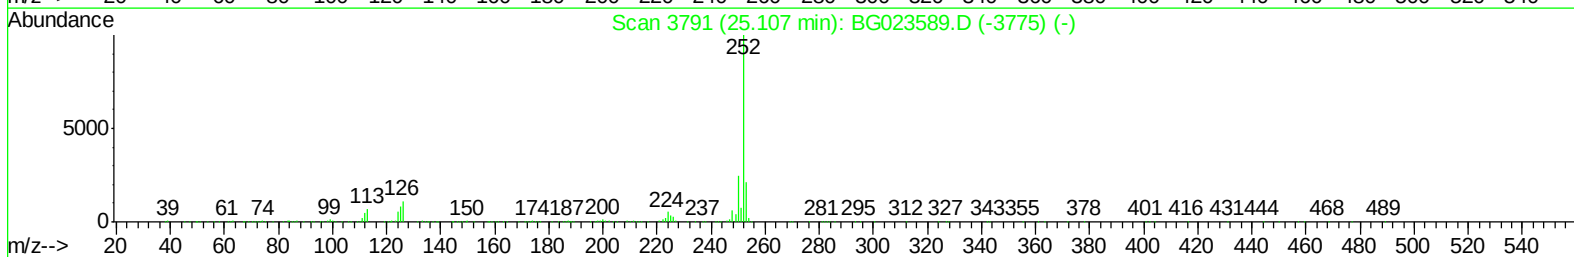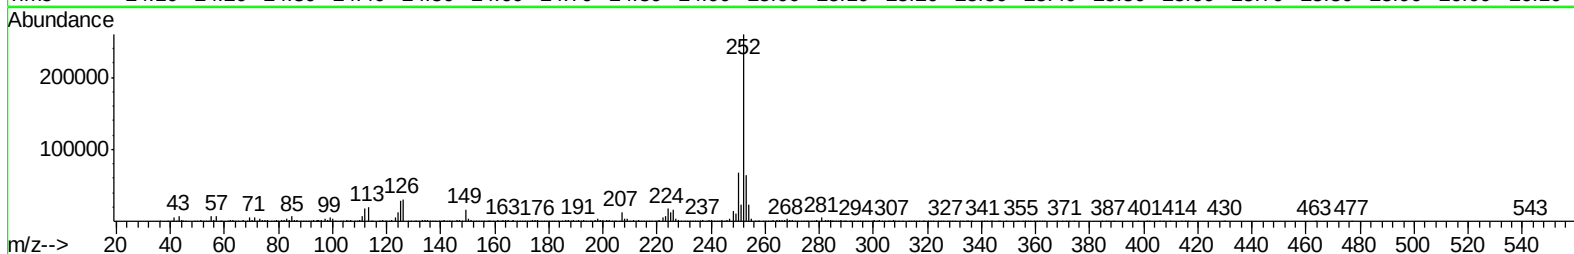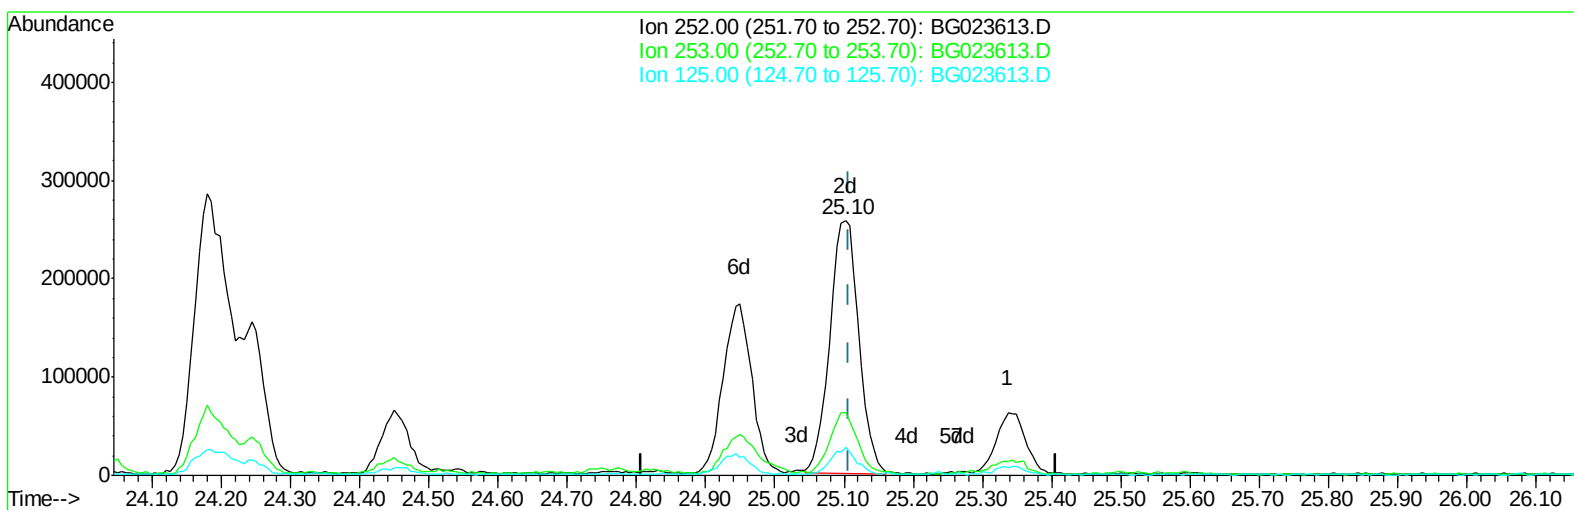

TIC: BG023613.D

(88) Benzo(a)pyrene (C)

25.102min (-0.005) 12.30ng/ul m

response 749756

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	24.59
125.00	15.00	10.89#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

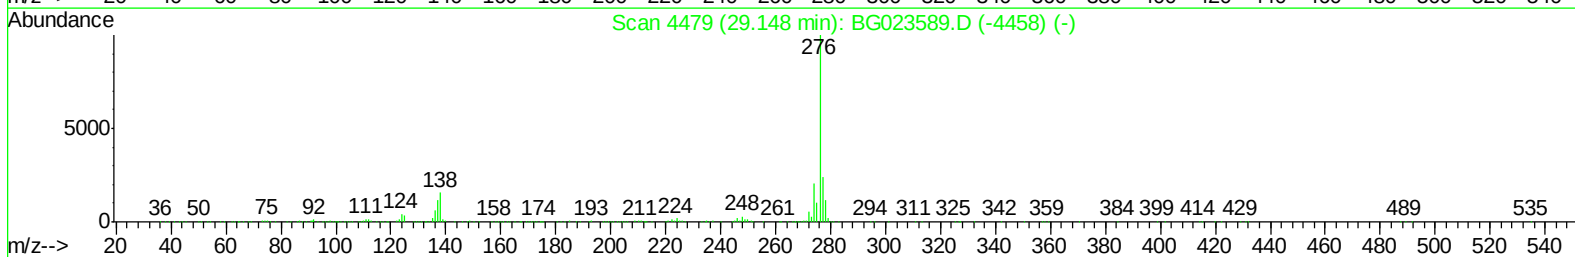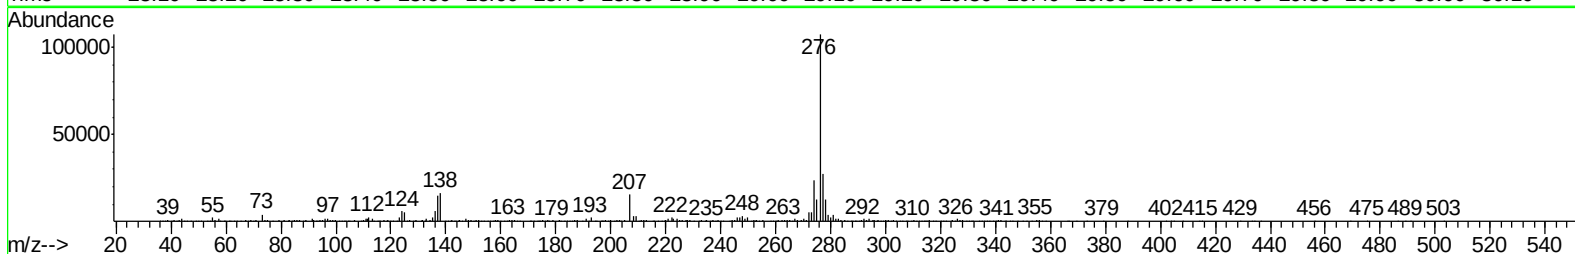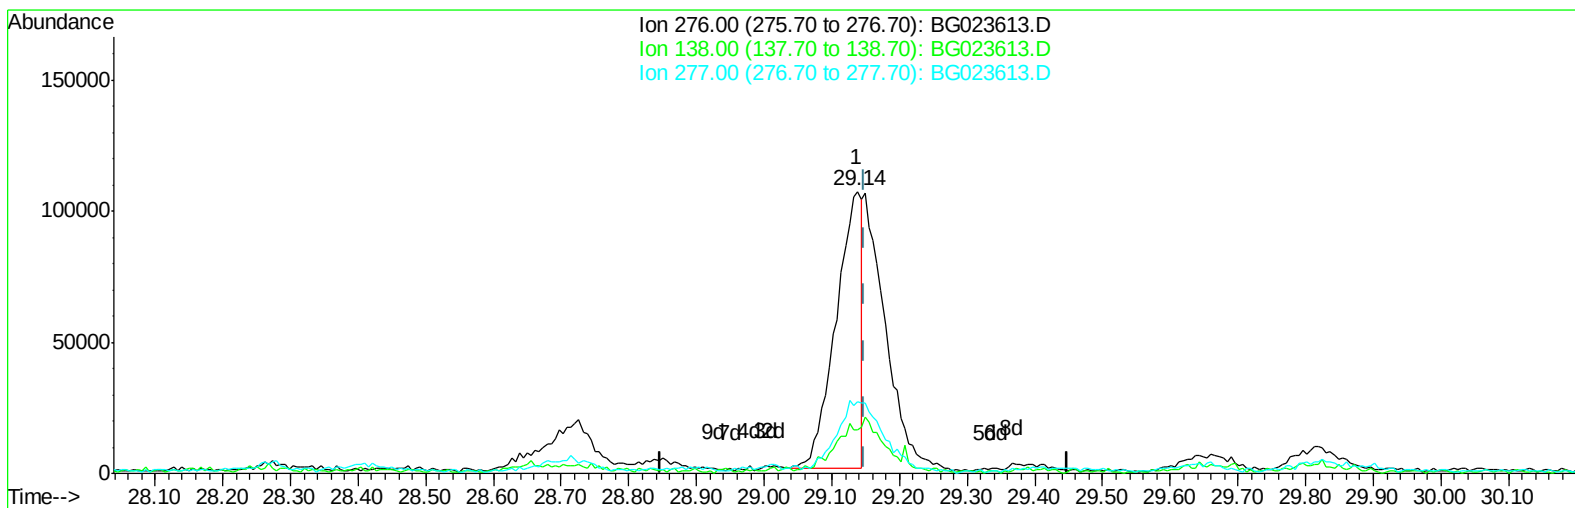

TIC: BG023613.D

(89) Indeno(1,2,3-cd)pyrene

29.138min (-0.011) 3.94ng/ul

response 282097

Ion	Exp%	Act%
276.00	100	100
138.00	26.00	15.29#
277.00	22.00	25.26
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

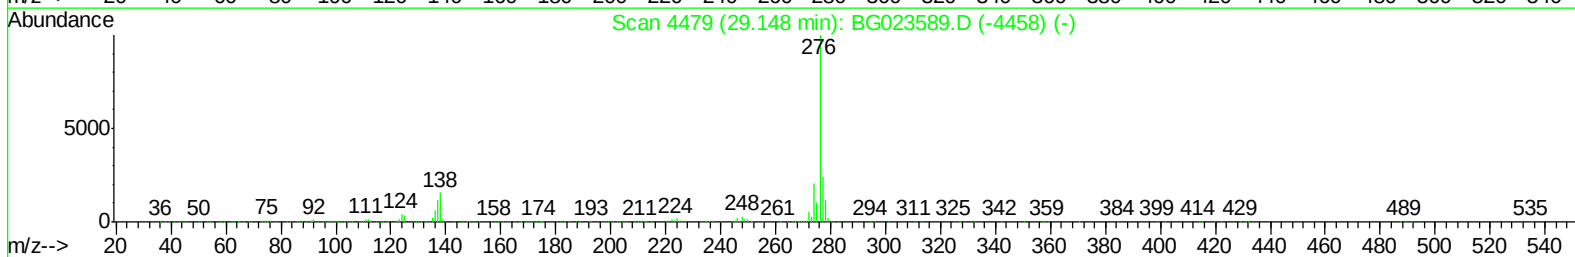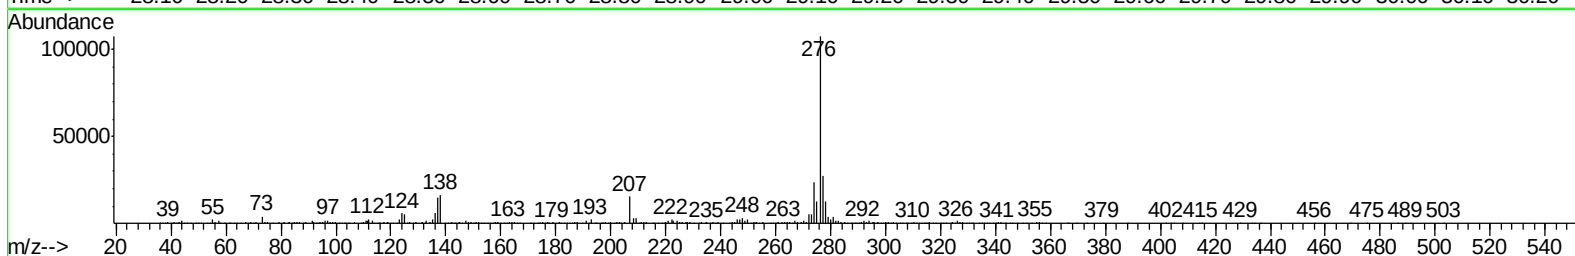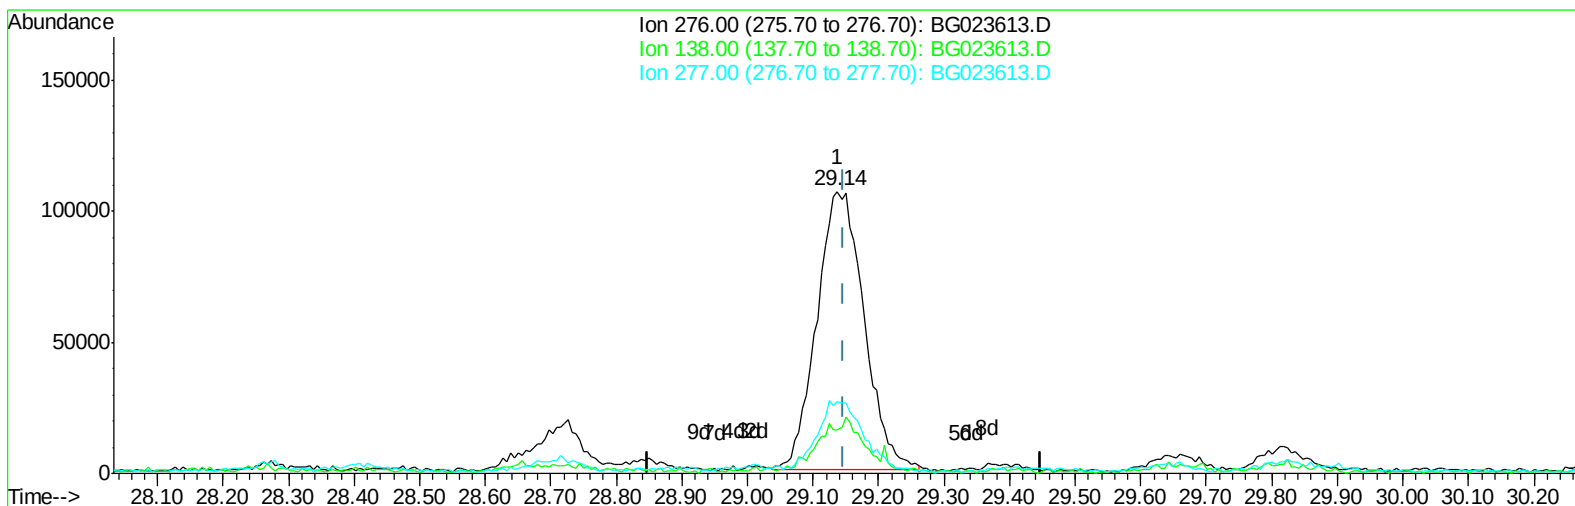

TIC: BG023613.D

(89) Indeno(1,2,3-cd)pyrene

29.138min (-0.011) 7.27ng/ul m

response 520903

Ion	Exp%	Act%
276.00	100	100
138.00	26.00	15.29#
277.00	22.00	25.26
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 05:54:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

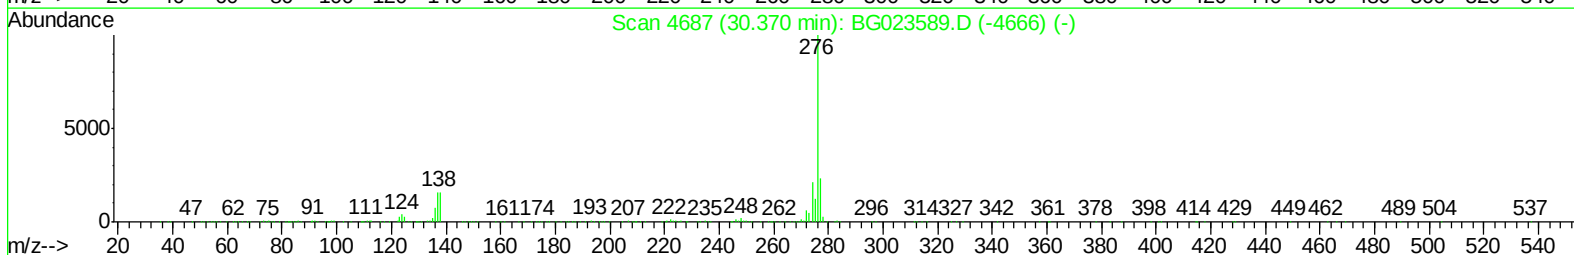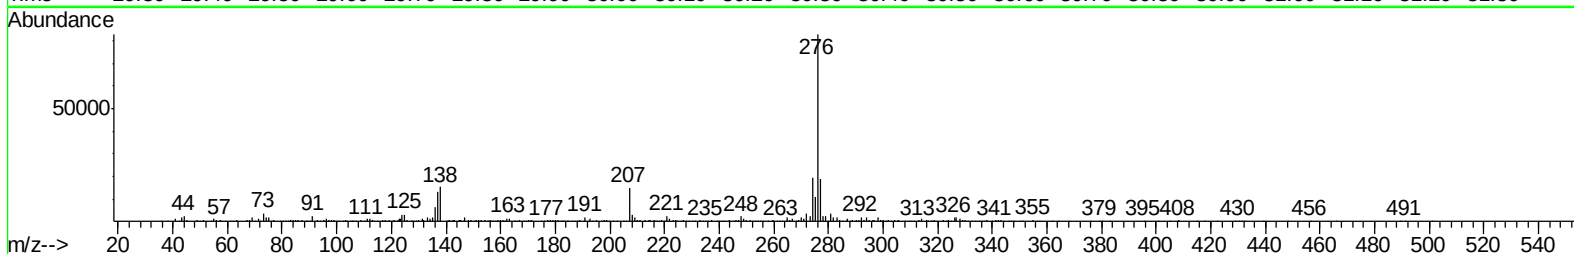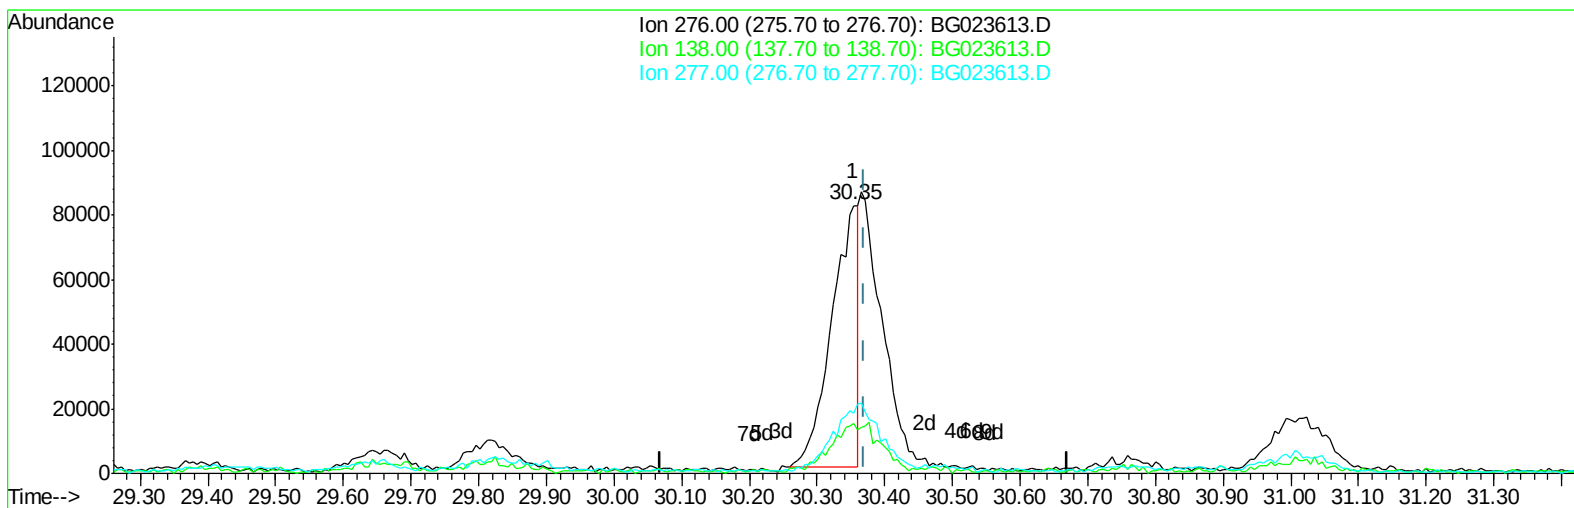

TIC: BG023613.D

(91) Benzo(g,h,i)perylene
30.354min (-0.017) 3.69ng/ul
response 218861

Ion	Exp%	Act%
276.00	100	100
138.00	27.60	18.51#
277.00	21.20	22.48
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 06:02:09 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

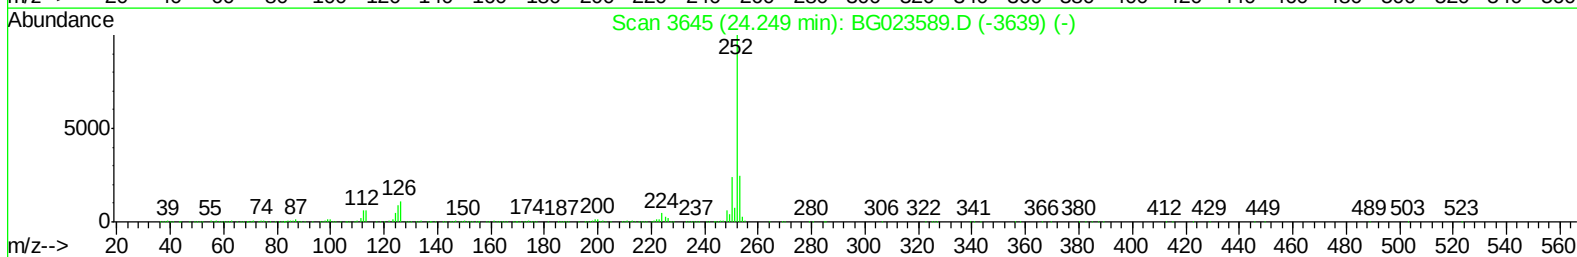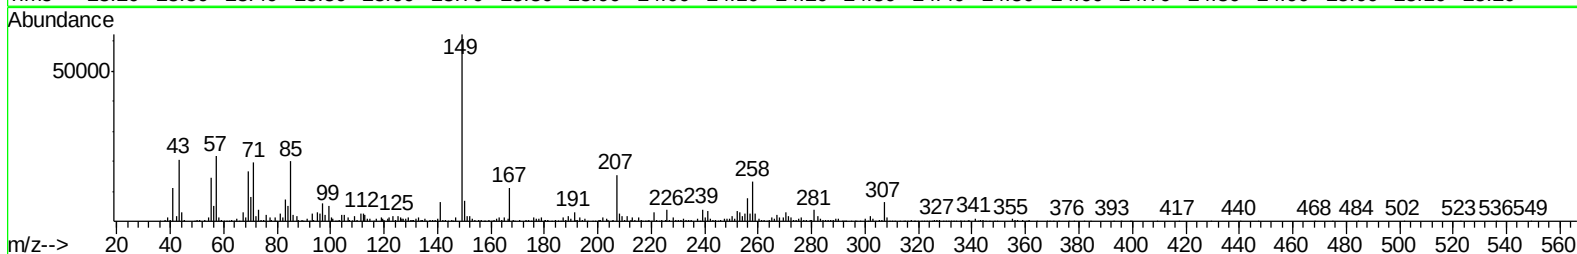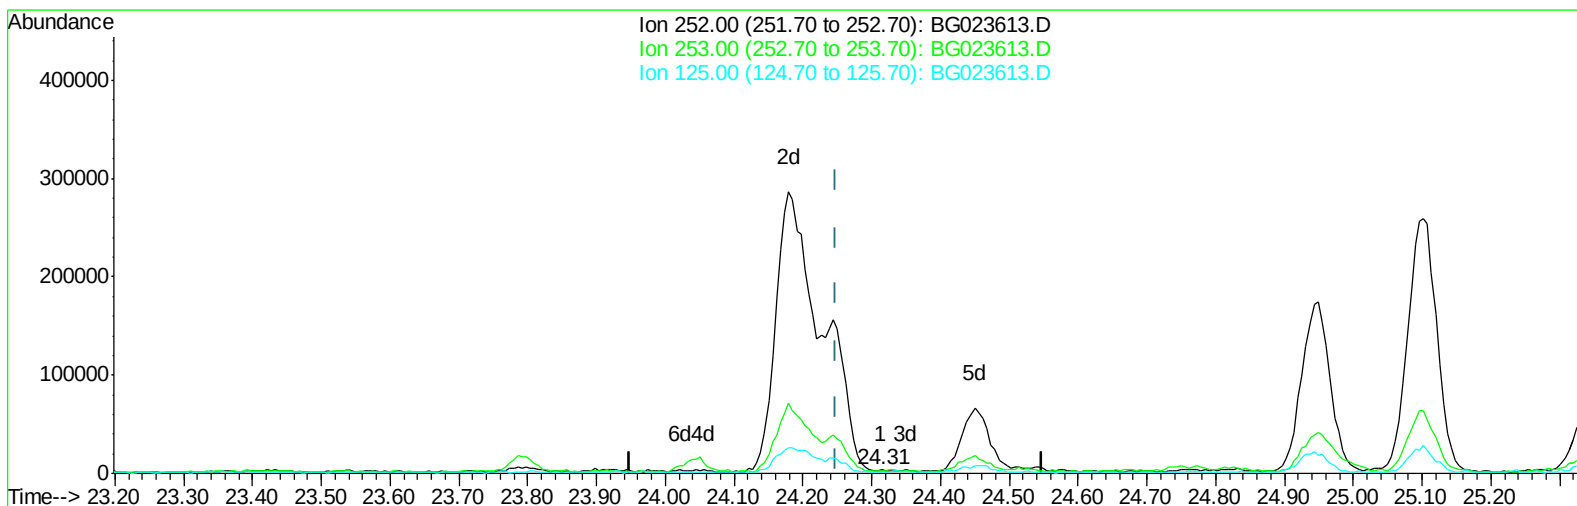

TIC: BG023613.D

(86) Benzo(k)fluoranthene

24.315min (+0.066) 0.02ng/ul

response 1004

Ion	Exp%	Act%
252.00	100	100
253.00	19.70	85.84#
125.00	13.30	53.14#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 06:02:09 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

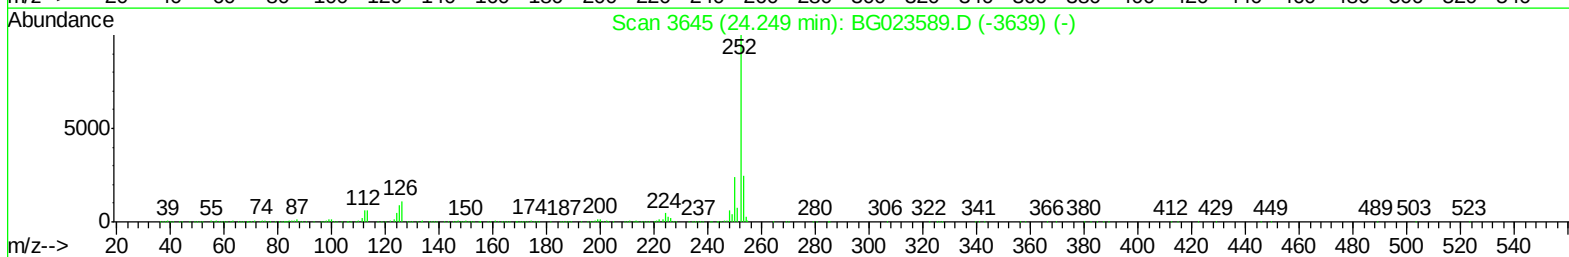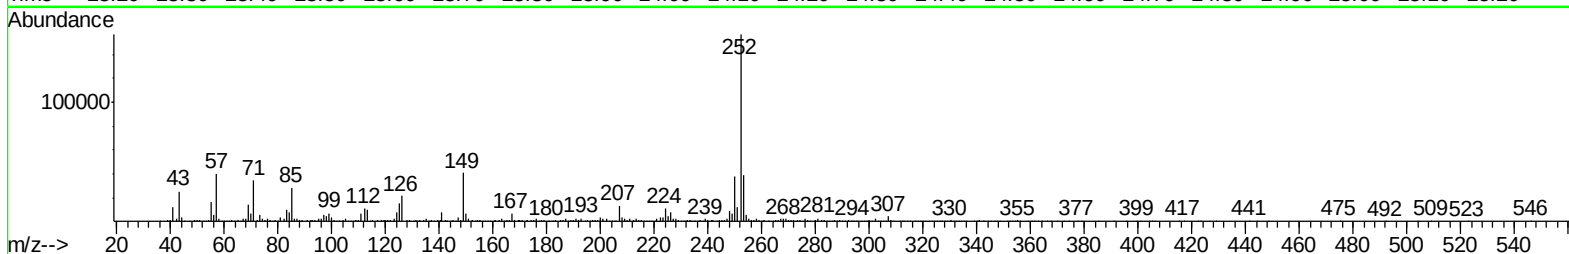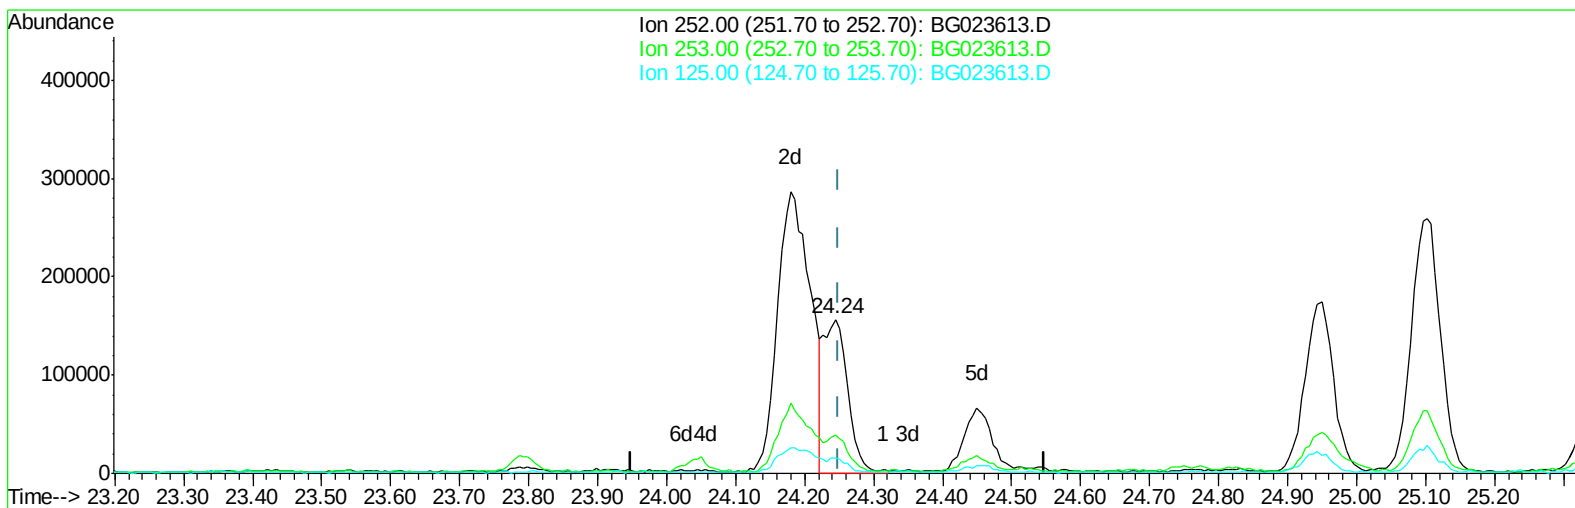

TIC: BG023613.D

(86) Benzo(k)fluoranthene

24.244min (-0.005) 6.17ng/ul m

response 383463

Ion	Exp%	Act%
252.00	100	100
253.00	19.70	25.00#
125.00	13.30	9.67#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 06:02:09 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

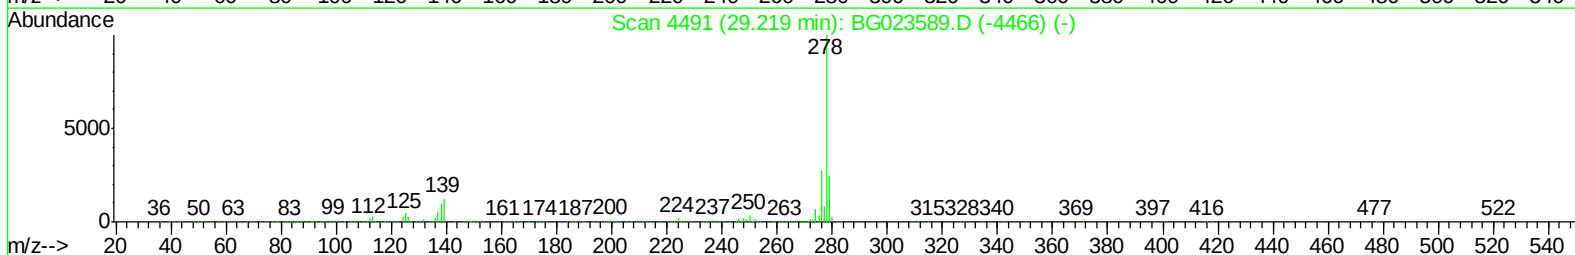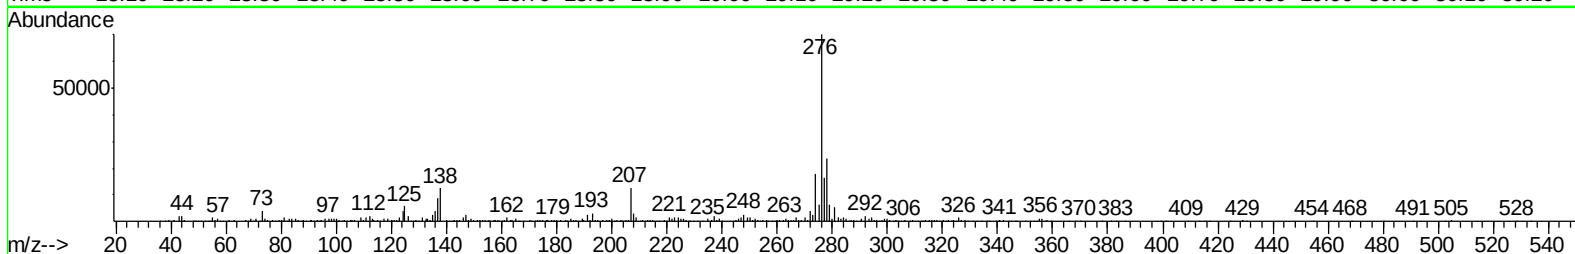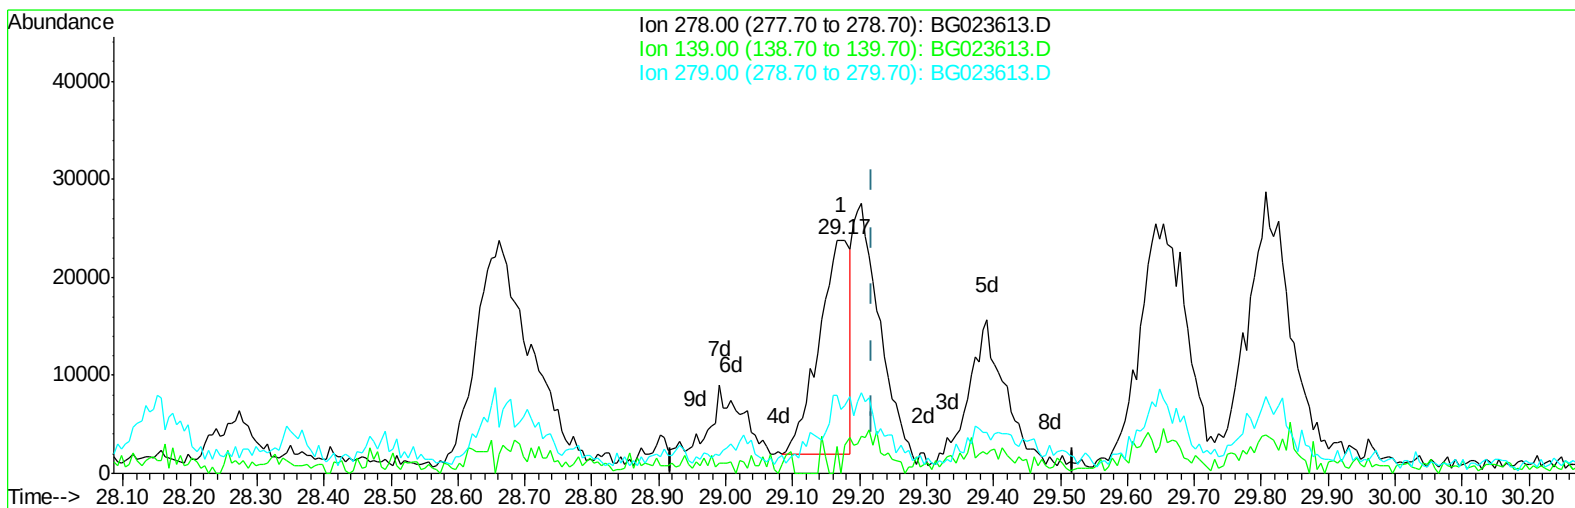

TIC: BG023613.D

(90) Dibenzo(a,h)anthracene

29.173min (-0.046) 1.13ng/ul

response 69081

Ion	Exp%	Act%
278.00	100	100
139.00	20.40	0.00#
279.00	23.90	27.25
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 06:02:09 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

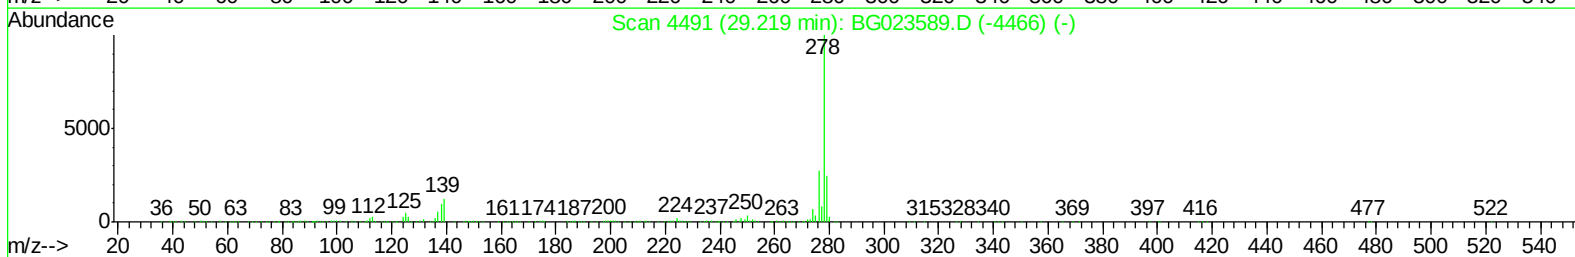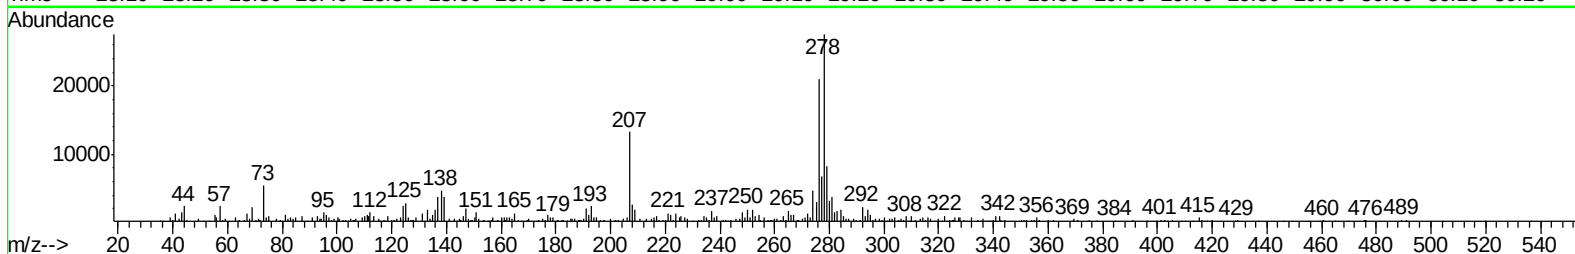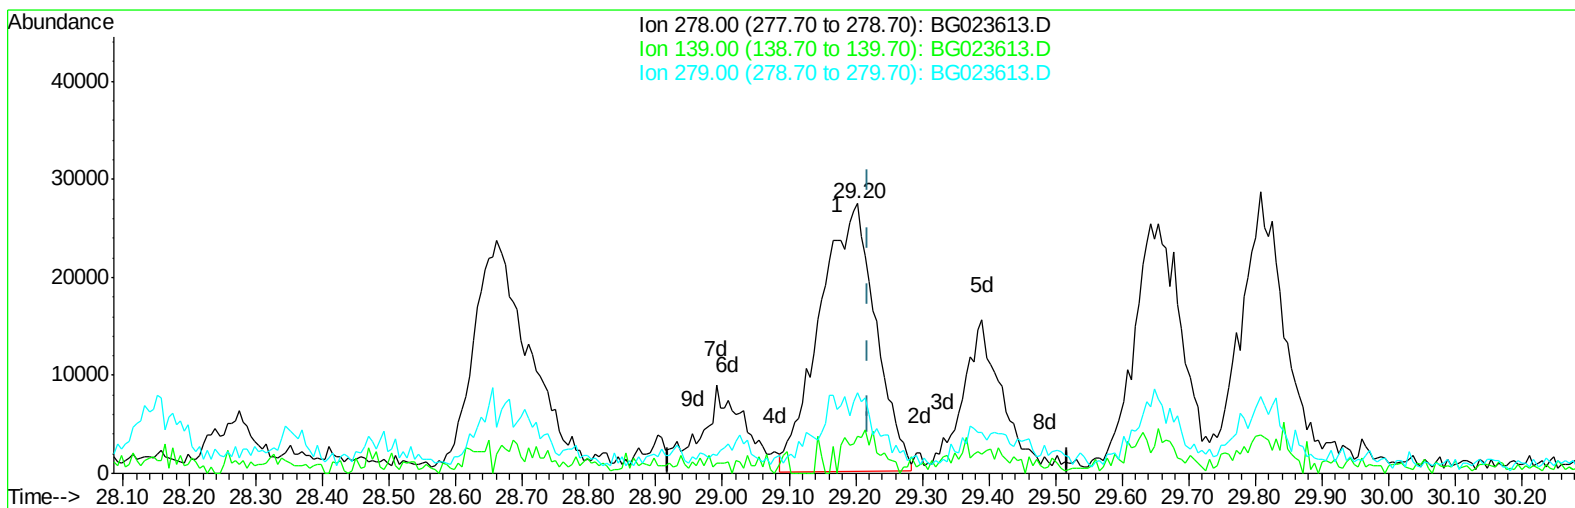

TIC: BG023613.D

(90) Dibenzo(a,h)anthracene

29.202min (-0.017) 2.61ng/ul m

response 159134

Ion	Exp%	Act%
278.00	100	100
139.00	20.40	13.70#
279.00	23.90	29.98#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
 Data File : BG023613.D
 Acq On : 11 Aug 2016 4:30
 Operator : UM/SJ
 Sample : H4384-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P001-SS001-0612-01

Manual Integrations
 APPROVED

sohil
 8/11/2016 6:14:31 PM

Quant Time: Aug 11 06:03:22 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 03:58:16 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	144954	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	693047	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	498349	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1138835	20.00	ng/ul	0.00
75) Chrysene-d12	21.87	240	1124921	20.00	ng/ul	0.00
83) Perylene-d12	25.27	264	1109936	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	10753	3.15	ng/uL	0.00
5) Phenol-d5	7.26	99	269529	18.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	176535	18.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	189782	19.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	217237	19.06	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	106589m	19.51	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	123259	19.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.56	165	223313	18.87	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	232572	16.75	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	787885	19.31	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	906451	19.74	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	119727	17.19	ng/ul	0.00
57) Fluorene-d10	15.78	176	719288	19.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	121921	16.69	ng/ul	0.00
70) Anthracene-d10	17.65	188	1034055	20.15	ng/ul	0.00
76) Pyrene-d10	19.94	212	1094159	19.22	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.03	264	997871	19.86	ng/ul	0.00

Target Compounds

						Qvalue
44) Dimethylphthalate	14.22	163	704652	17.44	ng/ul	98
47) Acenaphthylene	14.51	152	127453	2.65	ng/ul	97
69) Phenanthrene	17.59	178	722296	12.25	ng/ul	97
74) Fluoranthene	19.60	202	1232694m	20.42	ng/ul	
77) Pyrene	19.97	202	1450192	20.85	ng/ul	95
78) Butylbenzylphthalate	20.85	149	1499111	56.20	ng/ul#	83
80) Benzo(a)anthracene	21.85	228	786304	12.41	ng/ul	96
81) Bis(2-ethylhexyl)phthalate	21.72	149	222611	6.28	ng/ul	98
82) Chrysene	21.92	228	807881	14.02	ng/ul	95
85) Benzo(b)fluoranthene	24.18	252	948655m	15.03	ng/ul	
86) Benzo(k)fluoranthene	24.24	252	383463m	6.17	ng/ul	
88) Benzo(a)pyrene	25.10	252	749756m	12.30	ng/ul	
89) Indeno(1,2,3-cd)pyrene	29.14	276	520903m	7.27	ng/ul	
90) Dibenzo(a,h)anthracene	29.20	278	159134m	2.61	ng/ul	
91) Benzo(g,h,i)perylene	30.37	276	418650m	7.05	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023613.D
Acq On : 11 Aug 2016 4:30
Operator : UM/SJ
Sample : H4384-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS001-0612-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:14:31 PM

Quant Time: Aug 11 06:03:22 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

