

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
 Data File : BG023600.D
 Acq On : 10 Aug 2016 20:03
 Operator : UM/SJ
 Sample : H4384-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P001-SS002-0002-01

Manual Integrations
 APPROVED

sohil
 8/11/2016 6:12:52 PM

Quant Time: Aug 11 08:24:44 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 03:58:16 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	160524	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	742421	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	513270	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1238417	20.00	ng/ul	0.00
75) Chrysene-d12	21.87	240	1281258	20.00	ng/ul	0.00
83) Perylene-d12	25.26	264	1270193	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	14663	3.88	ng/uL	0.00
5) Phenol-d5	7.26	99	358018	22.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	250287	24.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	251031	22.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	268261	21.25	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	143815m	24.58	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	159848	23.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	284241	22.42	ng/ul	0.00
29) 4-Chloroaniline-d4	11.08	131	370555	24.91	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	1018770	24.24	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	1182024	24.99	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	176292	24.57	ng/ul	0.01
57) Fluorene-d10	15.78	176	917197	23.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	173026	21.78	ng/ul	0.00
70) Anthracene-d10	17.65	188	1378158	24.70	ng/ul	0.00
76) Pyrene-d10	19.94	212	1527428	23.55	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.02	264	1438326	25.02	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	14.23	163	818094	19.66 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023600.D
Acq On : 10 Aug 2016 20:03
Operator : UM/SJ
Sample : H4384-06
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
P001-SS002-0002-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:12:52 PM

Quant Time: Aug 11 08:24:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

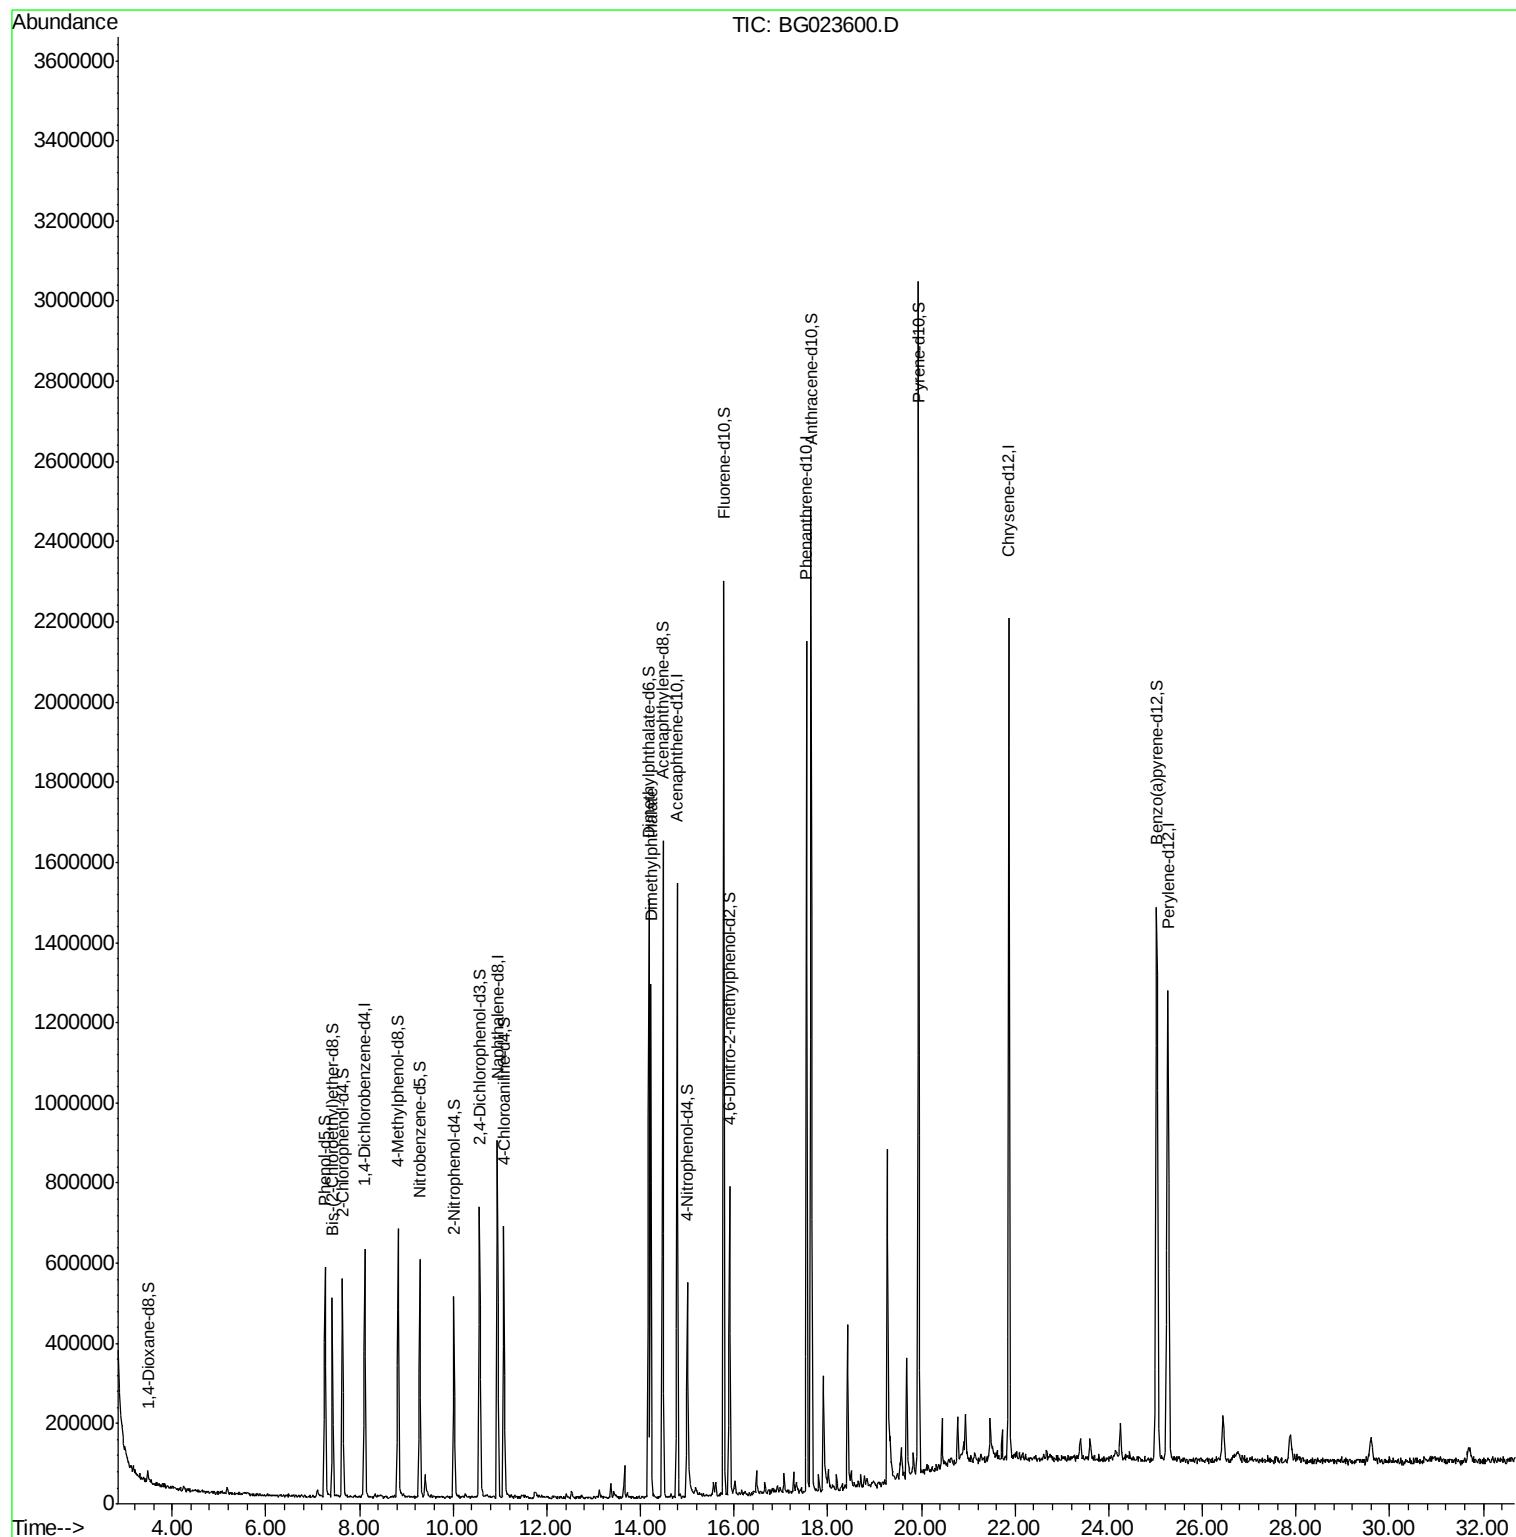

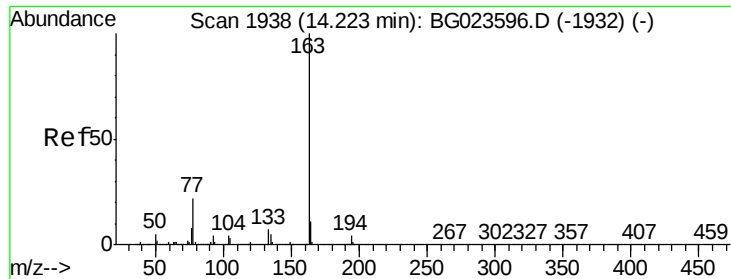

#44
 Dimethylphthalate
 Concen: 19.66 ng/ul
 RT: 14.23 min Scan# 1938
 Delta R.T. 0.00 min
 Lab File: BG023600.D
 Acq: 10 Aug 2016 20:03

Instrument :
 BNA_G
 ClientSampleId :
 P001-SS002-0002-01

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.6	3.4	5.2
164	10.5	8.8	13.2

Manual Integrations
 APPROVED

sohil
 8/11/2016 6:12:52 PM

