

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
 Data File : BG023603.D
 Acq On : 10 Aug 2016 21:56
 Operator : UM/SJ
 Sample : H4384-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P001-SS002-1218-01

Manual Integrations
 APPROVED

sohil
 8/11/2016 6:12:58 PM

Quant Time: Aug 11 05:19:55 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 03:58:16 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	149824	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	667127	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	454545	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1147093	20.00	ng/ul	0.00
75) Chrysene-d12	21.87	240	1248980	20.00	ng/ul	0.00
83) Perylene-d12	25.27	264	1208967	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	12942	3.67	ng/uL	0.00
5) Phenol-d5	7.27	99	294720	19.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	209305	21.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	212088	20.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	208007	17.65	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	116407	22.14	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	133321	22.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	233885	20.53	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	296958	22.22	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	837745	22.51	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	945762	22.58	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	140622m	22.13	ng/ul	0.01
57) Fluorene-d10	15.78	176	764350	22.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	141441m	19.22	ng/ul	0.00
70) Anthracene-d10	17.65	188	1170927	22.66	ng/ul	0.00
76) Pyrene-d10	19.94	212	1393637	22.04	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.03	264	1250597	22.85	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	14.22	163	271090	7.36 ng/ul#	99
69) Phenanthrene	17.59	178	65372	1.10 ng/ul	99
74) Fluoranthene	19.60	202	118037	1.94 ng/ul#	91
77) Pyrene	19.97	202	151936	1.97 ng/ul#	91
82) Chrysene	21.91	228	77118m	1.21 ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081016\
Data File : BG023603.D
Acq On : 10 Aug 2016 21:56
Operator : UM/SJ
Sample : H4384-09
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
P001-SS002-1218-01

Manual Integrations
APPROVED

sohil
8/11/2016 6:12:58 PM

Quant Time: Aug 11 05:19:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 03:58:16 2016
Response via : Initial Calibration

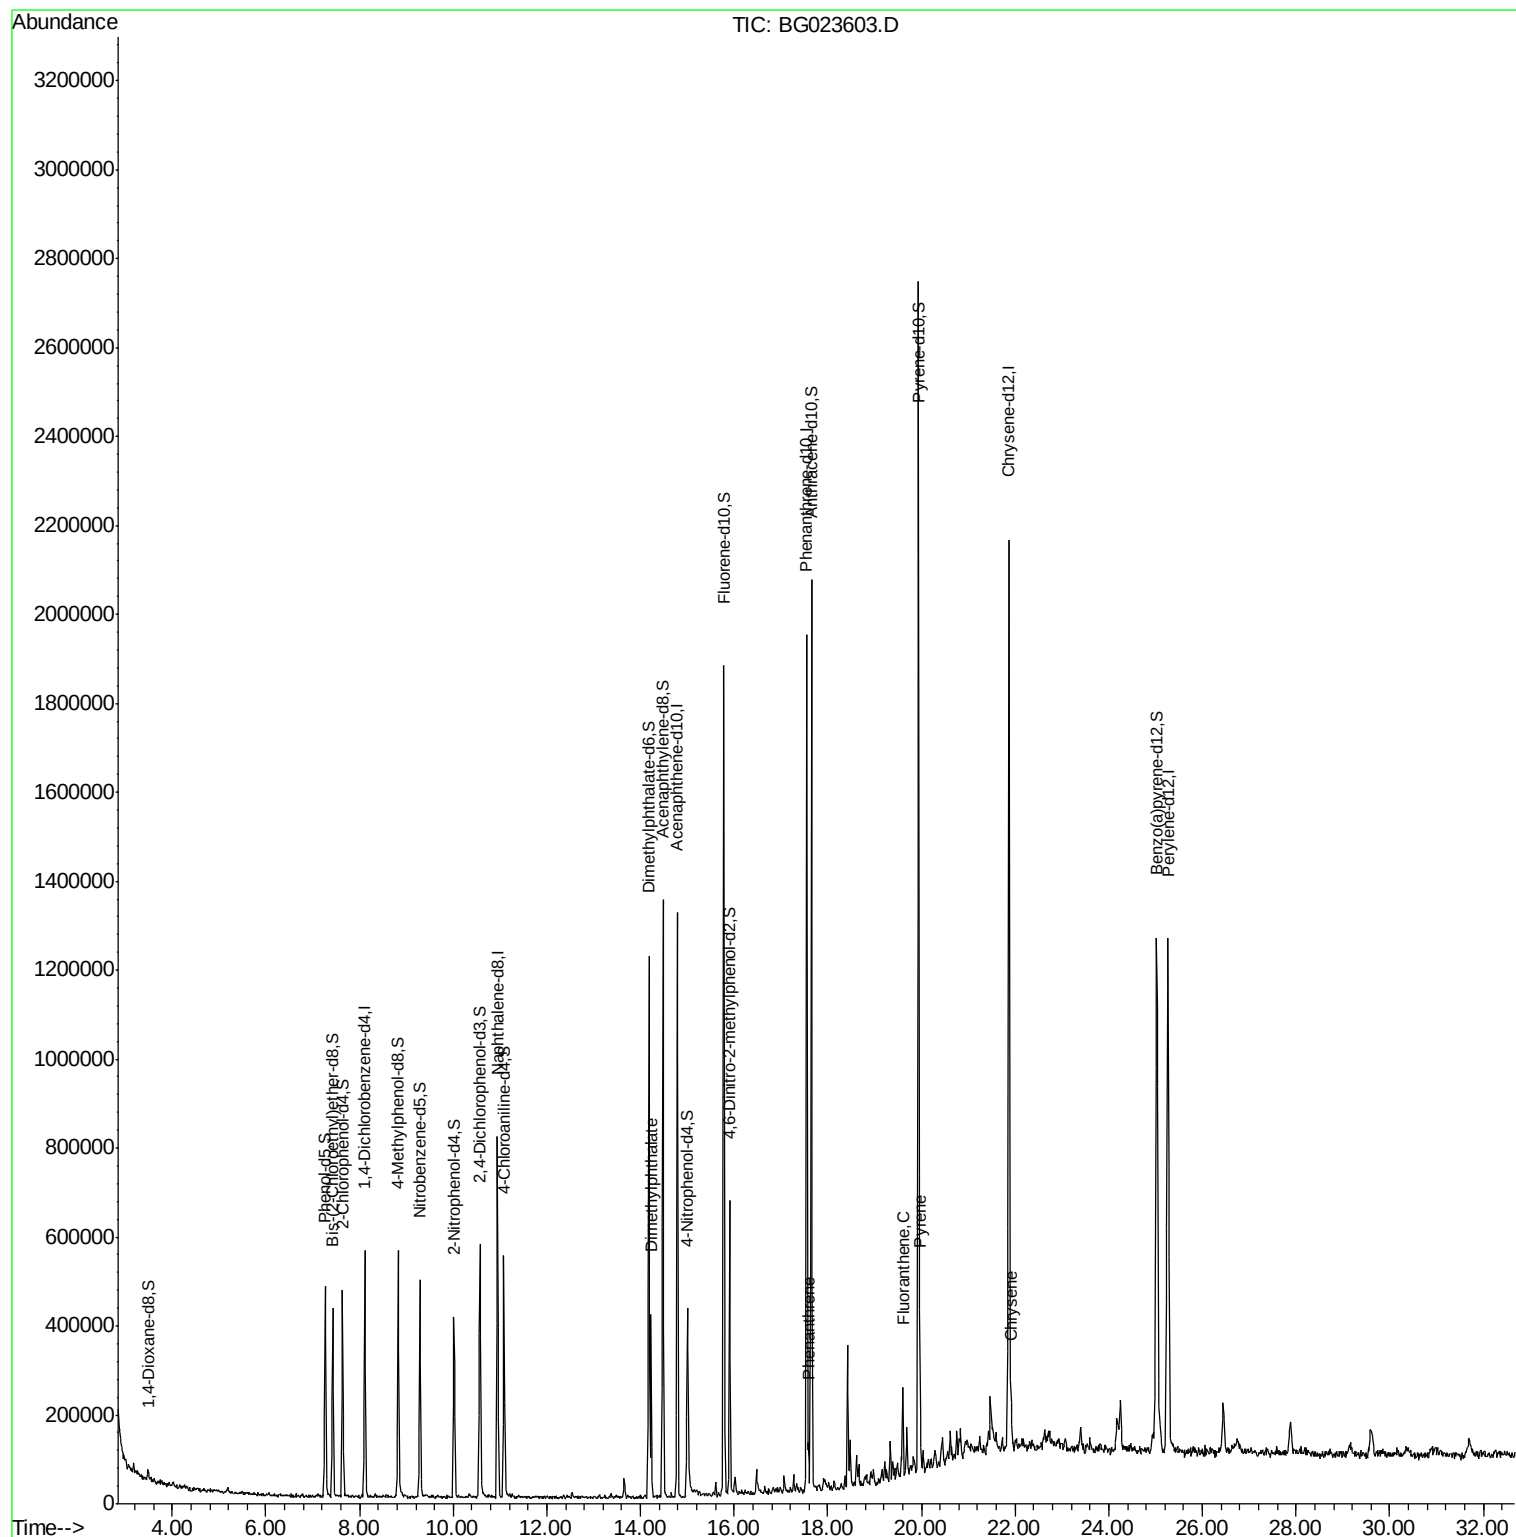

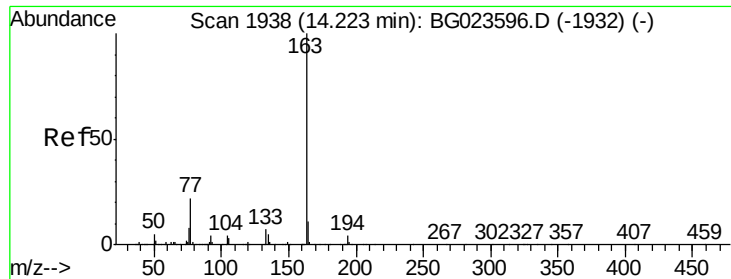





#44
Dimethylphthalate
Concen: 7.36 ng/ul
RT: 14.22 min Scan# 1938
Delta R.T. 0.00 min
Lab File: BG023603.D
Acq: 10 Aug 2016 21:56

Instrument :
BNA_G
ClientSampleId :
P001-SS002-1218-01

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	271090		
194	3.2		3.4	5.2#
164	11.1		8.8	13.2




Manual Integrations
APPROVED


sohil
8/11/2016 6:12:58 PM

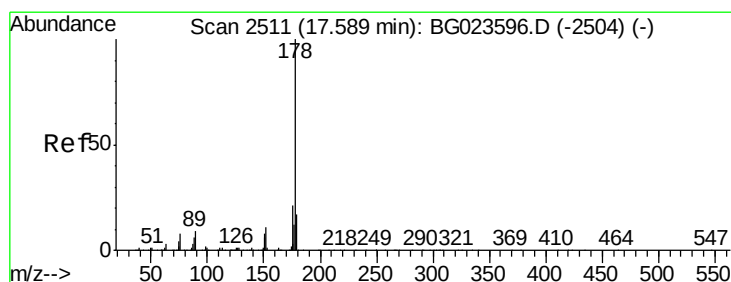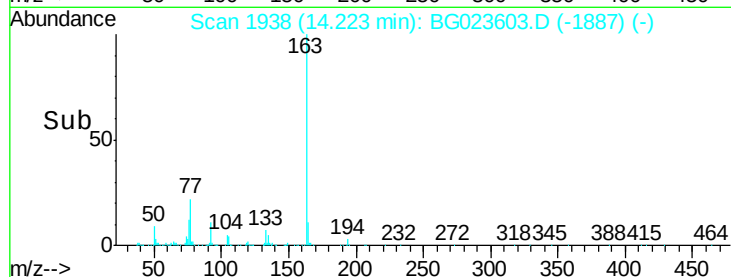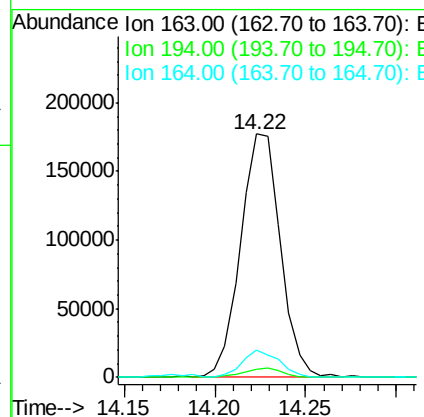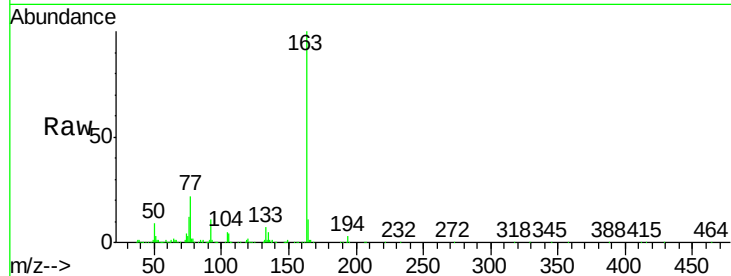

#69
Phenanthrene
Concen: 1.10 ng/ul
RT: 17.59 min Scan# 2512
Delta R.T. 0.01 min
Lab File: BG023603.D
Acq: 10 Aug 2016 21:56

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	65372		
179	15.6		12.9	19.3
176	19.5		15.8	23.8

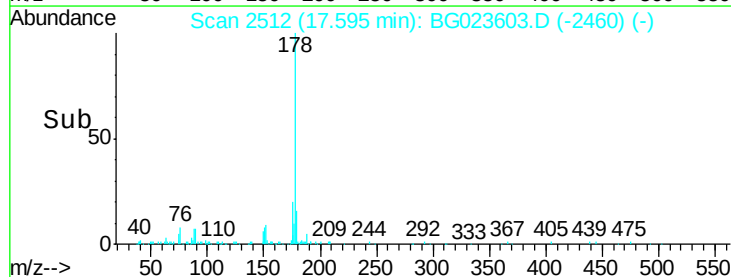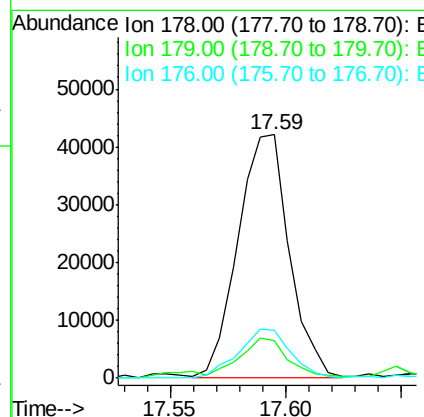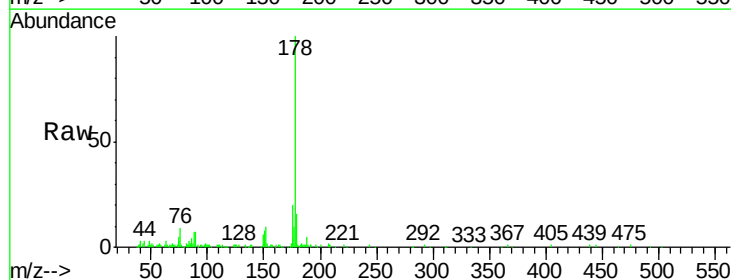

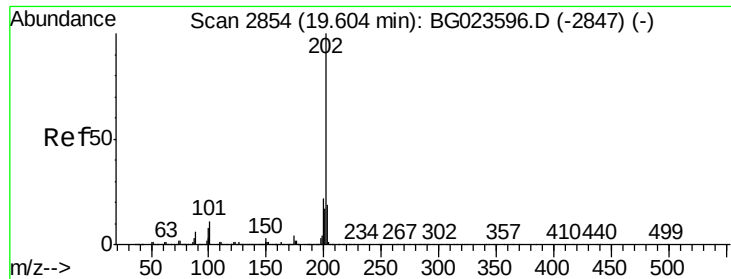

#74

Fluoranthene

Concen: 1.94 ng/ul

RT: 19.60 min Scan# 2854

Delta R.T. 0.00 min

Lab File: BG023603.D


Acq: 10 Aug 2016 21:56

Instrument :

BNA_G

ClientSampleId :




P001-SS002-1218-01

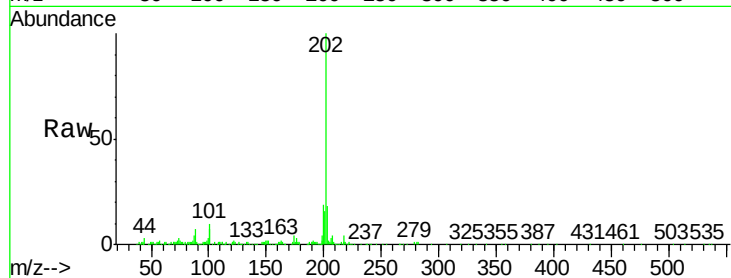

Tgt	Ion	Ratio	Resp	Lower	Upper
202	100		118037		
101	10.0	10.6	16.0#		
100	7.0	8.7	13.1#		

Manual Integrations
APPROVED

sohil
8/11/2016 6:12:58 PM

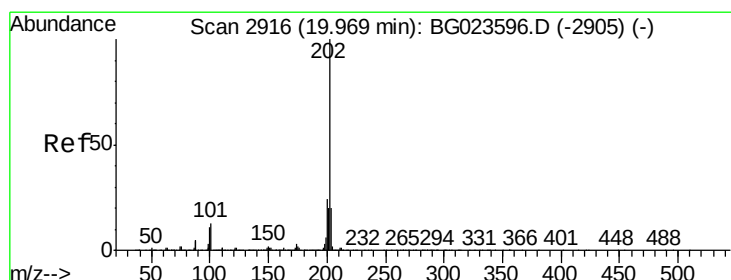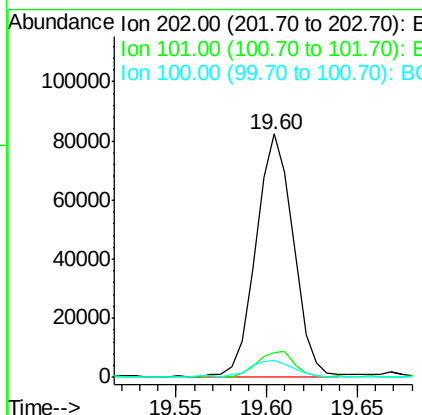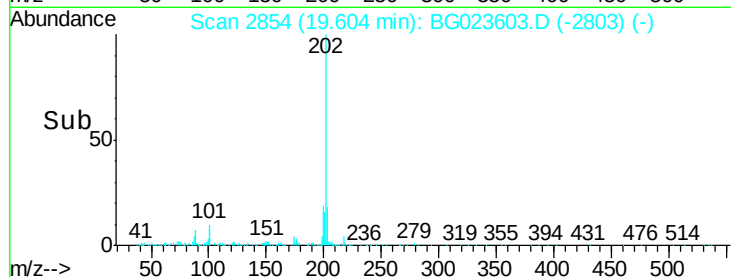

#77

Pyrene

Concen: 1.97 ng/ul




RT: 19.97 min Scan# 2916


Delta R.T. 0.00 min

Lab File: BG023603.D

Acq: 10 Aug 2016 21:56

Tgt	Ion	Ratio	Resp	Lower	Upper
202	100		151936		
101	10.4	12.5	18.7#		
100	10.6	10.2	15.4		

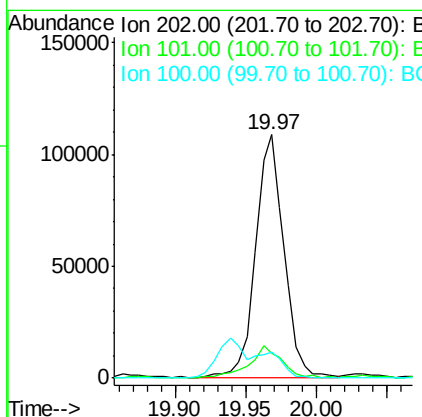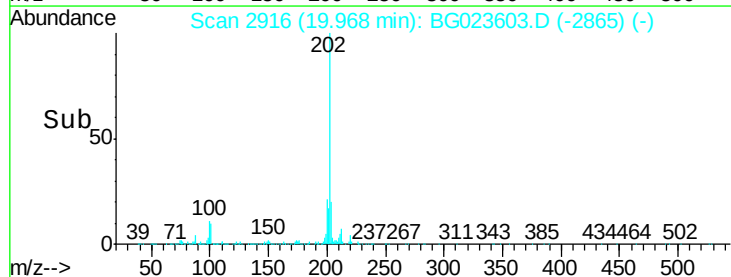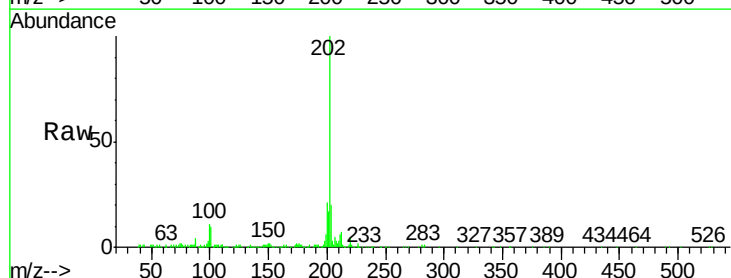

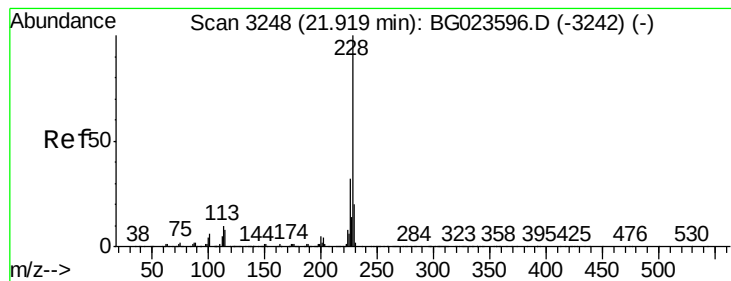

#82

Chrysene

Concen: 1.21 ng/ul m

RT: 21.91 min Scan# 3247

Delta R.T. -0.00 min

Lab File: BG023603.D


Acq: 10 Aug 2016 21:56

Instrument :

BNA_G

ClientSampleId :

P001-SS002-1218-01

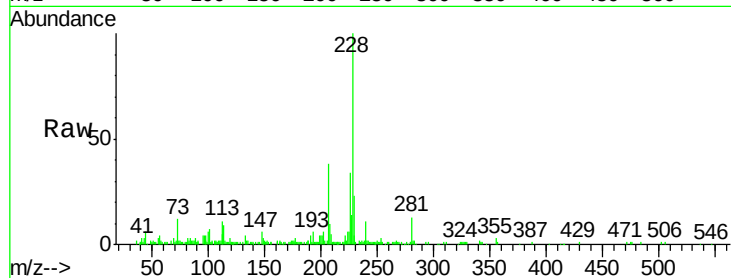

Tgt Ion: 228 Resp: 77118

Ion Ratio Lower Upper

228 100

226 33.9 24.2 36.4

229 23.0 15.0 22.6#

Manual Integrations

APPROVED

sohil

8/11/2016 6:12:58 PM

