

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081017\
 Data File : BG028264.D
 Acq On : 10 Aug 2017 18:43
 Operator : SJ/JU
 Sample : I4630-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA1

Quant Time: Aug 11 01:11:24 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 11 01:09:14 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	34702	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	145476	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	107826	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.71	188	315129	20.00	ng/ul	0.00
75) Chrysene-d12	22.04	240	365222	20.00	ng/ul	0.00
83) Perylene-d12	25.53	264	348942	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.84	96	3879	5.21	ng/uL	0.00
5) Phenol-d5	7.50	99	20321	5.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.67	67	54412	22.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.89	132	49915	20.76	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	38164	11.98	ng/ul	0.00
19) Nitrobenzene-d5	9.69	128	116	0.10	ng/ul	0.17
22) 2-Nitrophenol-d4	10.25	143	35780	28.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	66109	25.62	ng/ul	0.00
29) 4-Chloroaniline-d4	11.27	131	8378	2.92	ng/ul	-0.03
43) Dimethylphthalate-d6	14.35	166	316567	33.01	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	300621	27.80	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	12894	8.46	ng/ul	0.02
57) Fluorene-d10	15.94	176	258594	30.06	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	70556	34.47	ng/ul	0.00
70) Anthracene-d10	17.81	188	530519	35.11	ng/ul	0.00
76) Pyrene-d10	20.08	212	646259	34.51	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.30	264	580379	35.53	ng/ul	0.00

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
17) Hexachloroethane	9.47	117	2228	2.295	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081017\
 Data File : BG028264.D
 Acq On : 10 Aug 2017 18:43
 Operator : SJ/JU
 Sample : I4630-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 C0AA1

Quant Time: Aug 11 01:11:24 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 11 01:09:14 2017
 Response via : Initial Calibration

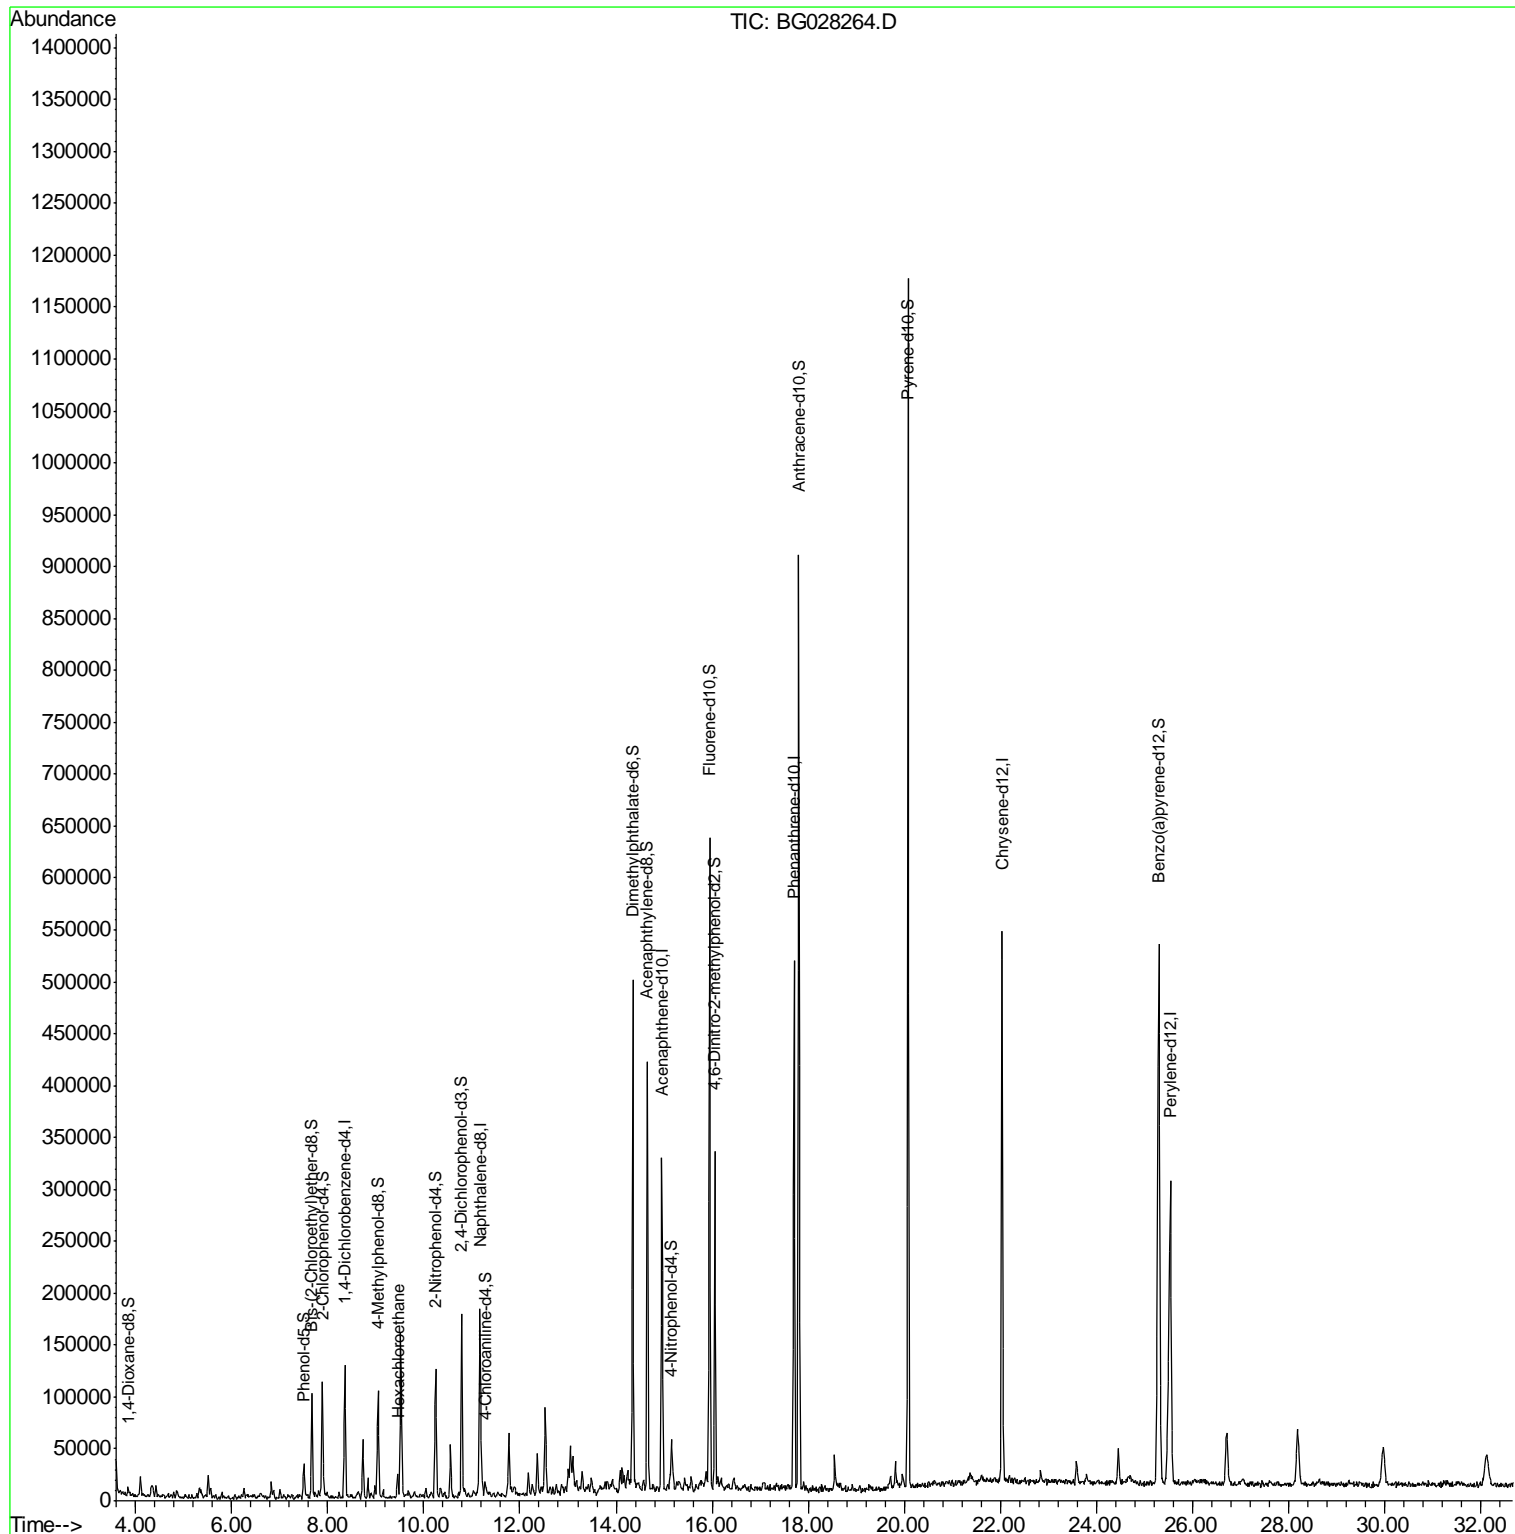

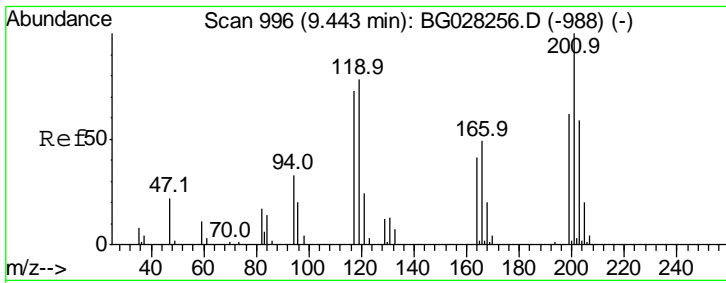

#17
 Hexachloroethane
 Concen: 2.295 ng/ul
 RT: 9.47 min Scan# 1001
 Delta R.T. 0.03 min
 Lab File: BG028264.D
 Acq: 10 Aug 2017 18:43

Instrument :
 BNA_G
ClientSampled :
 C0AA1

Tot Ion: 117 Resp: 2228

Ion	Ratio	Lower	Upper
117	100		
201	0.0	91.9	137.9#
199	0.0	64.3	96.5#

