

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081017\
 Data File : BG028288.D
 Acq On : 11 Aug 2017 11:49
 Operator : SJ/JU
 Sample : I4455-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG1

Quant Time: Aug 11 13:00:26 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 11 04:08:50 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	36868	20.00	ng/ul	0.00
18) Naphthalene-d8	11.18	136	161841	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	124663	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.71	188	336565	20.00	ng/ul	0.00
75) Chrysene-d12	22.03	240	393297	20.00	ng/ul	0.00
83) Perylene-d12	25.54	264	381088	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.84	96	3692	4.66	ng/uL	0.00
5) Phenol-d5	7.50	99	67912	16.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.67	67	44468	17.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.89	132	49032	19.19	ng/ul	0.00
13) 4-Methylphenol-d8	9.04	113	57185	16.90	ng/ul	0.00
19) Nitrobenzene-d5	9.52	128	26287	20.77	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	31647	22.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	56842	19.80	ng/ul	0.00
29) 4-Chloroaniline-d4	11.31	131	71986	22.53	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	235900	21.28	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	276555	22.12	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	36351	20.62	ng/ul	0.00
57) Fluorene-d10	15.95	176	217715	21.89	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	42581	19.48	ng/ul	0.00
70) Anthracene-d10	17.80	188	386915	23.97	ng/ul	0.00
76) Pyrene-d10	20.08	212	474106	23.51	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.30	264	560727	31.43	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.40	163	21489	2.105	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081017\
Data File : BG028288.D
Acq On : 11 Aug 2017 11:49
Operator : SJ/JU
Sample : I4455-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG1

Quant Time: Aug 11 13:00:26 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 11 04:08:50 2017
Response via : Initial Calibration

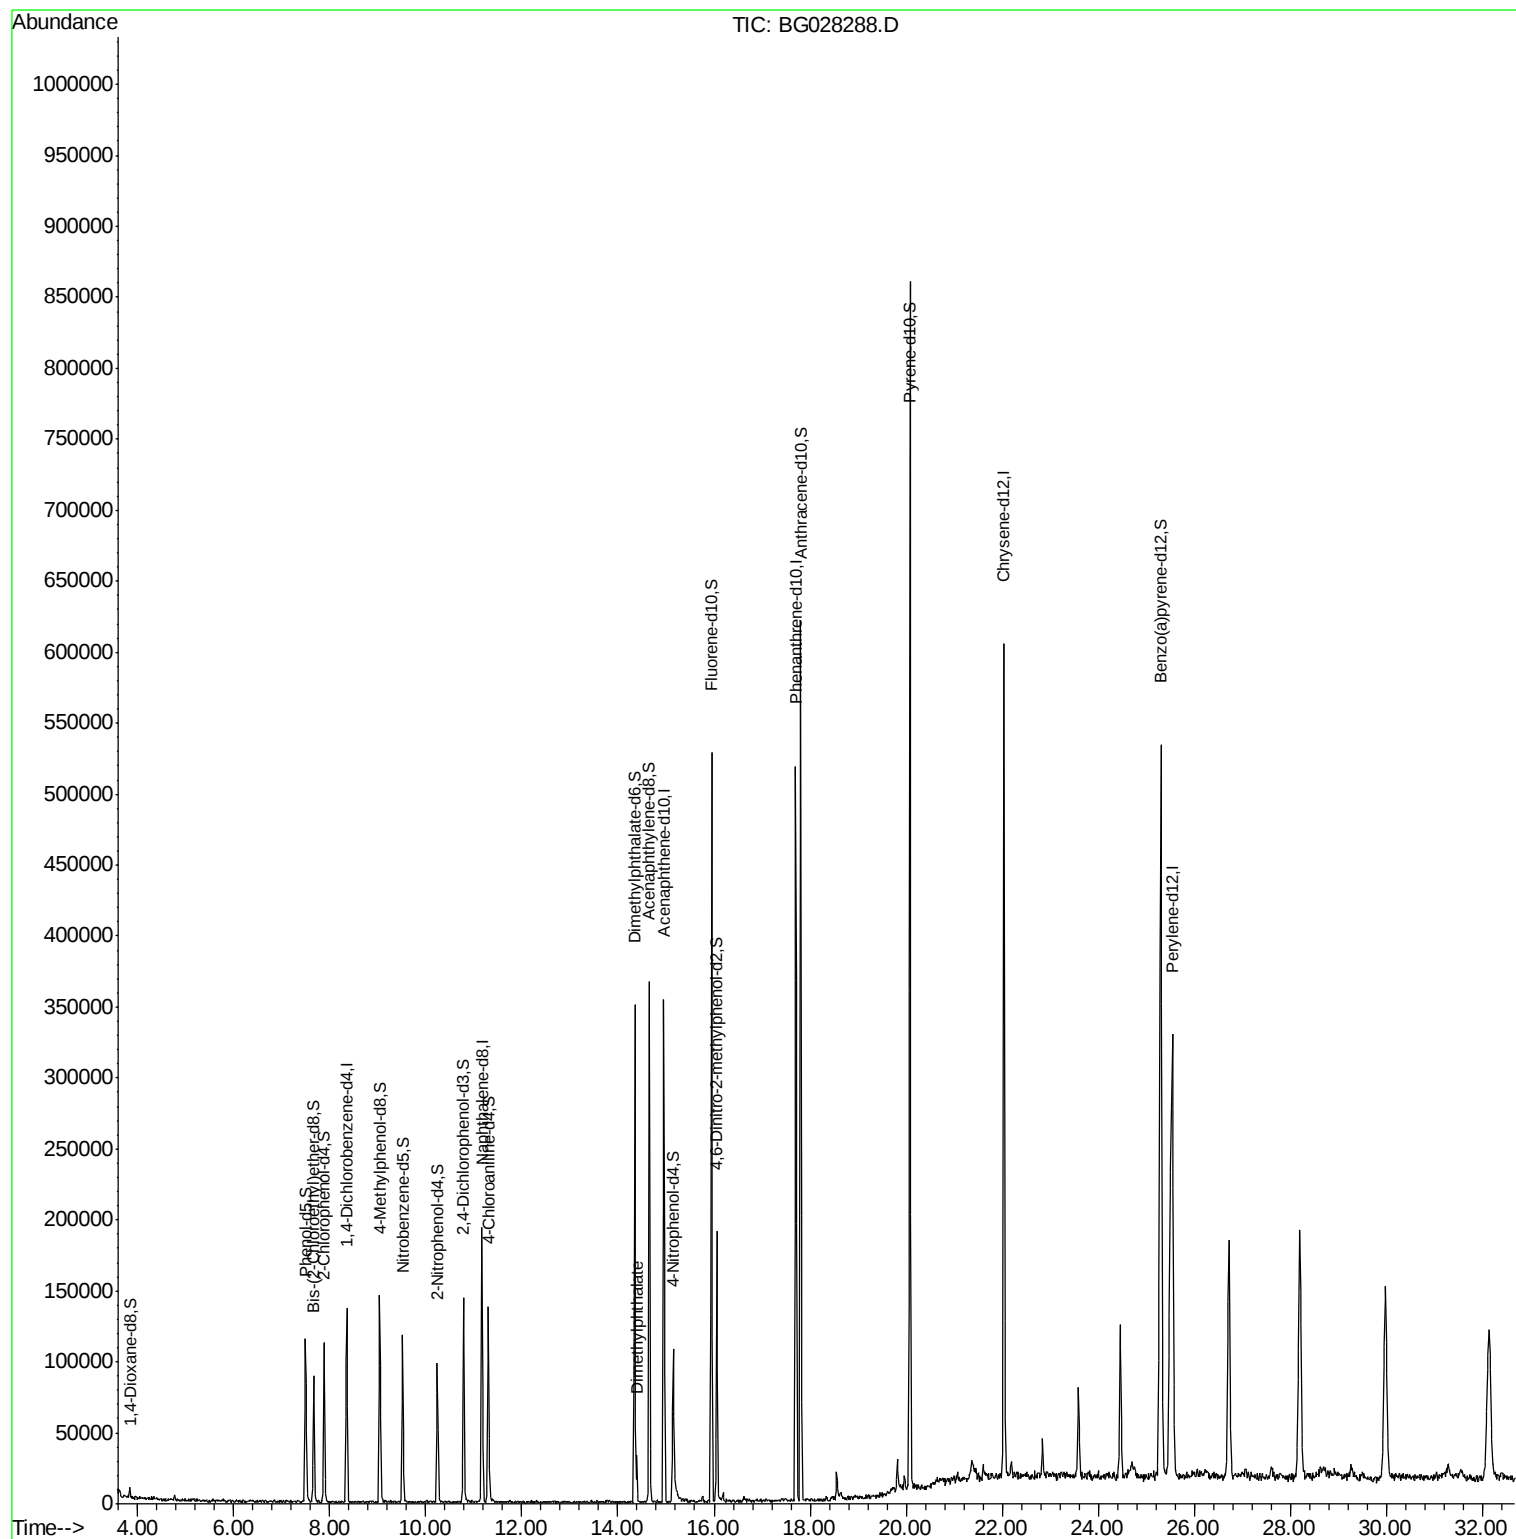

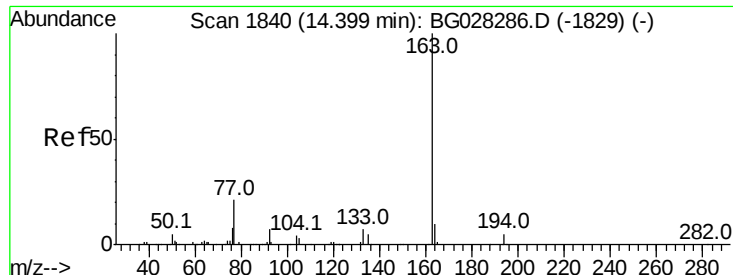

#44

Dimethylphthalate

Concen: 2.105 ng/ul

RT: 14.40 min Scan# 1839

Delta R.T. 0.00 min

Lab File: BG028288.D

Acq: 11 Aug 2017 11:49

Instrument :

BNA_G

ClientSampleId :

C0AG1


Tot Ion:163 Resp: 21489

Ion Ratio Lower Upper

163 100

194 3.4 3.4 5.0

164 10.5 9.0 13.4

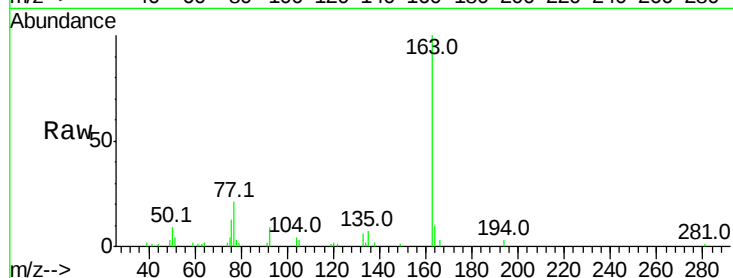

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

