
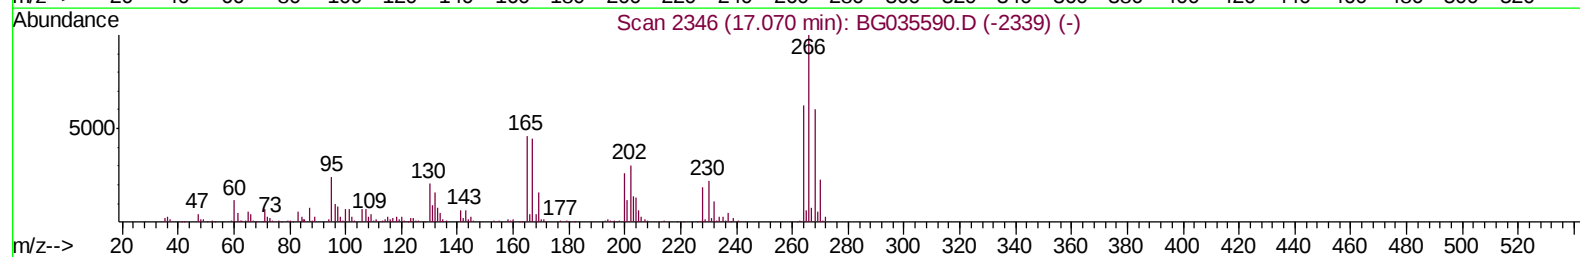
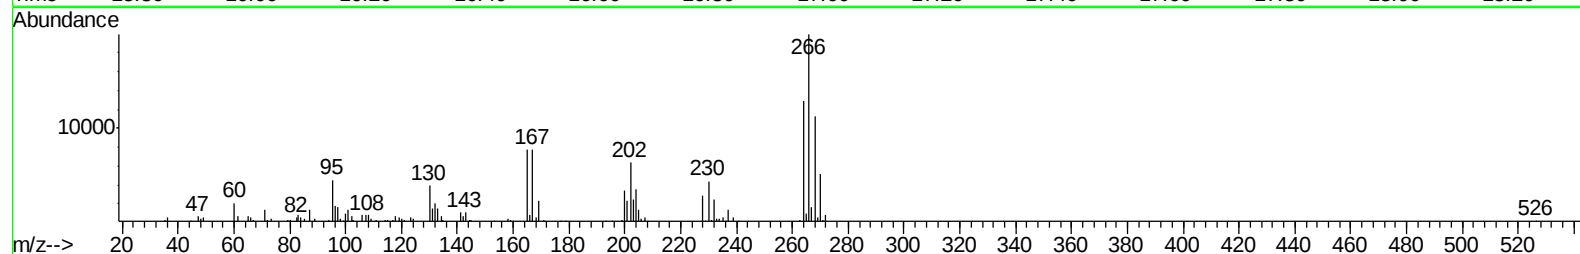


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG081018\
Data File : BG036268.D
Acq On : 10 Aug 2018 14:48
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 01:27:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

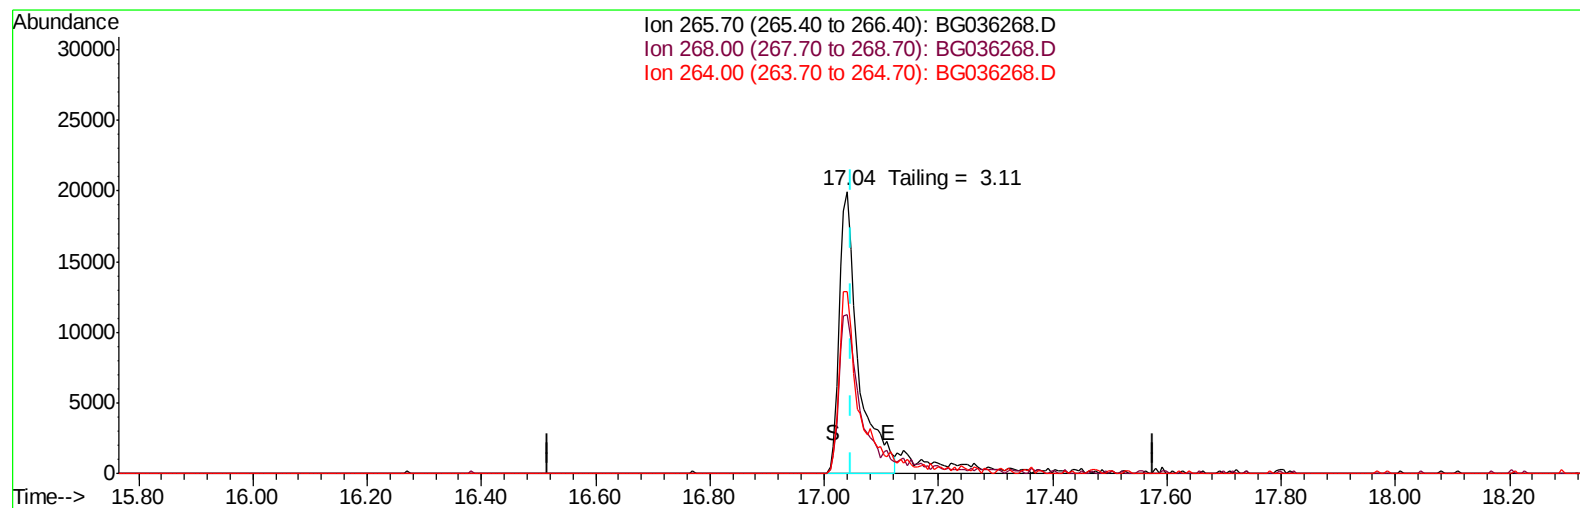

TIC: BG036268.D

(69) Pentachlorophenol (C)




17.040min (-0.007) 94970.71ng

response 46305

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	56.38
264.00	62.00	64.67
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG081018\
 Data File : BG036268.D
 Acq On : 10 Aug 2018 14:48
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 01:27:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 31 12:30:06 2018
 Response via : Initial Calibration

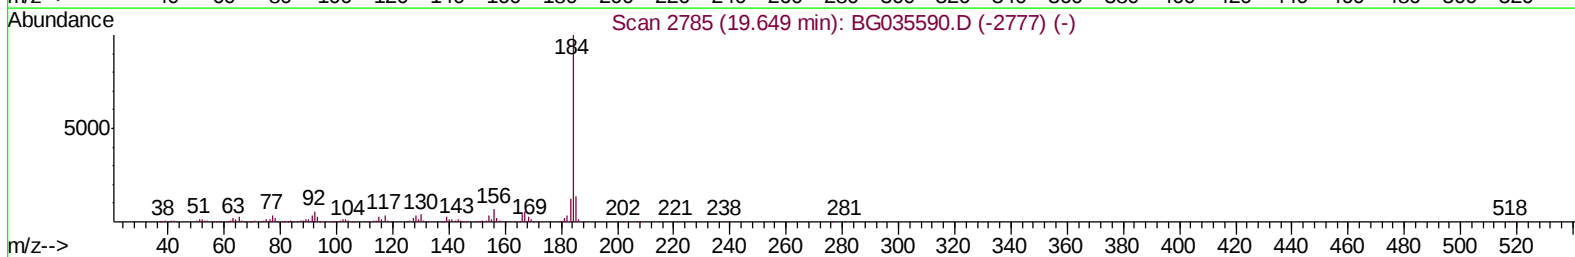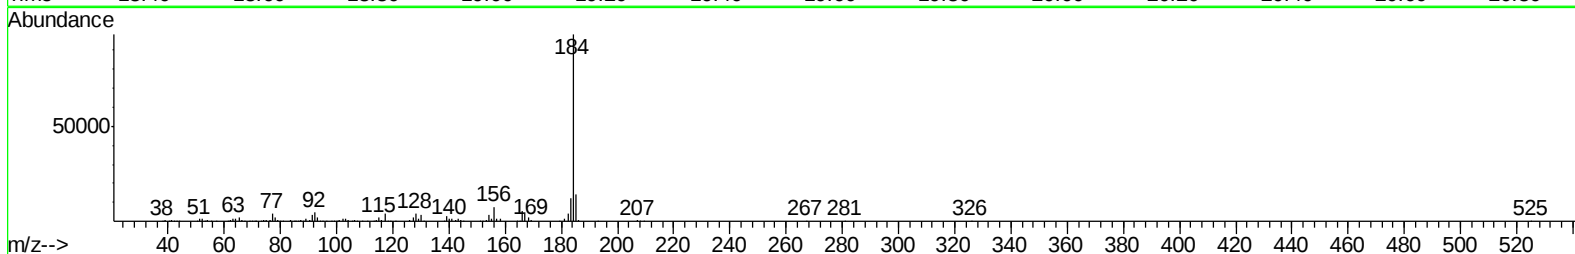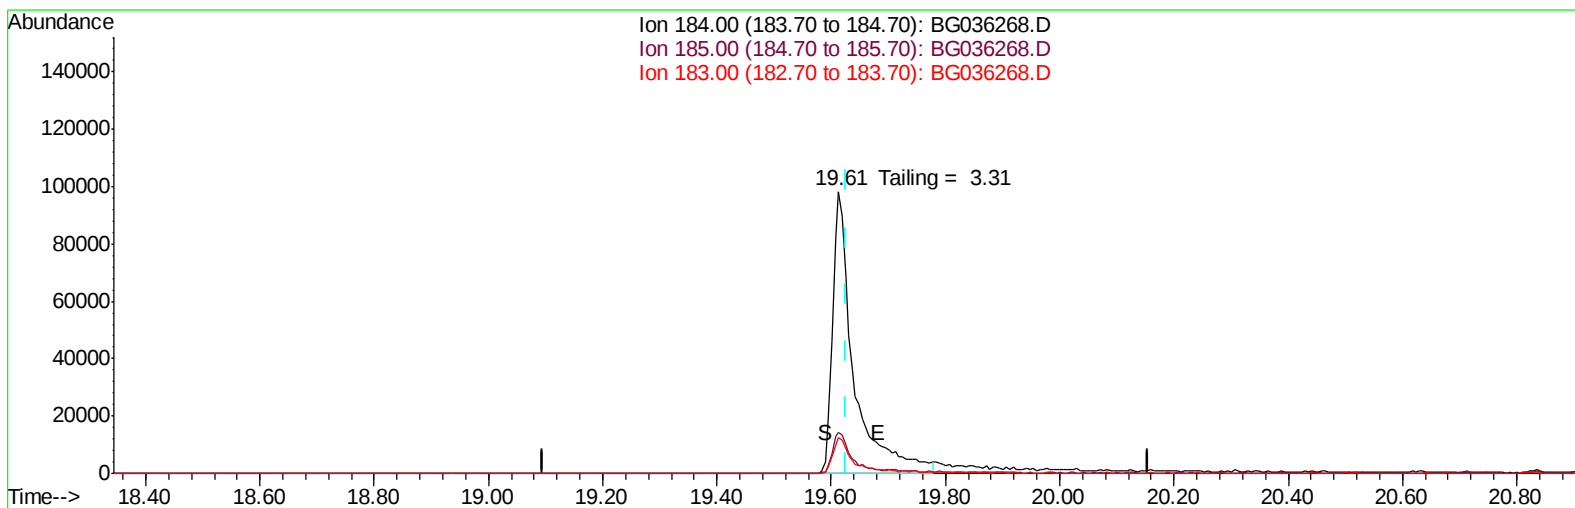

TIC: BG036268.D

(76) Benzidine

19.613min (-0.013) 54174.71ng

response 250671

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.62
183.00	13.30	12.76
0.00	0.00	0.00