
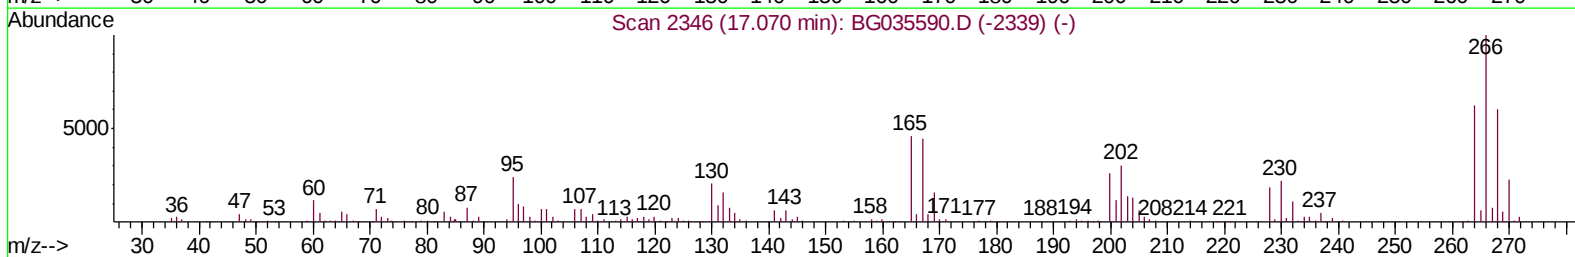
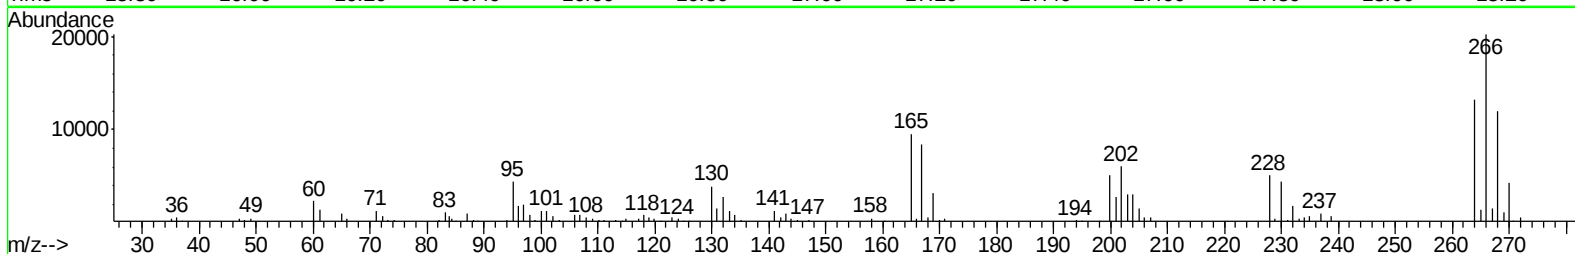


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG081018\
Data File : BG036286.D
Acq On : 11 Aug 2018 3:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 01:29:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

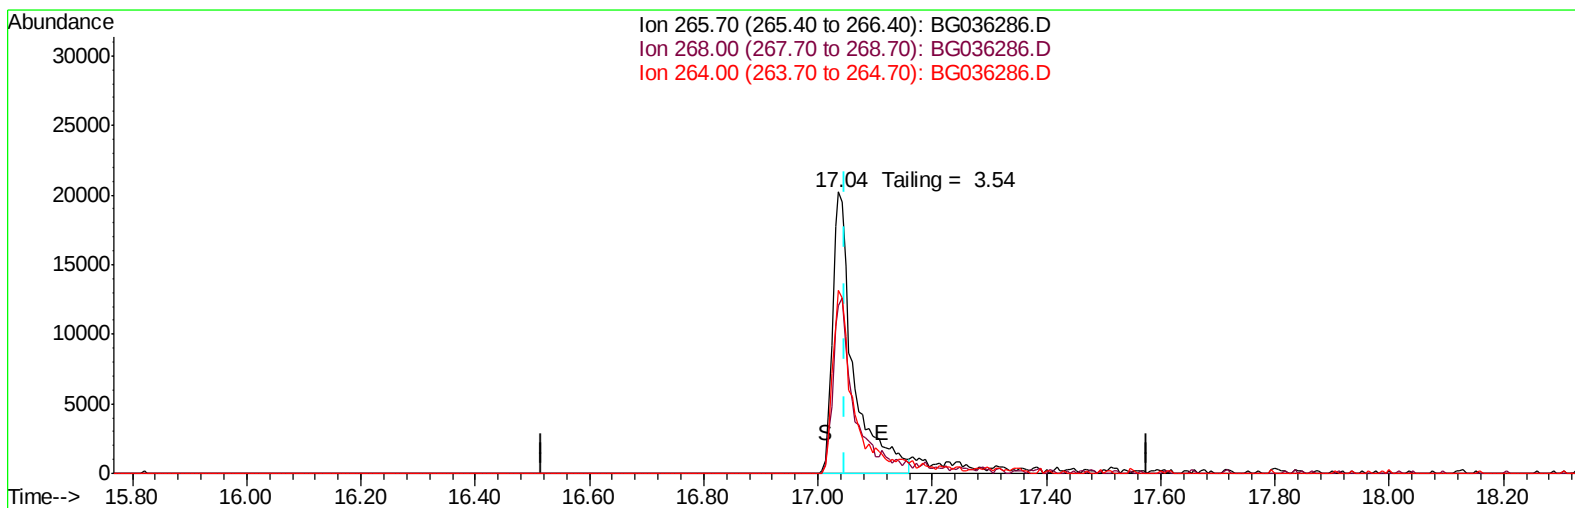

TIC: BG036286.D

(69) Pentachlorophenol (C)




17.036min (-0.011) 89375.92ng

response 51382

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.56
264.00	62.00	65.09
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG081018\
 Data File : BG036286.D
 Acq On : 11 Aug 2018 3:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 01:29:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 31 12:30:06 2018
 Response via : Initial Calibration

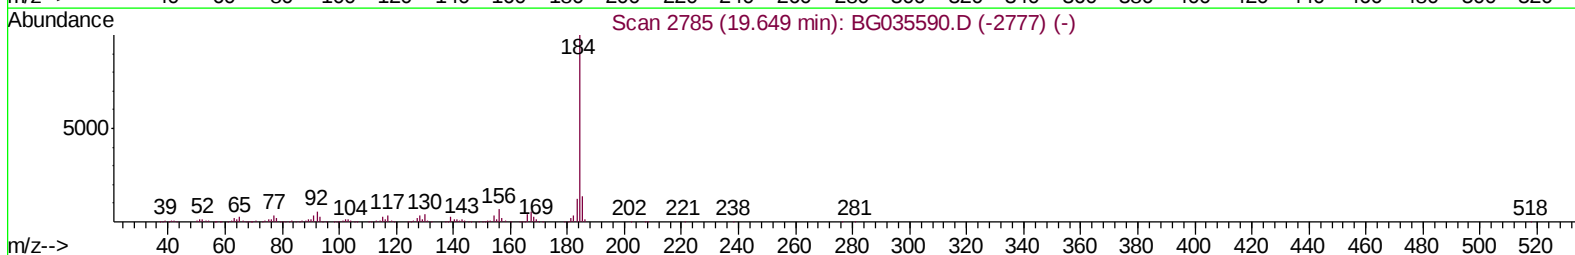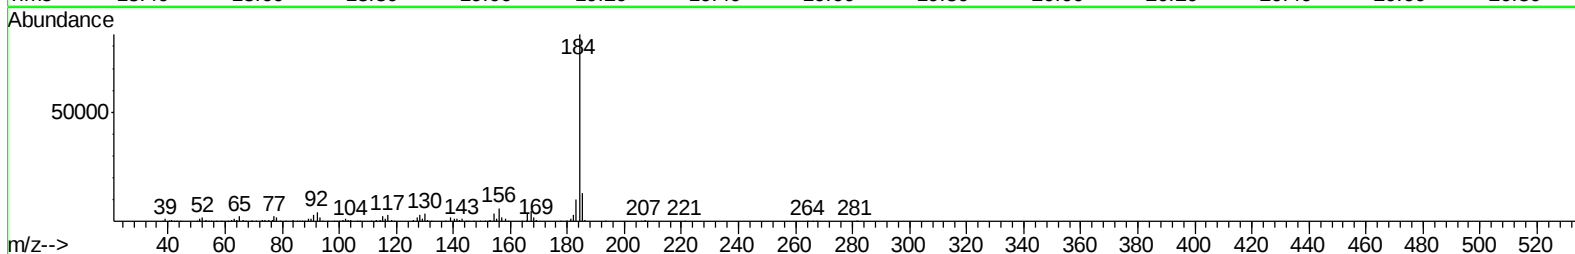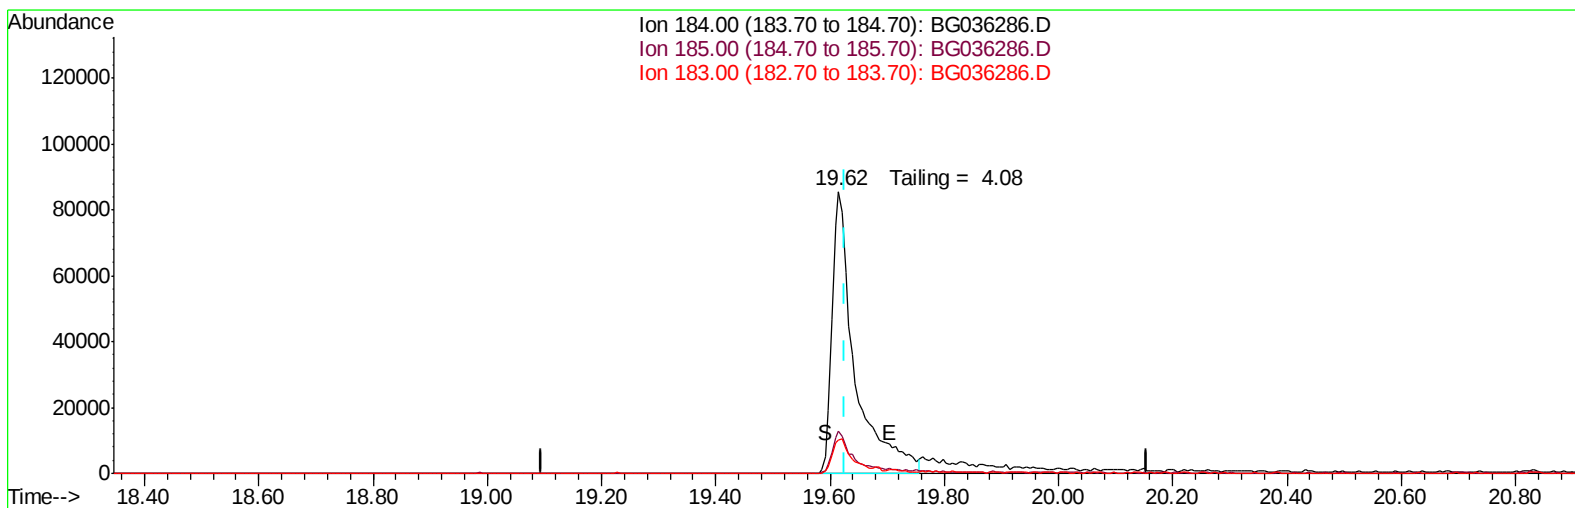

TIC: BG036286.D

(76) Benzidine

19.615min (-0.011) 12572.80ng

response 235346

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.02
183.00	13.30	11.87
0.00	0.00	0.00