

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG081018\
 Data File : BG036278.D
 Acq On : 10 Aug 2018 22:01
 Operator : JU/SJ
 Sample : J4379-24
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-101D

Quant Time: Aug 11 00:07:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 31 12:30:06 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	24165	20.00	ng	-0.02
21) Naphthalene-d8	10.81	136	85573	20.00	ng	-0.02
38) Acenaphthene-d10	14.63	164	63409	20.00	ng	-0.02
63) Phenanthrene-d10	17.38	188	177642	20.00	ng	-0.02
75) Chrysene-d12	21.64	240	191066	20.00	ng	-0.02
86) Perylene-d12	24.83	264	175573	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	81410	55.93	ng	0.00
7) Phenol-d6	7.18	99	66953	30.83	ng	-0.02
23) Nitrobenzene-d5	9.17	82	204526	99.84	ng	-0.02
41) 2,4,6-Tribromophenol	16.12	330	142319	170.28	ng	-0.02
44) 2-Fluorobiphenyl	13.25	172	477557	100.90	ng	-0.02
78) Terphenyl-d14	19.98	244	909023	104.87	ng	-0.02
Target Compounds						
2) 1,4-Dioxane	3.51	88	11869	16.022	ng	Qvalue # 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG081018\
Data File : BG036278.D
Acq On : 10 Aug 2018 22:01
Operator : JU/SJ
Sample : J4379-24
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-101D

Quant Time: Aug 11 00:07:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

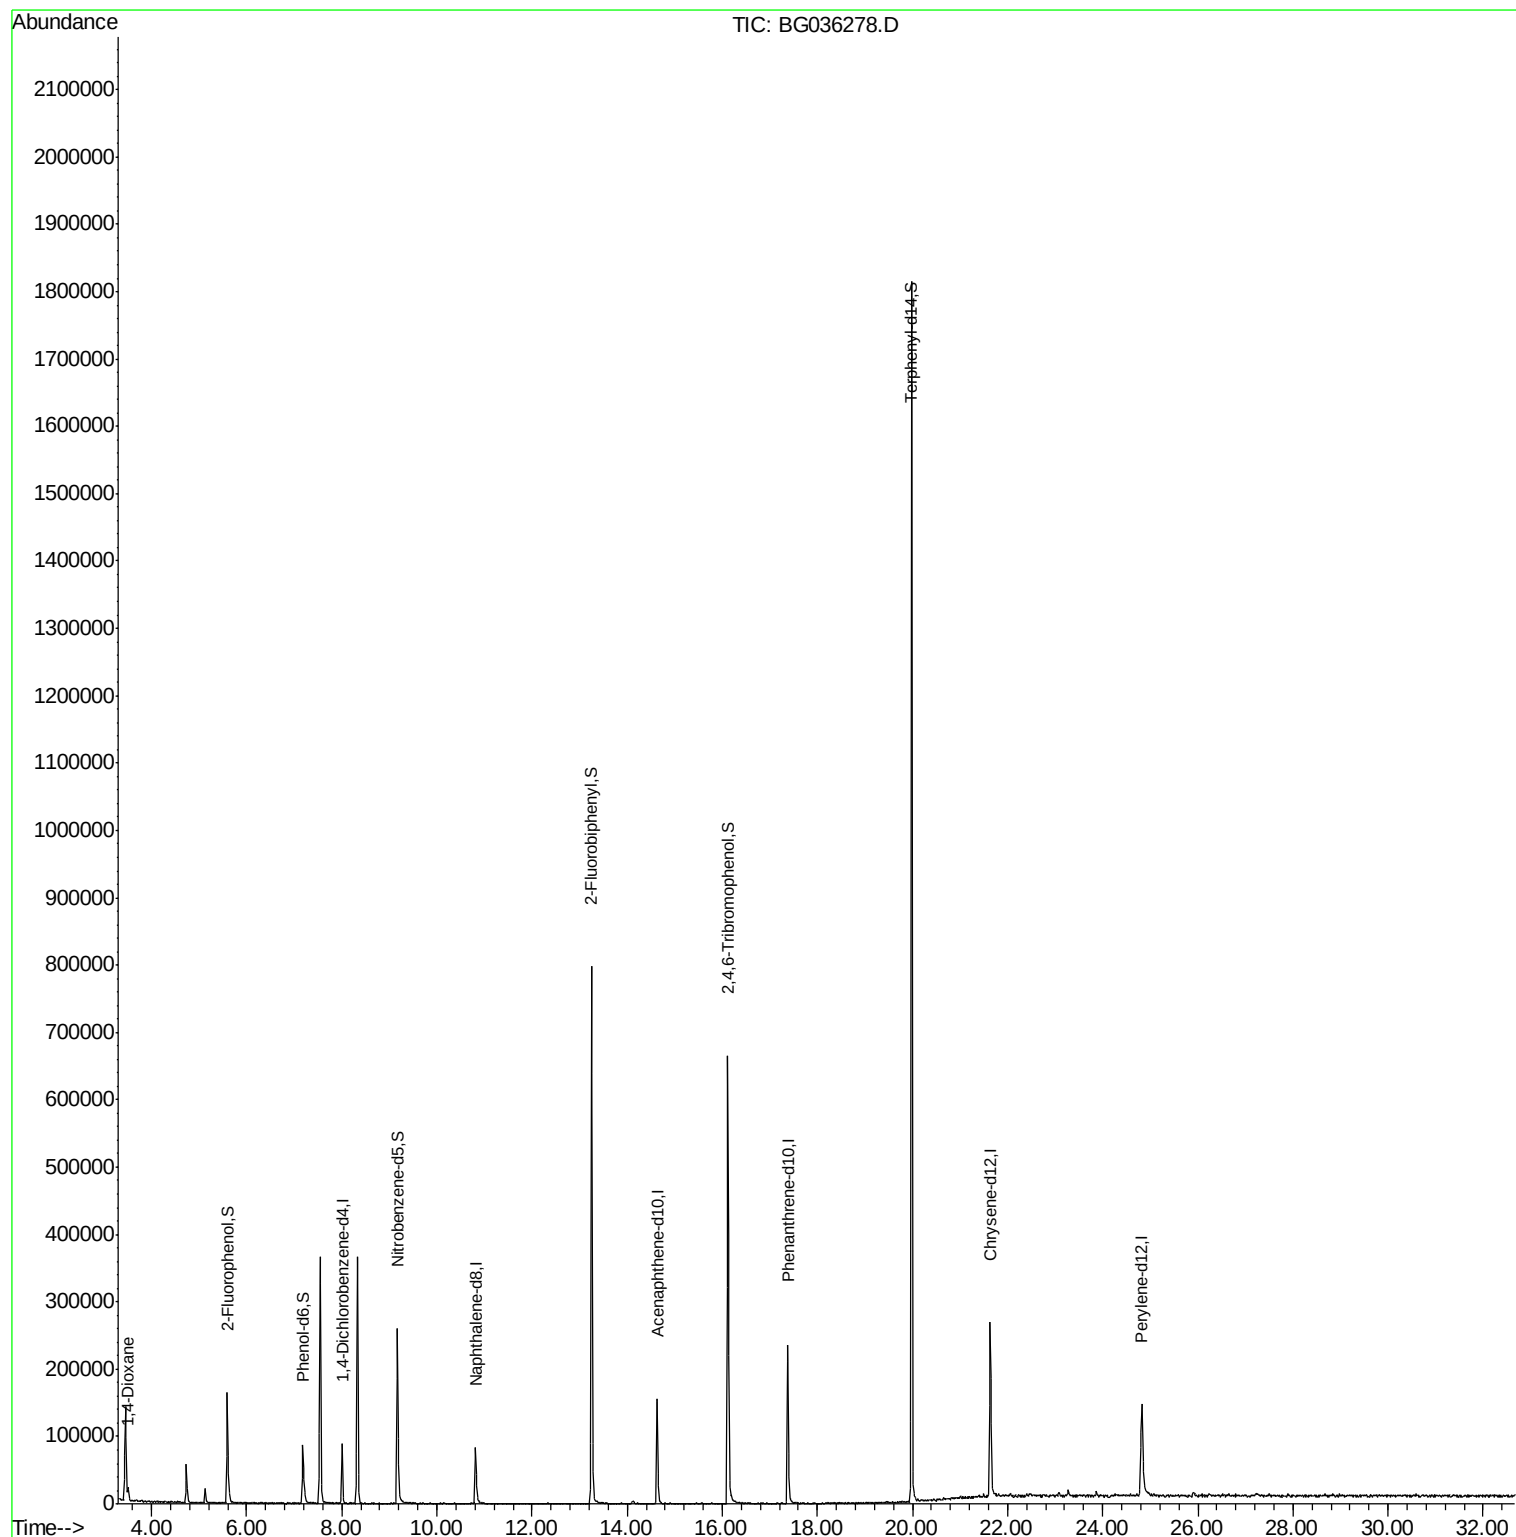




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 803
Delta R.T. -0.02 min
Lab File: BG036278.D
Acq: 10 Aug 2018 22:01

Instrument :
BNA_G
ClientSampled :
MW-101D

Tgt Ion:152 Resp: 24165
Ion Ratio Lower Upper
152 100
150 144.9 126.6 189.8
115 67.4 53.0 79.4

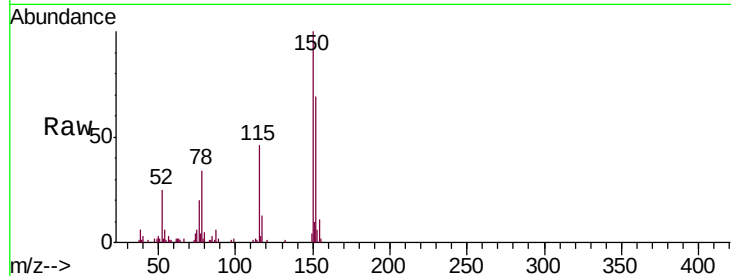


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

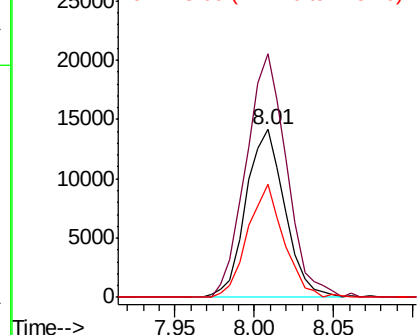



#2


1,4-Dioxane
Concen: 16.022 ng
RT: 3.51 min Scan# 37
Delta R.T. -0.02 min
Lab File: BG036278.D
Acq: 10 Aug 2018 22:01

Tgt Ion: 88 Resp: 11869
Ion Ratio Lower Upper
88 100
58 73.8 79.6 119.4#
43 36.4 27.4 41.0

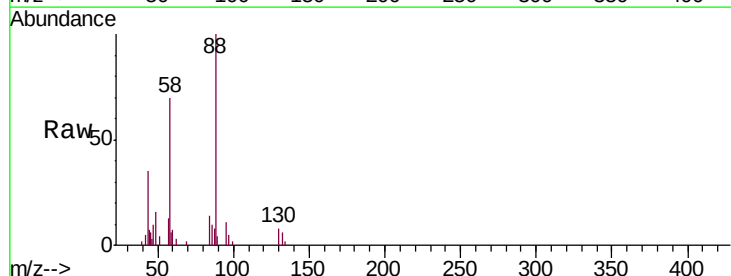

Abundance Ion 88.00 (87.70 to 88.70): BGC
Ion 58.00 (57.70 to 58.70): BGC
Ion 43.00 (42.70 to 43.70): BGC

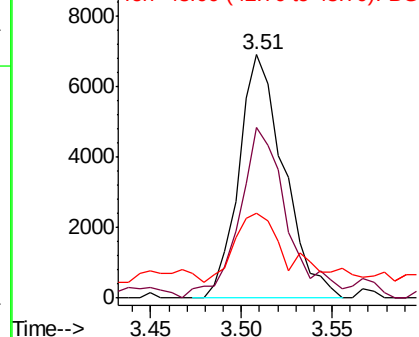



#5

2-Fluorophenol

Concen: 55.932 ng

RT: 5.60 min Scan# 393

Delta R.T. -0.00 min

Lab File: BG036278.D

Acq: 10 Aug 2018 22:01

Instrument :

BNA_G

ClientSampleId :

MW-101D


Tgt Ion: 112 Resp: 81410

Ion Ratio Lower Upper




112 100

64 58.8 56.3 84.5

63 33.8 30.1 45.1

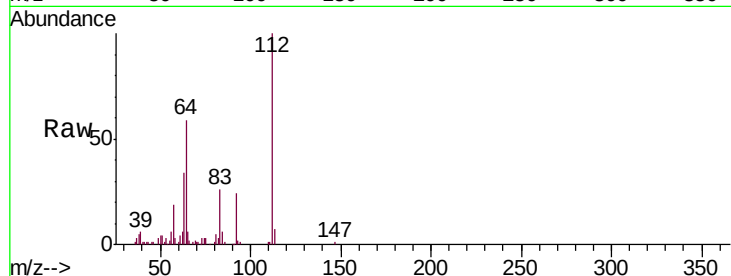

Abundance Ion 112.00 (111.70 to 112.70): BGC
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

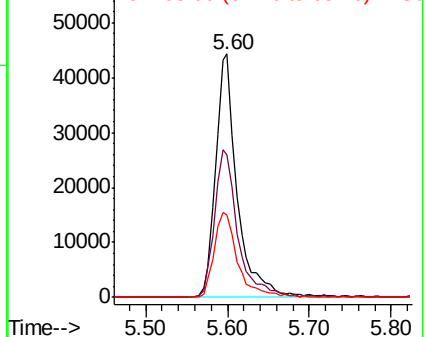

#7

Phenol-d6

Concen: 30.831 ng

RT: 7.18 min Scan# 662

Delta R.T. -0.02 min

Lab File: BG036278.D

Acq: 10 Aug 2018 22:01


Tgt Ion: 99 Resp: 66953

Ion Ratio Lower Upper



99 100


42 16.1 14.1 21.1

71 47.9 26.1 39.1#



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC




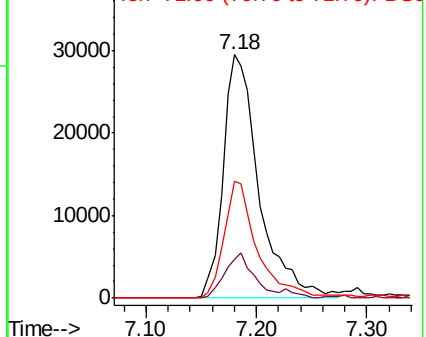


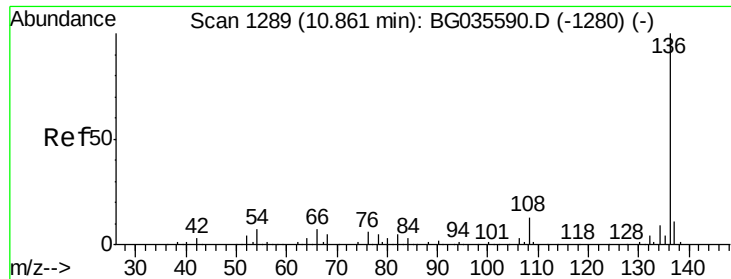

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.81 min Scan# 1280
Delta R.T. -0.02 min
Lab File: BG036278.D
Acq: 10 Aug 2018 22:01




Instrument :
BNA_G
ClientSampleId :
MW-101D


Tgt Ion: 136 Resp: 85573
Ion Ratio Lower Upper
136 100
137 11.4 9.2 13.8
54 7.0 10.3 15.5#
68 4.2 4.5 6.7#

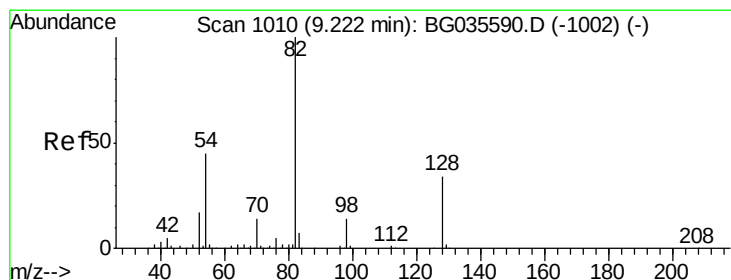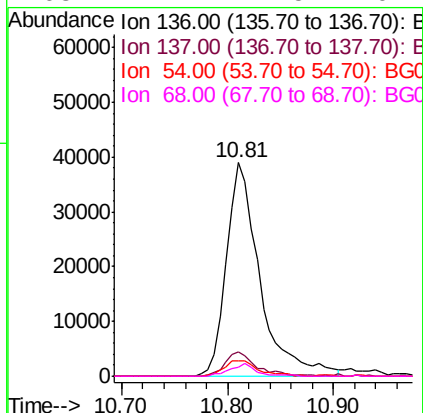

#23
Nitrobenzene-d5
Concen: 99.845 ng
RT: 9.17 min Scan# 1001
Delta R.T. -0.02 min
Lab File: BG036278.D
Acq: 10 Aug 2018 22:01

Tgt Ion: 82 Resp: 204526
Ion Ratio Lower Upper
82 100
128 32.3 29.7 44.5
54 44.3 43.1 64.7

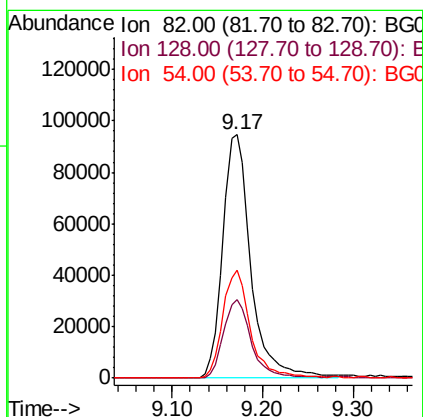

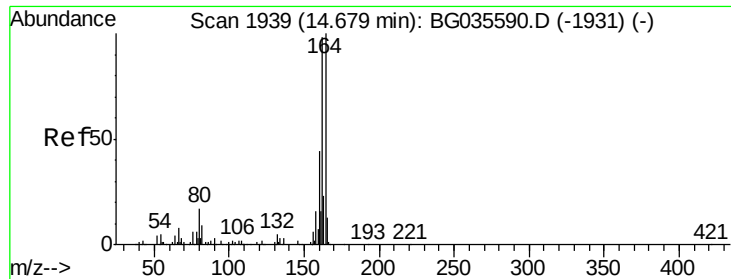

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.63 min Scan# 1930

Delta R.T. -0.02 min

Lab File: BG036278.D

Acq: 10 Aug 2018 22:01

Instrument :

BNA_G

ClientSampleId :

MW-101D


Tgt Ion:164 Resp: 63409

Ion Ratio Lower Upper

164 100

162 95.5 78.8 118.2




160 40.9 35.4 53.0



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

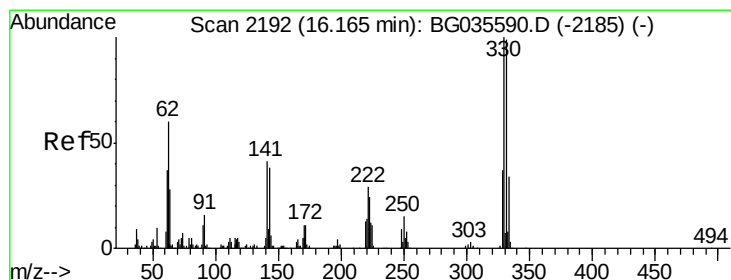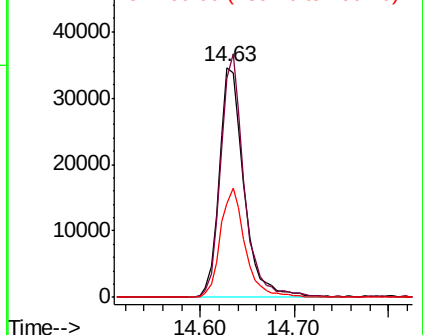

#41

2,4,6-Tribromophenol

Concen: 170.285 ng

RT: 16.12 min Scan# 2184

Delta R.T. -0.02 min

Lab File: BG036278.D

Acq: 10 Aug 2018 22:01


Tgt Ion:330 Resp: 142319

Ion Ratio Lower Upper

330 100

332 93.6 77.0 115.6



141 38.3 25.2 37.8#




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




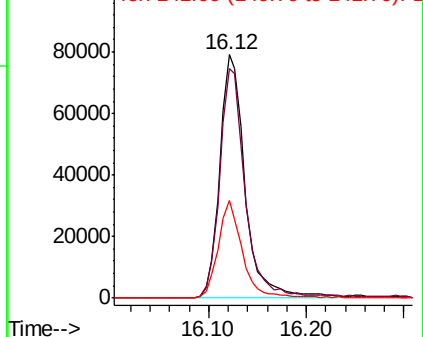


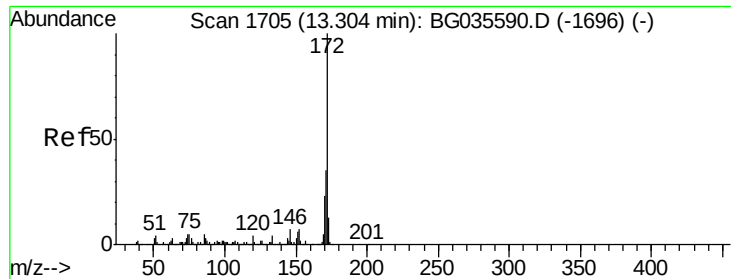

#44
 2-Fluorobiphenyl
 Concen: 100.901 ng
 RT: 13.25 min Scan# 1696
 Delta R.T. -0.02 min
 Lab File: BG036278.D
 Acq: 10 Aug 2018 22:01




Instrument :
 BNA_G
 ClientSampleId :
 MW-101D


Tgt Ion:	172	Resp:	477557
Ion	Ratio	Lower	Upper
172	100		
171	32.9	30.0	45.0
170	21.8	19.5	29.3

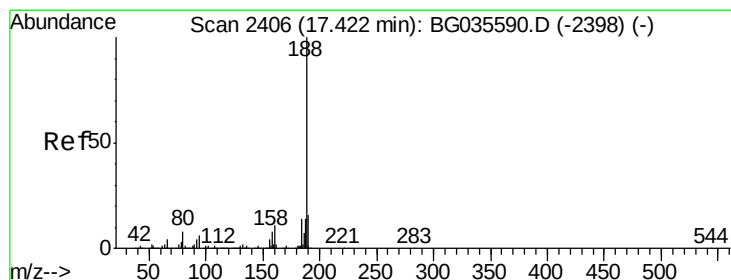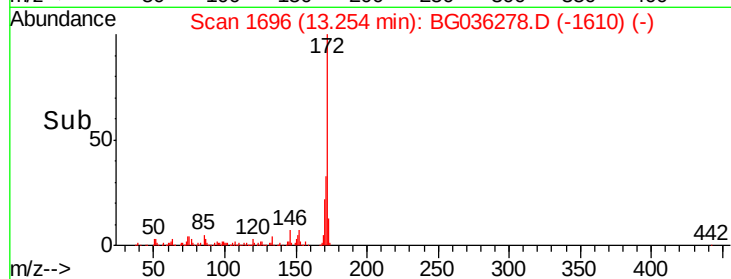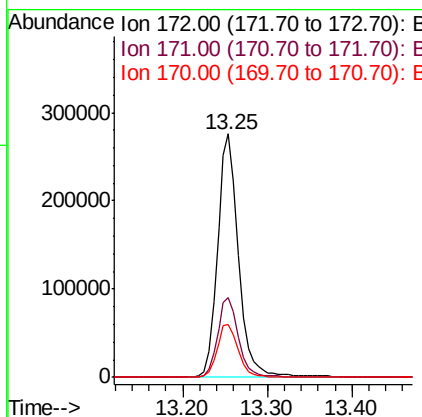

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.38 min Scan# 2398
 Delta R.T. -0.02 min
 Lab File: BG036278.D
 Acq: 10 Aug 2018 22:01

Tgt Ion:	188	Resp:	177642
Ion	Ratio	Lower	Upper
188	100		
94	6.0	6.9	10.3#
80	7.1	7.7	11.5#

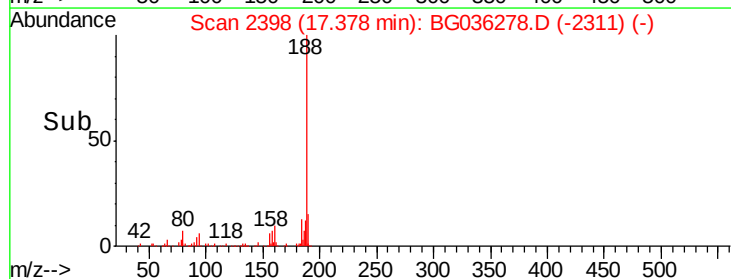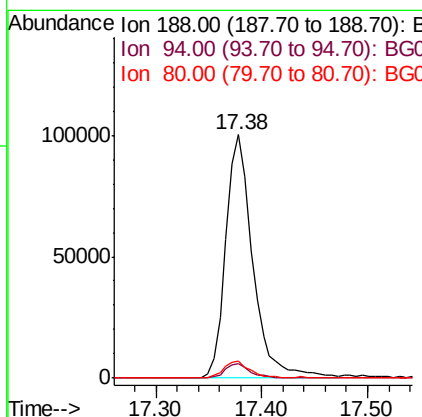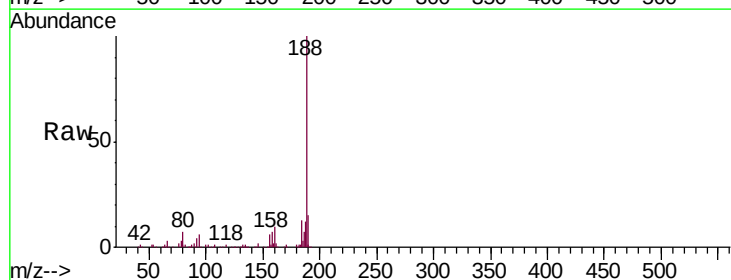



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.64 min Scan# 3123

Delta R.T. -0.02 min

Lab File: BG036278.D

Acq: 10 Aug 2018 22:01

Instrument :

BNA_G

ClientSampleId :

MW-101D


Tgt Ion:240 Resp: 191066

Ion Ratio Lower Upper

240 100

120 5.0 6.8 10.2#




236 26.2 20.9 31.3

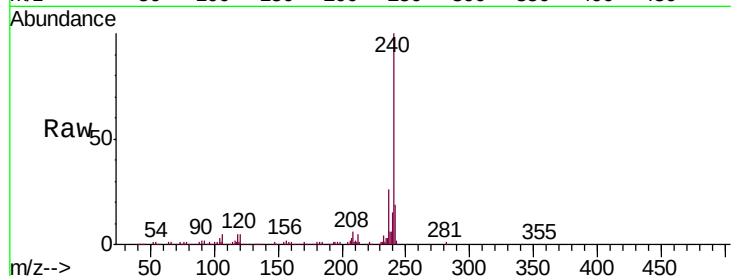

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

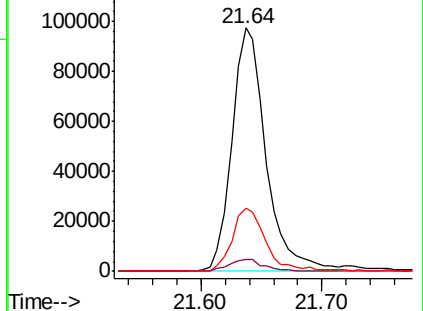

#78

Terphenyl-d14

Concen: 104.873 ng

RT: 19.98 min Scan# 2841

Delta R.T. -0.02 min

Lab File: BG036278.D

Acq: 10 Aug 2018 22:01


Tgt Ion:244 Resp: 909023

Ion Ratio Lower Upper

244 100

212 9.3 5.8 8.8#



122 6.8 7.0 10.4#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

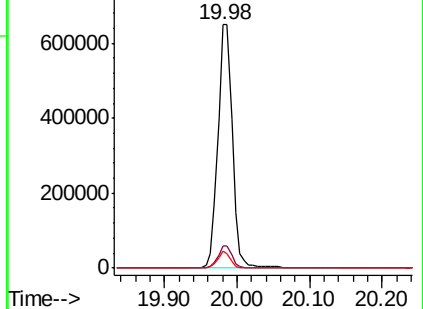

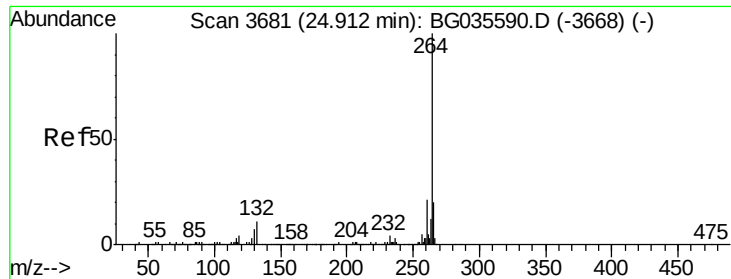

#86
Perylene-d12
Concen: 20.000 ng
RT: 24.83 min Scan# 3666
Delta R.T. -0.03 min
Lab File: BG036278.D
Acq: 10 Aug 2018 22:01

Instrument :
BNA_G
ClientSampleId :
MW-101D

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.1	17.4	26.0
265	25.5	17.7	26.5

