

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG081018\
 Data File : BG036294.D
 Acq On : 11 Aug 2018 9:11
 Operator : JU/SJ
 Sample : J4274-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HD-01-080918

Quant Time: Aug 13 01:13:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 31 12:30:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	27174	20.00	ng	-0.02
21) Naphthalene-d8	10.81	136	95379	20.00	ng	-0.02
38) Acenaphthene-d10	14.63	164	65724	20.00	ng	-0.02
63) Phenanthrene-d10	17.38	188	170014	20.00	ng	-0.02
75) Chrysene-d12	21.65	240	178753	20.00	ng	-0.01
86) Perylene-d12	24.84	264	147645	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	233047	142.38	ng	0.00
7) Phenol-d6	7.18	99	294851	120.74	ng	-0.01
23) Nitrobenzene-d5	9.17	82	258751	113.33	ng	-0.02
41) 2,4,6-Tribromophenol	16.12	330	133976	154.66	ng	-0.02
44) 2-Fluorobiphenyl	13.25	172	587690	119.80	ng	-0.02
78) Terphenyl-d14	19.98	244	1054984	130.10	ng	-0.02


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG081018\
Data File : BG036294.D
Acq On : 11 Aug 2018 9:11
Operator : JU/SJ
Sample : J4274-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HD-01-080918

Quant Time: Aug 13 01:13:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

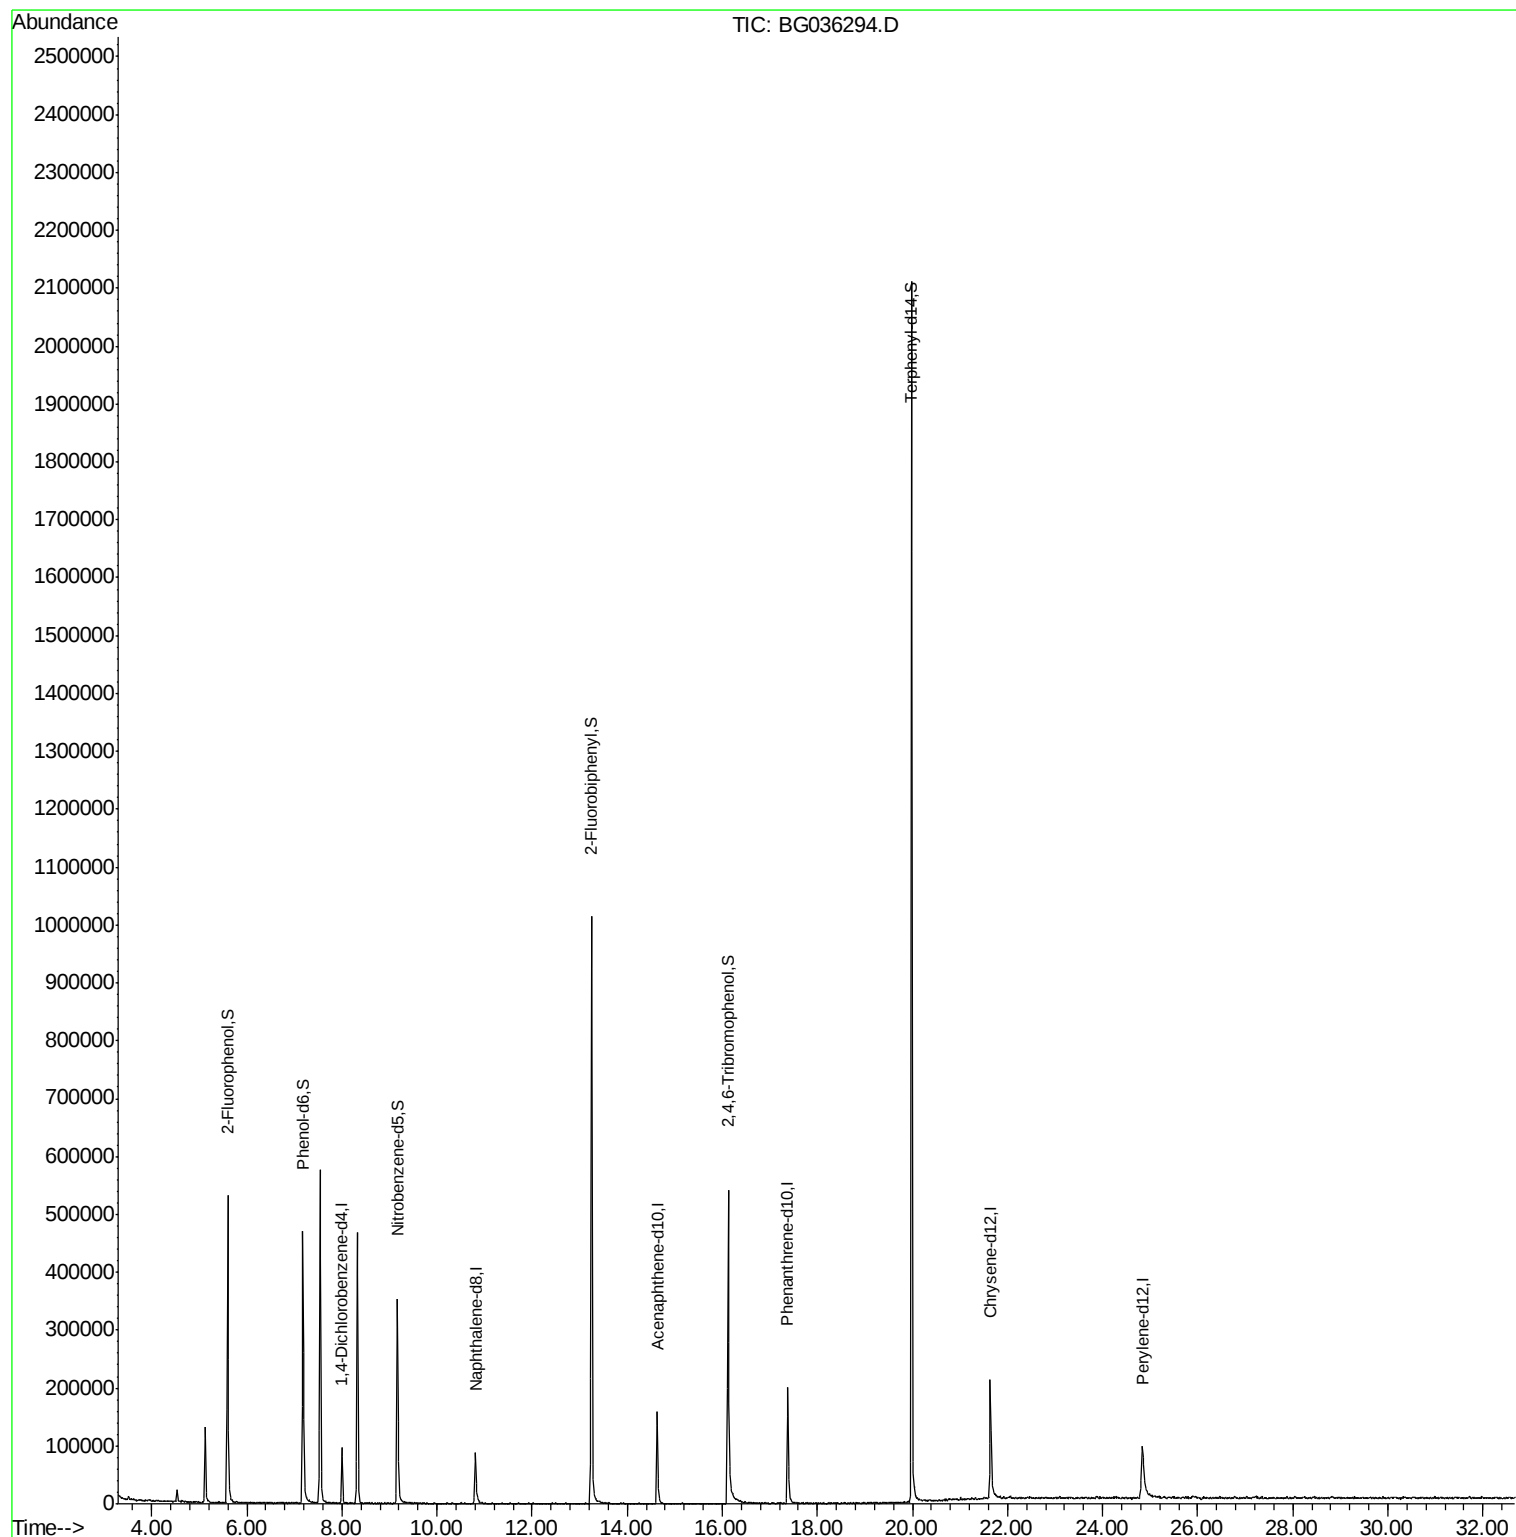




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 803
Delta R.T. -0.02 min
Lab File: BG036294.D
Acq: 11 Aug 2018 9:11

Instrument :
BNA_G
ClientSampleId :
HD-01-080918

Tgt Ion:152 Resp: 27174
Ion Ratio Lower Upper
152 100
150 144.6 126.6 189.8
115 63.0 53.0 79.4

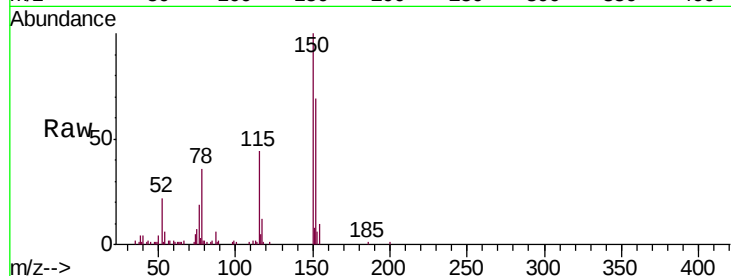


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

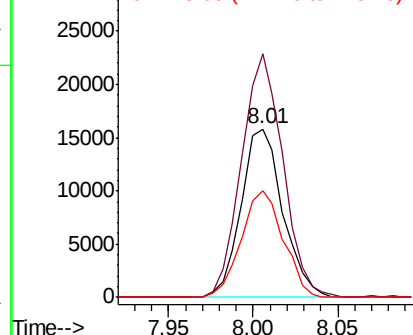



#5



2-Fluorophenol
Concen: 142.383 ng
RT: 5.60 min Scan# 393
Delta R.T. -0.01 min
Lab File: BG036294.D
Acq: 11 Aug 2018 9:11

Tgt Ion:112 Resp: 233047
Ion Ratio Lower Upper
112 100
64 67.1 56.3 84.5
63 37.2 30.1 45.1

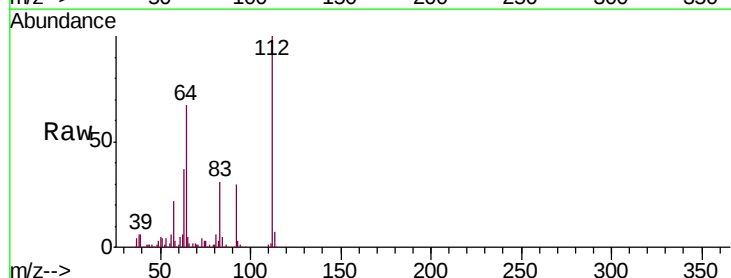

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

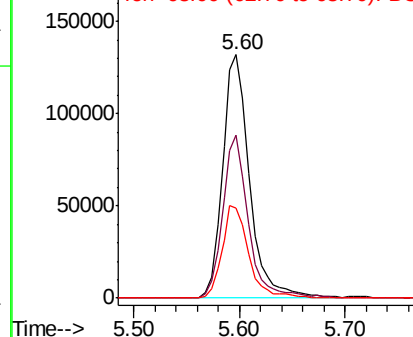

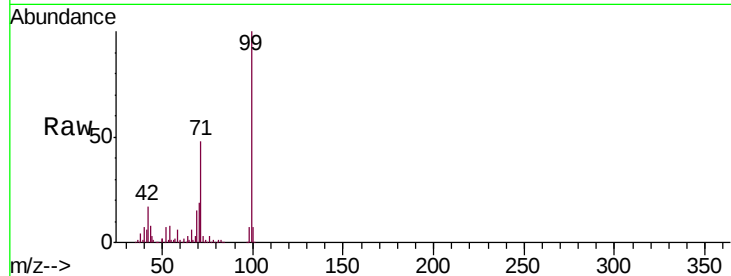

#7

Phenol-d6

Concen: 120.741 ng

RT: 7.18 min Scan# 663

Delta R.T. -0.01 min

Lab File: BG036294.D

Acq: 11 Aug 2018 9:11

Instrument :

BNA_G

ClientSampleId :

HD-01-080918





Tgt Ion: 99 Resp: 294851

Ion Ratio Lower Upper

99 100

42 17.3 14.1 21.1

71 47.8 26.1 39.1#

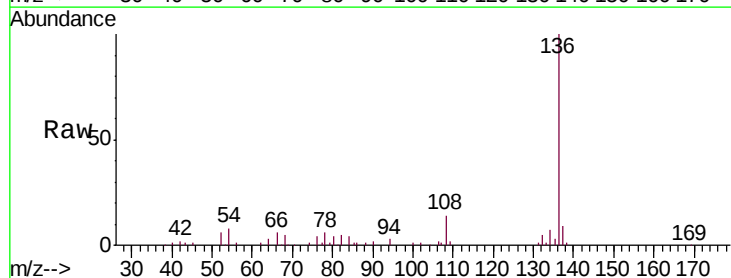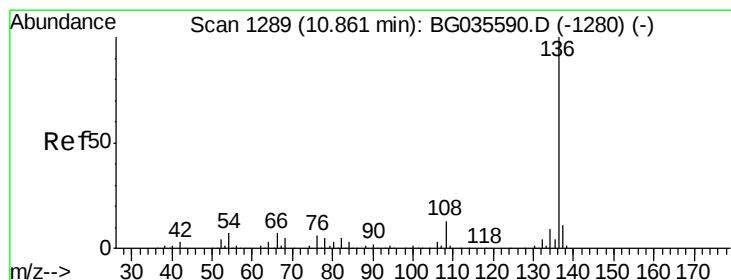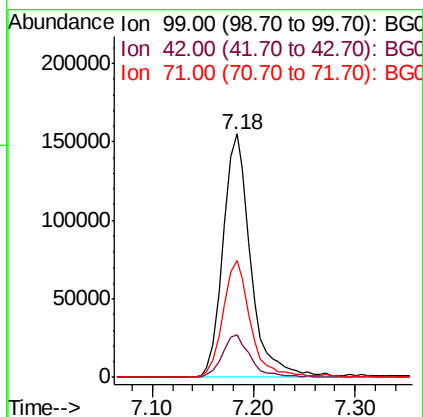

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.81 min Scan# 1280

Delta R.T. -0.02 min

Lab File: BG036294.D

Acq: 11 Aug 2018 9:11

Tgt Ion: 136 Resp: 95379


Ion Ratio Lower Upper


136 100

137 9.5 9.2 13.8

54 8.0 10.3 15.5#

68 4.8 4.5 6.7




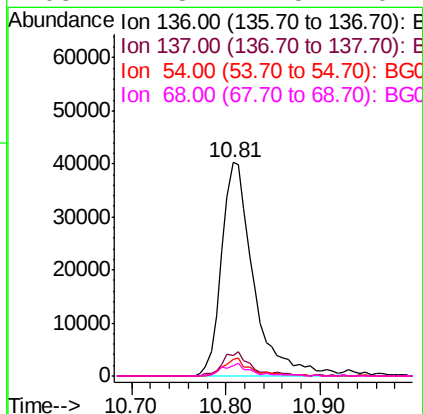


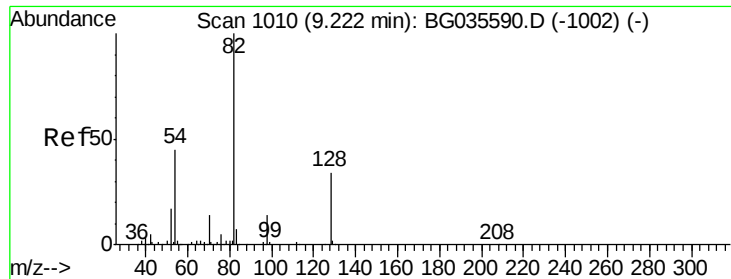

#23
 Nitrobenzene-d5
 Concen: 113.329 ng
 RT: 9.17 min Scan# 1001
 Delta R.T. -0.02 min
 Lab File: BG036294.D
 Acq: 11 Aug 2018 9:11




Instrument :
 BNA_G
 ClientSampleId :
 HD-01-080918


Tgt Ion	Ratio	Lower	Upper
82	100		
128	32.0	29.7	44.5
54	43.0	43.1	64.7#

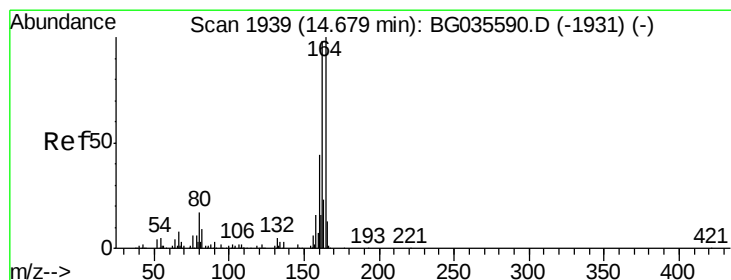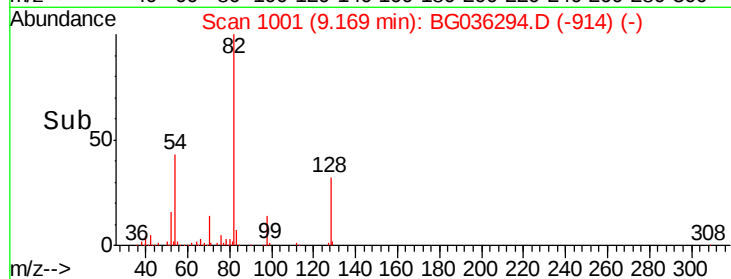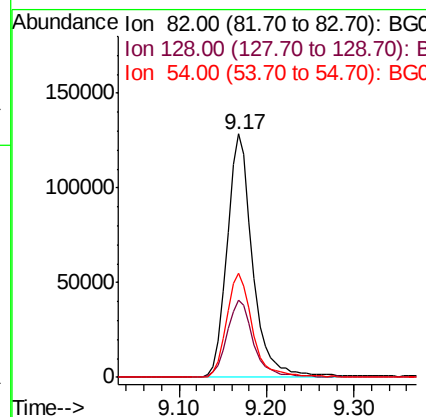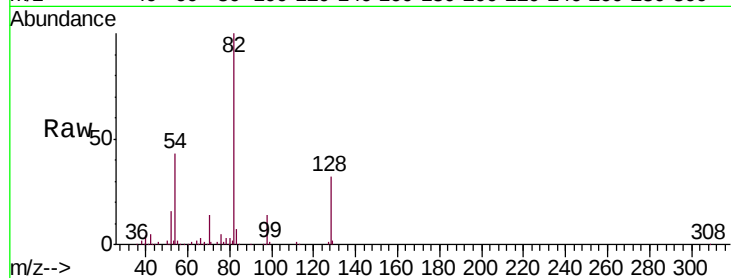

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.63 min Scan# 1931
 Delta R.T. -0.02 min
 Lab File: BG036294.D
 Acq: 11 Aug 2018 9:11

Tgt Ion	Ratio	Lower	Upper
164	100		
162	101.7	78.8	118.2
160	45.1	35.4	53.0

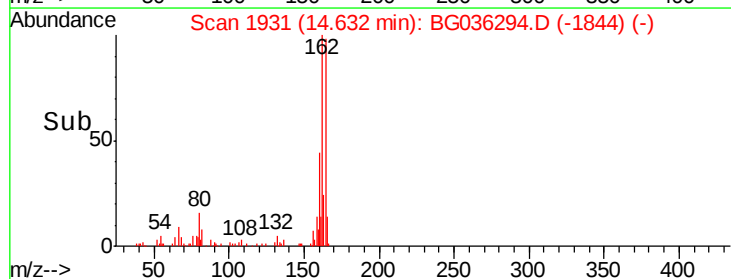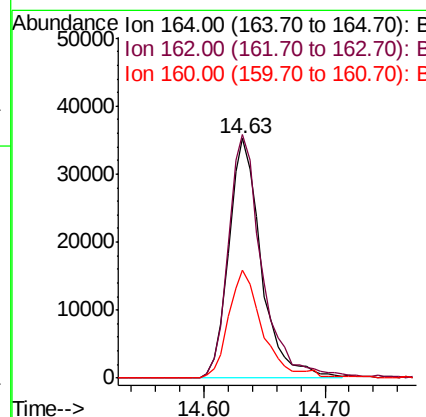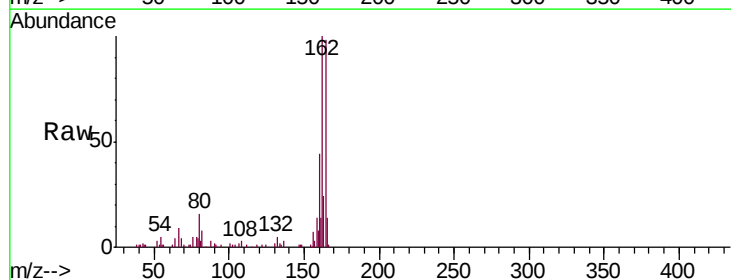







#41
 2,4,6-Tribromophenol
 Concen: 154.656 ng
 RT: 16.12 min Scan# 2185
 Delta R.T. -0.02 min
 Lab File: BG036294.D
 Acq: 11 Aug 2018 9:11

Instrument :
 BNA_G
 ClientSampleId :
 HD-01-080918

Tgt Ion:330 Resp: 133976
 Ion Ratio Lower Upper
 330 100
 332 99.4 77.0 115.6
 141 38.9 25.2 37.8#

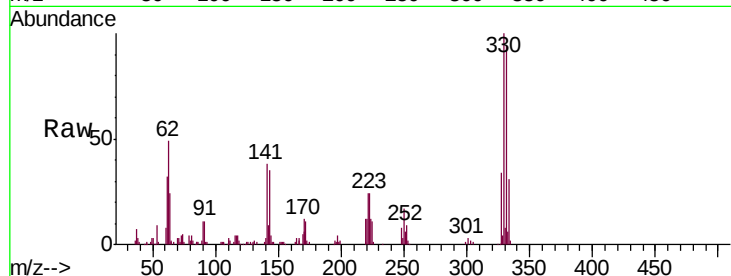


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

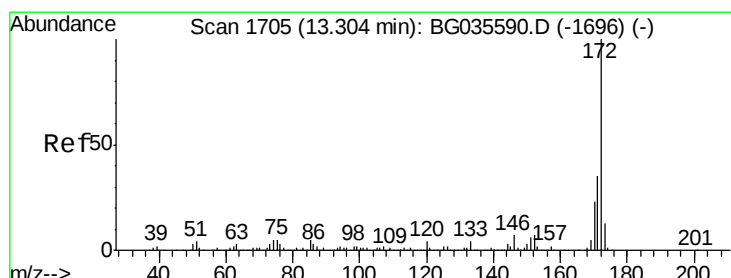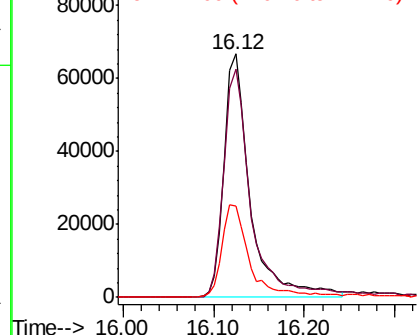




#44
 2-Fluorobiphenyl
 Concen: 119.797 ng
 RT: 13.25 min Scan# 1696
 Delta R.T. -0.02 min
 Lab File: BG036294.D
 Acq: 11 Aug 2018 9:11

Tgt Ion:172 Resp: 587690
 Ion Ratio Lower Upper
 172 100
 171 33.0 30.0 45.0
 170 22.1 19.5 29.3

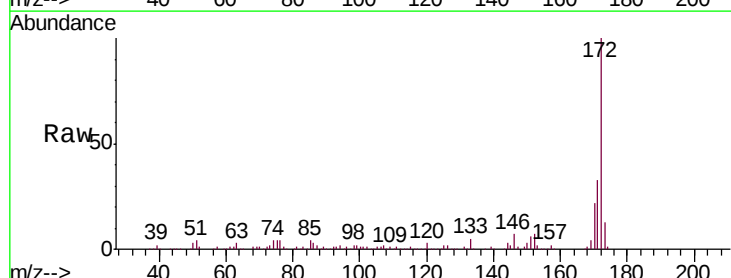

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

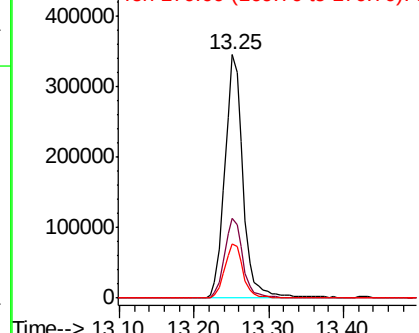

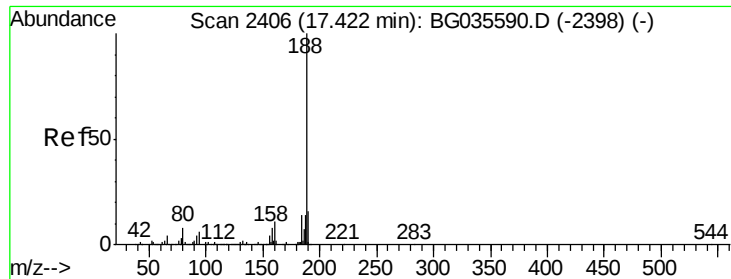

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.38 min Scan# 2398

Delta R.T. -0.02 min

Lab File: BG036294.D

Acq: 11 Aug 2018 9:11

Instrument :

BNA_G

ClientSampleId :

HD-01-080918


Tgt Ion:188 Resp: 170014

Ion Ratio Lower Upper

188 100

94 5.7 6.9 10.3#




80 8.1 7.7 11.5

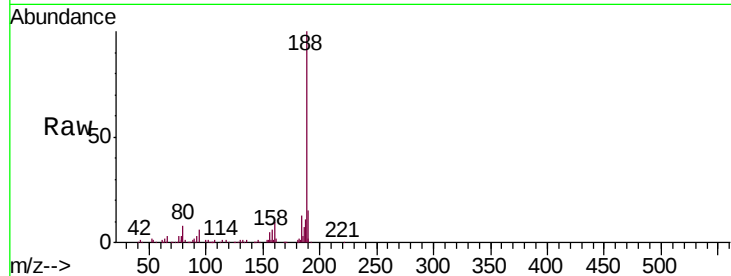

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

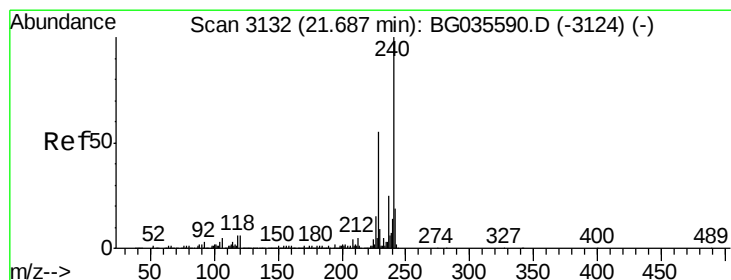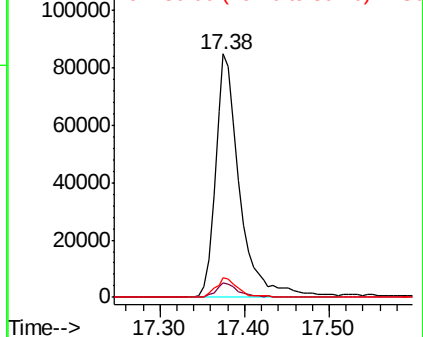

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.65 min Scan# 3125

Delta R.T. -0.01 min

Lab File: BG036294.D

Acq: 11 Aug 2018 9:11


Tgt Ion:240 Resp: 178753

Ion Ratio Lower Upper

240 100

120 4.6 6.8 10.2#



236 26.6 20.9 31.3

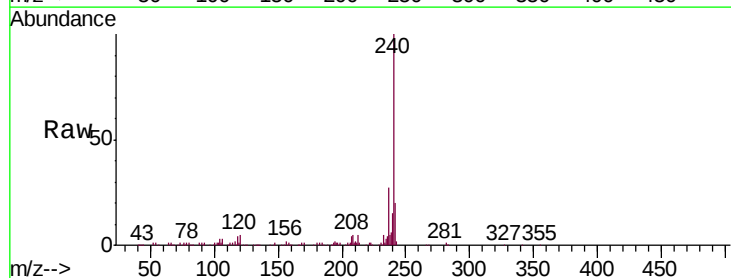


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

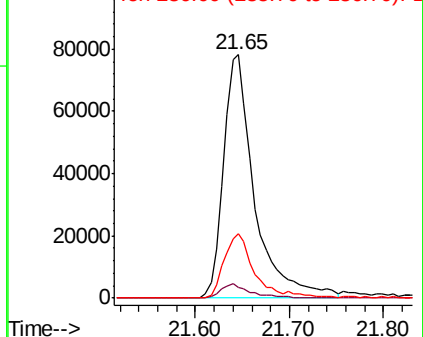



#78

Terphenyl-d14

Concen: 130.096 ng

RT: 19.98 min Scan# 2842

Delta R.T. -0.02 min

Lab File: BG036294.D

Acq: 11 Aug 2018 9:11

Instrument :

BNA_G

ClientSampleId :

HD-01-080918


Tgt Ion:244 Resp: 1054984

Ion Ratio Lower Upper

244 100

212 9.1 5.8 8.8#




122 6.5 7.0 10.4#

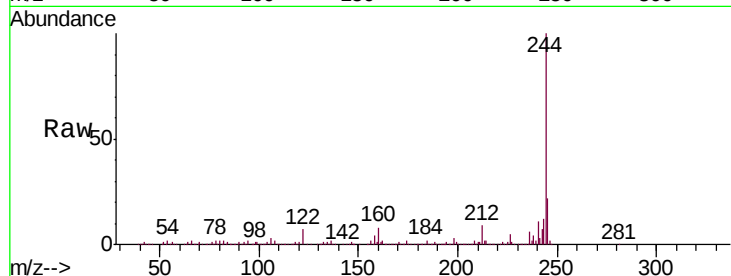

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

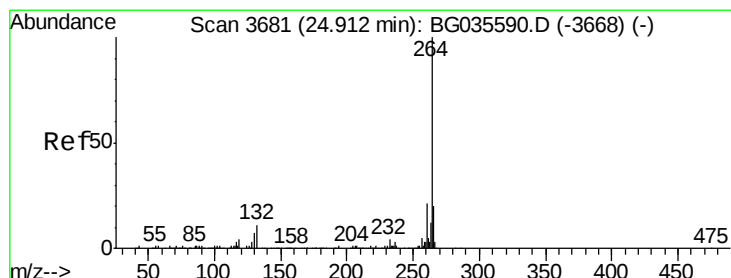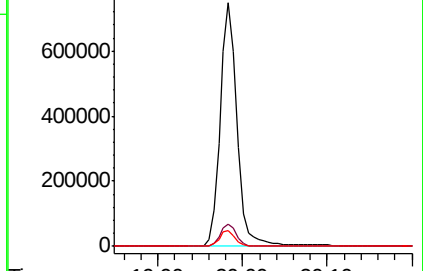

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.84 min Scan# 3668

Delta R.T. -0.02 min

Lab File: BG036294.D

Acq: 11 Aug 2018 9:11


Tgt Ion:264 Resp: 147645

Ion Ratio Lower Upper

264 100

260 22.9 17.4 26.0

265 23.1 17.7 26.5

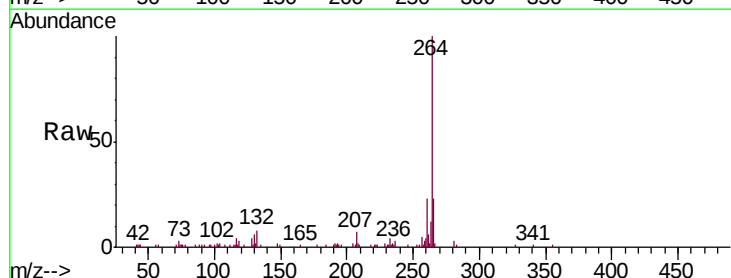

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

