


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081018\
 Data File : BG036286.D
 Acq On : 11 Aug 2018 3:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

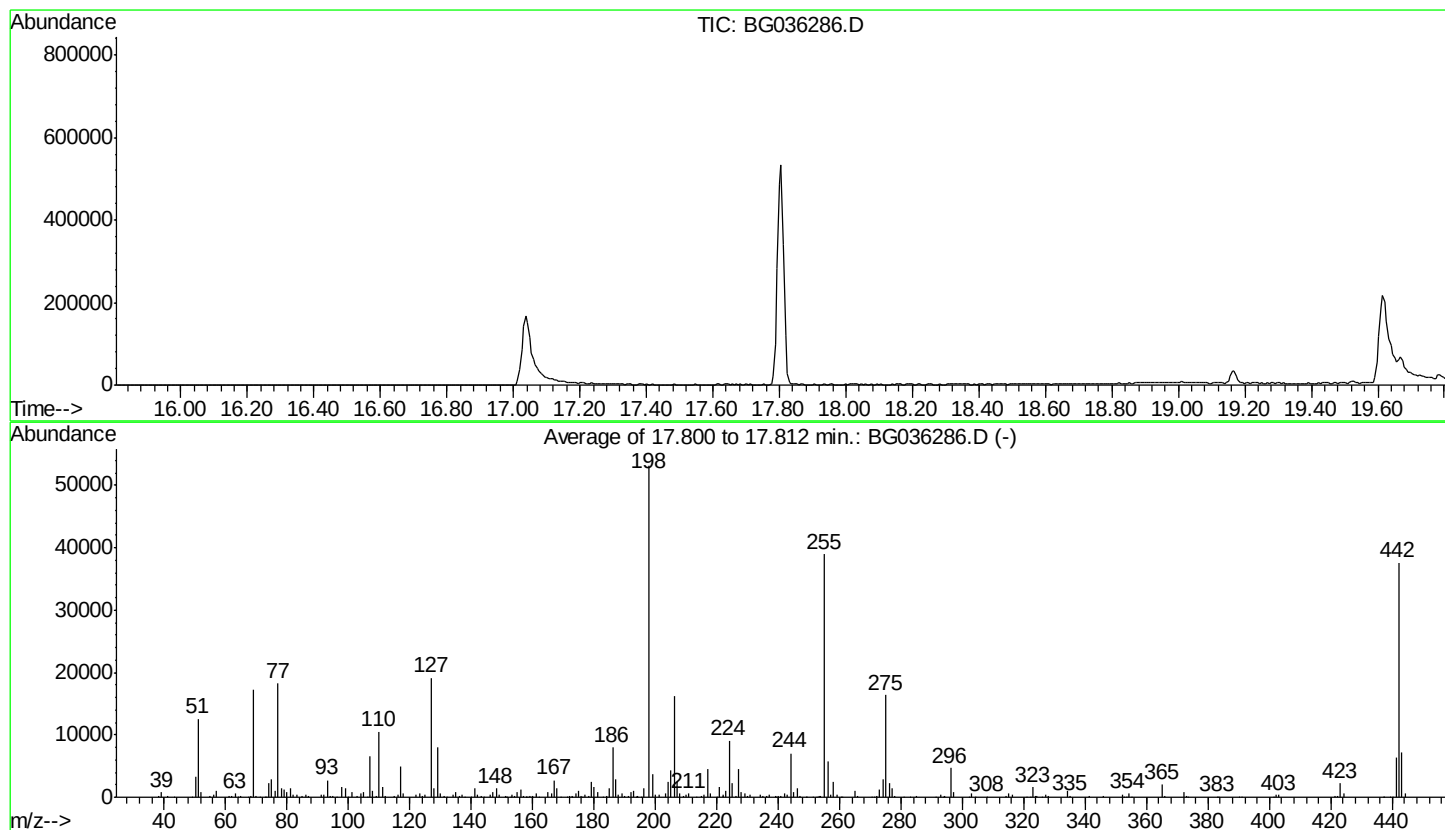

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.7	12577	PASS
68	69	0.00	2	1.1	190	PASS
69	198	0.00	100	32.5	17287	PASS
70	69	0.00	2	0.7	124	PASS
127	198	10	80	36.0	19130	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53146	PASS
199	198	5	9	6.8	3626	PASS
275	198	10	60	30.7	16330	PASS
365	198	1	100	3.7	1986	PASS
441	198	0.01	100	12.2	6458	PASS
442	198	50	100	70.8	37642	PASS
443	442	15	24	19.4	7286	PASS