

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081115\
 Data File : BG018390.D
 Acq On : 11 Aug 2015 20:36
 Operator : UM/MA
 Sample : G3154-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01Y4

Quant Time: Aug 12 01:03:00 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 12 00:54:17 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	109978	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	548353	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	346080	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	726737	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	636010	20.00	ng/ul	0.00
86) Perylene-d12	24.91	264	639188	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	10615	4.26	ng/uL	0.00
5) Phenol-d5	7.20	99	234954	23.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	146548	23.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	181182	23.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	183022	21.82	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	91825	21.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	99643	22.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	189585	20.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.97	131	197953	18.96	ng/ul	0.00
44) Dimethylphthalate-d6	14.07	166	580380	19.93	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	649539	17.71	ng/ul	0.00
52) 4-Nitrophenol-d4	14.86	143	68741	13.12	ng/ul	0.01
58) Fluorene-d10	15.66	176	421473	16.62	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.77	200	19993	5.59	ng/ul	0.00
71) Anthracene-d10	17.51	188	517957	14.90	ng/ul	0.00
79) Pyrene-d10	19.79	212	411754	12.48	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.68	264	254727	7.51	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.12	163	250845	8.73	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081115\
Data File : BG018390.D
Acq On : 11 Aug 2015 20:36
Operator : UM/MA
Sample : G3154-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01Y4

Quant Time: Aug 12 01:03:00 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 12 00:54:17 2015
Response via : Initial Calibration

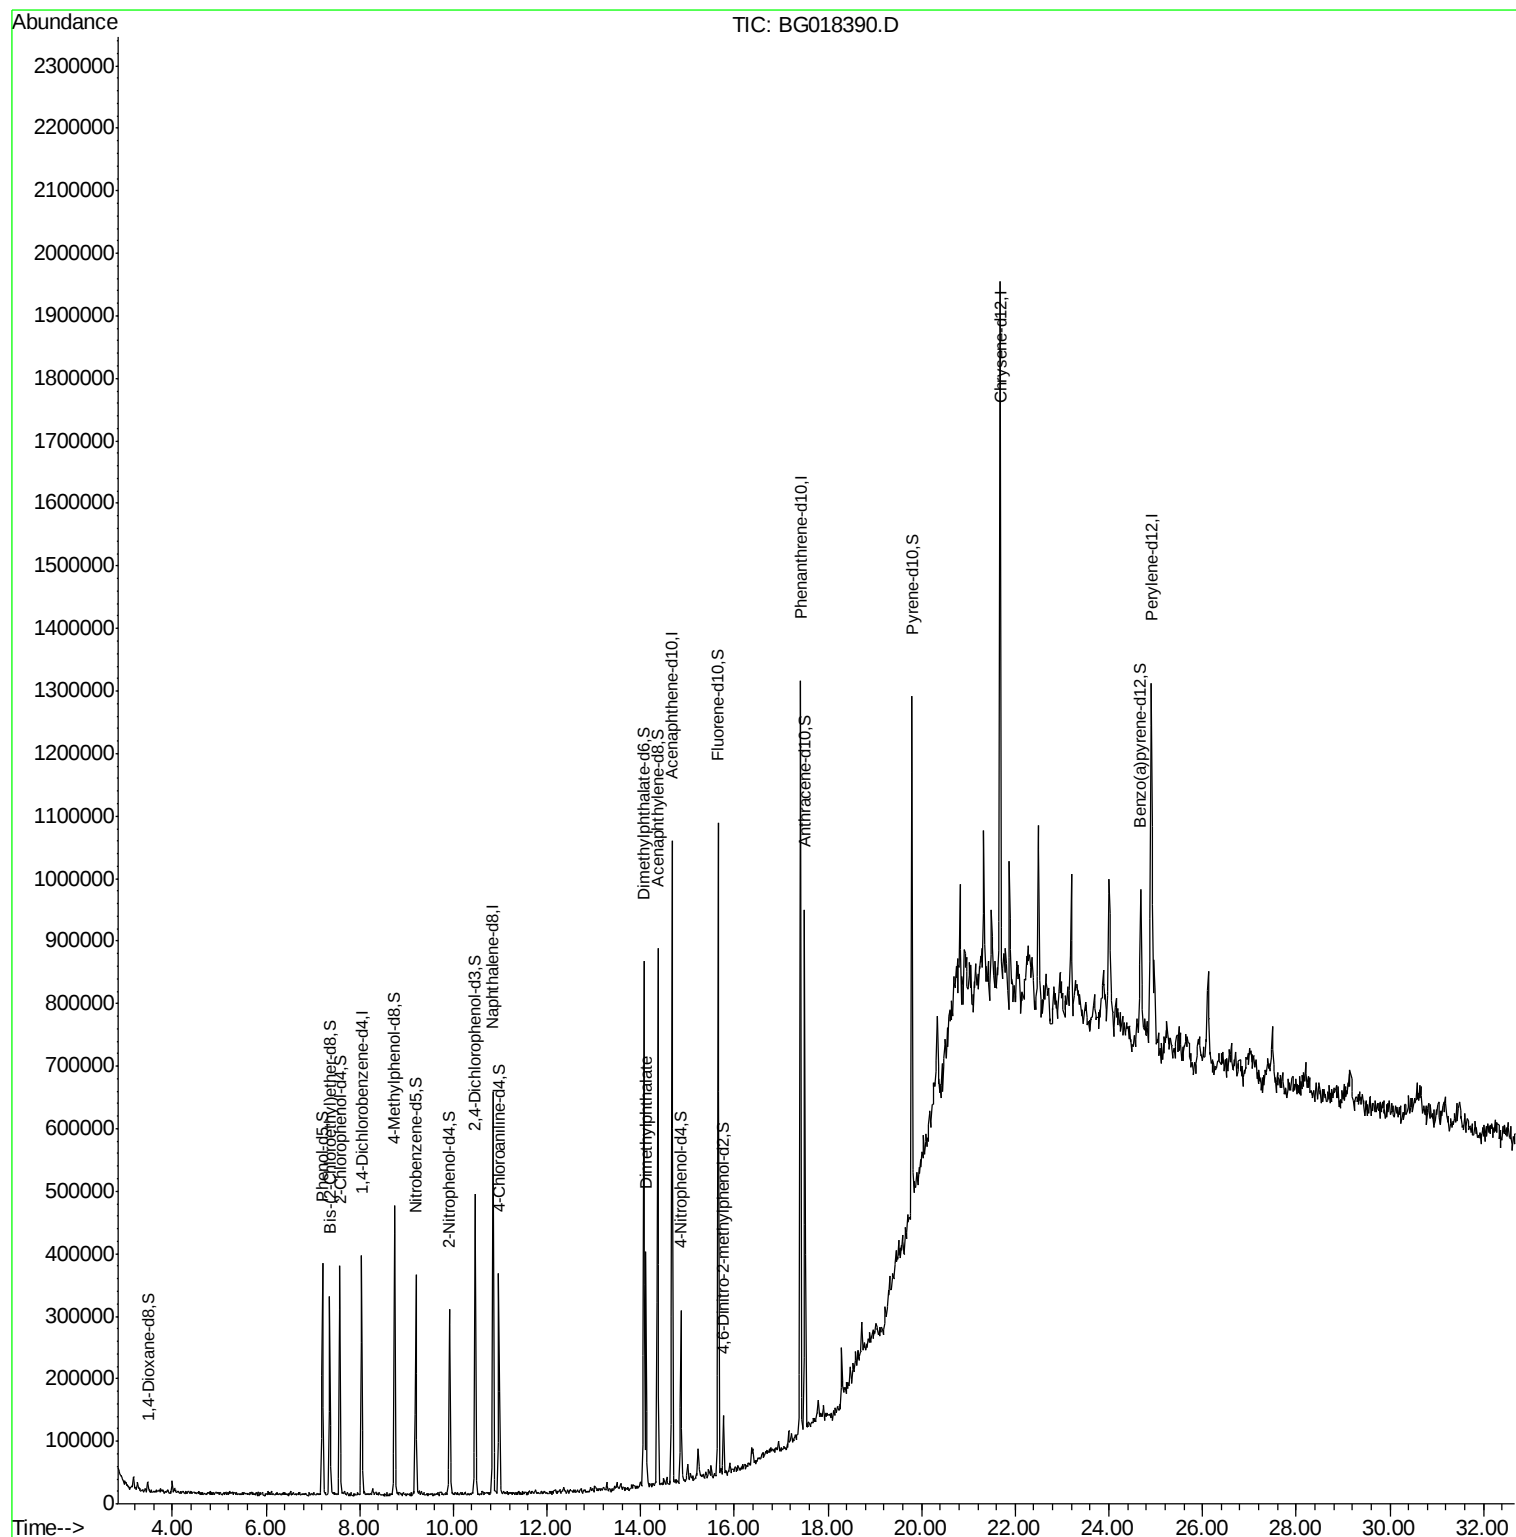


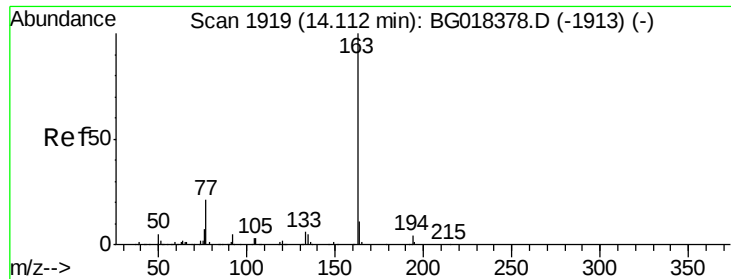

#45
 Dimethylphthalate
 Concen: 8.73 ng/ul
 RT: 14.12 min Scan# 1920
 Delta R.T. 0.01 min
 Lab File: BG018390.D
 Acq: 11 Aug 2015 20:36

Instrument :
 BNA_G
 ClientSampleId :
 C01Y4

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.2	2.9	4.3
164	10.1	7.7	11.5

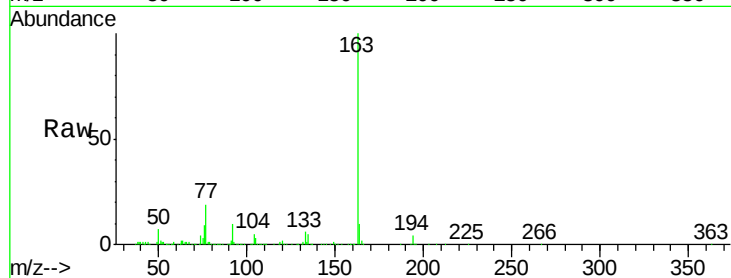

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

