




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

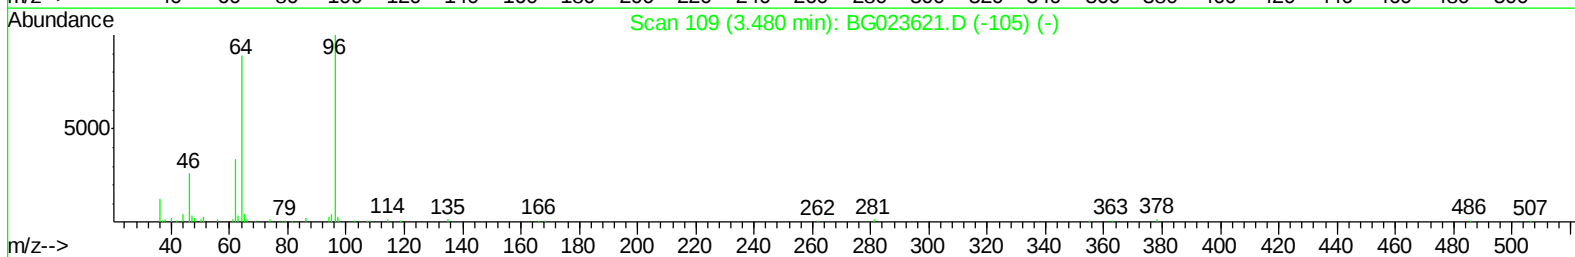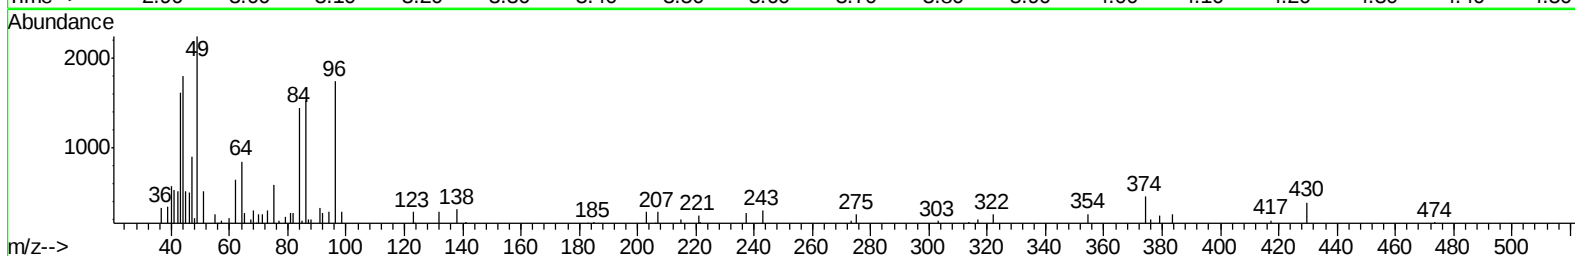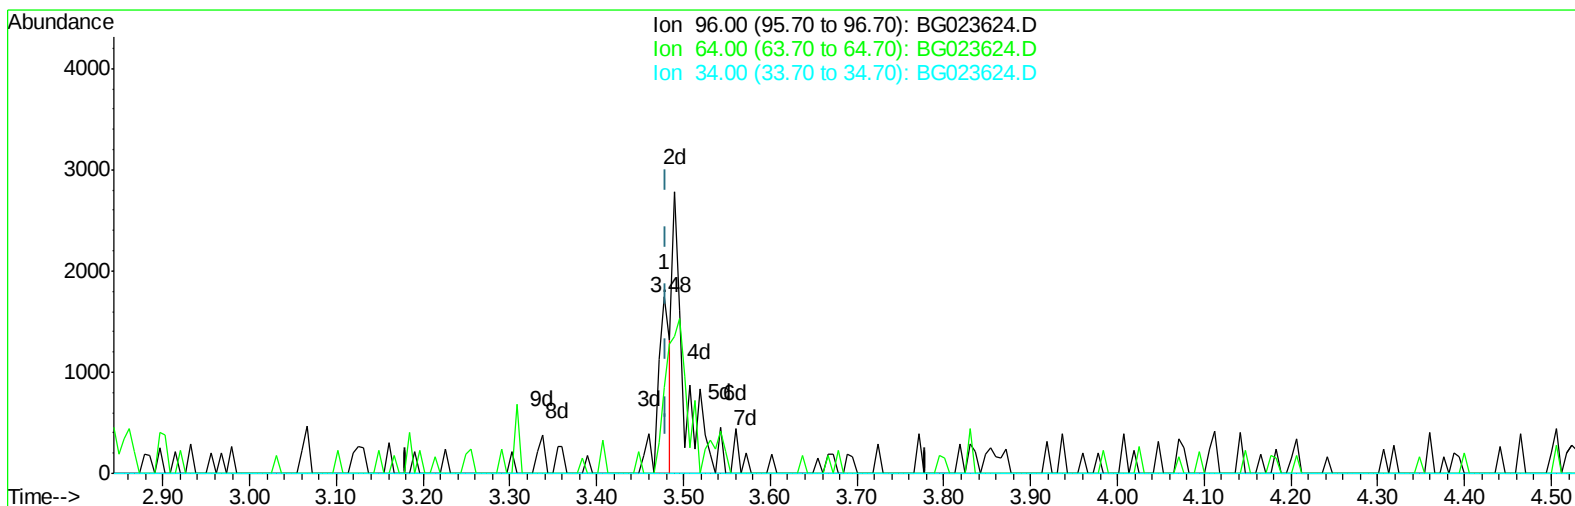

TIC: BG023624.D

(3) 1,4-Dioxane-d8 (S)

3.478min (-0.002) 0.29ng/uL

response 1471

Ion	Exp%	Act%
96.00	100	100
64.00	65.00	48.48#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

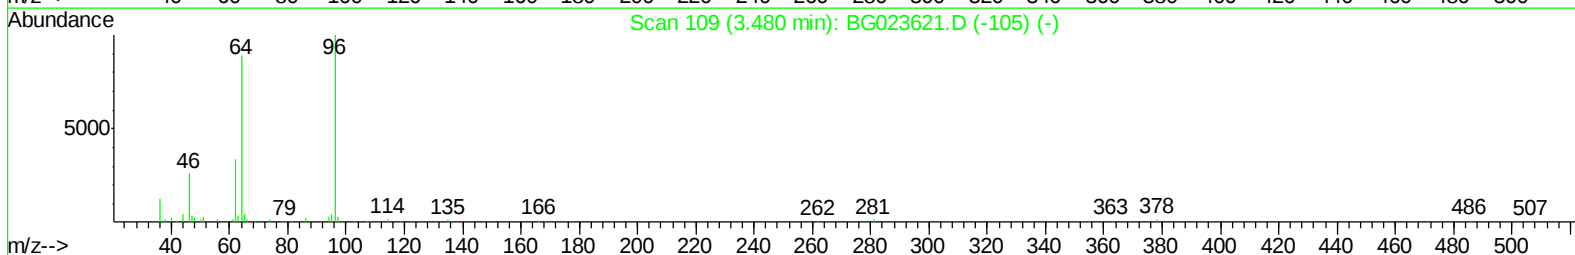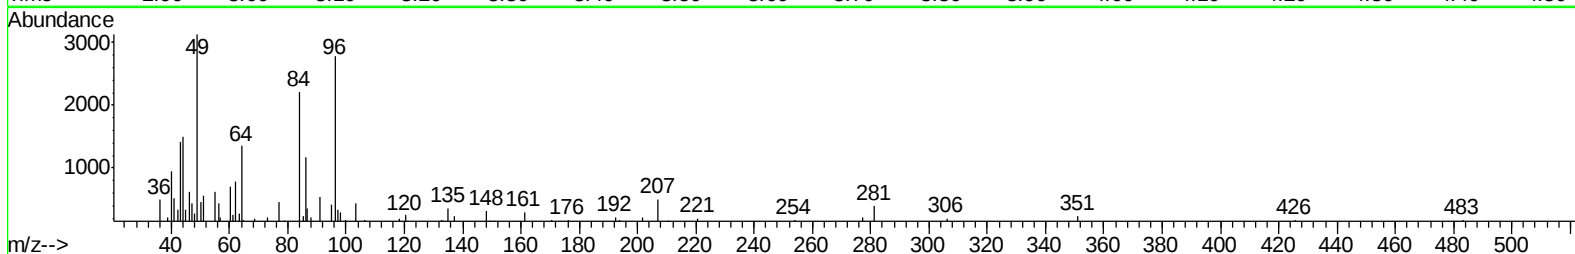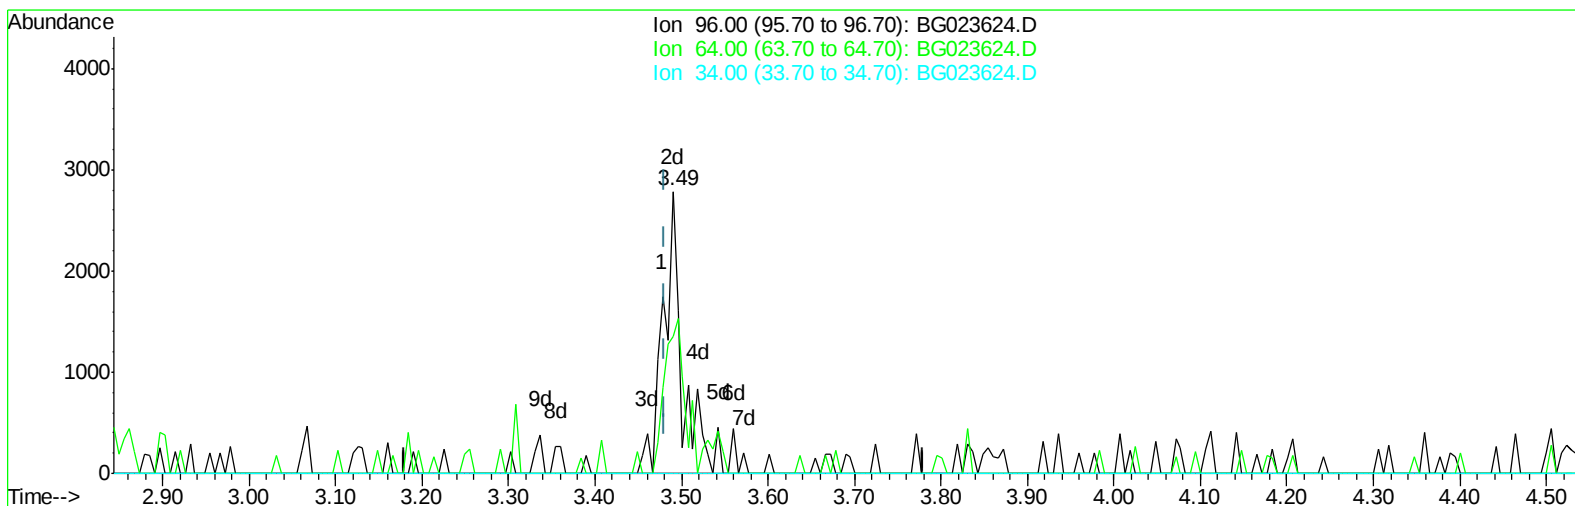

TIC: BG023624.D

(3) 1,4-Dioxane-d8 (S)

3.490min (+0.010) 0.83ng/uL m

response 4194

Ion	Exp%	Act%
96.00	100	100
64.00	65.00	48.60#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

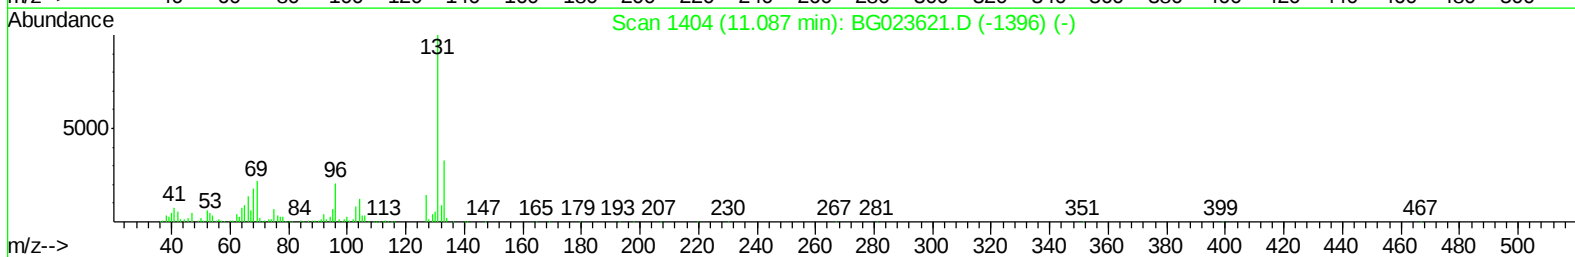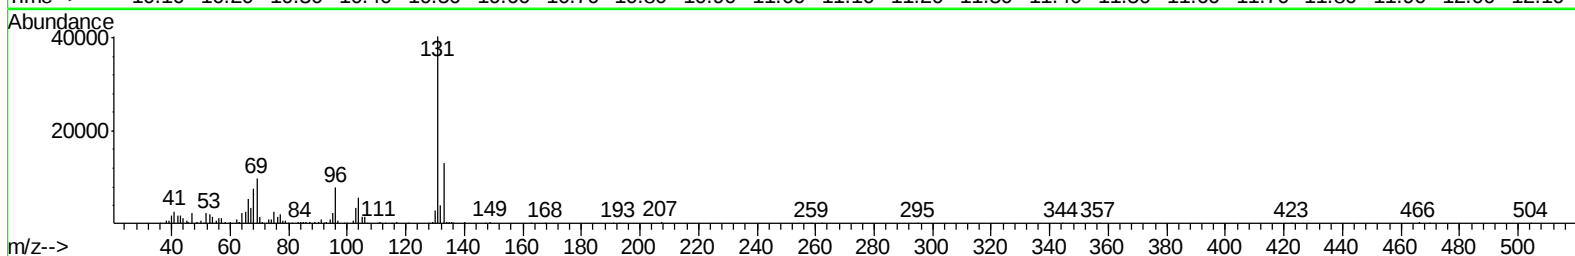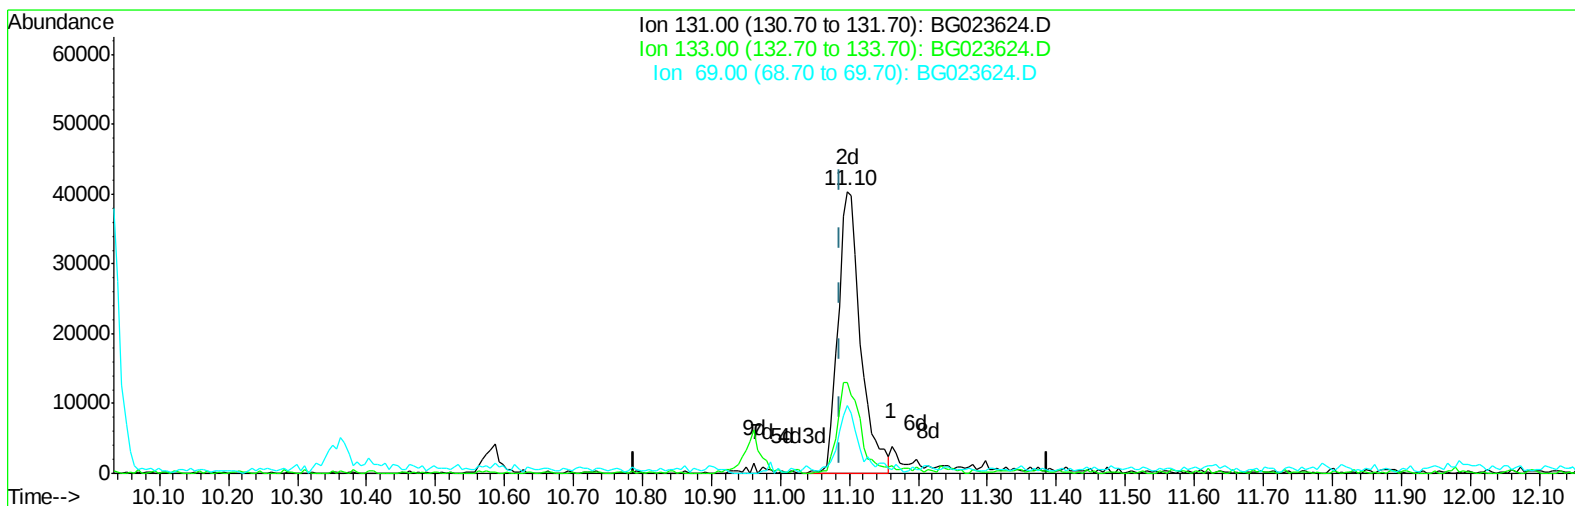

TIC: BG023624.D

(29) 4-Chloroaniline-d4 (S)

11.097min (+0.010) 4.56ng/ul m

response 92012

Ion	Exp%	Act%
131.00	100	100
133.00	33.10	32.15
69.00	15.40	24.11#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

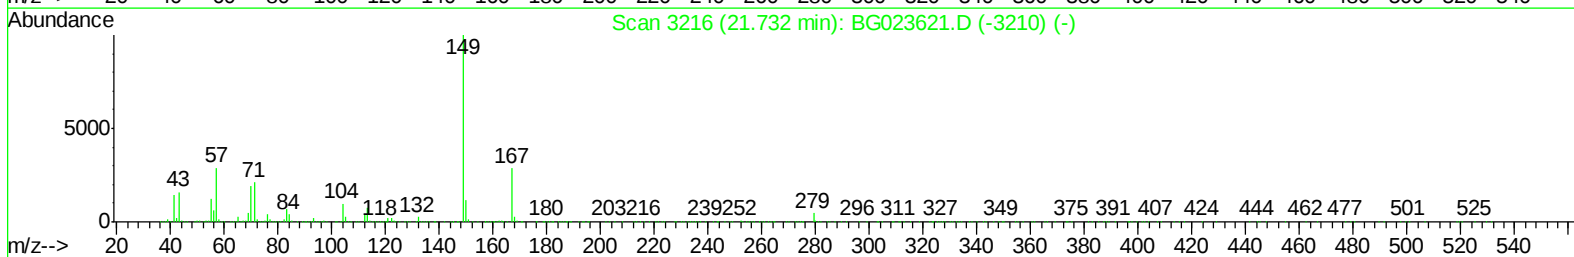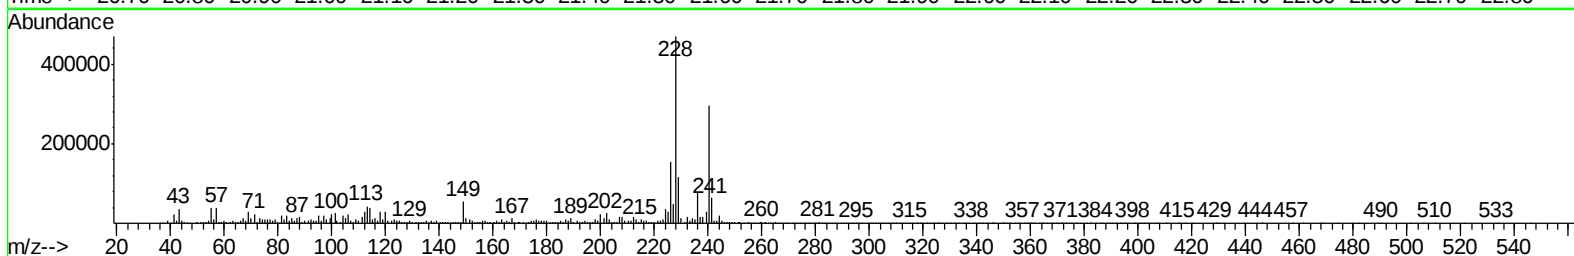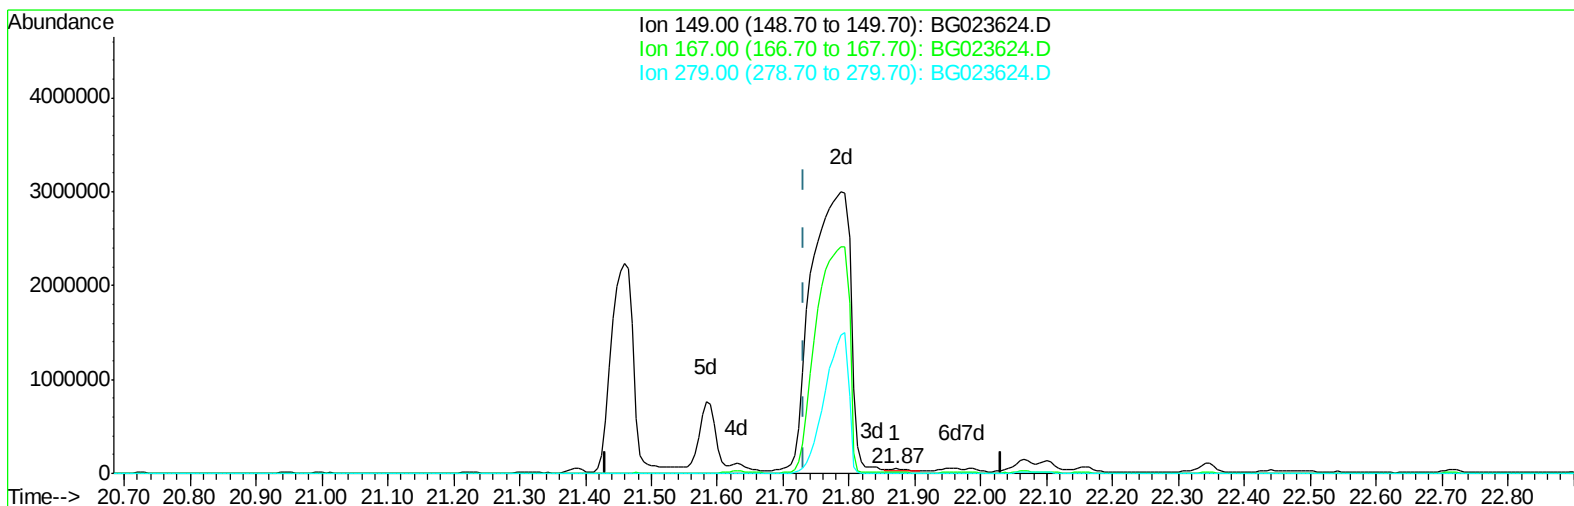

TIC: BG023624.D

(81) Bis(2-ethylhexyl)phthalate

21.871min (+0.139) 1.28ng/ul

response 49554

Ion	Exp%	Act%
149.00	100	100
167.00	27.40	23.21
279.00	3.60	3.41
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

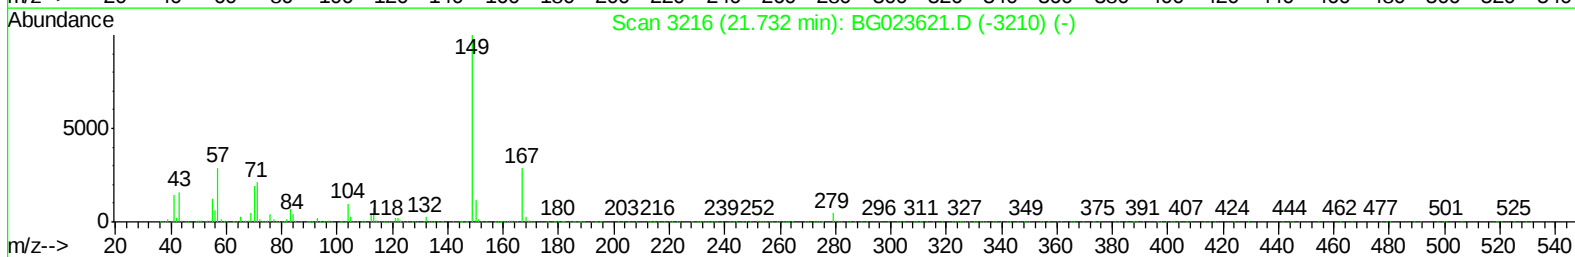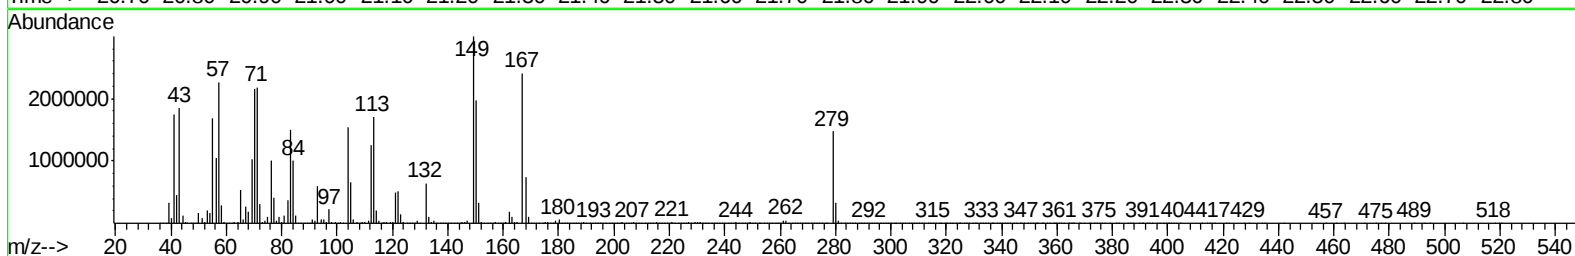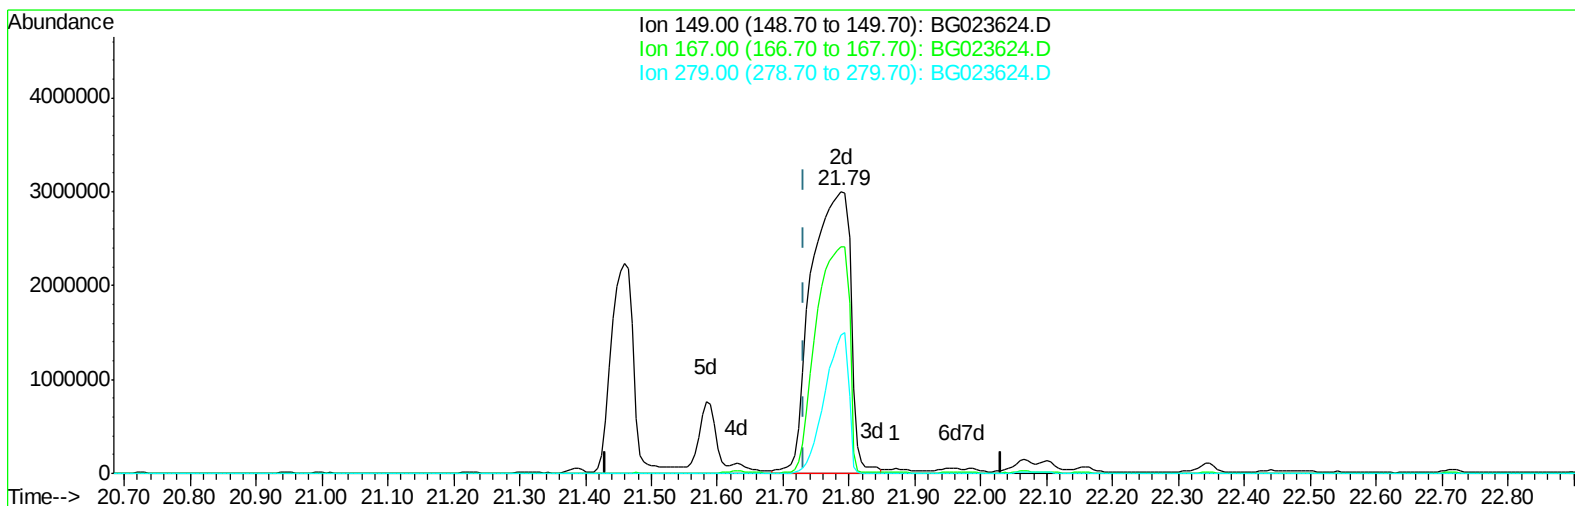

TIC: BG023624.D

(81) Bis(2-ethylhexyl)phthalate

21.788min (+0.057) 317.00ng/ul m

response 12273802

Ion	Exp%	Act%
149.00	100	100
167.00	27.40	80.36#
279.00	3.60	49.09#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
 Data File : BG023624.D
 Acq On : 11 Aug 2016 13:22
 Operator : UM/SJ
 Sample : H4362-01 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS004-2430-01

Manual Integrations
 APPROVED

sohil
 8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 12 03:45:04 2016
 Response via : Initial Calibration

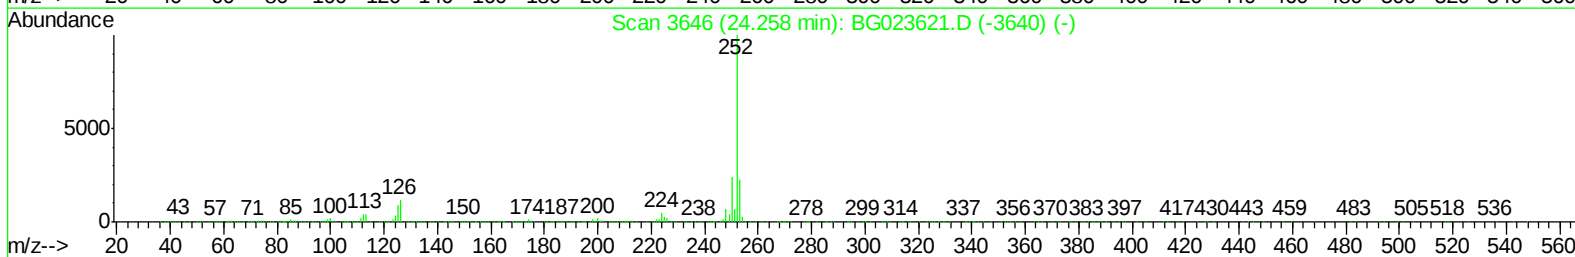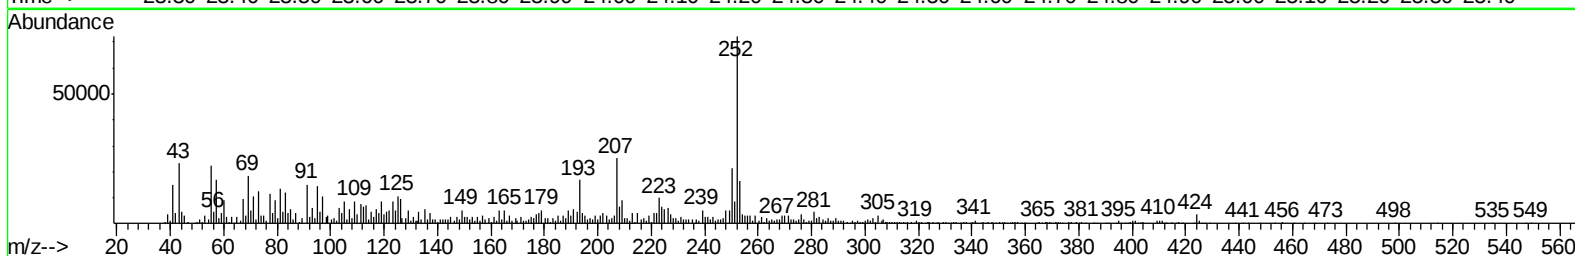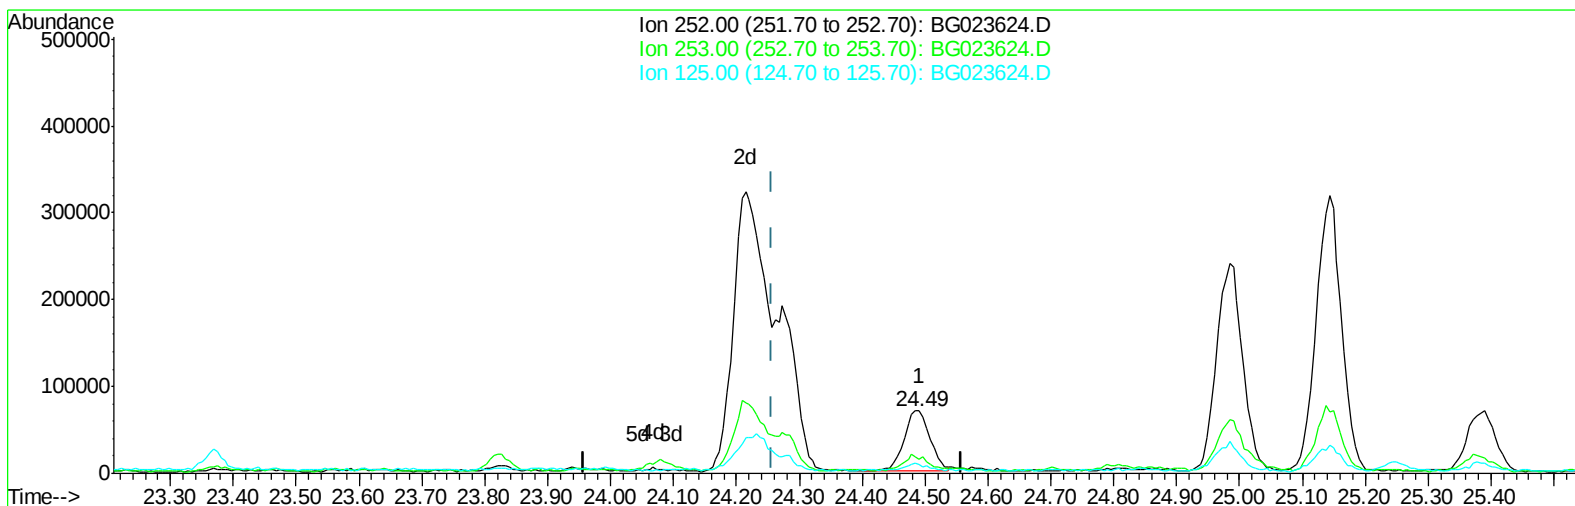

TIC: BG023624.D

(86) Benzo(k)fluoranthene

24.491min (+0.233) 2.95ng/ul

response 201329

Ion	Exp%	Act%
252.00	100	100
253.00	19.70	23.12
125.00	13.30	14.75
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
 Data File : BG023624.D
 Acq On : 11 Aug 2016 13:22
 Operator : UM/SJ
 Sample : H4362-01 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS004-2430-01

Manual Integrations
 APPROVED

sohil
 8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 12 03:45:04 2016
 Response via : Initial Calibration

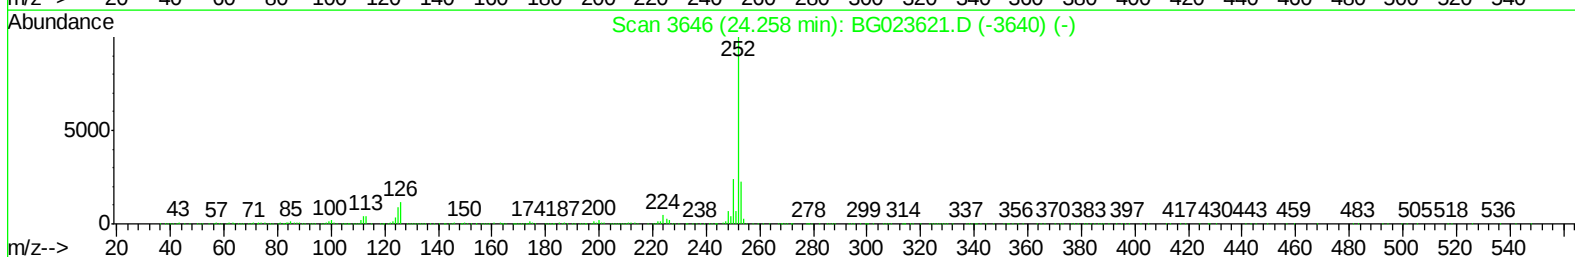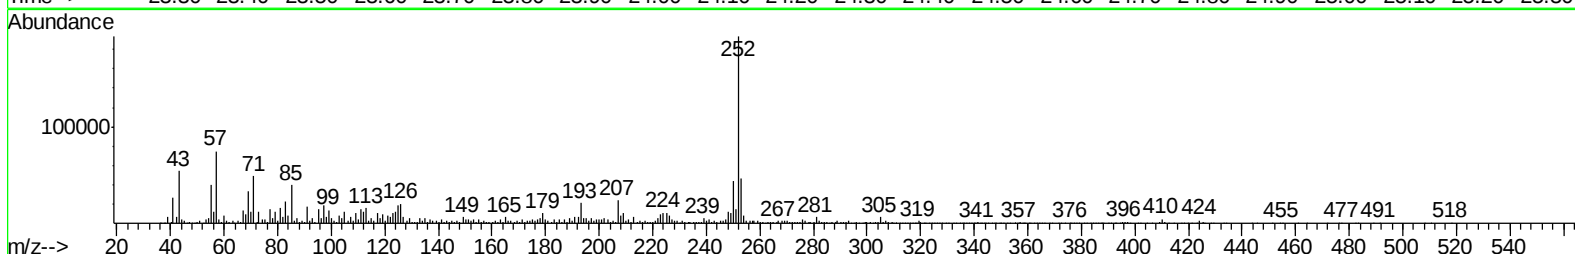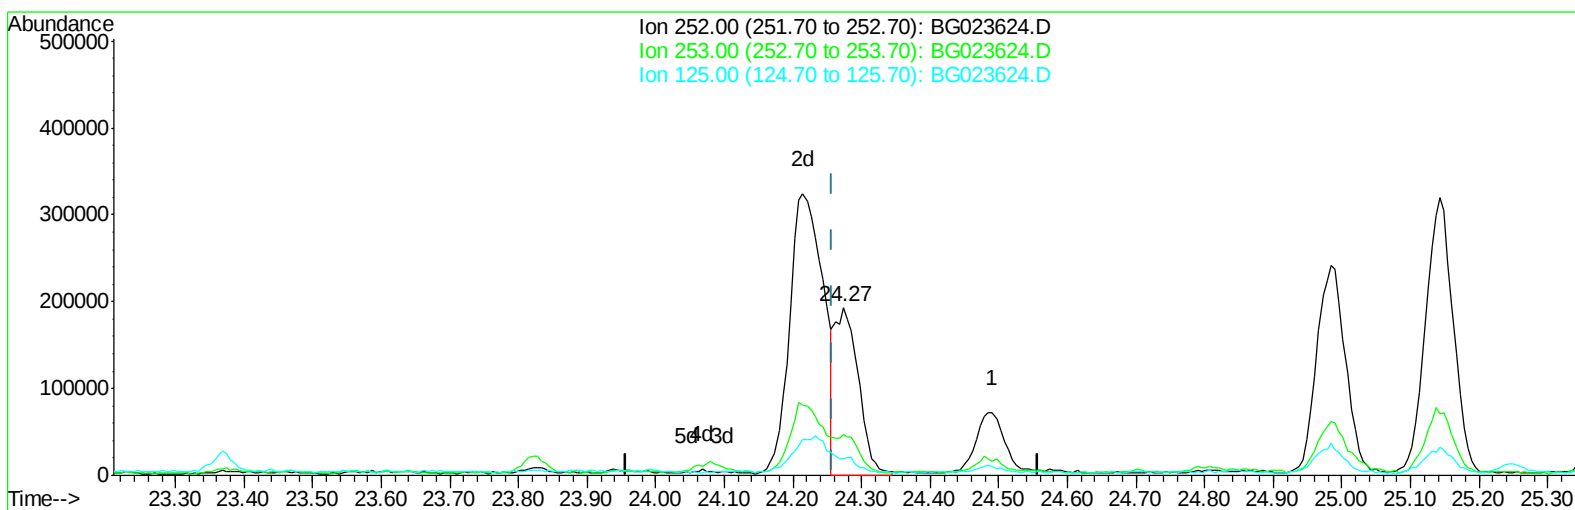

TIC: BG023624.D

(86) Benzo(k)fluoranthene

24.273min (+0.015) 6.69ng/ul m

response 456035

Ion	Exp%	Act%
252.00	100	100
253.00	19.70	24.22#
125.00	13.30	9.94#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

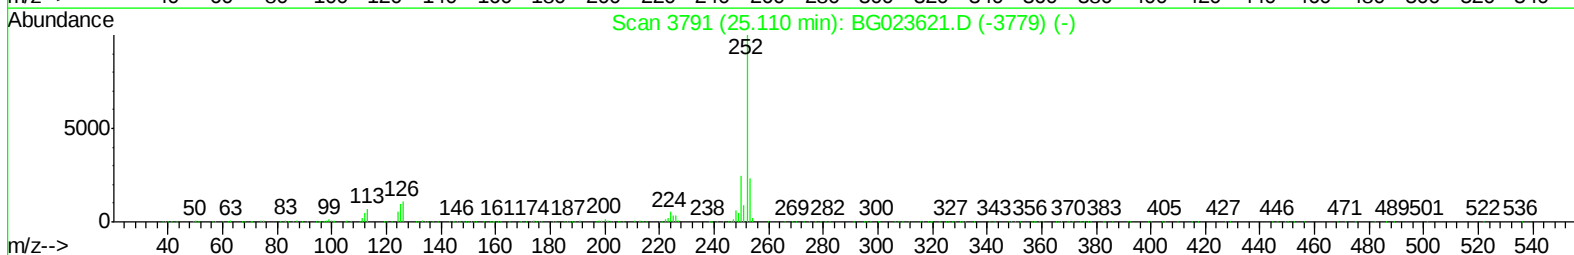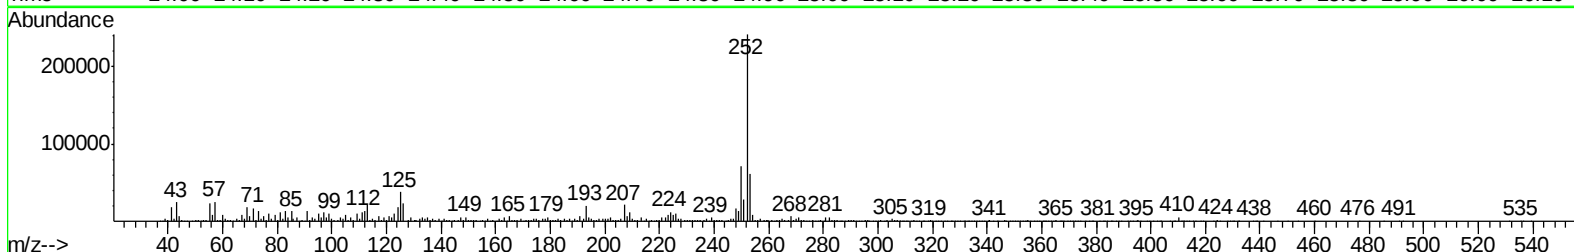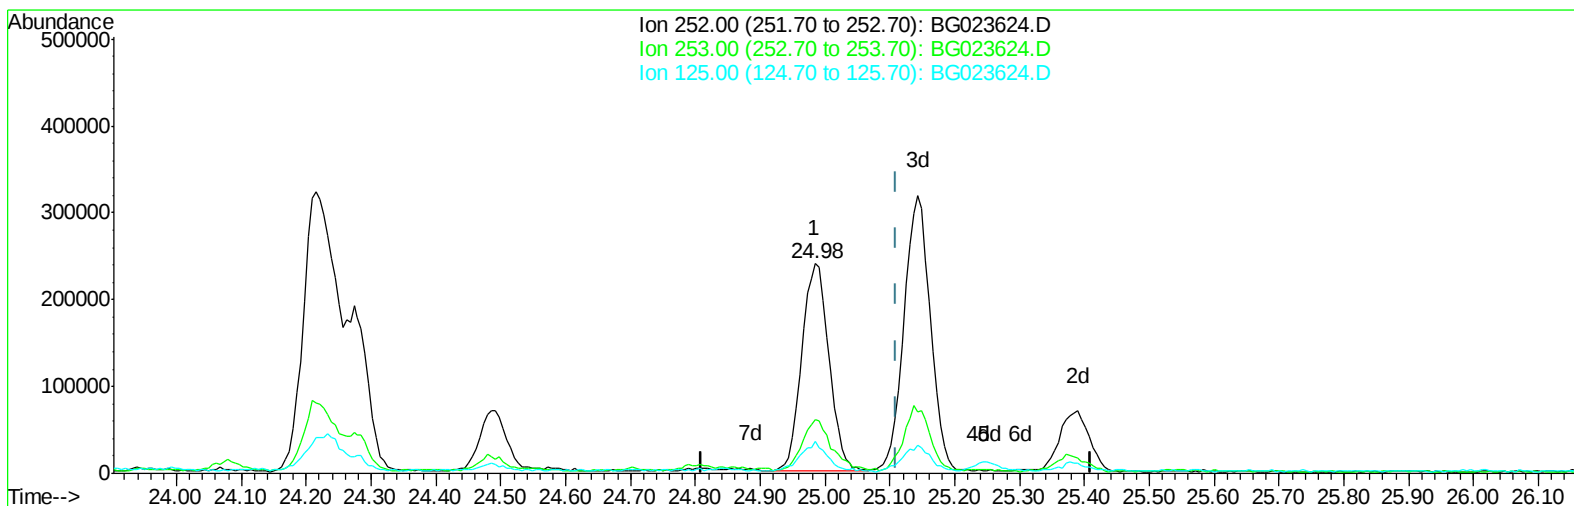

TIC: BG023624.D

(88) Benzo(a)pyrene (C)

24.984min (-0.126) 10.36ng/ul

response 692840

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	25.53
125.00	15.00	15.50
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

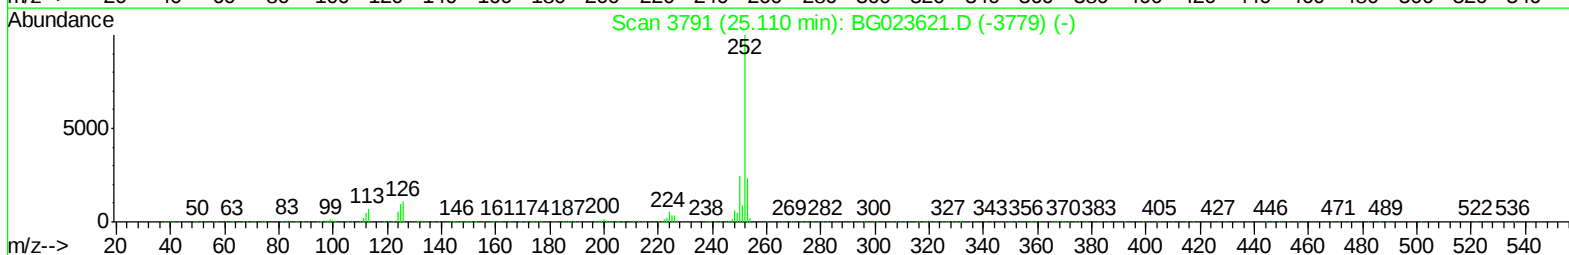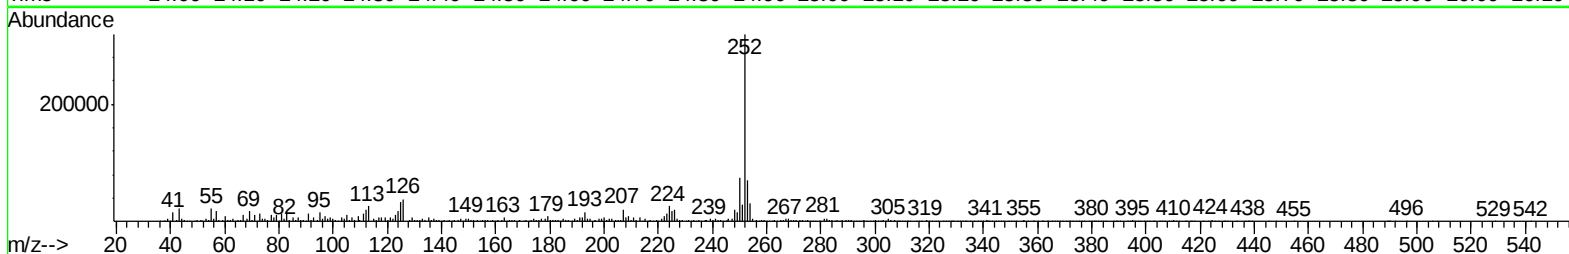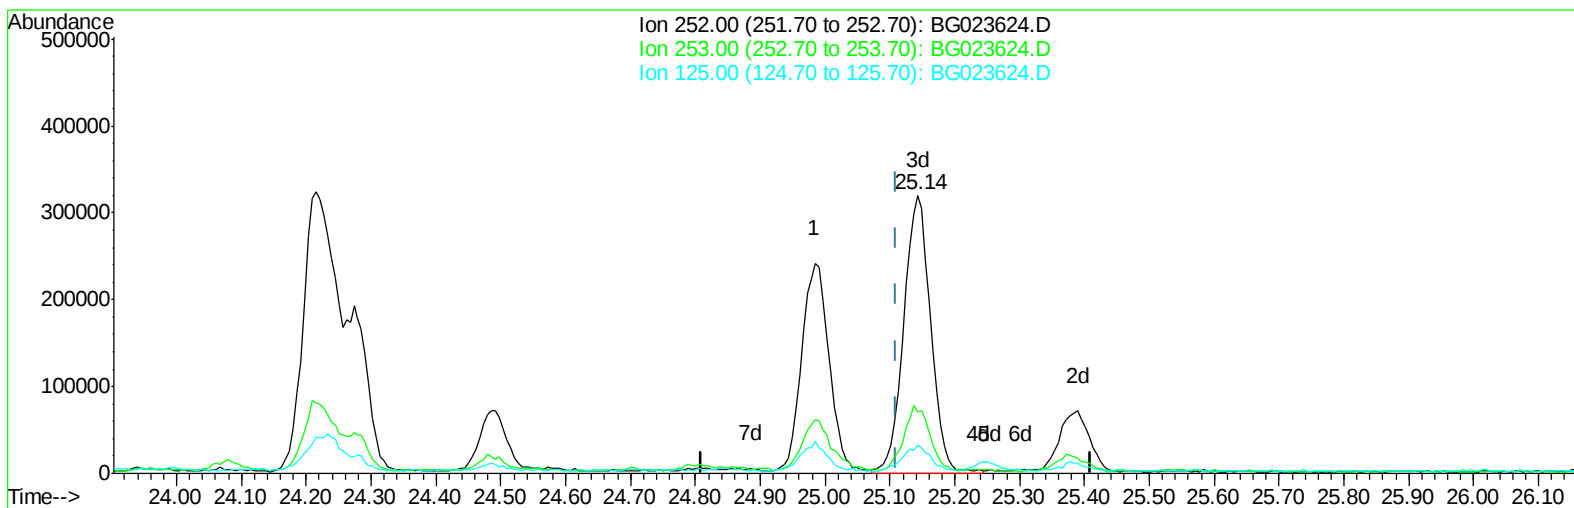

TIC: BG023624.D

(88) Benzo(a)pyrene (C)

25.143min (+0.033) 13.72ng/ul m

response 917671

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	21.94
125.00	15.00	10.32#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

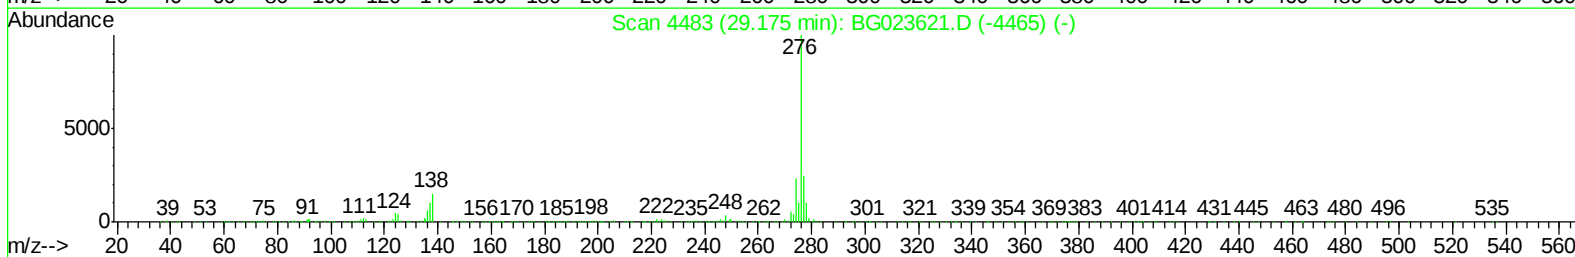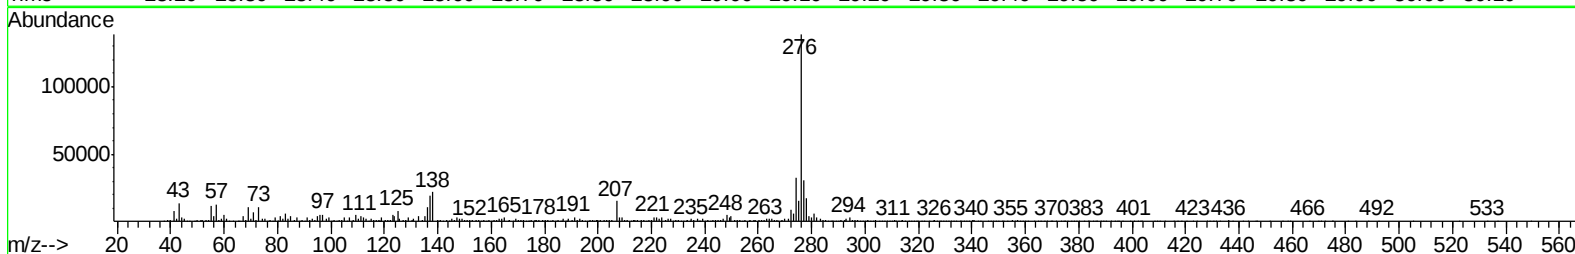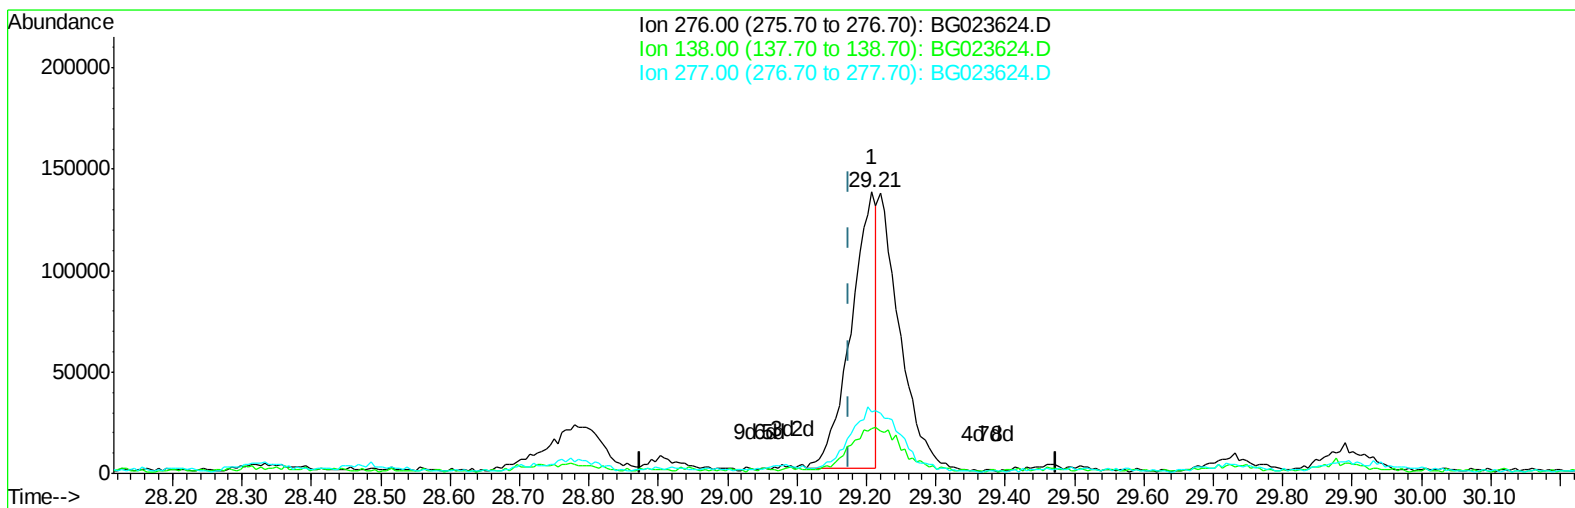

TIC: BG023624.D

(89) Indeno(1,2,3-cd)pyrene

29.208min (+0.033) 4.38ng/ul

response 344589

Ion	Exp%	Act%
276.00	100	100
138.00	26.00	15.81#
277.00	22.00	21.72
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
 Data File : BG023624.D
 Acq On : 11 Aug 2016 13:22
 Operator : UM/SJ
 Sample : H4362-01 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS004-2430-01

Manual Integrations
 APPROVED

sohil
 8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 12 03:45:04 2016
 Response via : Initial Calibration

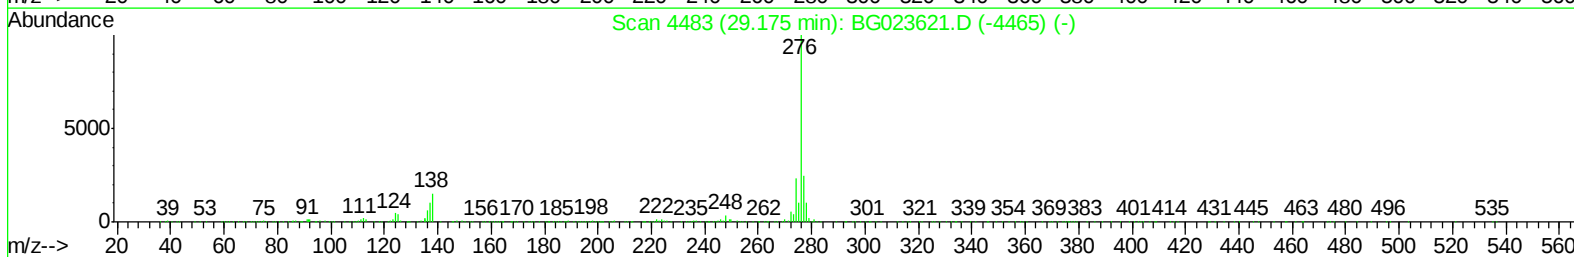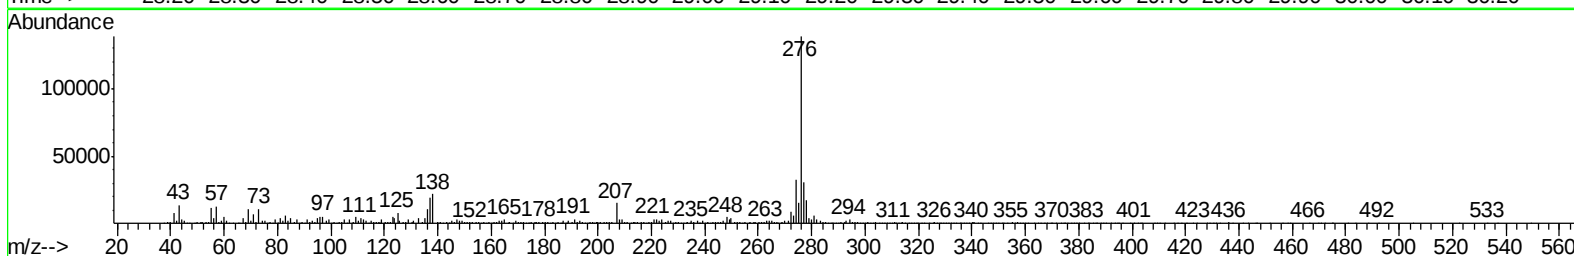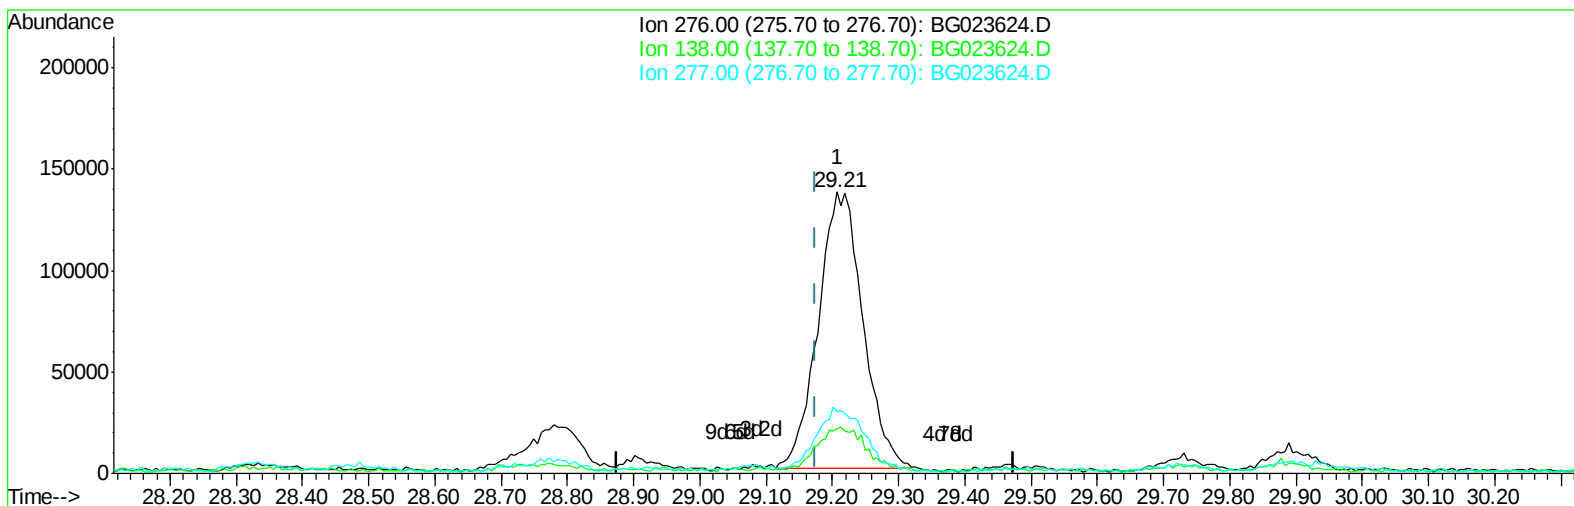

TIC: BG023624.D

(89) Indeno(1,2,3-cd)pyrene

29.208min (+0.033) 8.05ng/ul m

response 632950

Ion	Exp%	Act%
276.00	100	100
138.00	26.00	15.81#
277.00	22.00	21.72
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

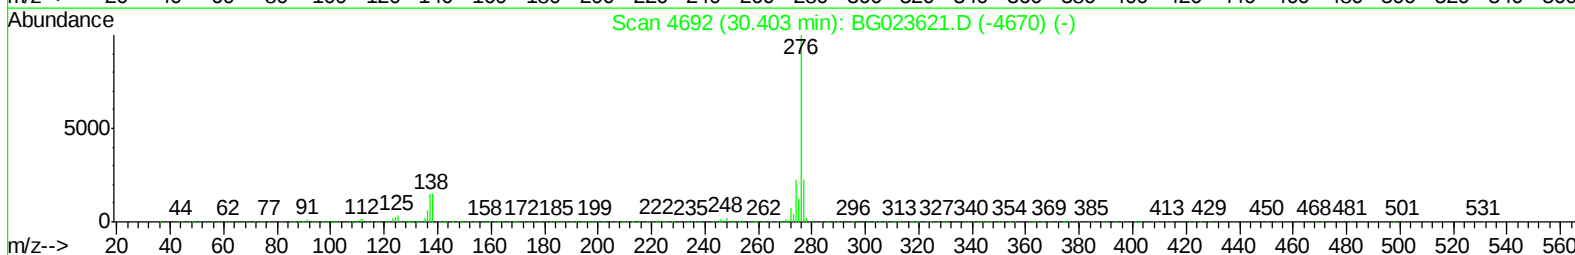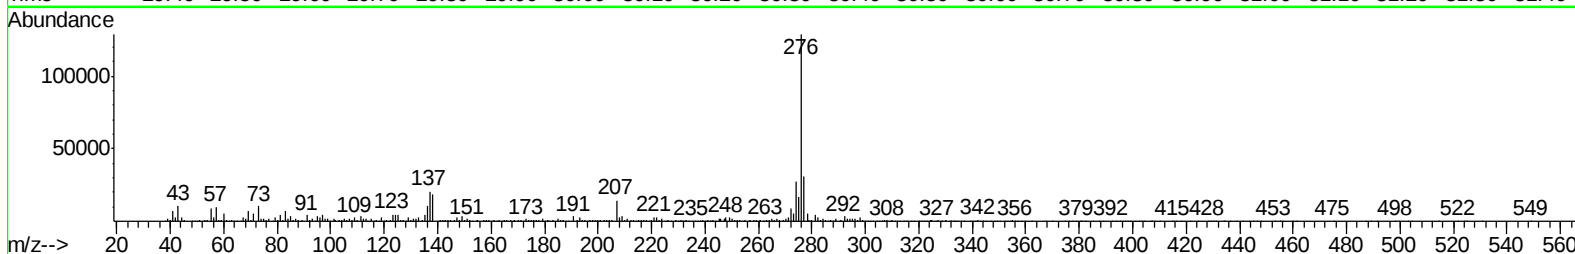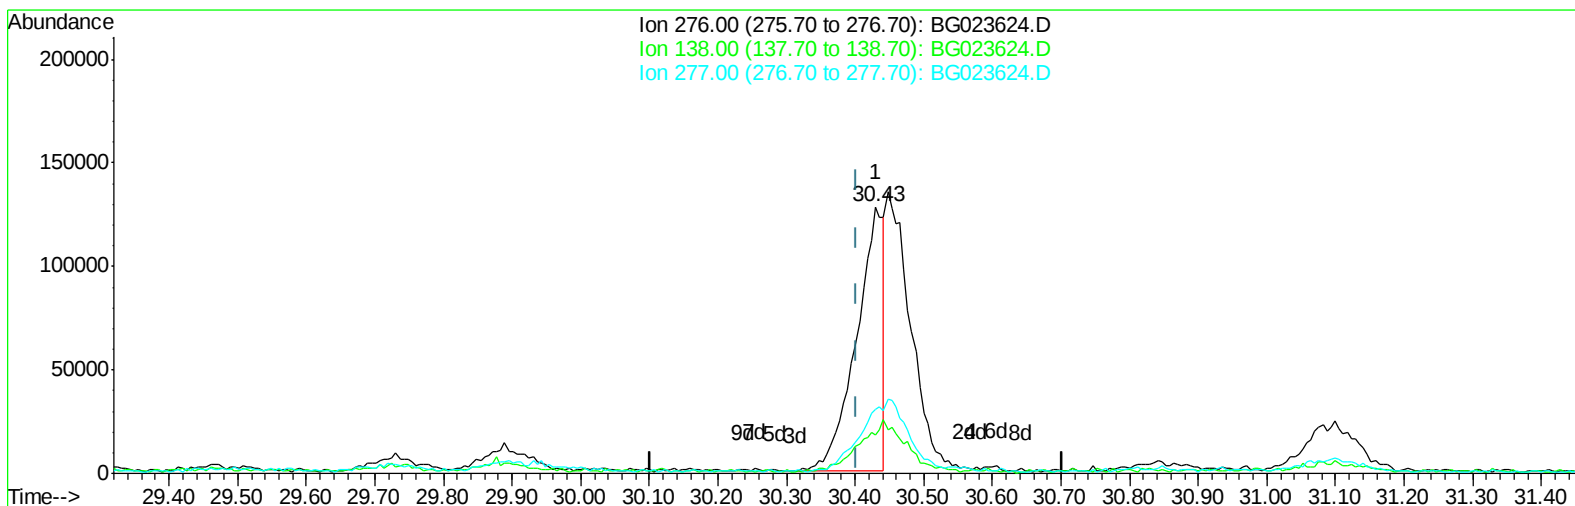

TIC: BG023624.D

(91) Benzo(g,h,i)perylene

30.430min (+0.027) 5.48ng/ul

response 356834

Ion	Exp%	Act%
276.00	100	100
138.00	27.60	14.35#
277.00	21.20	24.20
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Quant Time: Aug 12 03:45:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

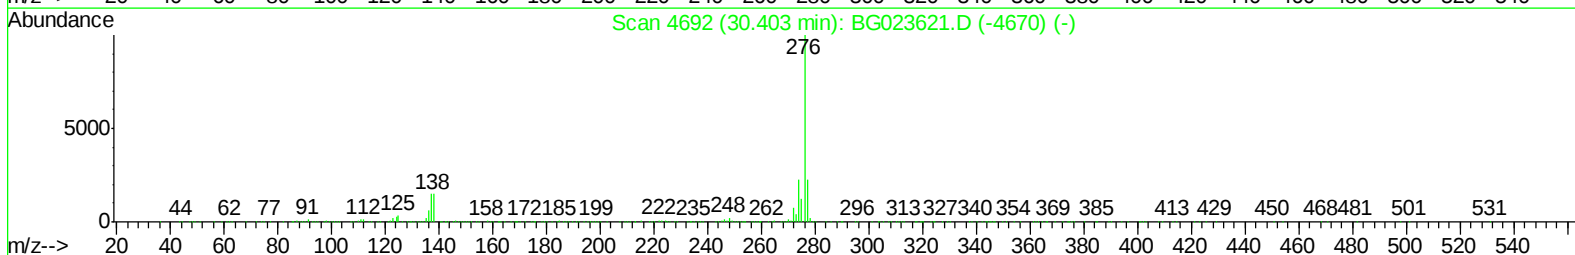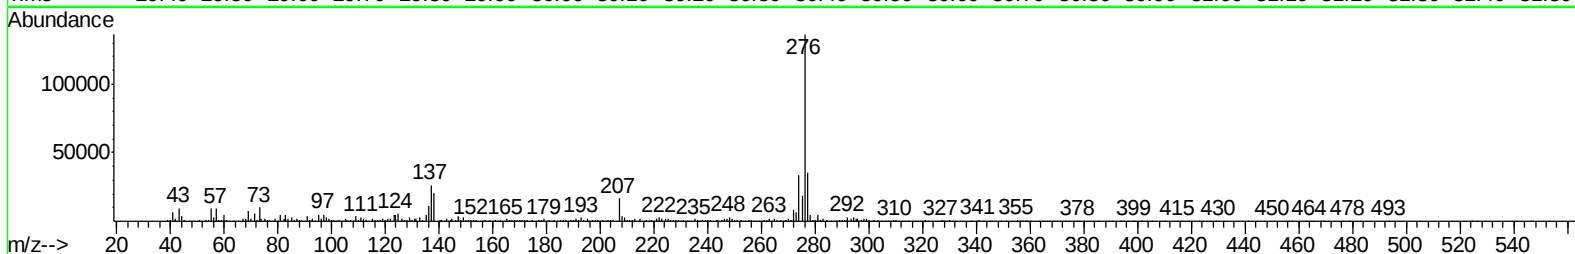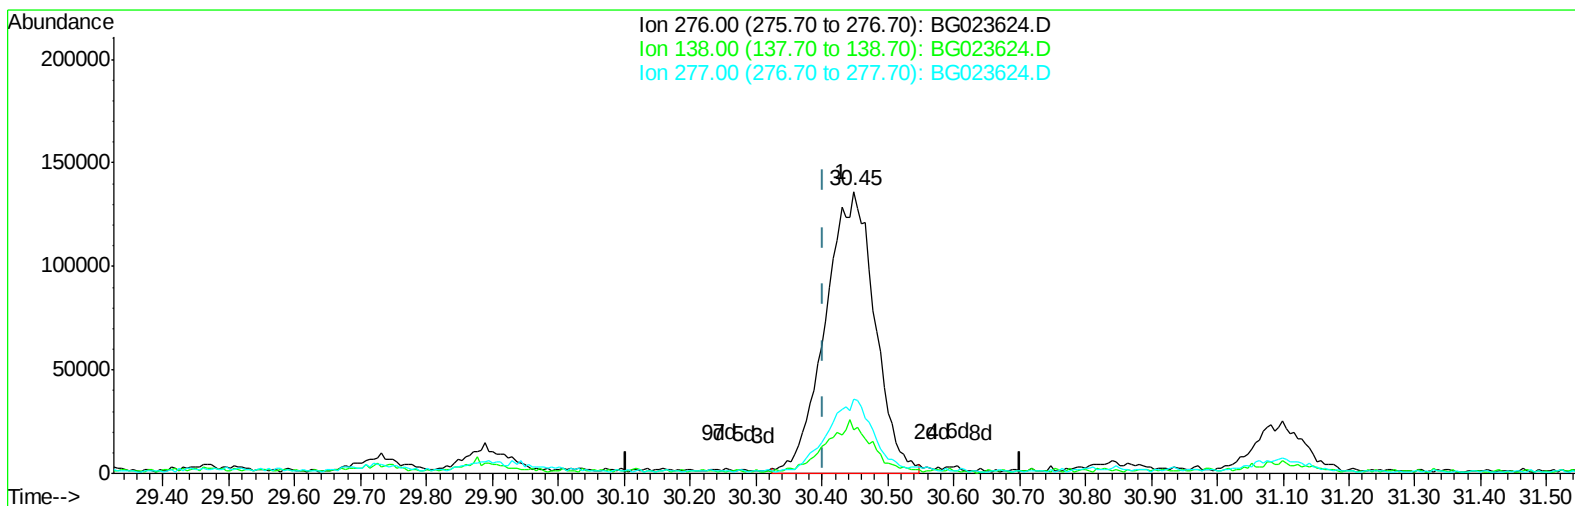

TIC: BG023624.D

(91) Benzo(g,h,i)perylene

30.447min (+0.045) 10.78ng/ul m

response 702435

Ion	Exp%	Act%
276.00	100	100
138.00	27.60	15.28#
277.00	21.20	26.31#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Quant Time: Aug 12 03:52:47 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

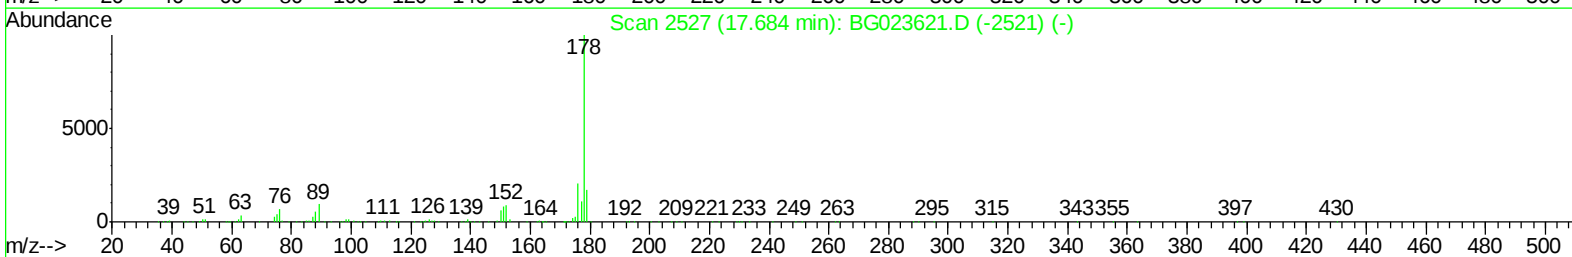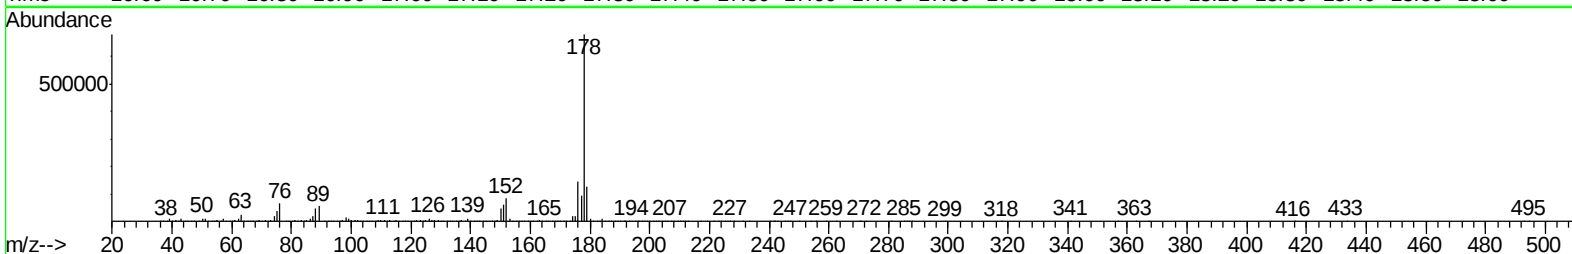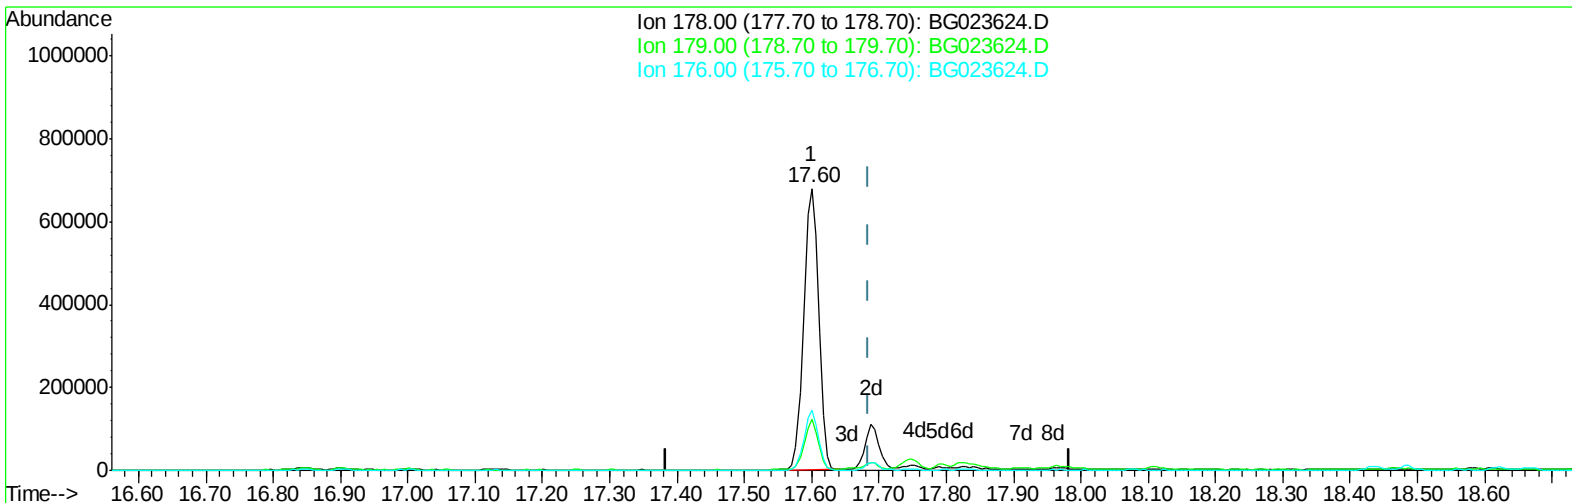

TIC: BG023624.D

(71) Anthracene

17.600min (-0.084) 13.80ng/ul

response 1062566

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	18.20
176.00	20.40	21.51
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Quant Time: Aug 12 03:52:47 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

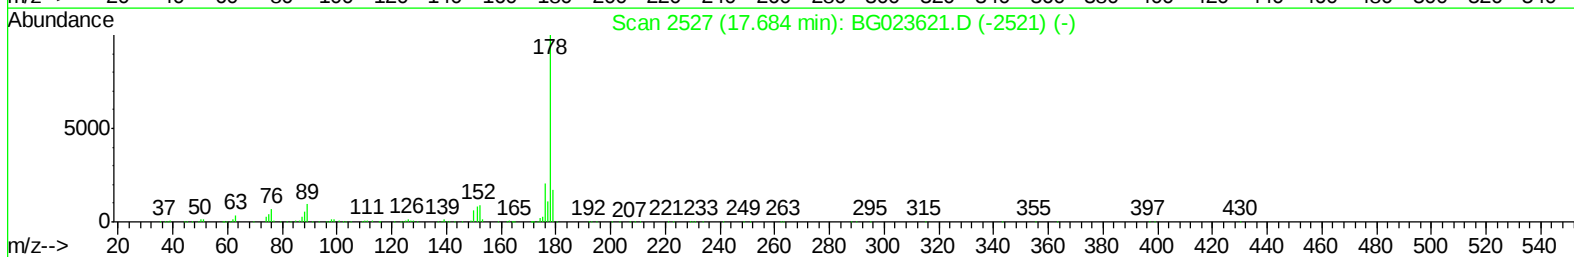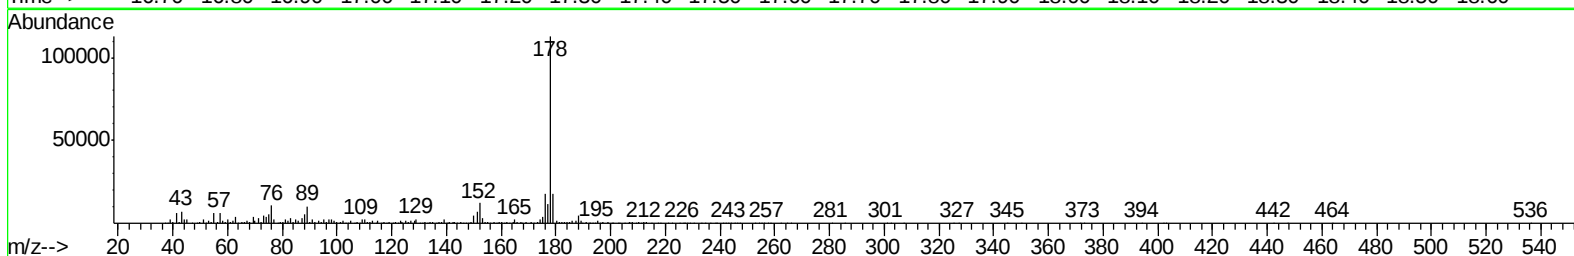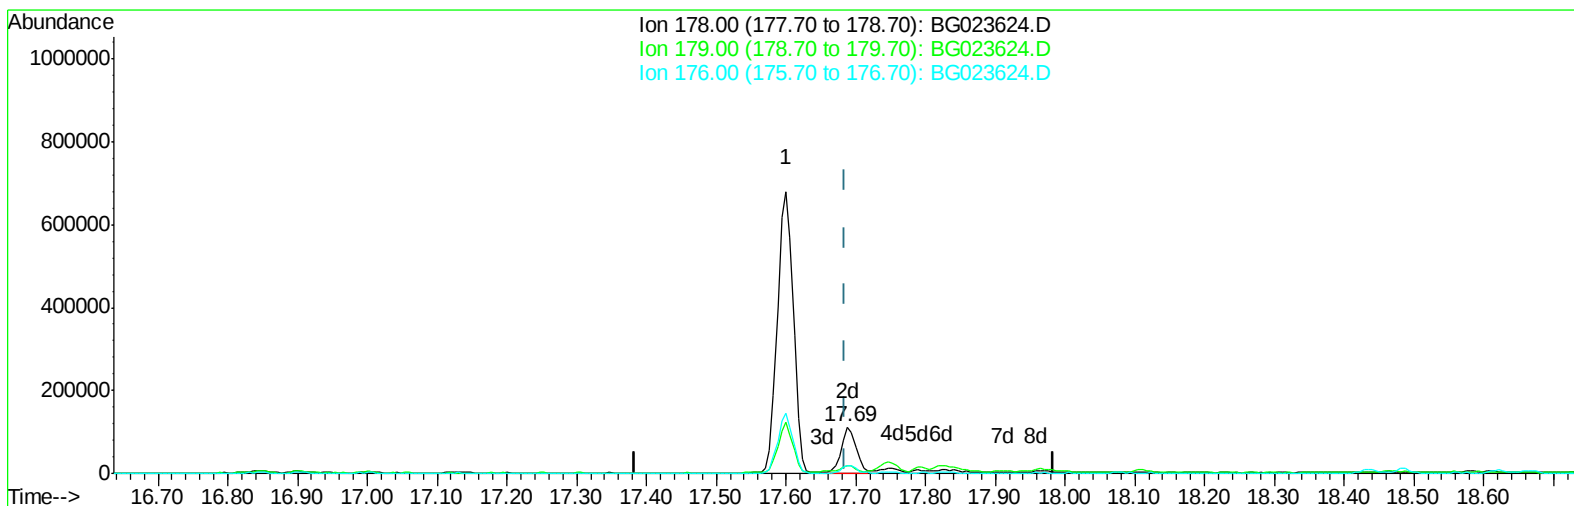

TIC: BG023624.D

(71) Anthracene

17.688min (+0.004) 2.18ng/ul m

response 167643

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	16.11
176.00	20.40	15.87#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:52:47 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

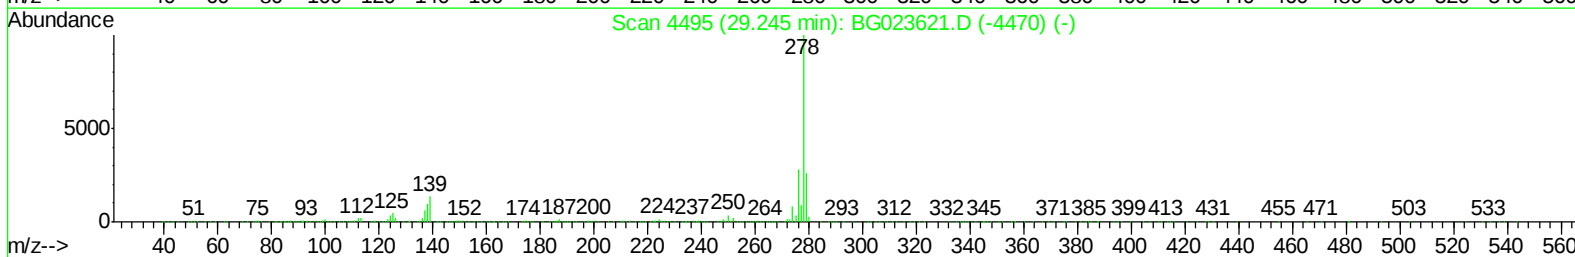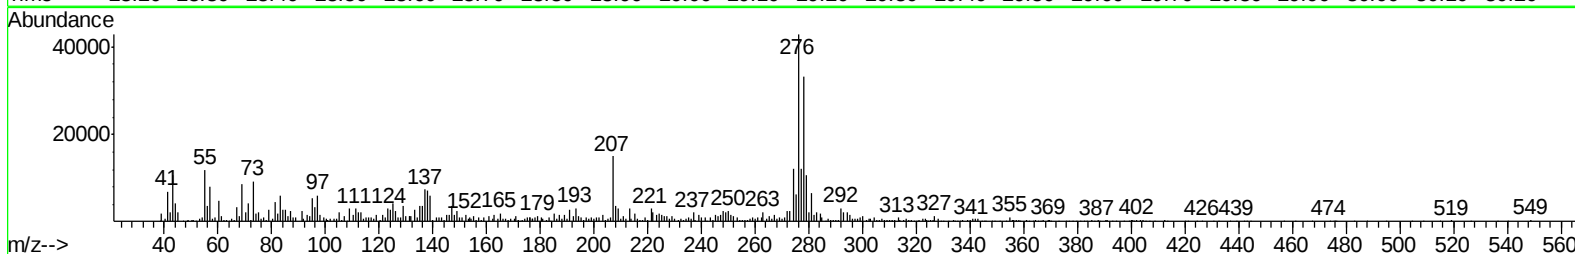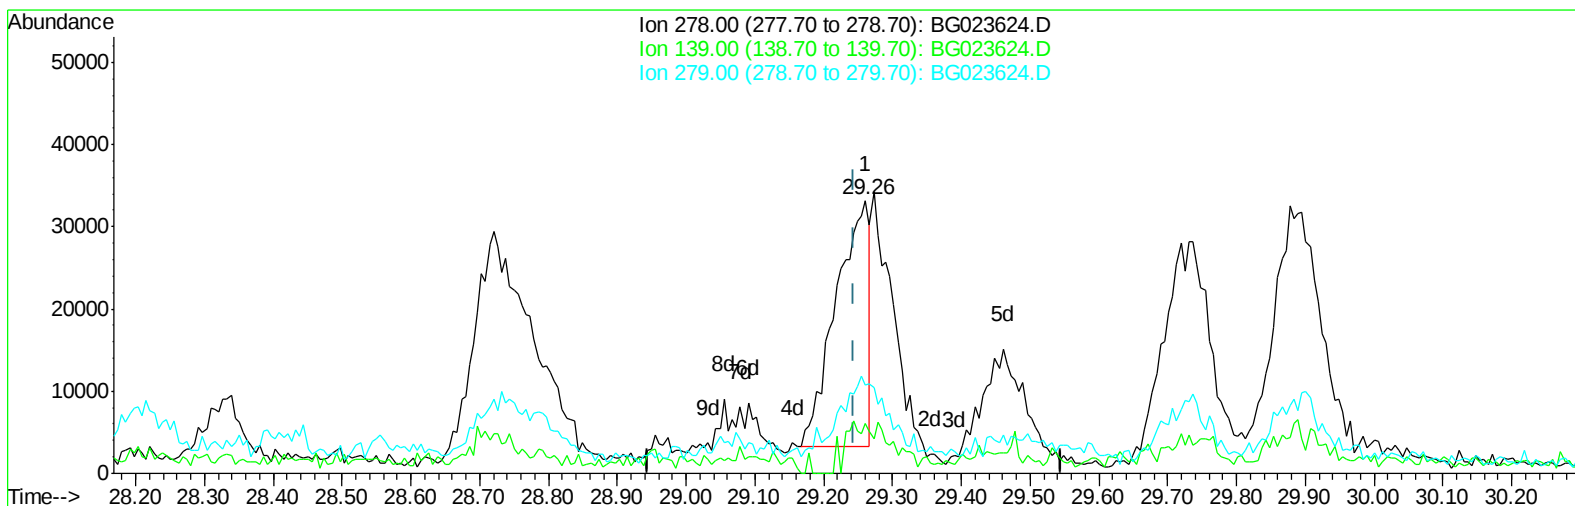

TIC: BG023624.D

(90) Dibenzo(a,h)anthracene

29.261min (+0.015) 1.52ng/ul

response 102023

Ion	Exp%	Act%
278.00	100	100
139.00	20.40	18.23
279.00	23.90	32.56#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:52:47 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 03:45:04 2016
Response via : Initial Calibration

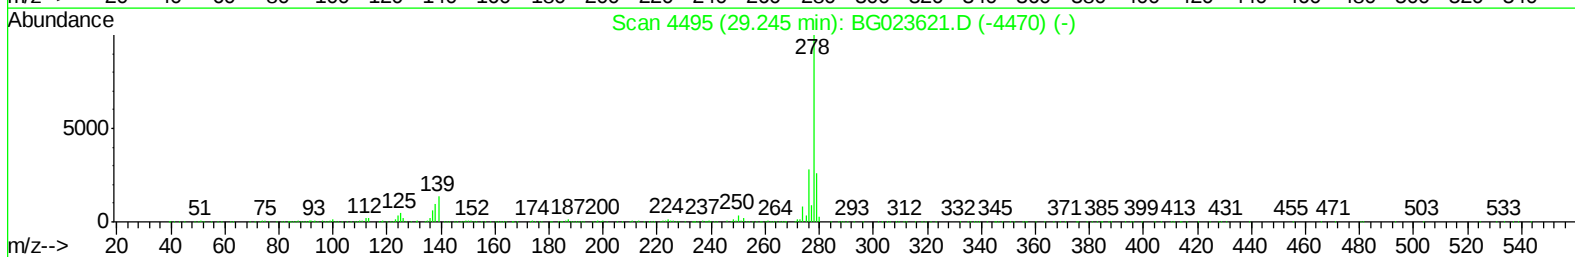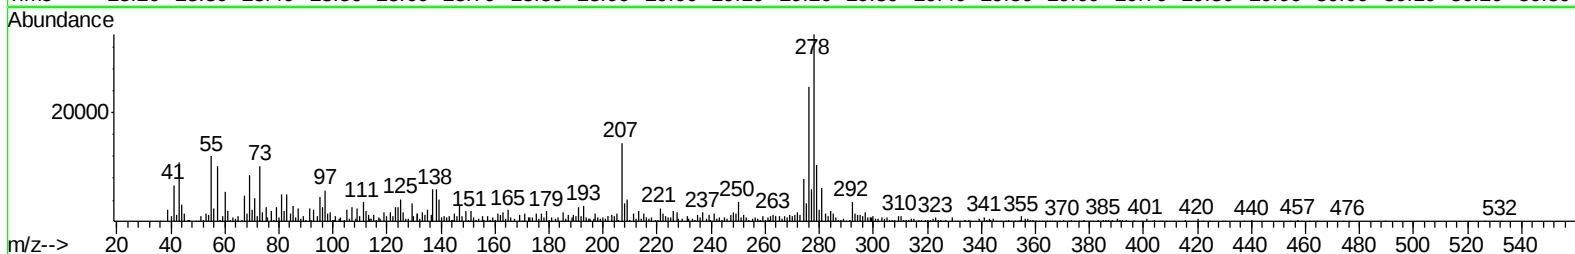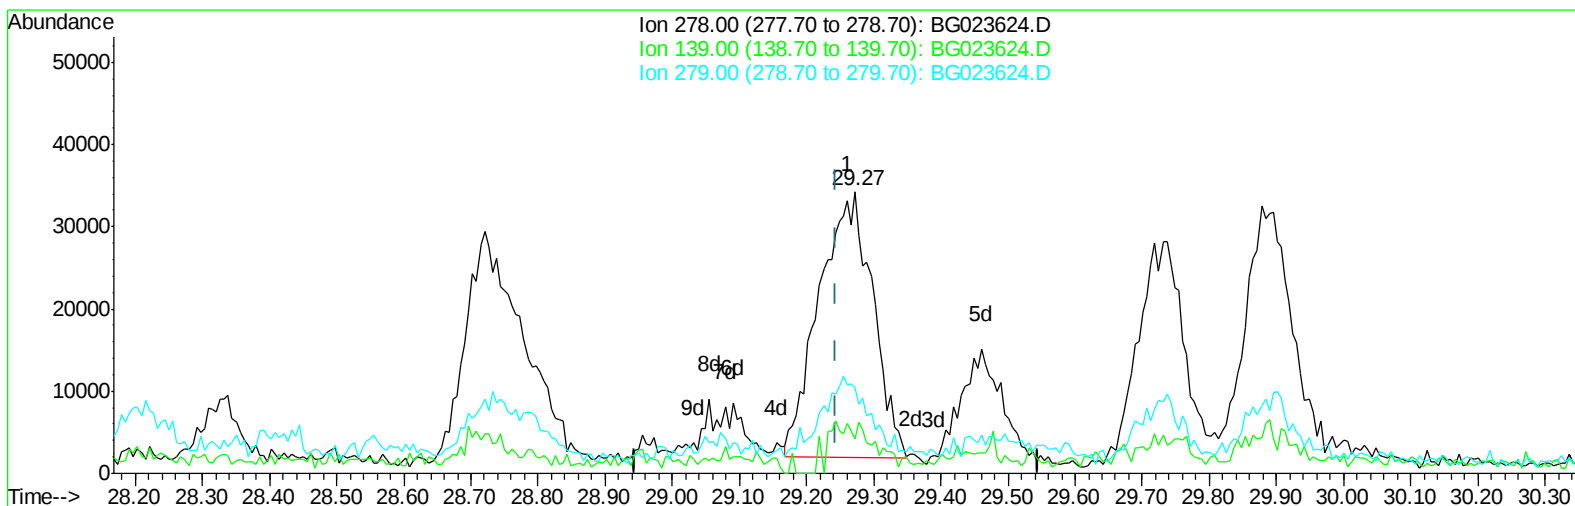

TIC: BG023624.D

(90) Dibenzo(a,h)anthracene

29.272min (+0.027) 2.66ng/ul m

response 178104

Ion	Exp%	Act%
278.00	100	100
139.00	20.40	12.12#
279.00	23.90	30.35#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081116\
 Data File : BG023624.D
 Acq On : 11 Aug 2016 13:22
 Operator : UM/SJ
 Sample : H4362-01 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS004-2430-01

Manual Integrations
 APPROVED

sohil
 8/12/2016 5:55:34 PM

Quant Time: Aug 12 03:53:44 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 12 03:45:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	215363	20.00	ng/ul	0.00
18) Naphthalene-d8	10.96	136	1006351	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	666743	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	1456947	20.00	ng/ul	0.00
75) Chrysene-d12	21.89	240	1228073	20.00	ng/ul	0.02
83) Perylene-d12	25.31	264	1218076	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	4194m	0.83	ng/uL	0.00
5) Phenol-d5	7.28	99	175276	8.08	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.44	67	143951	10.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	145955	9.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.84	113	95220	5.62	ng/ul	0.02
19) Nitrobenzene-d5	9.30	128	84553	10.66	ng/ul	0.00
22) 2-Nitrophenol-d4	10.03	143	113538	12.46	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	10.58	165	181487	10.56	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	92012m	4.56	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	613229	11.23	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	716369	11.66	ng/ul	0.00
51) 4-Nitrophenol-d4	15.02	143	50082	5.37	ng/ul	0.02
57) Fluorene-d10	15.78	176	560838	11.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.91	200	46487	4.97	ng/ul	0.00
70) Anthracene-d10	17.65	188	812463	12.38	ng/ul	0.00
76) Pyrene-d10	19.95	212	707917	11.39	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.07	264	640965	11.63	ng/ul	0.03

Target Compounds

						Qvalue
44) Dimethylphthalate	14.23	163	314256	5.81	ng/ul#	97
47) Acenaphthylene	14.52	152	111660	1.74	ng/ul	94
69) Phenanthrene	17.60	178	1066301	14.13	ng/ul	96
71) Anthracene	17.69	178	167643m	2.18	ng/ul	
73) Di-n-butylphthalate	18.50	149	129839	1.67	ng/ul#	96
74) Fluoranthene	19.61	202	1599469	20.71	ng/ul#	94
77) Pyrene	19.98	202	1912373	25.19	ng/ul	97
80) Benzo(a)anthracene	21.86	228	955264	13.81	ng/ul#	90
81) Bis(2-ethylhexyl)phthalate	21.79	149	12273802m	317.00	ng/ul	
82) Chrysene	21.94	228	1082303	17.21	ng/ul#	91
84) Di-n-octyl phthalate	23.02	149	3516058	57.15	ng/ul	100
85) Benzo(b)fluoranthene	24.21	252	1100526	15.88	ng/ul	96
86) Benzo(k)fluoranthene	24.27	252	456035m	6.69	ng/ul	
88) Benzo(a)pyrene	25.14	252	917671m	13.72	ng/ul	
89) Indeno(1,2,3-cd)pyrene	29.21	276	632950m	8.05	ng/ul	
90) Dibenzo(a,h)anthracene	29.27	278	178104m	2.66	ng/ul	
91) Benzo(g,h,i)perylene	30.45	276	702435m	10.78	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\HPCHEM1\BNA_G\Data\BG081116\
Data File : BG023624.D
Acq On : 11 Aug 2016 13:22
Operator : UM/SJ
Sample : H4362-01 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR001-SS004-2430-01

Manual Integrations
APPROVED

sohil
8/12/2016 5:55:34 PM

Quant Time: Aug 22 08:19:58 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

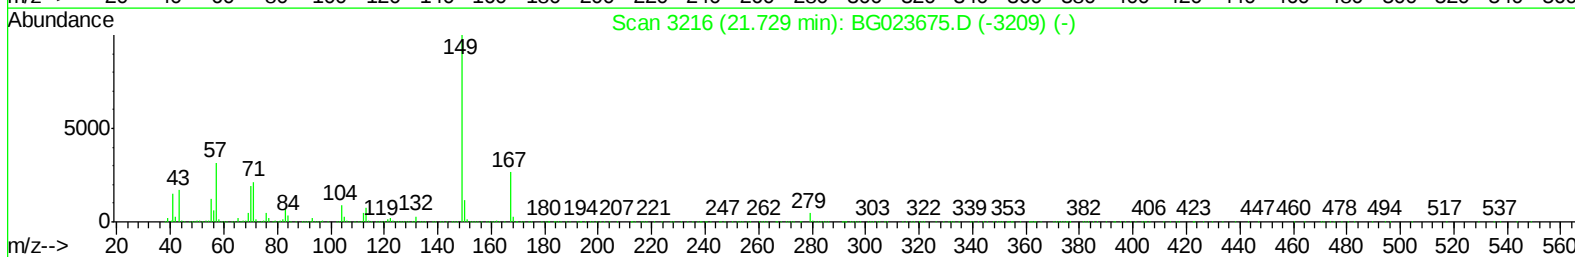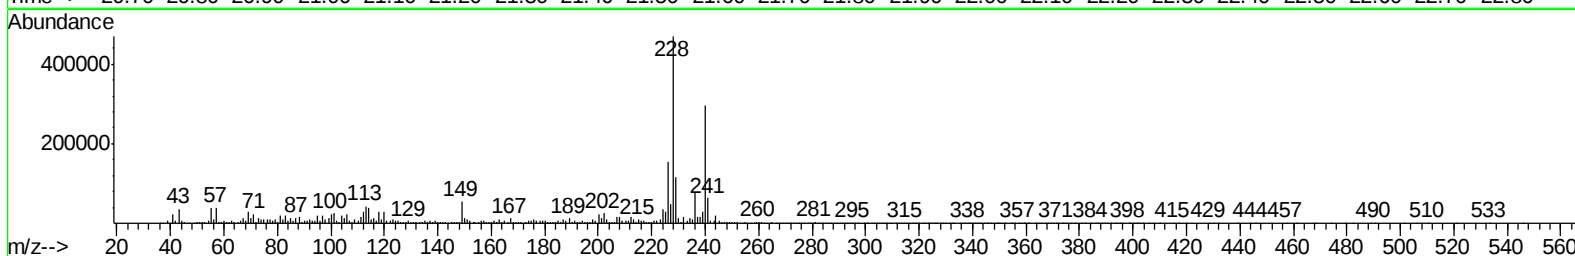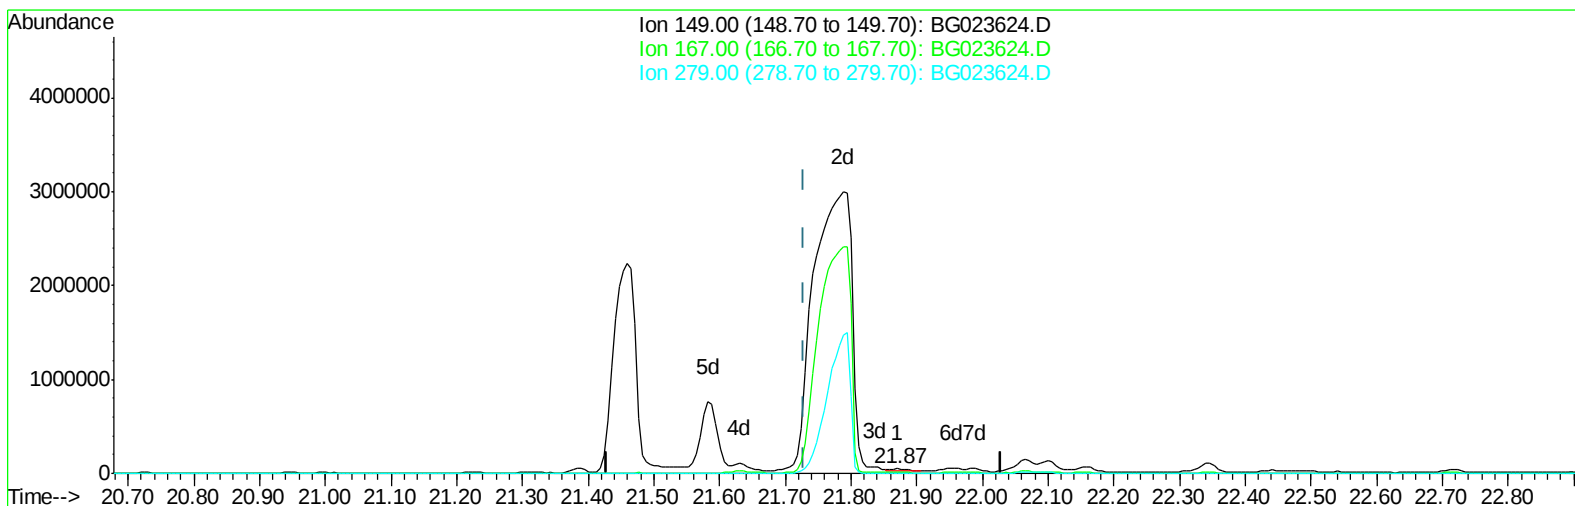

TIC: BG023624.D

(81) Bis(2-ethylhexyl)phthalate

21.871min (+0.142) 1.28ng/ul

response 49554

Ion	Exp%	Act%
149.00	100	100
167.00	27.40	23.21
279.00	3.60	3.41
0.00	0.00	0.00