

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
 Data File : BG049783.D
 Acq On : 11 Aug 2021 10:39
 Operator : CG/JU
 Sample : PB138258BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.410	60	63	70	rBV3	5958	9184	1.03%	0.098%
2	3.598	92	95	97	rVB3	1618	1287	0.14%	0.014%
3	3.692	109	111	112	rBV2	1412	1346	0.15%	0.014%
4	3.745	119	120	123	rBV2	1603	1989	0.22%	0.021%
5	3.839	132	136	151	rBV	78056	160236	17.98%	1.710%
6	4.233	199	203	204	rVB3	1623	1808	0.20%	0.019%
7	4.274	208	210	213	rBV2	1980	2049	0.23%	0.022%
8	4.667	275	277	279	rVB2	2225	1365	0.15%	0.015%
9	4.855	305	309	312	rVB4	1596	2539	0.28%	0.027%
10	4.891	312	315	317	rBV3	1840	1524	0.17%	0.016%
11	5.090	347	349	352	rVB2	1307	1393	0.16%	0.015%
12	5.237	372	374	377	rVB2	2144	1369	0.15%	0.015%
13	5.631	438	441	445	rBV2	1088	1976	0.22%	0.021%
14	5.678	448	449	452	rVB2	1331	1305	0.15%	0.014%
15	5.995	500	503	507	rBV3	2099	2867	0.32%	0.031%
16	6.612	606	608	611	rBV2	1399	1744	0.20%	0.019%
17	6.923	659	661	665	rBV2	1264	1492	0.17%	0.016%
18	7.199	702	708	720	rVB	152903	269849	30.28%	2.879%
19	7.358	729	735	746	rVB	95735	169927	19.07%	1.813%
20	7.522	760	763	764	rBV	1145	1353	0.15%	0.014%
21	7.569	764	771	780	rVV	147548	260351	29.22%	2.778%
22	7.734	795	799	802	rBV	991	1538	0.17%	0.016%
23	8.039	844	851	859	rVB2	93563	158954	17.84%	1.696%
24	8.421	914	916	919	rBV	1262	1322	0.15%	0.014%
25	8.750	965	972	983	rBV2	187292	340235	38.18%	3.631%
26	9.208	1042	1050	1062	rBV	158113	277192	31.11%	2.958%
27	9.349	1072	1074	1078	rVB2	1454	1661	0.19%	0.018%
28	9.937	1167	1174	1184	rVB2	142438	257762	28.93%	2.751%
29	10.483	1259	1267	1276	rBV	186231	346787	38.92%	3.700%
30	10.859	1324	1331	1341	rVB	128409	235358	26.41%	2.511%
31	10.994	1347	1354	1365	rBV	184885	338213	37.95%	3.609%
32	11.135	1376	1378	1381	rVB	1511	1358	0.15%	0.014%
33	11.294	1402	1405	1408	rBV	1501	1332	0.15%	0.014%
34	12.363	1581	1587	1589	rBV	1036	1582	0.18%	0.017%
35	12.445	1596	1601	1606	rBV3	2604	5121	0.57%	0.055%
36	12.862	1667	1672	1676	rVB2	910	1296	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
 Data File : BG049783.D
 Acq On : 11 Aug 2021 10:39
 Operator : CG/JU
 Sample : PB138258BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Title : SVOA CALIBRATION

37	12.950	1684	1687	1688	rBV2	1554	1388	0.16%	0.015%
38	13.103	1711	1713	1715	rBV	1297	1237	0.14%	0.013%
39	13.878	1841	1845	1847	rBV	916	1248	0.14%	0.013%
40	14.090	1874	1881	1889	rBV	364253	541111	60.72%	5.774%
41	14.384	1925	1931	1940	rVB	379690	601580	67.51%	6.419%
42	14.583	1962	1965	1968	rBV2	1084	1245	0.14%	0.013%
43	14.689	1977	1983	1991	rBV	207330	324362	36.40%	3.461%
44	14.895	2012	2018	2027	rBV	139836	254747	28.59%	2.718%
45	15.118	2054	2056	2059	rBV	1181	1682	0.19%	0.018%
46	15.682	2145	2152	2160	rBV	479766	739836	83.02%	7.895%
47	15.805	2167	2173	2184	rBV2	161420	253566	28.45%	2.706%
48	15.929	2189	2194	2199	rVB4	5030	8474	0.95%	0.090%
49	16.258	2248	2250	2254	rVB2	1111	1266	0.14%	0.014%
50	16.451	2281	2283	2286	rBV2	1142	1281	0.14%	0.014%
51	16.657	2312	2318	2319	rBV	1205	2007	0.23%	0.021%
52	16.675	2319	2321	2328	rVB	1538	1979	0.22%	0.021%
53	17.186	2405	2408	2410	rBV	1203	1269	0.14%	0.014%
54	17.233	2412	2416	2420	rVB	2158	2373	0.27%	0.025%
55	17.444	2446	2452	2459	rBV	249583	376465	42.25%	4.017%
56	17.544	2461	2469	2478	rBV2	521368	813570	91.30%	8.681%
57	17.761	2503	2506	2510	rVB	1593	1756	0.20%	0.019%
58	17.820	2512	2516	2518	rBV	1671	2313	0.26%	0.025%
59	17.879	2523	2526	2528	rBV	1492	1419	0.16%	0.015%
60	18.161	2571	2574	2576	rVB	1460	1652	0.19%	0.018%
61	18.596	2645	2648	2652	rVB	1119	1624	0.18%	0.017%
62	18.631	2652	2654	2657	rBV	1290	1260	0.14%	0.013%
63	18.930	2702	2705	2706	rBV2	2008	1591	0.18%	0.017%
64	18.942	2706	2707	2712	rVV2	1238	1659	0.19%	0.018%
65	19.001	2715	2717	2719	rBV	1762	1784	0.20%	0.019%
66	19.183	2744	2748	2750	rBV3	1666	2482	0.28%	0.026%
67	19.218	2750	2754	2757	rVB2	2120	2450	0.27%	0.026%
68	19.253	2757	2760	2762	rBV3	1609	1911	0.21%	0.020%
69	19.330	2771	2773	2776	rBV2	2606	2627	0.29%	0.028%
70	19.394	2780	2784	2787	rBV4	6770	10972	1.23%	0.117%
71	19.465	2792	2796	2801	rBV2	6633	10973	1.23%	0.117%
72	19.588	2816	2817	2818	rBV	2340	1449	0.16%	0.015%
73	19.682	2828	2833	2834	rBV5	2828	4189	0.47%	0.045%
74	19.700	2834	2836	2838	rVV3	2961	1962	0.22%	0.021%
75	19.741	2841	2843	2847	rBV3	2917	4266	0.48%	0.046%
76	19.788	2849	2851	2852	rBV2	1929	1356	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
 Data File : BG049783.D
 Acq On : 11 Aug 2021 10:39
 Operator : CG/JU
 Sample : PB138258BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK258

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Title : SVOA CALIBRATION

77	19.829	2852	2858	2864	rBV	643544	891127	100.00%	9.509%
78	19.923	2873	2874	2877	rBV3	2062	2035	0.23%	0.022%
79	20.082	2899	2901	2904	rBV3	3510	3856	0.43%	0.041%
80	20.146	2910	2912	2913	rBV2	2988	2322	0.26%	0.025%
81	20.176	2913	2917	2918	rBV3	5333	6740	0.76%	0.072%
82	20.834	3027	3029	3030	rVB2	5108	2843	0.32%	0.030%
83	21.721	3174	3180	3187	rBV	228850	380457	42.69%	4.060%
84	24.775	3690	3700	3712	rVB2	286729	821648	92.20%	8.768%
85	25.005	3730	3739	3749	rVB2	139698	400542	44.95%	4.274%
86	31.977	4924	4926	4927	rBV2	5579	2791	0.31%	0.030%




Sum of corrected areas: 9371406

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
Data File : BG049783.D
Acq On : 11 Aug 2021 10:39
Operator : CG/JU
Sample : PB138258BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK258

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

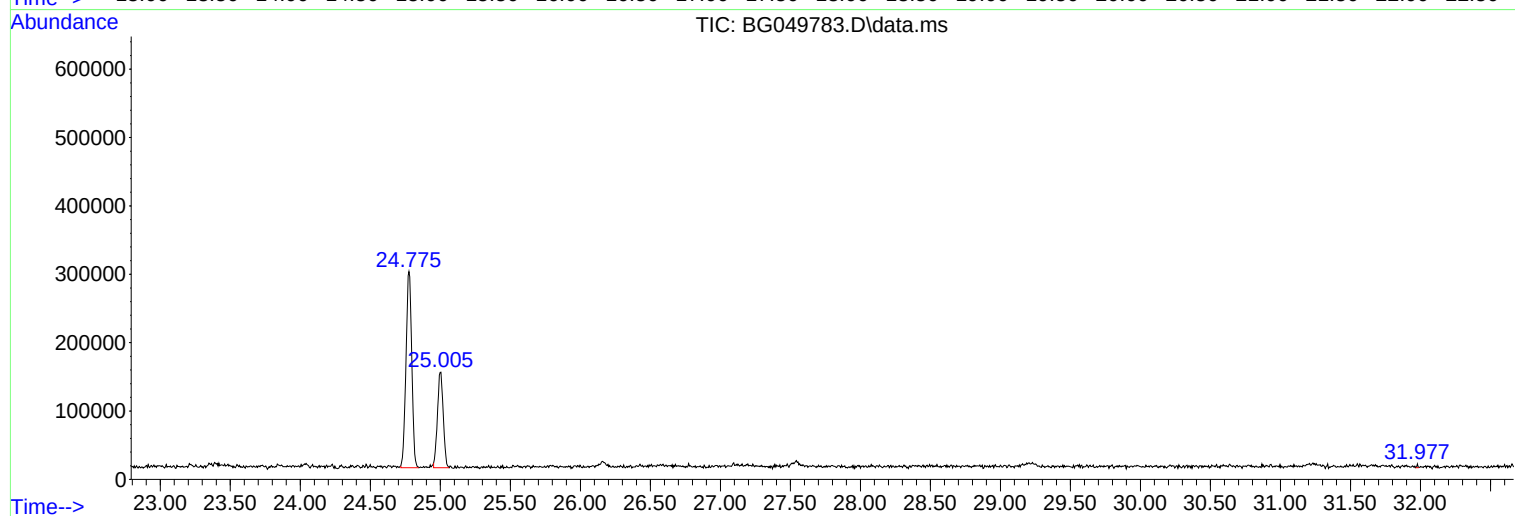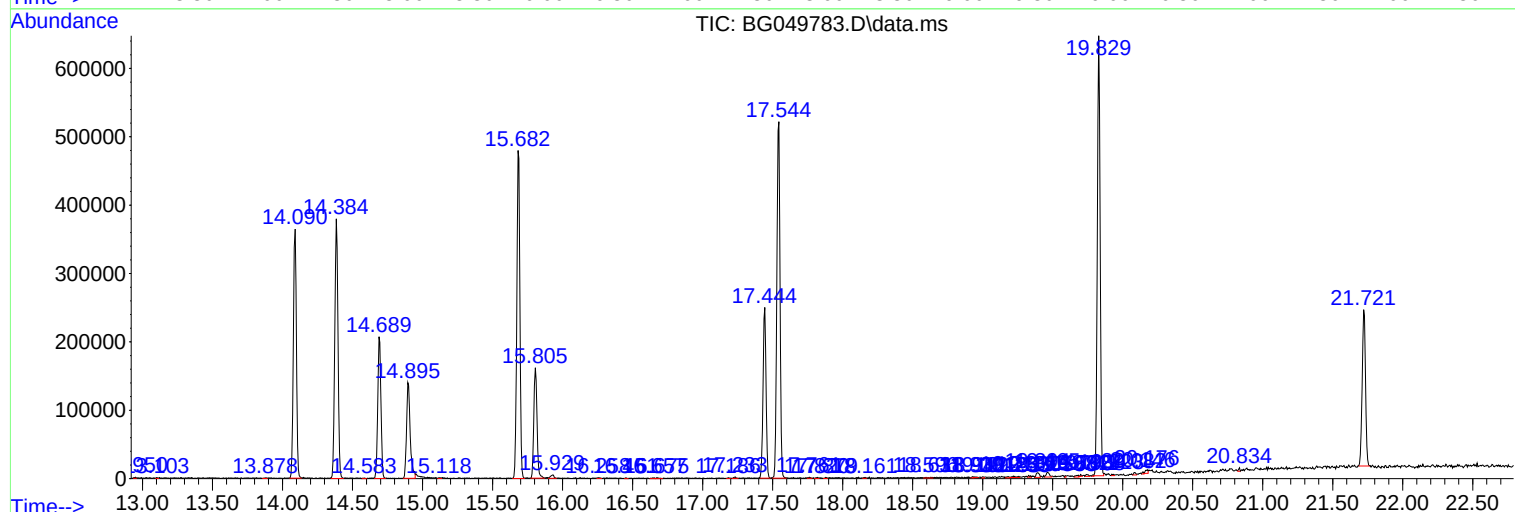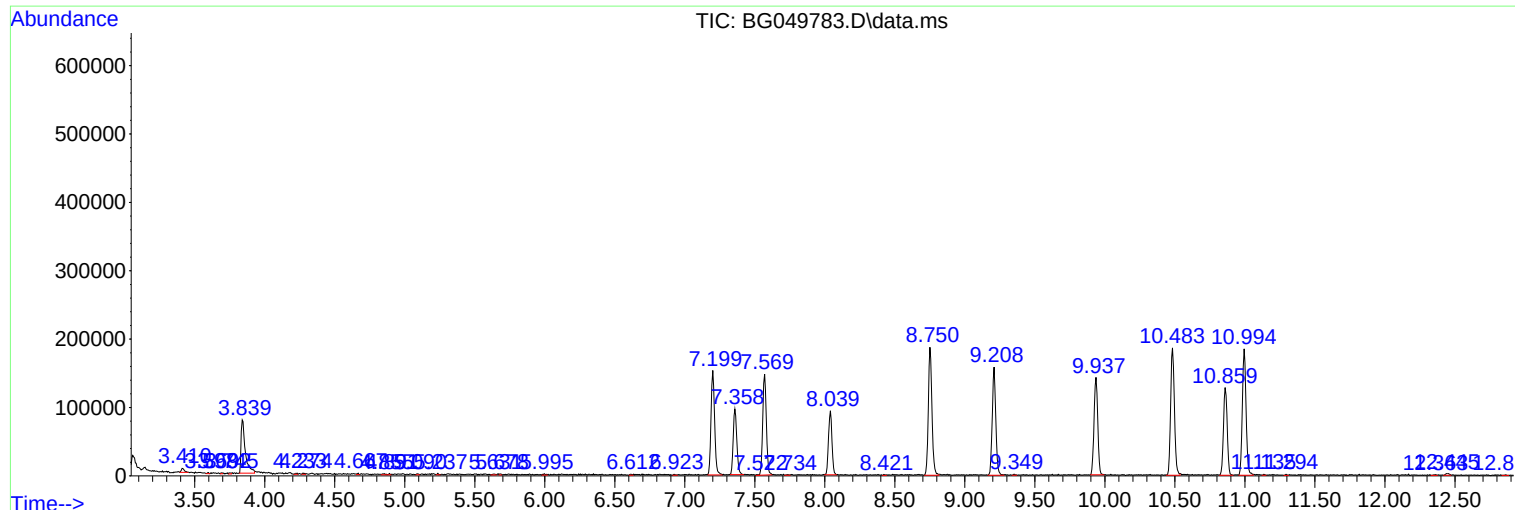

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
Data File : BG049783.D
Acq On : 11 Aug 2021 10:39
Operator : CG/JU
Sample : PB138258BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK258

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
Data File : BG049783.D
Acq On : 11 Aug 2021 10:39
Operator : CG/JU
Sample : PB138258BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK258

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------