

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
 Data File : BG049784.D
 Acq On : 11 Aug 2021 11:21
 Operator : CG/JU
 Sample : PB138246BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049784.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.408	61	63	75	rVB4	6840	14472	1.69%	0.155%
2	3.837	133	136	145	rBV	82217	154805	18.07%	1.661%
3	4.536	254	255	258	rBV2	1878	1447	0.17%	0.016%
4	4.724	284	287	290	rBV3	1671	1865	0.22%	0.020%
5	5.118	353	354	356	rVB	1813	1197	0.14%	0.013%
6	5.147	356	359	361	rBV2	1958	2414	0.28%	0.026%
7	5.270	378	380	384	rVB2	1317	1390	0.16%	0.015%
8	5.370	395	397	402	rVB5	1433	1826	0.21%	0.020%
9	5.417	402	405	407	rBV2	1493	1732	0.20%	0.019%
10	5.611	436	438	443	rVB4	1396	1492	0.17%	0.016%
11	5.752	459	462	466	rVB3	1517	1881	0.22%	0.020%
12	5.870	480	482	484	rBV2	1264	1165	0.14%	0.013%
13	5.987	498	502	504	rBV2	817	1156	0.13%	0.012%
14	6.152	527	530	533	rBV3	1026	1238	0.14%	0.013%
15	6.240	544	545	548	rVB	1412	1161	0.14%	0.012%
16	6.298	551	555	557	rBV2	1302	1738	0.20%	0.019%
17	6.557	598	599	605	rBV	1147	1730	0.20%	0.019%
18	7.197	701	708	721	rVB	145086	261398	30.52%	2.805%
19	7.356	728	735	742	rBV	95647	163523	19.09%	1.755%
20	7.567	763	771	778	rBV	145671	255302	29.81%	2.740%
21	8.031	844	850	858	rBV	96973	167520	19.56%	1.798%
22	8.202	876	879	881	rVB	1473	1319	0.15%	0.014%
23	8.231	881	884	887	rBV	1231	1355	0.16%	0.015%
24	8.360	904	906	909	rVB2	1547	1232	0.14%	0.013%
25	8.454	919	922	925	rVB2	1214	1243	0.15%	0.013%
26	8.748	965	972	982	rBV	185045	329775	38.50%	3.539%
27	9.206	1042	1050	1062	rVB	149899	275161	32.12%	2.953%
28	9.488	1096	1098	1101	rBV	1407	1320	0.15%	0.014%
29	9.694	1129	1133	1135	rBV	1025	1572	0.18%	0.017%
30	9.735	1138	1140	1144	rBV2	1861	2072	0.24%	0.022%
31	9.935	1166	1174	1182	rBV	139454	257661	30.08%	2.765%
32	10.481	1258	1267	1280	rBV	183044	348942	40.74%	3.745%
33	10.857	1324	1331	1341	rBV	131018	244155	28.50%	2.620%
34	10.992	1347	1354	1369	rBV	184741	333223	38.90%	3.576%
35	11.662	1465	1468	1470	rBV2	1443	1547	0.18%	0.017%
36	11.732	1477	1480	1483	rBV2	699	1214	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
 Data File : BG049784.D
 Acq On : 11 Aug 2021 11:21
 Operator : CG/JU
 Sample : PB138246BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 SBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Title : SVOA CALIBRATION

37	11.861	1500	1502	1507	rVB	1262	1687	0.20%	0.018%
38	12.249	1566	1568	1571	rVB	1855	1271	0.15%	0.014%
39	12.373	1585	1589	1591	rBV2	1058	1237	0.14%	0.013%
40	12.449	1598	1602	1606	rBV4	2414	4145	0.48%	0.044%
41	13.665	1805	1809	1810	rBV	925	1217	0.14%	0.013%
42	14.088	1874	1881	1889	rVB	357345	528758	61.73%	5.675%
43	14.382	1923	1931	1938	rBV	365773	594252	69.38%	6.377%
44	14.687	1977	1983	1992	rVB	224626	345785	40.37%	3.711%
45	14.893	2011	2018	2031	rBV	131513	252687	29.50%	2.712%
46	15.680	2143	2152	2161	rBV	483346	725329	84.68%	7.784%
47	15.803	2167	2173	2182	rBV2	160183	250008	29.19%	2.683%
48	15.921	2187	2193	2199	rVB5	4305	6901	0.81%	0.074%
49	16.079	2217	2220	2223	rBV5	1540	1370	0.16%	0.015%
50	16.250	2246	2249	2254	rBV	1311	1320	0.15%	0.014%
51	17.231	2411	2416	2417	rBV	1275	1694	0.20%	0.018%
52	17.442	2446	2452	2459	rBV	262050	404133	47.18%	4.337%
53	17.542	2462	2469	2478	rVB	499063	782928	91.40%	8.402%
54	17.853	2519	2522	2525	rVB	1221	1435	0.17%	0.015%
55	18.112	2563	2566	2567	rVB	1313	1352	0.16%	0.015%
56	18.482	2626	2629	2632	rVB	1056	1426	0.17%	0.015%
57	18.541	2636	2639	2641	rBV2	1285	1216	0.14%	0.013%
58	18.787	2678	2681	2683	rBV	1188	1443	0.17%	0.015%
59	19.140	2739	2741	2743	rBV2	1610	1442	0.17%	0.015%
60	19.392	2778	2784	2790	rBV5	6145	11520	1.34%	0.124%
61	19.463	2793	2796	2800	rVB2	6464	8953	1.05%	0.096%
62	19.504	2800	2803	2804	rBV2	1324	1231	0.14%	0.013%
63	19.598	2817	2819	2820	rBV2	1522	1226	0.14%	0.013%
64	19.739	2841	2843	2845	rBV2	2607	2615	0.31%	0.028%
65	19.780	2848	2850	2851	rBV2	2252	1840	0.21%	0.020%
66	19.827	2851	2858	2864	rBV	599715	856561	100.00%	9.192%
67	19.886	2867	2868	2871	rVV3	2667	2490	0.29%	0.027%
68	20.062	2896	2898	2901	rBV3	2042	2133	0.25%	0.023%
69	20.403	2954	2956	2958	rBV3	2352	1630	0.19%	0.017%
70	21.719	3174	3180	3190	rVB	256645	413756	48.30%	4.440%
71	24.773	3690	3700	3713	rVB2	295801	819496	95.67%	8.795%
72	24.997	3728	3738	3750	rBV3	151923	439408	51.30%	4.716%


Sum of corrected areas: 9318138

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
Data File : BG049784.D
Acq On : 11 Aug 2021 11:21
Operator : CG/JU
Sample : PB138246BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK246

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

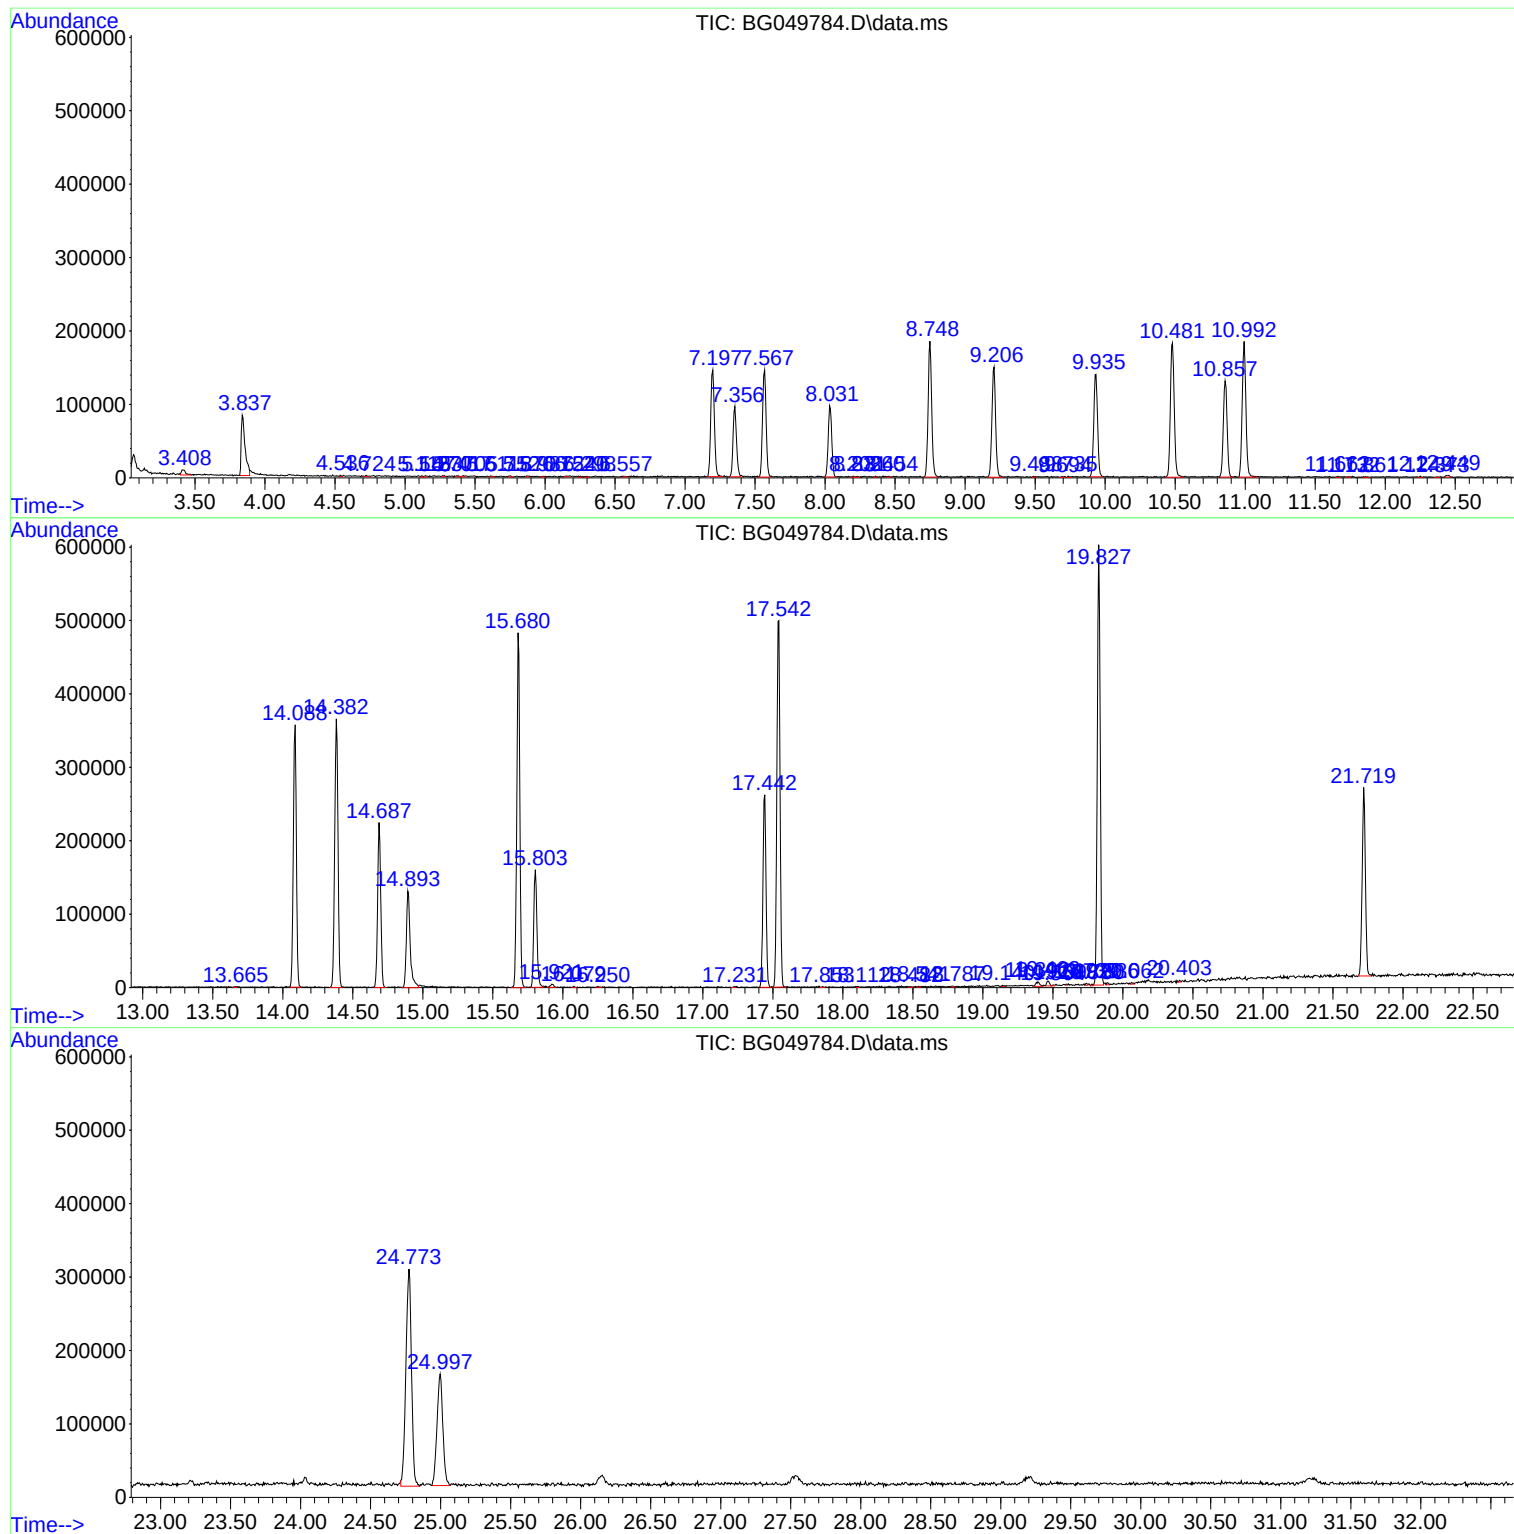

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
Data File : BG049784.D
Acq On : 11 Aug 2021 11:21
Operator : CG/JU
Sample : PB138246BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK246

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
Data File : BG049784.D
Acq On : 11 Aug 2021 11:21
Operator : CG/JU
Sample : PB138246BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK246

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
