

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
 Data File : BG049796.D
 Acq On : 11 Aug 2021 20:21
 Operator : CG/JU
 Sample : PB138270BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.148	17	19	24	rVB4	8187	9323	0.84%	0.082%
2	3.424	61	66	71	rVB3	7480	12827	1.16%	0.113%
3	3.812	129	132	133	rBV	1197	1561	0.14%	0.014%
4	3.841	133	137	157	rVV	98914	214198	19.34%	1.894%
5	3.977	158	160	163	rVB4	2032	1700	0.15%	0.015%
6	4.488	242	247	248	rBV4	1715	2291	0.21%	0.020%
7	4.505	248	250	254	rVV4	1505	1601	0.14%	0.014%
8	4.552	257	258	262	rBV3	1294	1907	0.17%	0.017%
9	4.881	311	314	317	rVB	1957	1962	0.18%	0.017%
10	5.433	405	408	410	rBV2	1155	1486	0.13%	0.013%
11	5.980	498	501	505	rVB3	1017	1517	0.14%	0.013%
12	6.873	652	653	658	rVB2	1430	1542	0.14%	0.014%
13	7.102	690	692	695	rVB	1359	1539	0.14%	0.014%
14	7.196	702	708	719	rBV2	183123	314647	28.41%	2.783%
15	7.354	727	735	745	rBV	115928	200987	18.15%	1.778%
16	7.566	762	771	783	rBV	175671	305489	27.58%	2.702%
17	7.648	783	785	791	rVB2	1171	2187	0.20%	0.019%
18	8.036	845	851	858	rBV	105845	188496	17.02%	1.667%
19	8.136	865	868	874	rVB2	1339	2060	0.19%	0.018%
20	8.747	964	972	981	rBV2	213059	387898	35.02%	3.431%
21	9.205	1043	1050	1058	rBV	179998	319941	28.88%	2.830%
22	9.434	1086	1089	1094	rBV	1080	1727	0.16%	0.015%
23	9.933	1166	1174	1182	rBV	165691	302342	27.30%	2.674%
24	10.480	1257	1267	1278	rBV	217859	397265	35.87%	3.514%
25	10.856	1323	1331	1340	rBV	146957	264686	23.90%	2.341%
26	10.991	1345	1354	1369	rBV	214892	397195	35.86%	3.513%
27	12.442	1597	1601	1607	rVB4	2707	4327	0.39%	0.038%
28	14.086	1874	1881	1892	rVB	453960	656283	59.25%	5.805%
29	14.380	1924	1931	1941	rBV	441538	701723	63.35%	6.206%
30	14.686	1976	1983	1990	rBV	252371	381203	34.42%	3.372%
31	14.891	2012	2018	2030	rBV	178335	326646	29.49%	2.889%
32	15.678	2144	2152	2161	rBV	593221	881384	79.57%	7.795%
33	15.802	2167	2173	2182	rBV	226985	330763	29.86%	2.925%
34	15.919	2189	2193	2198	rVB2	8142	9376	0.85%	0.083%
35	16.460	2282	2285	2288	rBV	1099	1462	0.13%	0.013%
36	17.217	2409	2414	2415	rBV	1182	1967	0.18%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
 Data File : BG049796.D
 Acq On : 11 Aug 2021 20:21
 Operator : CG/JU
 Sample : PB138270BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK270

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Title : SVOA CALIBRATION

37	17.306	2423	2429	2432	rBV	1322	2261	0.20%	0.020%
38	17.441	2445	2452	2461	rVV	304505	463949	41.89%	4.103%
39	17.541	2461	2469	2478	rVV	644933	987468	89.15%	8.734%
40	17.611	2478	2481	2484	rVB	1986	2202	0.20%	0.019%
41	18.052	2554	2556	2559	rBV2	1412	1591	0.14%	0.014%
42	18.851	2689	2692	2693	rVB2	2006	1745	0.16%	0.015%
43	18.874	2693	2696	2697	rBV	1521	1594	0.14%	0.014%
44	19.033	2720	2723	2725	rBV	1640	1503	0.14%	0.013%
45	19.391	2778	2784	2788	rBV2	9130	12004	1.08%	0.106%
46	19.420	2788	2789	2792	rVV2	1804	1798	0.16%	0.016%
47	19.467	2792	2797	2801	rVB2	8401	13145	1.19%	0.116%
48	19.620	2821	2823	2827	rBV3	1645	1746	0.16%	0.015%
49	19.720	2837	2840	2843	rBV2	2169	3474	0.31%	0.031%
50	19.773	2848	2849	2852	rVB3	2427	1589	0.14%	0.014%
51	19.826	2852	2858	2864	rBV	765959	1107655	100.00%	9.797%
52	19.920	2871	2874	2875	rBV3	1813	1693	0.15%	0.015%
53	20.002	2883	2888	2889	rBV3	1345	2124	0.19%	0.019%
54	20.043	2893	2895	2897	rBV3	2117	1588	0.14%	0.014%
55	20.102	2901	2905	2907	rBV3	3625	6605	0.60%	0.058%
56	20.284	2934	2936	2939	rVB4	3258	3548	0.32%	0.031%
57	20.319	2939	2942	2943	rBV2	2322	1937	0.17%	0.017%
58	20.631	2993	2995	2996	rBV2	2887	1501	0.14%	0.013%
59	20.695	3005	3006	3008	rBV2	3823	2809	0.25%	0.025%
60	21.717	3174	3180	3186	rBV	292132	479519	43.29%	4.241%
61	24.026	3569	3573	3582	rVB5	15417	32230	2.91%	0.285%
62	24.772	3688	3700	3710	rVB3	360837	1032290	93.20%	9.130%
63	24.989	3728	3737	3748	rVB3	176180	503251	45.43%	4.451%




Sum of corrected areas: 11306327

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
Data File : BG049796.D
Acq On : 11 Aug 2021 20:21
Operator : CG/JU
Sample : PB138270BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK270

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

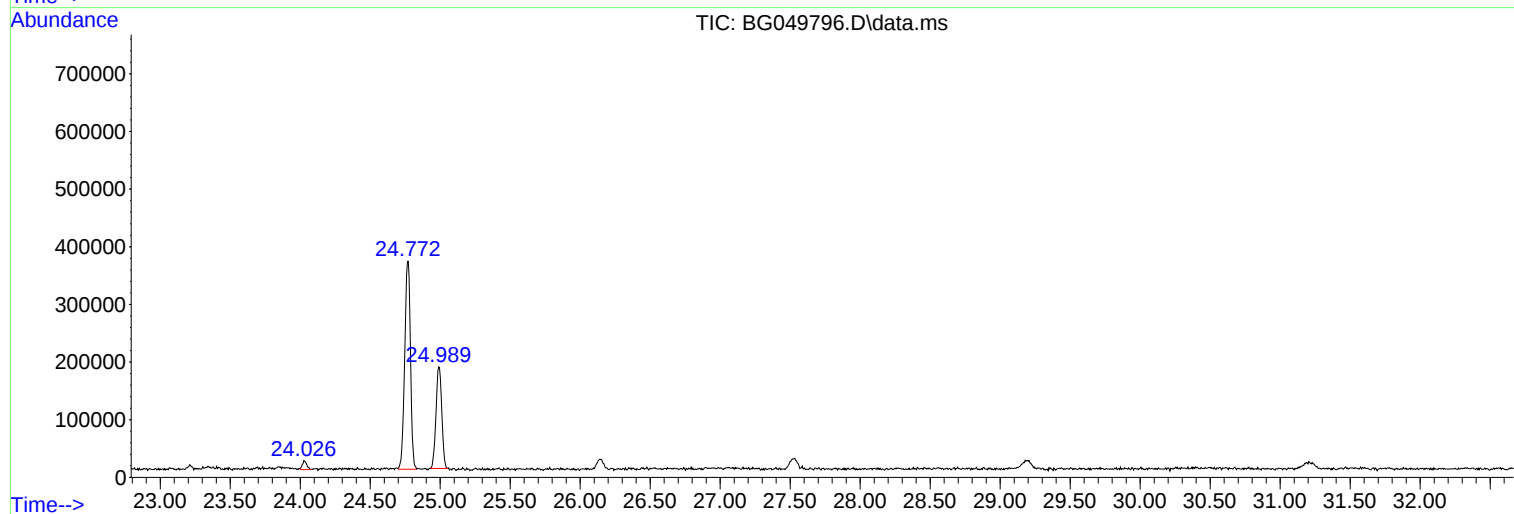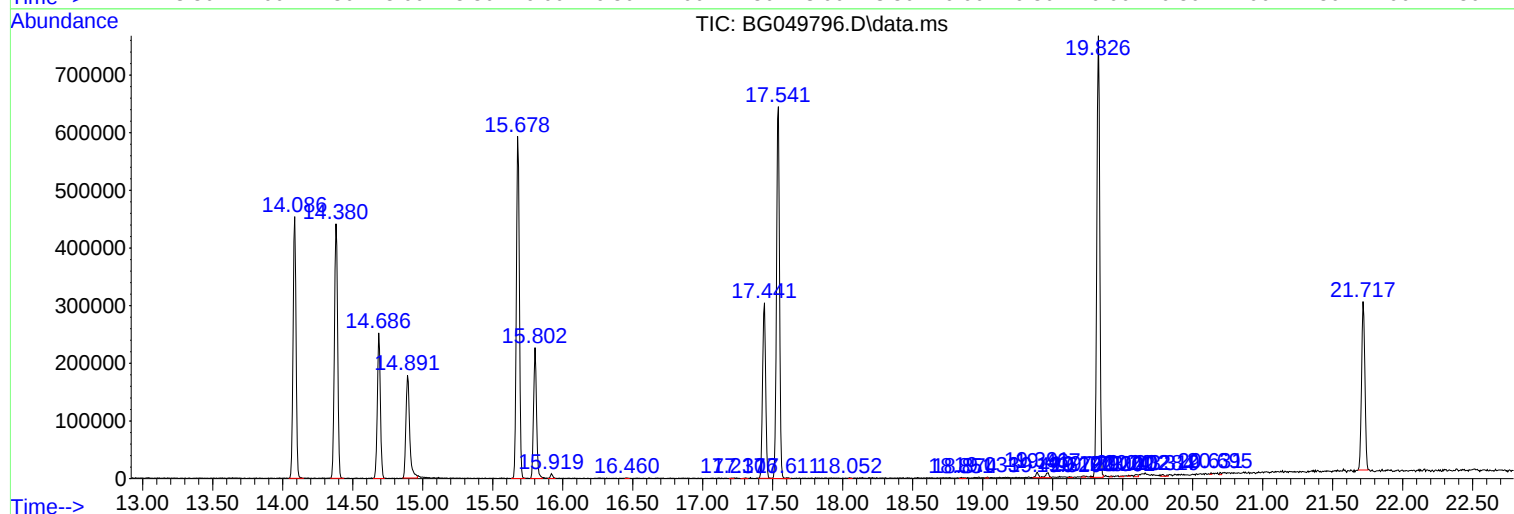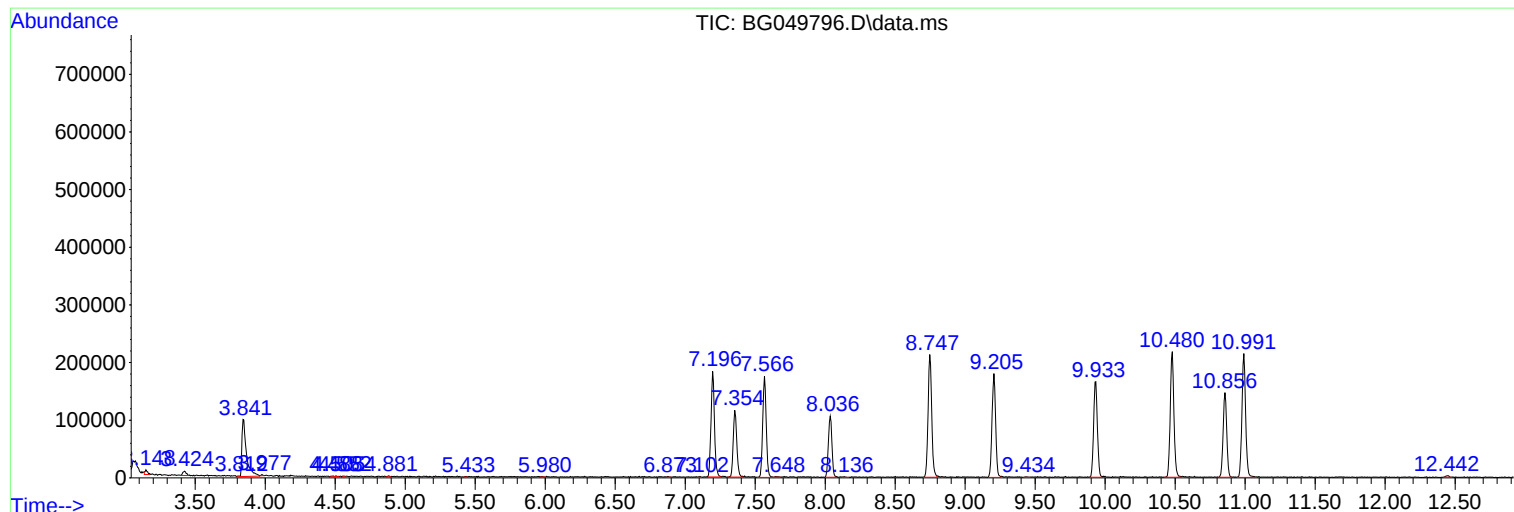

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
Data File : BG049796.D
Acq On : 11 Aug 2021 20:21
Operator : CG/JU
Sample : PB138270BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK270

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081121\
Data File : BG049796.D
Acq On : 11 Aug 2021 20:21
Operator : CG/JU
Sample : PB138270BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK270

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
