
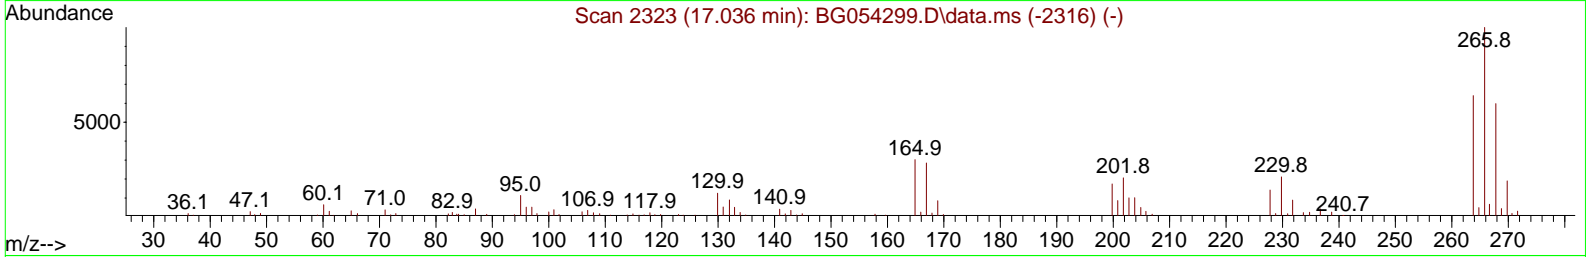
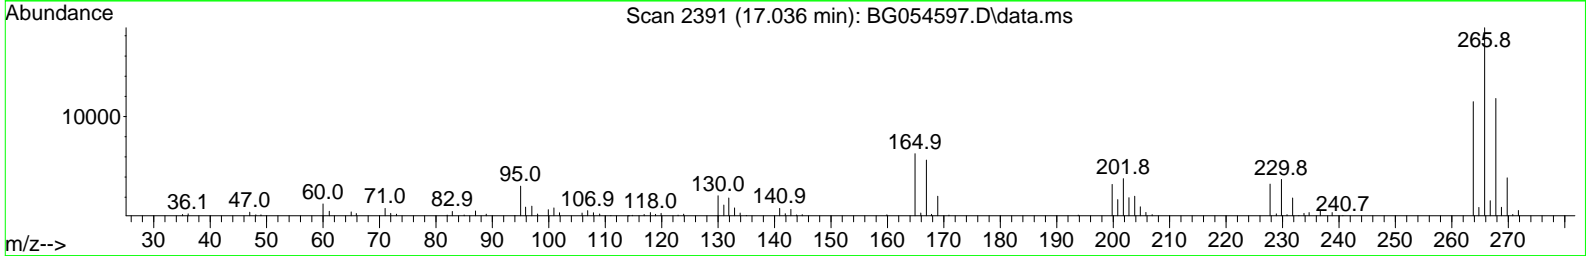


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081122\
 Data File : BG054597.D
 Acq On : 11 Aug 2022 9:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 08:19:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 14:48:51 2022
 Response via : Initial Calibration

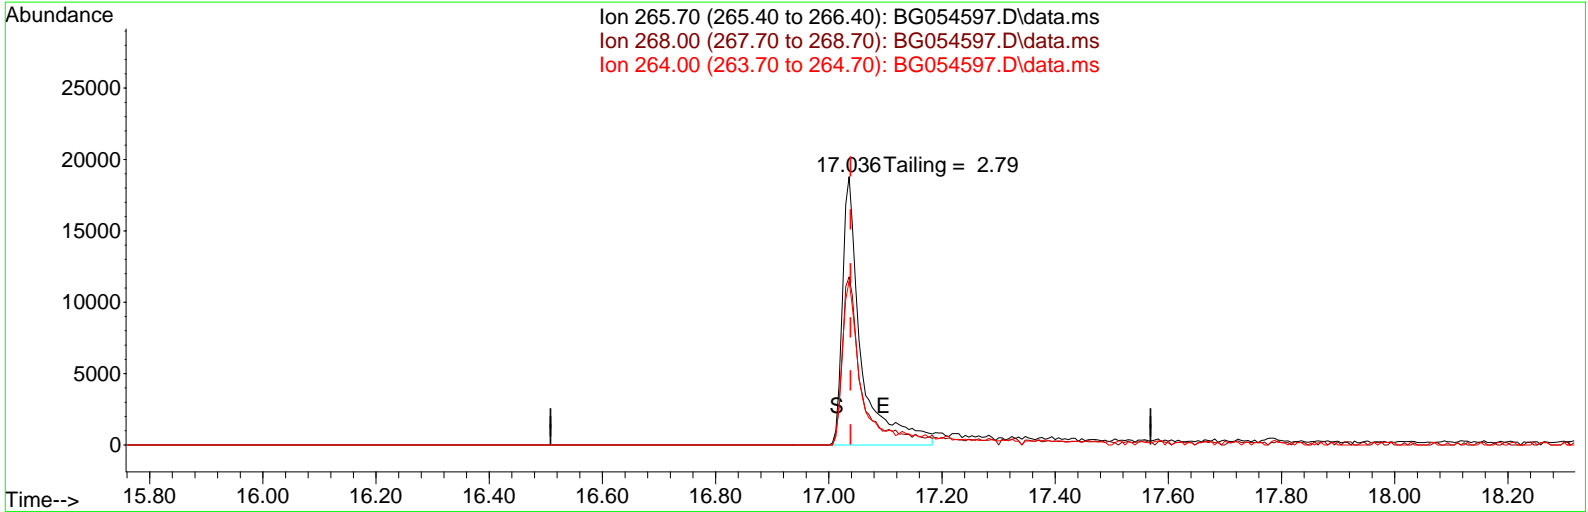

TIC: BG054597.D\data.ms

(70) Pentachlorophenol (C)




17.036min (-0.003) 14007.23 ng

response 38909

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	62.68
264.00	66.20	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081122\
 Data File : BG054597.D
 Acq On : 11 Aug 2022 9:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 08:19:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 14:48:51 2022
 Response via : Initial Calibration

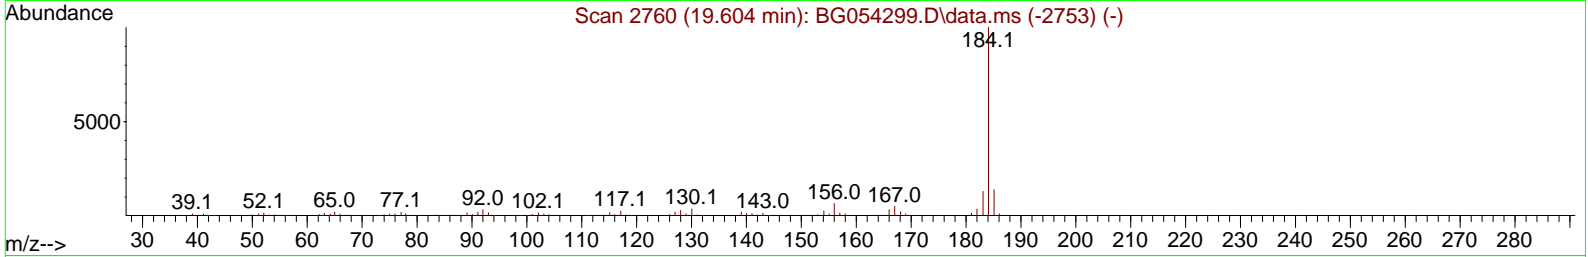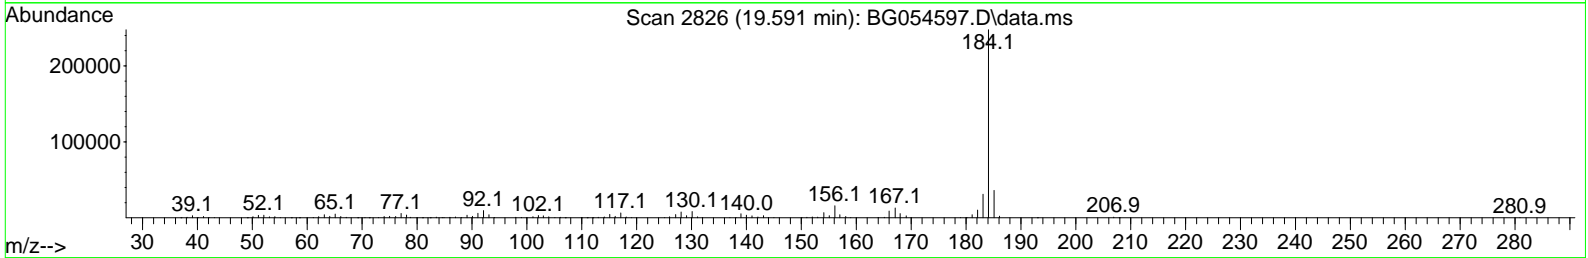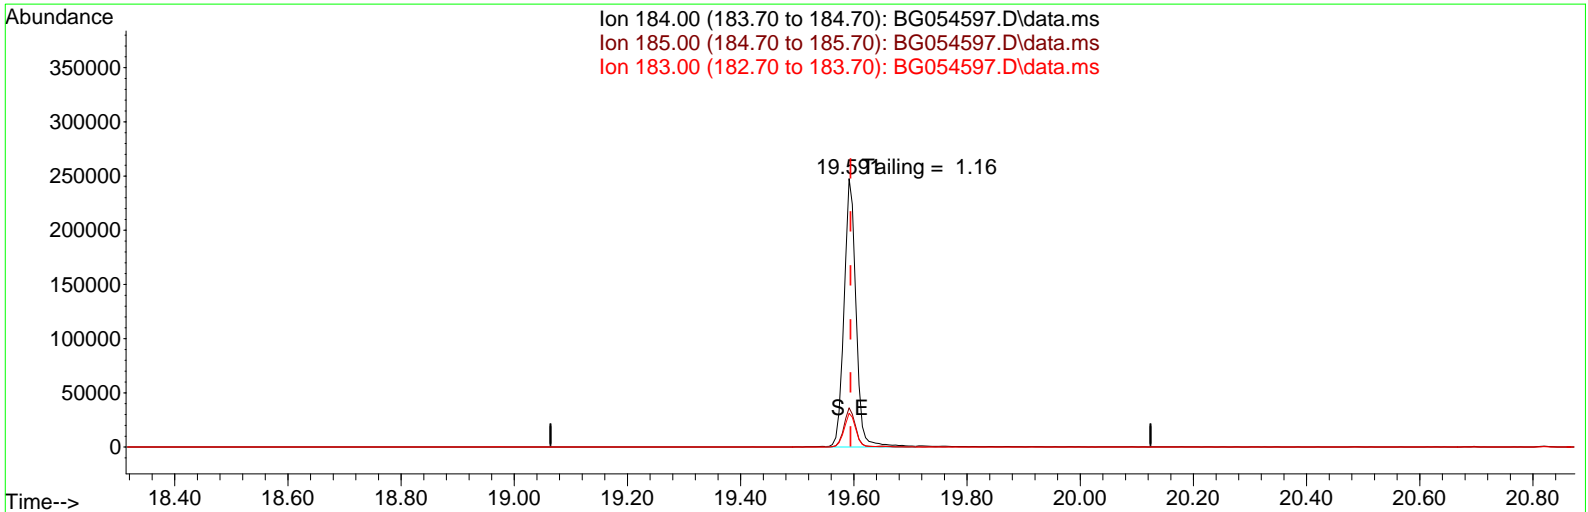

TIC: BG054597.D\data.ms

(77) Benzidine

19.591min (-0.003) 280333.67 ng

response 365548

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.63
183.00	11.10	12.57
0.00	0.00	0.00