


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081122\
Data File : BG054597.D
Acq On : 11 Aug 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 13 00:32:40 2022

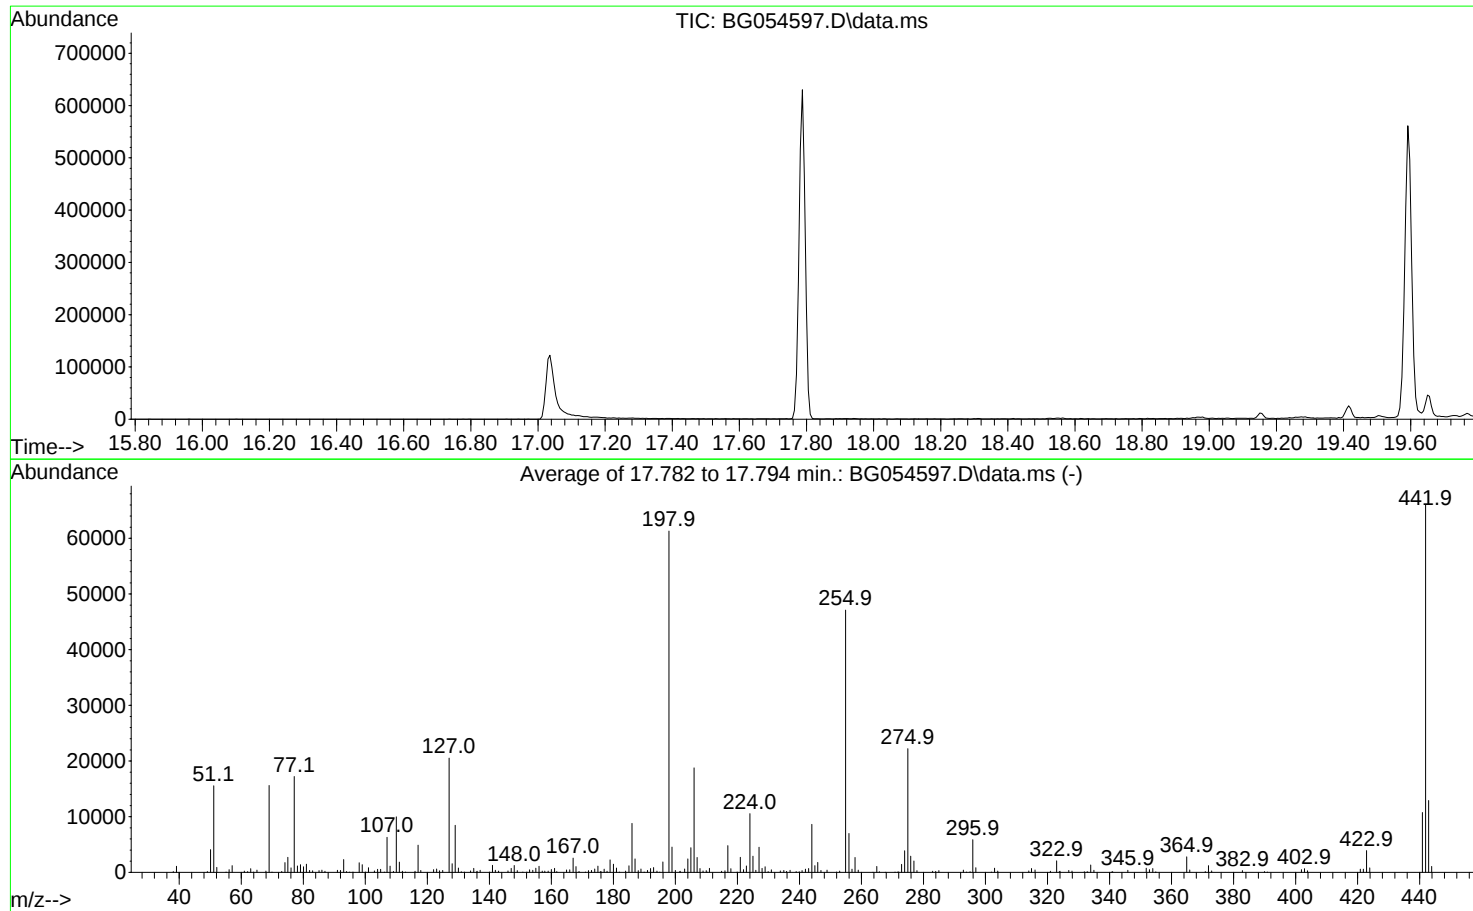




AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	15537	PASS
68	69	0.00	2	1.5	232	PASS
69	198	0.00	100	25.5	15605	PASS
70	69	0.00	2	0.3	52	PASS
127	198	10	80	33.5	20517	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61307	PASS
199	198	5	9	7.4	4556	PASS
275	198	10	60	36.2	22219	PASS
365	198	1	100	4.6	2791	PASS
441	198	0.01	100	17.5	10745	PASS
442	442	50	100	100.0	66077	PASS
443	442	15	24	19.5	12909	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081122\
Data File : BG054597.D
Acq On : 11 Aug 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 12 08:19:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

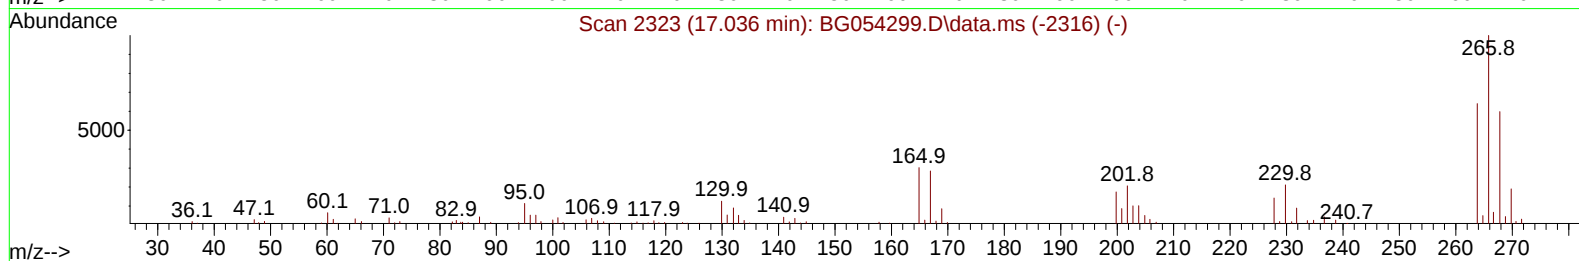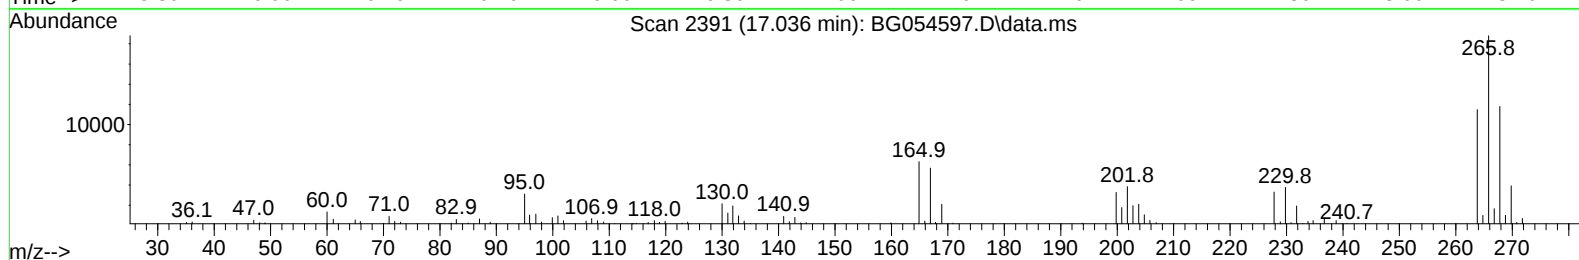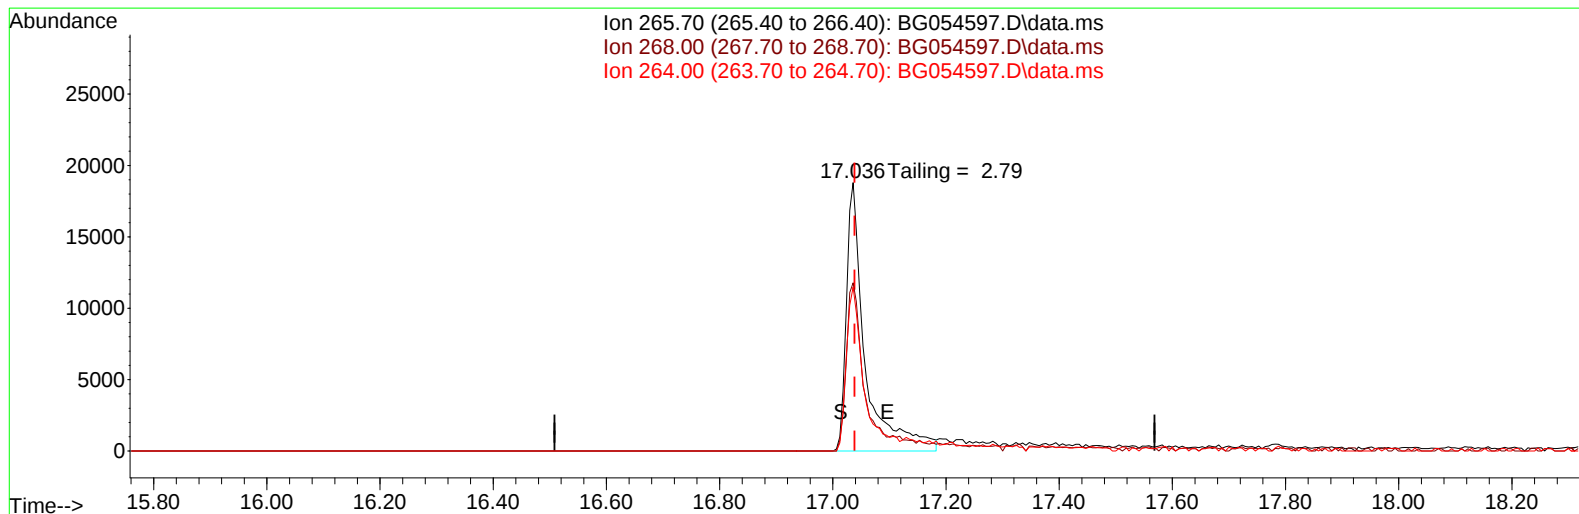

TIC: BG054597.D\data.ms

(70) Pentachlorophenol (C)

17.036min (-0.003) 14007.23 ng




response 38909

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	62.68
264.00	66.20	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081122\
Data File : BG054597.D
Acq On : 11 Aug 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 12 08:19:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

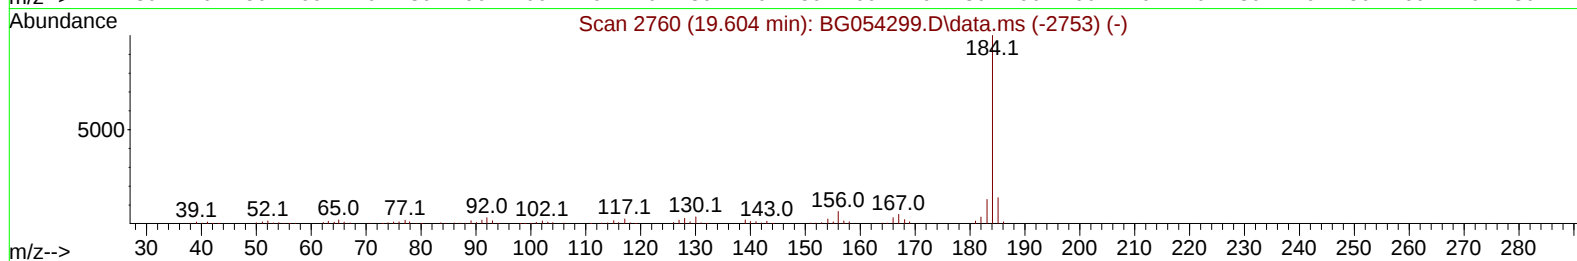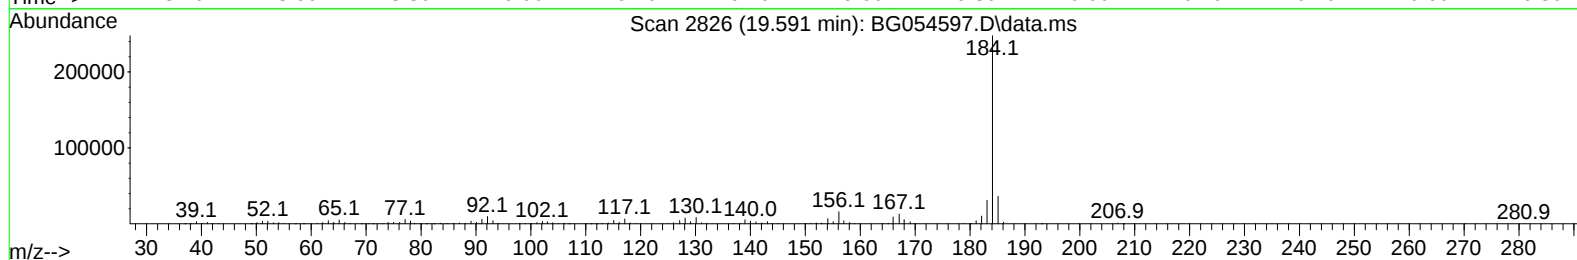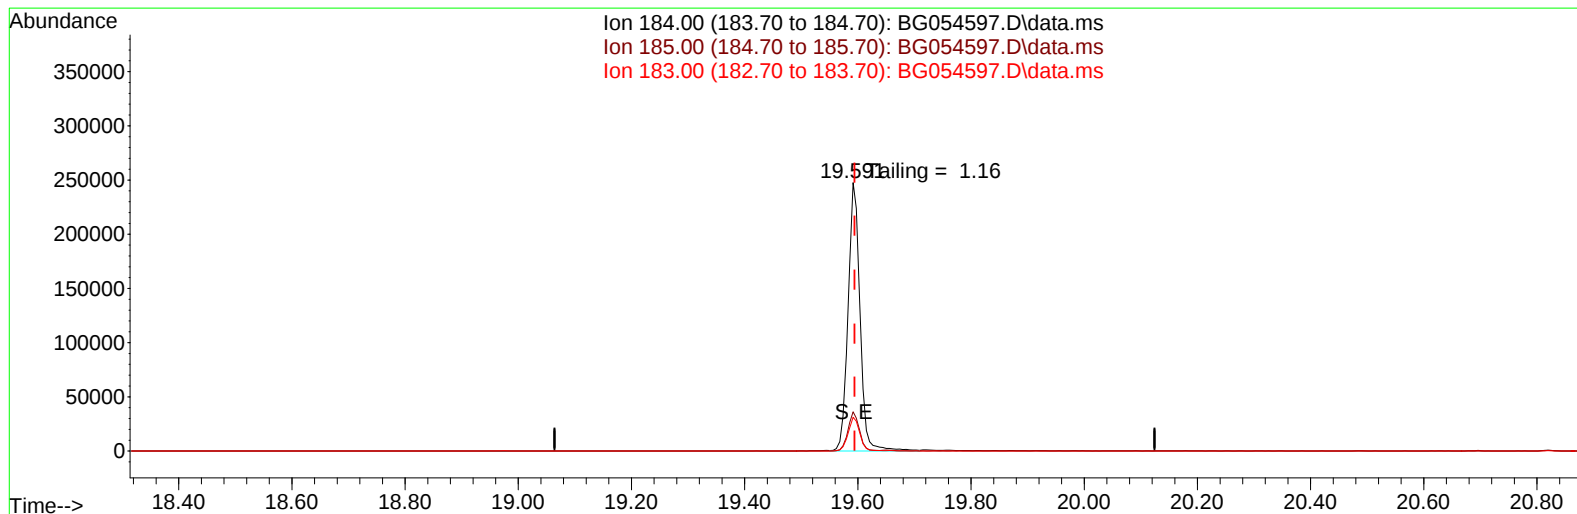

TIC: BG054597.D\data.ms

(77) Benzidine**19.591min (-0.003) 280333.67 ng****response 365548**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.63
183.00	11.10	12.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/11/2022	BNA_G	<u>BG054597.D</u>
Compound Name	Response	Retention Time
DDT	212983	20.819
DDD	11026	20.385
DDE	688	19.879
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11714	224697	5.21

Instrument :
BNA_G
ClientSampleId :
DFTPP