

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081215\
 Data File : BG018400.D
 Acq On : 12 Aug 2015 16:39
 Operator : UM/MA
 Sample : MDL-02-S
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MDL-02-S

Quant Time: Aug 13 02:09:18 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 02:05:44 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	154761	20.00	ng/ul	0.00
18) Naphthalene-d8	10.83	136	693836	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.65	164	461418	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.40	188	1117996	20.00	ng/ul	0.00
78) Chrysene-d12	21.66	240	1058127	20.00	ng/ul	0.00
86) Perylene-d12	24.88	264	1080302	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.46	96	14924	4.26	ng/uL	0.00
5) Phenol-d5	7.19	99	331323	23.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	211087	24.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.56	132	254760	23.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	282312	23.92	ng/ul	0.00
19) Nitrobenzene-d5	9.18	128	140997	26.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.91	143	150148	27.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.45	165	280777	24.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.96	131	404811	30.64	ng/ul	0.00
44) Dimethylphthalate-d6	14.05	166	969216	24.97	ng/ul	0.00
47) Acenaphthylene-d8	14.35	160	1163231	23.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	180171	25.80	ng/ul	0.00
58) Fluorene-d10	15.64	176	838215	24.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.75	200	126657	23.03	ng/ul	-0.01
71) Anthracene-d10	17.49	188	1300680	24.33	ng/ul	0.00
79) Pyrene-d10	19.78	212	1399392	25.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.65	264	1438865	25.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
35) 1-Methylnaphthalene	12.70	142	53223	2.05	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081215\
Data File : BG018400.D
Acq On : 12 Aug 2015 16:39
Operator : UM/MA
Sample : MDL-02-S
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MDL-02-S

Quant Time: Aug 13 02:09:18 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 13 02:05:44 2015
Response via : Initial Calibration

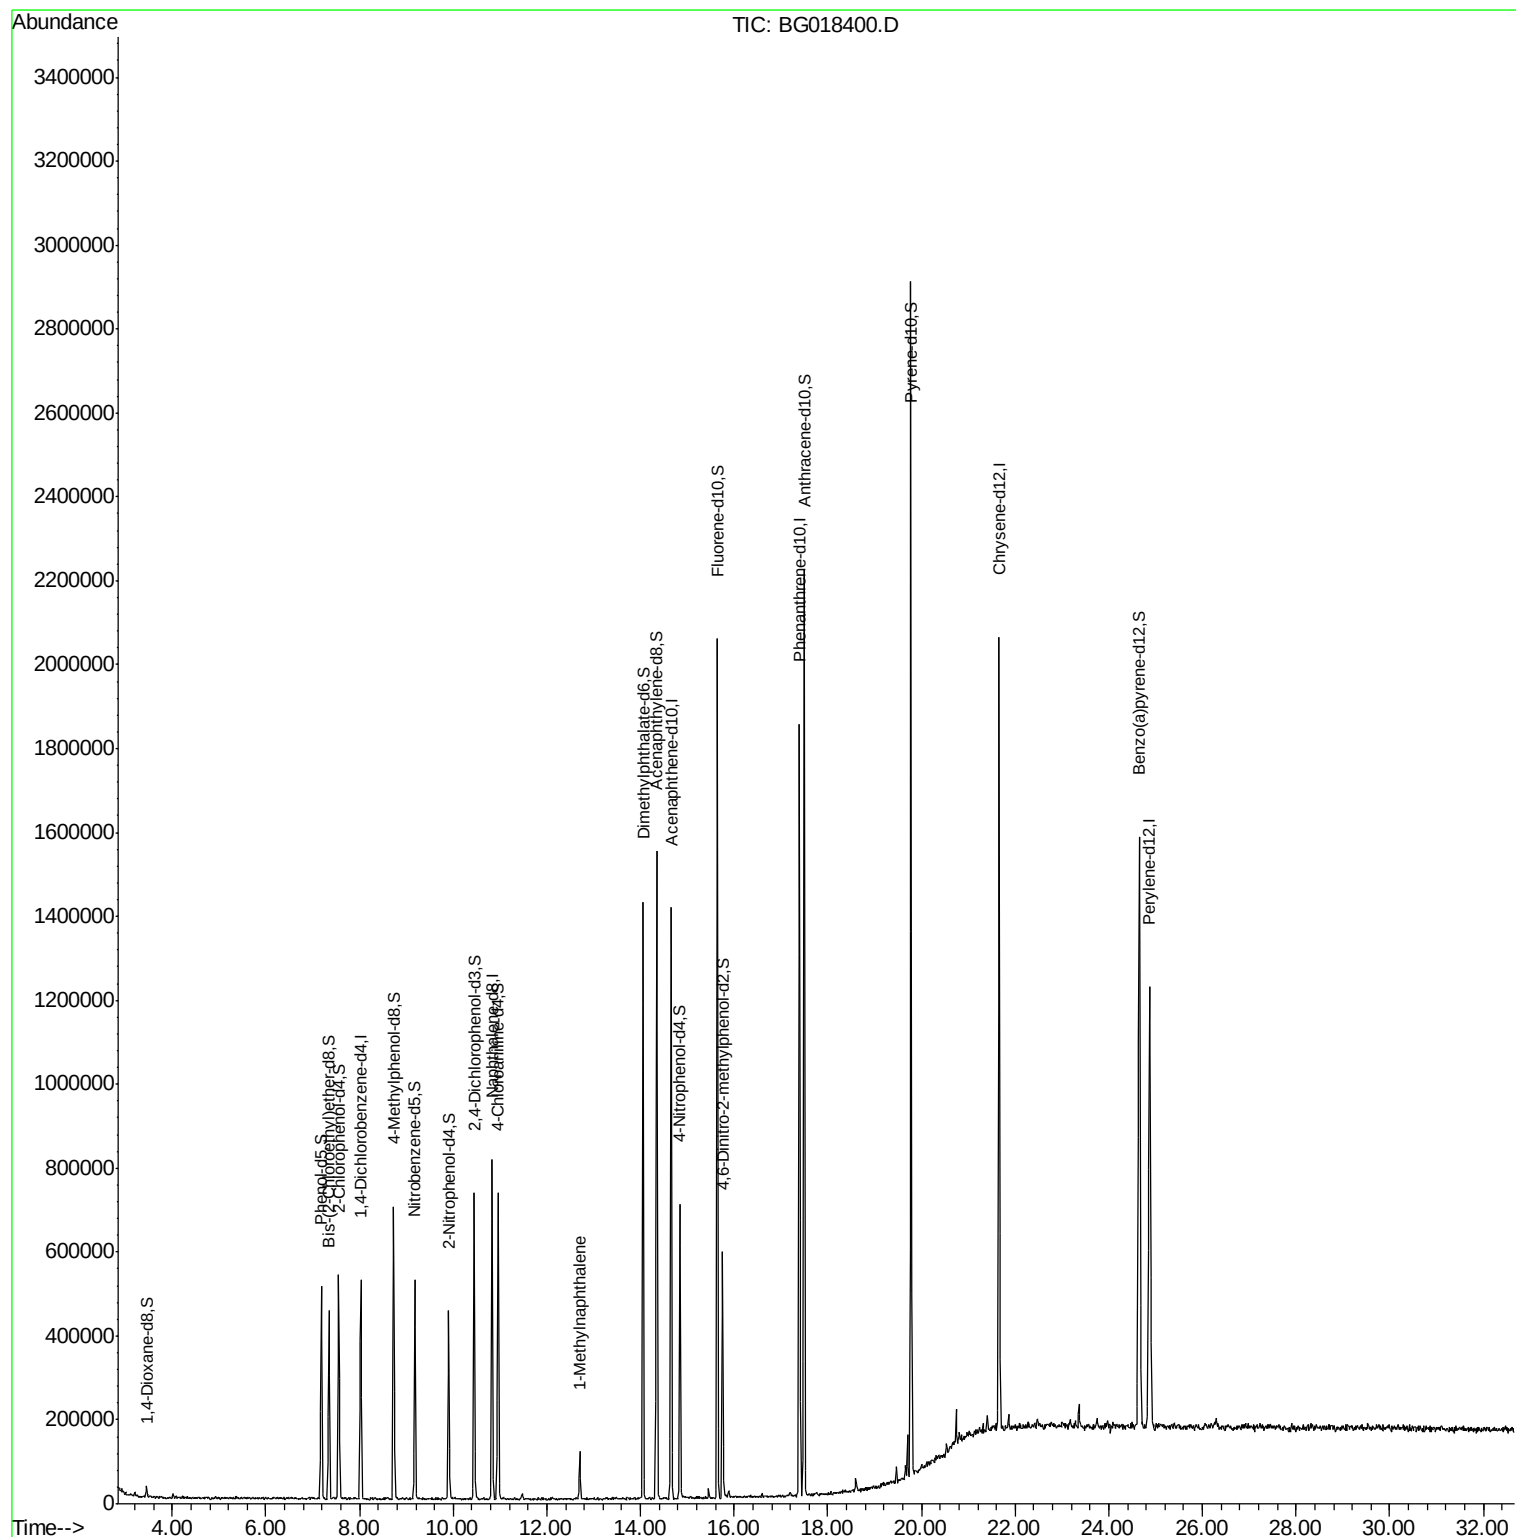

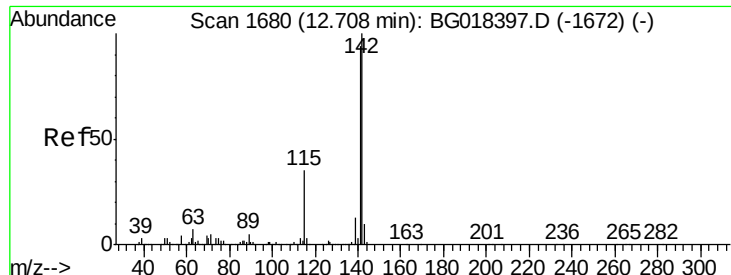

#35

1-Methylnaphthalene

Concen: 2.05 ng/ul

RT: 12.70 min Scan# 1679

Delta R.T. -0.00 min

Lab File: BG018400.D

Acq: 12 Aug 2015 16:39

Instrument :

BNA_G

ClientSampleId :

MDL-02-S


Tgt Ion:142 Resp: 53223

Ion Ratio Lower Upper

142 100

141 106.7 77.1 115.7

116 3.2 3.5 5.3#

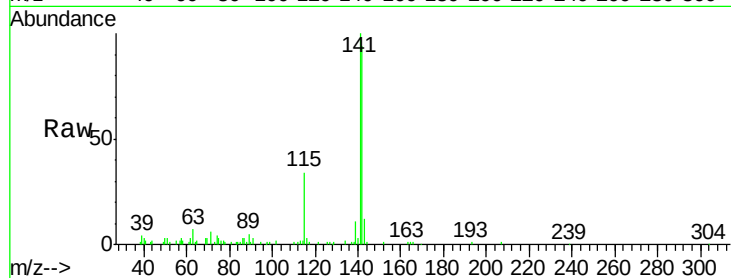

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

