

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081215\
 Data File : BG018414.D
 Acq On : 13 Aug 2015 2:11
 Operator : UM/MA
 Sample : MDL-07-S-ML
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MDL-07-S-ML

Quant Time: Aug 13 04:48:17 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 04:07:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	100084	20.00	ng/ul	0.00
18) Naphthalene-d8	10.83	136	441449	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.65	164	297055	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.39	188	734383	20.00	ng/ul	0.00
78) Chrysene-d12	21.65	240	707582	20.00	ng/ul	0.00
86) Perylene-d12	24.86	264	718233	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	9404	4.15	ng/uL	0.00
5) Phenol-d5	7.18	99	205854	22.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	132891	23.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	161854	23.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	179752	23.55	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	86198	25.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.90	143	94150	26.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	180566	24.28	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	257661	30.65	ng/ul	0.00
44) Dimethylphthalate-d6	14.05	166	645272	25.82	ng/ul	0.00
47) Acenaphthylene-d8	14.34	160	782651	24.87	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	111551	24.81	ng/ul	0.00
58) Fluorene-d10	15.64	176	556573	25.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.75	200	71267	19.73	ng/ul	0.00
71) Anthracene-d10	17.49	188	891471	25.38	ng/ul	0.00
79) Pyrene-d10	19.77	212	960712	26.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.64	264	989258	25.94	ng/ul	0.00


Target Compounds					Qvalue
35) 1-Methylnaphthalene	12.70	142	41790	2.53 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081215\
Data File : BG018414.D
Acq On : 13 Aug 2015 2:11
Operator : UM/MA
Sample : MDL-07-S-ML
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MDL-07-S-ML

Quant Time: Aug 13 04:48:17 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 13 04:07:48 2015
Response via : Initial Calibration

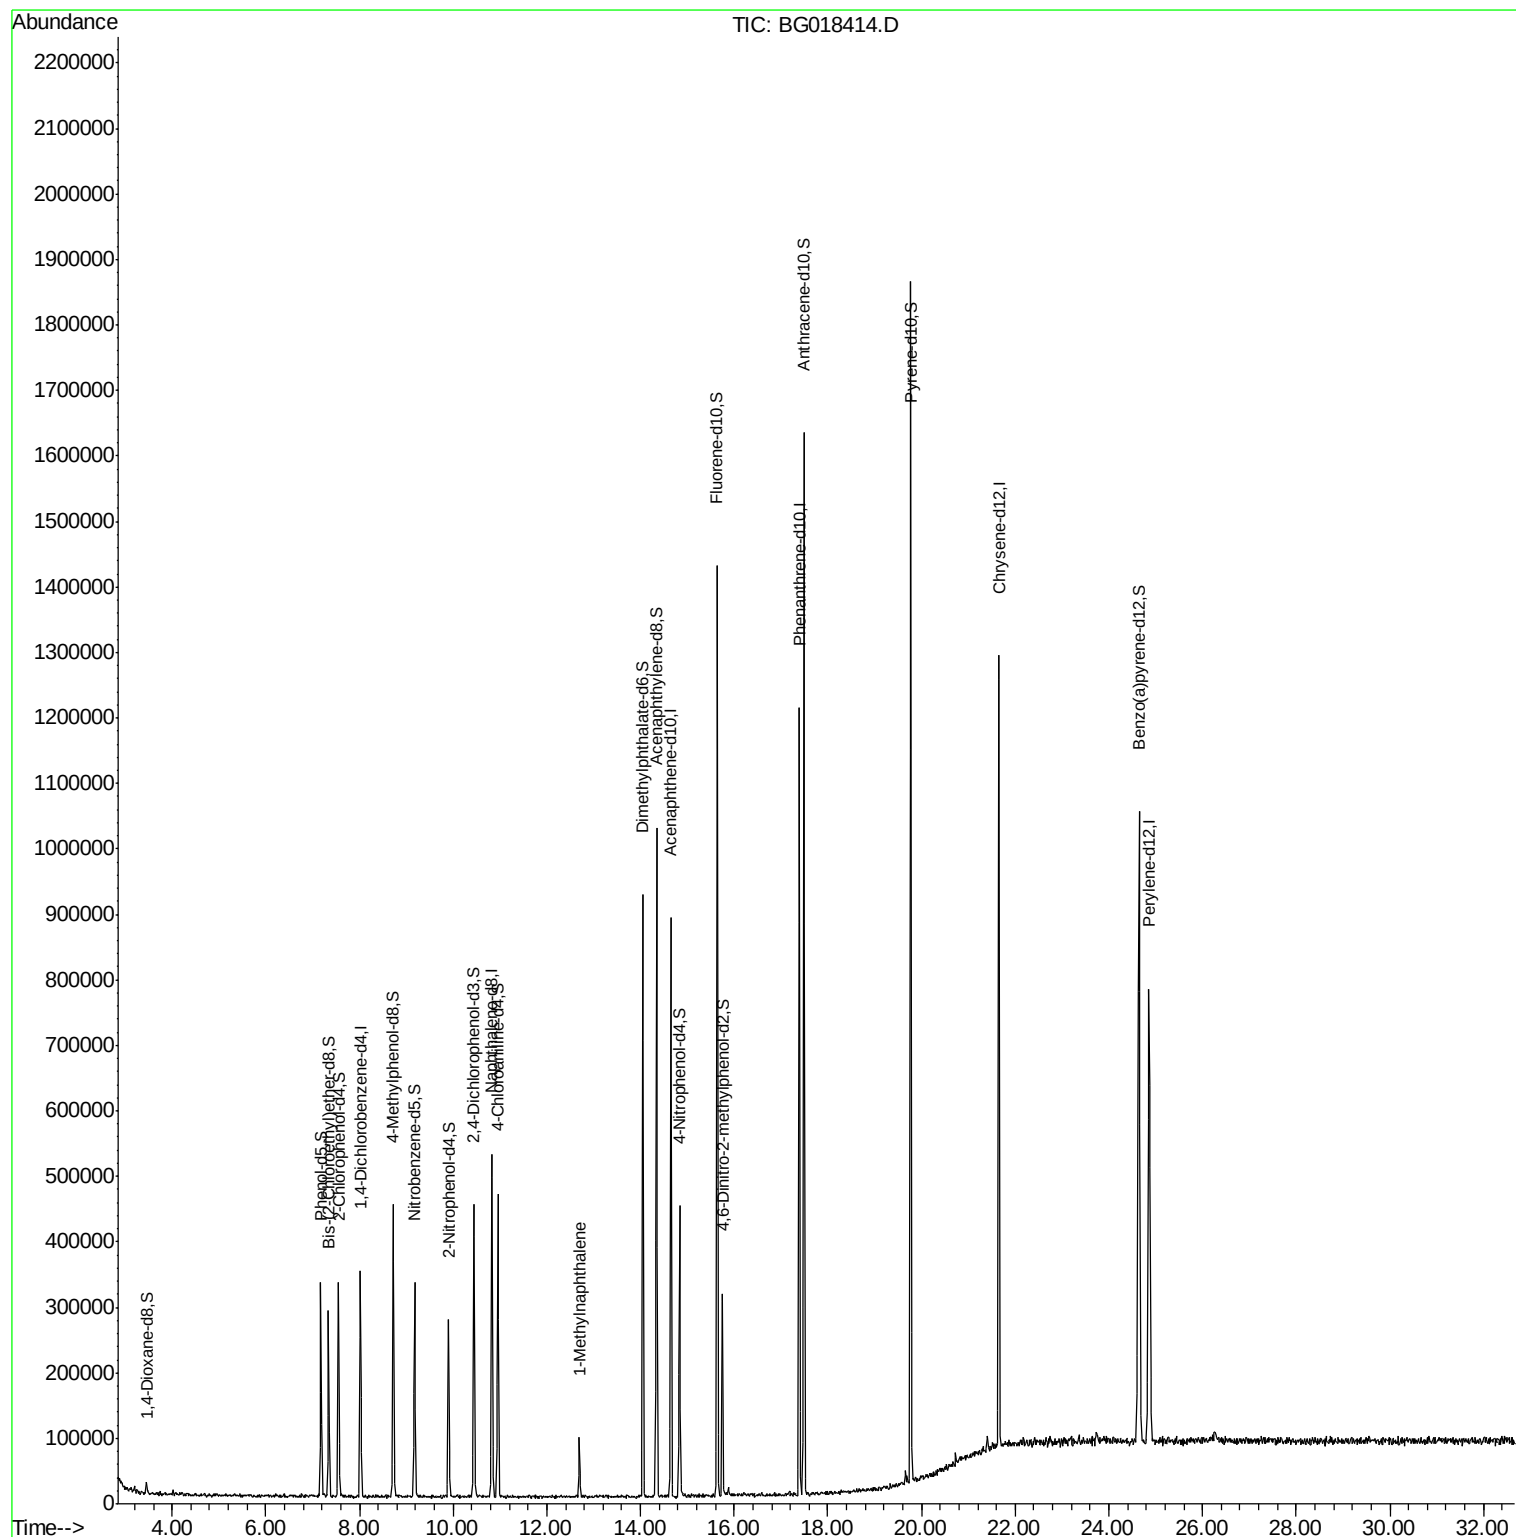

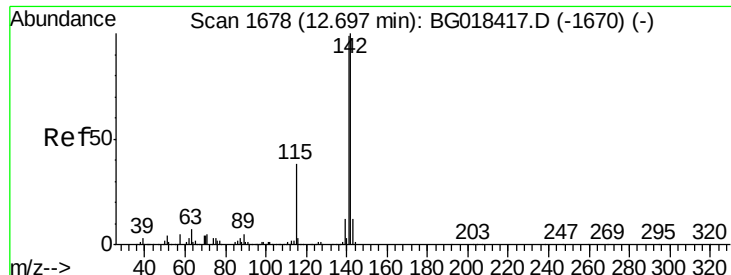

#35

1-Methylnaphthalene

Concen: 2.53 ng/ul

RT: 12.70 min Scan# 1678

Delta R.T. -0.00 min

Lab File: BG018414.D

Acq: 13 Aug 2015 2:11

Instrument :

BNA_G

ClientSampleId :

MDL-07-S-ML


Tgt Ion:142 Resp: 41790

Ion Ratio Lower Upper

142 100

141 96.3 77.1 115.7

116 3.9 3.5 5.3

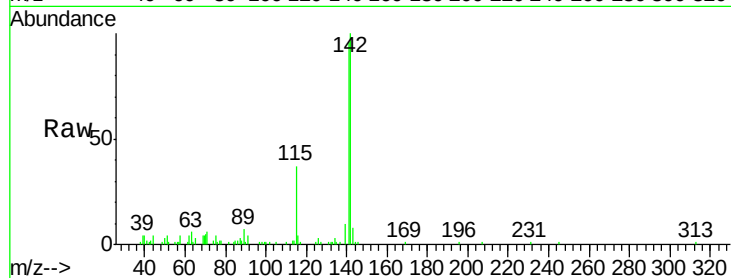

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

