

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081216\
 Data File : BG023674.D
 Acq On : 13 Aug 2016 2:37
 Operator : UM/SJ
 Sample : H4385-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P002-SS002-0612-01

Quant Time: Aug 13 03:24:31 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 03:19:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	116613	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.95	136	525378	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.79	164	355121	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.65	188	651222	20.00	ng/ul	0.09
75) Chrysene-d12	22.02	240	805	20.00	ng/ul	0.12
83) Perylene-d12	25.29	264	803913	20.00	ng/ul	-0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	6174	2.25	ng/uL	0.00
5) Phenol-d5	7.27	99	167318	14.24	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.43	67	113476	15.08	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.64	132	121662	15.18	ng/ul	-0.02
13) 4-Methylphenol-d8	8.83	113	129524	14.12	ng/ul	-0.02
19) Nitrobenzene-d5	9.29	128	68686	16.59	ng/ul	-0.01
22) 2-Nitrophenol-d4	10.03	143	80008	16.82	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.58	165	143061	15.95	ng/ul	-0.01
29) 4-Chloroaniline-d4	11.09	131	139642	13.27	ng/ul	-0.02
43) Dimethylphthalate-d6	14.18	166	503558	17.32	ng/ul	-0.01
46) Acenaphthylene-d8	14.48	160	595969	18.21	ng/ul	-0.01
51) 4-Nitrophenol-d4	15.01	143	65355	13.17	ng/ul	0.00
57) Fluorene-d10	15.78	176	449038	16.71	ng/ul	-0.01
62) 4,6-Dinitro-2-methylphenol	16.02	200	114	0.03	ng/ul	0.09
70) Anthracene-d10	17.65	188	651222	22.20	ng/ul	-0.01
76) Pyrene-d10	20.09	212	1043	25.60	ng/ul	0.13
87) Benzo(a)pyrene-d12	25.05	264	650528	17.88	ng/ul	-0.04

Target Compounds


					Qvalue
44) Dimethylphthalate	14.23	163	156957	5.45 ng/ul	99
47) Acenaphthylene	14.51	152	93486	2.73 ng/ul#	92
69) Phenanthrene	17.69	178	64875	1.92 ng/ul	96
71) Anthracene	17.69	178	67700	1.97 ng/ul	96
74) Fluoranthene	19.98	202	1121661	32.49 ng/ul	97
77) Pyrene	20.12	202	25920	520.85 ng/ul#	70
78) Butylbenzylphthalate	20.97	149	1013	53.07 ng/ul#	2
79) 3,3'-Dichlorobenzidine	21.92	252	7603	536.03 ng/ul#	17
80) Benzo(a)anthracene	21.93	228	608785	13428.81 ng/ul	91
81) Bis(2-ethylhexyl)phthalate	21.86	149	5259	207.21 ng/ul#	82
82) Chrysene	22.09	228	41482	1006.33 ng/ul#	29
85) Benzo(b)fluoranthene	24.21	252	632522	13.83 ng/ul#	95
86) Benzo(k)fluoranthene	24.26	252	205603	4.57 ng/ul#	92
88) Benzo(a)pyrene	24.97	252	348586	7.90 ng/ul	97
89) Indeno(1,2,3-cd)pyrene	29.19	276	307912	5.94 ng/ul#	88
91) Benzo(g,h,i)perylene	30.42	276	289814	6.74 ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081216\
Data File : BG023674.D
Acq On : 13 Aug 2016 2:37
Operator : UM/SJ
Sample : H4385-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0612-01

Quant Time: Aug 13 03:24:31 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 03:19:50 2016
Response via : Initial Calibration

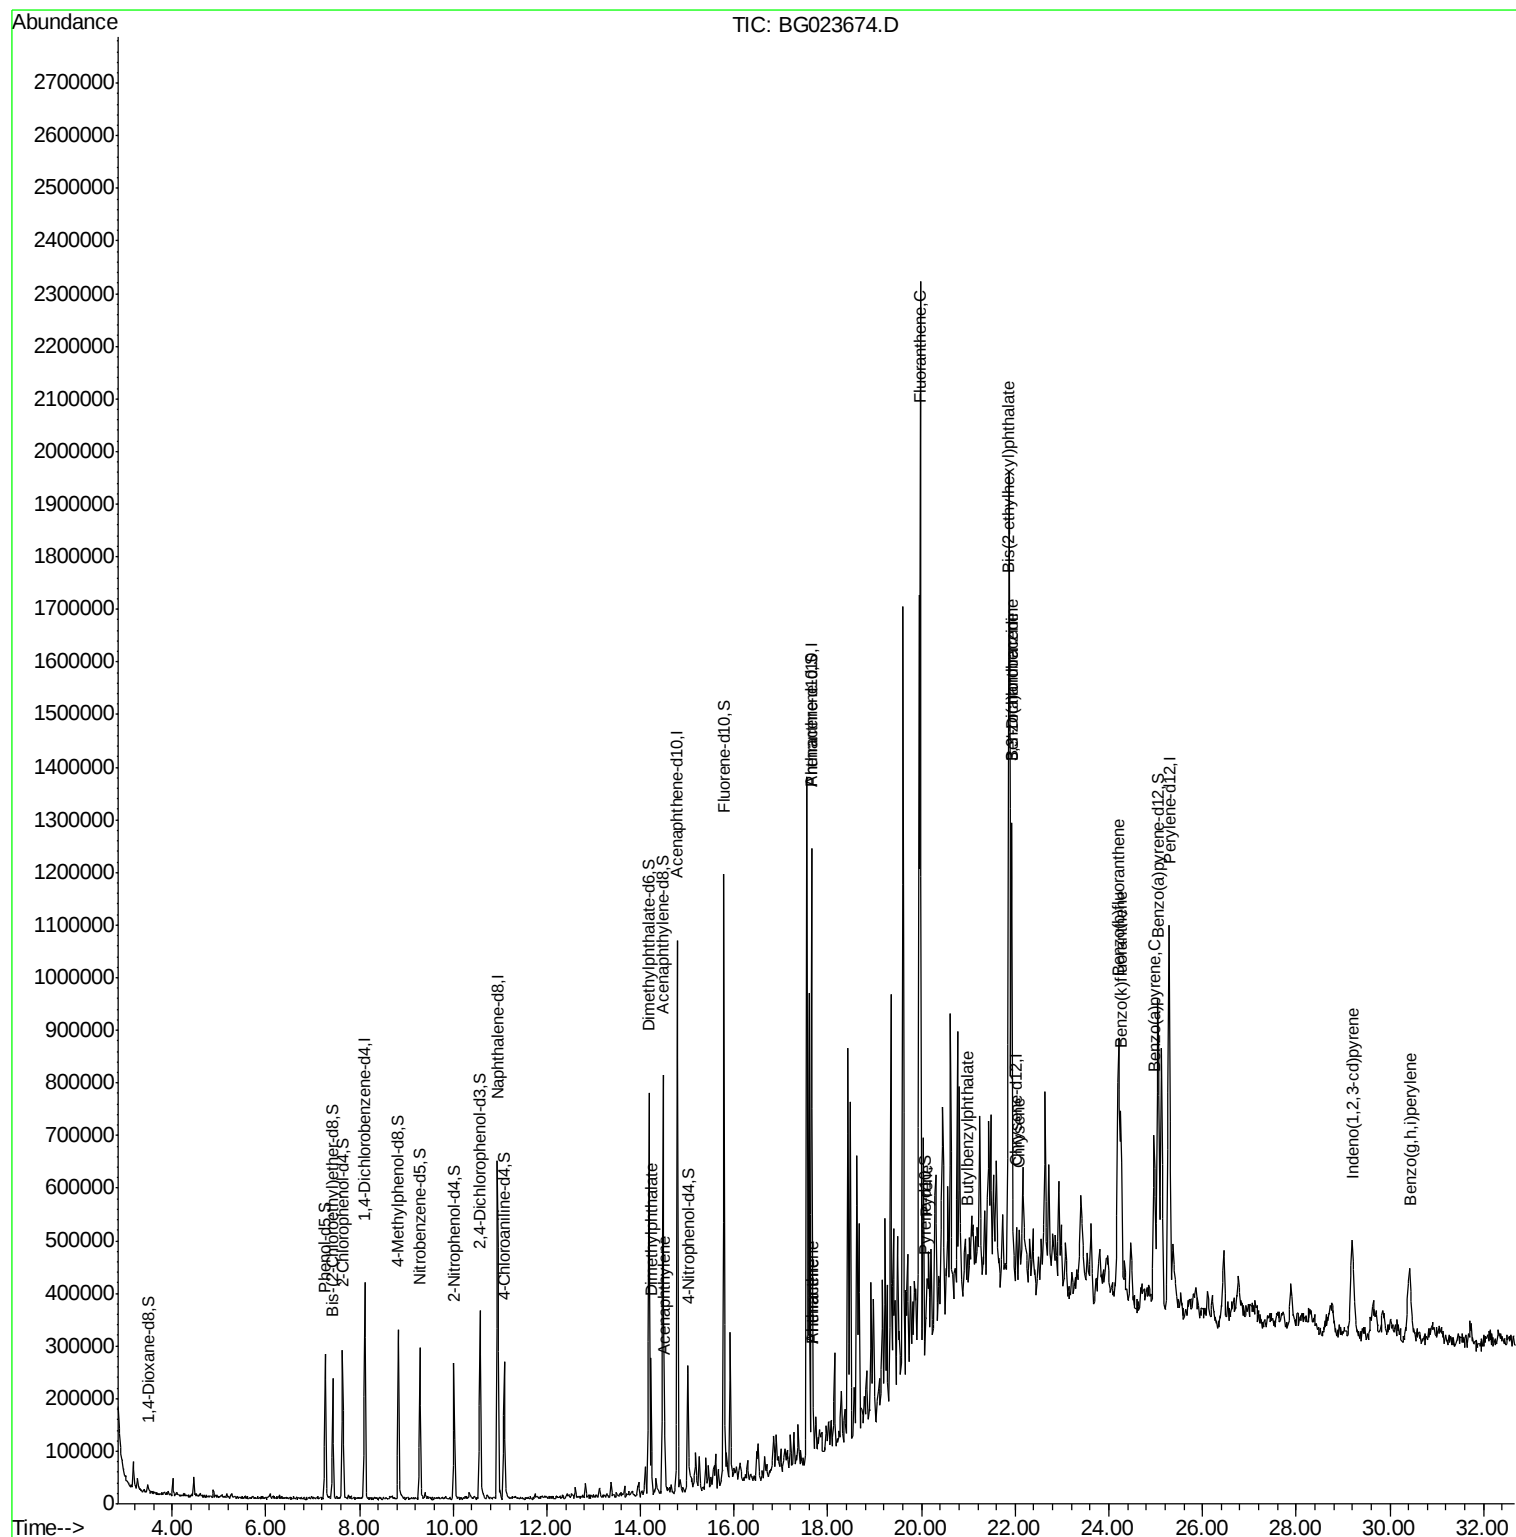



#44

Dimethylphthalate

Concen: 5.45 ng/ul

RT: 14.23 min Scan# 1938

Delta R.T. -0.01 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37





Instrument :

BNA_G

ClientSampleId :

P002-SS002-0612-01

Tgt Ion:	163	Resp:	156957
Ion Ratio		Lower	Upper
163	100		
194	4.4	3.4	5.2
164	11.3	8.8	13.2

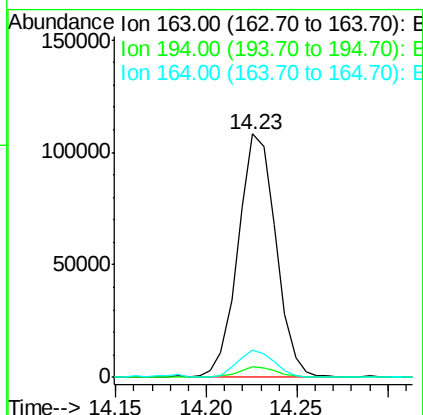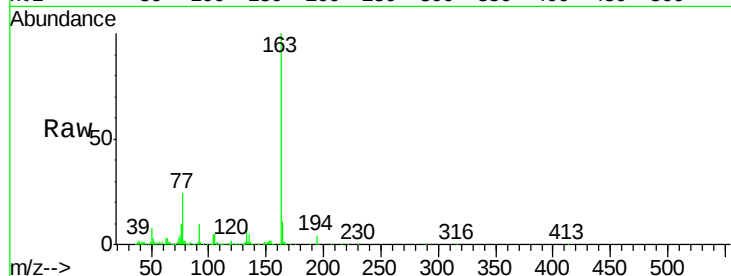

#47

Acenaphthylene

Concen: 2.73 ng/ul




RT: 14.51 min Scan# 1987


Delta R.T. -0.01 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37

Tgt Ion:	152	Resp:	93486
Ion Ratio		Lower	Upper
152	100		
151	18.3	17.5	26.3
153	10.9	11.1	16.7#

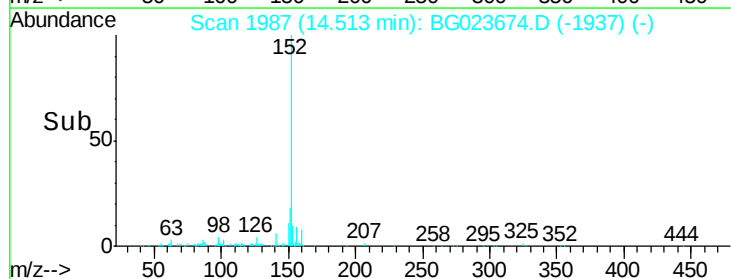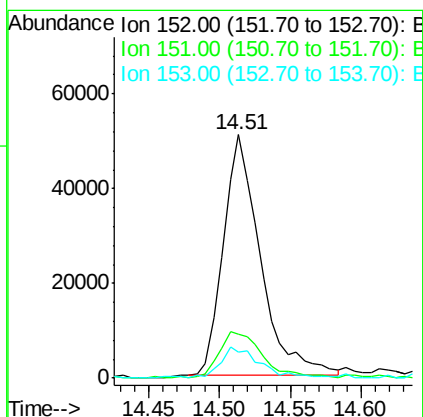

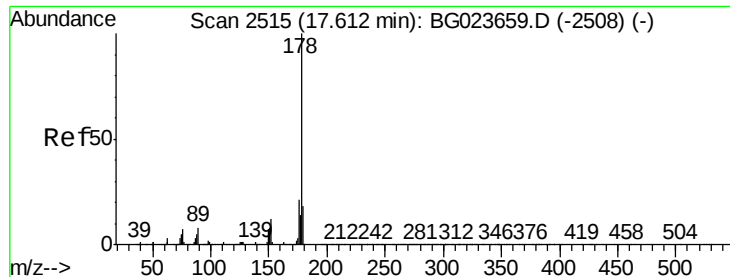

#69

Phenanthrene

Concen: 1.92 ng/ul

RT: 17.69 min Scan# 2527

Delta R.T. 0.07 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37

Instrument :

BNA_G

ClientSampleId :

P002-SS002-0612-01





Tgt Ion:178 Resp: 64875

Ion Ratio Lower Upper

178 100

179 14.6 12.9 19.3

176 17.8 15.8 23.8

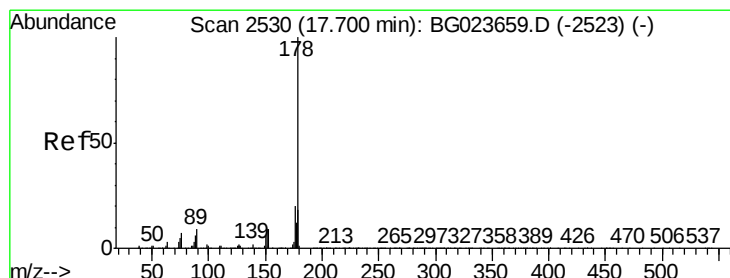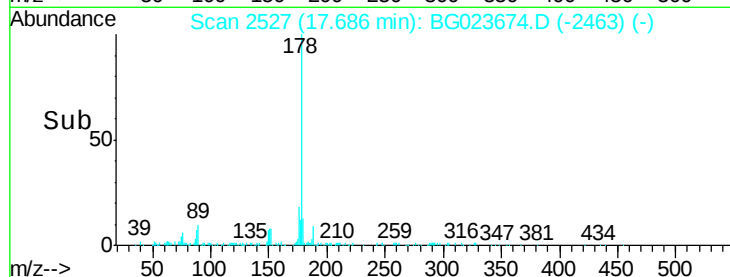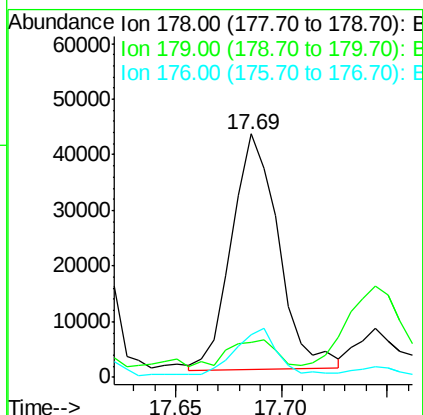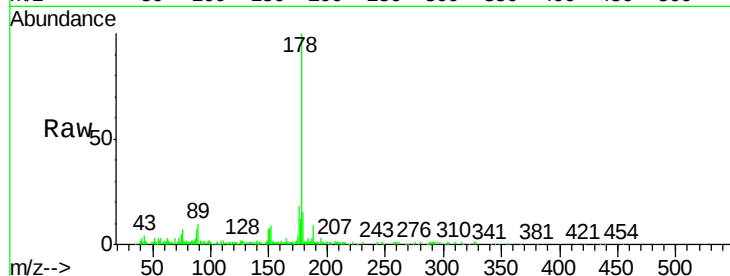

#71

Anthracene

Concen: 1.97 ng/ul

RT: 17.69 min Scan# 2527

Delta R.T. -0.01 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37




Tgt Ion:178 Resp: 67700


Ion Ratio Lower Upper

178 100

179 14.6 12.3 18.5

176 17.8 16.3 24.5

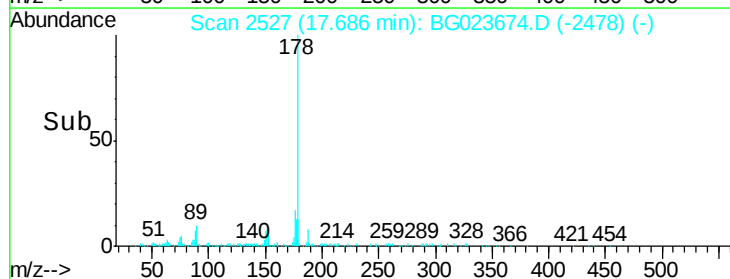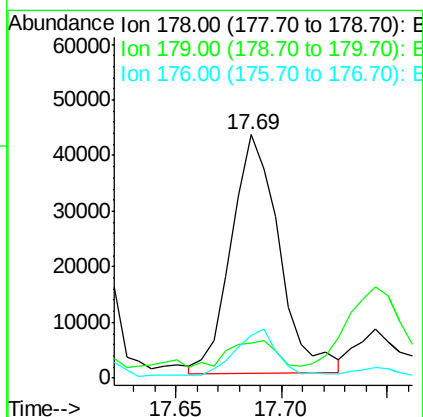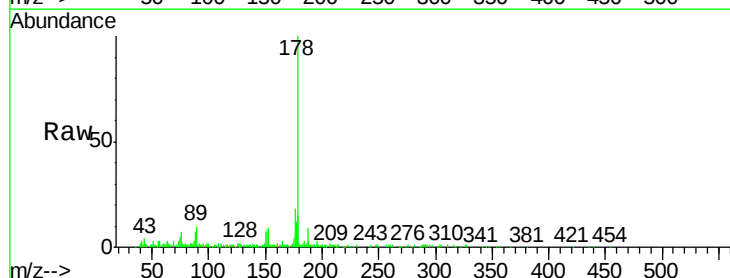

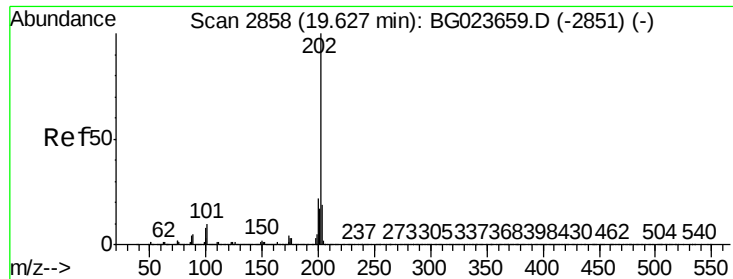

#74

Fluoranthene

Concen: 32.49 ng/ul

RT: 19.98 min Scan# 2917

Delta R.T. 0.35 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37

Instrument :

BNA_G

ClientSampleId :

P002-SS002-0612-01


Tgt Ion:202 Resp: 1121661

Ion Ratio Lower Upper

202 100

101 11.6 10.6 16.0




100 10.0 8.7 13.1

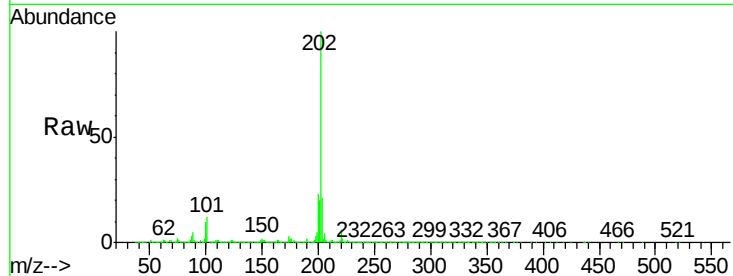

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

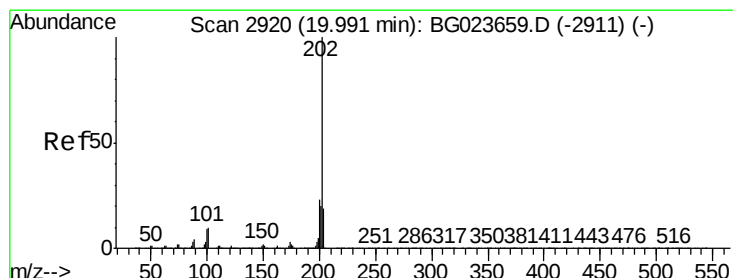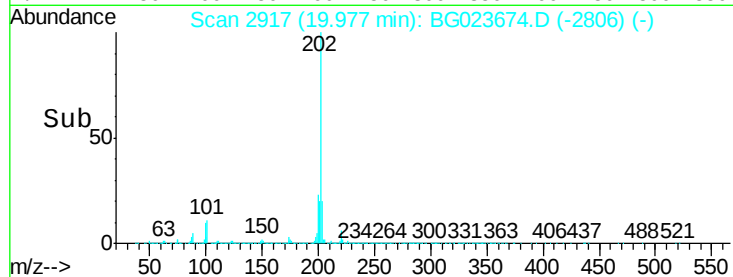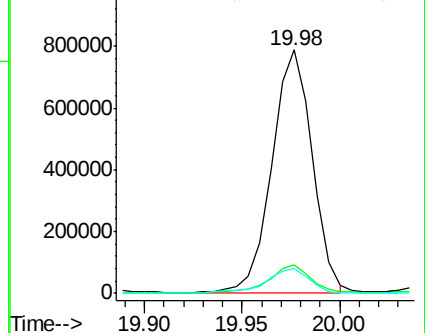

#77

Pyrene

Concen: 520.85 ng/ul

RT: 20.12 min Scan# 2941

Delta R.T. 0.13 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37


Tgt Ion:202 Resp: 25920

Ion Ratio Lower Upper

202 100

101 36.0 12.5 18.7#



100 9.5 10.2 15.4#

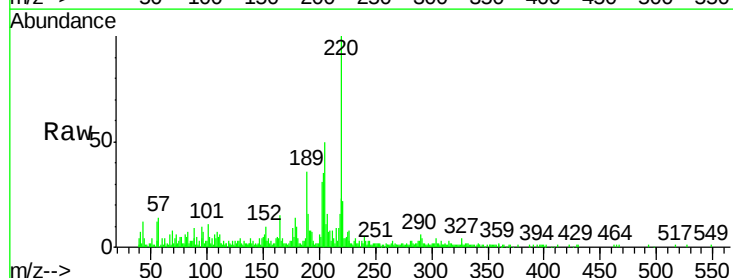


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

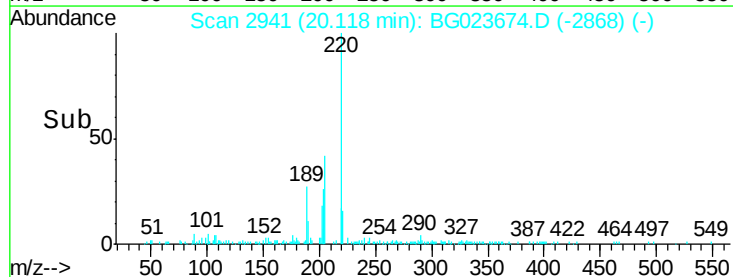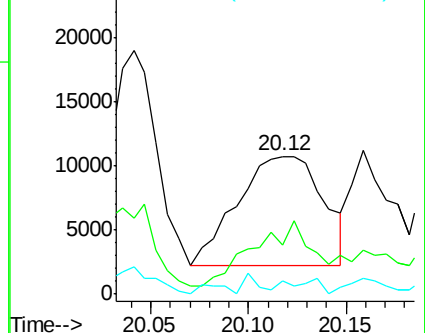



#78

Butylbenzylphthalate

Concen: 53.07 ng/ul

RT: 20.97 min Scan# 3086

Delta R.T. 0.11 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37

Instrument :

BNA_G

ClientSampleId :

P002-SS002-0612-01


Tgt Ion:149 Resp: 1013

Ion Ratio Lower Upper

149 100

91 130.4 54.2 81.4#




206 95.0 14.1 21.1#

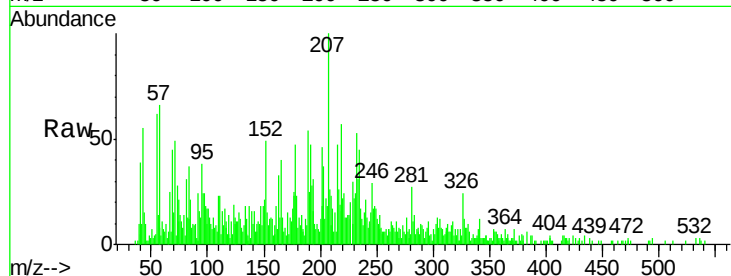

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BG023659.D (-3060) (-)

Ion 206.00 (205.70 to 206.70): E

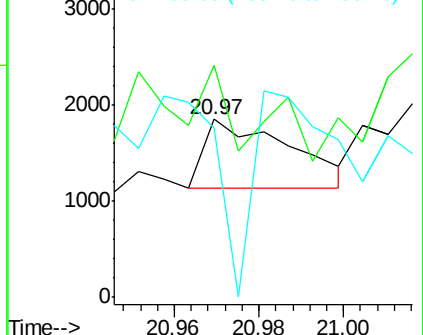

#79

3,3'-Dichlorobenzidine

Concen: 536.03 ng/ul

RT: 21.92 min Scan# 3248

Delta R.T. 0.14 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37


Tgt Ion:252 Resp: 7603

Ion Ratio Lower Upper

252 100

254 120.7 51.4 77.2#



126 67.1 10.7 16.1#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 254.00 (253.70 to 254.70): E

Ion 126.00 (125.70 to 126.70): E

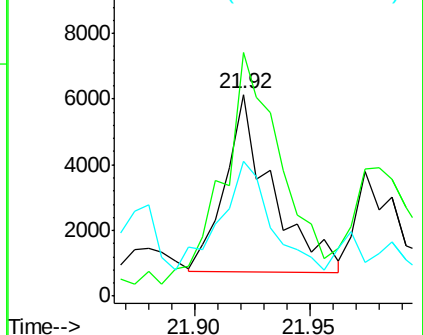

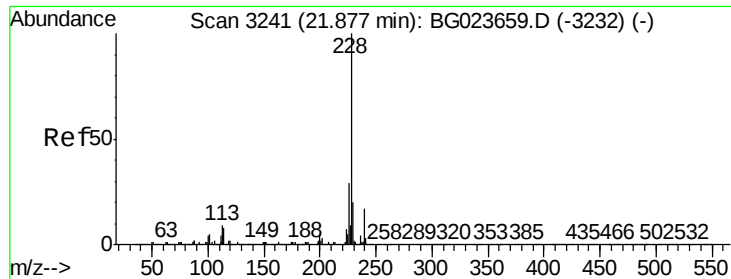

#80

Benzo(a)anthracene

Concen: 13428.81 ng/ul

RT: 21.93 min Scan# 3249

Delta R.T. 0.05 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37

Instrument :

BNA_G

ClientSampleId :

P002-SS002-0612-01





Tgt Ion: 228 Resp: 608785

Ion Ratio Lower Upper

228 100

229 23.1 15.4 23.2

226 33.1 22.8 34.2

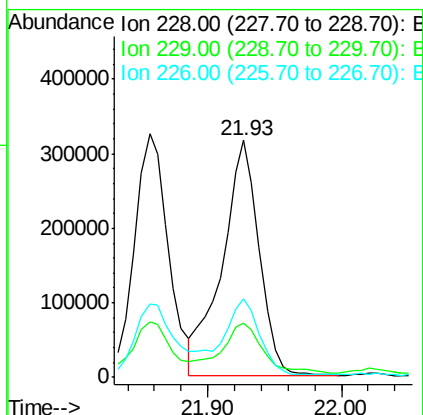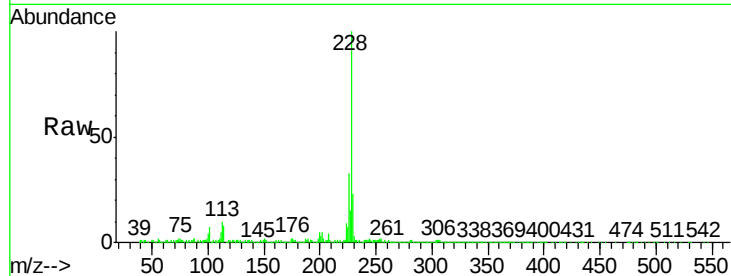

#81

Bis(2-ethylhexyl)phthalate

Concen: 207.21 ng/ul

RT: 21.86 min Scan# 3237

Delta R.T. 0.11 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37




Tgt Ion: 149 Resp: 5259


Ion Ratio Lower Upper

149 100

167 19.3 21.9 32.9#

279 15.4 2.9 4.3#

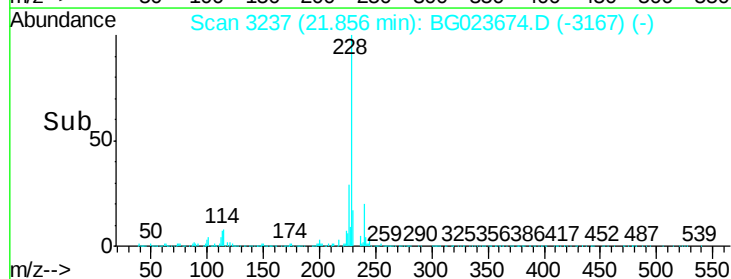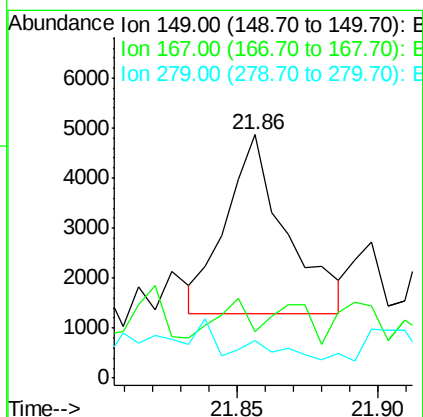

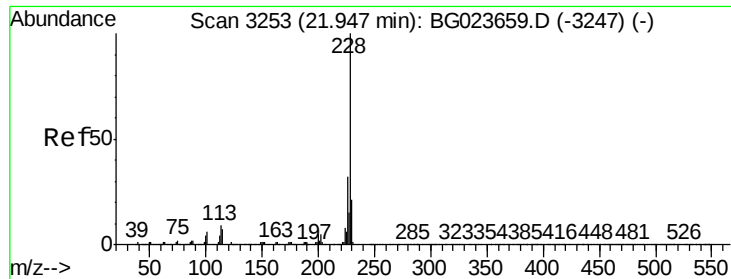

#82

Chrysene

Concen: 1006.33 ng/ul

RT: 22.09 min Scan# 3276

Delta R.T. 0.14 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37

Instrument :

BNA_G

ClientSampleId :

P002-SS002-0612-01


Tgt Ion:228 Resp: 41482

Ion Ratio Lower Upper

228 100

226 70.3 24.2 36.4#




229 49.3 15.0 22.6#

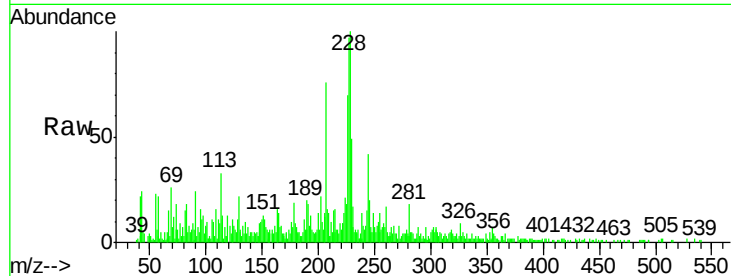

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

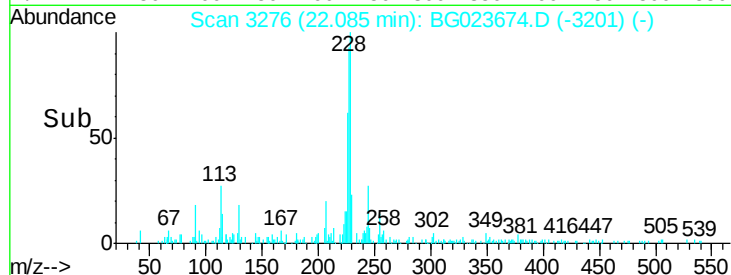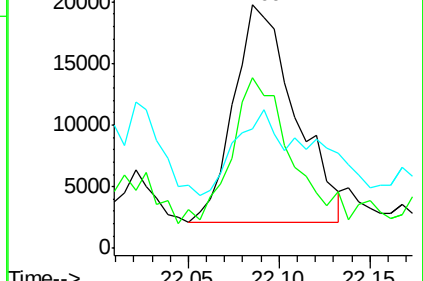

#85

Benzo(b)fluoranthene

Concen: 13.83 ng/ul

RT: 24.21 min Scan# 3637

Delta R.T. -0.03 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37


Tgt Ion:252 Resp: 632522

Ion Ratio Lower Upper

252 100

253 23.8 18.2 27.2



125 9.7 10.8 16.2#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E




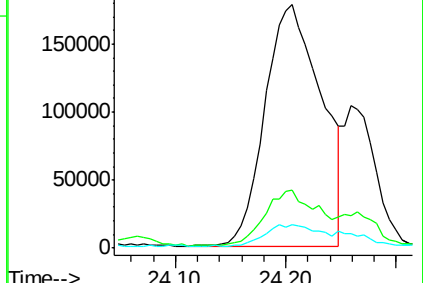


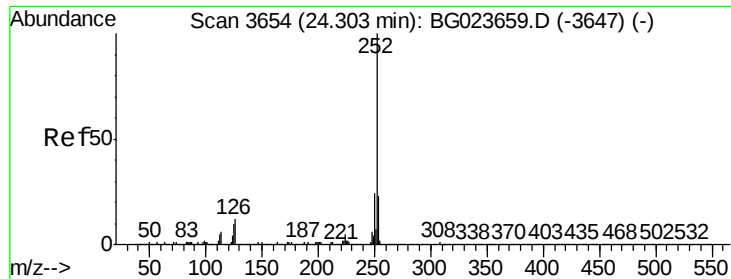

#86
Benzo(k)fluoranthene
Concen: 4.57 ng/ul
RT: 24.26 min Scan# 3646
Delta R.T. -0.04 min
Lab File: BG023674.D
Acq: 13 Aug 2016 2:37




Instrument :
BNA_G
ClientSampleId :
P002-SS002-0612-01


Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	15.8	23.6
125	10.3	10.6	16.0

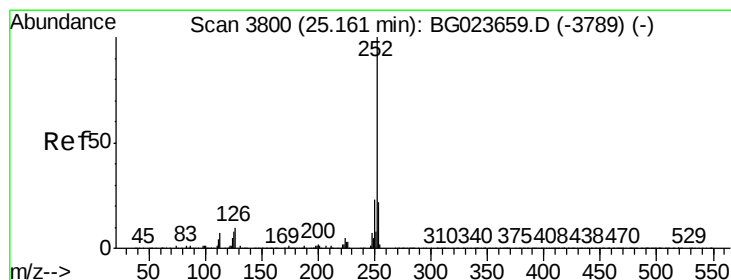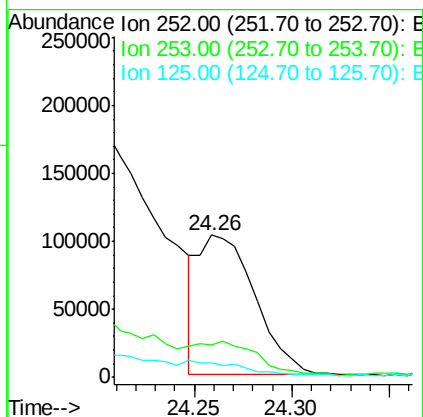

#88
Benzo(a)pyrene
Concen: 7.90 ng/ul
RT: 24.97 min Scan# 3767
Delta R.T. -0.19 min
Lab File: BG023674.D
Acq: 13 Aug 2016 2:37

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.8	19.0	28.4
125	12.3	12.0	18.0

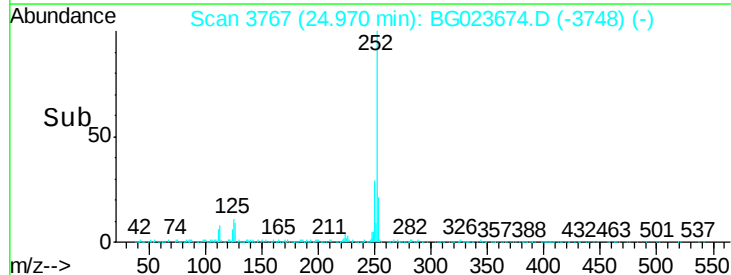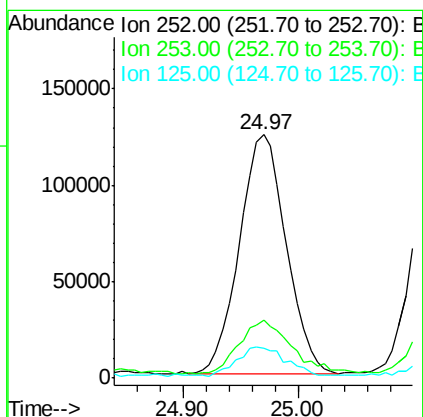



#89

Indeno(1,2,3-cd)pyrene

Concen: 5.94 ng/ul

RT: 29.19 min Scan# 4486

Delta R.T. -0.08 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37





Instrument :

BNA_G

ClientSampleId :

P002-SS002-0612-01

Tgt Ion:	276	Resp:	307912
Ion Ratio	Lower	Upper	
276	100		
138	18.2	20.8	31.2#
277	26.2	17.6	26.4

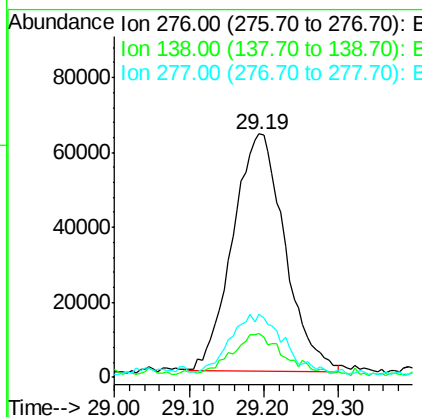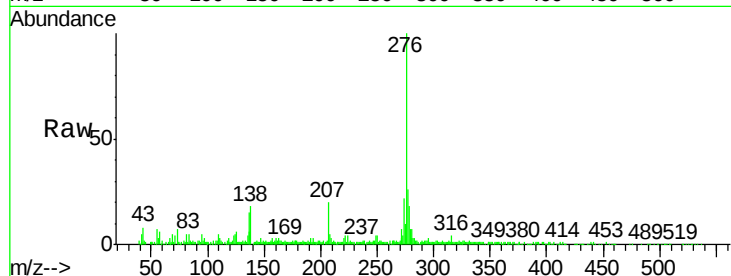

#91

Benzo(g,h,i)perylene

Concen: 6.74 ng/ul

RT: 30.42 min Scan# 4695

Delta R.T. -0.09 min

Lab File: BG023674.D

Acq: 13 Aug 2016 2:37

Tgt Ion:	276	Resp:	289814
Ion Ratio	Lower	Upper	
276	100		
138	17.9	22.1	33.1#
277	23.2	17.0	25.4

