

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081216\
 Data File : BG023658.D
 Acq On : 12 Aug 2016 16:13
 Operator : UM/SJ
 Sample : H4360-13MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS003-0206-01MSD

Manual Integrations
 APPROVED

sohil
 8/15/2016 6:49:35 PM

Quant Time: Aug 13 03:15:56 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 01:31:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	228587	20.00	ng/ul	0.00
18) Naphthalene-d8	10.96	136	1048941	20.00	ng/ul	0.01
35) Acenaphthene-d10	14.80	164	665480	20.00	ng/ul	0.01
61) Phenanthrene-d10	17.56	188	1091509	20.00	ng/ul	0.00
75) Chrysene-d12	21.89	240	973260	20.00	ng/ul	0.00
83) Perylene-d12	25.31	264	1001392	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	5854	1.09	ng/uL	0.01
5) Phenol-d5	7.28	99	385944	16.76	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.43	67	232235m	15.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	281565	17.92	ng/ul	0.01
13) 4-Methylphenol-d8	8.83	113	274939	15.29	ng/ul	0.01
19) Nitrobenzene-d5	9.30	128	140937	17.05	ng/ul	0.01
22) 2-Nitrophenol-d4	10.03	143	181765	19.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.58	165	317544	17.73	ng/ul	0.01
29) 4-Chloroaniline-d4	11.10	131	52513	2.50	ng/ul	0.01
43) Dimethylphthalate-d6	14.19	166	905477	16.62	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	1056129	17.22	ng/ul	0.00
51) 4-Nitrophenol-d4	15.01	143	96097	10.33	ng/ul	0.01
57) Fluorene-d10	15.79	176	725890	14.42	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.93	200	53444	7.63	ng/ul	0.02
70) Anthracene-d10	17.66	188	840874	17.10	ng/ul	0.00
76) Pyrene-d10	19.96	212	779120	15.81	ng/ul	0.01
87) Benzo(a)pyrene-d12	25.07	264	741635	16.36	ng/ul	0.02

Target Compounds

						Qvalue
6) Phenol	7.30	94	394632	16.46	ng/ul#	70
10) 2-Chlorophenol	7.68	128	279705	17.48	ng/ul#	83
15) N-Nitroso-di-n-propylamine	8.92	70	276991	15.97	ng/ul#	85
33) 4-Chloro-3-methylphenol	12.25	107	345848m	14.88	ng/ul	
44) Dimethylphthalate	14.23	163	532744	9.87	ng/ul	99
49) Acenaphthene	14.86	153	730842	16.72	ng/ul	94
52) 4-Nitrophenol	15.03	109	92148m	9.89	ng/ul	
54) 2,4-Dinitrotoluene	15.17	165	235685	13.30	ng/ul#	76
68) Pentachlorophenol	17.22	266	95347	12.96	ng/ul	87
69) Phenanthrene	17.60	178	174186	3.08	ng/ul	96
74) Fluoranthene	19.62	202	309485	5.35	ng/ul#	91
77) Pyrene	19.98	202	1223541	20.34	ng/ul#	92
80) Benzo(a)anthracene	21.86	228	147657	2.69	ng/ul#	92
81) Bis(2-ethylhexyl)phthalate	21.74	149	39223	1.28	ng/ul#	75
82) Chrysene	21.93	228	180834	3.63	ng/ul#	91
85) Benzo(b)fluoranthene	24.22	252	238603	4.19	ng/ul#	75
86) Benzo(k)fluoranthene	24.28	252	83074m	1.48	ng/ul	
88) Benzo(a)pyrene	25.14	252	157704	2.87	ng/ul#	90
89) Indeno(1,2,3-cd)pyrene	29.24	276	97099m	1.50	ng/ul	
91) Benzo(g,h,i)perylene	30.49	276	93982m	1.75	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081216\
Data File : BG023658.D
Acq On : 12 Aug 2016 16:13
Operator : UM/SJ
Sample : H4360-13MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
PR001-SS003-0206-01MSD

Manual Integrations
APPROVED

sohil
8/15/2016 6:49:35 PM

Quant Time: Aug 13 03:15:56 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 01:31:24 2016
Response via : Initial Calibration

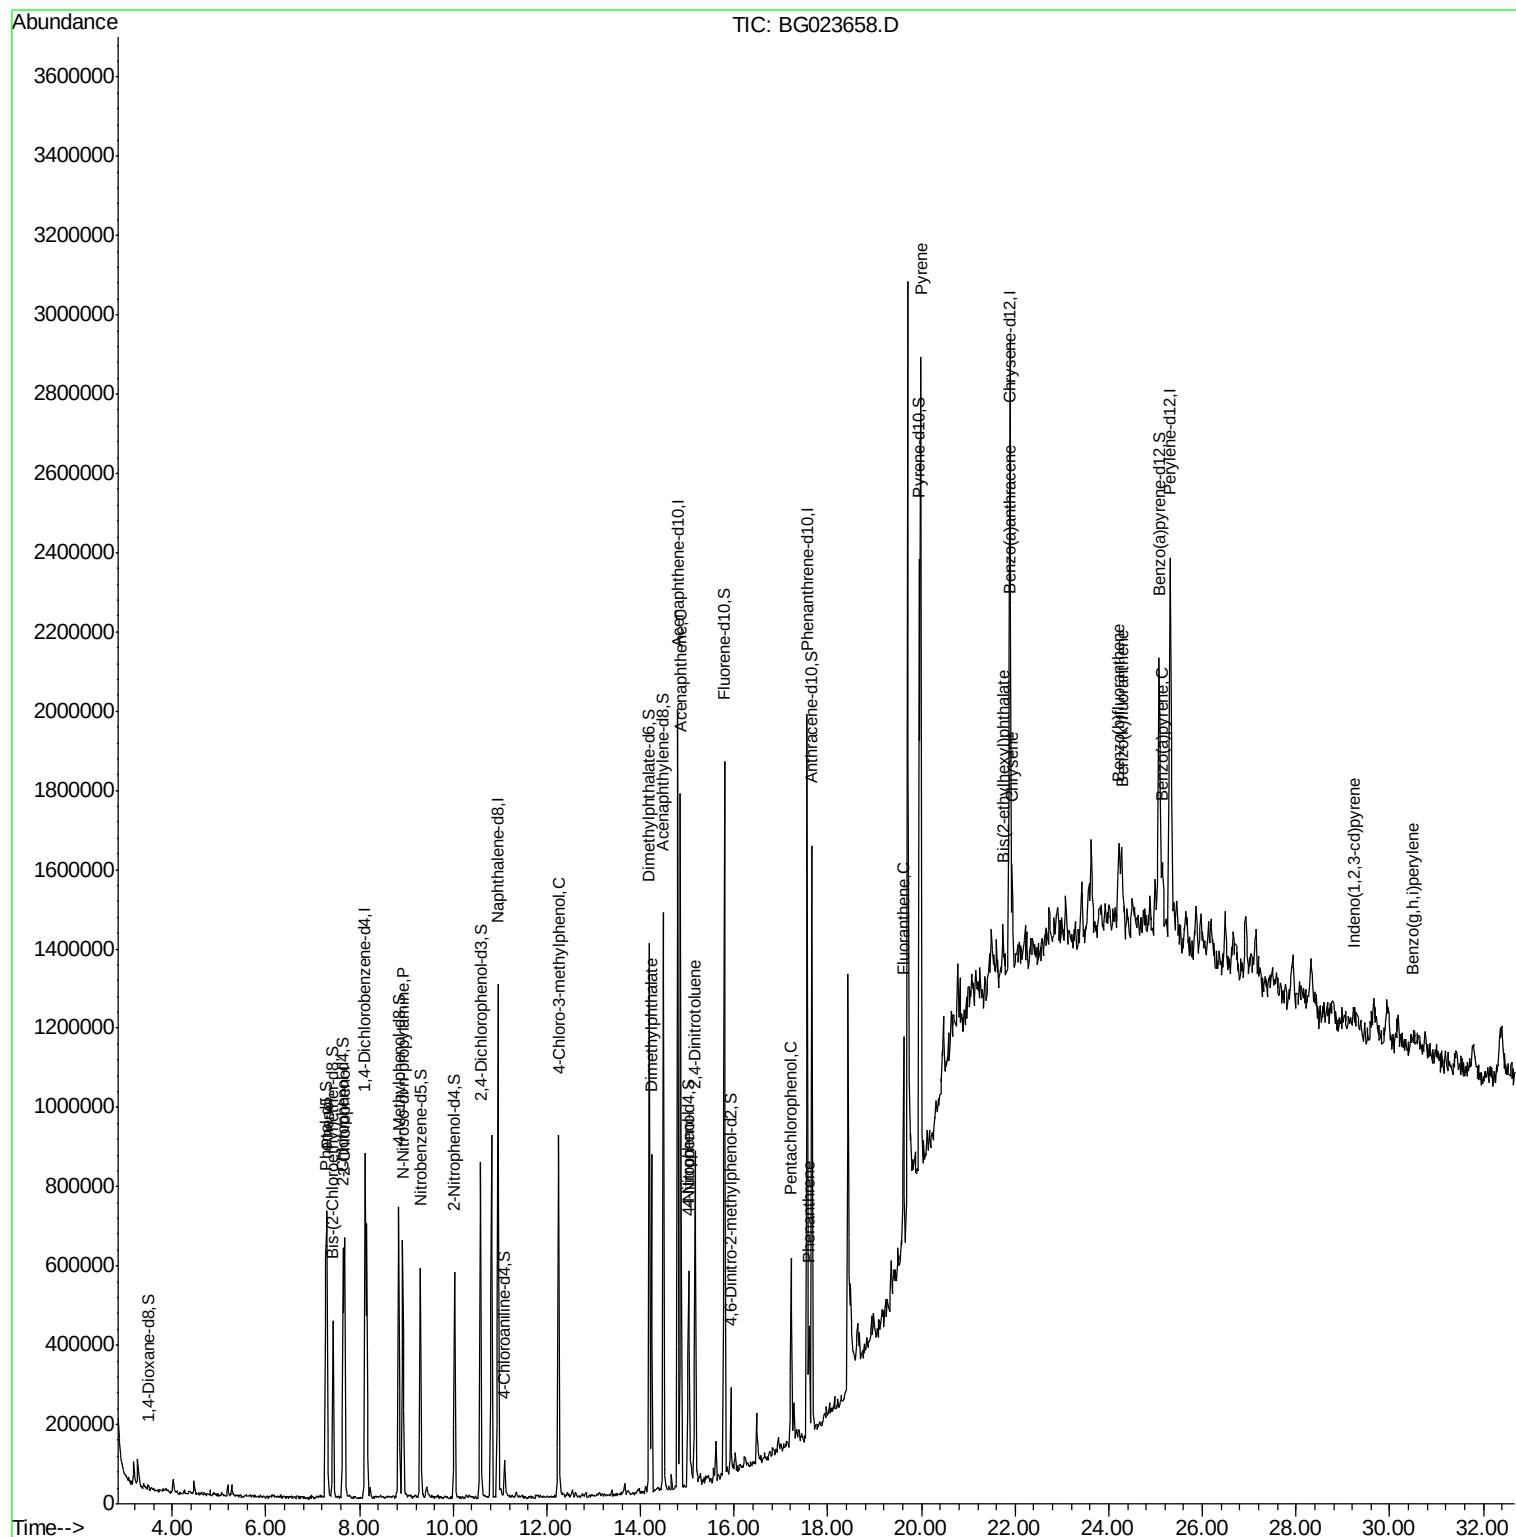

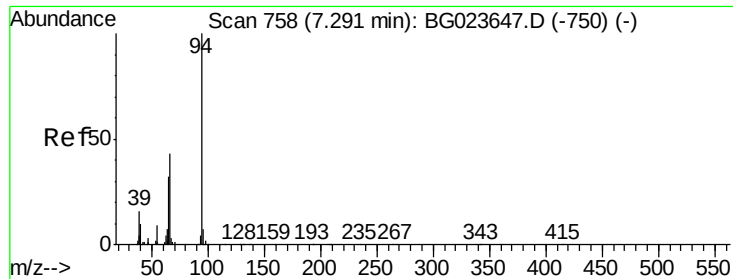

#6

Phenol

Concen: 16.46 ng/ul

RT: 7.30 min Scan# 760

Delta R.T. 0.01 min

Lab File: BG023658.D

Acq: 12 Aug 2016 16:13

Instrument :

BNA_G





ClientSampleId :

PR001-SS003-0206-01MSD

Tgt Ion:	94	Resp:	394632
Ion Ratio	Lower	Upper	
94	100		
65	31.8	16.8	25.2#
66	46.4	22.6	33.8#

Manual Integrations
APPROVED

sohil
8/15/2016 6:49:35 PM

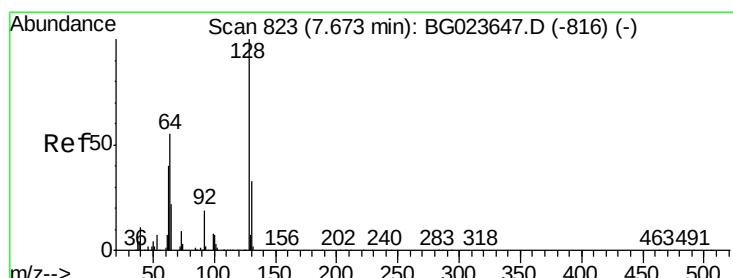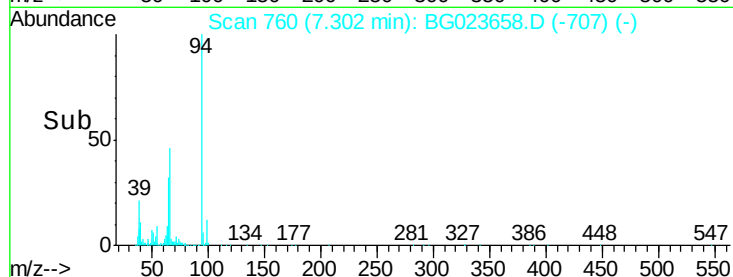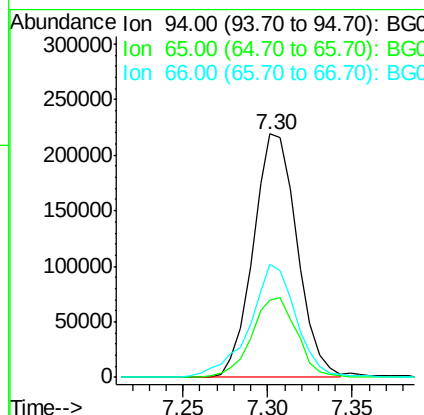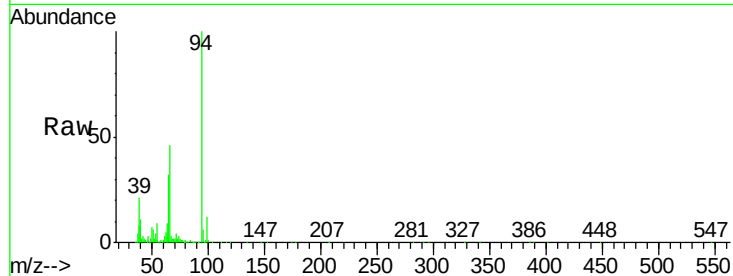

#10

2-Chlorophenol

Concen: 17.48 ng/ul




RT: 7.68 min Scan# 825




Delta R.T. 0.01 min

Lab File: BG023658.D

Acq: 12 Aug 2016 16:13

Tgt Ion:	128	Resp:	279705
Ion Ratio	Lower	Upper	
128	100		
64	59.5	34.2	51.4#
130	31.0	27.0	40.4

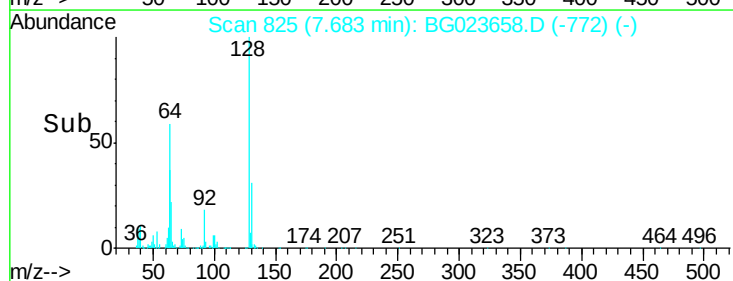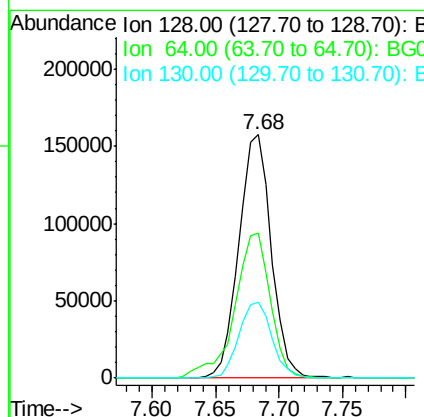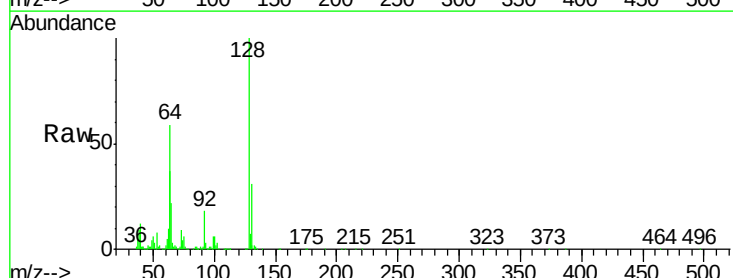

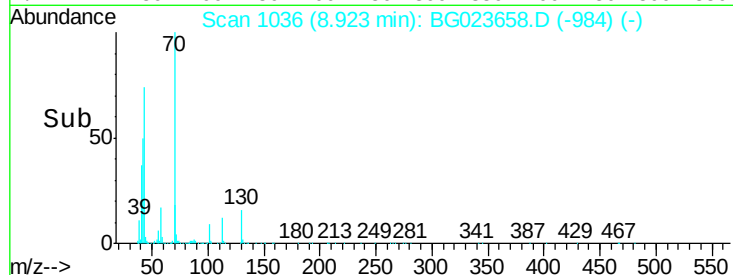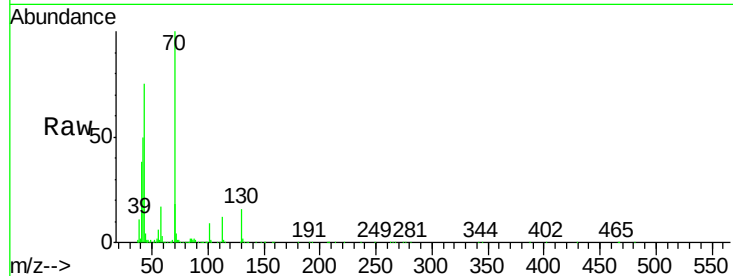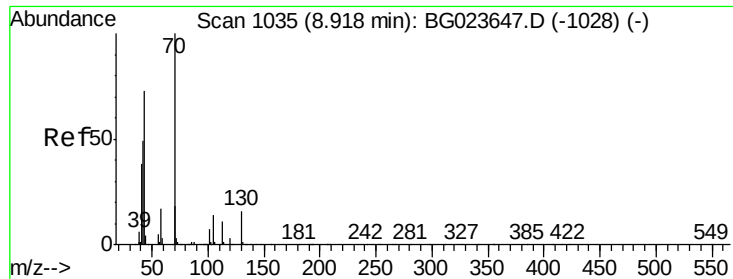





#15
N-Nitroso-di-n-propylamine
Concen: 15.97 ng/ul
RT: 8.92 min Scan# 1036
Delta R.T. 0.00 min
Lab File: BG023658.D
Acq: 12 Aug 2016 16:13

Instrument :
BNA_G
ClientSampleId :
PR001-SS003-0206-01MSD

Tgt Ion	Ratio	Lower	Upper
70	100		
42	49.8	31.4	47.2#
101	8.6	8.6	13.0#
130	16.0	19.0	28.4#


Manual Integrations
APPROVED


sohil
8/15/2016 6:49:35 PM

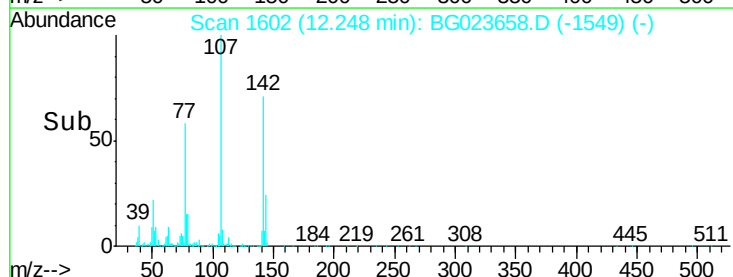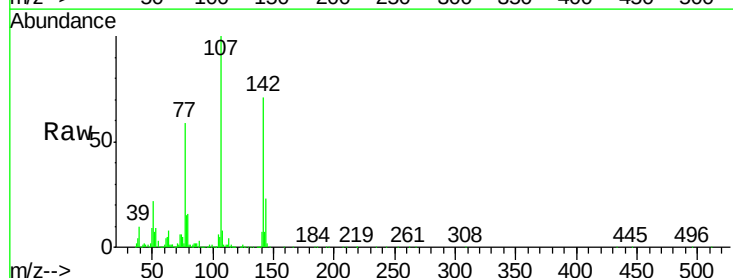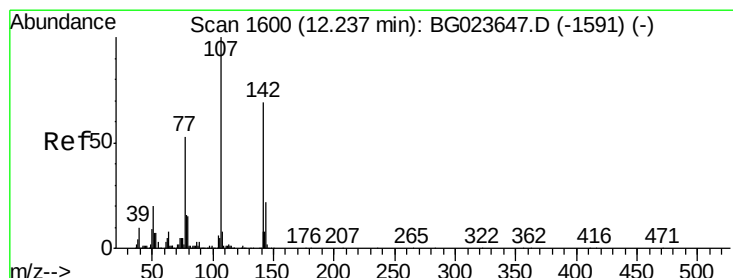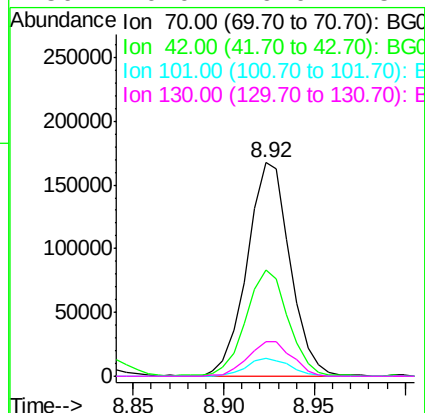

#33
4-Chloro-3-methylphenol
Concen: 14.88 ng/ul m
RT: 12.25 min Scan# 1602
Delta R.T. 0.01 min
Lab File: BG023658.D
Acq: 12 Aug 2016 16:13

Tgt Ion	Ratio	Lower	Upper
107	100		
144	23.5	22.7	34.1
142	70.6	71.6	107.4#

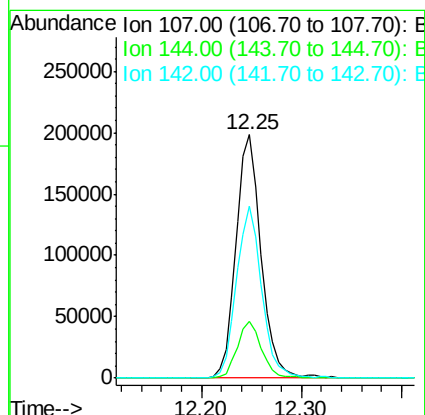

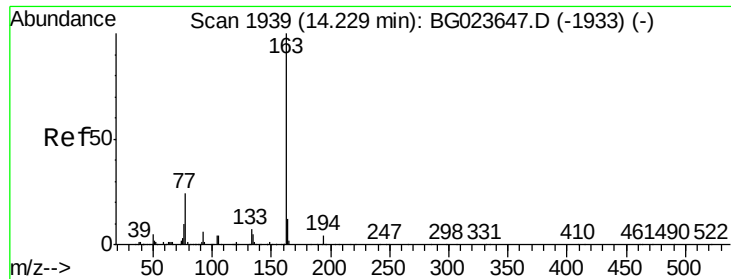





#44
Dimethylphthalate
Concen: 9.87 ng/ul
RT: 14.23 min Scan# 1940
Delta R.T. 0.00 min
Lab File: BG023658.D
Acq: 12 Aug 2016 16:13

Instrument :
BNA_G
ClientSampleId :
PR001-SS003-0206-01MSD

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.4	5.2
164	11.3	8.8	13.2




Manual Integrations
APPROVED


sohil
8/15/2016 6:49:35 PM

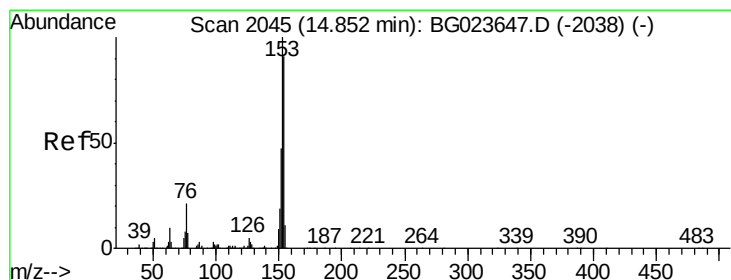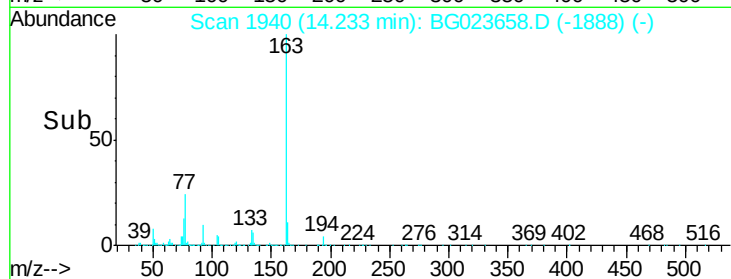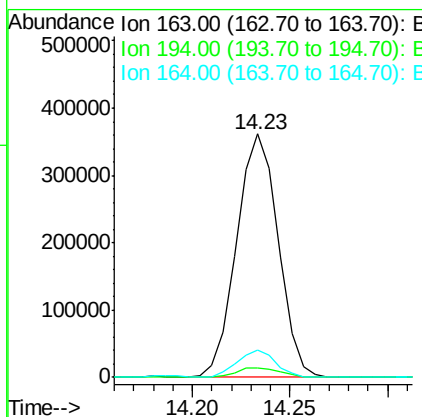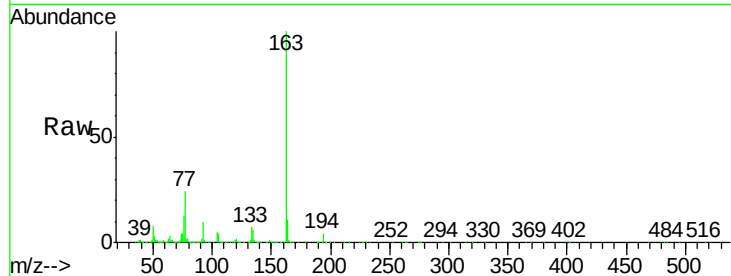

#49
Acenaphthene
Concen: 16.72 ng/ul
RT: 14.86 min Scan# 2046
Delta R.T. 0.00 min
Lab File: BG023658.D
Acq: 12 Aug 2016 16:13

Tgt Ion	Ratio	Lower	Upper
153	100		
152	49.5	37.3	55.9
154	91.8	68.2	102.2

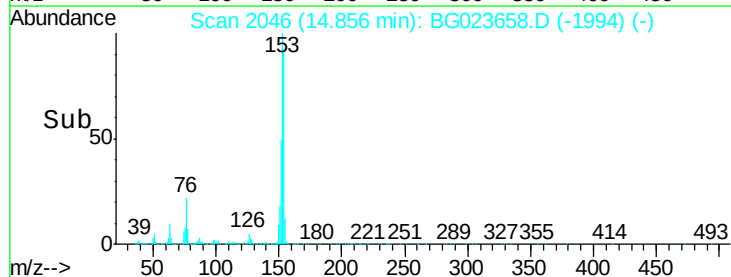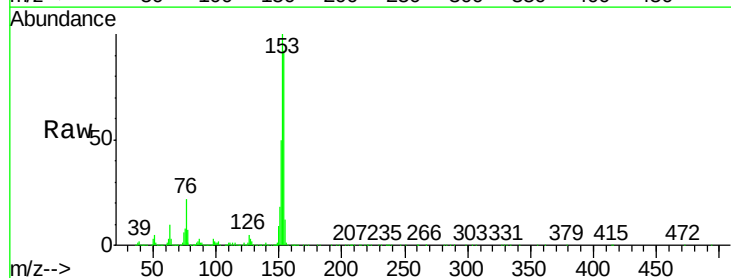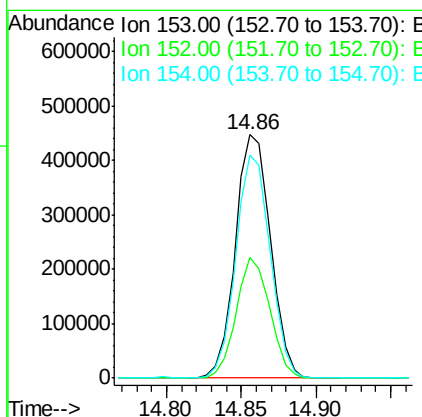

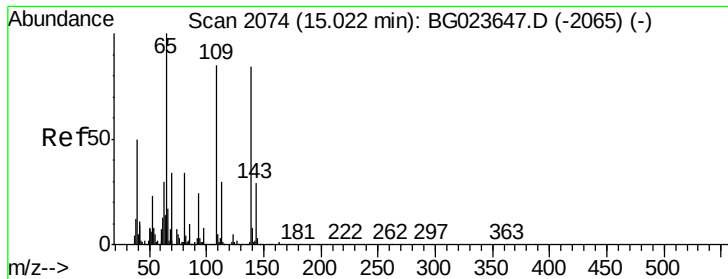

#52

4-Nitrophenol

Concen: 9.89 ng/ul m

RT: 15.03 min Scan# 2075

Delta R.T. 0.00 min

Lab File: BG023658.D


Acq: 12 Aug 2016 16:13

Instrument :

BNA_G

ClientSampleId :




PR001-SS003-0206-01MSD

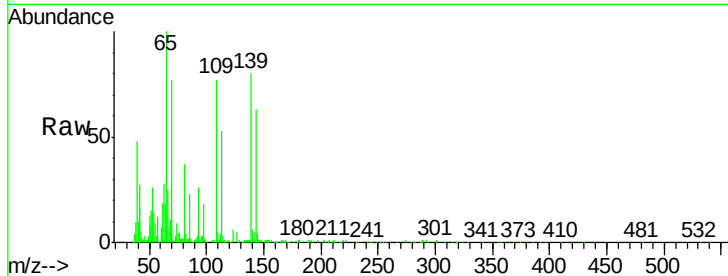

Tgt Ion:	109	Resp:	92148
Ion Ratio	Lower	Upper	
109	100		
139	102.7	136.1	204.1#
65	129.1	106.0	159.0

Manual Integrations
APPROVED

sohil
8/15/2016 6:49:35 PM

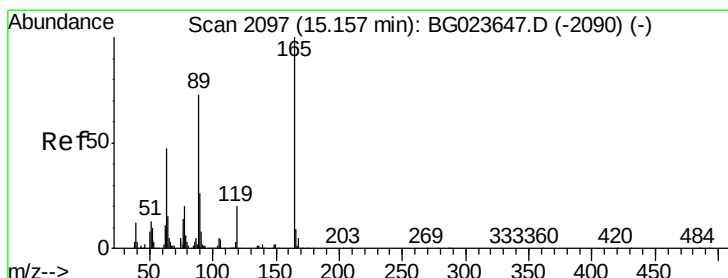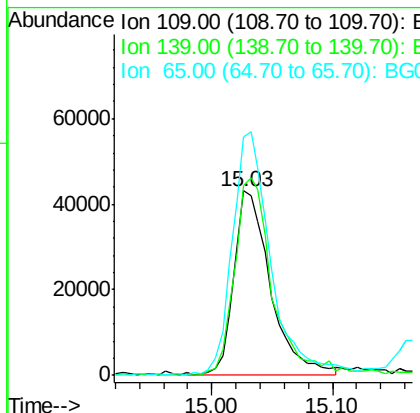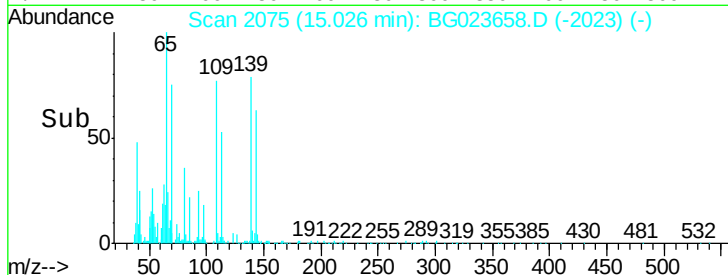

#54

2,4-Dinitrotoluene


Concen: 13.30 ng/ul

RT: 15.17 min Scan# 2099



Delta R.T. 0.01 min


Lab File: BG023658.D

Acq: 12 Aug 2016 16:13

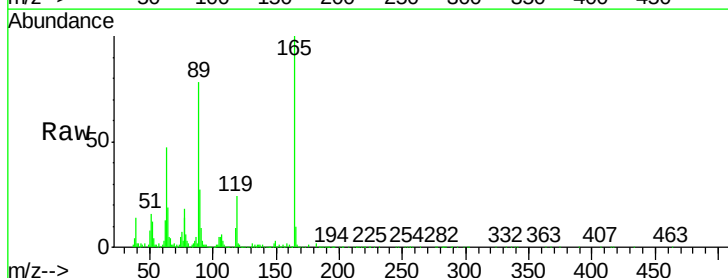

Tgt Ion:	165	Resp:	235685
Ion Ratio	Lower	Upper	
165	100		
63	46.8	25.7	38.5#
182	2.1	2.1	3.1#

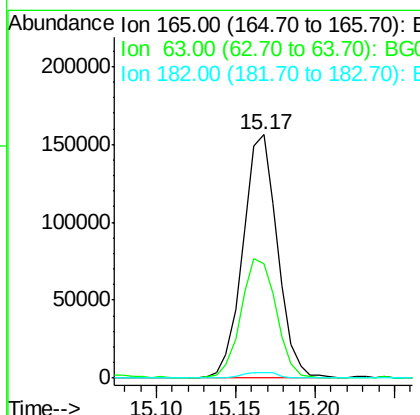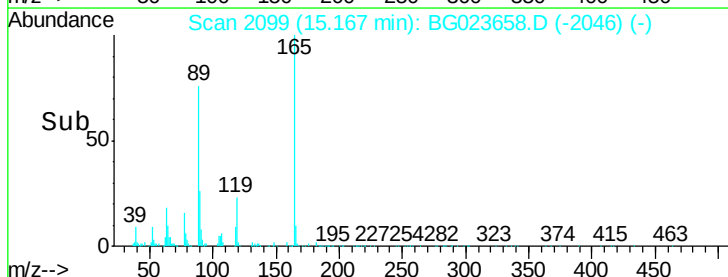

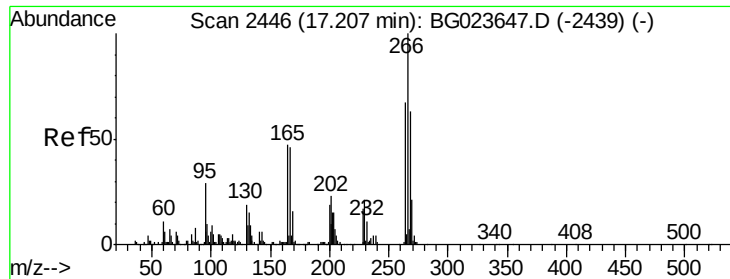


#68
 Pentachlorophenol
 Concen: 12.96 ng/ul
 RT: 17.22 min Scan# 2448
 Delta R.T. 0.01 min
 Lab File: BG023658.D
 Acq: 12 Aug 2016 16:13

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS003-0206-01MSD

Tgt Ion	Ratio	Lower	Upper
266	100		
264	58.5	54.7	82.1
268	60.9	57.8	86.8

Manual Integrations
 APPROVED

sohil
 8/15/2016 6:49:35 PM



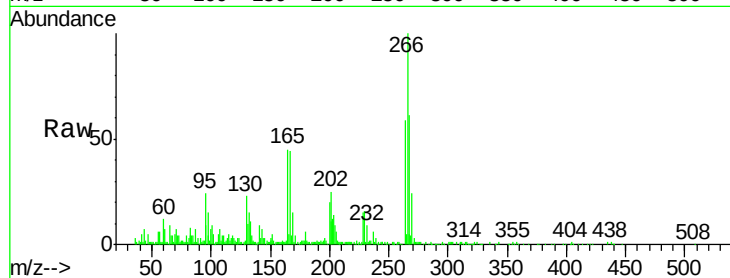


Abundance

Ion 265.70 (265.40 to 266.40): E


Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

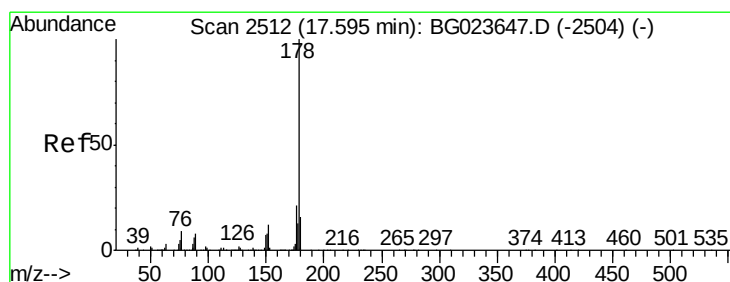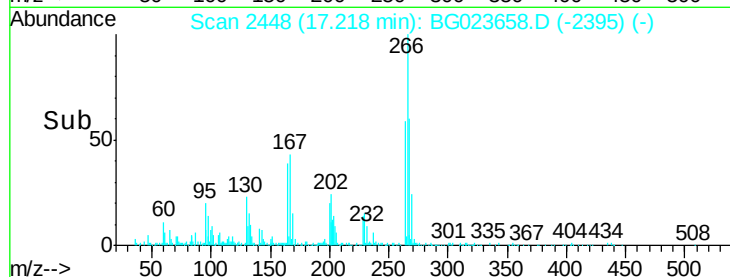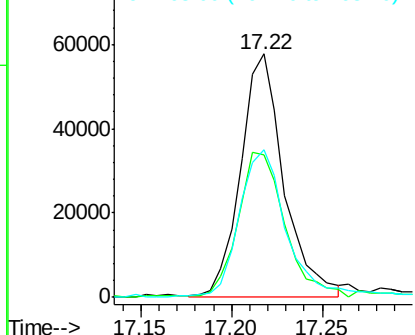

#69
 Phenanthrene
 Concen: 3.08 ng/ul
 RT: 17.60 min Scan# 2513
 Delta R.T. 0.00 min
 Lab File: BG023658.D
 Acq: 12 Aug 2016 16:13

Tgt Ion	Ratio	Lower	Upper
178	100		
179	14.8	12.9	19.3
176	18.0	15.8	23.8


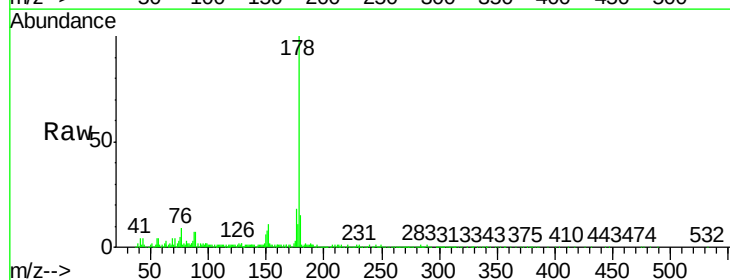



Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

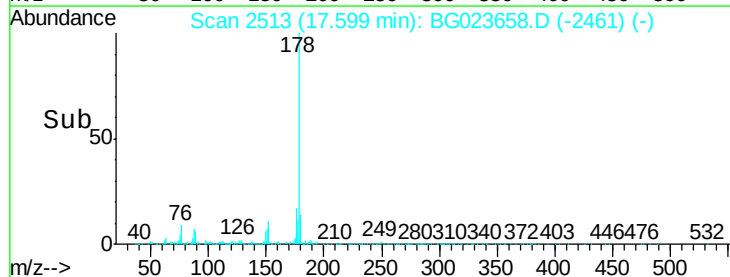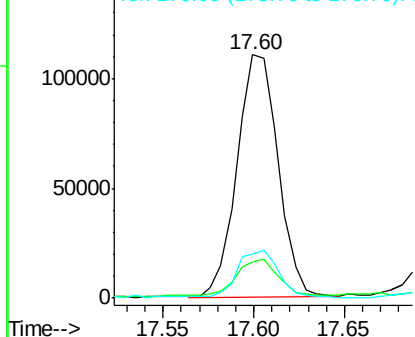

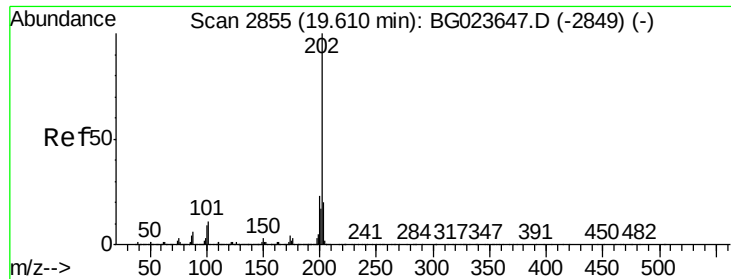





#74
Fluoranthene
Concen: 5.35 ng/ul
RT: 19.62 min Scan# 2857
Delta R.T. 0.01 min
Lab File: BG023658.D
Acq: 12 Aug 2016 16:13

Instrument :
BNA_G
ClientSampleId :
PR001-SS003-0206-01MSD

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	9.8	10.6	16.0#
100	7.0	8.7	13.1#




Manual Integrations
APPROVED


sohil
8/15/2016 6:49:35 PM

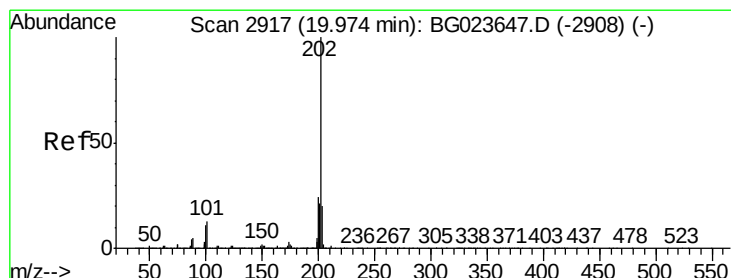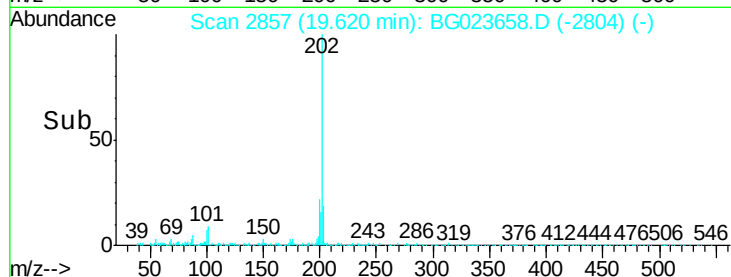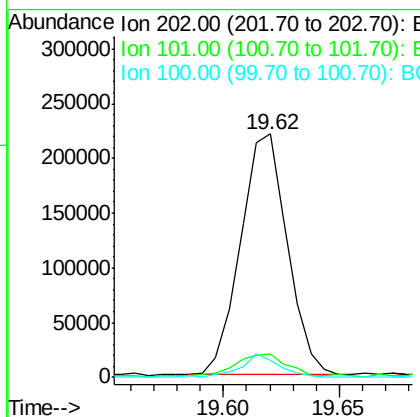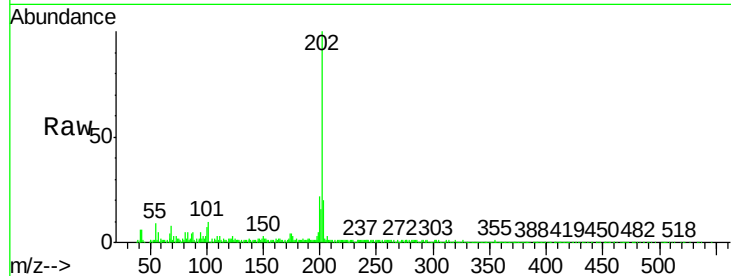

#77
Pyrene
Concen: 20.34 ng/ul
RT: 19.98 min Scan# 2919
Delta R.T. 0.01 min
Lab File: BG023658.D
Acq: 12 Aug 2016 16:13

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	11.5	12.5	18.7#
100	10.5	10.2	15.4

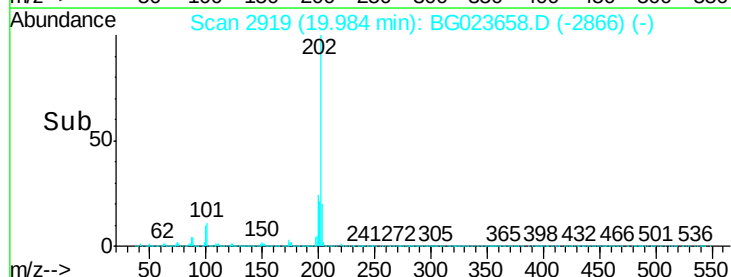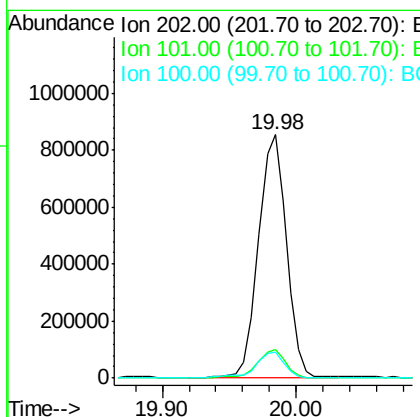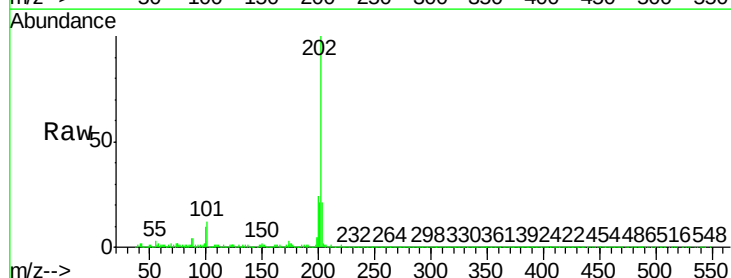

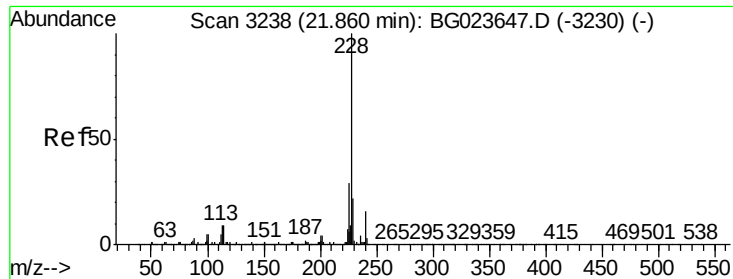

#80

Benzo(a)anthracene

Concen: 2.69 ng/ul

RT: 21.86 min Scan# 3239

Delta R.T. 0.00 min

Lab File: BG023658.D

Acq: 12 Aug 2016 16:13

Instrument :

BNA_G





ClientSampleId :

PR001-SS003-0206-01MSD

Tgt Ion:	228	Resp:	147657
Ion Ratio		Lower	Upper
228	100		
229	26.7	15.4	23.2#
226	29.6	22.8	34.2

Manual Integrations
APPROVED

sohil
8/15/2016 6:49:35 PM

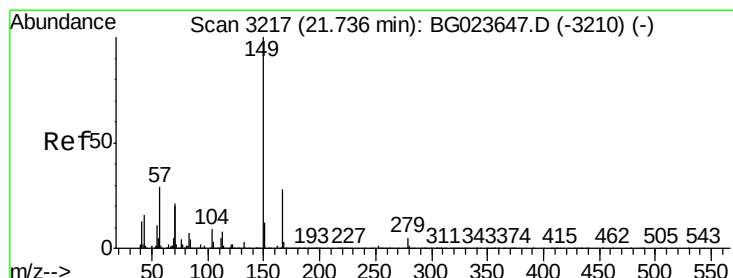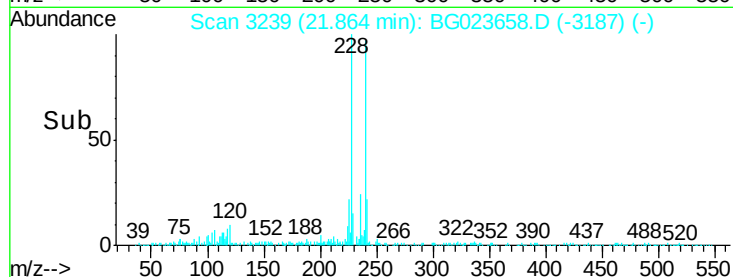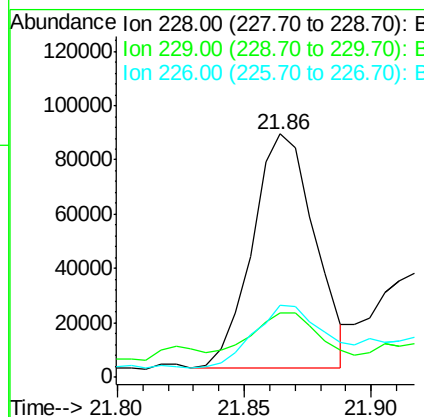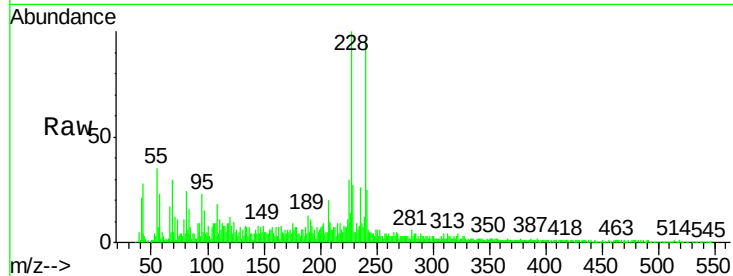

#81

Bis(2-ethylhexyl)phthalate

Concen: 1.28 ng/ul




RT: 21.74 min Scan# 3218


Delta R.T. 0.00 min

Lab File: BG023658.D

Acq: 12 Aug 2016 16:13

Tgt Ion:	149	Resp:	39223
Ion Ratio		Lower	Upper
149	100		
167	40.1	21.9	32.9#
279	11.9	2.9	4.3#

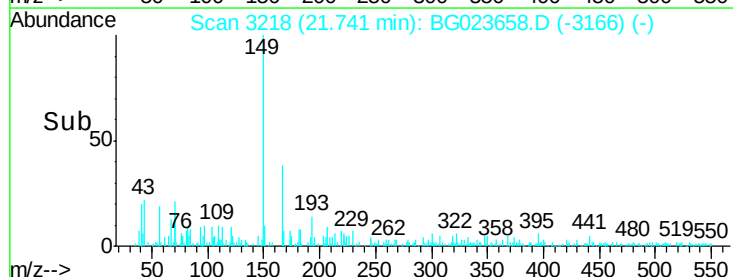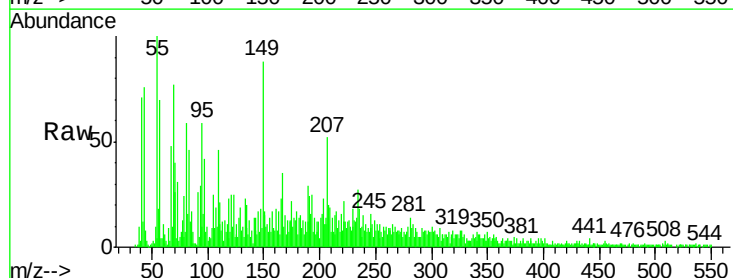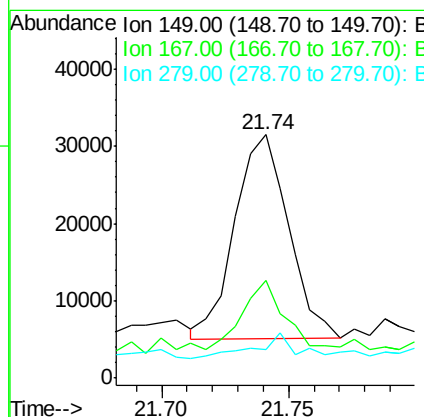

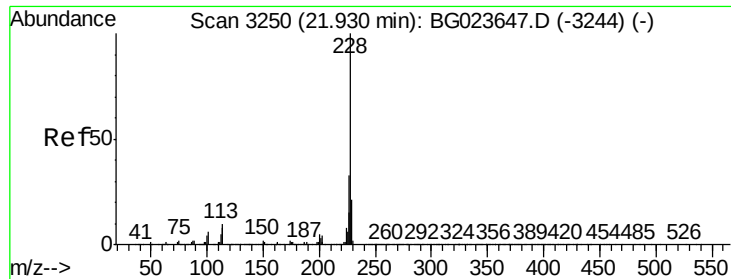

#82

Chrysene

Concen: 3.63 ng/ul

RT: 21.93 min Scan# 3251

Delta R.T. 0.00 min

Lab File: BG023658.D

Acq: 12 Aug 2016 16:13

Instrument :

BNA_G





ClientSampleId :

PR001-SS003-0206-01MSD

Tgt Ion:	228	Resp:	180834
Ion Ratio	Lower	Upper	
228	100		
226	34.9	24.2	36.4
229	23.1	15.0	22.6#

Manual Integrations
APPROVED

sohil
8/15/2016 6:49:35 PM

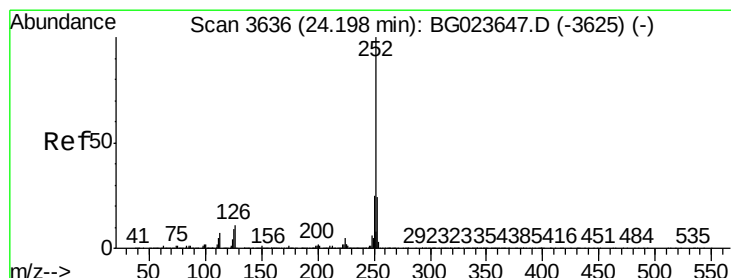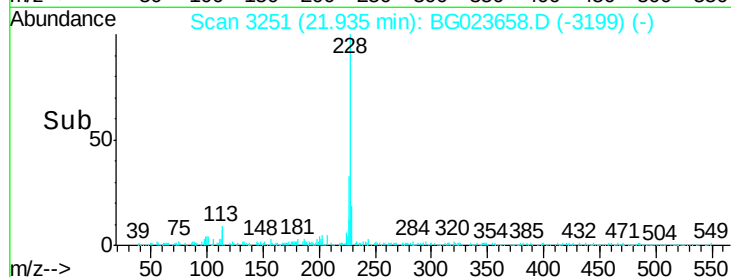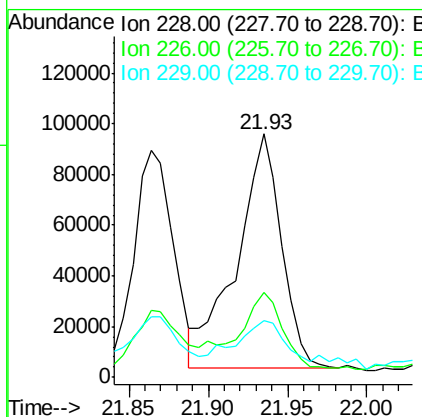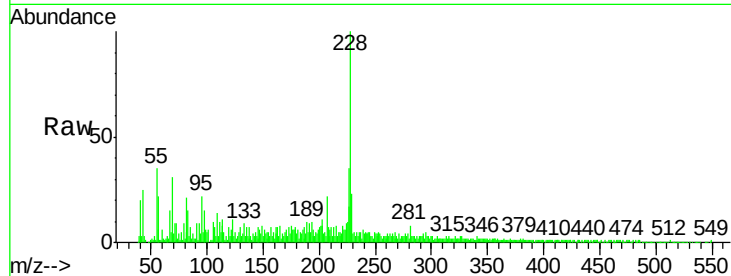

#85

Benzo(b)fluoranthene

Concen: 4.19 ng/ul




RT: 24.22 min Scan# 3640


Delta R.T. 0.02 min

Lab File: BG023658.D

Acq: 12 Aug 2016 16:13

Tgt Ion:	252	Resp:	238603
Ion Ratio	Lower	Upper	
252	100		
253	41.5	18.2	27.2#
125	13.9	10.8	16.2

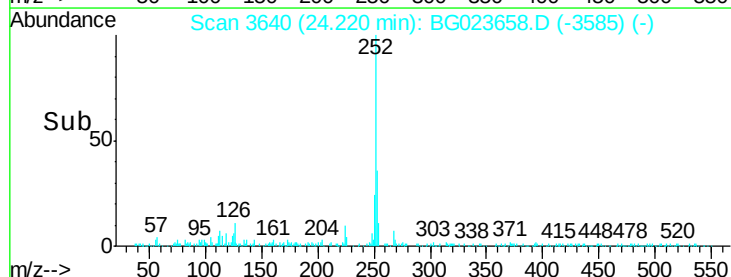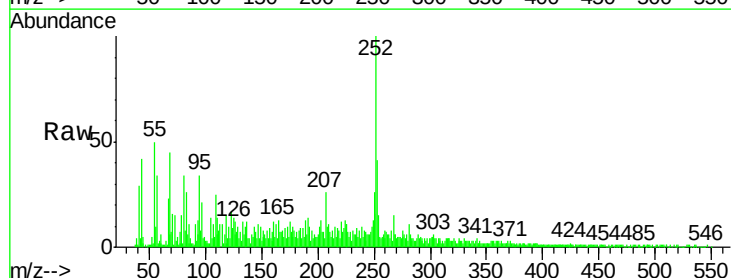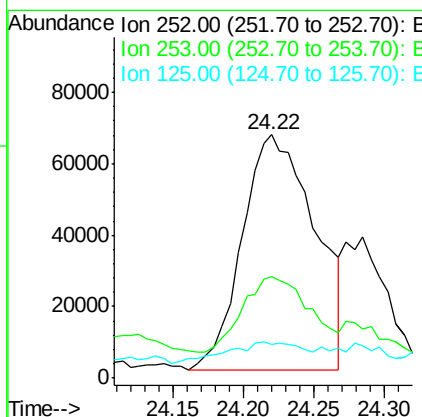

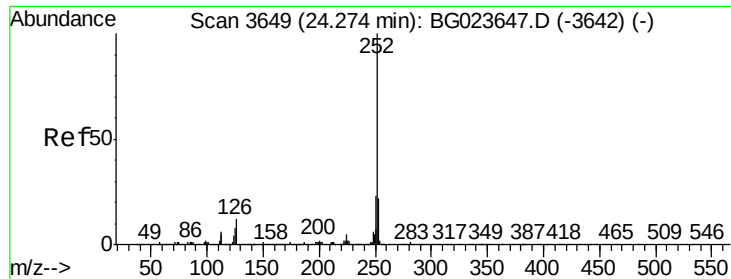





#86
Benzo(k)fluoranthene
Concen: 1.48 ng/ul m
RT: 24.28 min Scan# 3651
Delta R.T. 0.01 min
Lab File: BG023658.D
Acq: 12 Aug 2016 16:13

Instrument :
BNA_G
ClientSampleId :
PR001-SS003-0206-01MSD

Tgt Ion	Ratio	Lower	Upper
252	100		
253	34.7	15.8	23.6#
125	22.6	10.6	16.0#




Manual Integrations
APPROVED


sohil
8/15/2016 6:49:35 PM

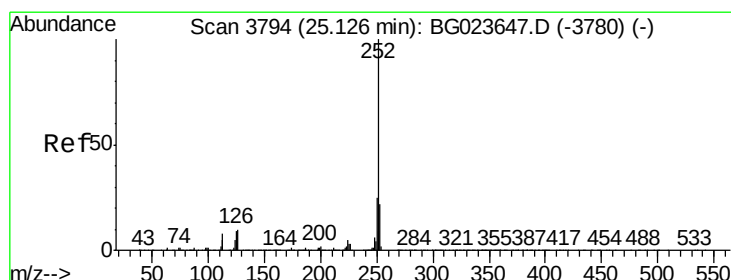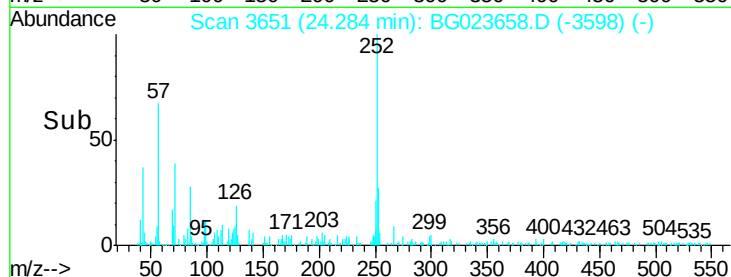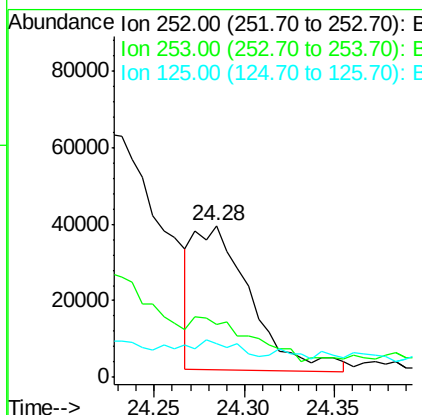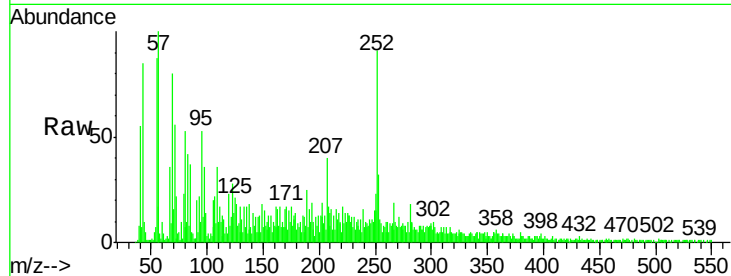

#88
Benzo(a)pyrene
Concen: 2.87 ng/ul
RT: 25.14 min Scan# 3797
Delta R.T. 0.02 min
Lab File: BG023658.D
Acq: 12 Aug 2016 16:13

Tgt Ion	Ratio	Lower	Upper
252	100		
253	29.5	19.0	28.4#
125	18.0	12.0	18.0#

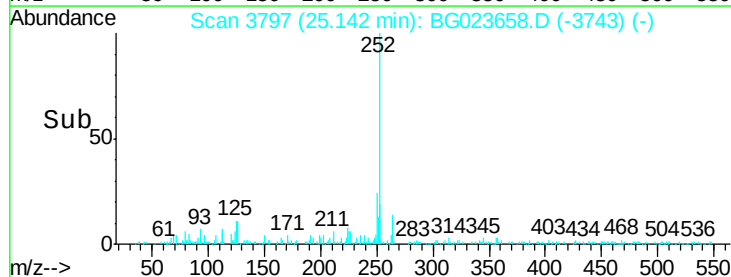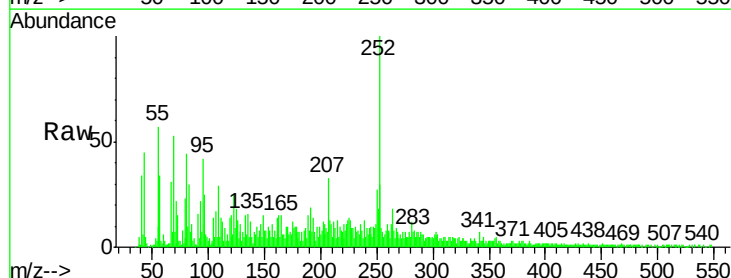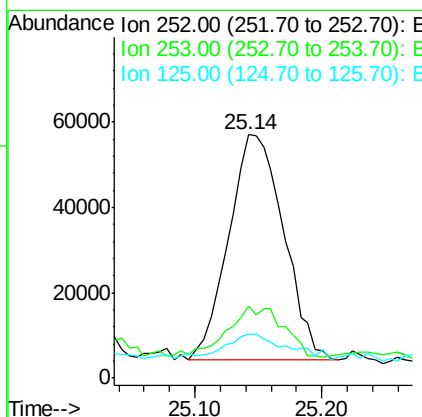

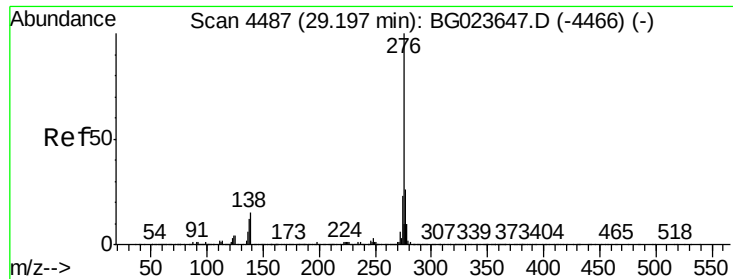





#89
 Indeno(1,2,3-cd)pyrene
 Concen: 1.50 ng/ul m
 RT: 29.24 min Scan# 4495
 Delta R.T. 0.05 min
 Lab File: BG023658.D
 Acq: 12 Aug 2016 16:13

Instrument :
 BNA_G
 ClientSampleId :
 PR001-SS003-0206-01MSD

Tgt Ion	Ratio	Lower	Upper
276	100		
138	22.7	20.8	31.2
277	37.1	17.6	26.4

Manual Integrations
 APPROVED

sohil
 8/15/2016 6:49:35 PM

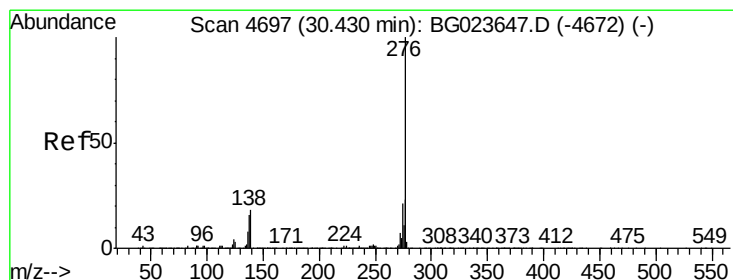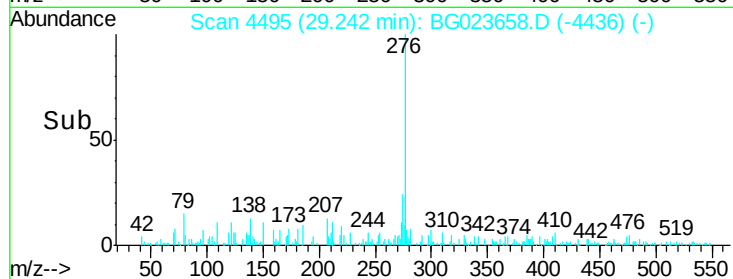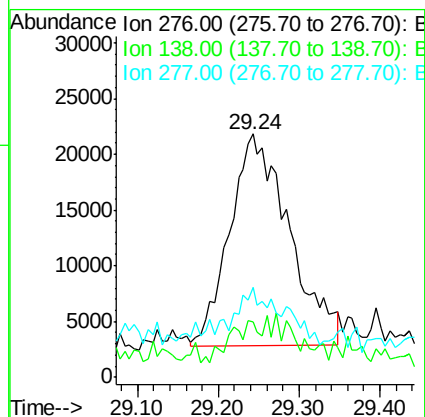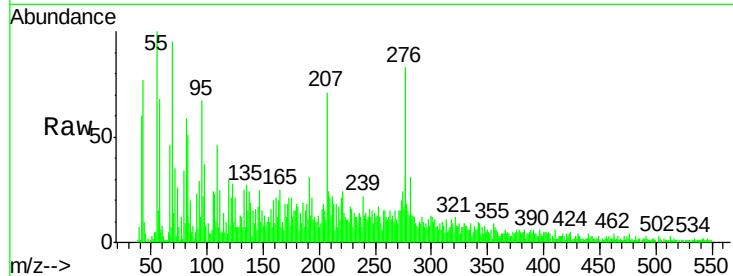

#91
 Benzo(g,h,i)perylene
 Concen: 1.75 ng/ul m
 RT: 30.49 min Scan# 4708
 Delta R.T. 0.06 min
 Lab File: BG023658.D
 Acq: 12 Aug 2016 16:13

Tgt Ion	Ratio	Lower	Upper
276	100		
138	16.6	22.1	33.1
277	34.5	17.0	25.4

