

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081220\
 Data File : BG046228.D
 Acq On : 12 Aug 2020 12:57
 Operator : CG/JU
 Sample : L3612-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBFN9

Quant Time: Aug 12 13:39:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG072320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 12 13:12:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.95	152	99289	20.00	ng/ul	0.00
18) Naphthalene-d8	10.74	136	381162	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.58	164	248568	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.31	188	584104	20.00	ng/ul	0.00
78) Chrysene-d12	21.56	240	630280	20.00	ng/ul	0.00
86) Perylene-d12	24.67	264	678247	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.42	96	9423	4.69	ng/uL	0.00
5) Phenol-d5	7.11	99	206596	26.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.28	67	124719	25.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.48	132	168874	27.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	170381	25.92	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	83678	31.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	96749	35.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.37	165	182651	29.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.87	131	228636	32.61	ng/ul	0.00
44) Dimethylphthalate-d6	13.98	166	607684	31.35	ng/ul	0.00
47) Acenaphthylene-d8	14.26	160	727066	31.60	ng/ul	0.00
52) 4-Nitrophenol-d4	14.76	143	87553	27.65	ng/ul	0.00
58) Fluorene-d10	15.57	176	548473	31.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.67	200	92527	31.65	ng/ul	0.00
71) Anthracene-d10	17.41	188	850977	31.59	ng/ul	0.00
79) Pyrene-d10	19.70	212	1007604	30.23	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.46	264	1164856	30.99	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	14.03	163	140207	7.211	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081220\
Data File : BG046228.D
Acq On : 12 Aug 2020 12:57
Operator : CG/JU
Sample : L3612-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBFN9

Quant Time: Aug 12 13:39:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG072320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 12 13:12:31 2020
Response via : Initial Calibration

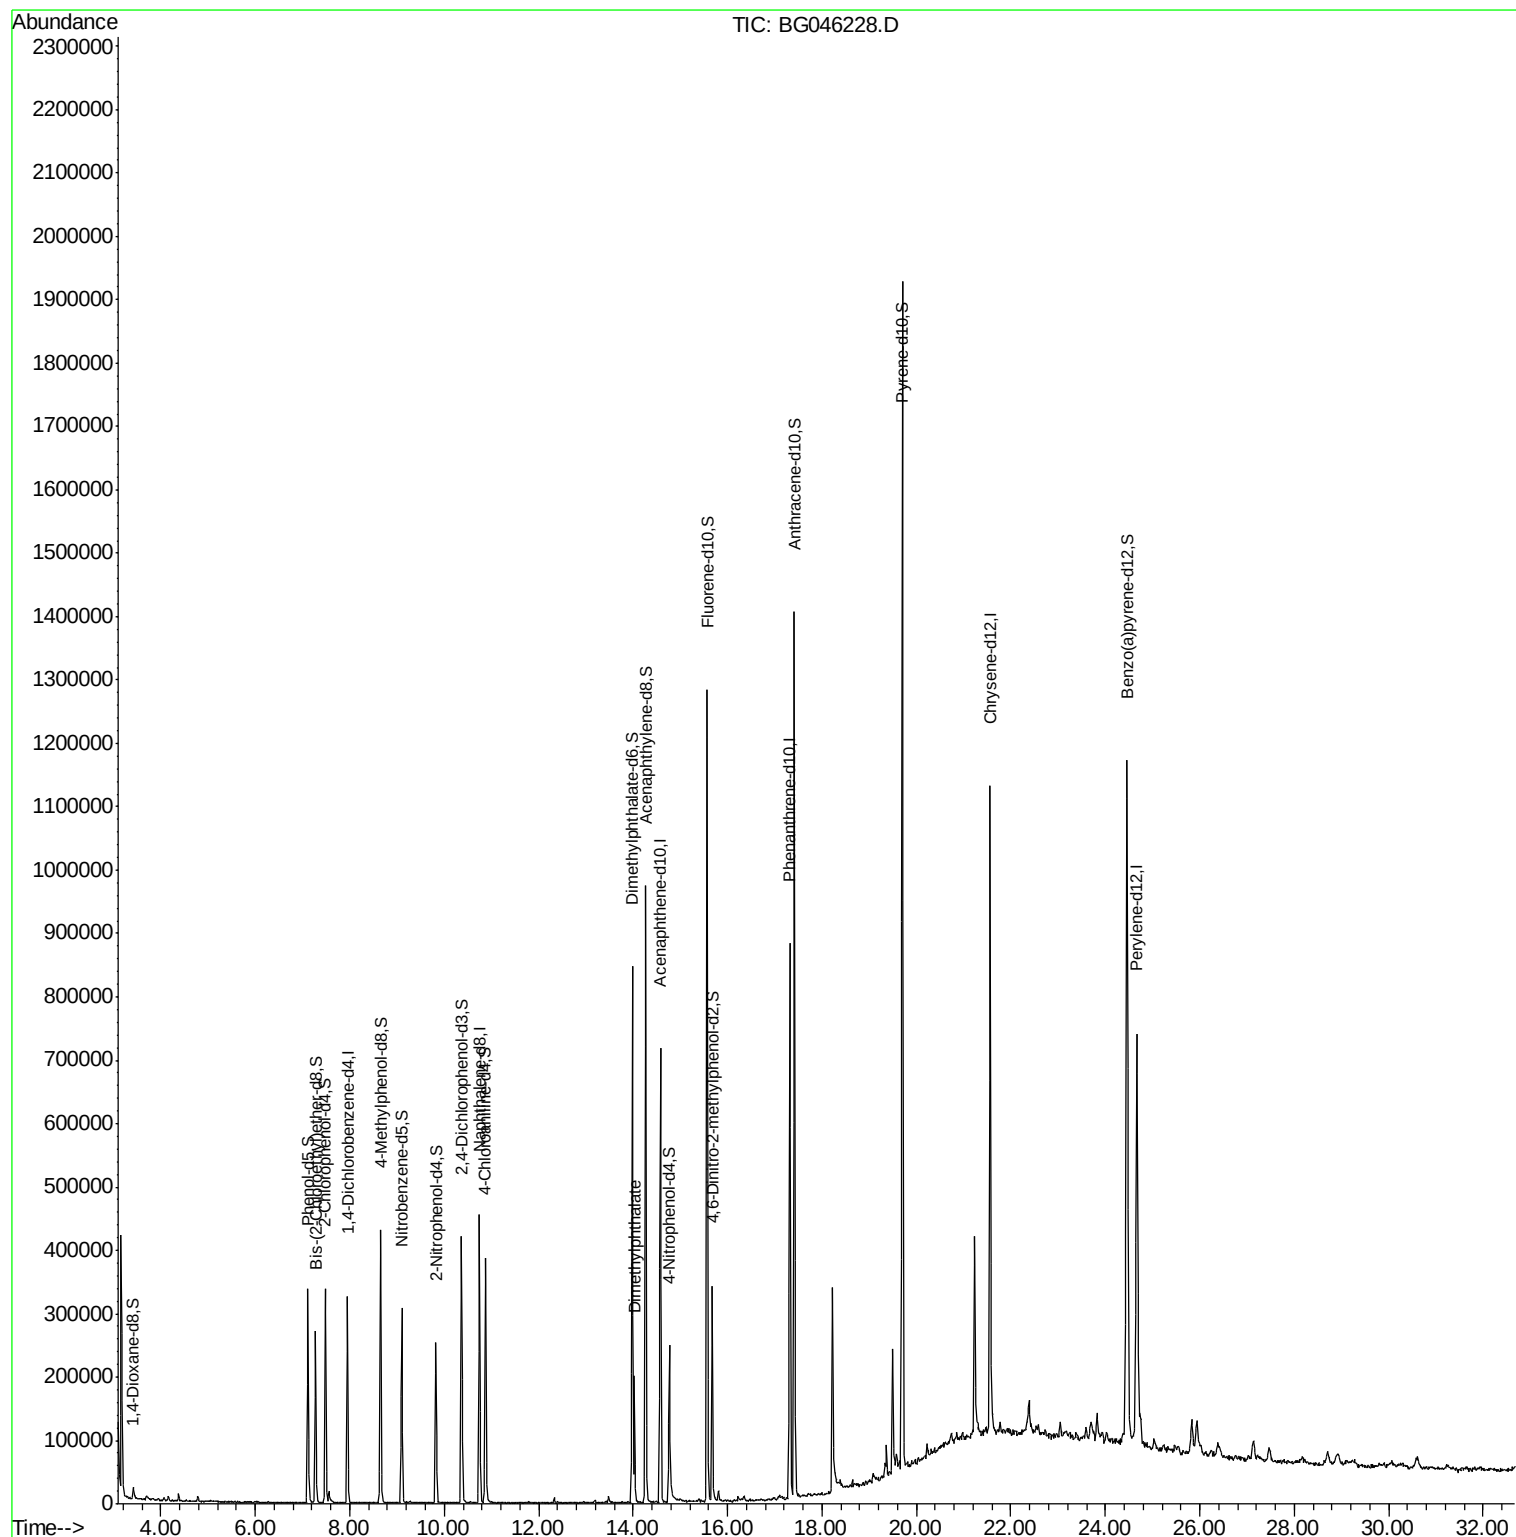

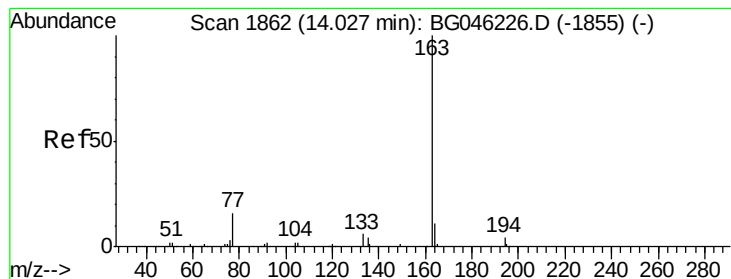

#45

Dimethylphthalate

Concen: 7.211 ng/ul

RT: 14.03 min Scan# 1862

Delta R.T. 0.00 min

Lab File: BG046228.D

Acq: 12 Aug 2020 12:57

Instrument :

BNA_G

ClientSampleId :

DBFN9


Tot Ion:163 Resp: 140207

Ion Ratio Lower Upper

163 100

194 4.8 3.4 5.0

164 10.2 8.7 13.1

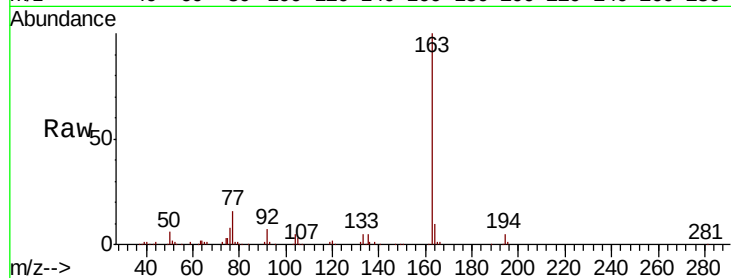

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

