
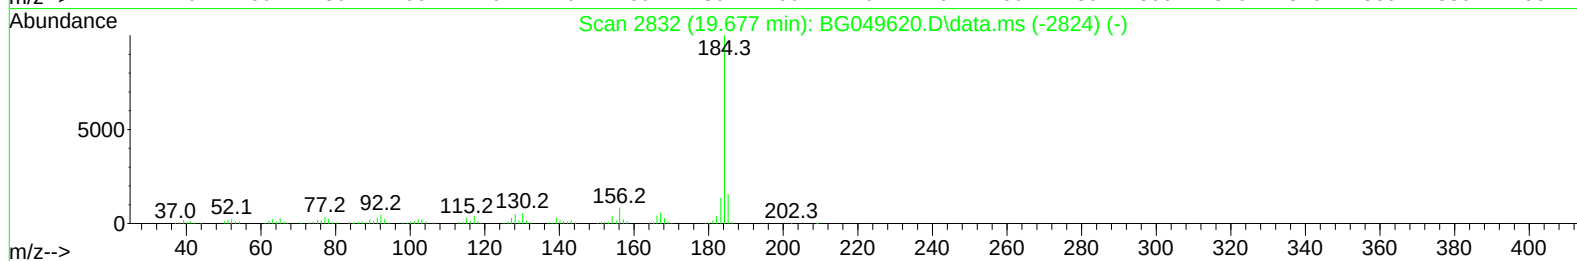
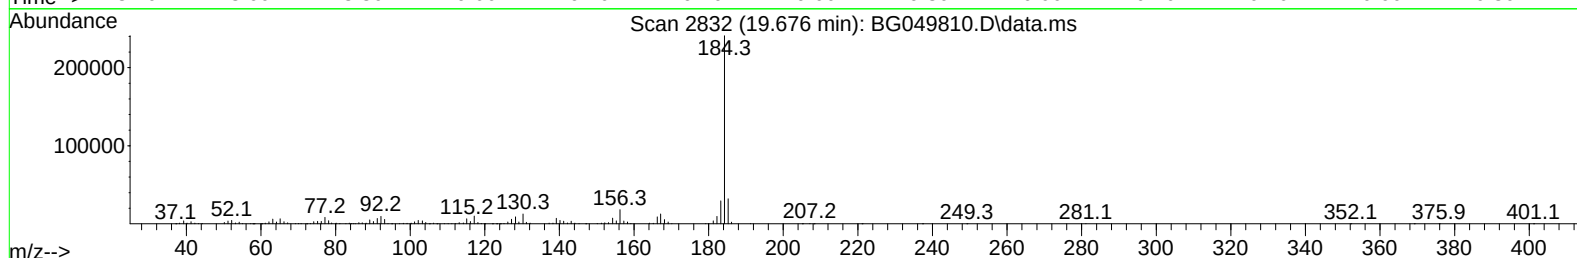


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
Data File : BG049810.D
Acq On : 12 Aug 2021 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 11:13:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

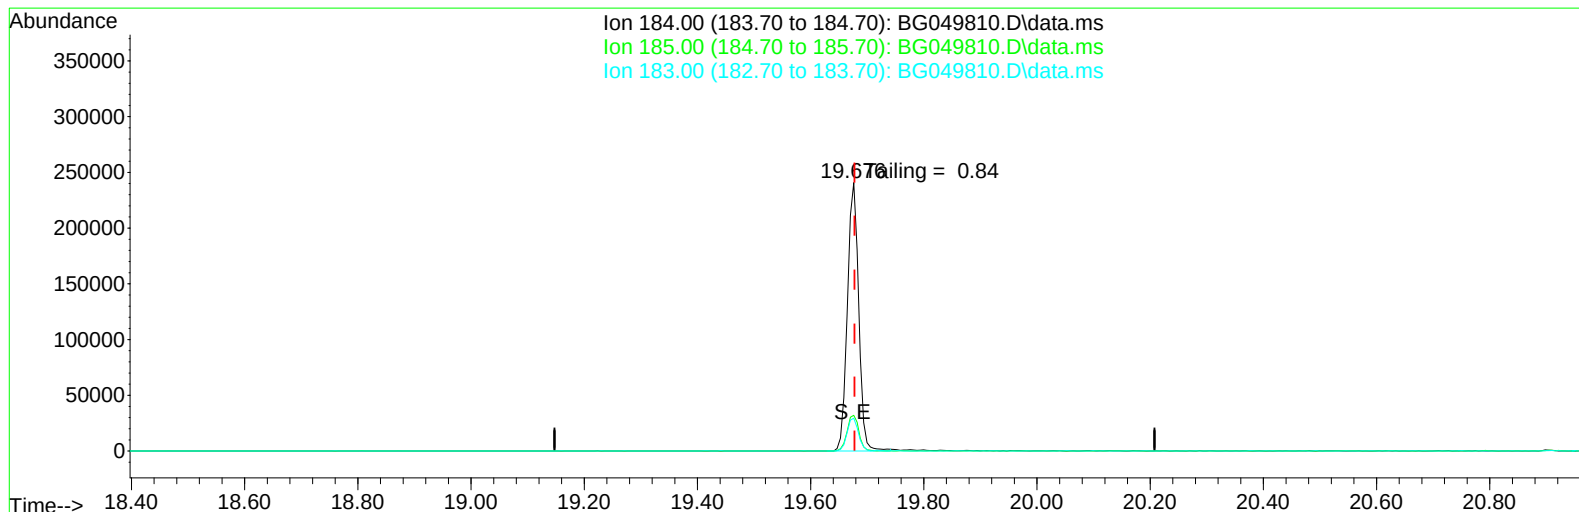




TIC: BG049810.D\data.ms

(77) Benzidine**19.676min (-0.001) 16477.22 ng****response 332679**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.33
183.00	11.70	12.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
Data File : BG049810.D
Acq On : 12 Aug 2021 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 11:13:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

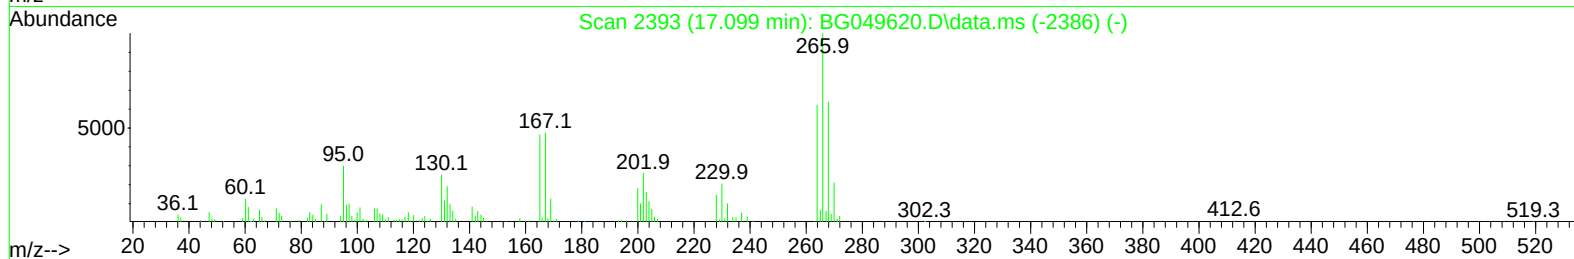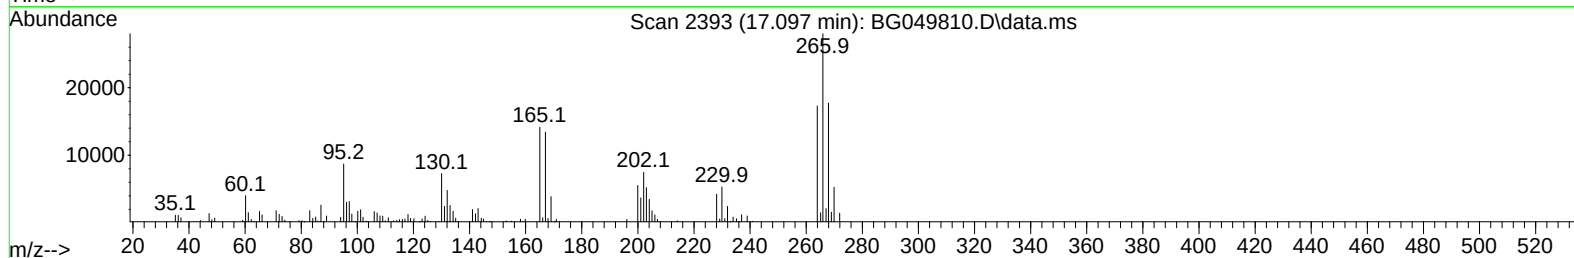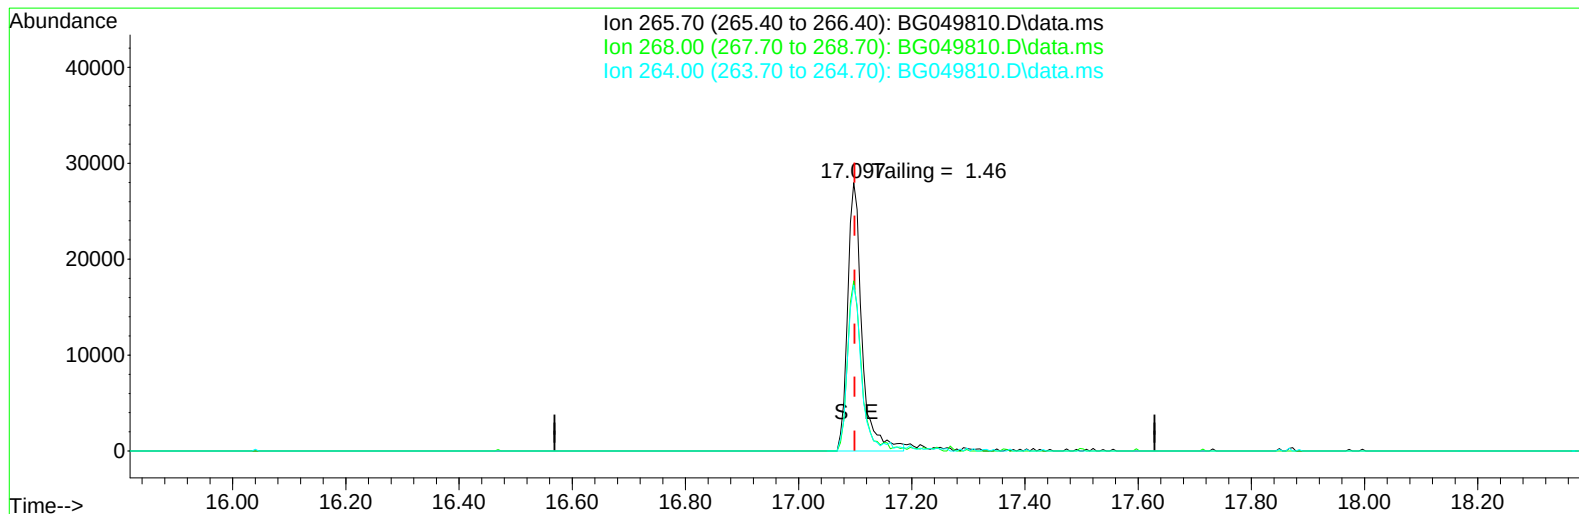

TIC: BG049810.D\data.ms

(70) Pentachlorophenol (C)

17.097min (-0.001) 13934.76 ng

response 49960

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.38
264.00	61.30	61.84
0.00	0.00	0.00