

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
 Data File : BG049818.D
 Acq On : 12 Aug 2021 15:04
 Operator : CG/JU
 Sample : M3335-01 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OR-02-080921

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.137	13	17	23	rVB2	10119	17839	3.26%	0.365%
2	5.111	349	353	357	rBV4	4193	6999	1.28%	0.143%
3	5.587	428	434	442	rBV2	78148	131497	24.06%	2.689%
4	7.197	701	708	717	rBV	84868	157008	28.72%	3.210%
5	8.031	843	850	861	rVB	126939	221786	40.57%	4.535%
6	9.206	1040	1050	1057	rBV	54019	102494	18.75%	2.096%
7	10.856	1321	1331	1340	rBV2	179424	336931	61.64%	6.889%
8	13.306	1741	1748	1757	rVB	145807	237157	43.39%	4.849%
9	14.005	1862	1867	1873	rBV4	3667	6861	1.26%	0.140%
10	14.686	1976	1983	1990	rVV	307643	475540	87.00%	9.723%
11	14.751	1990	1994	1999	rVB6	6024	11214	2.05%	0.229%
12	15.080	2049	2050	2057	rVB6	5782	7871	1.44%	0.161%
13	15.162	2059	2064	2068	rBV3	4044	6732	1.23%	0.138%
14	15.309	2085	2089	2094	rBV4	5033	7761	1.42%	0.159%
15	15.521	2121	2125	2130	rVB4	6660	9080	1.66%	0.186%
16	15.738	2155	2162	2165	rBV5	10533	18644	3.41%	0.381%
17	16.179	2230	2237	2243	rBV2	128426	197101	36.06%	4.030%
18	16.384	2266	2272	2274	rBV4	7088	11233	2.06%	0.230%
19	16.408	2274	2276	2280	rVB3	7780	8209	1.50%	0.168%
20	16.901	2353	2360	2361	rBV4	4571	7417	1.36%	0.152%
21	17.095	2389	2393	2397	rVB6	4540	6542	1.20%	0.134%
22	17.177	2403	2407	2412	rVV4	8840	11098	2.03%	0.227%
23	17.236	2412	2417	2419	rVV5	7387	13497	2.47%	0.276%
24	17.254	2419	2420	2428	rVB3	7690	12797	2.34%	0.262%
25	17.441	2446	2452	2457	rBV	345199	546615	100.00%	11.176%
26	17.483	2457	2459	2465	rVB	58983	75034	13.73%	1.534%
27	17.577	2471	2475	2480	rVB	11681	18140	3.32%	0.371%
28	17.800	2510	2513	2516	rBV4	4919	7918	1.45%	0.162%
29	17.847	2518	2521	2525	rVB4	9195	12111	2.22%	0.248%
30	17.923	2530	2534	2537	rVB4	6487	8480	1.55%	0.173%
31	18.094	2559	2563	2567	rBV6	5278	7049	1.29%	0.144%
32	18.317	2596	2601	2606	rBV2	17627	29851	5.46%	0.610%
33	18.370	2606	2610	2617	rVB2	19119	30973	5.67%	0.633%
34	18.440	2617	2622	2627	rBV8	7243	15342	2.81%	0.314%
35	18.517	2629	2635	2639	rBV4	23453	46354	8.48%	0.948%
36	18.611	2647	2651	2656	rBV5	8867	15097	2.76%	0.309%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
 Data File : BG049818.D
 Acq On : 12 Aug 2021 15:04
 Operator : CG/JU
 Sample : M3335-01 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OR-02-080921

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.663	2656	2660	2662	rBV5	7514	6694	1.22%	0.137%
38	18.710	2662	2668	2669	rBV6	5975	9760	1.79%	0.200%
39	18.810	2682	2685	2687	rBV4	10444	11967	2.19%	0.245%
40	18.851	2690	2692	2694	rBV3	6468	7148	1.31%	0.146%
41	18.934	2703	2706	2708	rBV4	4692	6193	1.13%	0.127%
42	19.033	2719	2723	2726	rBV6	5763	7921	1.45%	0.162%
43	19.110	2733	2736	2739	rBV5	9366	11633	2.13%	0.238%
44	19.233	2751	2757	2761	rBV4	23328	42938	7.86%	0.878%
45	19.374	2777	2781	2783	rBV5	12491	20537	3.76%	0.420%
46	19.415	2786	2788	2791	rVB3	7429	8512	1.56%	0.174%
47	19.498	2797	2802	2808	rVB	110635	157479	28.81%	3.220%
48	19.556	2808	2812	2814	rBV5	8107	11801	2.16%	0.241%
49	19.733	2840	2842	2845	rVB4	12064	9206	1.68%	0.188%
50	19.856	2853	2863	2871	rBV	105415	209200	38.27%	4.277%
51	19.926	2873	2875	2883	rVB8	10083	19553	3.58%	0.400%
52	20.050	2891	2896	2900	rVB	242564	301615	55.18%	6.167%
53	20.343	2944	2946	2951	rVB2	28873	31517	5.77%	0.644%
54	20.443	2961	2963	2967	rVB3	17423	19158	3.50%	0.392%
55	20.508	2972	2974	2977	rVV4	11209	11591	2.12%	0.237%
56	20.655	2995	2999	3001	rBV5	15000	20479	3.75%	0.419%
57	20.690	3003	3005	3011	rVV7	14073	22145	4.05%	0.453%
58	21.436	3129	3132	3136	rBV2	28623	42049	7.69%	0.860%
59	21.724	3174	3181	3186	rBV	296534	545462	99.79%	11.152%
60	25.008	3732	3740	3752	rVB2	186600	509183	93.15%	10.411%
61	27.369	4140	4142	4143	rBV2	14009	11019	2.02%	0.225%


Sum of corrected areas: 4891032

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
Data File : BG049818.D
Acq On : 12 Aug 2021 15:04
Operator : CG/JU
Sample : M3335-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-02-080921

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

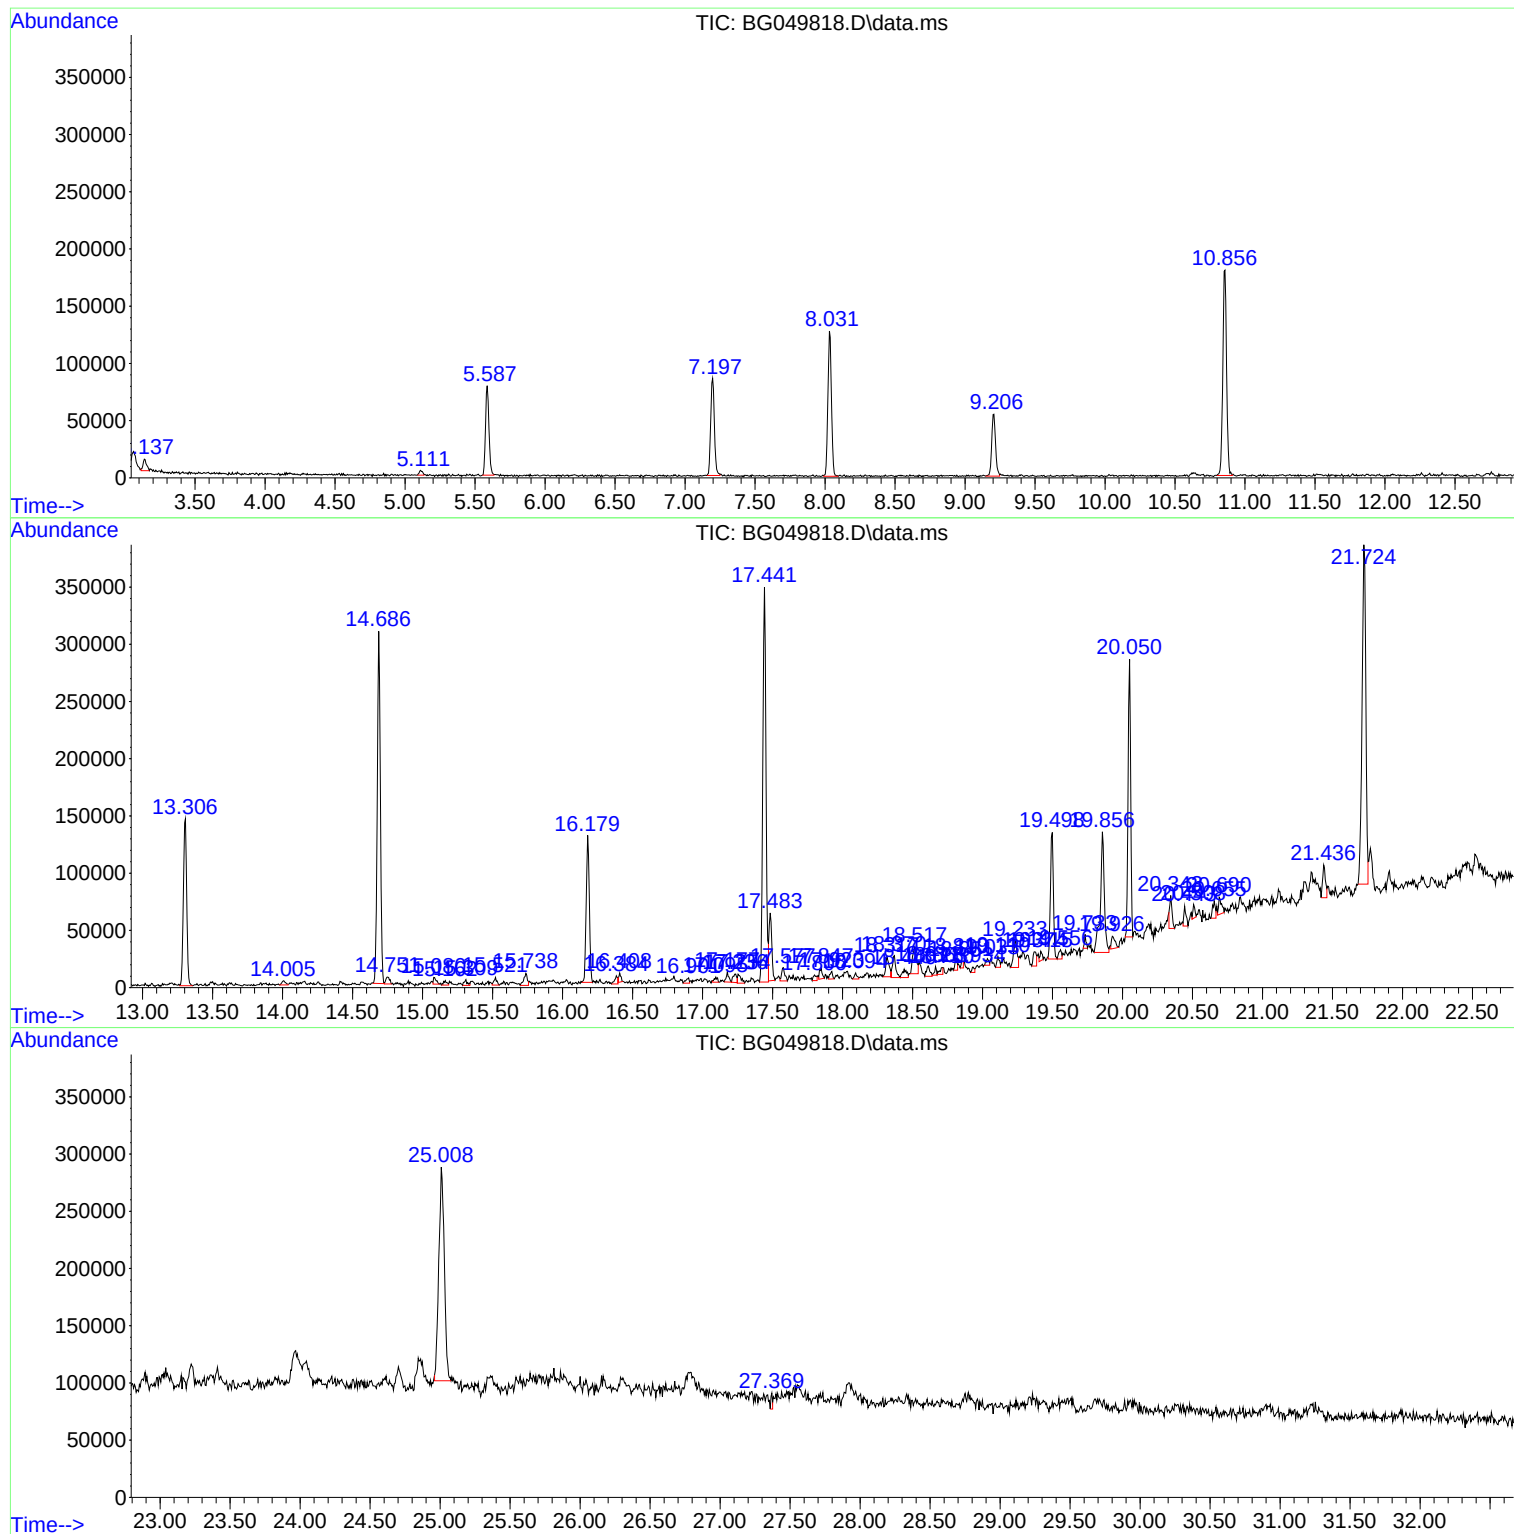

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
Data File : BG049818.D
Acq On : 12 Aug 2021 15:04
Operator : CG/JU
Sample : M3335-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-02-080921

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
Data File : BG049818.D
Acq On : 12 Aug 2021 15:04
Operator : CG/JU
Sample : M3335-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-02-080921

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
