


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
 Data File : BG049810.D
 Acq On : 12 Aug 2021 9:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 03 15:15:33 2021

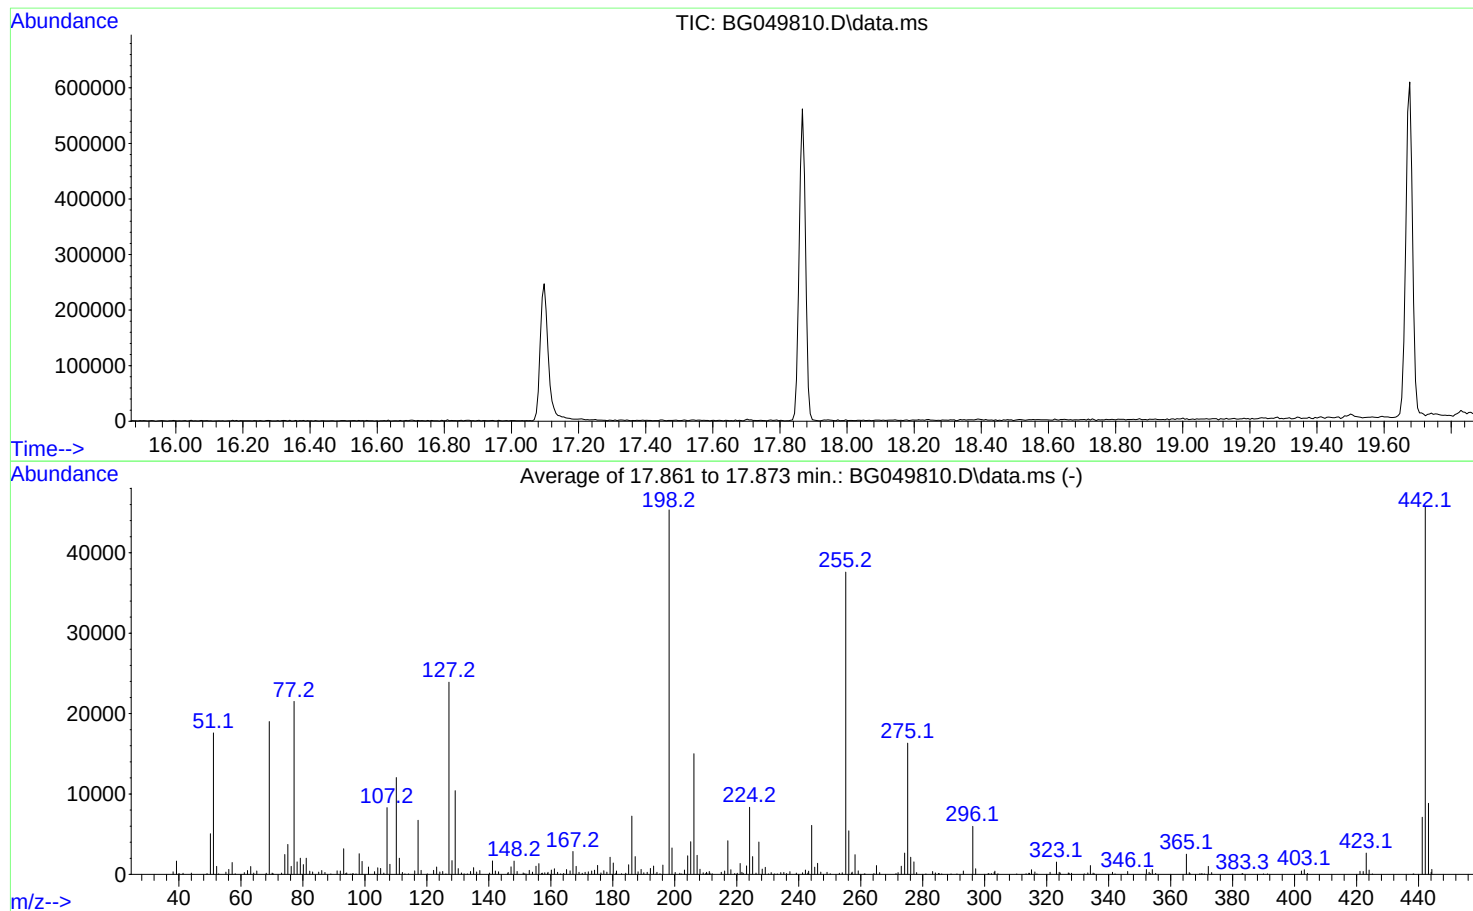




AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	17602	PASS
68	69	0.00	2	0.8	144	PASS
69	198	0.00	100	41.9	19009	PASS
70	69	0.00	2	0.9	162	PASS
127	198	10	80	52.7	23896	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45333	PASS
199	198	5	9	7.2	3280	PASS
275	198	10	60	36.0	16317	PASS
365	198	1	100	5.5	2501	PASS
441	198	0.01	100	15.7	7110	PASS
442	442	100	100	100.0	45755	PASS
443	442	15	24	19.3	8842	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
Data File : BG049810.D
Acq On : 12 Aug 2021 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 12 11:13:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

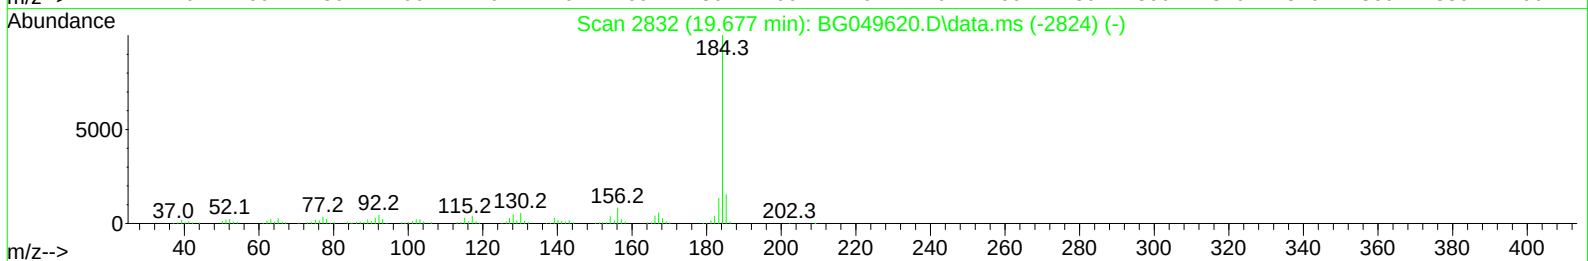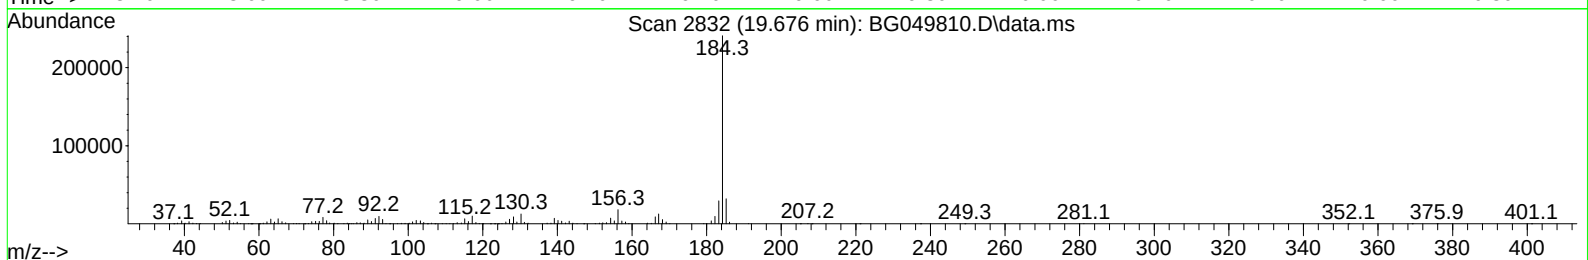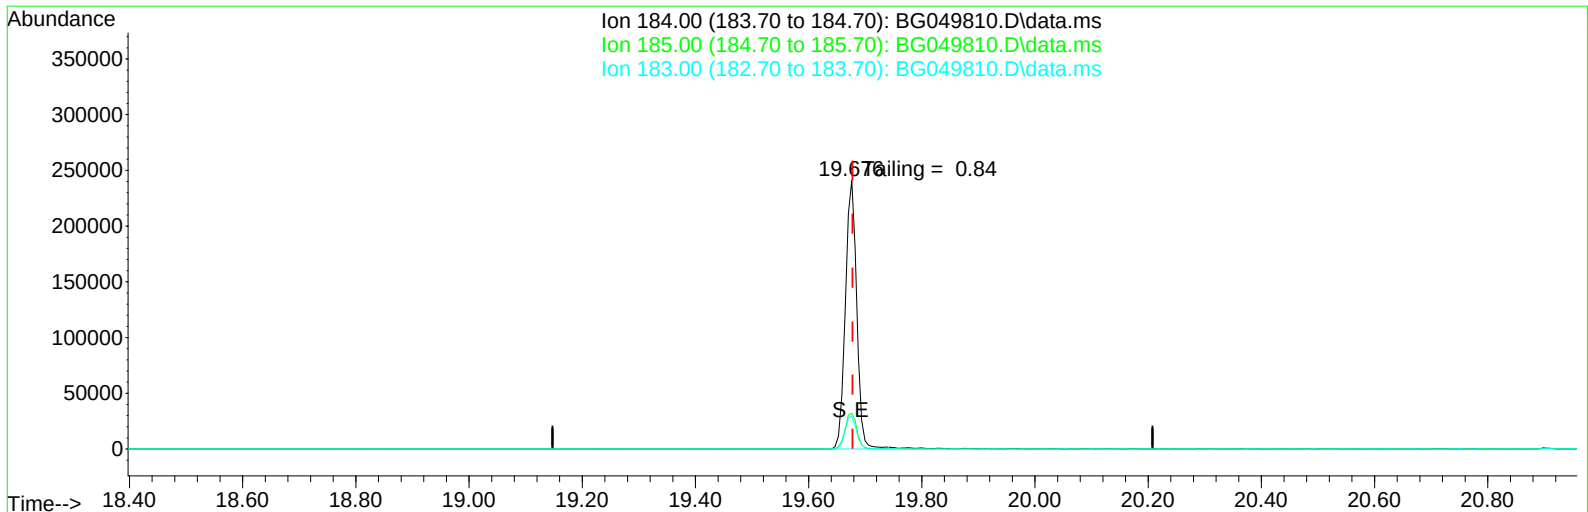

TIC: BG049810.D\data.ms

(77) Benzidine

19.676min (-0.001) 16477.22 ng




response 332679

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.33
183.00	11.70	12.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081221\
Data File : BG049810.D
Acq On : 12 Aug 2021 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 12 11:13:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

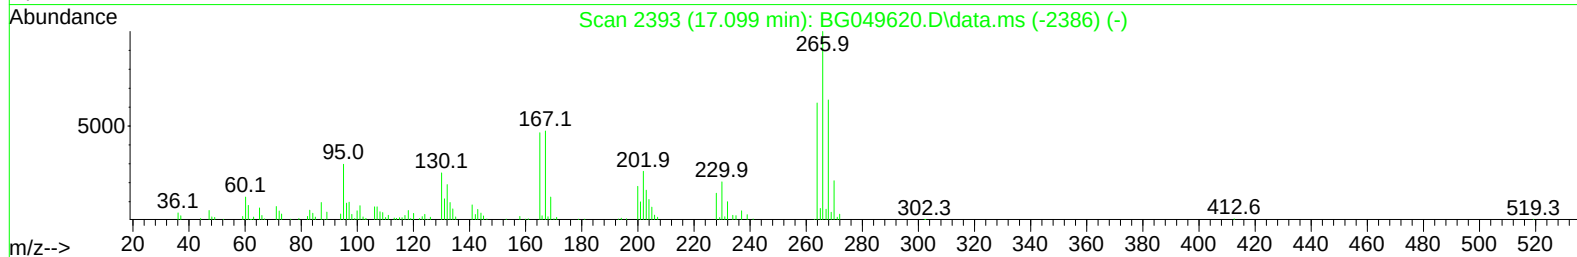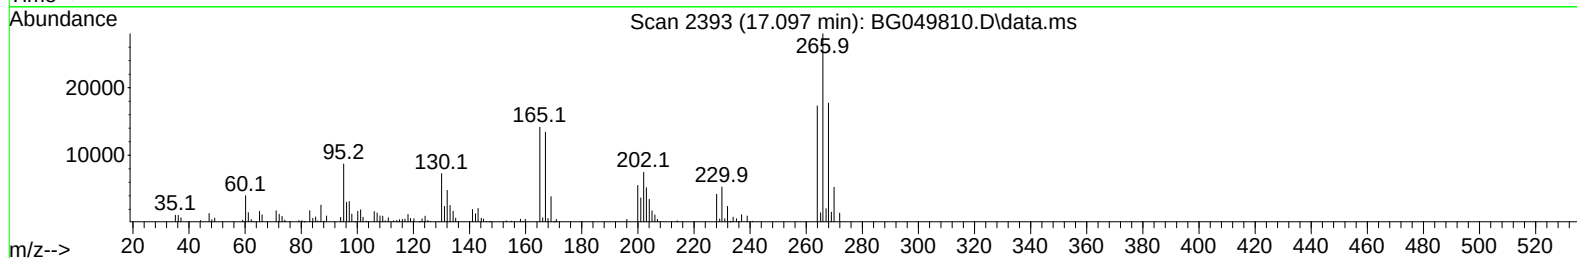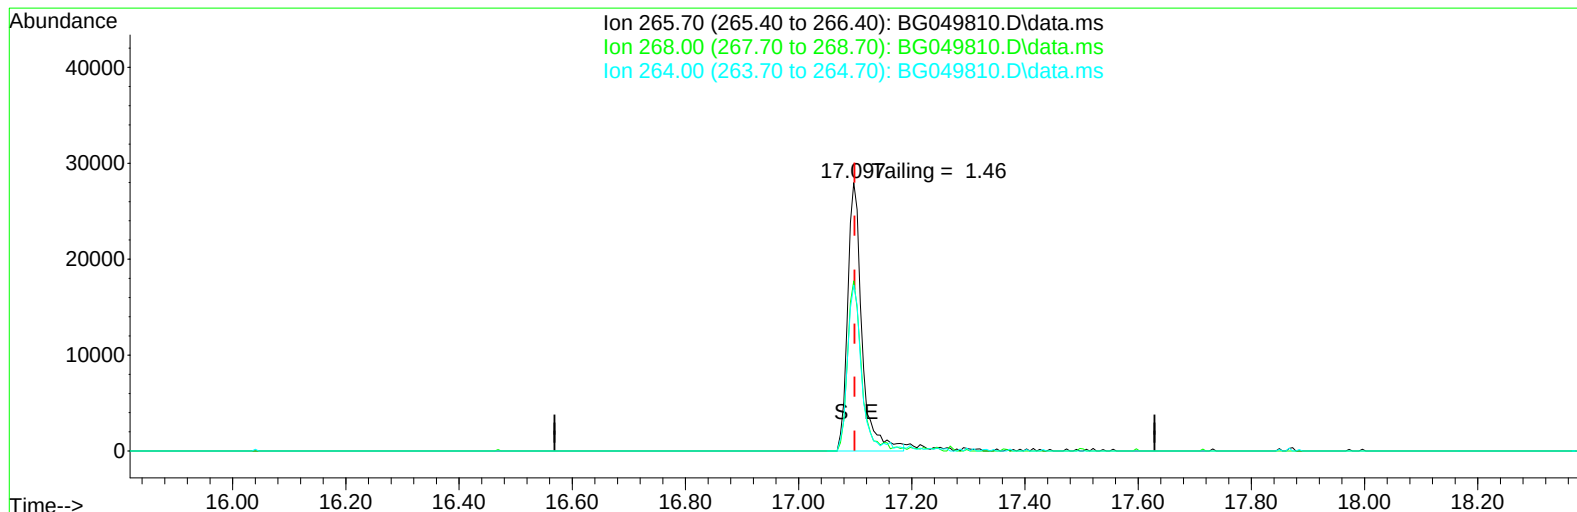

TIC: BG049810.D\data.ms

(70) Pentachlorophenol (C)

17.097min (-0.001) 13934.76 ng

response 49960

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.38
264.00	61.30	61.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/12/2021	BNA_G	BG049810.D
Compound Name	Response	Retention Time
DDT	159379	20.9
DDD	646	20.45
DDE	360	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1006	160385	0.63