

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
 Data File : BG062367.D
 Acq On : 12 Aug 2024 15:16
 Operator : MA/JU
 Sample : P3502-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCXT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	18	22	27	rVB2	11174	16242	0.80%	0.094%
2	3.823	87	91	102	rBV	34297	57135	2.82%	0.329%
3	4.116	138	141	142	rBV2	2843	3086	0.15%	0.018%
4	4.163	146	149	154	rVB3	2690	4490	0.22%	0.026%
5	7.106	643	650	660	rVB	61886	106995	5.28%	0.616%
6	7.283	673	680	694	rVB	167434	275381	13.60%	1.586%
7	7.482	706	714	725	rBV	188132	319282	15.77%	1.839%
8	7.952	788	794	802	rBV	166523	278470	13.75%	1.604%
9	8.646	905	912	920	rBV	173945	290921	14.37%	1.676%
10	9.104	981	990	1001	rBV	202214	355268	17.54%	2.046%
11	9.826	1104	1113	1119	rBV	155784	270829	13.37%	1.560%
12	9.950	1131	1134	1136	rBV3	2478	3236	0.16%	0.019%
13	10.361	1197	1204	1211	rBV	274364	467699	23.10%	2.694%
14	10.749	1261	1270	1277	rBV	247878	435069	21.49%	2.506%
15	10.872	1283	1291	1298	rBV	153185	276238	13.64%	1.591%
16	12.335	1532	1540	1547	rVB2	5125	8925	0.44%	0.051%
17	13.980	1810	1820	1827	rBV	602723	857065	42.33%	4.937%
18	14.267	1862	1869	1876	rVB	655141	1033123	51.02%	5.951%
19	14.573	1913	1921	1930	rBV	497660	753603	37.22%	4.341%
20	14.749	1945	1951	1959	rBV	78110	130019	6.42%	0.749%
21	14.984	1986	1991	1995	rBV4	1832	2895	0.14%	0.017%
22	15.313	2043	2047	2050	rBV2	3291	4137	0.20%	0.024%
23	15.389	2055	2060	2064	rBV3	1906	3164	0.16%	0.018%
24	15.566	2083	2090	2098	rBV	907781	1382178	68.26%	7.962%
25	15.671	2101	2108	2117	rBV	217627	317270	15.67%	1.828%
26	15.801	2127	2130	2136	rBV2	3075	4114	0.20%	0.024%
27	16.723	2283	2287	2291	rBV2	1553	2948	0.15%	0.017%
28	17.310	2381	2387	2395	rVB	666400	979629	48.38%	5.643%
29	17.410	2397	2404	2412	rVV2	1080177	1634457	80.72%	9.415%
30	18.209	2536	2540	2546	rBV3	24711	40173	1.98%	0.231%
31	18.280	2550	2552	2556	rVB3	2968	3872	0.19%	0.022%
32	18.679	2618	2620	2622	rBV3	1832	2121	0.10%	0.012%
33	19.161	2697	2702	2704	rVB3	2620	3457	0.17%	0.020%
34	19.261	2714	2719	2723	rBV3	15419	21032	1.04%	0.121%
35	19.302	2723	2726	2727	rBV3	2099	2225	0.11%	0.013%
36	19.331	2727	2731	2734	rVV	15395	21552	1.06%	0.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
 Data File : BG062367.D
 Acq On : 12 Aug 2024 15:16
 Operator : MA/JU
 Sample : P3502-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCXT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	19.484	2753	2757	2760	rBV3	13551	17528	0.87%	0.101%
38	19.637	2777	2783	2786	rBV6	6990	11264	0.56%	0.065%
39	19.695	2786	2793	2801	rBV	1399337	2016238	99.57%	11.614%
40	19.825	2814	2815	2819	rBV3	2177	3242	0.16%	0.019%
41	19.872	2821	2823	2826	rVV3	2282	2575	0.13%	0.015%
42	19.924	2829	2832	2835	rVB4	1813	2410	0.12%	0.014%
43	20.071	2855	2857	2860	rBV3	1963	2234	0.11%	0.013%
44	20.253	2882	2888	2890	rBV6	4430	6720	0.33%	0.039%
45	20.670	2957	2959	2965	rBV6	5339	6126	0.30%	0.035%
46	20.741	2968	2971	2976	rVB	11741	13083	0.65%	0.075%
47	20.894	2994	2997	3000	rBV4	1939	2275	0.11%	0.013%
48	21.240	3051	3056	3061	rBV	57241	73570	3.63%	0.424%
49	21.469	3091	3095	3098	rBV6	6606	8385	0.41%	0.048%
50	21.552	3102	3109	3119	rVV	719392	1124326	55.52%	6.476%
51	21.775	3142	3147	3153	rVB	69329	99220	4.90%	0.572%
52	22.022	3187	3189	3192	rBV4	3122	2404	0.12%	0.014%
53	22.215	3220	3222	3225	rBV4	3118	3129	0.15%	0.018%
54	22.362	3242	3247	3254	rBV	58244	94680	4.68%	0.545%
55	23.038	3356	3362	3369	rVB	41910	73869	3.65%	0.425%
56	23.214	3390	3392	3400	rVB8	8151	12924	0.64%	0.074%
57	23.273	3400	3402	3407	rBV4	3173	3504	0.17%	0.020%
58	23.813	3488	3494	3501	rVB3	27154	60295	2.98%	0.347%
59	24.430	3588	3599	3613	rVV	763049	2024947	100.00%	11.664%
60	24.642	3625	3635	3644	rBV	427058	1163756	57.47%	6.703%
61	24.724	3645	3649	3658	rVB4	22702	55973	2.76%	0.322%
62	24.906	3679	3680	3682	rBV2	3537	2077	0.10%	0.012%
63	25.341	3752	3754	3758	rBV5	4059	5409	0.27%	0.031%
64	25.811	3830	3834	3842	rVB7	16300	40812	2.02%	0.235%
65	27.121	4049	4057	4066	rVB7	15744	45581	2.25%	0.263%
66	27.567	4131	4133	4134	rBV	2769	2176	0.11%	0.013%
67	27.902	4188	4190	4192	rBV3	2881	2516	0.12%	0.014%
68	28.683	4321	4323	4325	rBV3	5325	6233	0.31%	0.036%
69	32.196	4919	4921	4922	rBV2	3801	2867	0.14%	0.017%


Sum of corrected areas: 17360648

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
Data File : BG062367.D
Acq On : 12 Aug 2024 15:16
Operator : MA/JU
Sample : P3502-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

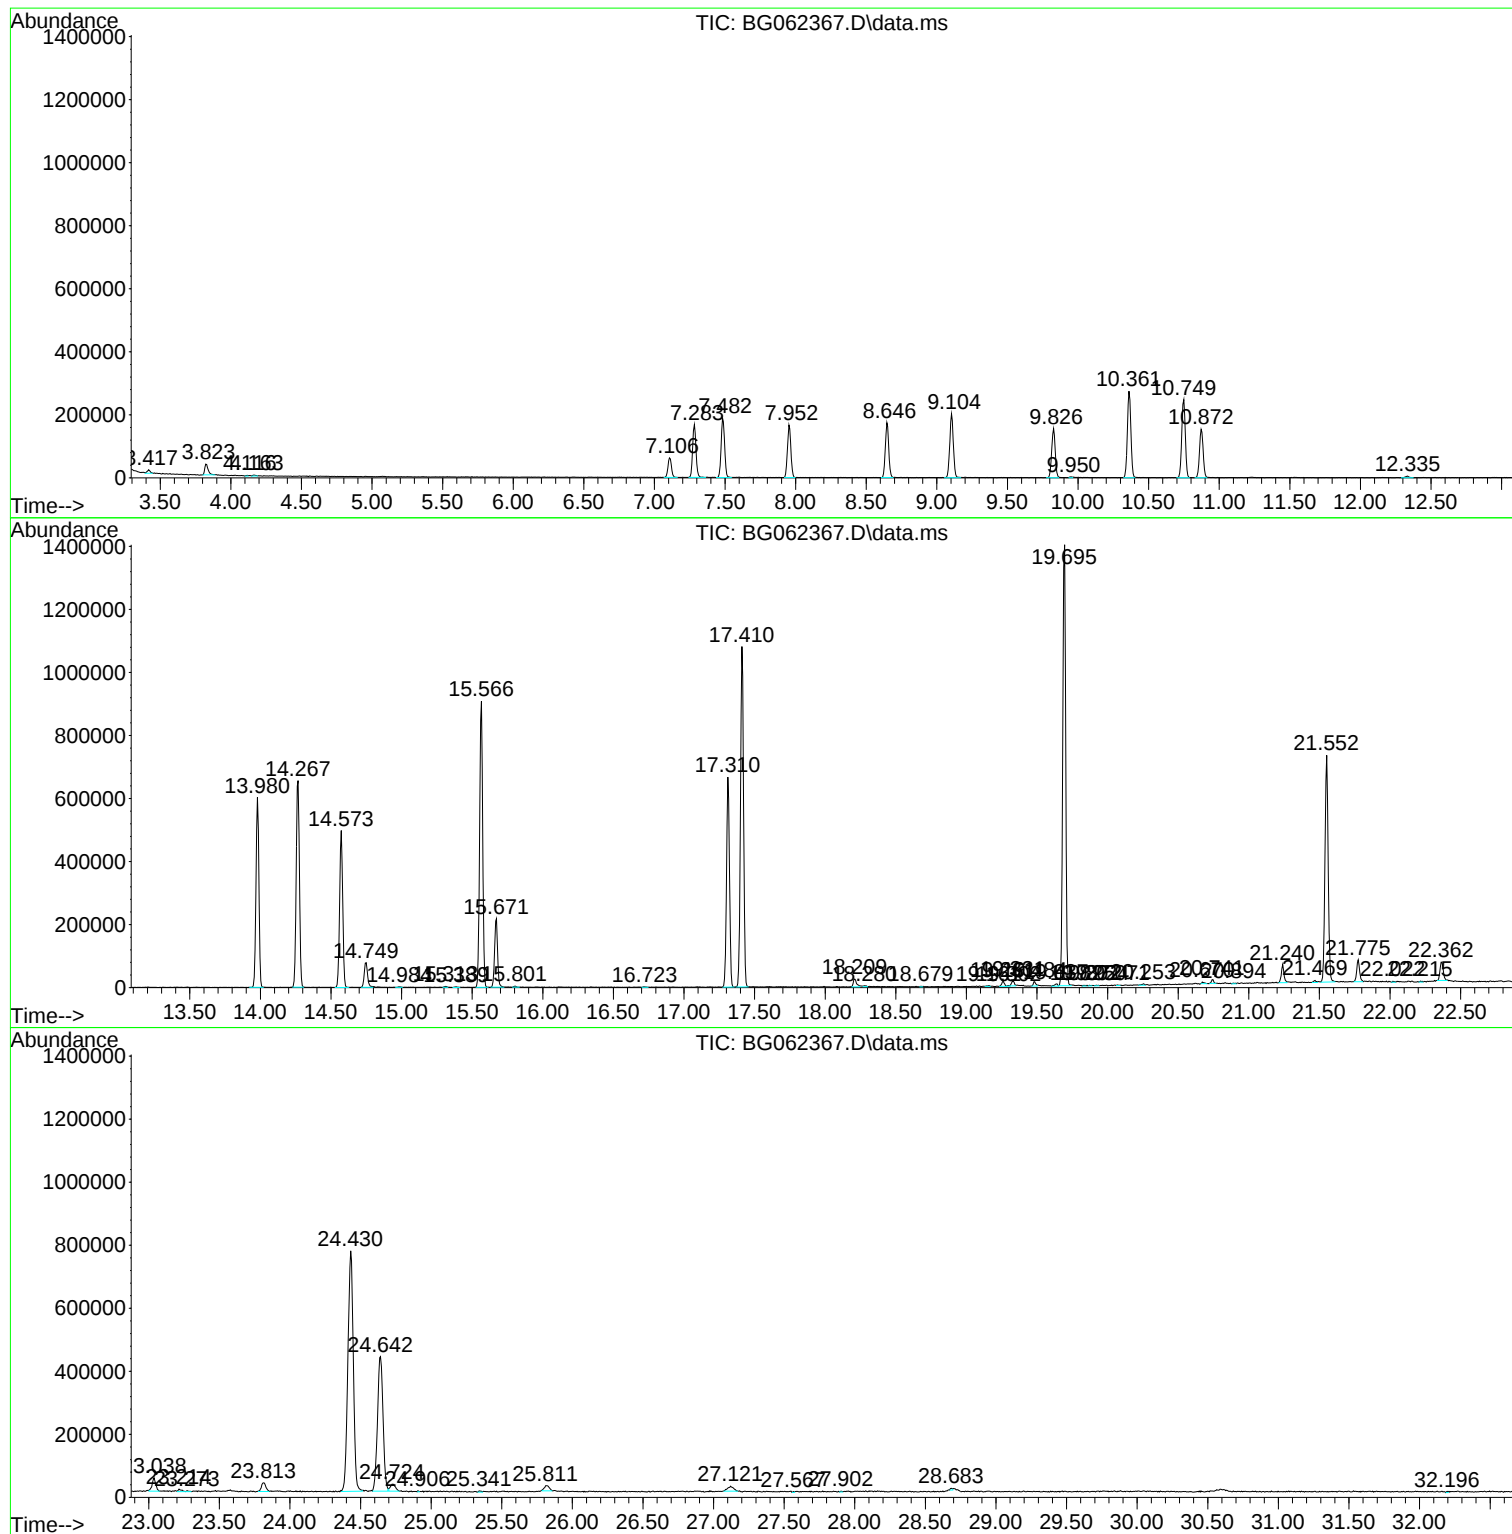

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
Data File : BG062367.D
Acq On : 12 Aug 2024 15:16
Operator : MA/JU
Sample : P3502-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
Data File : BG062367.D
Acq On : 12 Aug 2024 15:16
Operator : MA/JU
Sample : P3502-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc