

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
 Data File : BG062369.D
 Acq On : 12 Aug 2024 16:38
 Operator : MA/JU
 Sample : P3538-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH7N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.420	18	22	26	rVB2	10827	15083	0.75%	0.084%
2	3.825	86	91	98	rBV	67002	113501	5.62%	0.628%
3	7.109	644	650	659	rVB	63036	104352	5.16%	0.578%
4	7.279	671	679	689	rBV	172429	292488	14.48%	1.620%
5	7.485	707	714	724	rVB	195223	324871	16.08%	1.799%
6	7.955	787	794	802	rVB	173575	295753	14.64%	1.638%
7	8.648	905	912	919	rBV	180312	301146	14.91%	1.667%
8	9.106	981	990	998	rBV	213236	373674	18.50%	2.069%
9	9.218	1004	1009	1016	rVB4	5901	10182	0.50%	0.056%
10	9.829	1106	1113	1120	rBV	160872	283141	14.01%	1.568%
11	10.363	1197	1204	1217	rBV	288447	498081	24.65%	2.758%
12	10.745	1261	1269	1277	rBV	261701	461209	22.83%	2.554%
13	10.874	1282	1291	1303	rBV	279789	496013	24.55%	2.747%
14	11.526	1399	1402	1407	rBV5	1662	3011	0.15%	0.017%
15	12.331	1535	1539	1545	rVB4	5442	8413	0.42%	0.047%
16	13.982	1813	1820	1827	rBV	607058	880968	43.60%	4.878%
17	14.264	1861	1868	1876	rBV	703786	1083897	53.65%	6.002%
18	14.569	1914	1920	1929	rVB	524893	802139	39.70%	4.442%
19	14.746	1943	1950	1959	rBV	71417	112903	5.59%	0.625%
20	15.386	2053	2059	2063	rBV2	1754	2509	0.12%	0.014%
21	15.562	2082	2089	2096	rBV	951913	1432171	70.89%	7.930%
22	15.668	2102	2107	2117	rBV	212568	309569	15.32%	1.714%
23	15.809	2126	2131	2133	rVB3	3150	3963	0.20%	0.022%
24	16.249	2201	2206	2212	rVB2	2632	3963	0.20%	0.022%
25	17.089	2344	2349	2350	rBV	2113	2038	0.10%	0.011%
26	17.313	2380	2387	2395	rVB	688235	1044666	51.71%	5.784%
27	17.413	2397	2404	2414	rVB	1105701	1628882	80.62%	9.019%
28	18.211	2535	2540	2548	rVV4	18408	32233	1.60%	0.178%
29	18.282	2548	2552	2556	rVB	3085	5288	0.26%	0.029%
30	19.140	2694	2698	2701	rBV3	1668	2372	0.12%	0.013%
31	19.257	2714	2718	2723	rVB2	13390	20287	1.00%	0.112%
32	19.328	2726	2730	2736	rVV2	16742	23968	1.19%	0.133%
33	19.398	2739	2742	2748	rVB5	3294	5191	0.26%	0.029%
34	19.480	2752	2756	2762	rVV5	10973	14057	0.70%	0.078%
35	19.633	2777	2782	2786	rBV3	7221	9287	0.46%	0.051%
36	19.692	2786	2792	2800	rBV	1389203	2007979	99.39%	11.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
 Data File : BG062369.D
 Acq On : 12 Aug 2024 16:38
 Operator : MA/JU
 Sample : P3538-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH7N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	20.244	2884	2886	2891	rVB6	1910	2628	0.13%	0.015%
38	20.408	2909	2914	2915	rBV3	1572	2262	0.11%	0.013%
39	20.673	2955	2959	2962	rBV6	6517	9759	0.48%	0.054%
40	20.743	2968	2971	2976	rVB2	9567	8801	0.44%	0.049%
41	21.243	3051	3056	3063	rVB	36302	46649	2.31%	0.258%
42	21.460	3091	3093	3099	rVB6	3887	5665	0.28%	0.031%
43	21.548	3101	3108	3121	rBV	754201	1207610	59.77%	6.687%
44	21.701	3132	3134	3137	rBV3	3215	3784	0.19%	0.021%
45	21.771	3141	3146	3154	rBV	52793	83467	4.13%	0.462%
46	22.306	3235	3237	3238	rBV2	3317	2373	0.12%	0.013%
47	22.365	3242	3247	3255	rVV	54835	90989	4.50%	0.504%
48	23.034	3356	3361	3370	rVB2	36078	66635	3.30%	0.369%
49	23.510	3440	3442	3447	rBV6	2835	3297	0.16%	0.018%
50	23.810	3487	3493	3501	rVB3	28922	60850	3.01%	0.337%
51	24.432	3587	3599	3613	rBV	753052	2020375	100.00%	11.187%
52	24.638	3624	3634	3644	rBV	462967	1246277	61.69%	6.901%
53	24.720	3644	3648	3655	rVB4	21500	50715	2.51%	0.281%
54	25.425	3766	3768	3769	rBV2	4819	3021	0.15%	0.017%
55	25.813	3828	3834	3845	rVB6	18574	52737	2.61%	0.292%
56	26.077	3877	3879	3880	rBV2	3768	2554	0.13%	0.014%
57	26.095	3880	3882	3883	rVV2	2638	2119	0.10%	0.012%
58	27.111	4050	4055	4066	rVB9	15521	50560	2.50%	0.280%
59	27.511	4121	4123	4125	rBV3	2668	2237	0.11%	0.012%
60	27.552	4128	4130	4132	rBV3	3292	2933	0.15%	0.016%
61	28.838	4347	4349	4351	rBV3	3153	2554	0.13%	0.014%
62	29.719	4497	4499	4502	rBV4	2721	2655	0.13%	0.015%
63	30.189	4577	4579	4581	rVB3	3182	2101	0.10%	0.012%
64	30.571	4639	4644	4645	rBV5	6367	10271	0.51%	0.057%
65	31.558	4810	4812	4815	rBV4	2895	2180	0.11%	0.012%
66	32.075	4898	4900	4901	rBV2	3141	2494	0.12%	0.014%


Sum of corrected areas: 18059800

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
Data File : BG062369.D
Acq On : 12 Aug 2024 16:38
Operator : MA/JU
Sample : P3538-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH7N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

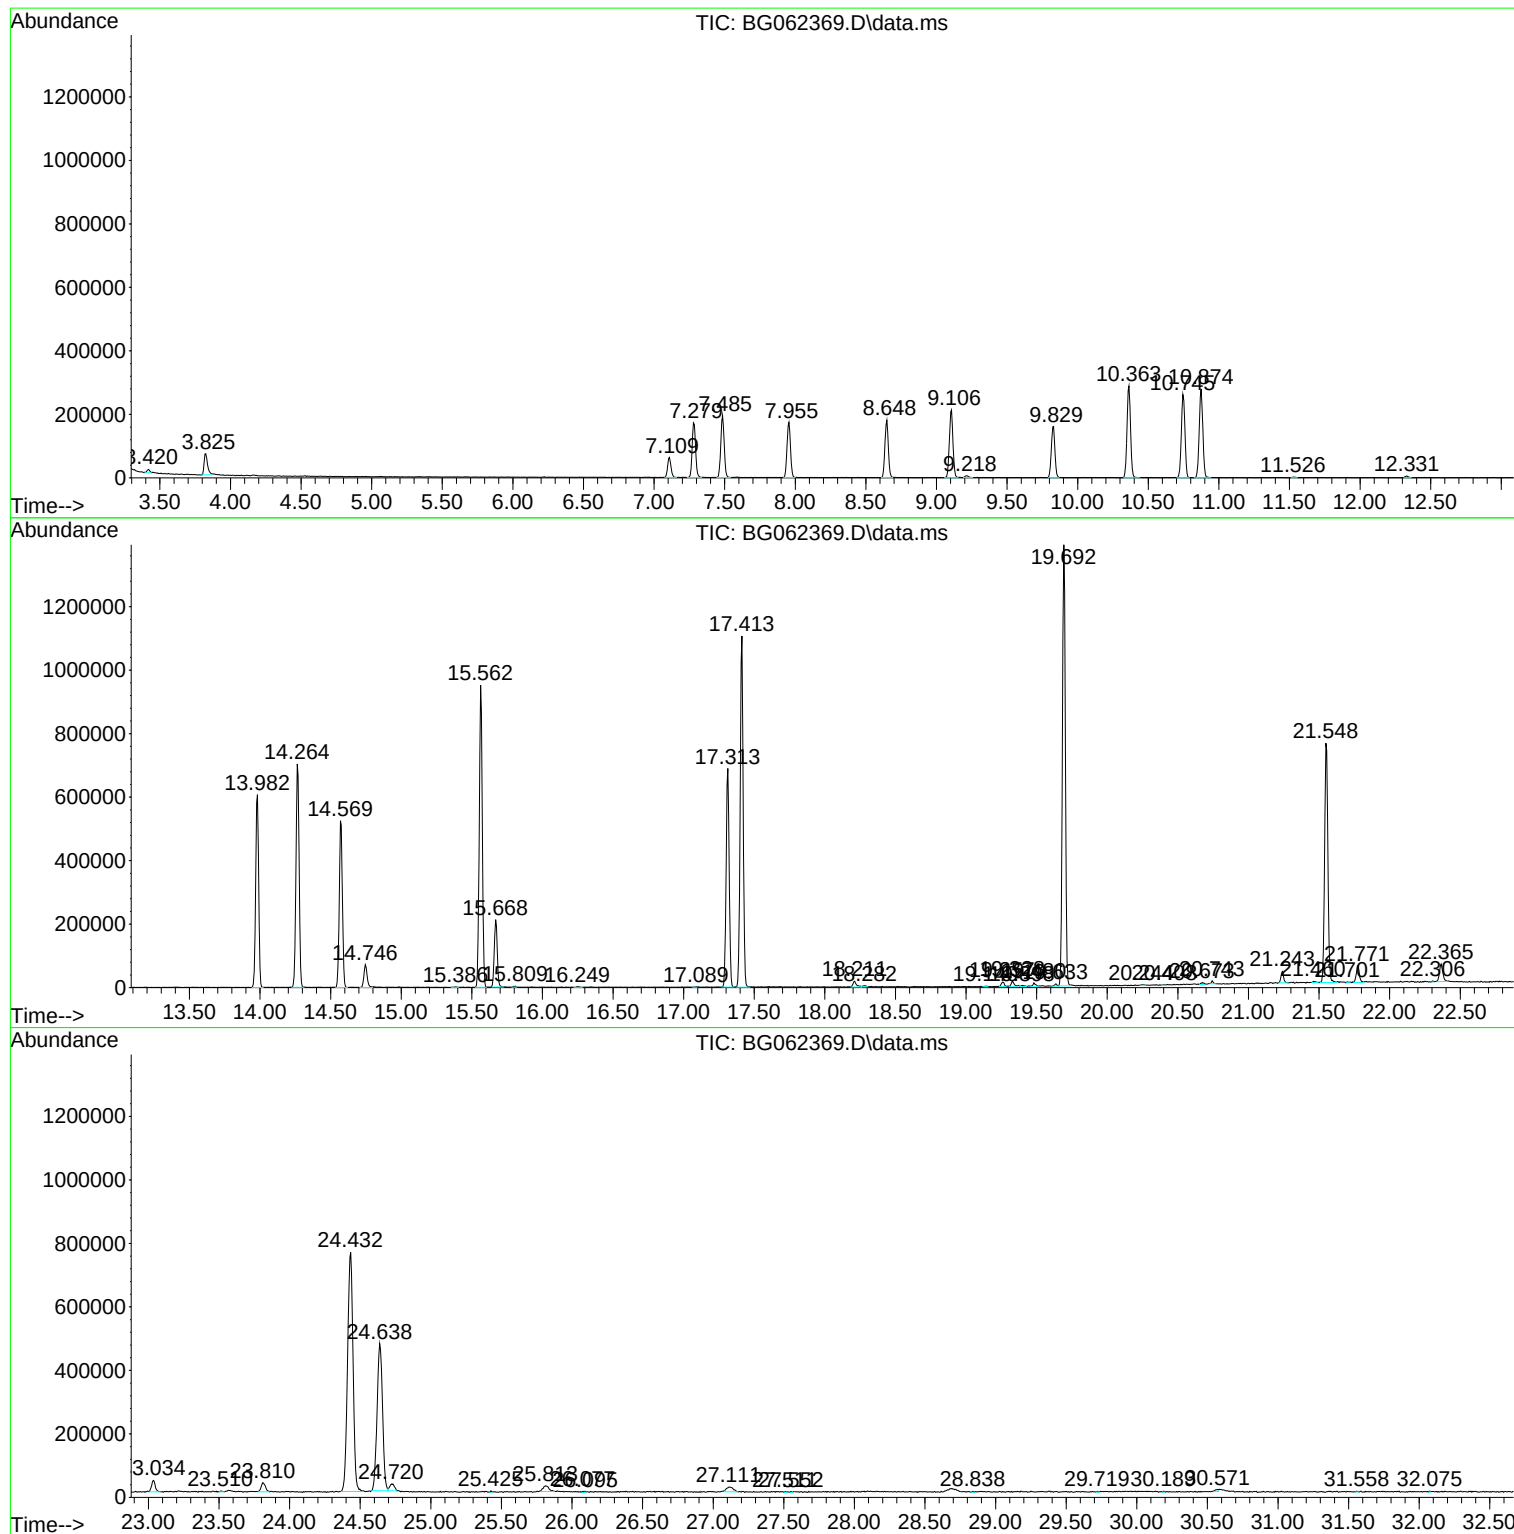

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
Data File : BG062369.D
Acq On : 12 Aug 2024 16:38
Operator : MA/JU
Sample : P3538-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH7N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
Data File : BG062369.D
Acq On : 12 Aug 2024 16:38
Operator : MA/JU
Sample : P3538-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH7N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc