

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
 Data File : BG062375.D
 Acq On : 12 Aug 2024 20:44
 Operator : MA/JU
 Sample : PB162636BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK636

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.414	18	21	27	rVB	14961	20832	1.16%	0.120%
2	3.820	85	90	105	rVB	163765	273512	15.26%	1.570%
3	4.272	166	167	171	rBV2	1974	2793	0.16%	0.016%
4	7.103	643	649	661	rBV	191357	325561	18.16%	1.869%
5	7.280	673	679	687	rBV	147685	235849	13.16%	1.354%
6	7.485	706	714	722	rBV	165485	284017	15.85%	1.630%
7	7.949	785	793	803	rVB	175504	298015	16.63%	1.711%
8	8.642	904	911	924	rBV	230790	393068	21.93%	2.256%
9	9.101	982	989	997	rBV	174535	303121	16.91%	1.740%
10	9.823	1105	1112	1120	rBV	138577	238313	13.30%	1.368%
11	10.358	1196	1203	1212	rBV	231313	401941	22.43%	2.307%
12	10.745	1261	1269	1279	rVB	260531	462517	25.81%	2.655%
13	10.875	1283	1291	1301	rBV	257020	465871	25.99%	2.674%
14	12.326	1535	1538	1545	rVB2	2950	4869	0.27%	0.028%
15	13.976	1813	1819	1828	rVB	510265	742606	41.43%	4.263%
16	14.264	1861	1868	1877	rBV	581200	886826	49.48%	5.091%
17	14.570	1913	1920	1928	rBV	524620	811712	45.29%	4.659%
18	14.746	1943	1950	1961	rBV	254807	408207	22.78%	2.343%
19	15.562	2082	2089	2096	rBV	816277	1200478	66.98%	6.891%
20	15.668	2101	2107	2118	rBV	201016	288808	16.11%	1.658%
21	15.803	2126	2130	2133	rBV	2538	3364	0.19%	0.019%
22	16.350	2218	2223	2225	rBV2	2218	2682	0.15%	0.015%
23	17.090	2347	2349	2355	rVB2	1556	2665	0.15%	0.015%
24	17.313	2380	2387	2393	rBV	729896	1100798	61.42%	6.319%
25	17.407	2396	2403	2416	rBV	927322	1396707	77.93%	8.017%
26	18.206	2535	2539	2542	rBV4	4725	6306	0.35%	0.036%
27	19.257	2713	2718	2723	rBV3	12018	18324	1.02%	0.105%
28	19.328	2726	2730	2735	rVV2	10812	14786	0.82%	0.085%
29	19.398	2739	2742	2745	rVB4	2157	2101	0.12%	0.012%
30	19.504	2755	2760	2763	rVB4	2005	3444	0.19%	0.020%
31	19.534	2763	2765	2768	rBV3	1838	1830	0.10%	0.011%
32	19.633	2779	2782	2785	rVV3	3427	4229	0.24%	0.024%
33	19.692	2785	2792	2800	rVV	1209662	1719497	95.94%	9.870%
34	19.745	2800	2801	2806	rVB3	2244	2208	0.12%	0.013%
35	20.168	2868	2873	2875	rBV3	2409	3790	0.21%	0.022%
36	20.244	2884	2886	2889	rVB4	2791	2932	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
 Data File : BG062375.D
 Acq On : 12 Aug 2024 20:44
 Operator : MA/JU
 Sample : PB162636BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK636

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	20.567	2938	2941	2944	rBV5	1835	2524	0.14%	0.014%
38	20.673	2956	2959	2961	rBV2	4811	4852	0.27%	0.028%
39	20.744	2967	2971	2978	rBV5	4321	7025	0.39%	0.040%
40	21.237	3051	3055	3059	rBV3	14430	18225	1.02%	0.105%
41	21.407	3083	3084	3086	rBV2	2886	2264	0.13%	0.013%
42	21.548	3101	3108	3117	rBV	799120	1276982	71.25%	7.330%
43	21.772	3142	3146	3153	rVB2	26944	37264	2.08%	0.214%
44	22.365	3242	3247	3252	rVB	33444	53042	2.96%	0.304%
45	22.535	3274	3276	3277	rVB2	3594	1948	0.11%	0.011%
46	22.553	3277	3279	3283	rBV5	2835	3719	0.21%	0.021%
47	22.770	3313	3316	3317	rBV3	4220	4100	0.23%	0.024%
48	23.035	3354	3361	3371	rBV2	32373	65520	3.66%	0.376%
49	23.810	3485	3493	3501	rBV	32623	72342	4.04%	0.415%
50	23.916	3509	3511	3515	rBV5	2371	1828	0.10%	0.010%
51	24.427	3586	3598	3613	rBV	660959	1792264	100.00%	10.288%
52	24.638	3624	3634	3643	rBV	522418	1369113	76.39%	7.859%
53	24.721	3644	3648	3656	rVB2	35782	79343	4.43%	0.455%
54	25.520	3782	3784	3788	rBV5	2772	3630	0.20%	0.021%
55	25.807	3826	3833	3843	rVB3	33330	96222	5.37%	0.552%
56	26.001	3864	3866	3869	rBV4	2908	4388	0.24%	0.025%
57	27.117	4047	4056	4068	rVV4	26645	93654	5.23%	0.538%
58	27.211	4070	4072	4073	rBV2	2528	2069	0.12%	0.012%
59	27.558	4129	4131	4134	rBV3	2725	2488	0.14%	0.014%
60	28.181	4235	4237	4238	rBV2	3003	2577	0.14%	0.015%
61	28.680	4314	4322	4337	rVB9	19990	80390	4.49%	0.461%
62	29.679	4490	4492	4494	rBV3	2704	2332	0.13%	0.013%
63	31.265	4760	4762	4764	rBV3	2251	2743	0.15%	0.016%
64	31.511	4802	4804	4806	rBV3	3485	3409	0.19%	0.020%




Sum of corrected areas: 17420836

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
Data File : BG062375.D
Acq On : 12 Aug 2024 20:44
Operator : MA/JU
Sample : PB162636BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK636

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

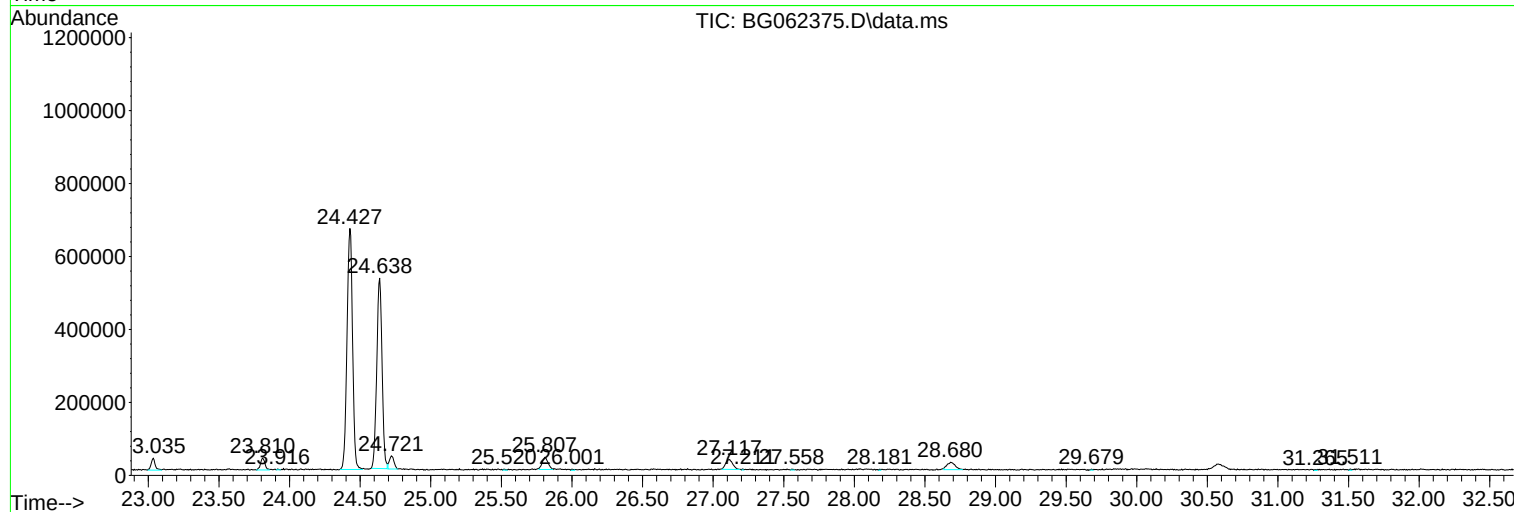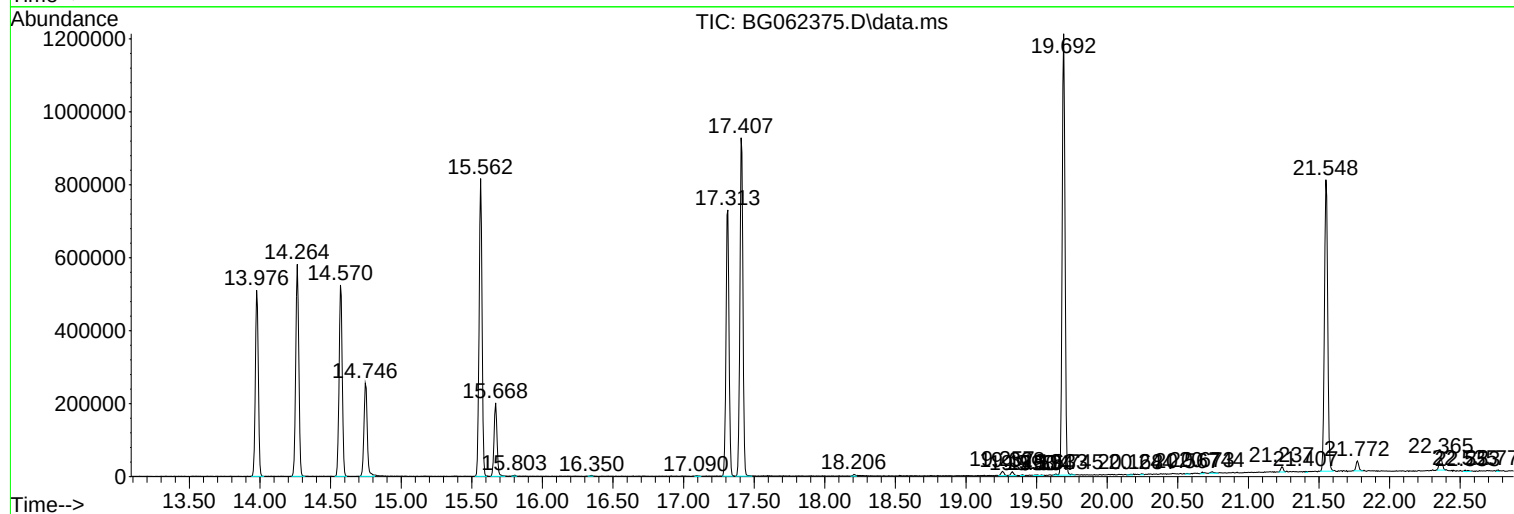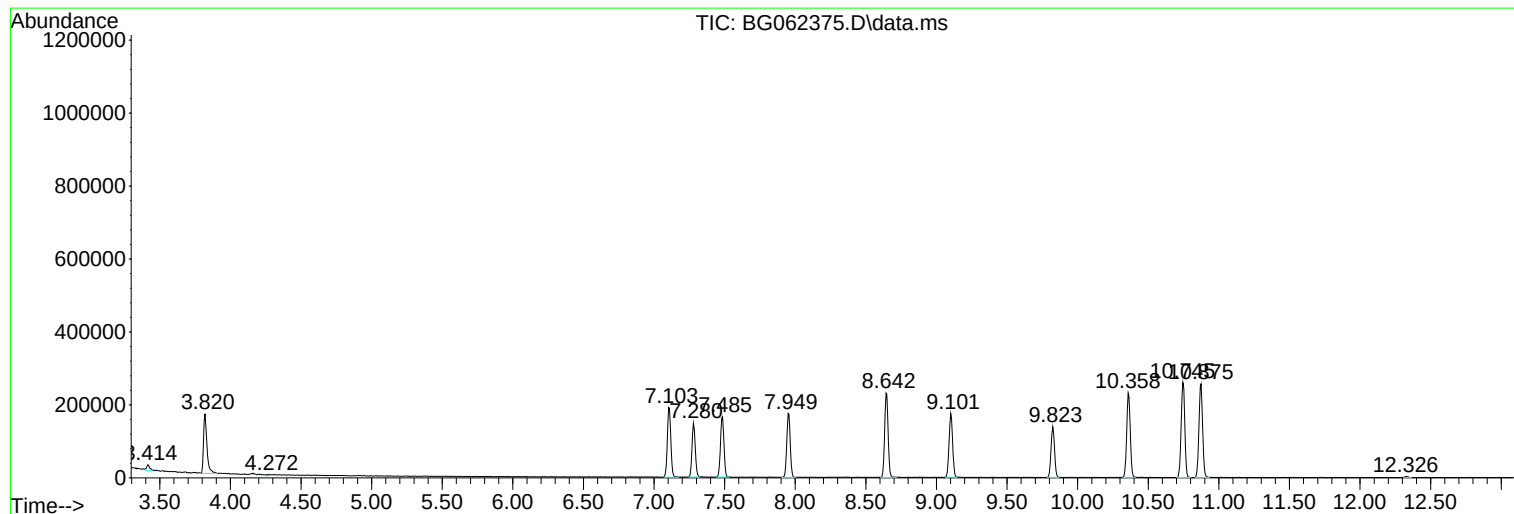

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
Data File : BG062375.D
Acq On : 12 Aug 2024 20:44
Operator : MA/JU
Sample : PB162636BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK636

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081224\
Data File : BG062375.D
Acq On : 12 Aug 2024 20:44
Operator : MA/JU
Sample : PB162636BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK636

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc