




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:03:43 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

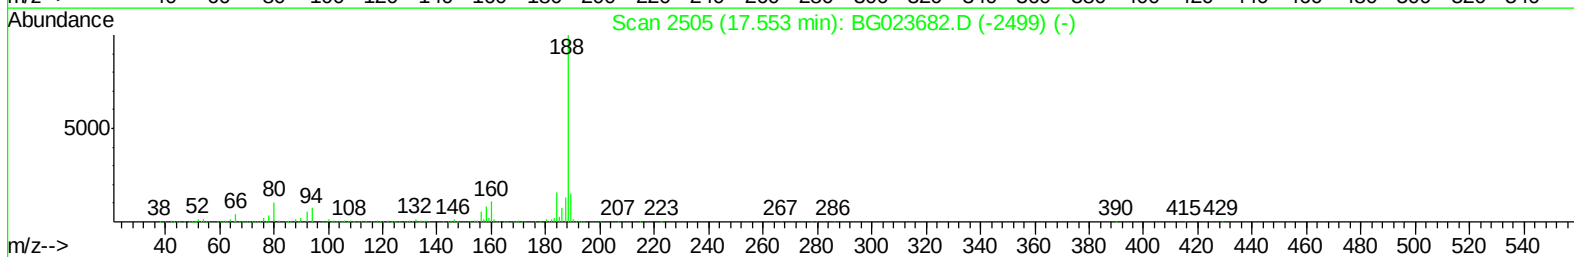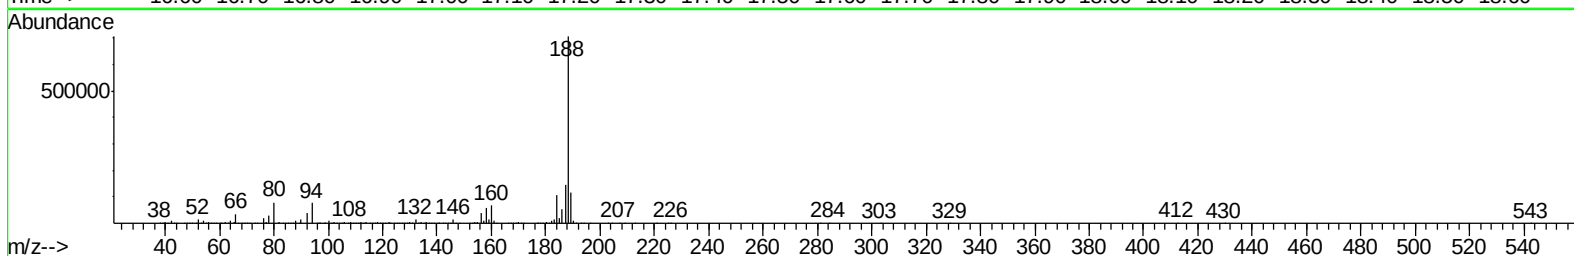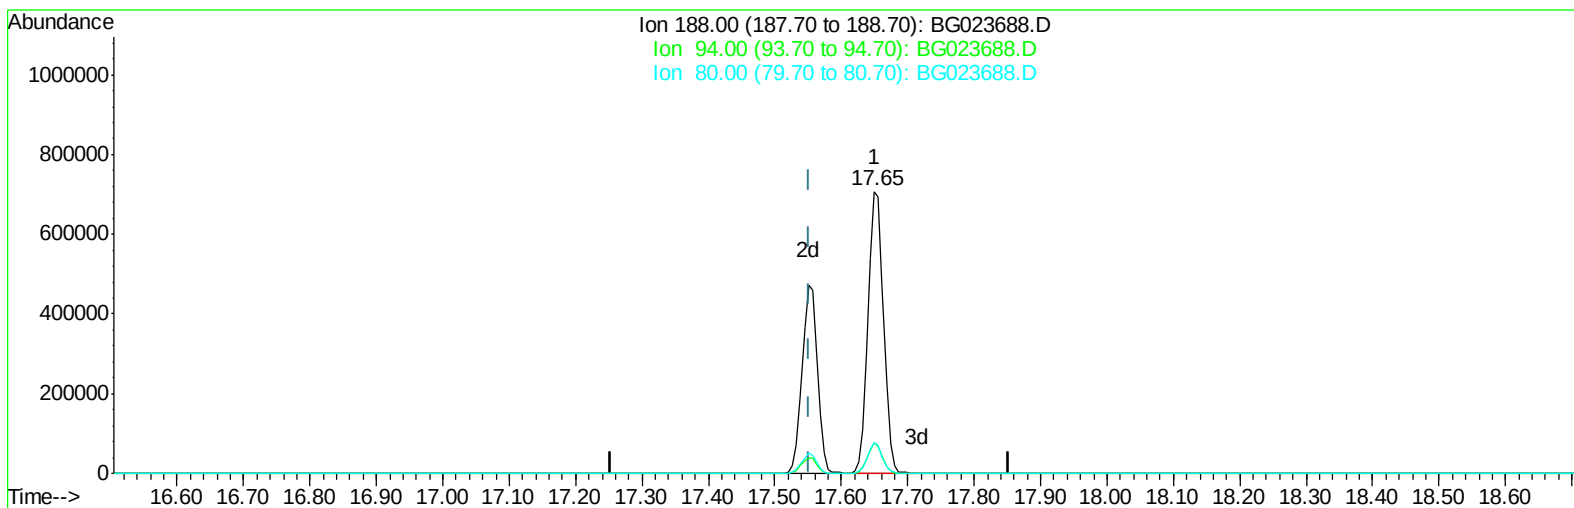

TIC: BG023688.D

(61) Phenanthrene-d10 (I)

17.650min (+0.097) 20.00ng/ul

response 1118828

Ion	Exp%	Act%
188.00	100	100
94.00	10.30	10.87
80.00	10.90	11.02
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:07:48 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

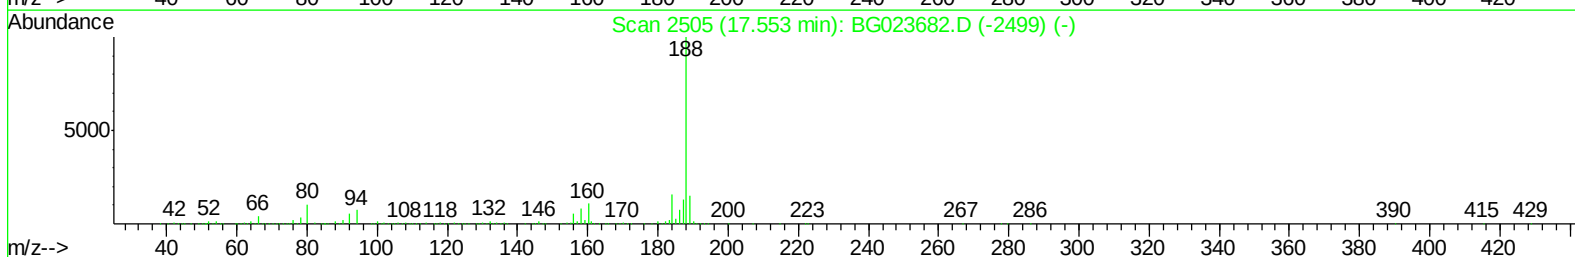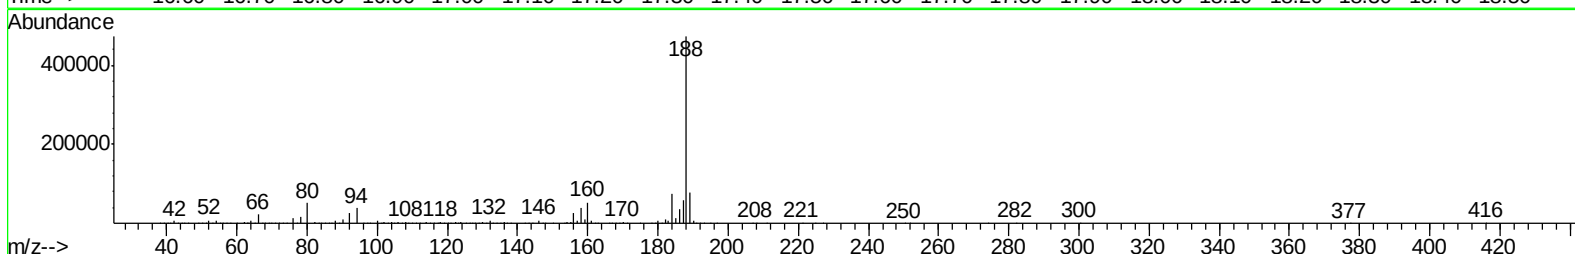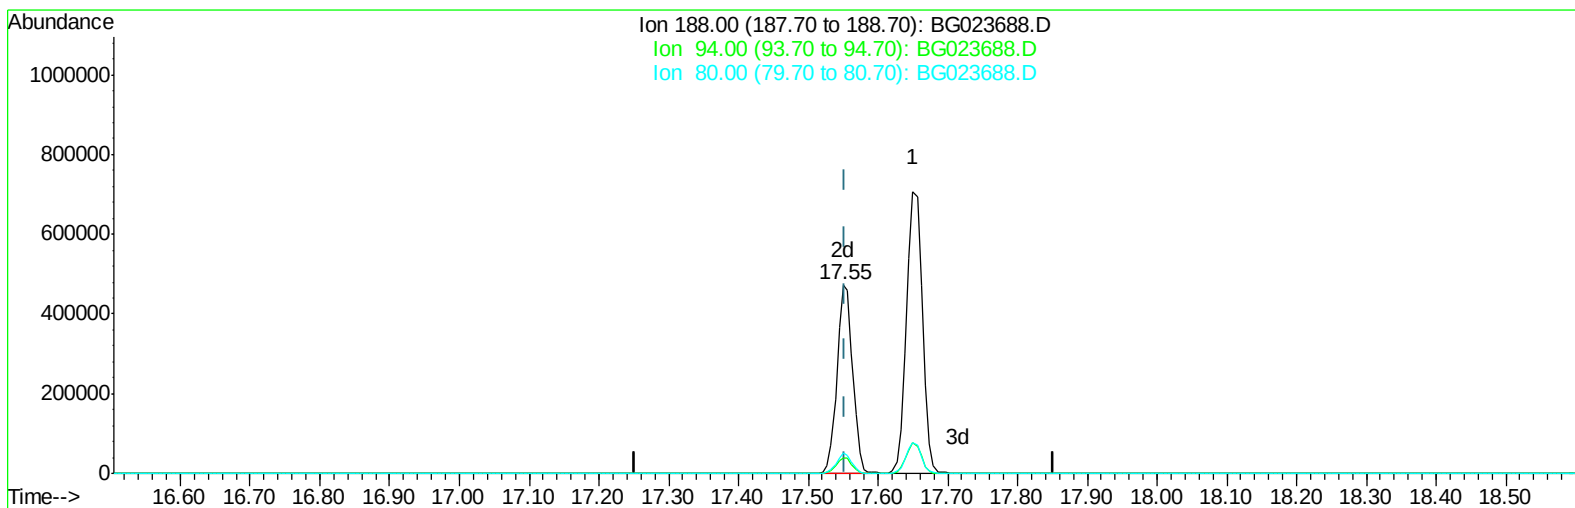

TIC: BG023688.D

(61) Phenanthrene-d10 (I)

17.550min (-0.002) 20.00ng/ul m

response 734731

Ion	Exp%	Act%
188.00	100	100
94.00	10.30	8.21#
80.00	10.90	10.86
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:07:48 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

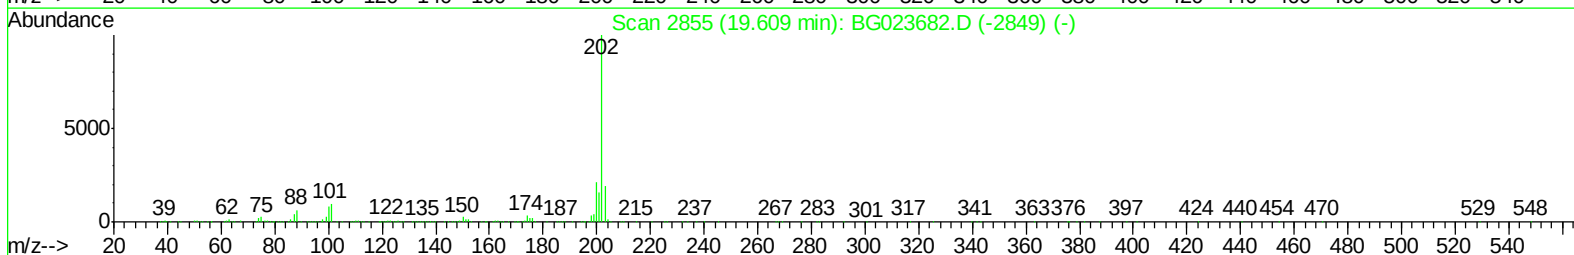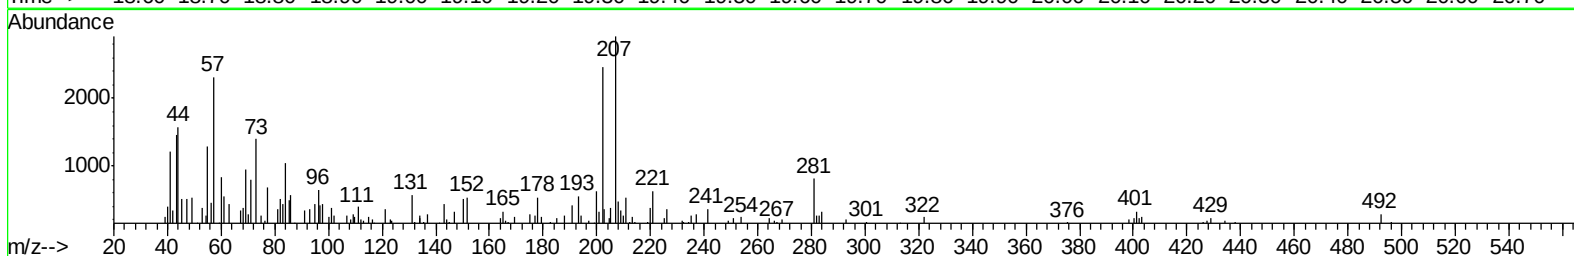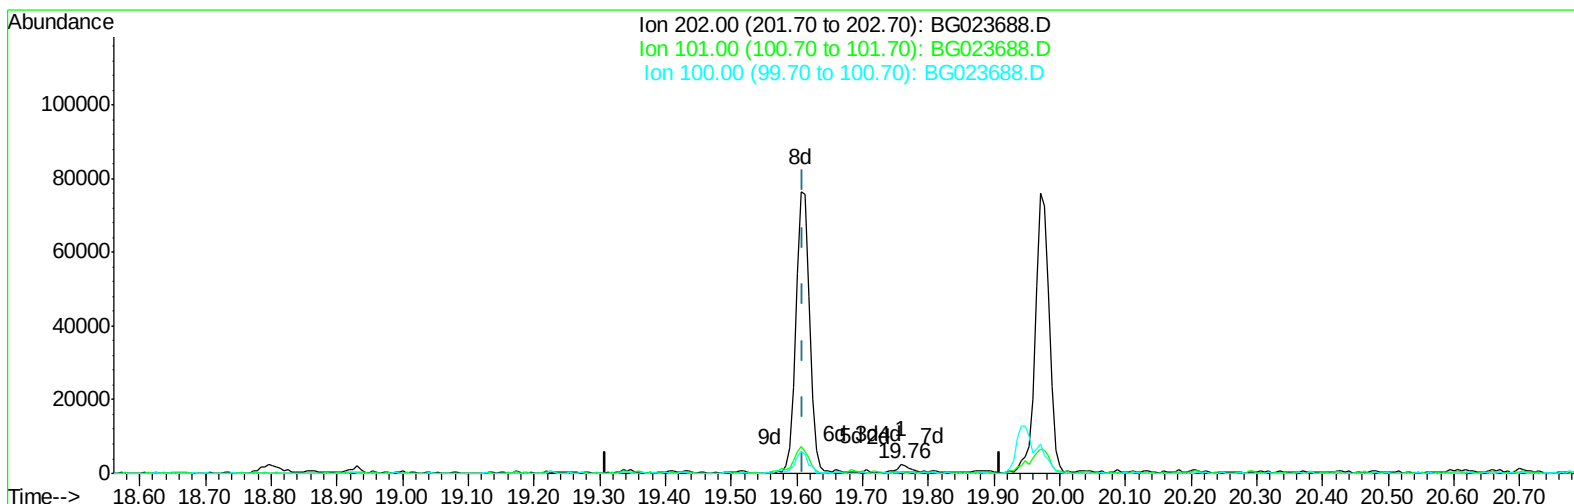

TIC: BG023688.D

(74) Fluoranthene (C)

19.759min (+0.150) 0.06ng/ul

response 2453

Ion	Exp%	Act%
202.00	100	100
101.00	13.30	15.11
100.00	10.90	9.92
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:07:48 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

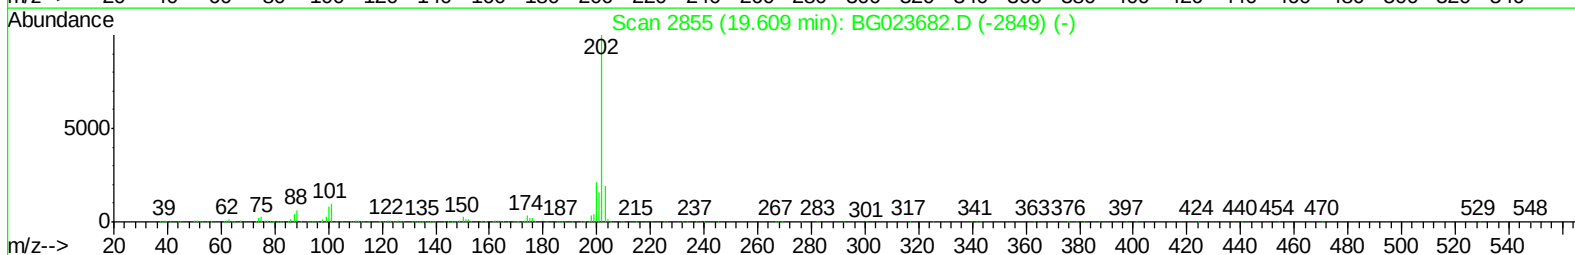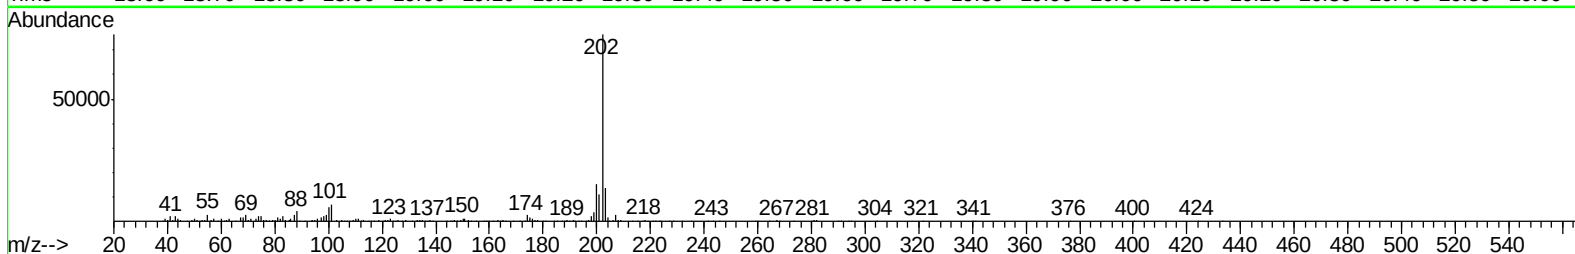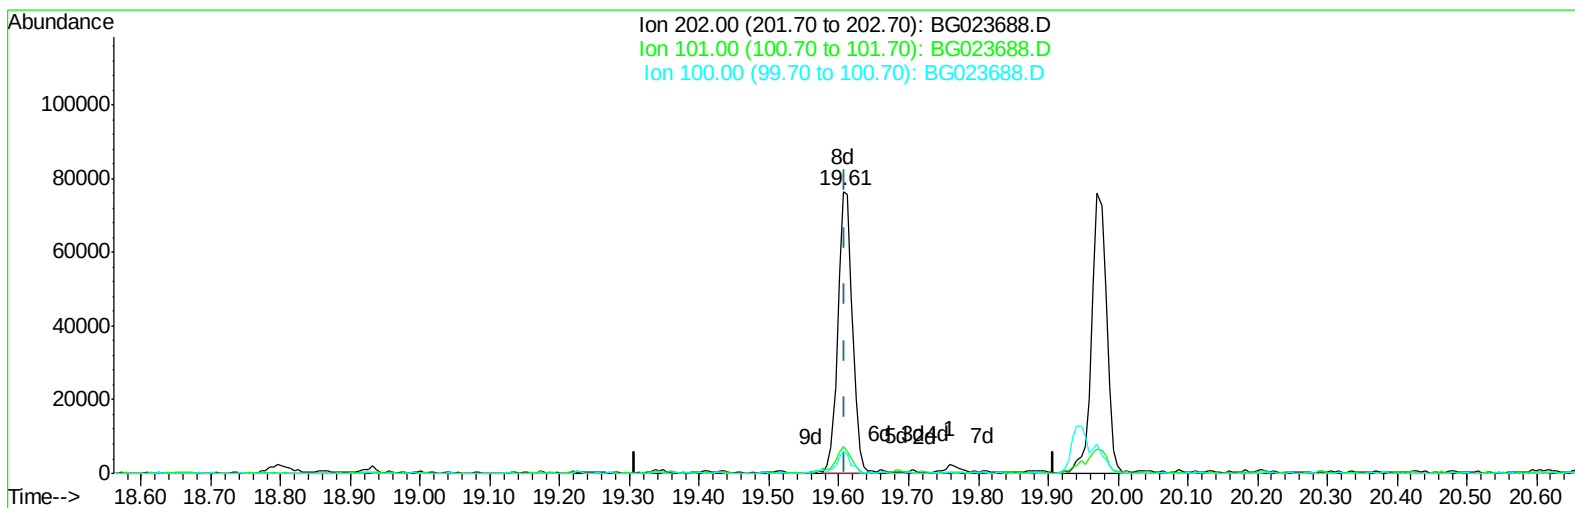

TIC: BG023688.D

(74) Fluoranthene (C)

19.606min (-0.002) 2.86ng/ul m

response 111358

Ion	Exp%	Act%
202.00	100	100
101.00	13.30	9.34#
100.00	10.90	7.80#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:07:48 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

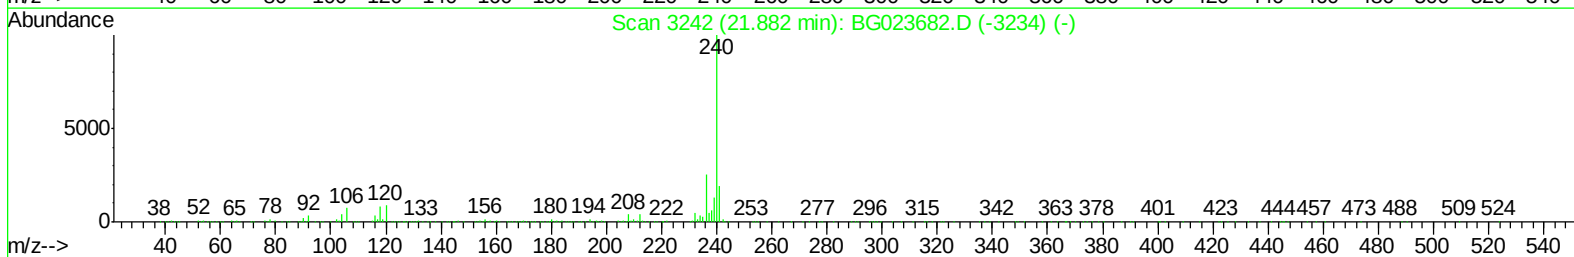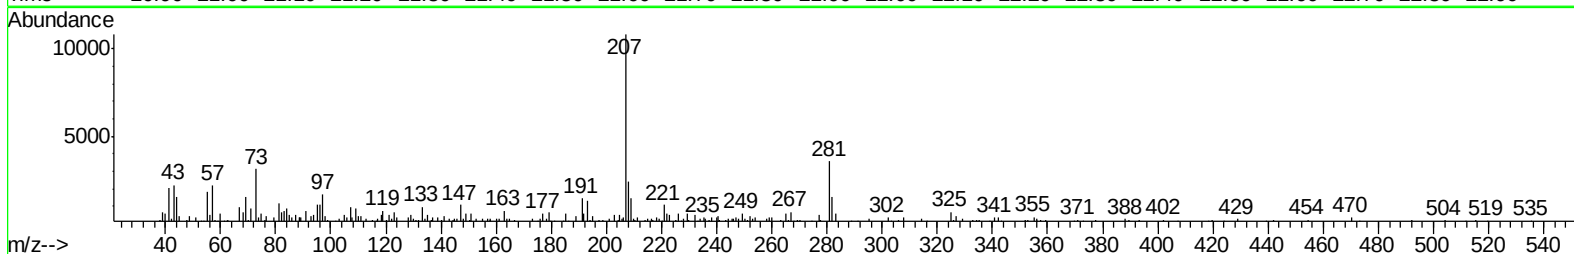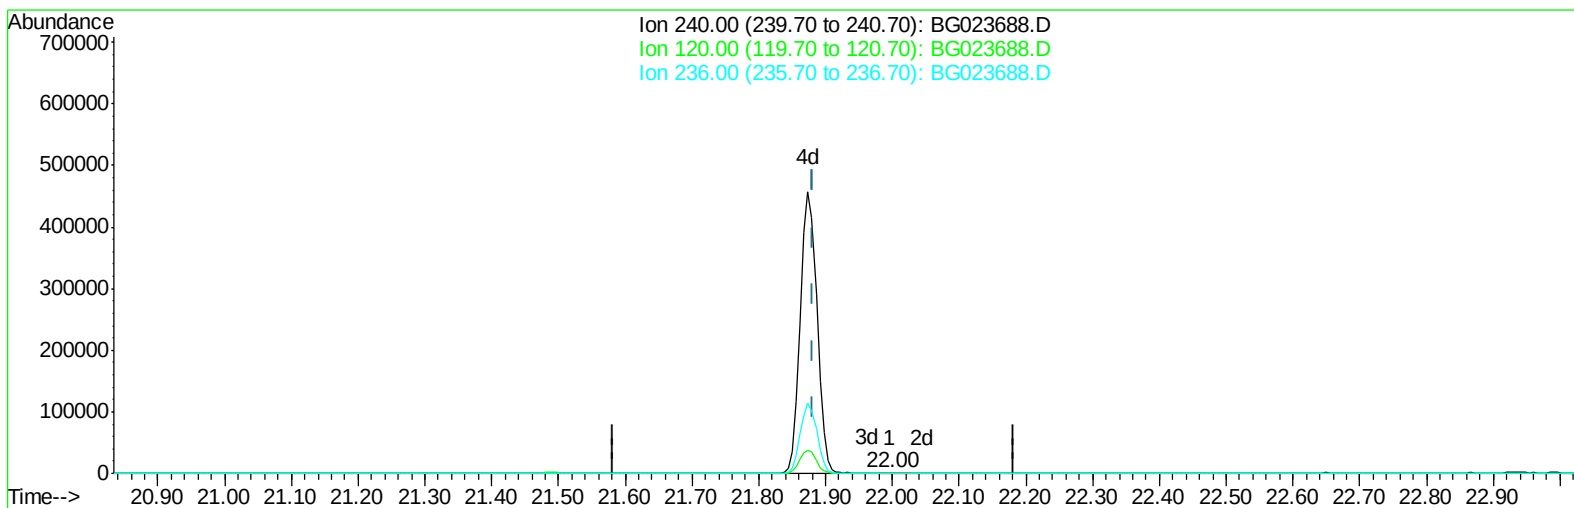

TIC: BG023688.D

(75) Chrysene-d12 (I)

21.997min (+0.115) 20.00ng/ul

response 1441

Ion	Exp%	Act%
240.00	100	100
120.00	14.40	23.84#
236.00	26.10	35.09#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:07:48 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

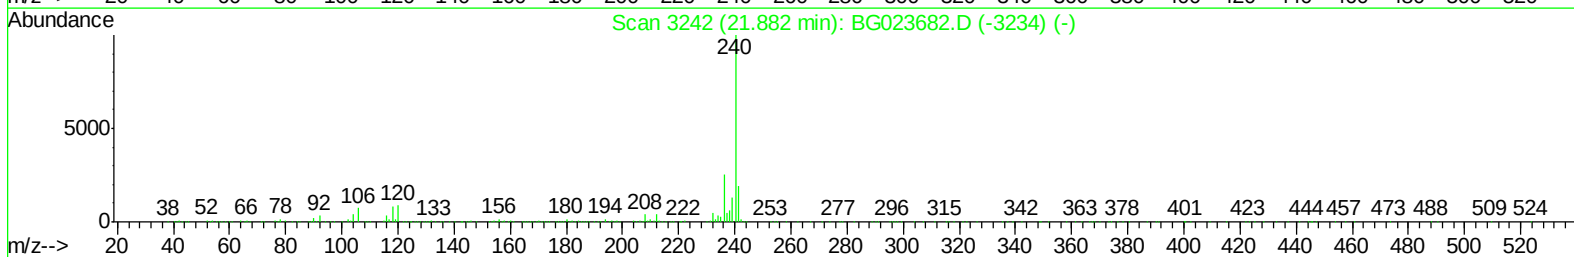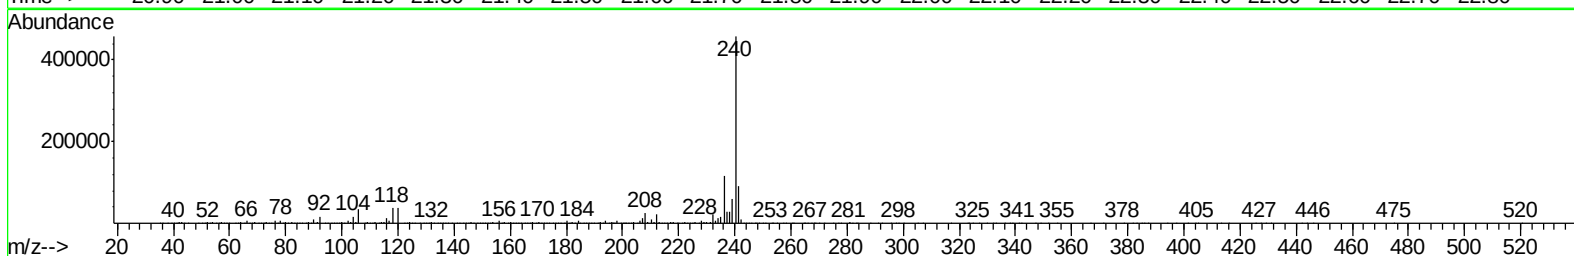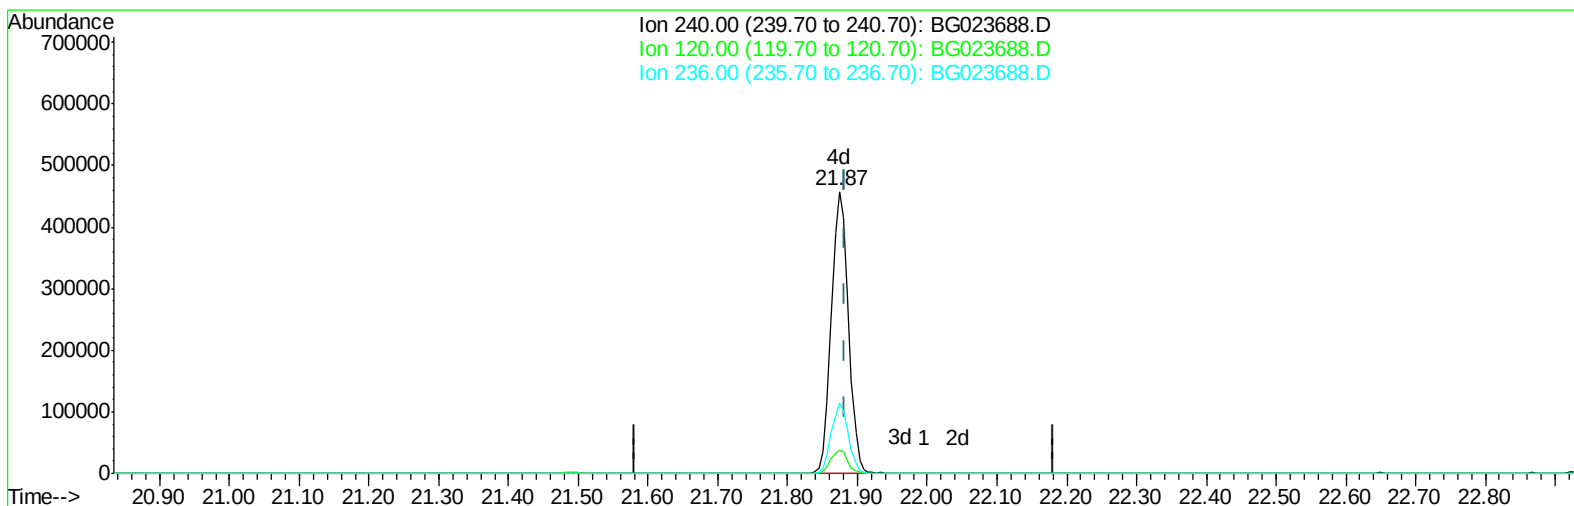

TIC: BG023688.D

(75) Chrysene-d12 (I)

21.874min (-0.008) 20.00ng/ul m

response 777822

Ion	Exp%	Act%
240.00	100	100
120.00	14.40	8.05#
236.00	26.10	25.09
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:10:10 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

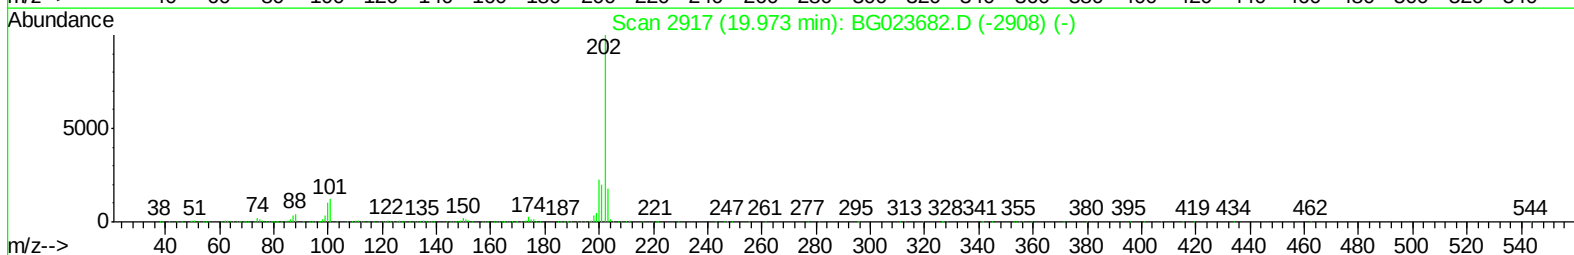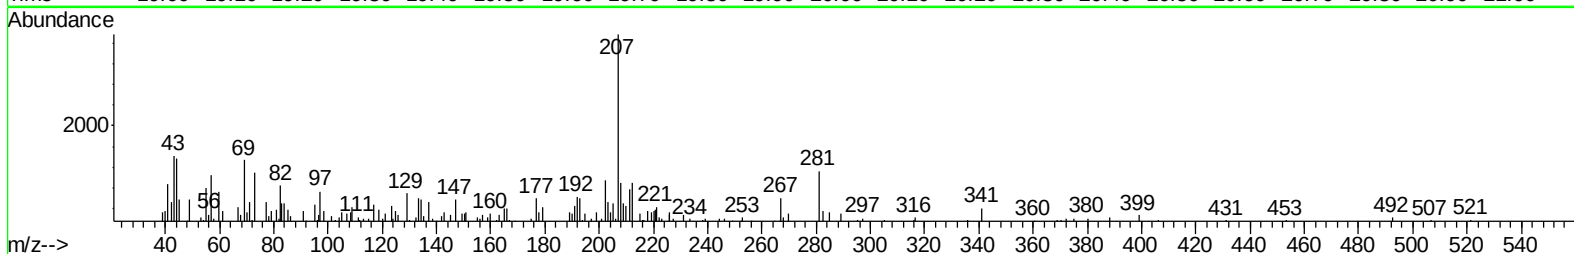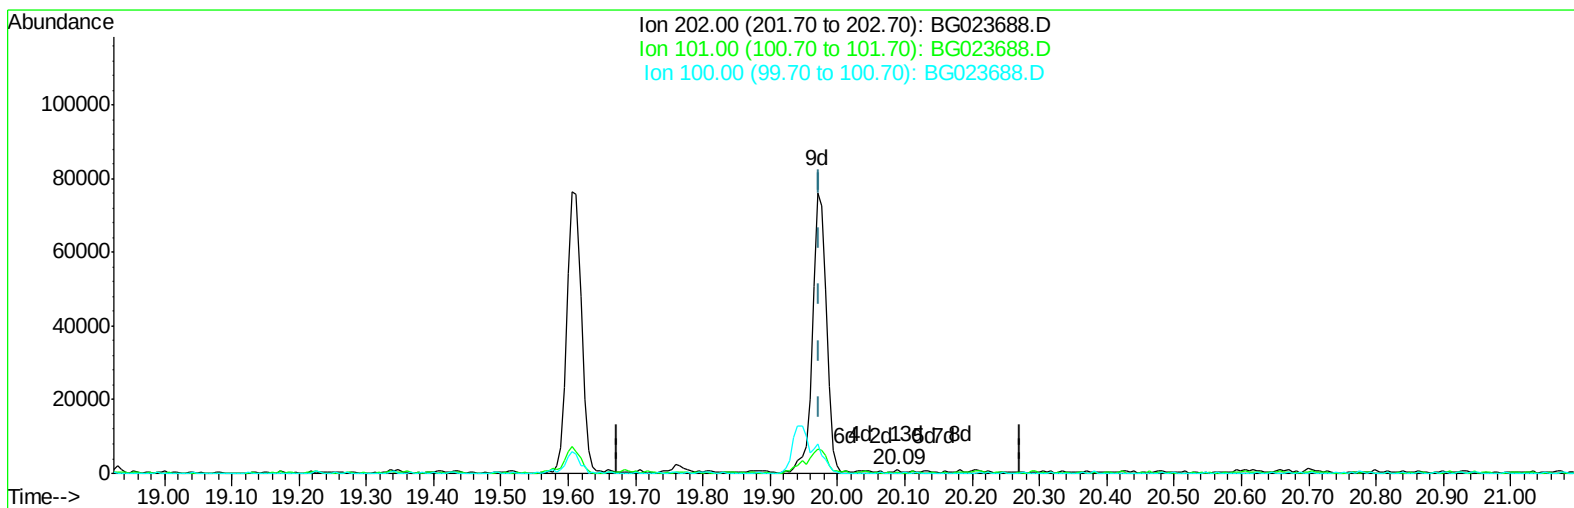

TIC: BG023688.D

(77) Pyrene

20.088min (+0.115) 0.02ng/ul

response 725

Ion	Exp%	Act%
202.00	100	100
101.00	15.60	26.43#
100.00	12.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:10:10 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

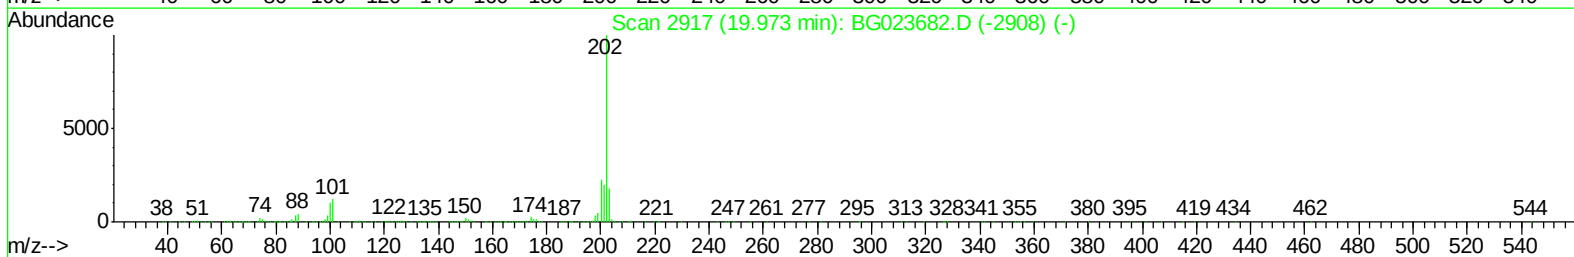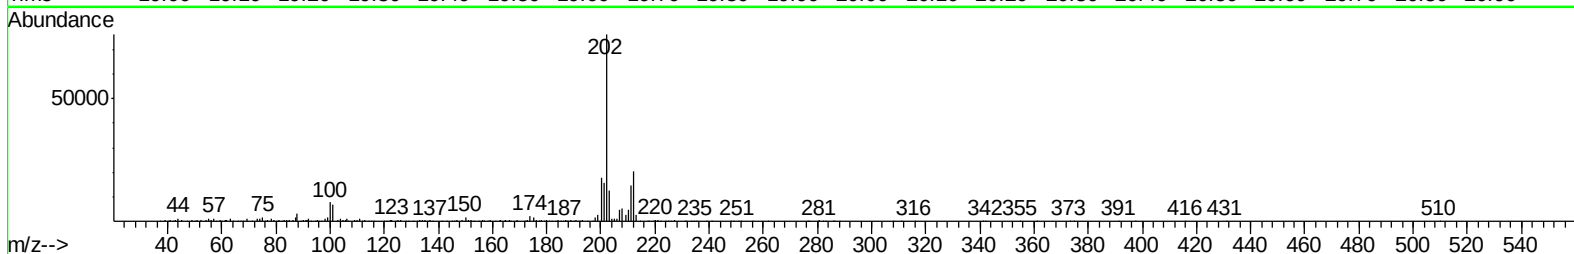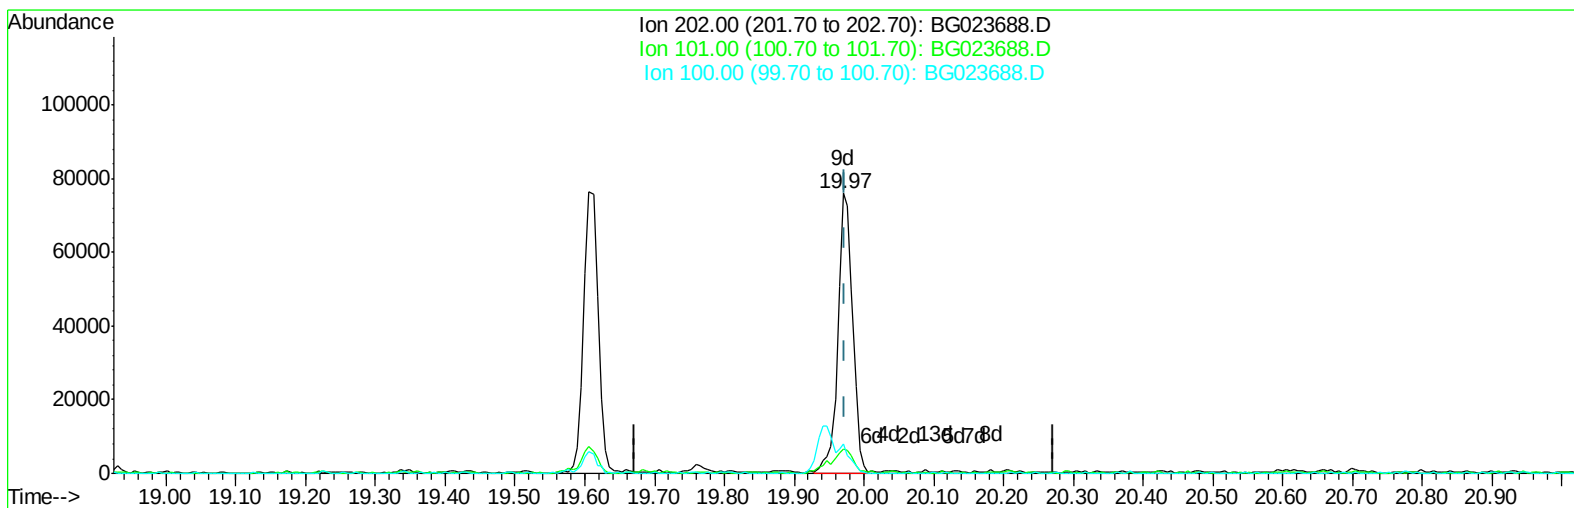

TIC: BG023688.D

(77) Pyrene

19.971min (-0.002) 2.34ng/ul m

response 112359

Ion	Exp%	Act%
202.00	100	100
101.00	15.60	8.91#
100.00	12.80	10.30
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:10:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

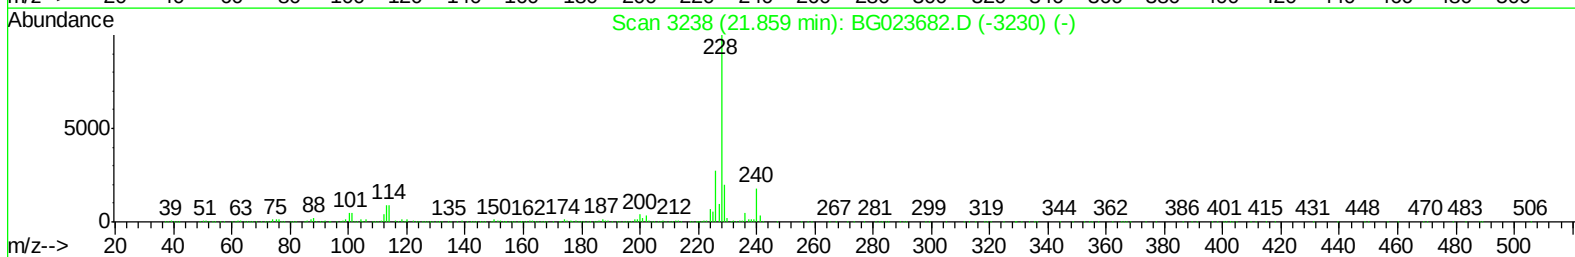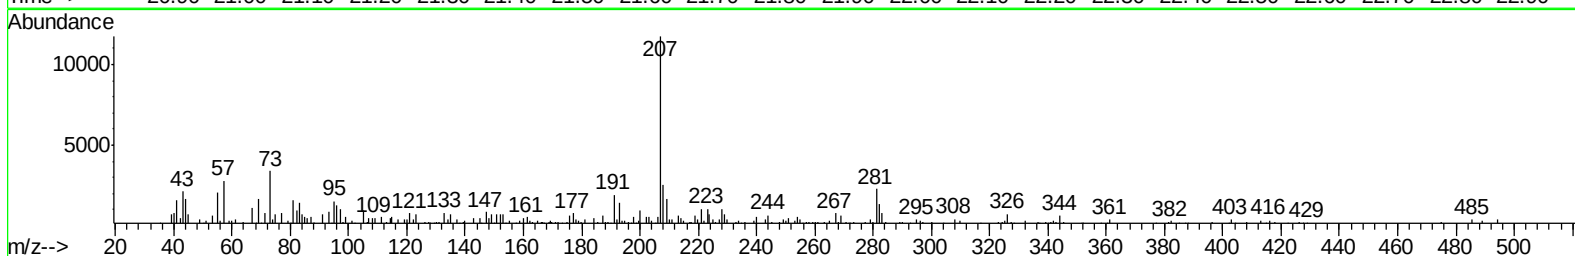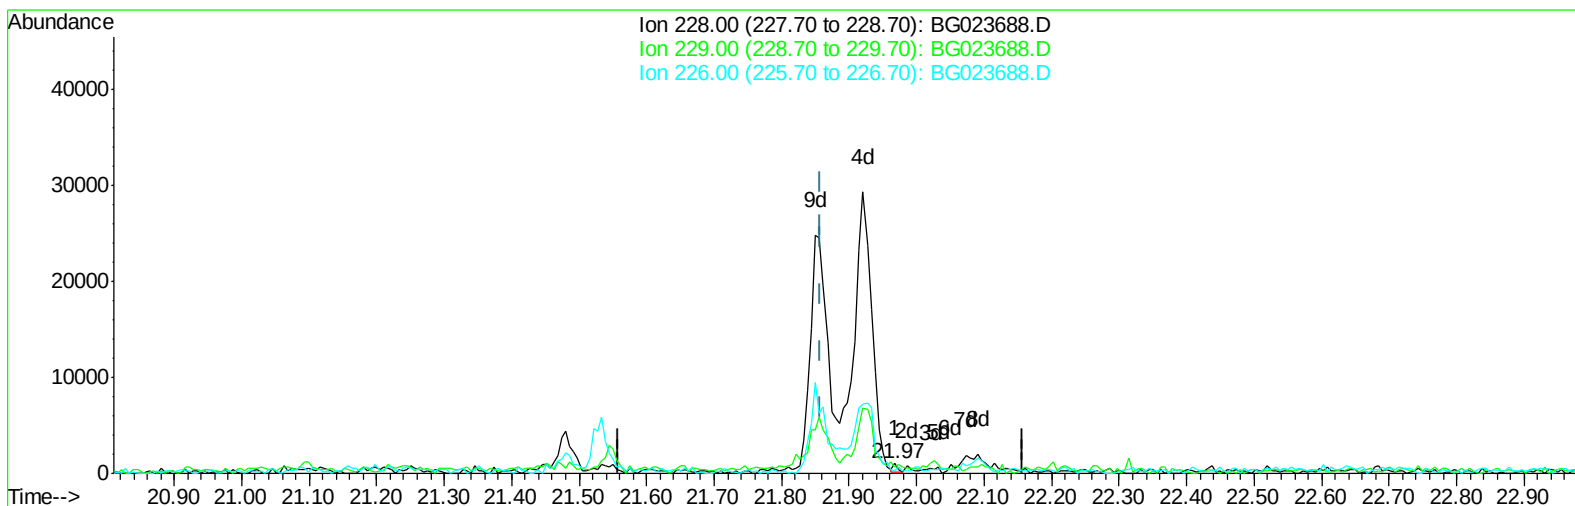

TIC: BG023688.D

(80) Benzo(a)anthracene
21.968min (+0.109) 0.01ng/ul

response 410

Ion	Exp%	Act%
228.00	100	100
229.00	19.30	68.03#
226.00	28.50	24.98
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:10:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

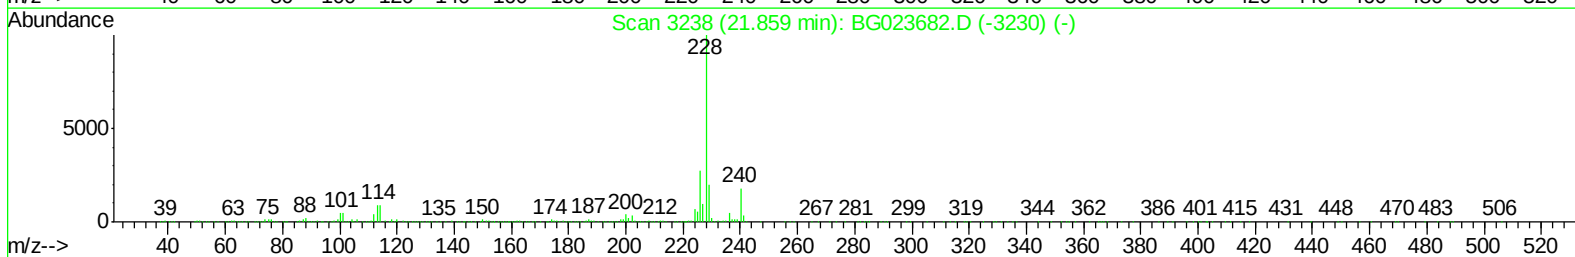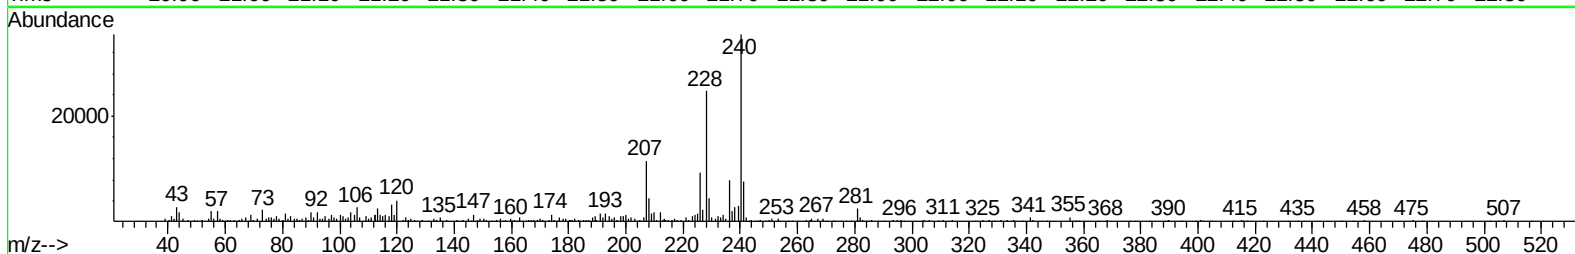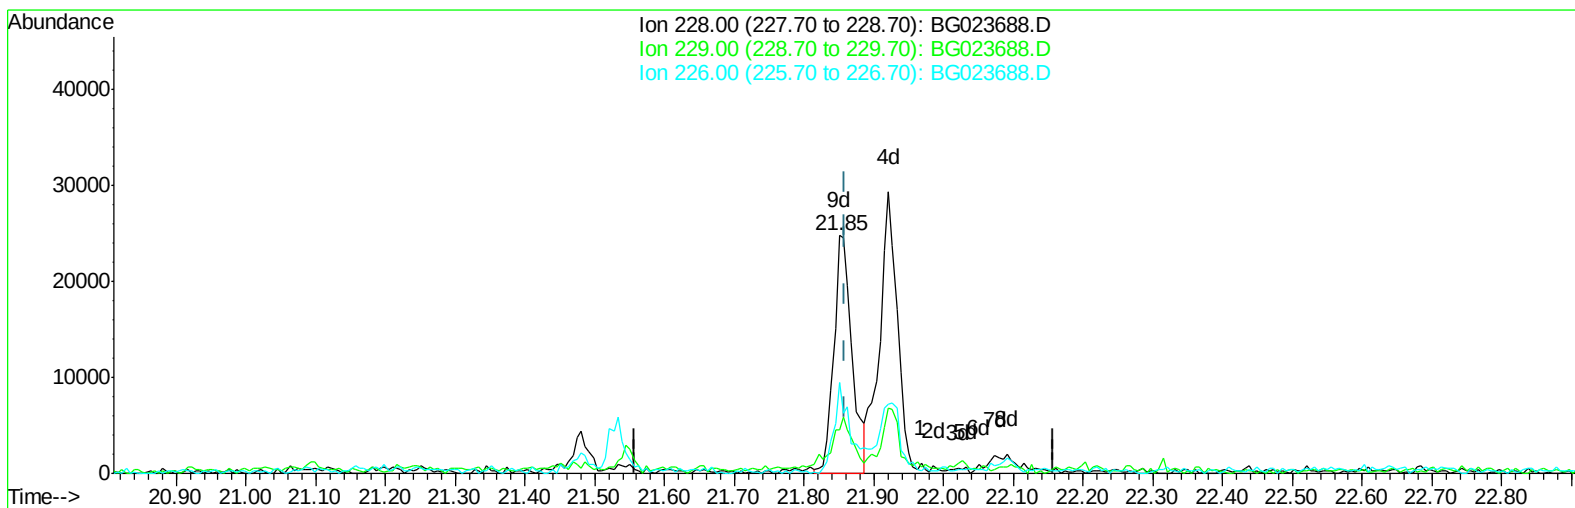

TIC: BG023688.D

(80) Benzo(a)anthracene

21.850min (-0.008) 1.03ng/ul m

response 45274

Ion	Exp%	Act%
228.00	100	100
229.00	19.30	18.38
226.00	28.50	38.03#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Quant Time: Aug 15 13:10:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

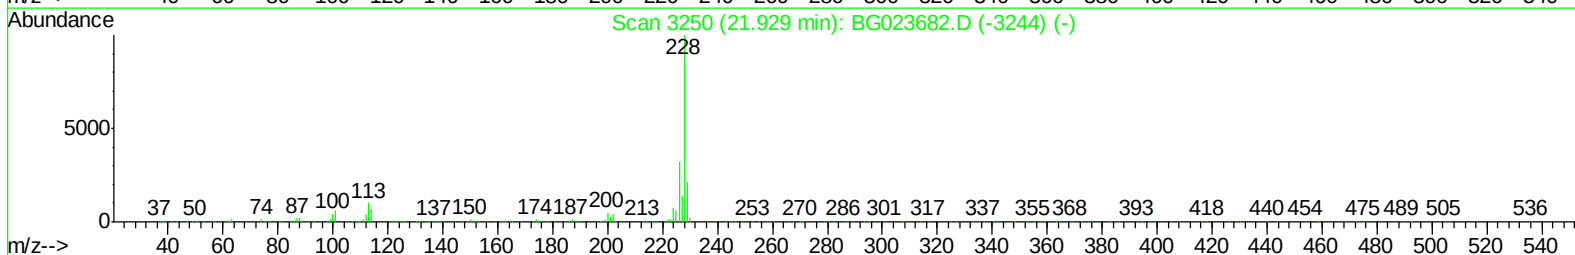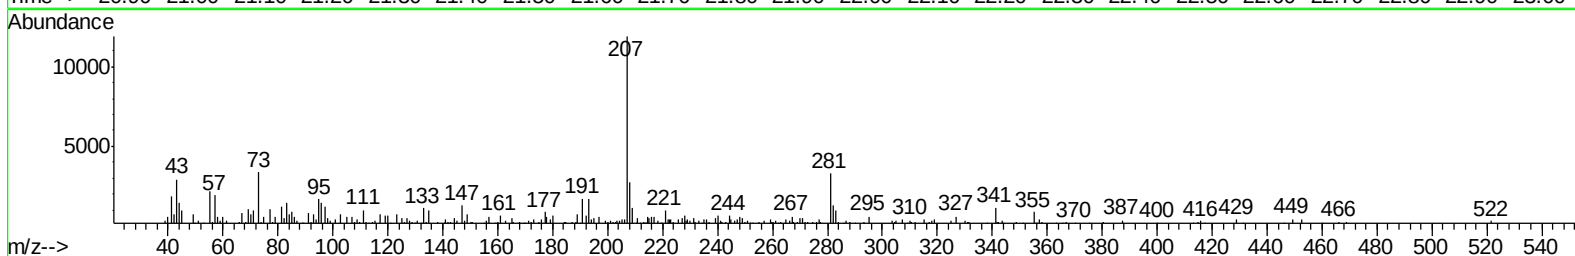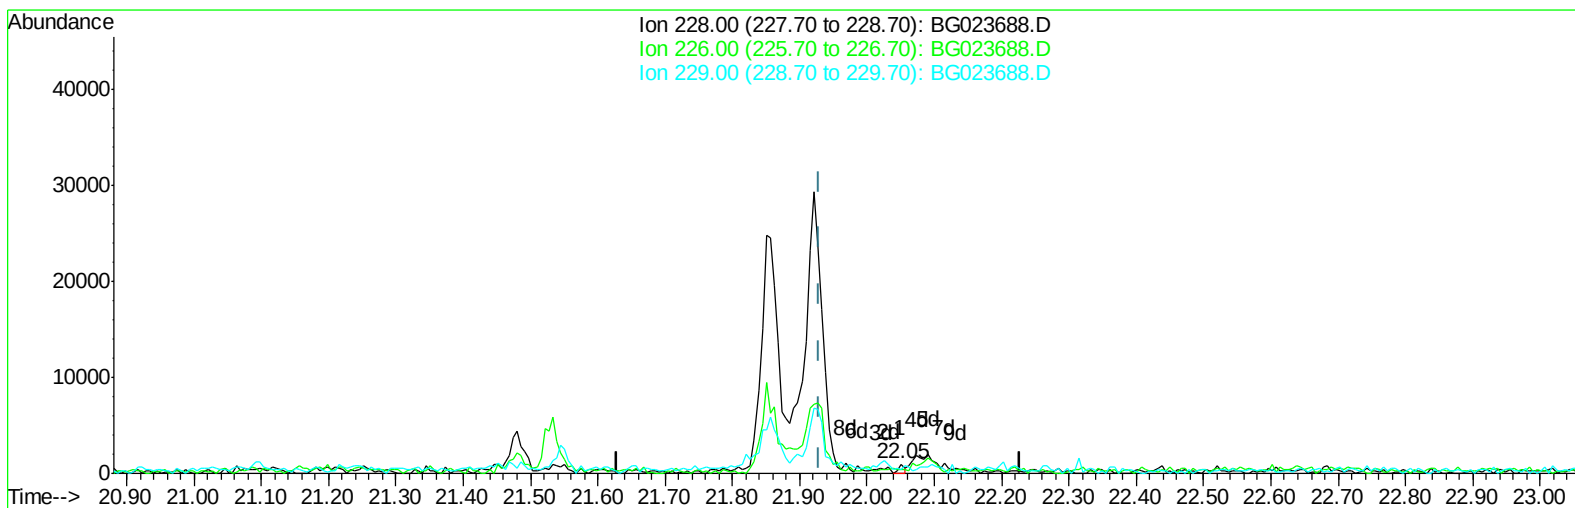

TIC: BG023688.D

(82) Chrysene

22.050min (+0.121) 0.02ng/ul

response 646

Ion	Exp%	Act%
228.00	100	100
226.00	30.30	41.09#
229.00	18.80	38.07#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:10:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

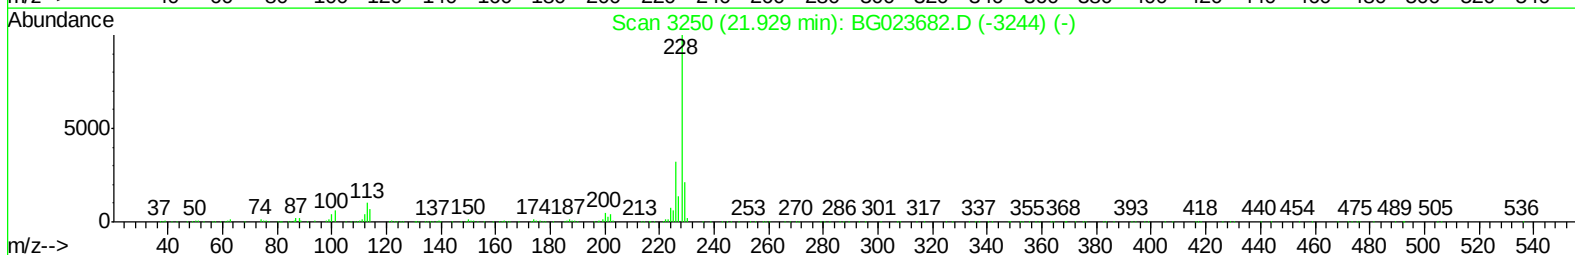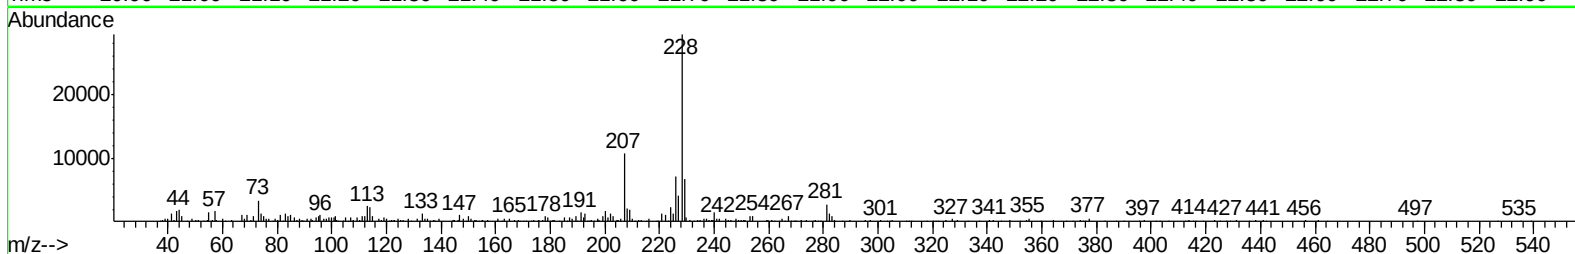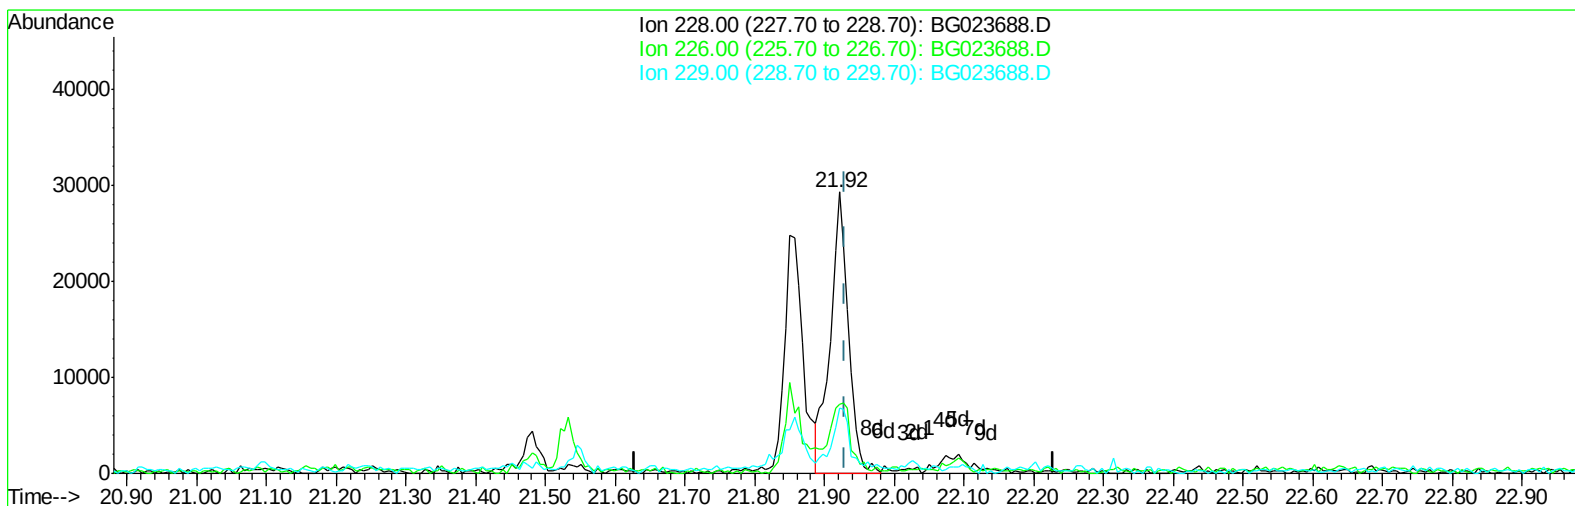

TIC: BG023688.D

(82) Chrysene

21.921min (-0.008) 1.33ng/ul m

response 53128

Ion	Exp%	Act%
228.00	100	100
226.00	30.30	24.45
229.00	18.80	23.18#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:10:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

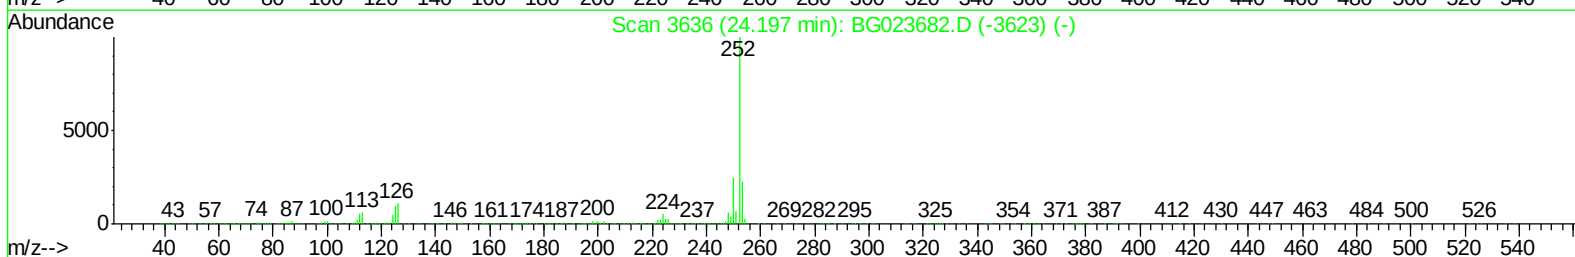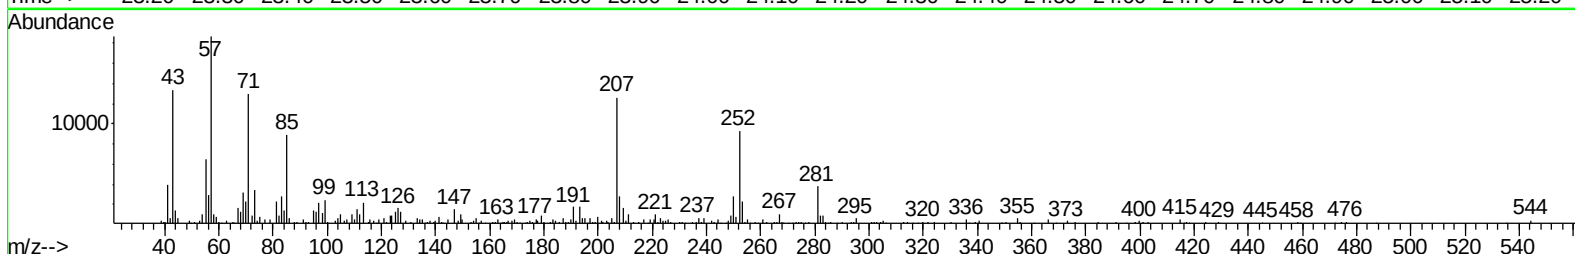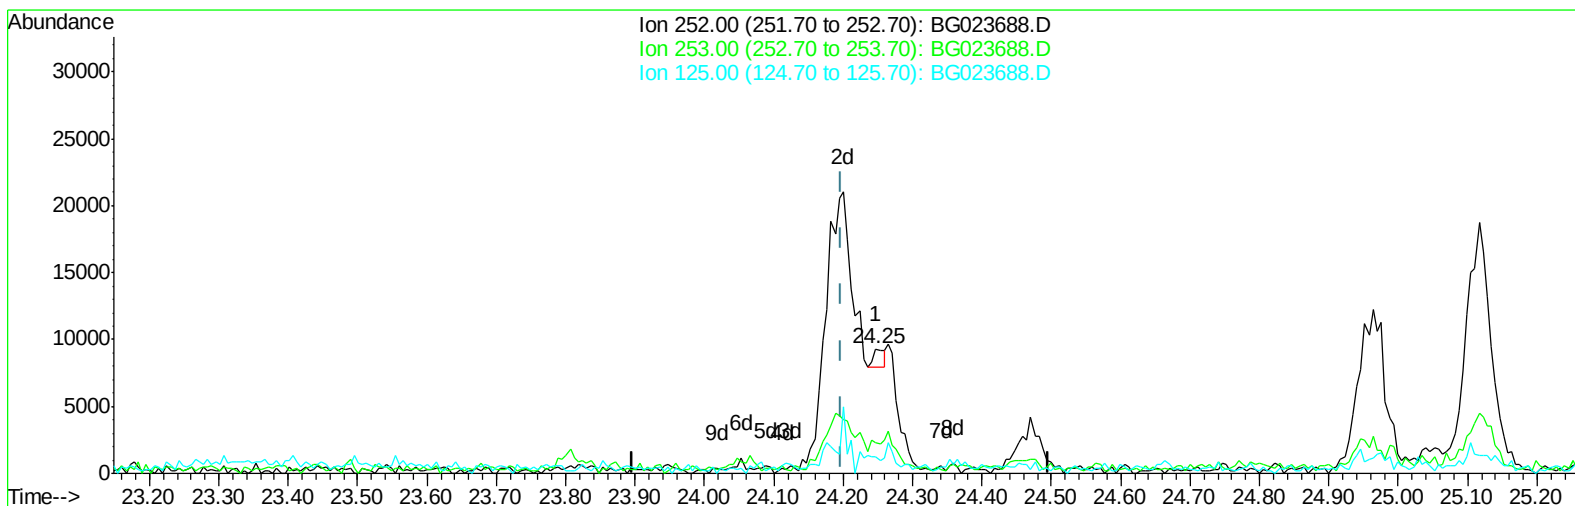

TIC: BG023688.D

(85) Benzo(b)fluoranthene

24.247min (+0.050) 0.04ng/ul

response 1572

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	25.05
125.00	13.50	13.77
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Quant Time: Aug 15 13:10:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

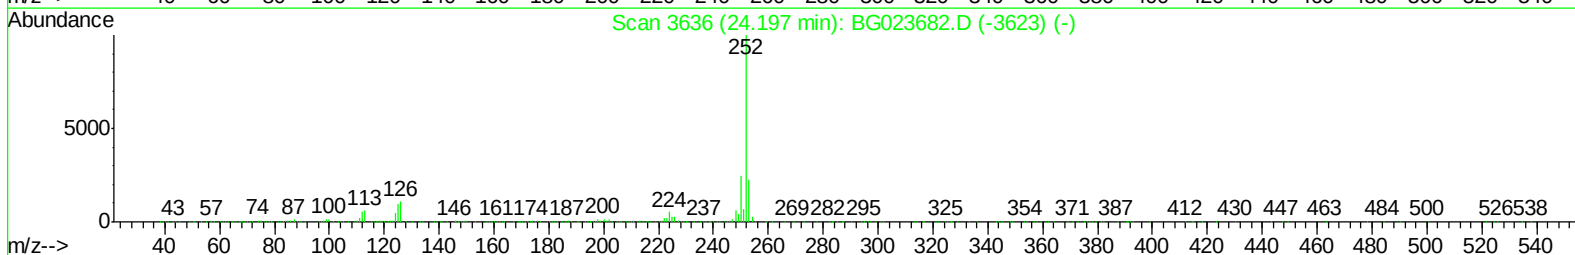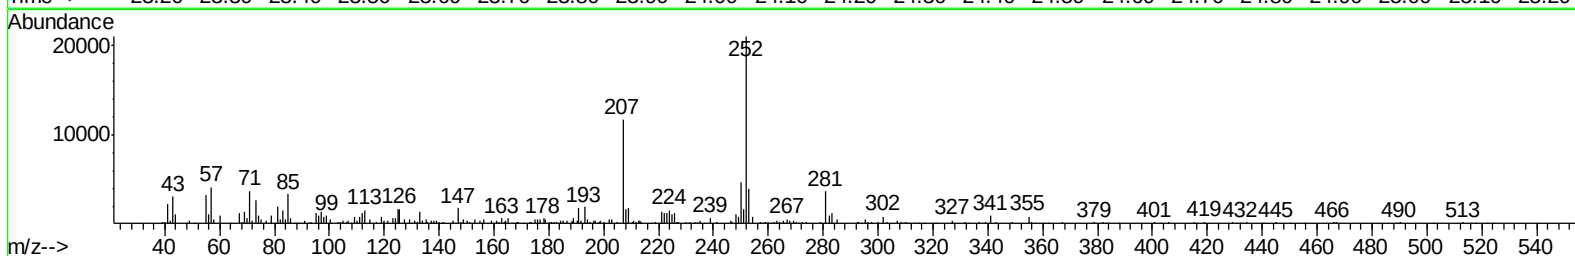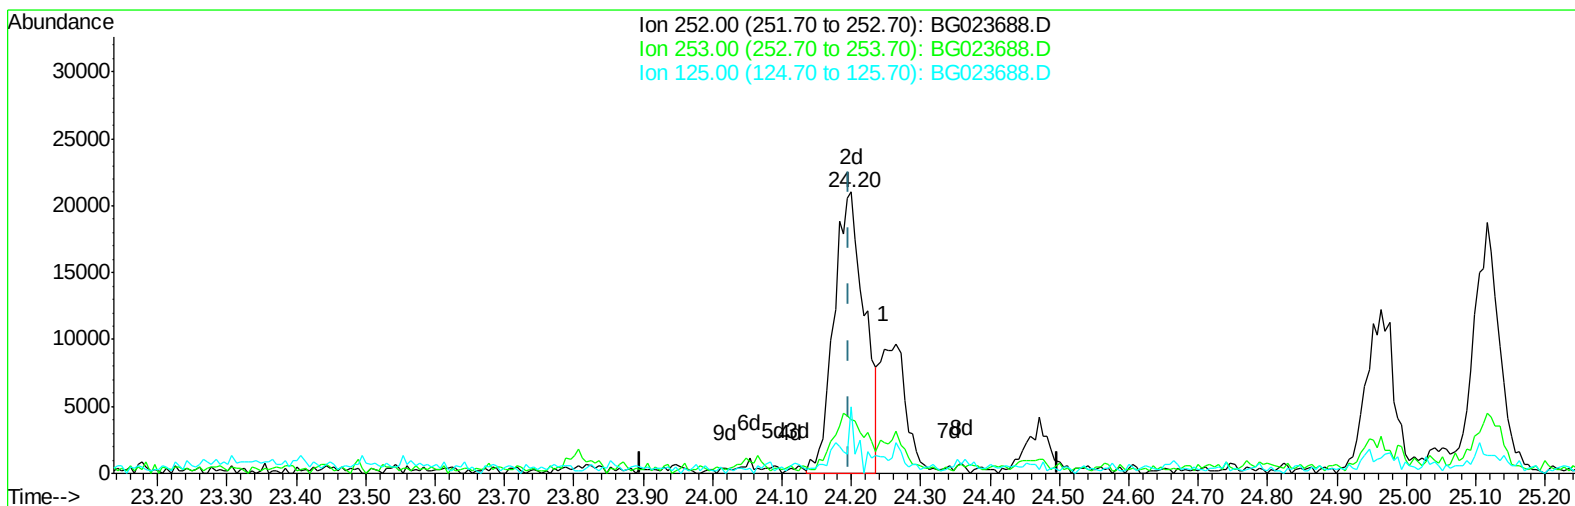

TIC: BG023688.D

(85) Benzo(b)fluoranthene

24.200min (+0.003) 1.46ng/ul m

response 65077

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	19.05
125.00	13.50	8.24#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:42:59 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

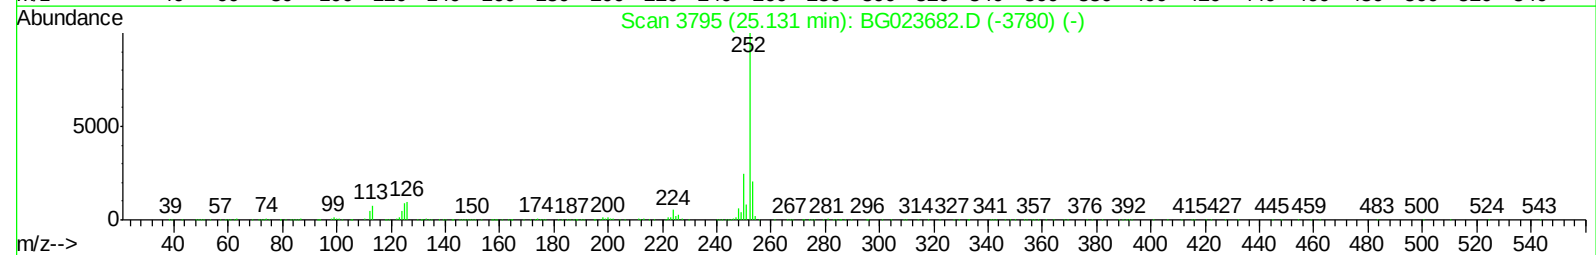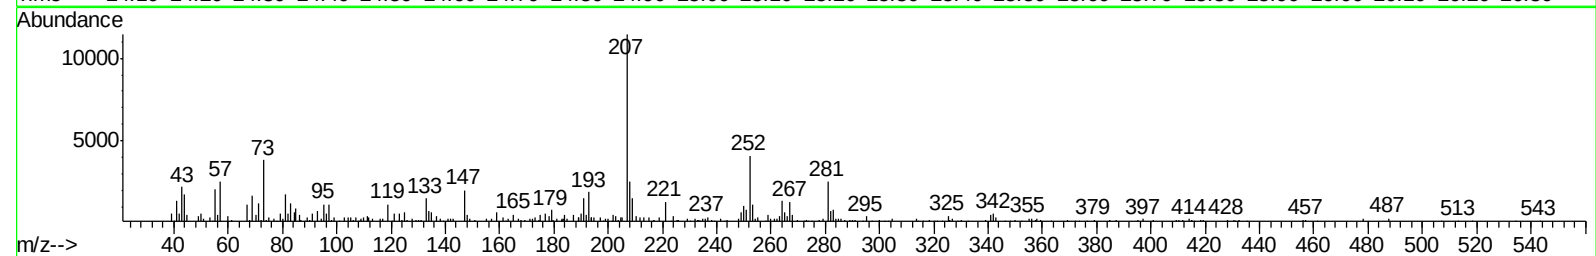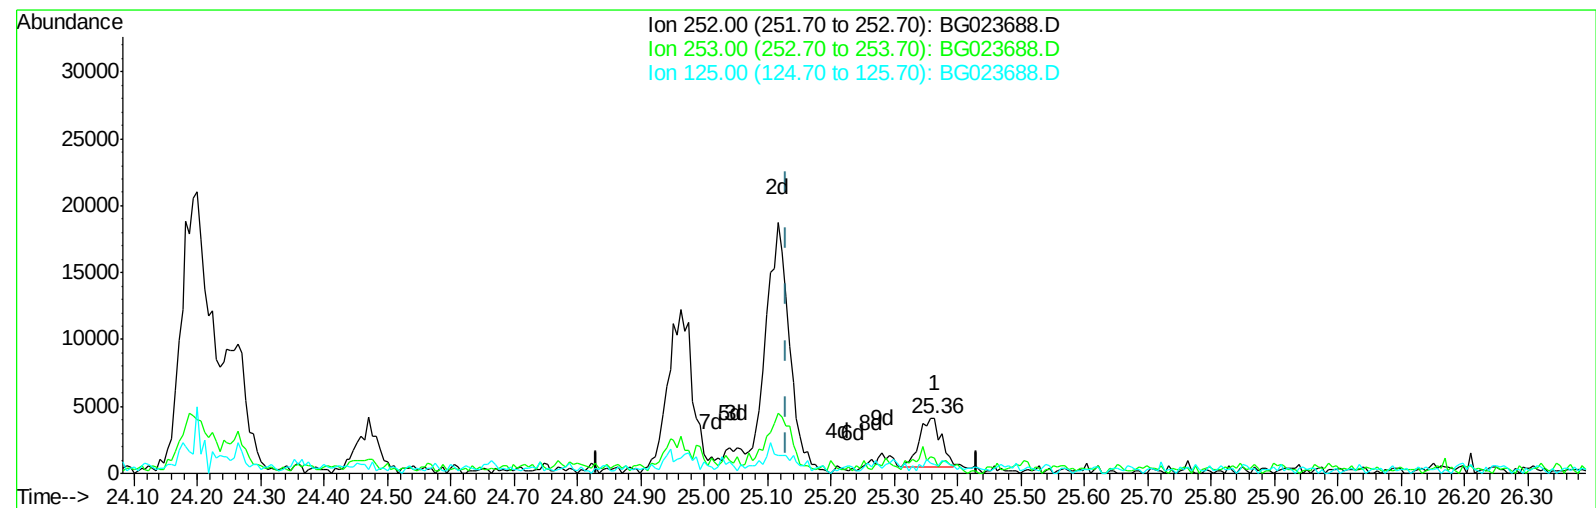

TIC: BG023688.D

(88) Benzo(a)pyrene (C)

25.363min (+0.233) 0.21ng/ul

response 8872

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	28.03
125.00	15.00	16.18
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:42:59 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

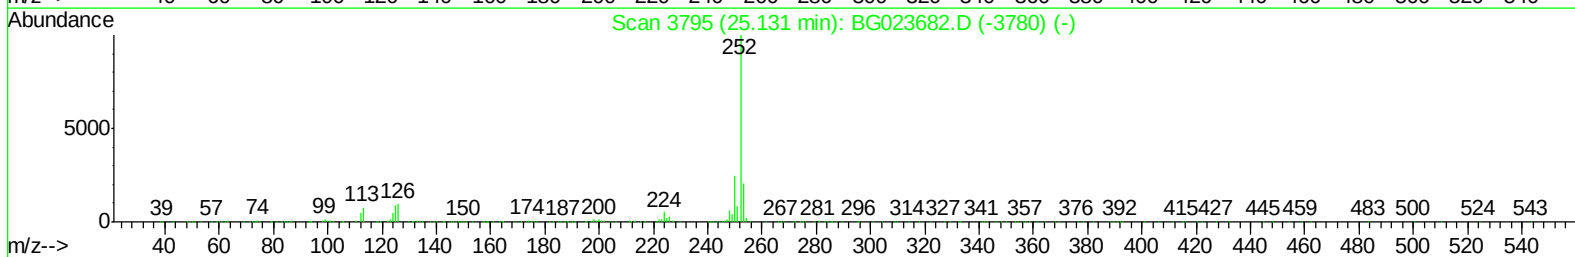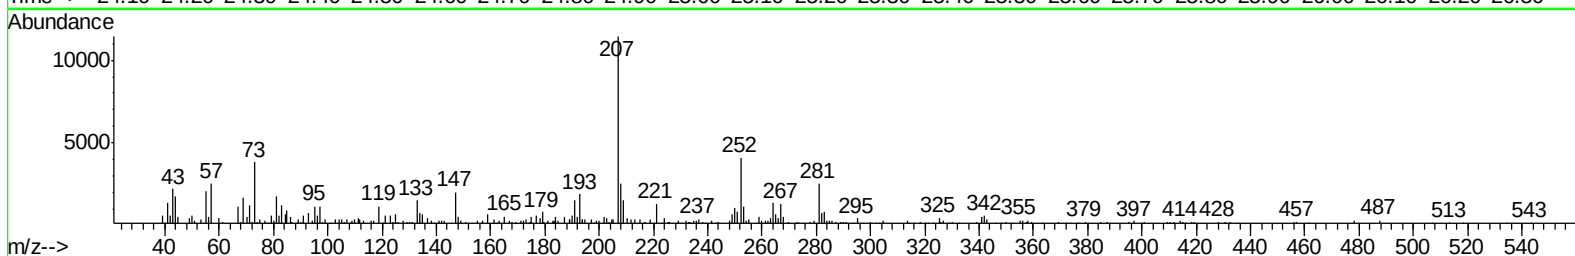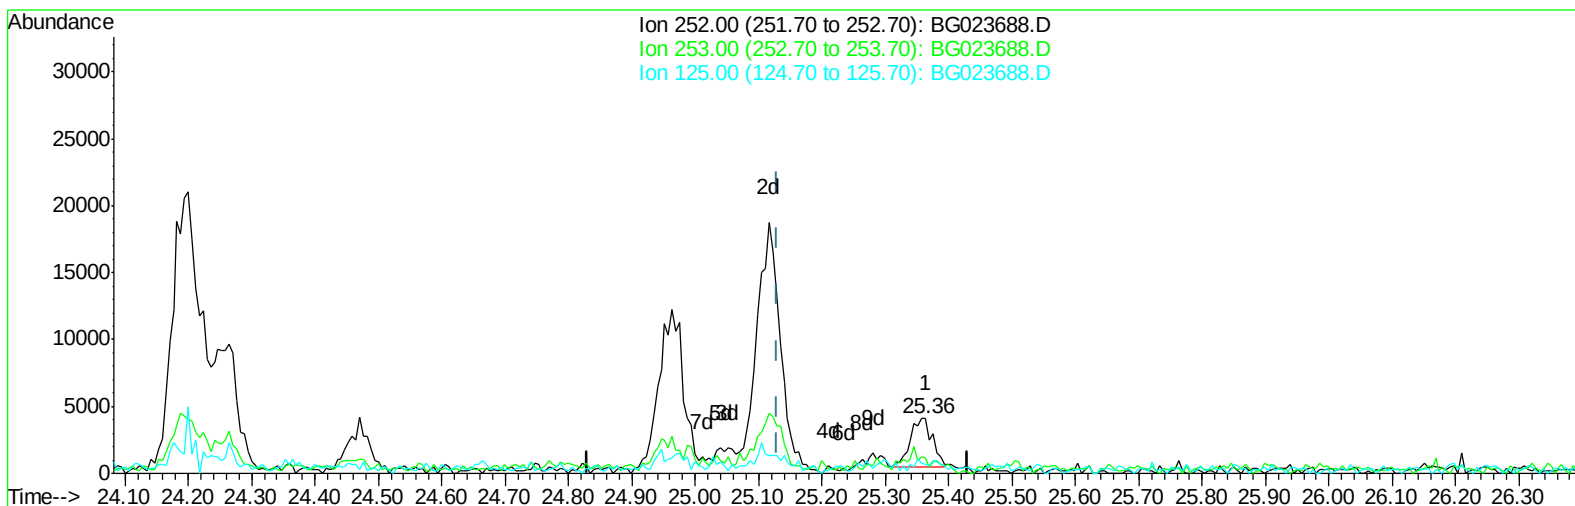

TIC: BG023688.D

(88) Benzo(a)pyrene (C)

25.363min (+0.233) 0.21ng/ul

response 8872

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	28.03
125.00	15.00	16.18
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:42:59 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

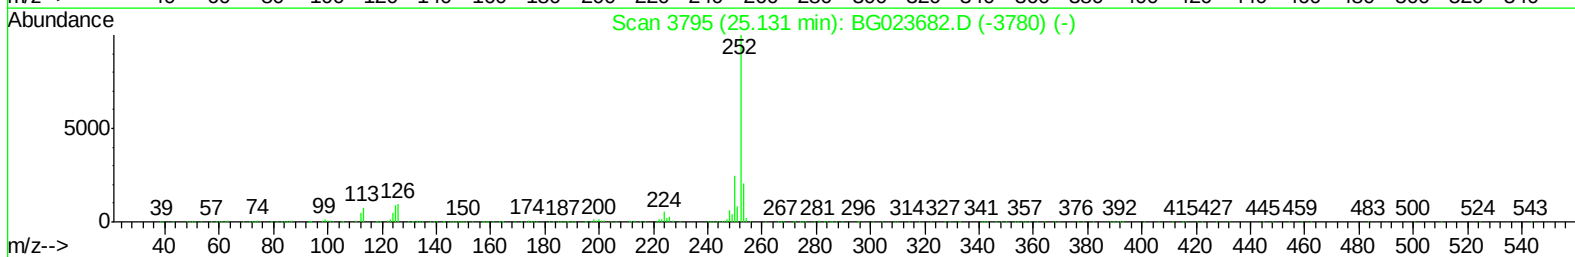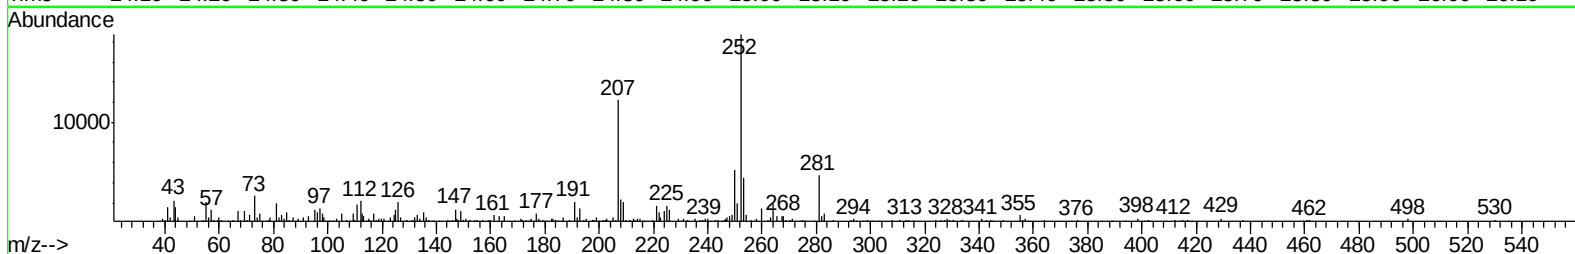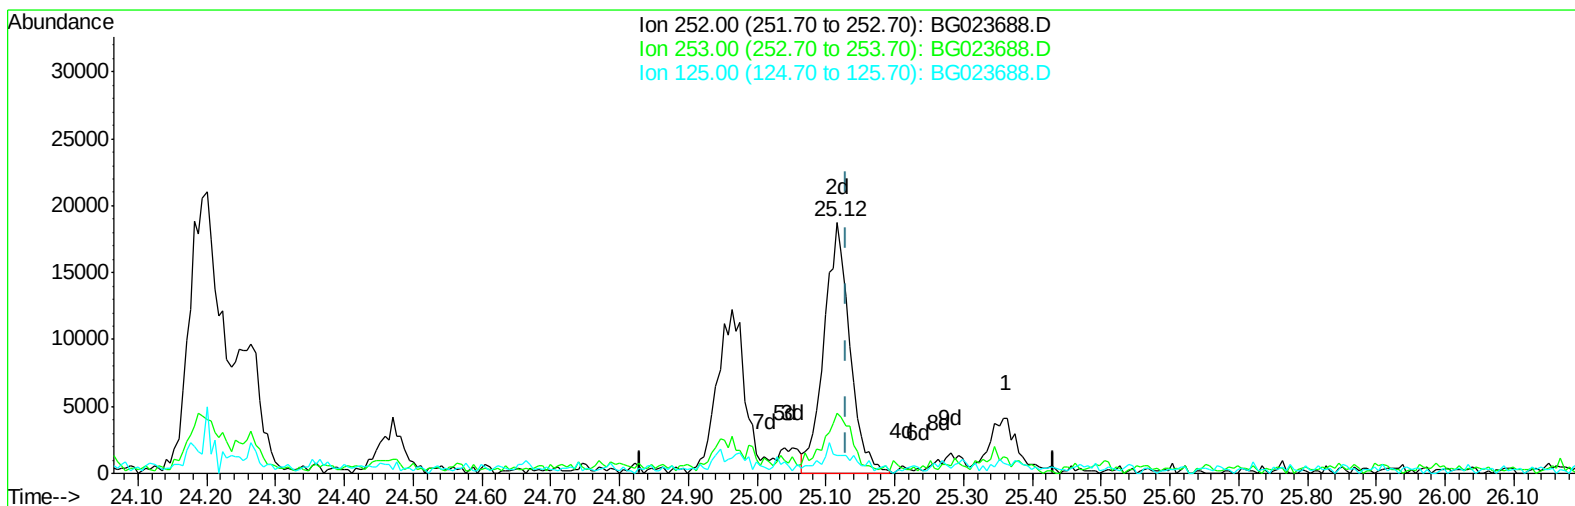

TIC: BG023688.D

(88) Benzo(a)pyrene (C)

25.116min (-0.014) 1.13ng/ul m

response 48637

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	23.83
125.00	15.00	7.04#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:44:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

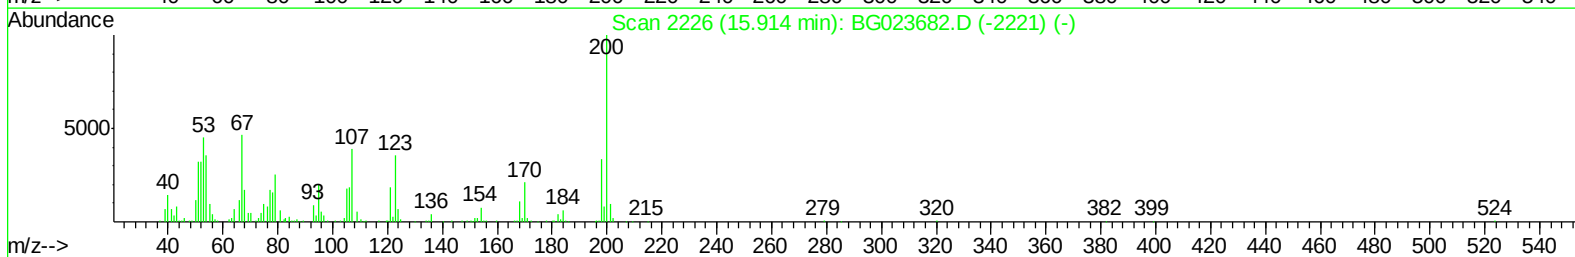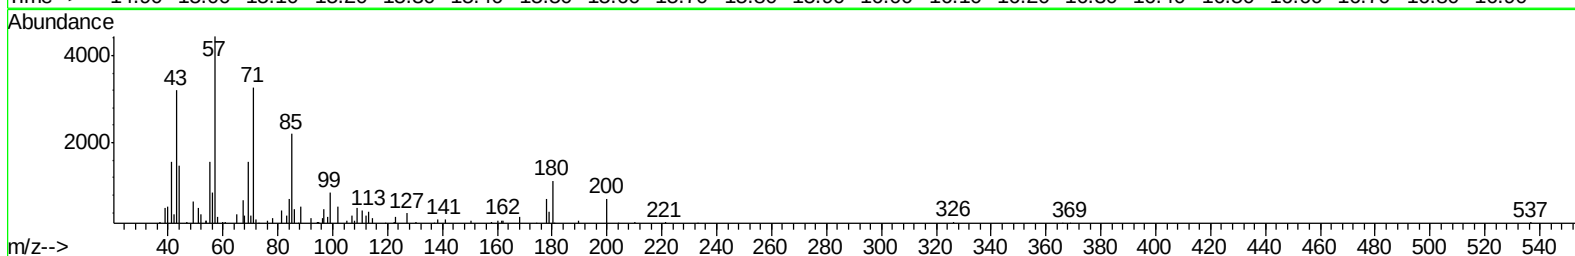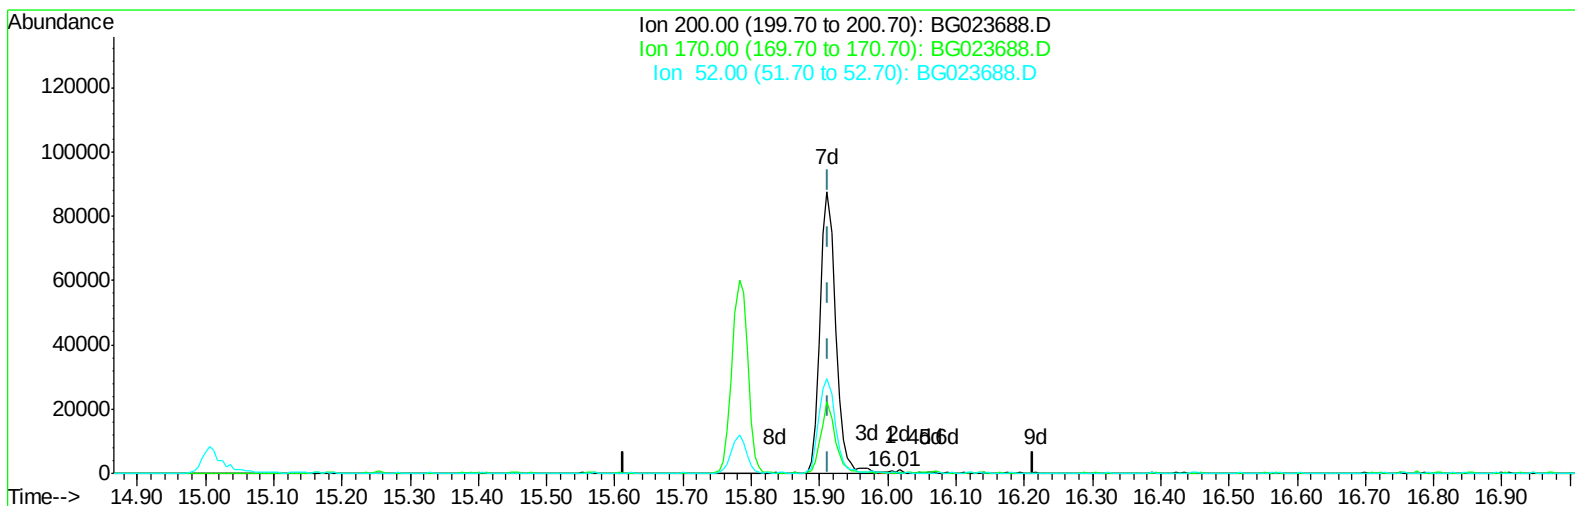

TIC: BG023688.D

(62) 4,6-Dinitro-2-methylphenol-d2 (S)

16.005min (+0.092) 0.15ng/ul

response 728

Ion	Exp%	Act%
200.00	100	100
170.00	15.20	0.00#
52.00	32.20	50.91#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:44:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

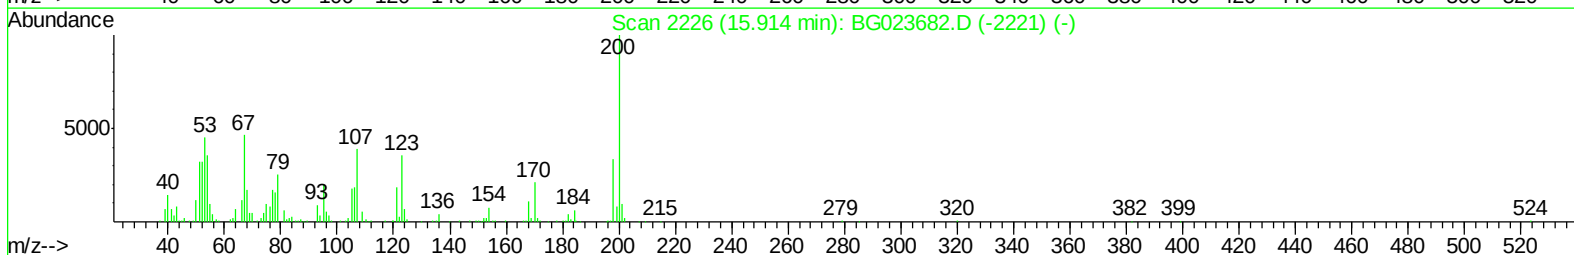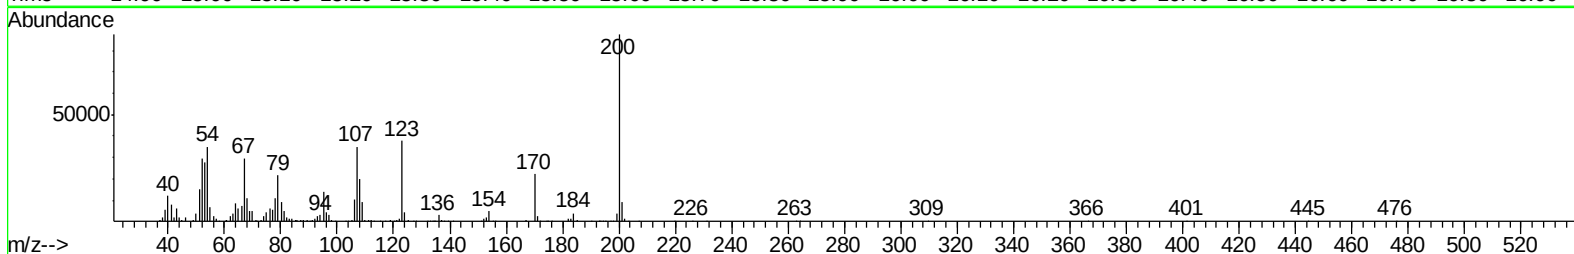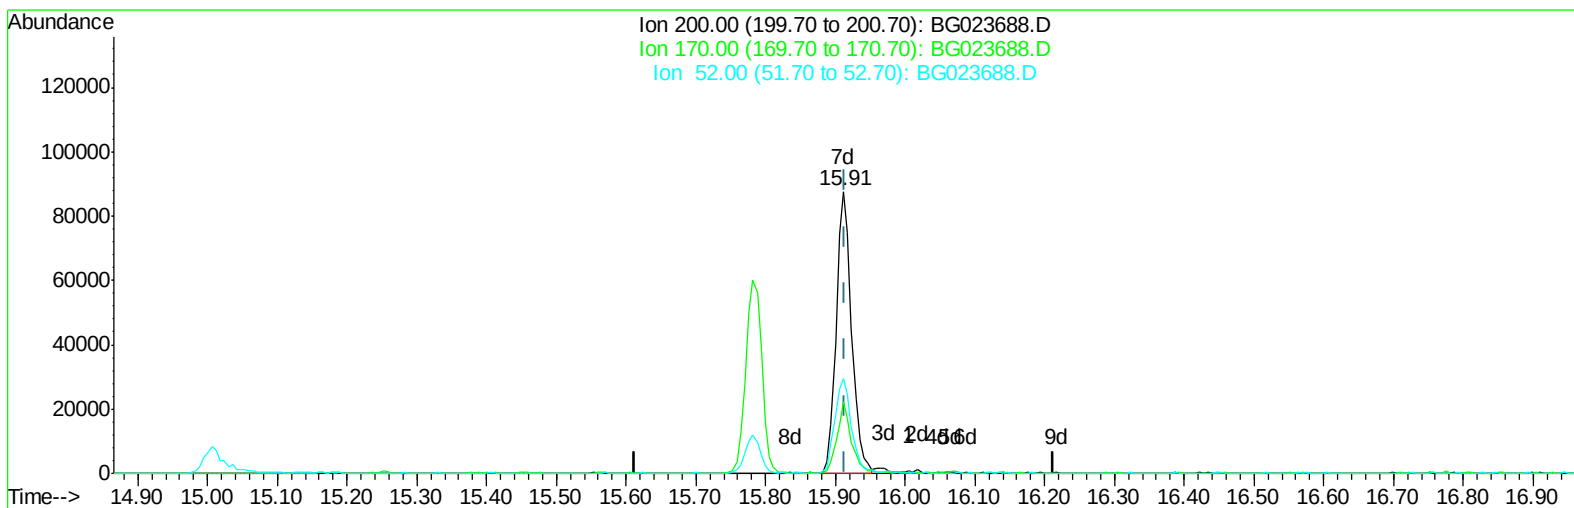

TIC: BG023688.D

(62) 4,6-Dinitro-2-methylphenol-d2 (S)

15.911min (-0.002) 28.68ng/ul m

response 135174

Ion	Exp%	Act%
200.00	100	100
170.00	15.20	25.37#
52.00	32.20	33.61
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
 Data File : BG023688.D
 Acq On : 13 Aug 2016 14:39
 Operator : UM/SJ
 Sample : H4388-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PR002-SS003-0206-02

Manual Integrations
 APPROVED

umangi
 8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:46:03 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 15 11:28:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	95806	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	453316	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	312577	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	734731m	20.00	ng/ul	0.00
75) Chrysene-d12	21.87	240	777822m	20.00	ng/ul	0.00
83) Perylene-d12	25.28	264	782530	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	12015	5.33	ng/uL	0.00
5) Phenol-d5	7.26	99	283483	29.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	191776	31.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	205099	31.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	212715	28.23	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	118898	33.28	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	136913	33.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	232731	30.07	ng/ul	0.00
29) 4-Chloroaniline-d4	11.08	131	248273	27.34	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	822749	32.15	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	971839	33.74	ng/ul	0.00
51) 4-Nitrophenol-d4	15.01	143	128947	29.51	ng/ul	0.00
57) Fluorene-d10	15.78	176	773335	32.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.91	200	135174m	28.68	ng/ul	0.00
70) Anthracene-d10	17.65	188	1118828	33.80	ng/ul	0.00
76) Pyrene-d10	19.95	212	1236116	31.40	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.04	264	1215964	34.33	ng/ul	0.00

Target Compounds

						Ovalue
6) Phenol	7.29	94	15750	1.57	ng/ul#	75
44) Dimethylphthalate	14.23	163	359174	14.17	ng/ul	99
69) Phenanthrene	17.60	178	51142	1.34	ng/ul	97
74) Fluoranthene	19.61	202	111358m	2.86	ng/ul	
77) Pyrene	19.97	202	112359m	2.34	ng/ul	
80) Benzo(a)anthracene	21.85	228	45274m	1.03	ng/ul	
82) Chrysene	21.92	228	53128m	1.33	ng/ul	
85) Benzo(b)fluoranthene	24.20	252	65077m	1.46	ng/ul	
88) Benzo(a)pyrene	25.12	252	48637m	1.13	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023688.D
Acq On : 13 Aug 2016 14:39
Operator : UM/SJ
Sample : H4388-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS003-0206-02

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:08 PM

Quant Time: Aug 15 13:46:03 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

