




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:28:57 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

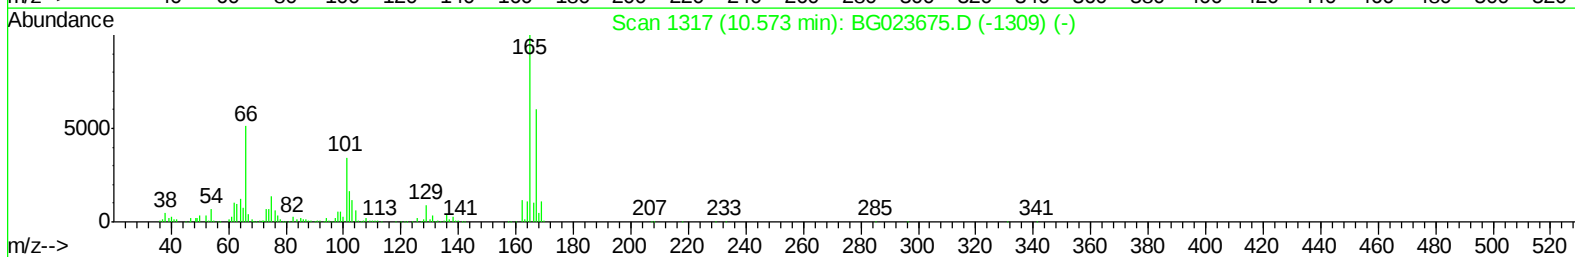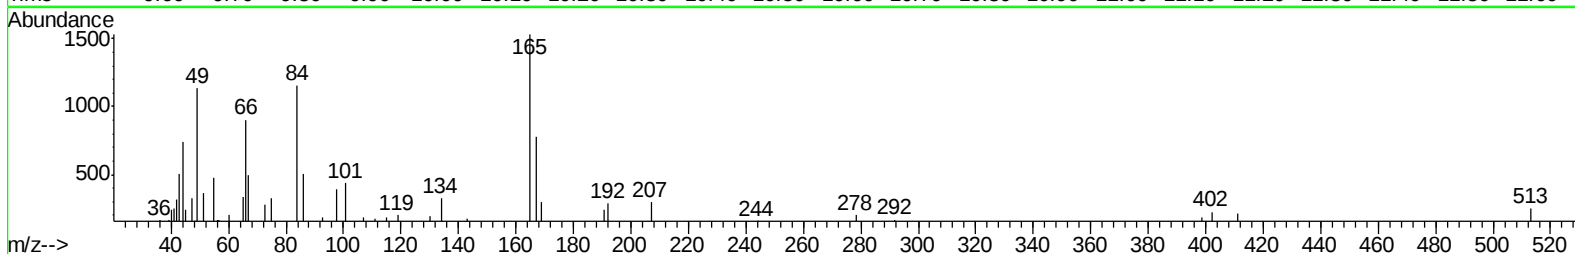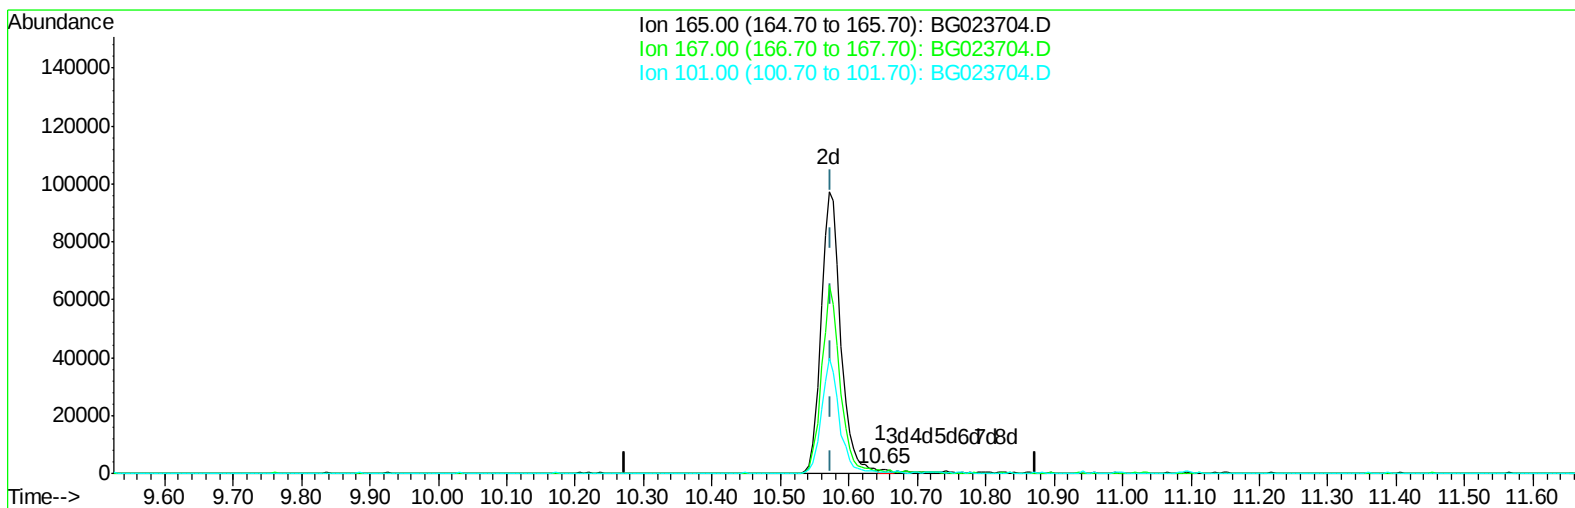

TIC: BG023704.D

(26) 2,4-Dichlorophenol-d3 (S)

10.648min (+0.074) 0.17ng/ul

response 1471

Ion	Exp%	Act%
165.00	100	100
167.00	60.90	50.88
101.00	31.80	28.61
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:28:57 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

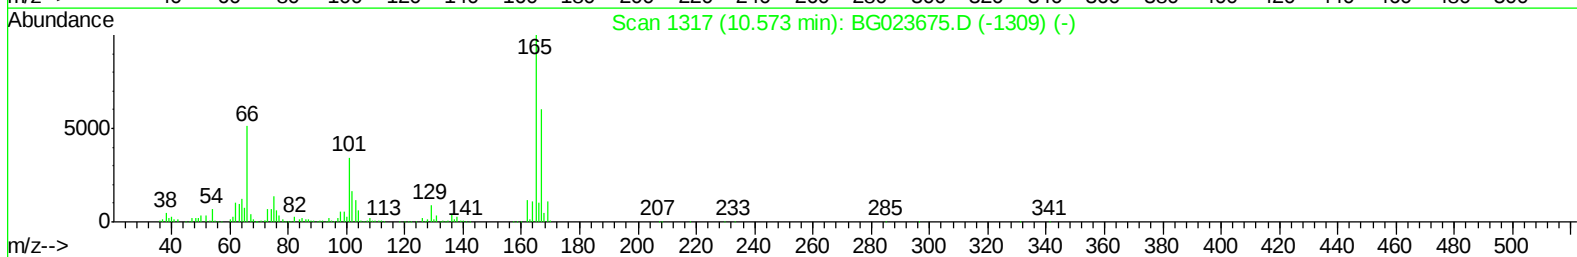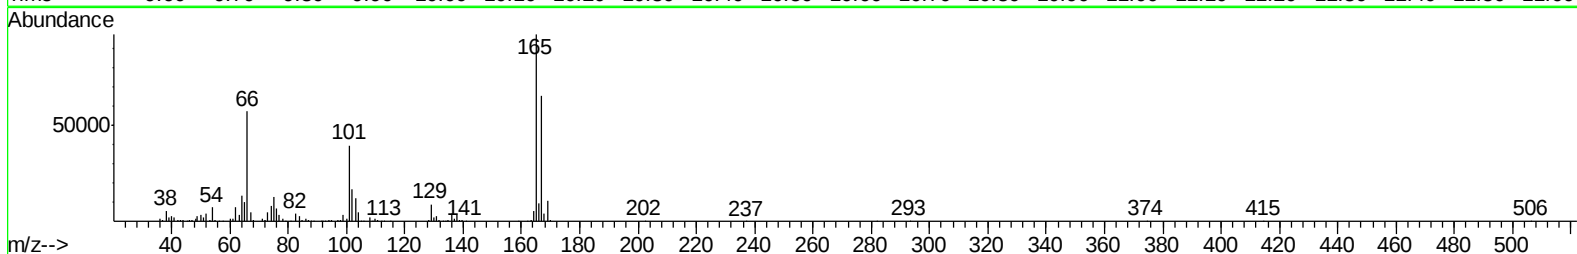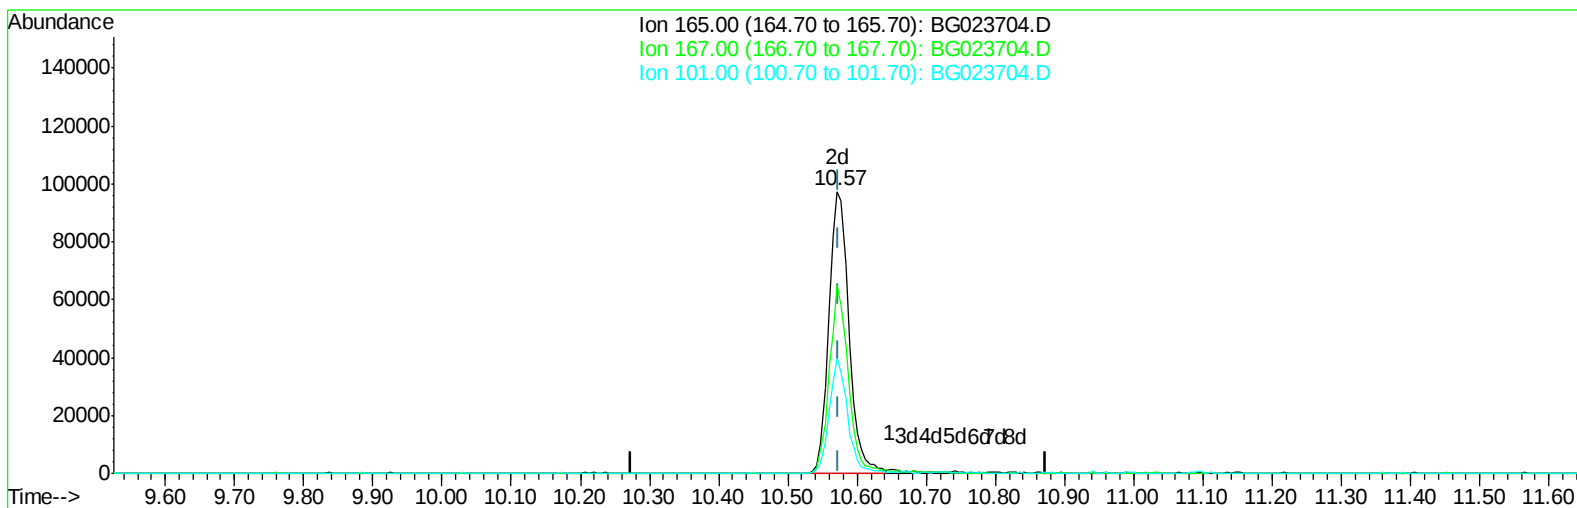

TIC: BG023704.D

(26) 2,4-Dichlorophenol-d3 (S)

10.571min (-0.002) 21.97ng/ul m

response 194993

Ion	Exp%	Act%
165.00	100	100
167.00	60.90	66.95
101.00	31.80	40.70#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
 Data File : BG023704.D
 Acq On : 14 Aug 2016 1:25
 Operator : UM/SJ
 Sample : H4385-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P002-SS002-0206-01

Manual Integrations
 APPROVED

umangi
 8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:28:57 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 06:38:14 2016
 Response via : Initial Calibration

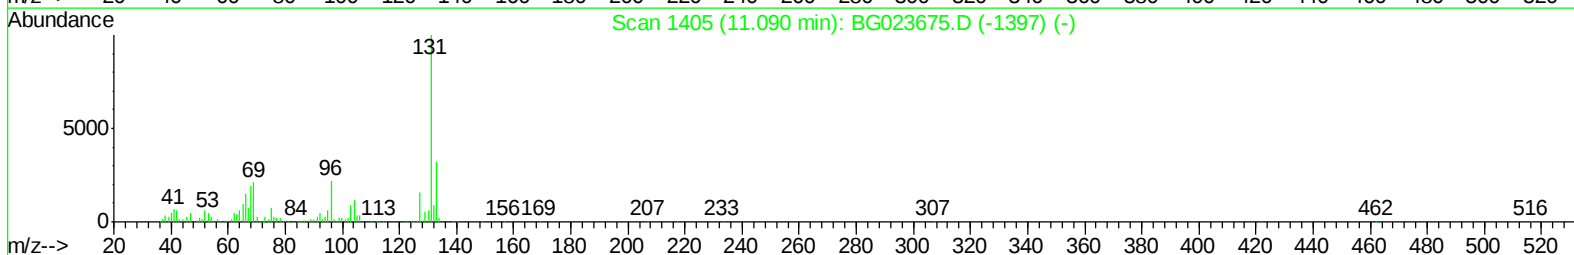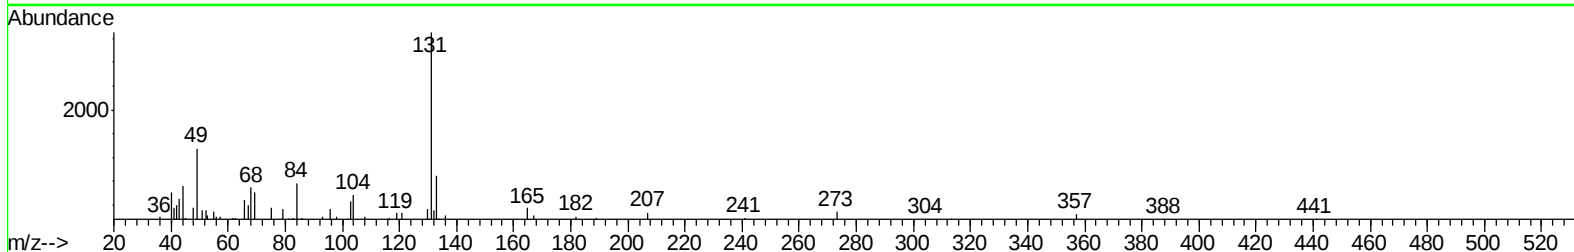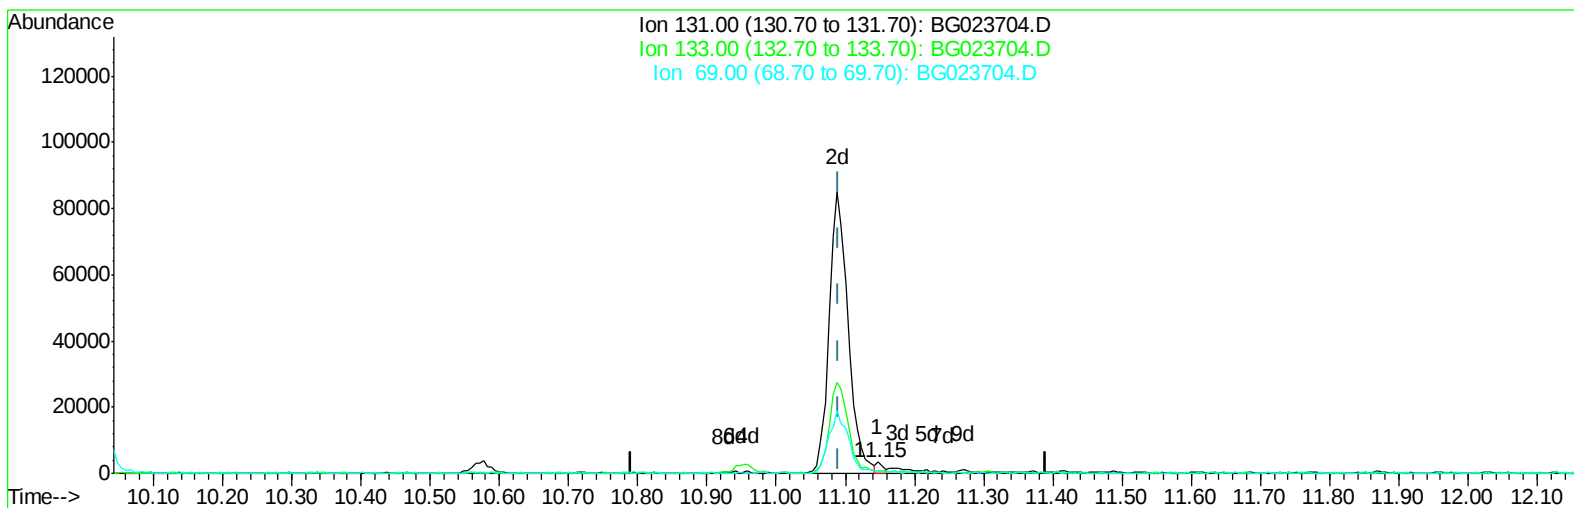

TIC: BG023704.D

(29) 4-Chloroaniline-d4 (S)
 11.147min (+0.057) 0.22ng/ul
 response 2266

Ion	Exp%	Act%
131.00	100	100
133.00	33.10	27.26
69.00	15.40	18.25
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:28:57 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

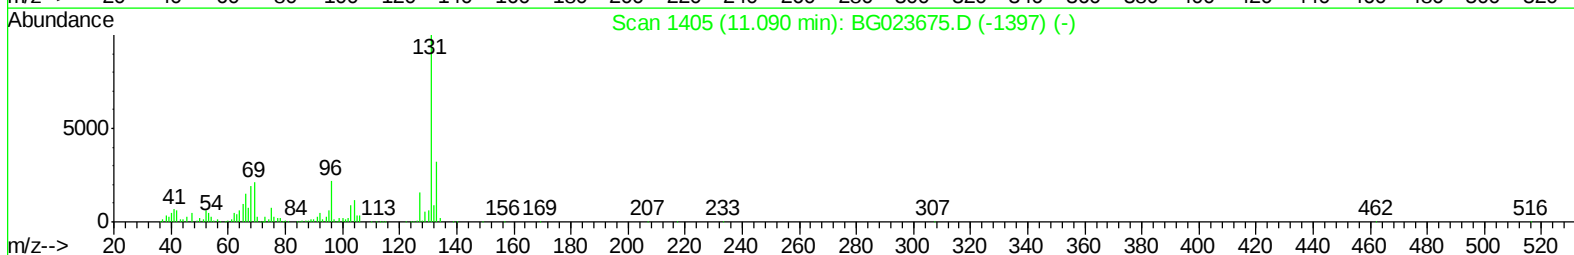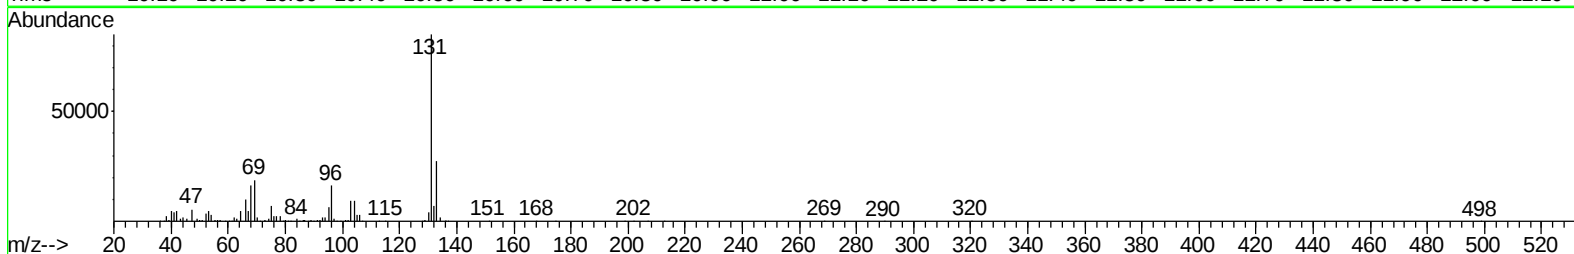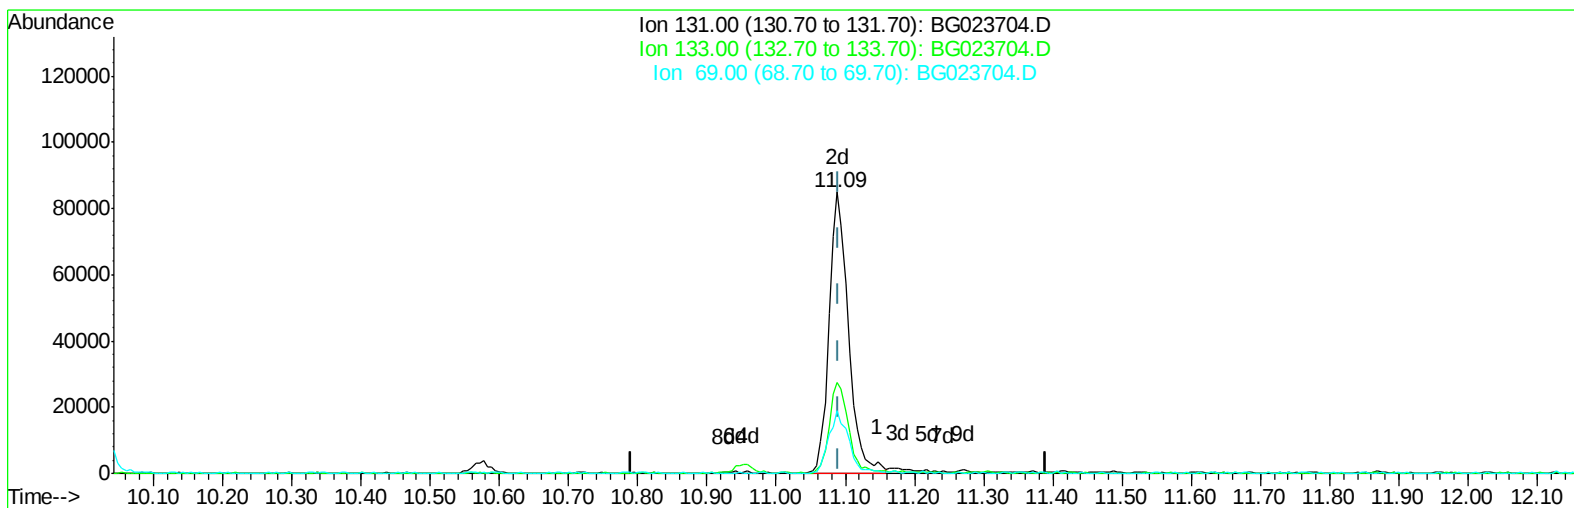

TIC: BG023704.D

(29) 4-Chloroaniline-d4 (S)
11.088min (-0.002) 15.78ng/ul m
response 164254

Ion	Exp%	Act%
131.00	100	100
133.00	33.10	32.45
69.00	15.40	22.08#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

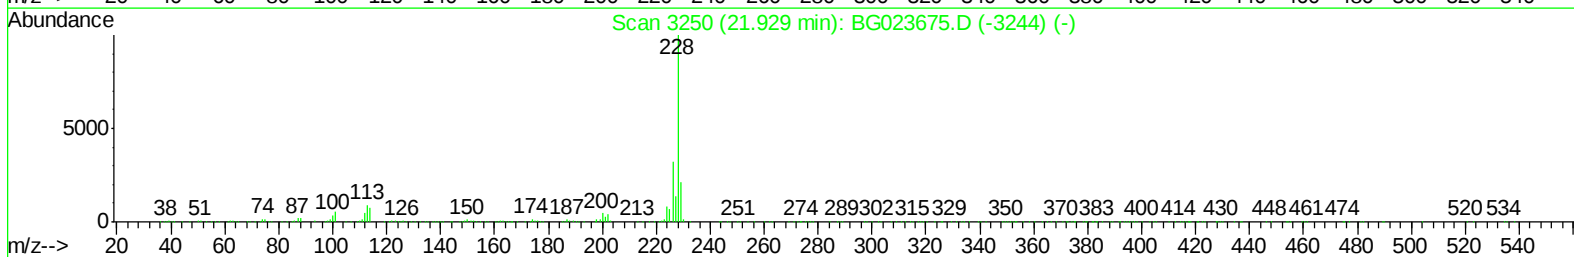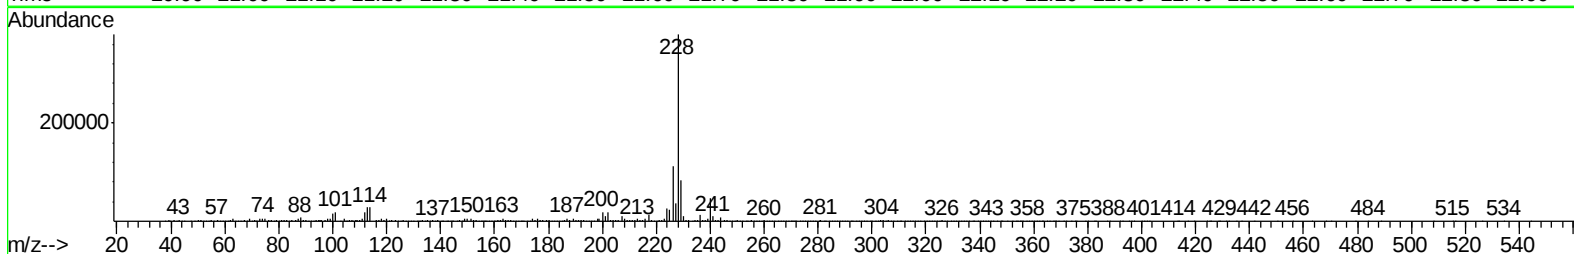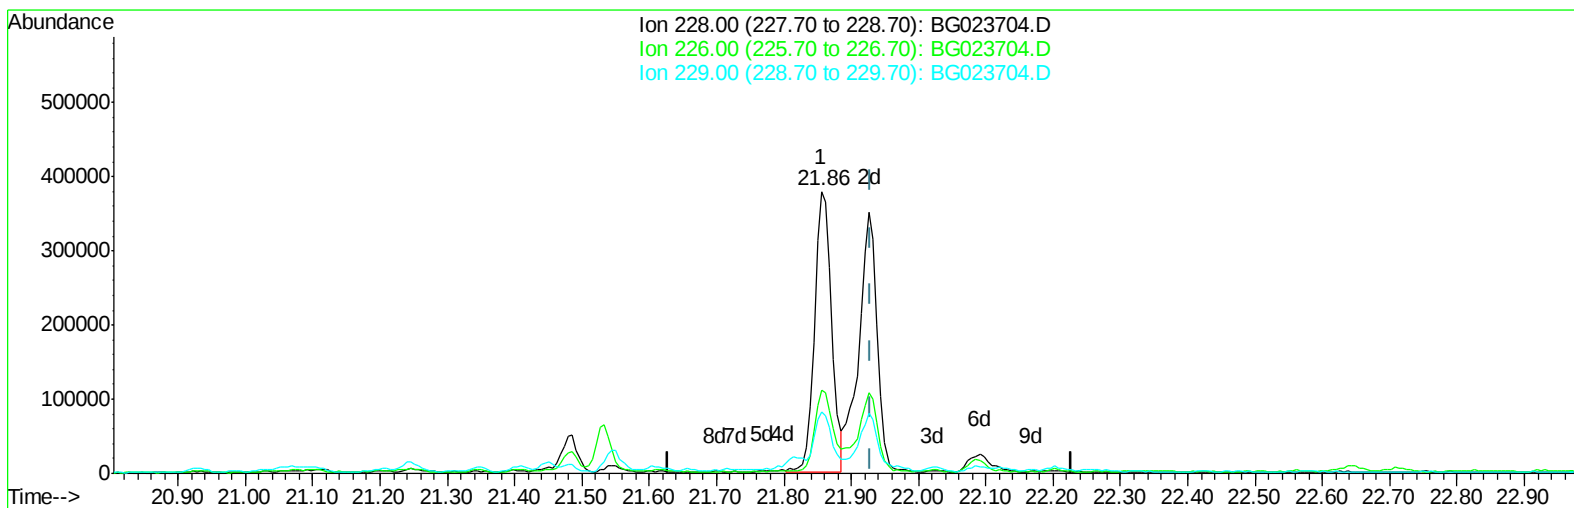

TIC: BG023704.D

(82) Chrysene

21.856min (-0.073) 19.93ng/ul

response 681637

Ion	Exp%	Act%
228.00	100	100
226.00	30.30	29.52
229.00	18.80	21.75
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

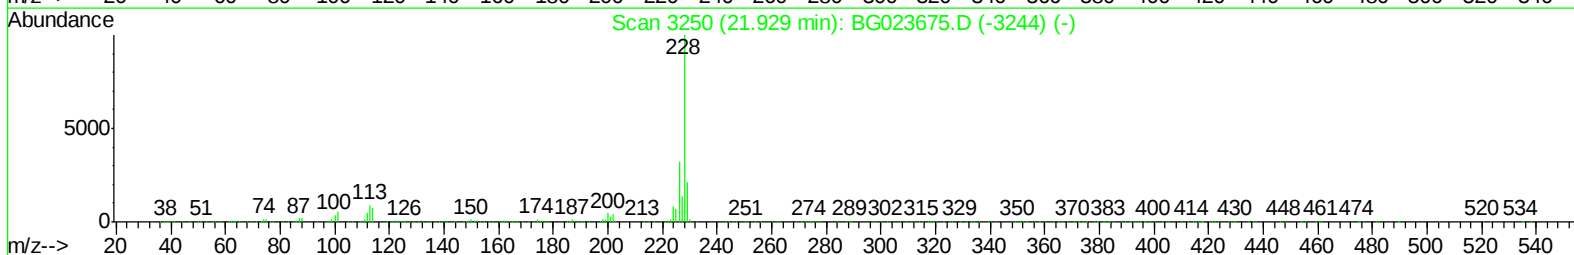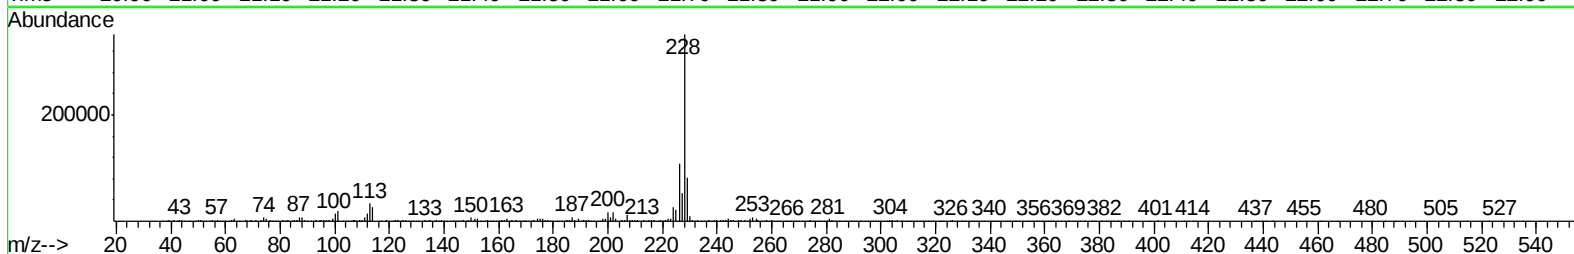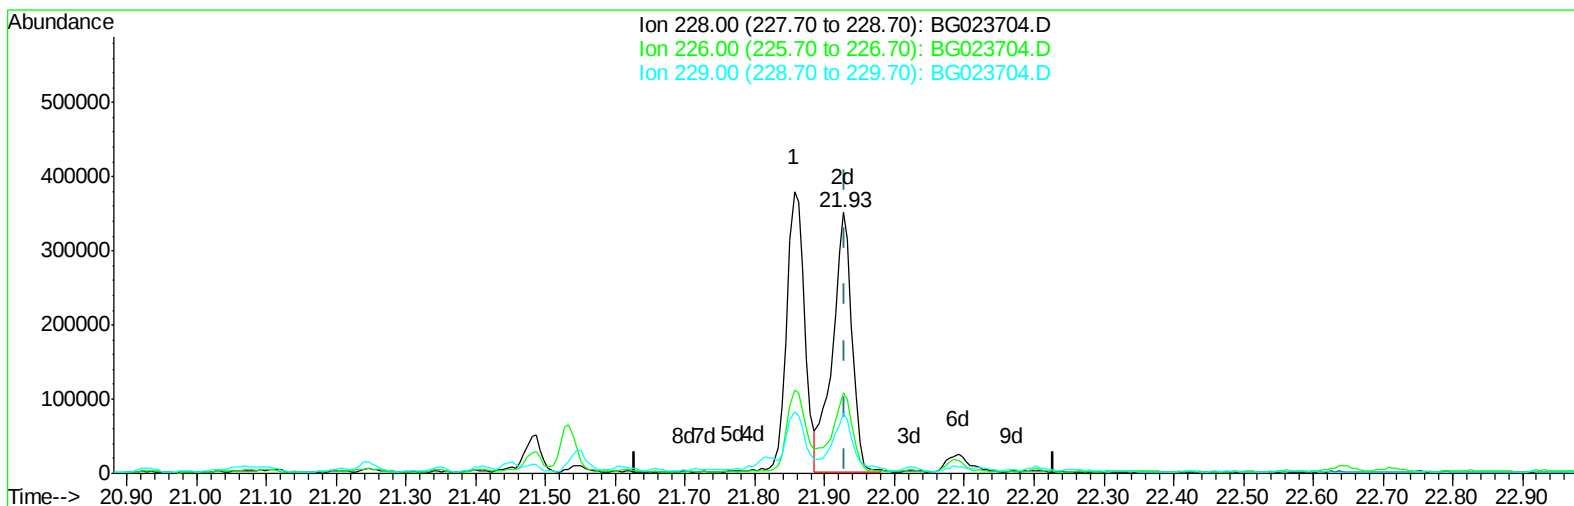

TIC: BG023704.D

(82) Chrysene

21.927min (-0.002) 19.87ng/ul m

response 679584

Ion	Exp%	Act%
228.00	100	100
226.00	30.30	31.06
229.00	18.80	23.02#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

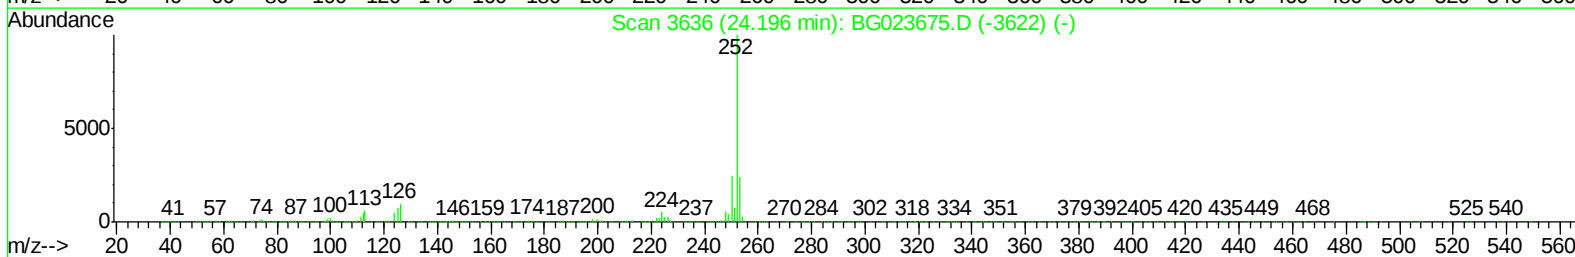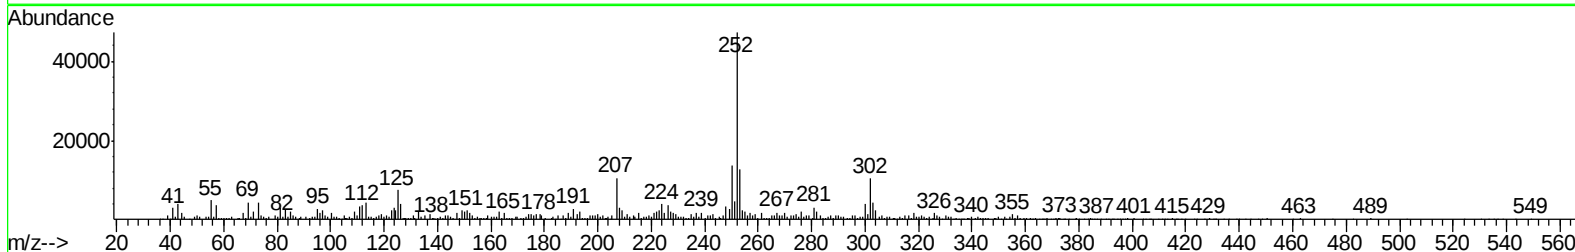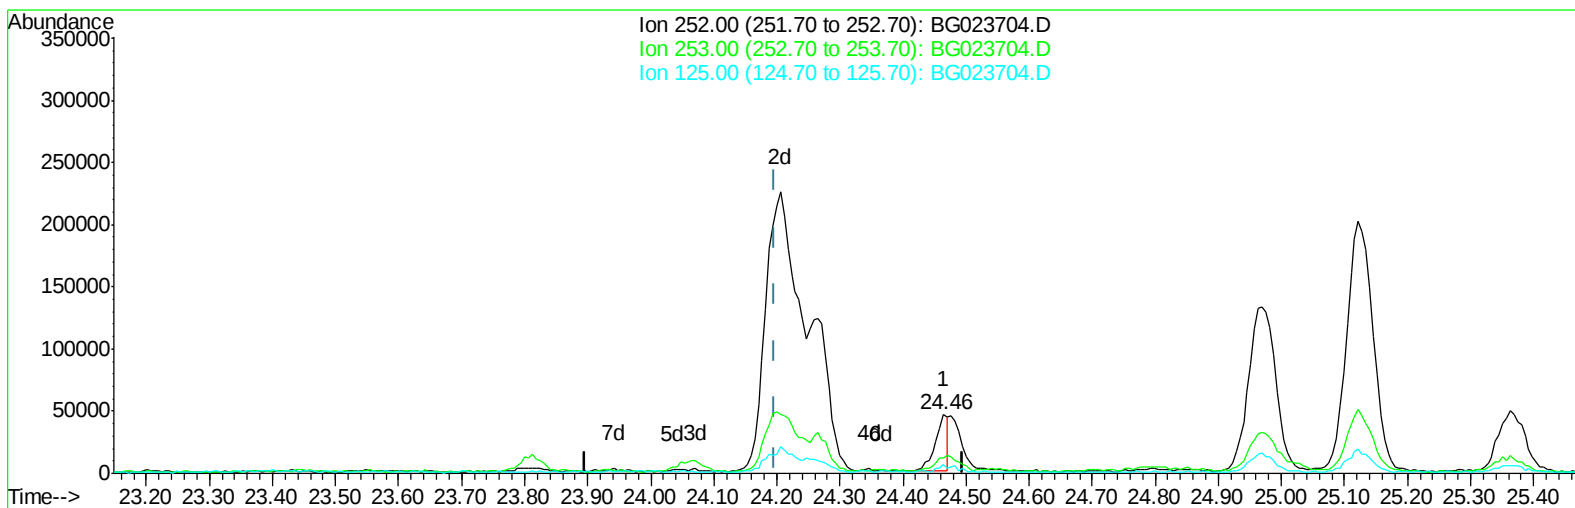

TIC: BG023704.D

(85) Benzo(b)fluoranthene

24.464min (+0.268) 1.67ng/ul

response 65173

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	26.73
125.00	13.50	15.83
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

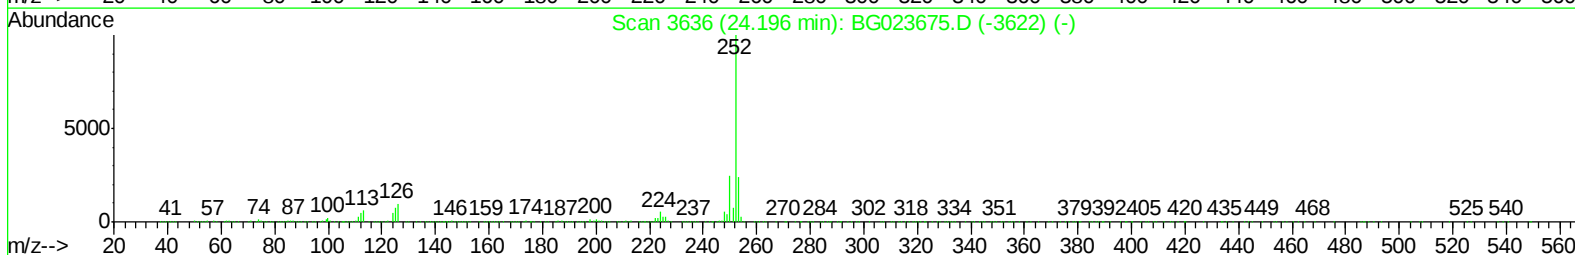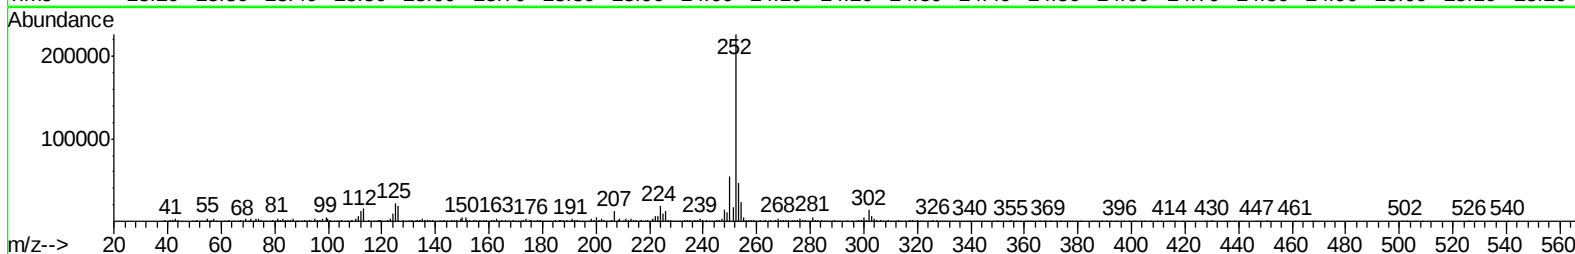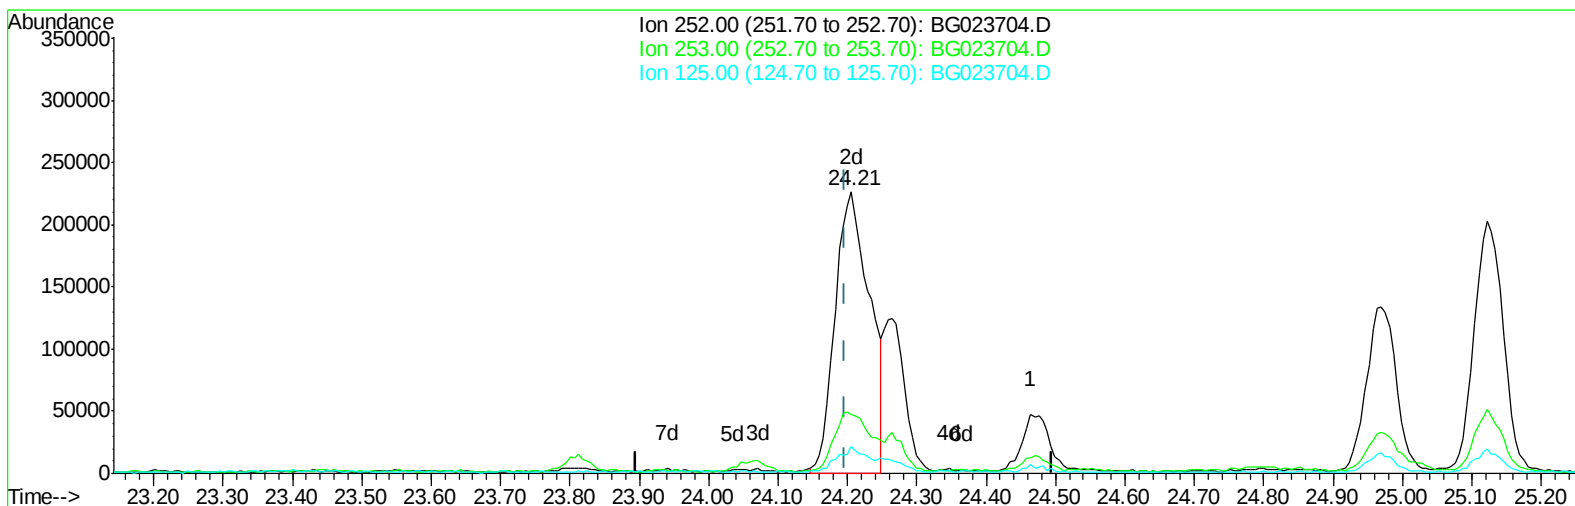

TIC: BG023704.D

(85) Benzo(b)fluoranthene

24.206min (+0.010) 19.97ng/ul m

response 780729

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	20.83
125.00	13.50	9.38#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

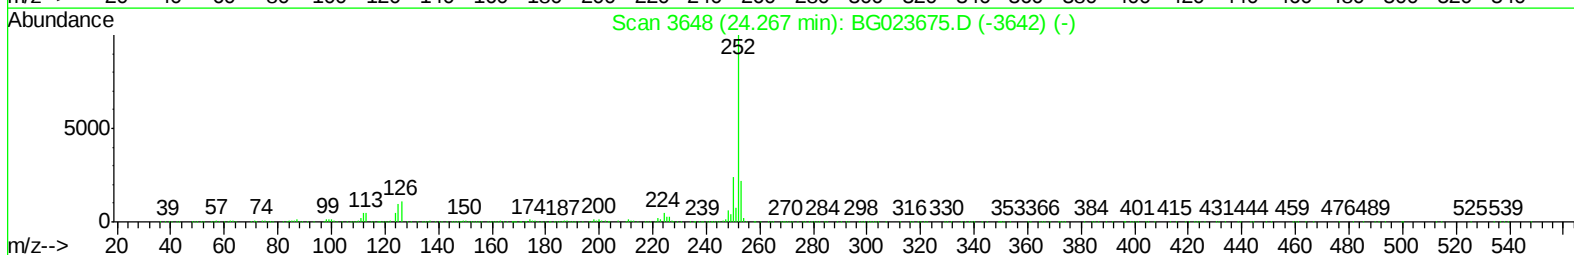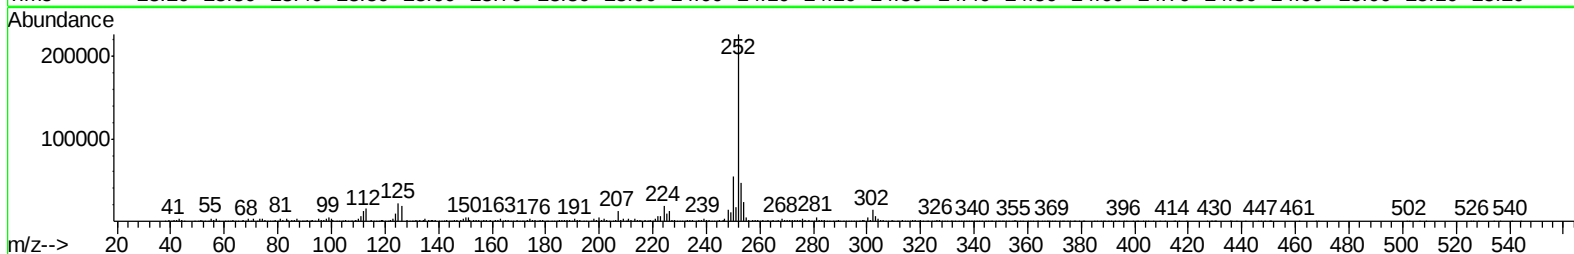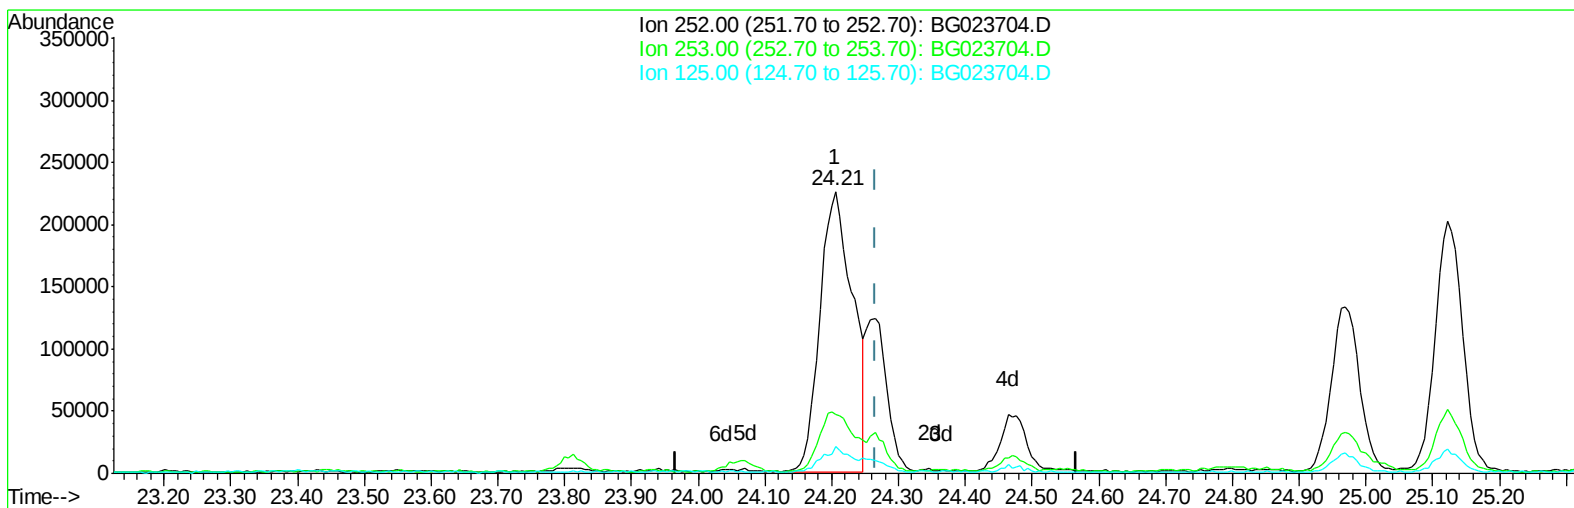

TIC: BG023704.D

(86) Benzo(k)fluoranthene

24.206min (-0.061) 20.12ng/ul

response 774415

Ion	Exp%	Act%
252.00	100	100
253.00	19.70	20.83
125.00	13.30	9.38#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
 Data File : BG023704.D
 Acq On : 14 Aug 2016 1:25
 Operator : UM/SJ
 Sample : H4385-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P002-SS002-0206-01

Manual Integrations
 APPROVED

umangi
 8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 06:38:14 2016
 Response via : Initial Calibration

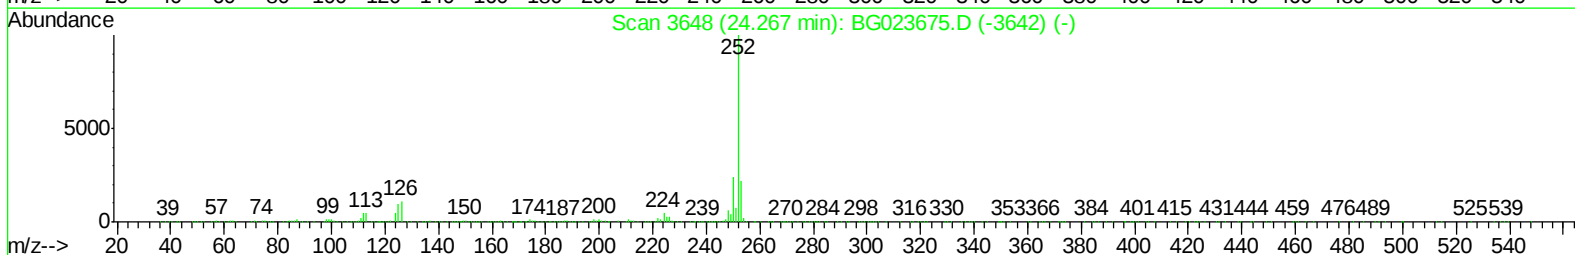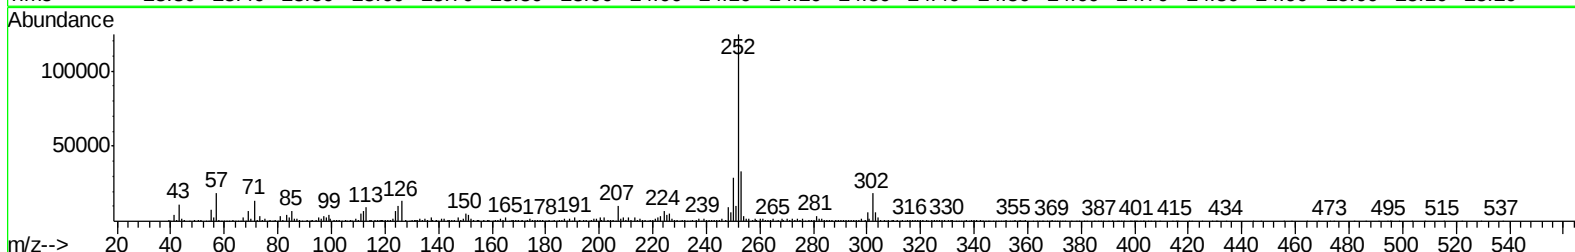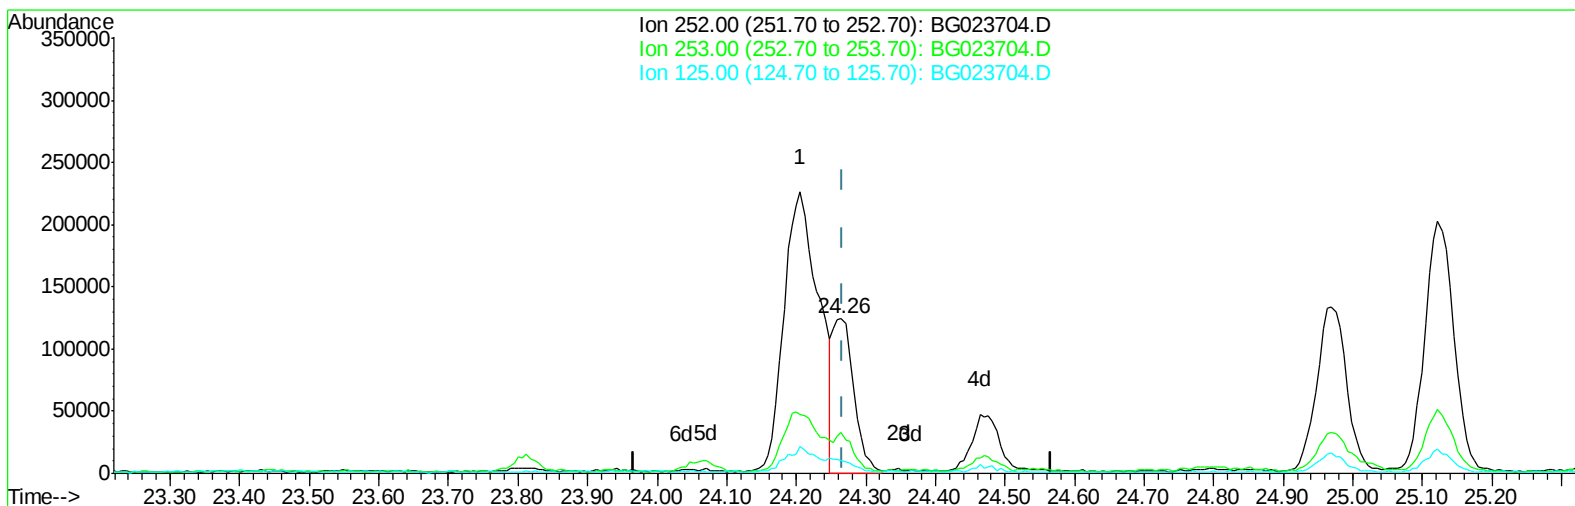

TIC: BG023704.D

(86) Benzo(k)fluoranthene

24.265min (-0.002) 6.89ng/ul m

response 265240

Ion	Exp%	Act%
252.00	100	100
253.00	19.70	26.66#
125.00	13.30	8.31#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

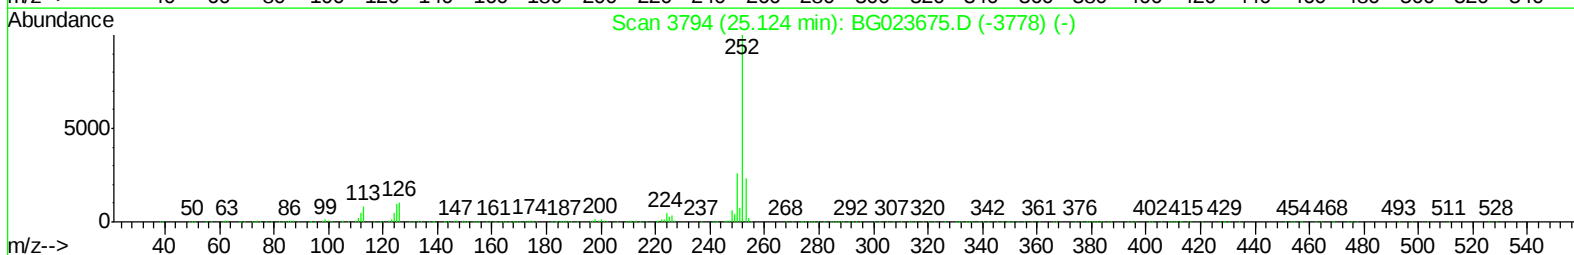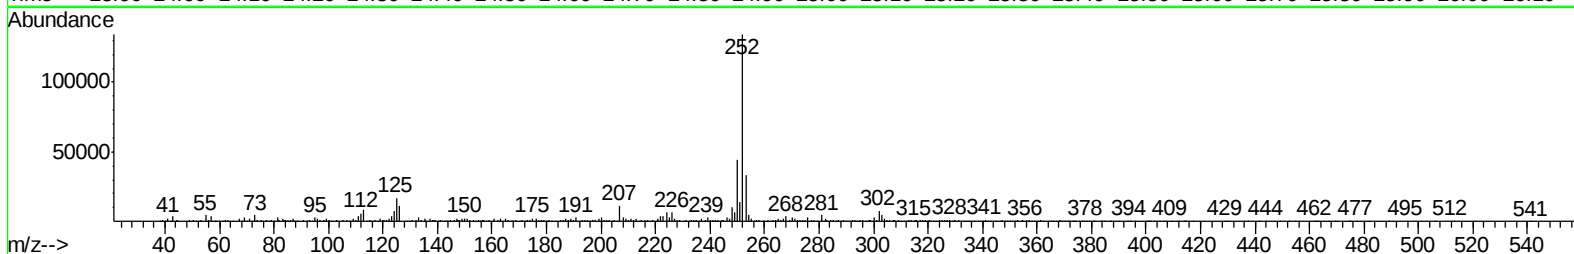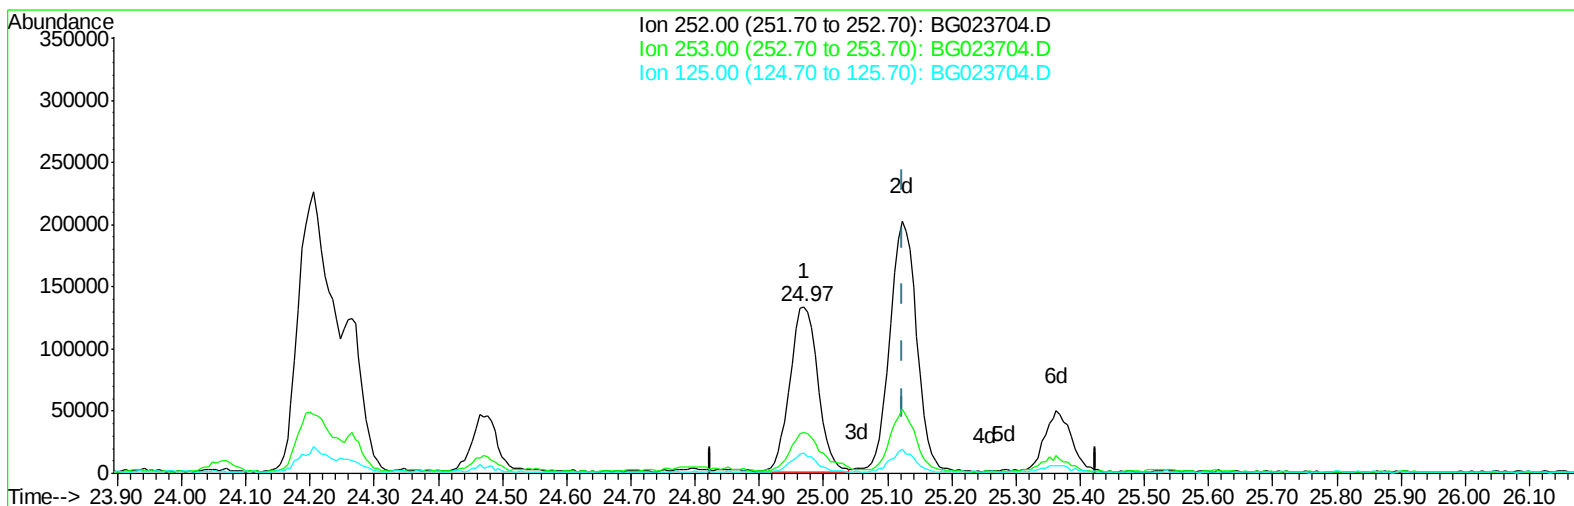

TIC: BG023704.D

(88) Benzo(a)pyrene (C)

24.969min (-0.155) 10.57ng/ul

response 398892

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	24.77
125.00	15.00	12.44
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

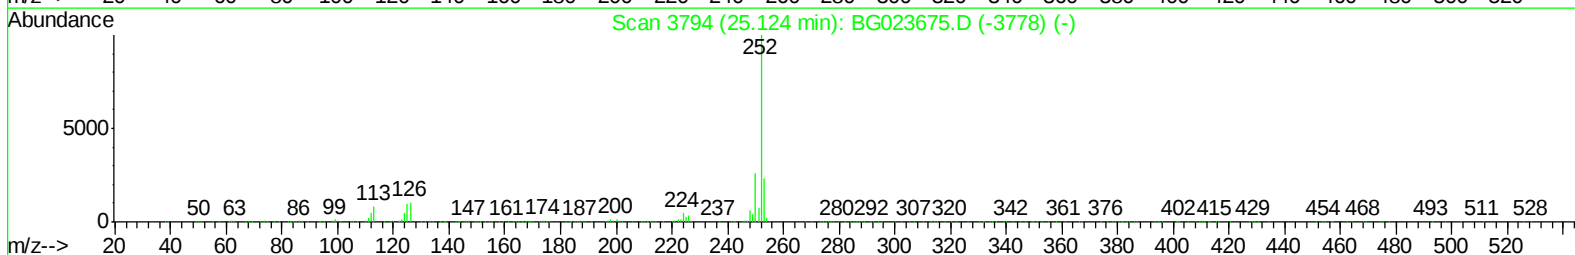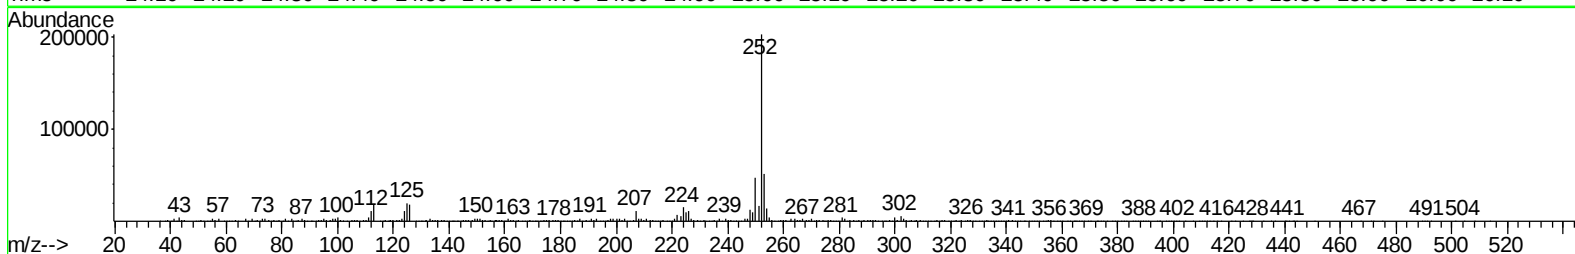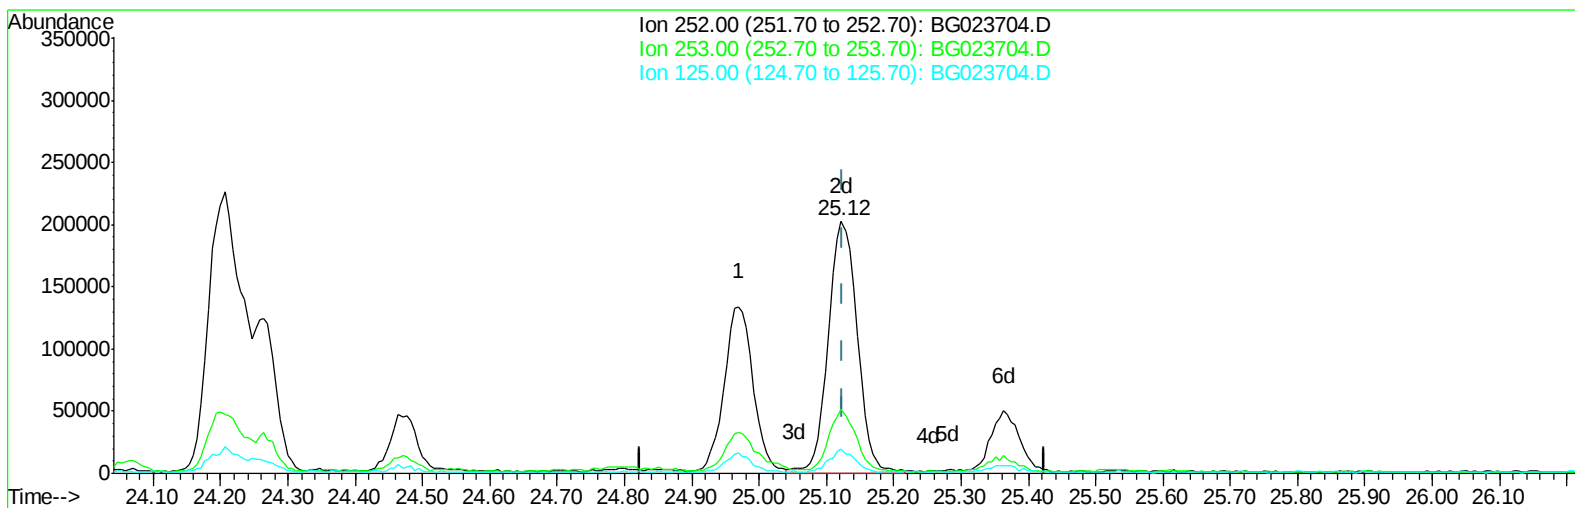

TIC: BG023704.D

(88) Benzo(a)pyrene (C)

25.122min (-0.002) 16.06ng/ul m

response 605996

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	25.21
125.00	15.00	9.72#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

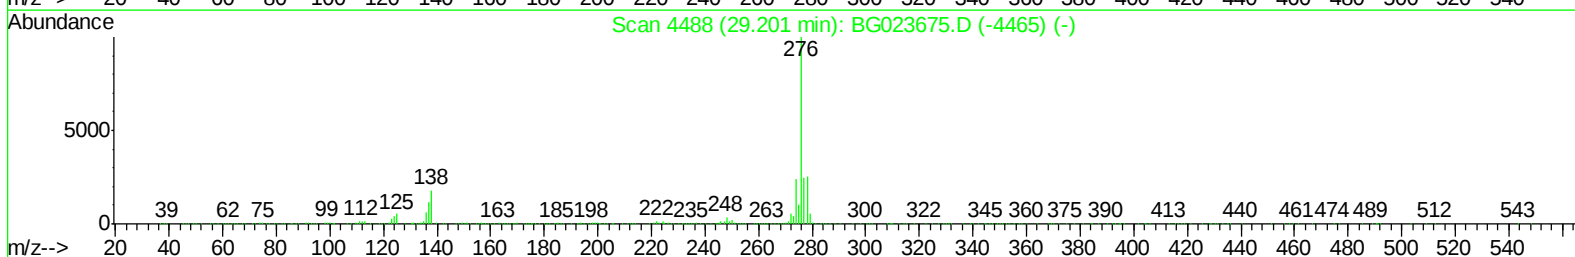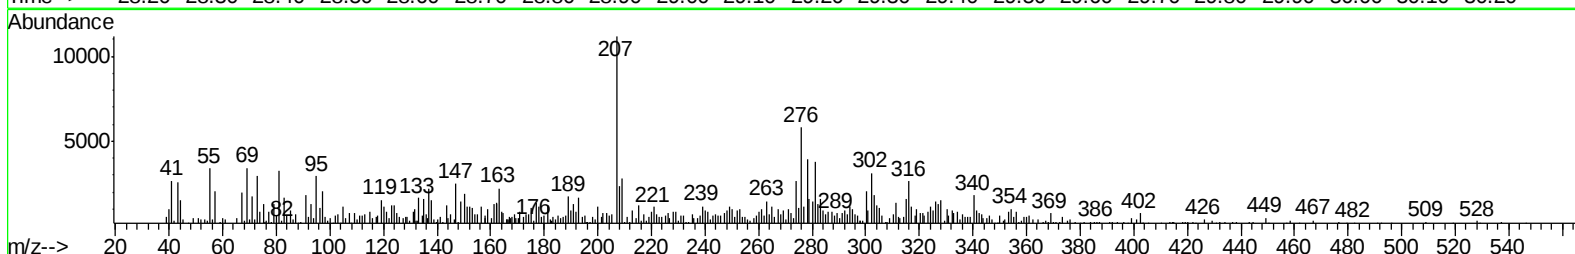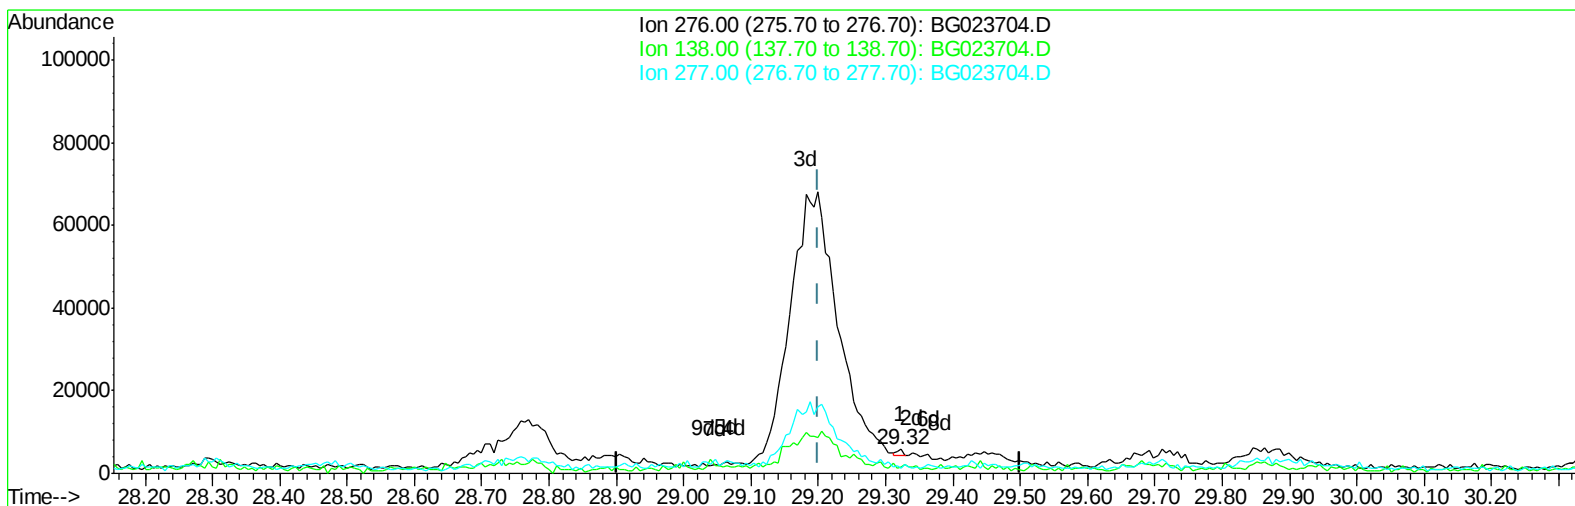

TIC: BG023704.D

(89) Indeno(1,2,3-cd)pyrene

29.322min (+0.121) 0.02ng/ul

response 799

Ion	Exp%	Act%
276.00	100	100
138.00	26.00	26.45
277.00	22.00	20.11
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
 Data File : BG023704.D
 Acq On : 14 Aug 2016 1:25
 Operator : UM/SJ
 Sample : H4385-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P002-SS002-0206-01

Manual Integrations
 APPROVED

umangi
 8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 06:38:14 2016
 Response via : Initial Calibration

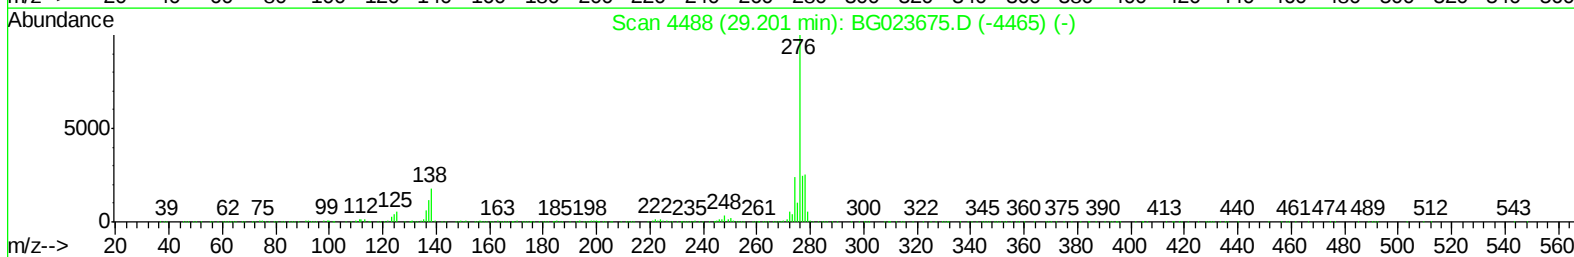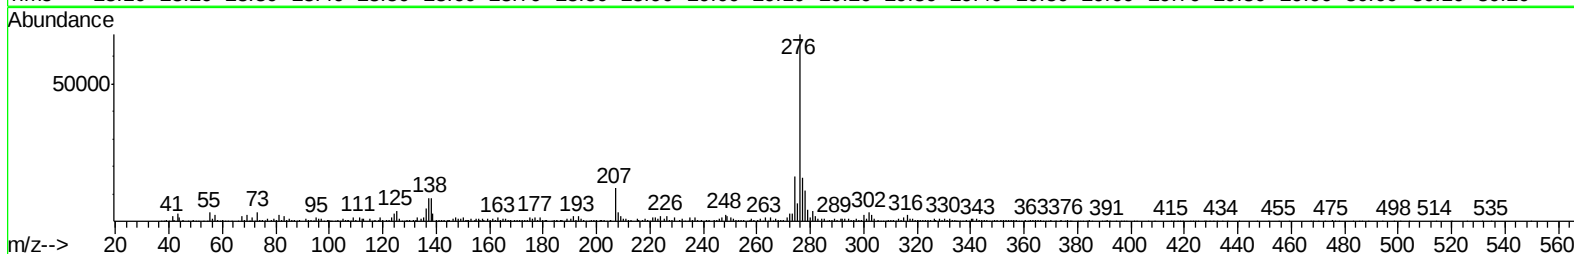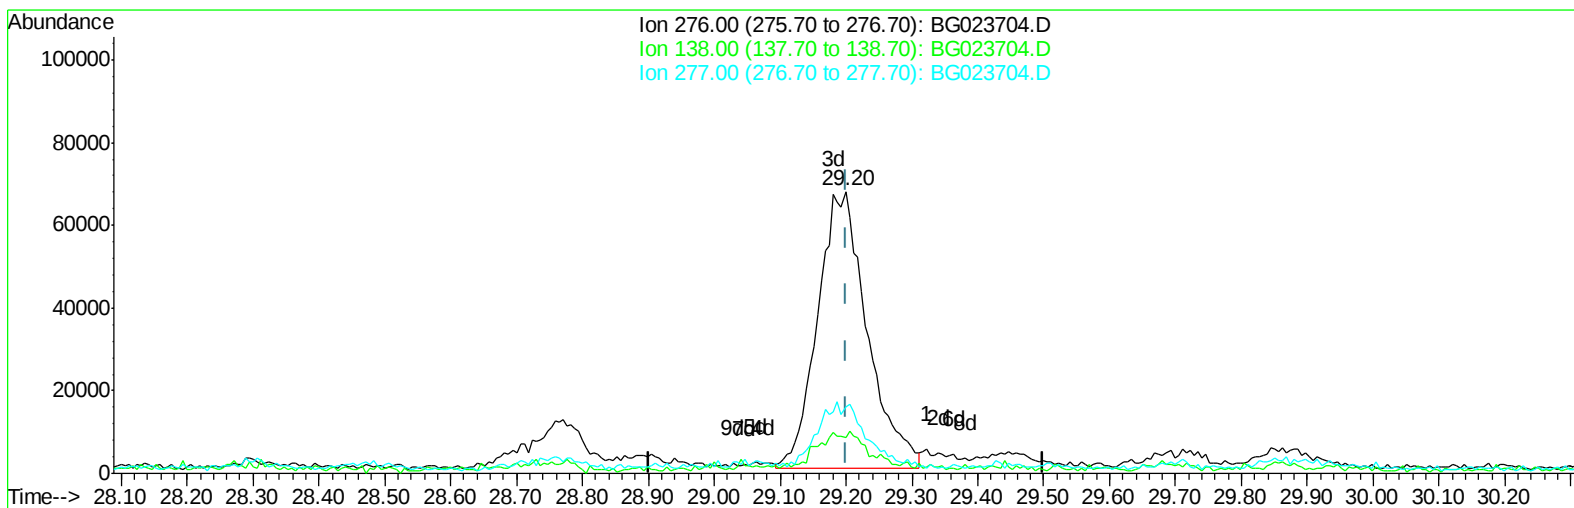

TIC: BG023704.D

(89) Indeno(1,2,3-cd)pyrene
 29.199min (-0.002) 7.79ng/ul m

response 345655

Ion	Exp%	Act%
276.00	100	100
138.00	26.00	12.67#
277.00	22.00	23.80
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

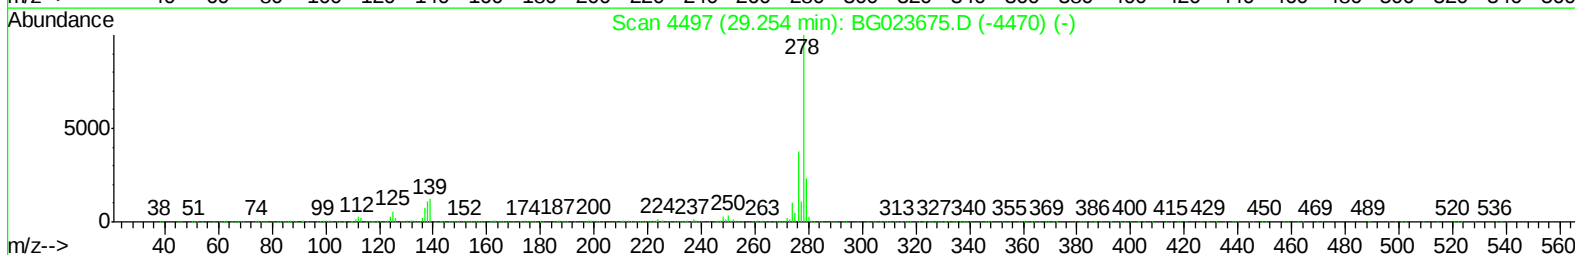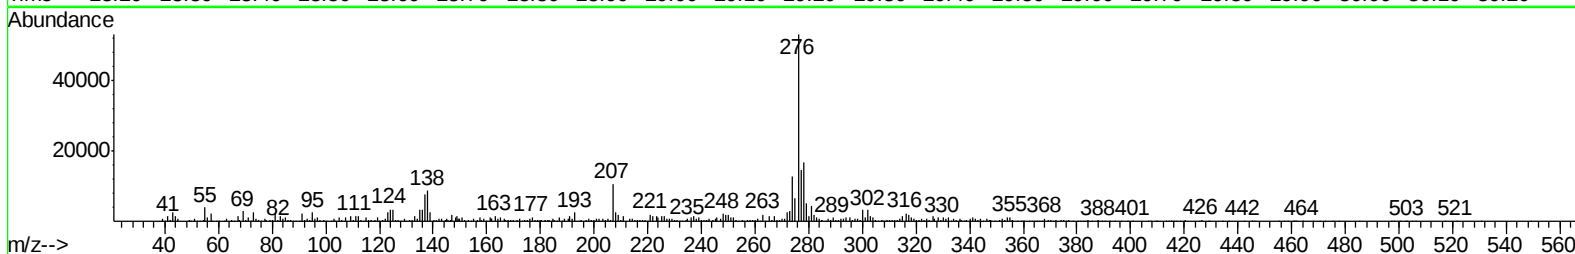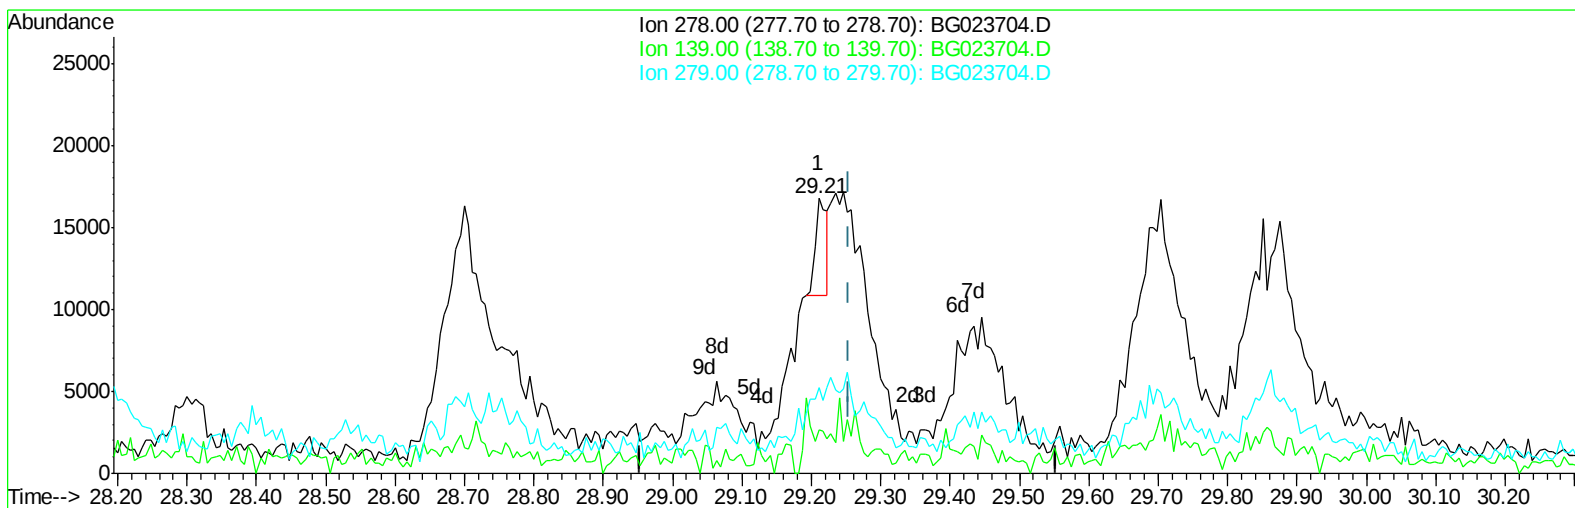

TIC: BG023704.D

(90) Dibenzo(a,h)anthracene

29.211min (-0.043) 0.18ng/ul

response 6860

Ion	Exp%	Act%
278.00	100	100
139.00	20.40	15.97#
279.00	23.90	31.02#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

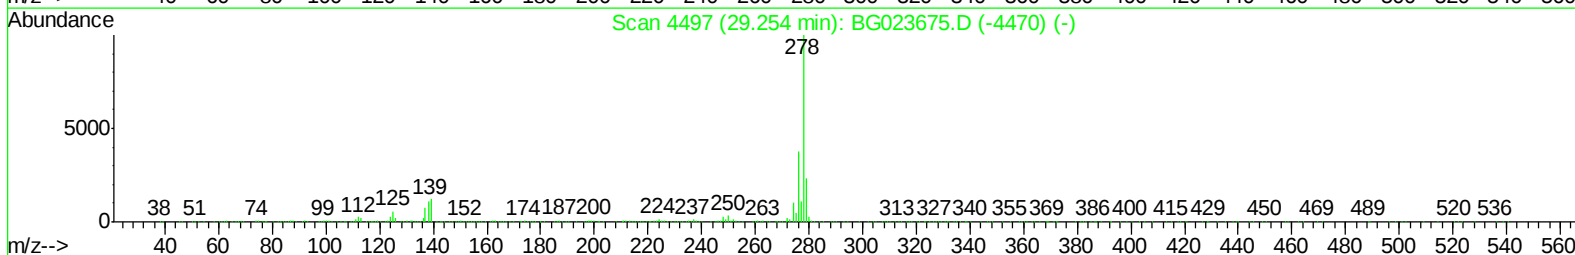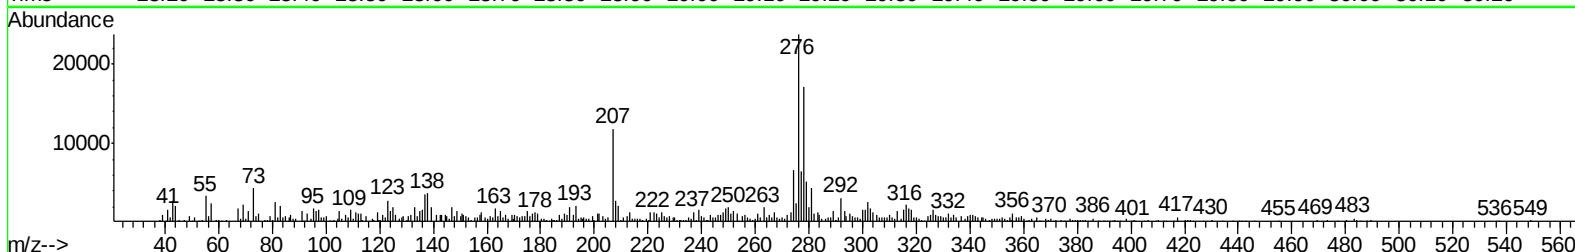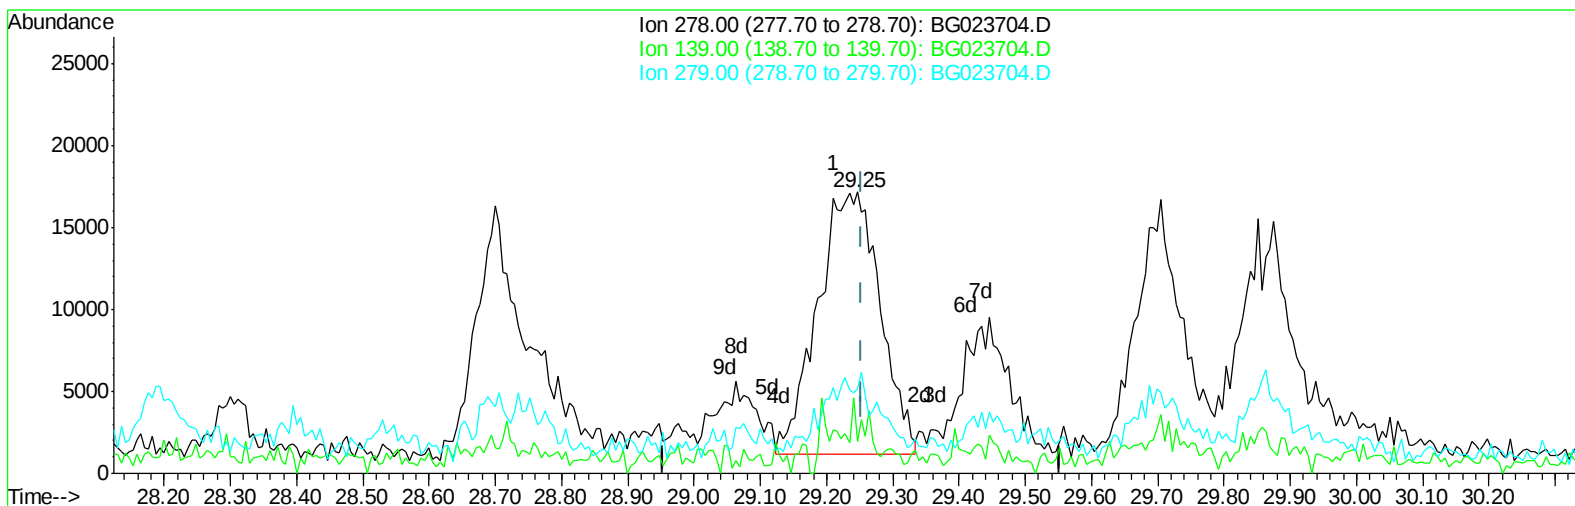

TIC: BG023704.D

(90) Dibenzo(a,h)anthracene

29.246min (-0.008) 2.75ng/ul m

response 103922

Ion	Exp%	Act%
278.00	100	100
139.00	20.40	11.52#
279.00	23.90	29.93#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

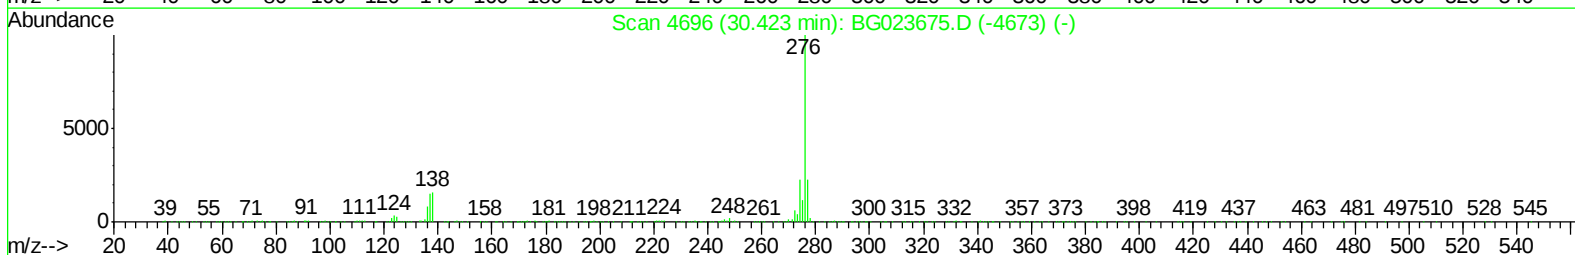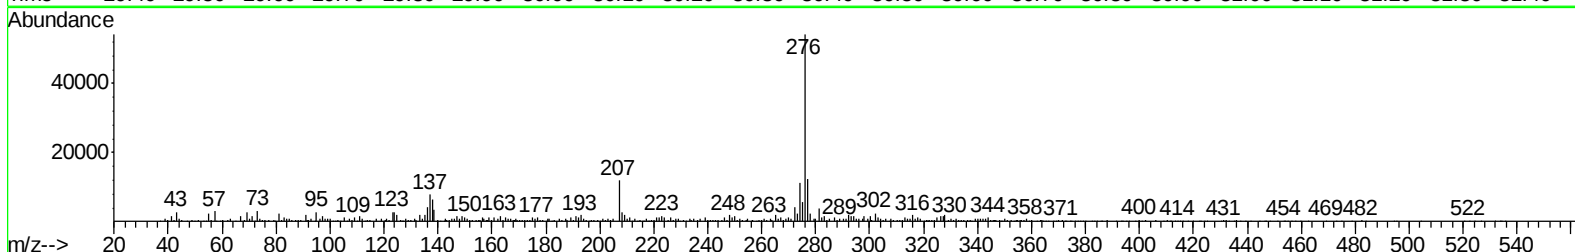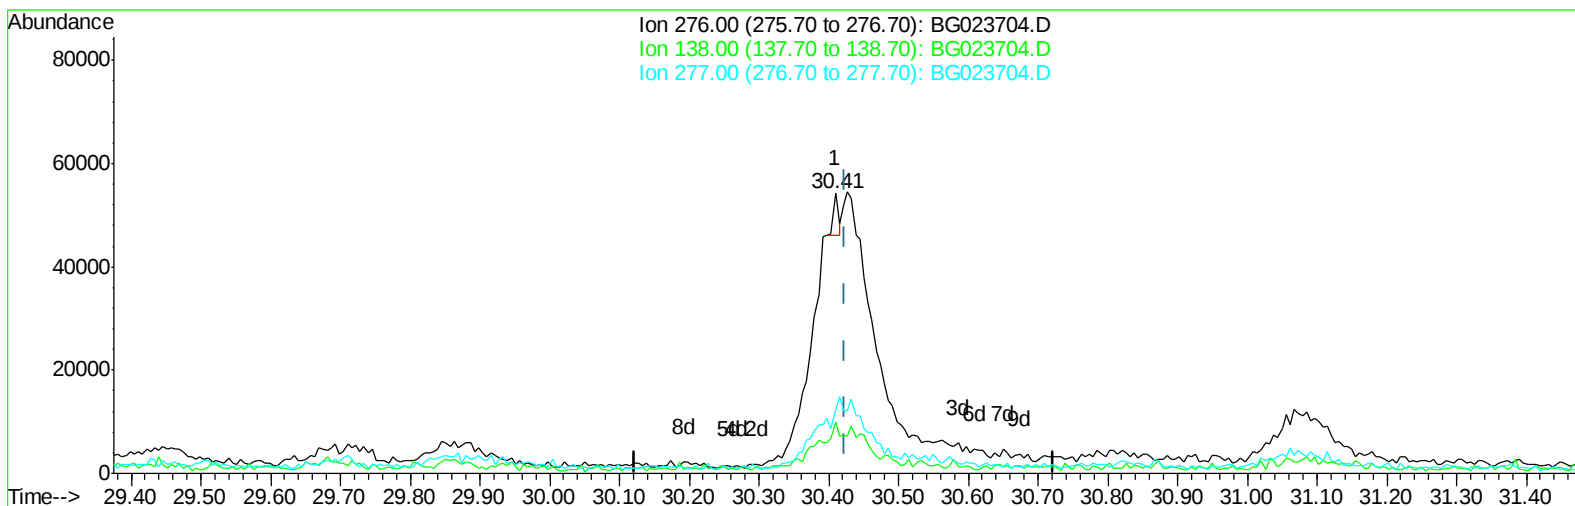

TIC: BG023704.D

(91) Benzo(g,h,i)perylene
30.409min (-0.014) 0.10ng/ul
response 3611

Ion	Exp%	Act%
276.00	100	100
138.00	27.60	18.40#
277.00	21.20	23.08
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
 Data File : BG023704.D
 Acq On : 14 Aug 2016 1:25
 Operator : UM/SJ
 Sample : H4385-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P002-SS002-0206-01

Manual Integrations
 APPROVED

umangi
 8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:34:51 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 06:38:14 2016
 Response via : Initial Calibration

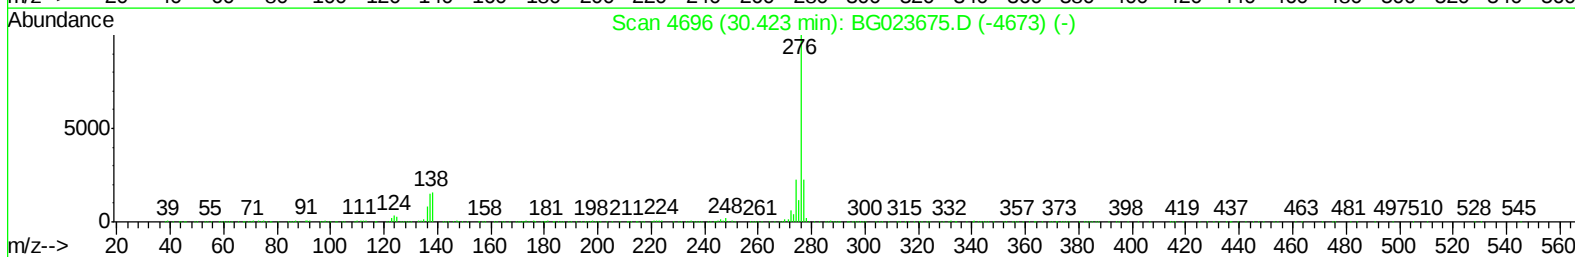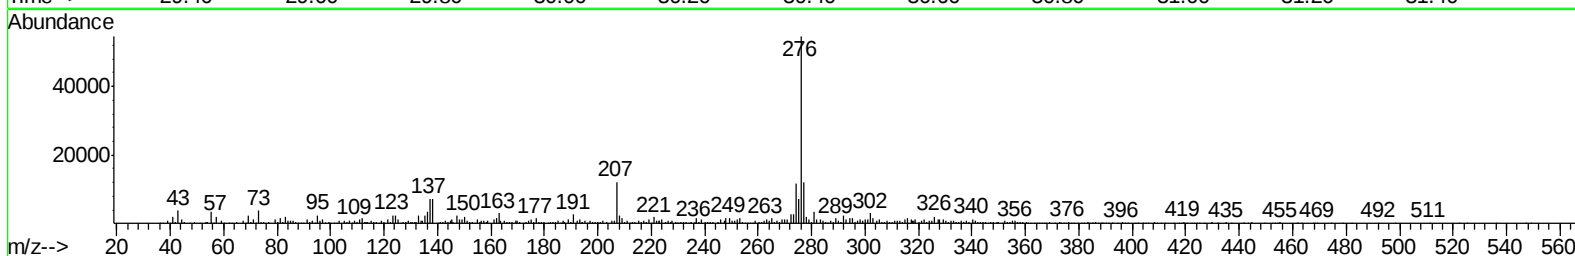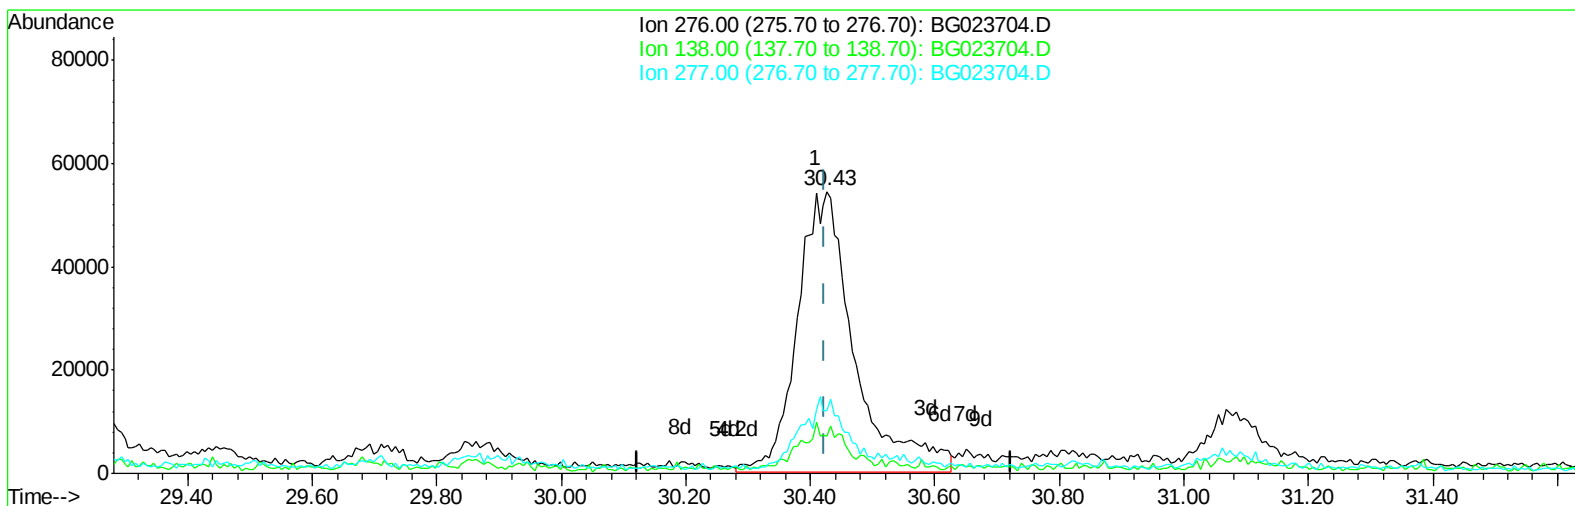

TIC: BG023704.D

(91) Benzo(g,h,i)perylene

30.427min (+0.004) 9.38ng/ul m

response 344860

Ion	Exp%	Act%
276.00	100	100
138.00	27.60	13.02#
277.00	21.20	22.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
 Data File : BG023704.D
 Acq On : 14 Aug 2016 1:25
 Operator : UM/SJ
 Sample : H4385-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P002-SS002-0206-01

Manual Integrations
 APPROVED

umangi
 8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:42:00 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 06:38:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	116737	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	519648	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	322642	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	666866	20.00	ng/ul	0.00
75) Chrysene-d12	21.88	240	667947	20.00	ng/ul	0.00
83) Perylene-d12	25.29	264	687260	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	8533	3.11	ng/uL	0.00
5) Phenol-d5	7.27	99	255587	21.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	167373	22.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	180992	22.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	184841	20.13	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	92659	22.62	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	111151	23.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	194993m	21.97	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	164254m	15.78	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	609394	23.07	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	718921	24.18	ng/ul	0.00
51) 4-Nitrophenol-d4	15.01	143	80393	17.83	ng/ul	0.00
57) Fluorene-d10	15.78	176	526229	21.56	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.92	200	75965	17.76	ng/ul	0.00
70) Anthracene-d10	17.65	188	733059	24.40	ng/ul	0.00
76) Pyrene-d10	19.95	212	800632	23.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.05	264	781067	25.11	ng/ul	0.00

Target Compounds

						Ovalue
44) Dimethylphthalate	14.23	163	255675	9.77	ng/ul	99
47) Acenaphthylene	14.51	152	85181	2.74	ng/ul	98
49) Acenaphthene	14.85	153	25804	1.22	ng/ul	93
58) Fluorene	15.84	166	45800	1.75	ng/ul#	97
69) Phenanthrene	17.60	178	800992	23.19	ng/ul	99
71) Anthracene	17.69	178	141294	4.01	ng/ul	96
72) Carbazole	17.96	167	50015	1.76	ng/ul	95
74) Fluoranthene	19.61	202	1186591	33.56	ng/ul#	90
77) Pyrene	19.98	202	1235715	29.93	ng/ul#	92
80) Benzo(a)anthracene	21.86	228	675361	17.95	ng/ul	97
81) Bis(2-ethylhexyl)phthalate	21.73	149	34372	1.63	ng/ul#	95
82) Chrysene	21.93	228	679584m	19.87	ng/ul	
85) Benzo(b)fluoranthene	24.21	252	780729m	19.97	ng/ul	
86) Benzo(k)fluoranthene	24.26	252	265240m	6.89	ng/ul	
88) Benzo(a)pyrene	25.12	252	605996m	16.06	ng/ul	
89) Indeno(1,2,3-cd)pyrene	29.20	276	345655m	7.79	ng/ul	
90) Dibenzo(a,h)anthracene	29.25	278	103922m	2.75	ng/ul	
91) Benzo(g,h,i)perylene	30.43	276	344860m	9.38	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG081316\
Data File : BG023704.D
Acq On : 14 Aug 2016 1:25
Operator : UM/SJ
Sample : H4385-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P002-SS002-0206-01

Manual Integrations
APPROVED

umangi
8/16/2016 6:59:47 PM

Quant Time: Aug 15 19:42:00 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 06:38:14 2016
Response via : Initial Calibration

