

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081316\
 Data File : BG023685.D
 Acq On : 13 Aug 2016 12:45
 Operator : UM/SJ
 Sample : H4388-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PR002-SS002-3642-01

Quant Time: Aug 15 11:47:37 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 15 11:28:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	88438	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	410227	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	281970	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	671467	20.00	ng/ul	0.00
75) Chrysene-d12	21.88	240	698829	20.00	ng/ul	0.00
83) Perylene-d12	25.28	264	680038	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	4715	2.27	ng/uL	0.00
5) Phenol-d5	7.27	99	120774	13.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	82202	14.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	88347	14.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	93217	13.40	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	51064	15.79	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	57654	15.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.58	165	95791	13.67	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	124297	15.12	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	404473	17.52	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	443950	17.09	ng/ul	0.00
51) 4-Nitrophenol-d4	15.02	143	53099	13.47	ng/ul	0.01
57) Fluorene-d10	15.78	176	354354	16.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.91	200	51377	11.93	ng/ul	0.00
70) Anthracene-d10	17.65	188	551746	18.24	ng/ul	0.00
76) Pyrene-d10	19.94	212	602043	17.02	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.04	264	557978	18.13	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.23	163	189499	8.29	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081316\
Data File : BG023685.D
Acq On : 13 Aug 2016 12:45
Operator : UM/SJ
Sample : H4388-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PR002-SS002-3642-01

Quant Time: Aug 15 11:47:37 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 11:28:11 2016
Response via : Initial Calibration

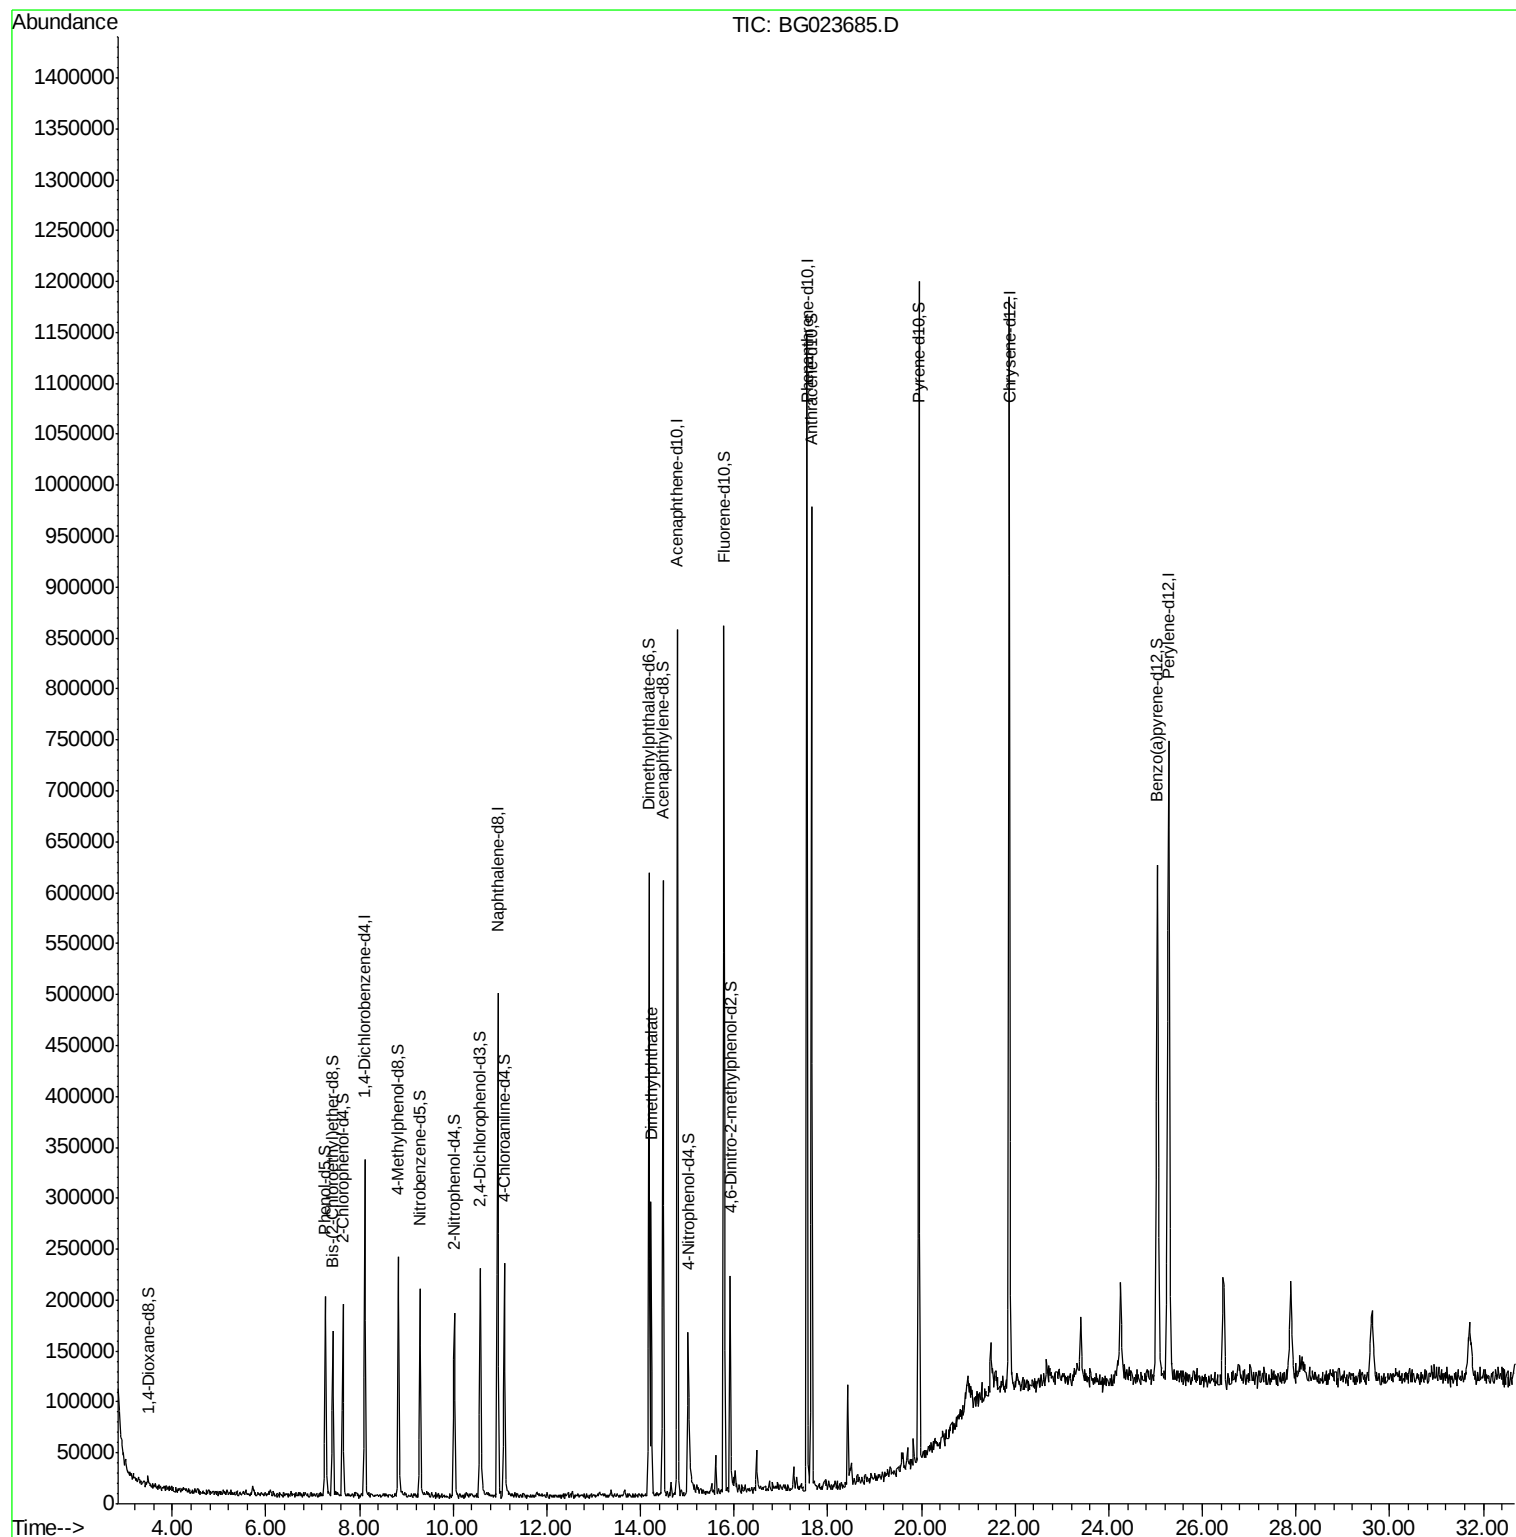

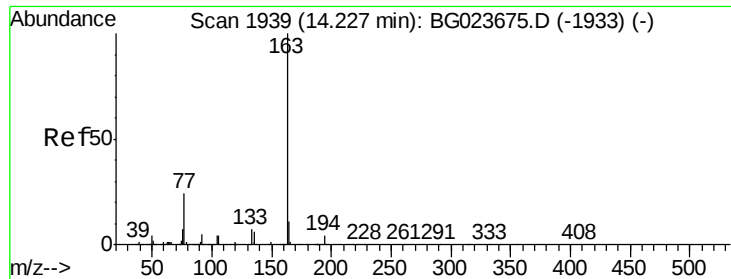

#44

Dimethylphthalate

Concen: 8.29 ng/ul

RT: 14.23 min Scan# 1939

Delta R.T. 0.00 min

Lab File: BG023685.D

Acq: 13 Aug 2016 12:45

Instrument :

BNA_G

ClientSampleId :

PR002-SS002-3642-01


Tot Ion:163 Resp: 189499

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 9.6 8.8 13.2

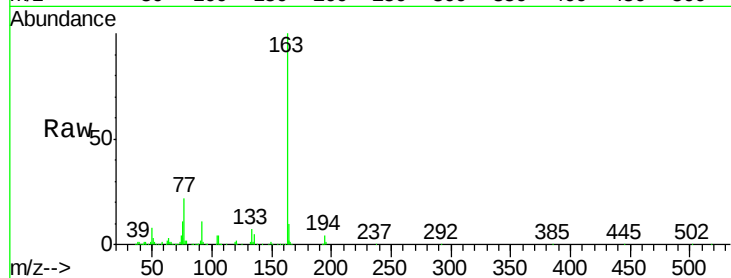

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

