

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081320\
 Data File : BG046261.D
 Acq On : 13 Aug 2020 23:04
 Operator : CG/JU
 Sample : L3629-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BFM55

Manual Integrations
 APPROVED

Sohil
 8/14/2020 2:52:36 PM

Quant Time: Aug 14 07:58:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 13:50:19 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.95	152	122385	20.00	ng/ul	0.00
2) Naphthalene-d8	10.75	136	481651	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.57	164	308932	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.32	188	695353	20.00	ng/ul	0.00
18) Chrysene-d12	21.56	240	694809	20.00	ng/ul	0.00
23) Perylene-d12	24.67	264	734178	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.37	165	134347	16.20	ng/ul	0.00
7) Acenaphthylene-d8	14.27	160	511564	17.99	ng/ul	0.00
10) Fluorene-d10	15.57	176	389063	17.86	ng/ul	0.00
15) Anthracene-d10	17.41	188	573872	17.80	ng/ul	0.00
19) Pyrene-d10	19.70	212	664757	18.59	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.46	264	715117	17.85	ng/ul	0.00
Target Compounds				Qvalue		
14) Phenanthrene	17.36	178	62833	1.643	ng/ul	99
17) Fluoranthene	19.37	202	184477	4.325	ng/ul	98
20) Pyrene	19.73	202	185251	4.062	ng/ul	98
21) Benzo(a)anthracene	21.54	228	99326	2.197	ng/ul	95
22) Chrysene	21.61	228	115925	2.653	ng/ul	95
24) Benzo(b)fluoranthene	23.69	252	159197	3.279	ng/ul	98
25) Benzo(k)fluoranthene	23.75	252	59299m	1.231	ng/ul	
27) Benzo(a)pyrene	24.52	252	108911	2.443	ng/ul	100
28) Indeno(1,2,3-cd)pyrene	28.17	276	84474	1.514	ng/ul	95
30) Benzo(g,h,i)perylene	29.26	276	81297	1.741	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081320\
Data File : BG046261.D
Acq On : 13 Aug 2020 23:04
Operator : CG/JU
Sample : L3629-08
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BFM55

Quant Time: Aug 14 07:58:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 13 13:50:19 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
8/14/2020 2:52:36 PM

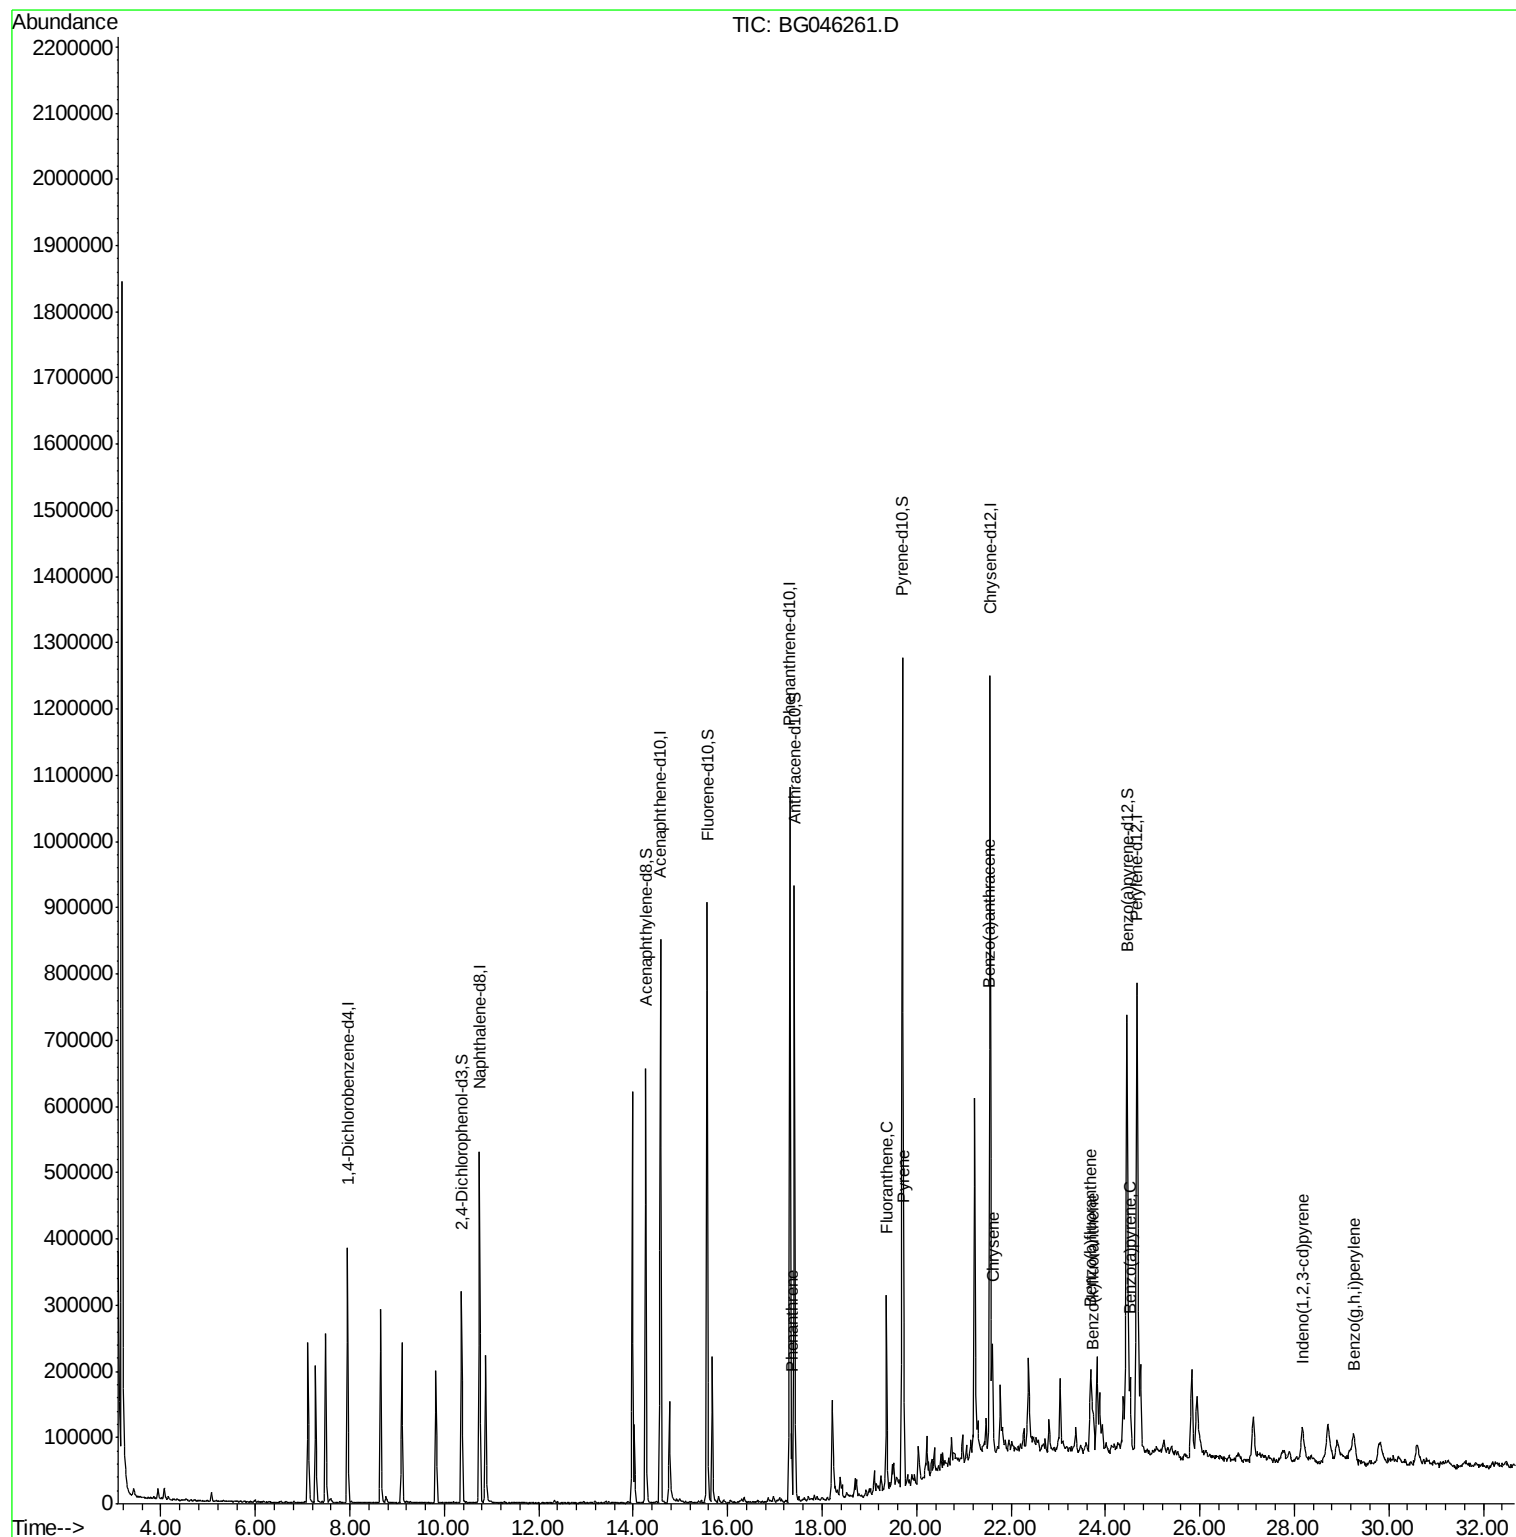

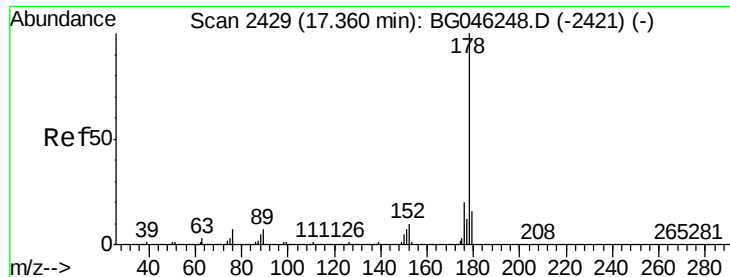

#14

Phenanthrene

Concen: 1.643 ng/ul

RT: 17.36 min Scan# 2429

Delta R.T. 0.00 min

Lab File: BG046261.D

Acq: 13 Aug 2020 23:04

Instrument :

BNA_G


ClientSampled :

BFM55




Tot Ion:178	Resp:	62833
Ion Ratio	Lower	Upper
178	100	
179	15.7	12.8 19.2
176	18.8	15.8 23.8

Manual Integrations
APPROVED

Sohil
8/14/2020 2:52:36 PM

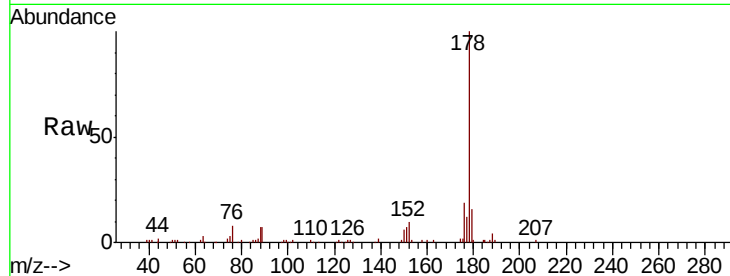

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

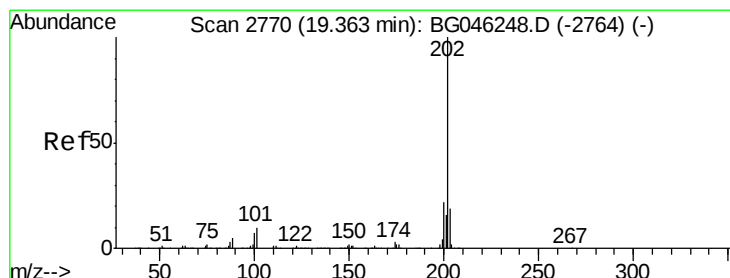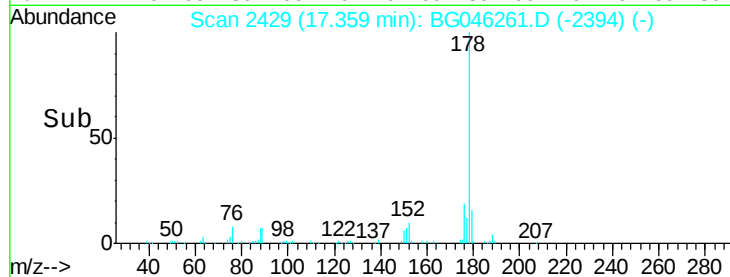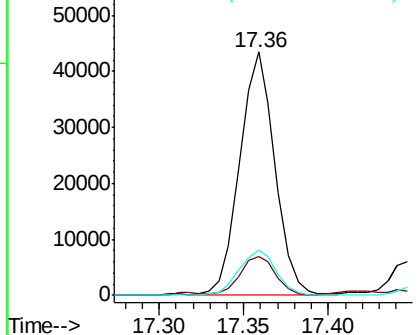

#17

Fluoranthene

Concen: 4.325 ng/ul


RT: 19.37 min Scan# 2771

Delta R.T. 0.00 min



Lab File: BG046261.D


Acq: 13 Aug 2020 23:04

Tgt Ion:202	Resp:	184477
Ion Ratio	Lower	Upper
202	100	
101	9.5	7.8 11.6
100	6.4	5.9 8.9

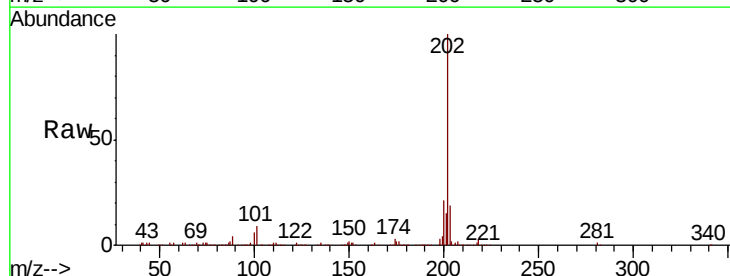

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

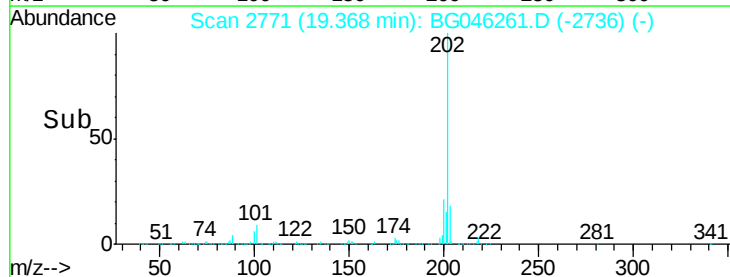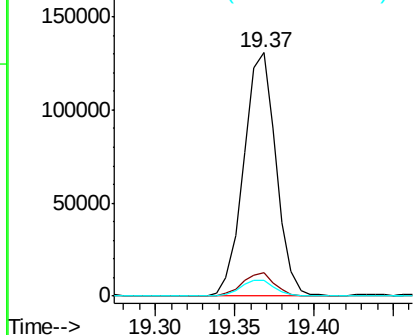

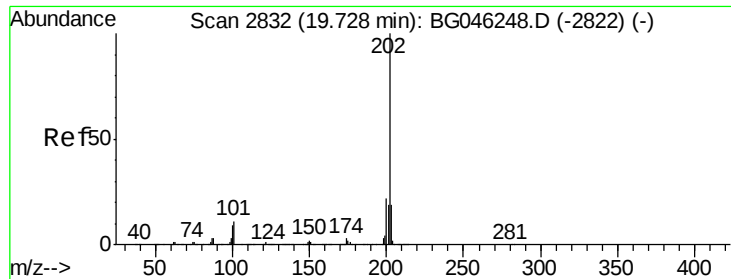





#20
Pvrene
Concen: 4.062 ng/ul
RT: 19.73 min Scan# 2832
Delta R.T. 0.00 min
Lab File: BG046261.D
Acq: 13 Aug 2020 23:04

Instrument :
BNA_G
ClientSampleId :
BFM55

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	10.4	8.9	13.3
100	9.0	7.9	11.9




Manual Integrations
APPROVED


Sohil
8/14/2020 2:52:36 PM

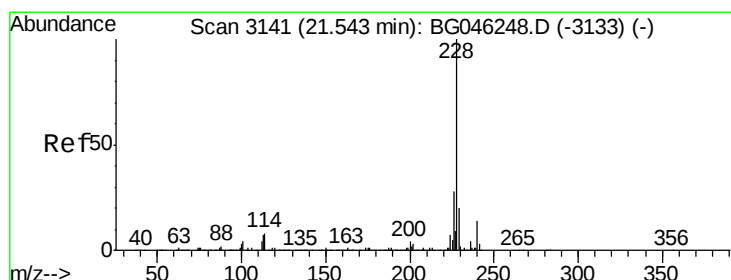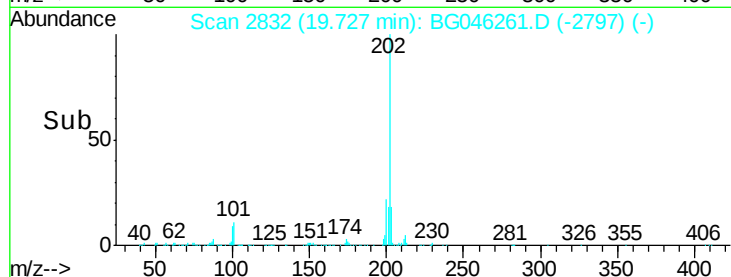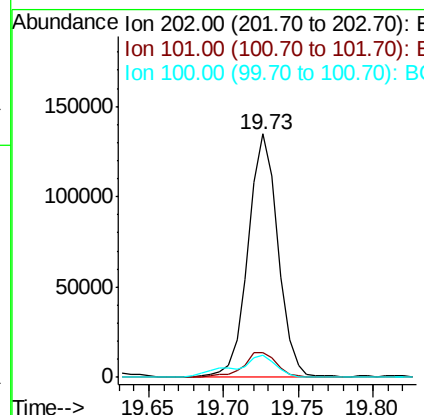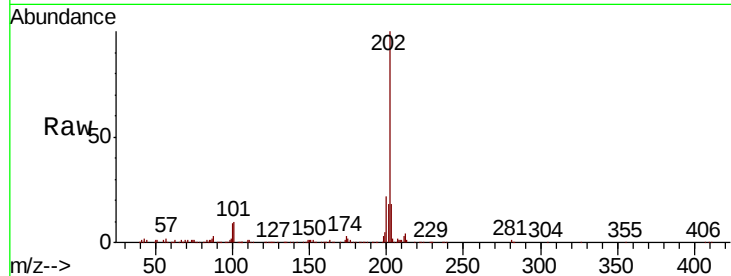

#21
Benzo(a)anthracene
Concen: 2.197 ng/ul
RT: 21.54 min Scan# 3141
Delta R.T. -0.00 min
Lab File: BG046261.D
Acq: 13 Aug 2020 23:04

Tgt Ion	Ratio	Resp Lower	Upper
228	100		
229	19.1	16.6	25.0
226	31.3	22.6	33.8

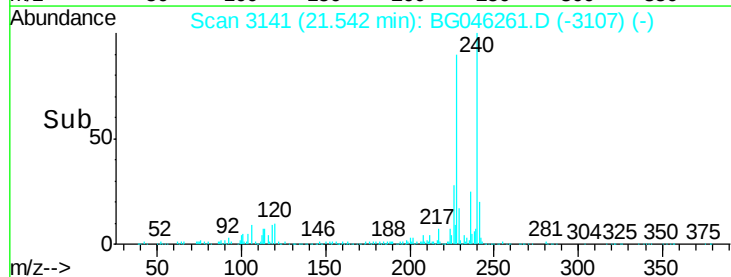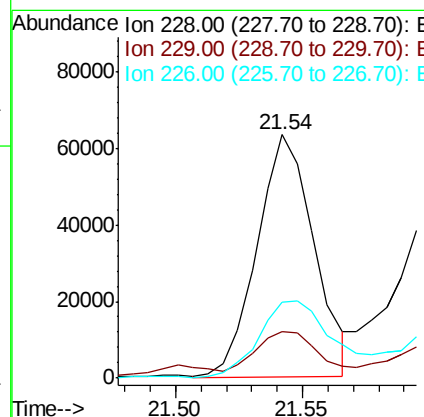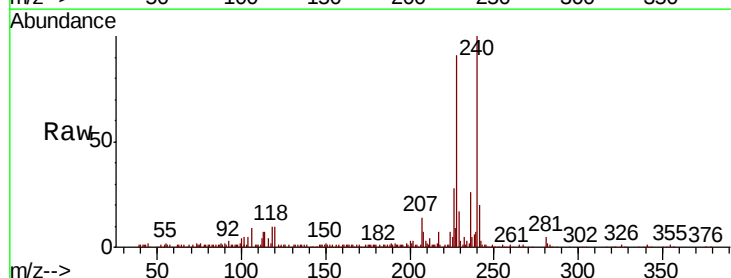

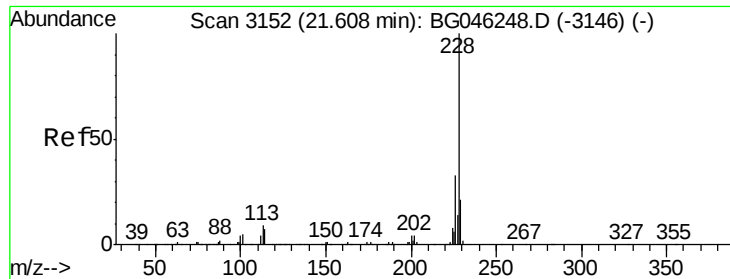

#22

Chrysene

Concen: 2.653 ng/ul

RT: 21.61 min Scan# 3152

Delta R.T. 0.00 min

Lab File: BG046261.D

Acq: 13 Aug 2020 23:04

Instrument :

BNA_G





ClientSampleId :

BFM55

Tot Ion:	228	Resp:	115925
Ion Ratio		Lower	Upper
228	100		
226	28.5	25.5	38.3
229	22.4	17.0	25.4

Manual Integrations
APPROVED

Sohil
8/14/2020 2:52:36 PM

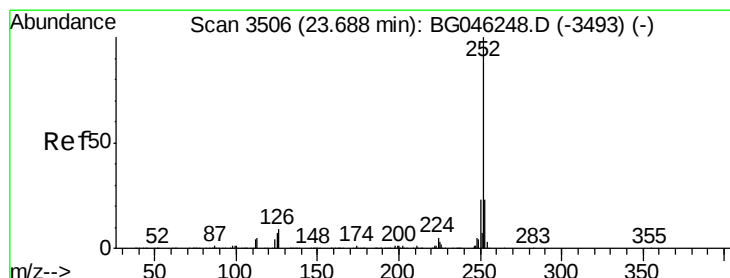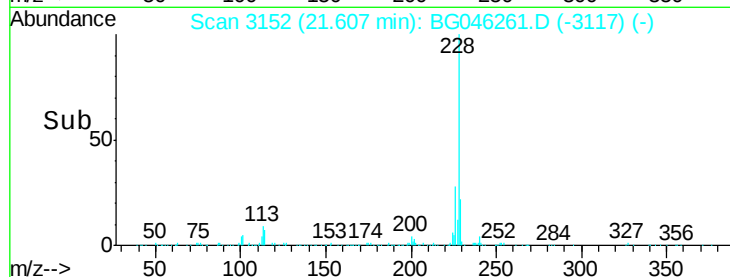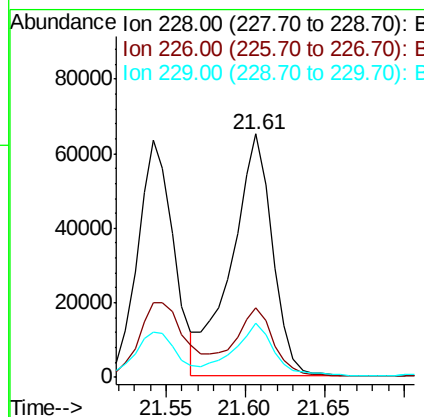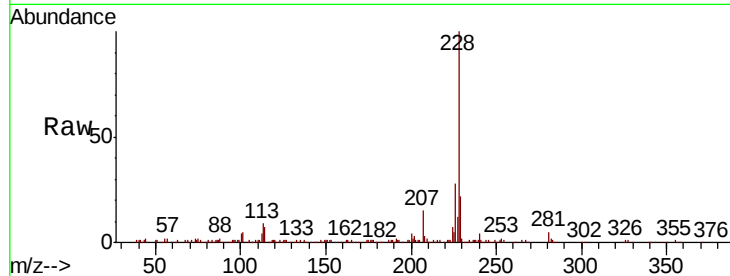

#24

Benzo(b)fluoranthene

Concen: 3.279 ng/ul




RT: 23.69 min Scan# 3506


Delta R.T. 0.00 min

Lab File: BG046261.D

Acq: 13 Aug 2020 23:04

Tgt Ion:	252	Resp:	159197
Ion Ratio		Lower	Upper
252	100		
253	21.4	17.8	26.6
125	7.4	6.4	9.6

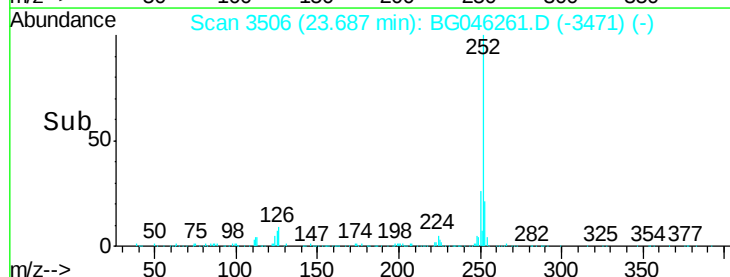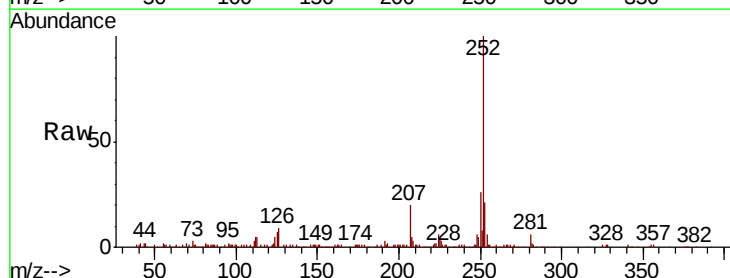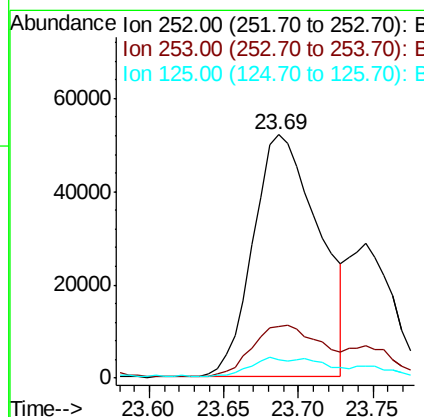

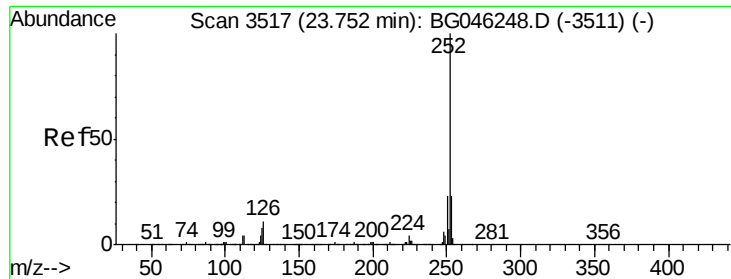





#25
Benzo(k)fluoranthene
Concen: 1.231 ng/ul m
RT: 23.75 min Scan# 3516
Delta R.T. -0.00 min
Lab File: BG046261.D
Acq: 13 Aug 2020 23:04

Instrument :
BNA_G
ClientSampleId :
BFM55

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.8	18.5	27.7
125	8.7	6.2	9.2




Manual Integrations
APPROVED


Sohil
8/14/2020 2:52:36 PM

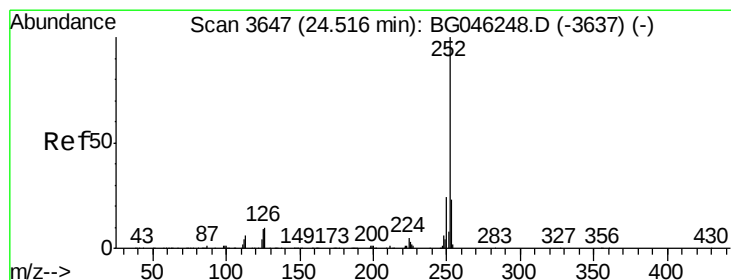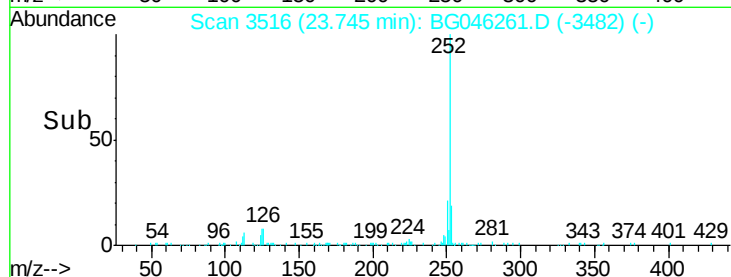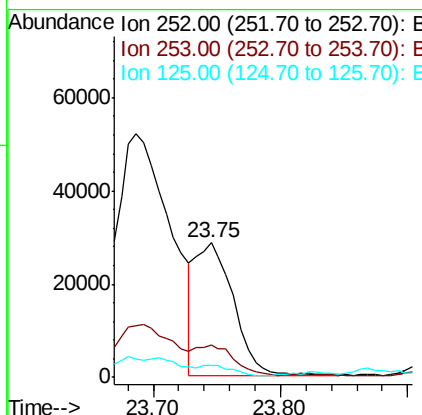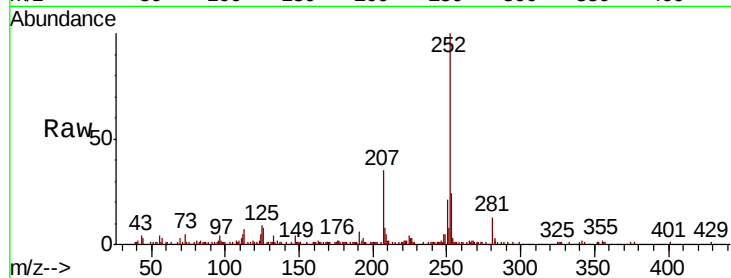

#27
Benzo(a)pyrene
Concen: 2.443 ng/ul
RT: 24.52 min Scan# 3648
Delta R.T. -0.00 min
Lab File: BG046261.D
Acq: 13 Aug 2020 23:04

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.8	26.8
125	9.0	7.1	10.7

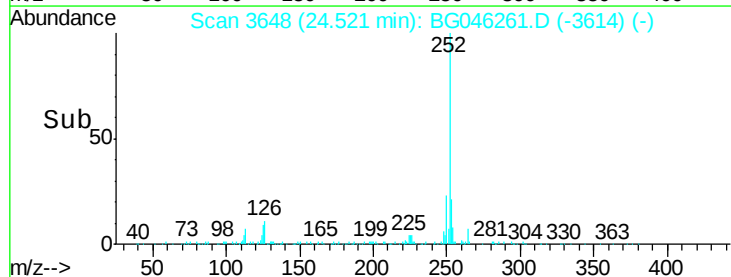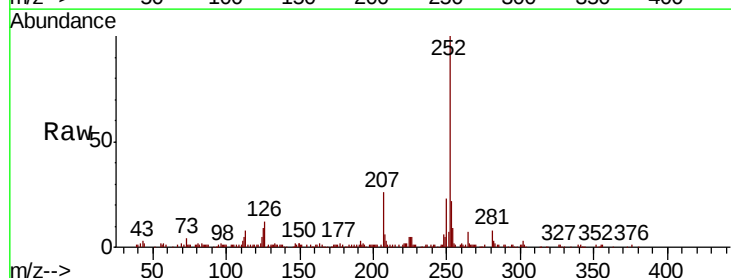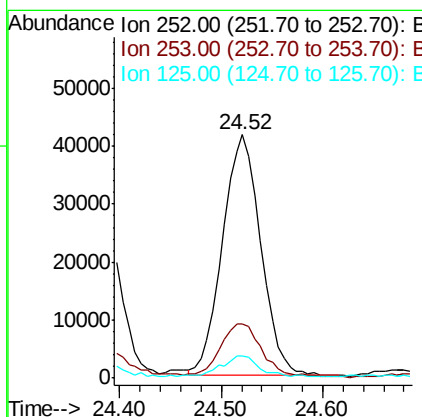

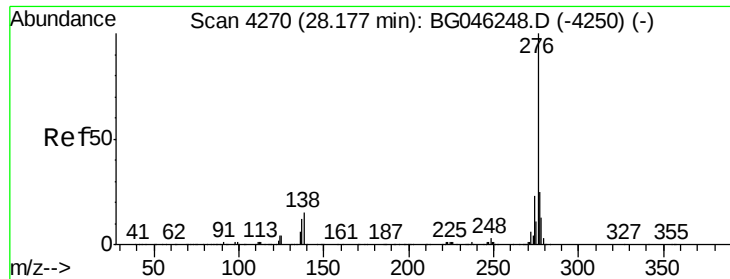

#28





Indeno(1,2,3-cd)pyrene
Concen: 1.514 ng/ul
RT: 28.17 min Scan# 4269
Delta R.T. -0.00 min
Lab File: BG046261.D
Acq: 13 Aug 2020 23:04

Instrument :
BNA_G
ClientSampled :
BFM55

Tot Ion	Ratio	Lower	Upper
276	100		
138	18.4	13.2	19.8
277	27.8	19.9	29.9

Manual Integrations
APPROVED

Sohil
8/14/2020 2:52:36 PM

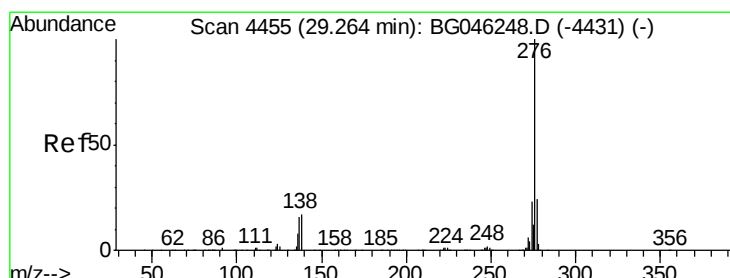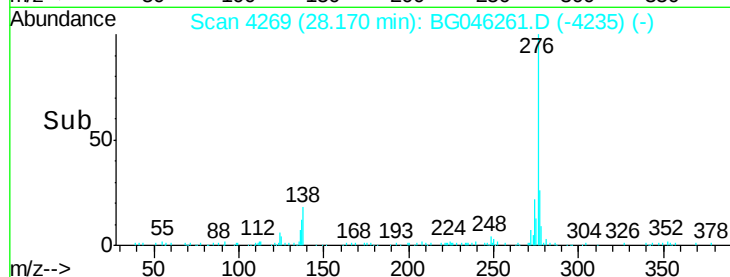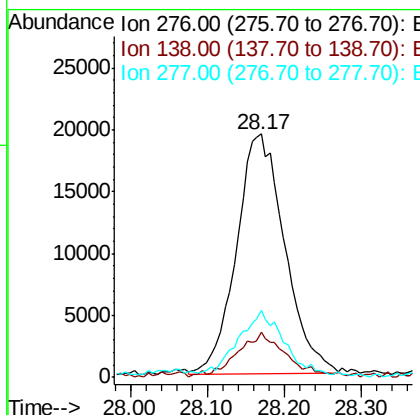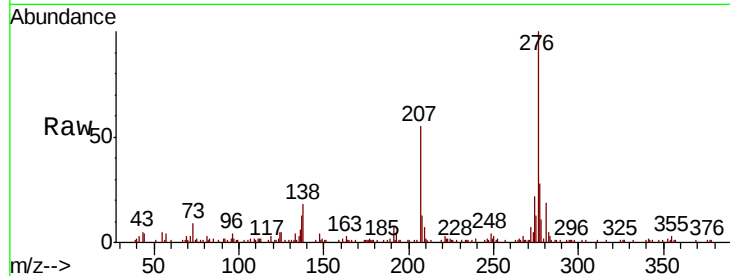

#30

Benzo(g,h,i)perylene
Concen: 1.741 ng/ul
RT: 29.26 min Scan# 4454
Delta R.T. -0.01 min
Lab File: BG046261.D
Acq: 13 Aug 2020 23:04

Tgt Ion	Ratio	Lower	Upper
276	100		
138	17.8	12.9	19.3
277	21.0	19.4	29.0

