

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
 Data File : BG062380.D
 Acq On : 13 Aug 2024 11:27
 Operator : MA/JU
 Sample : P3502-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCXU0

Quant Time: Aug 13 12:48:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 09 01:00:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	54836	20.000	ng/u1	0.00
20) Naphthalene-d8	10.751	136	262426	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.575	164	201415	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.313	188	462063	20.000	ng/u1	0.00
79) Chrysene-d12	21.554	240	432235	20.000	ng/u1	0.00
88) Perylene-d12	24.644	264	499751	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	3440	2.705	ng/uL	0.00
4) Pyridine-d5	3.819	84	53626	13.404	ng/u1	0.00
7) Phenol-d5	7.109	99	82177	15.701	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.279	67	49331	15.311	ng/u1	0.00
11) 2-Chlorophenol-d4	7.485	132	59576	15.887	ng/u1	0.00
15) 4-Methylphenol-d8	8.648	113	49611	11.380	ng/u1	0.00
21) Nitrobenzene-d5	9.106	128	28491	17.607	ng/u1	0.00
24) 2-Nitrophenol-d4	9.823	143	31243	20.525	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	71100	16.082	ng/u1	0.00
31) 4-Chloroaniline-d4	10.874	131	69683	10.867	ng/u1	0.00
46) Dimethylphthalate-d6	13.982	166	251376	16.176	ng/u1	0.00
49) Acenaphthylene-d8	14.264	160	280315	15.909	ng/u1	0.00
54) 4-Nitrophenol-d4	14.746	143	35421	16.281	ng/u1	0.00
60) Fluorene-d10	15.562	176	235527	16.885	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.668	200	27664	20.216	ng/u1	0.00
73) Anthracene-d10	17.412	188	378350	16.977	ng/u1	0.00
81) Pyrene-d10	19.692	212	451412	17.571	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.432	264	461716	17.283	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	16.960	266	23274	7.217	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
Data File : BG062380.D
Acq On : 13 Aug 2024 11:27
Operator : MA/JU
Sample : P3502-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXU0

Quant Time: Aug 13 12:48:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 09 01:00:03 2024
Response via : Initial Calibration

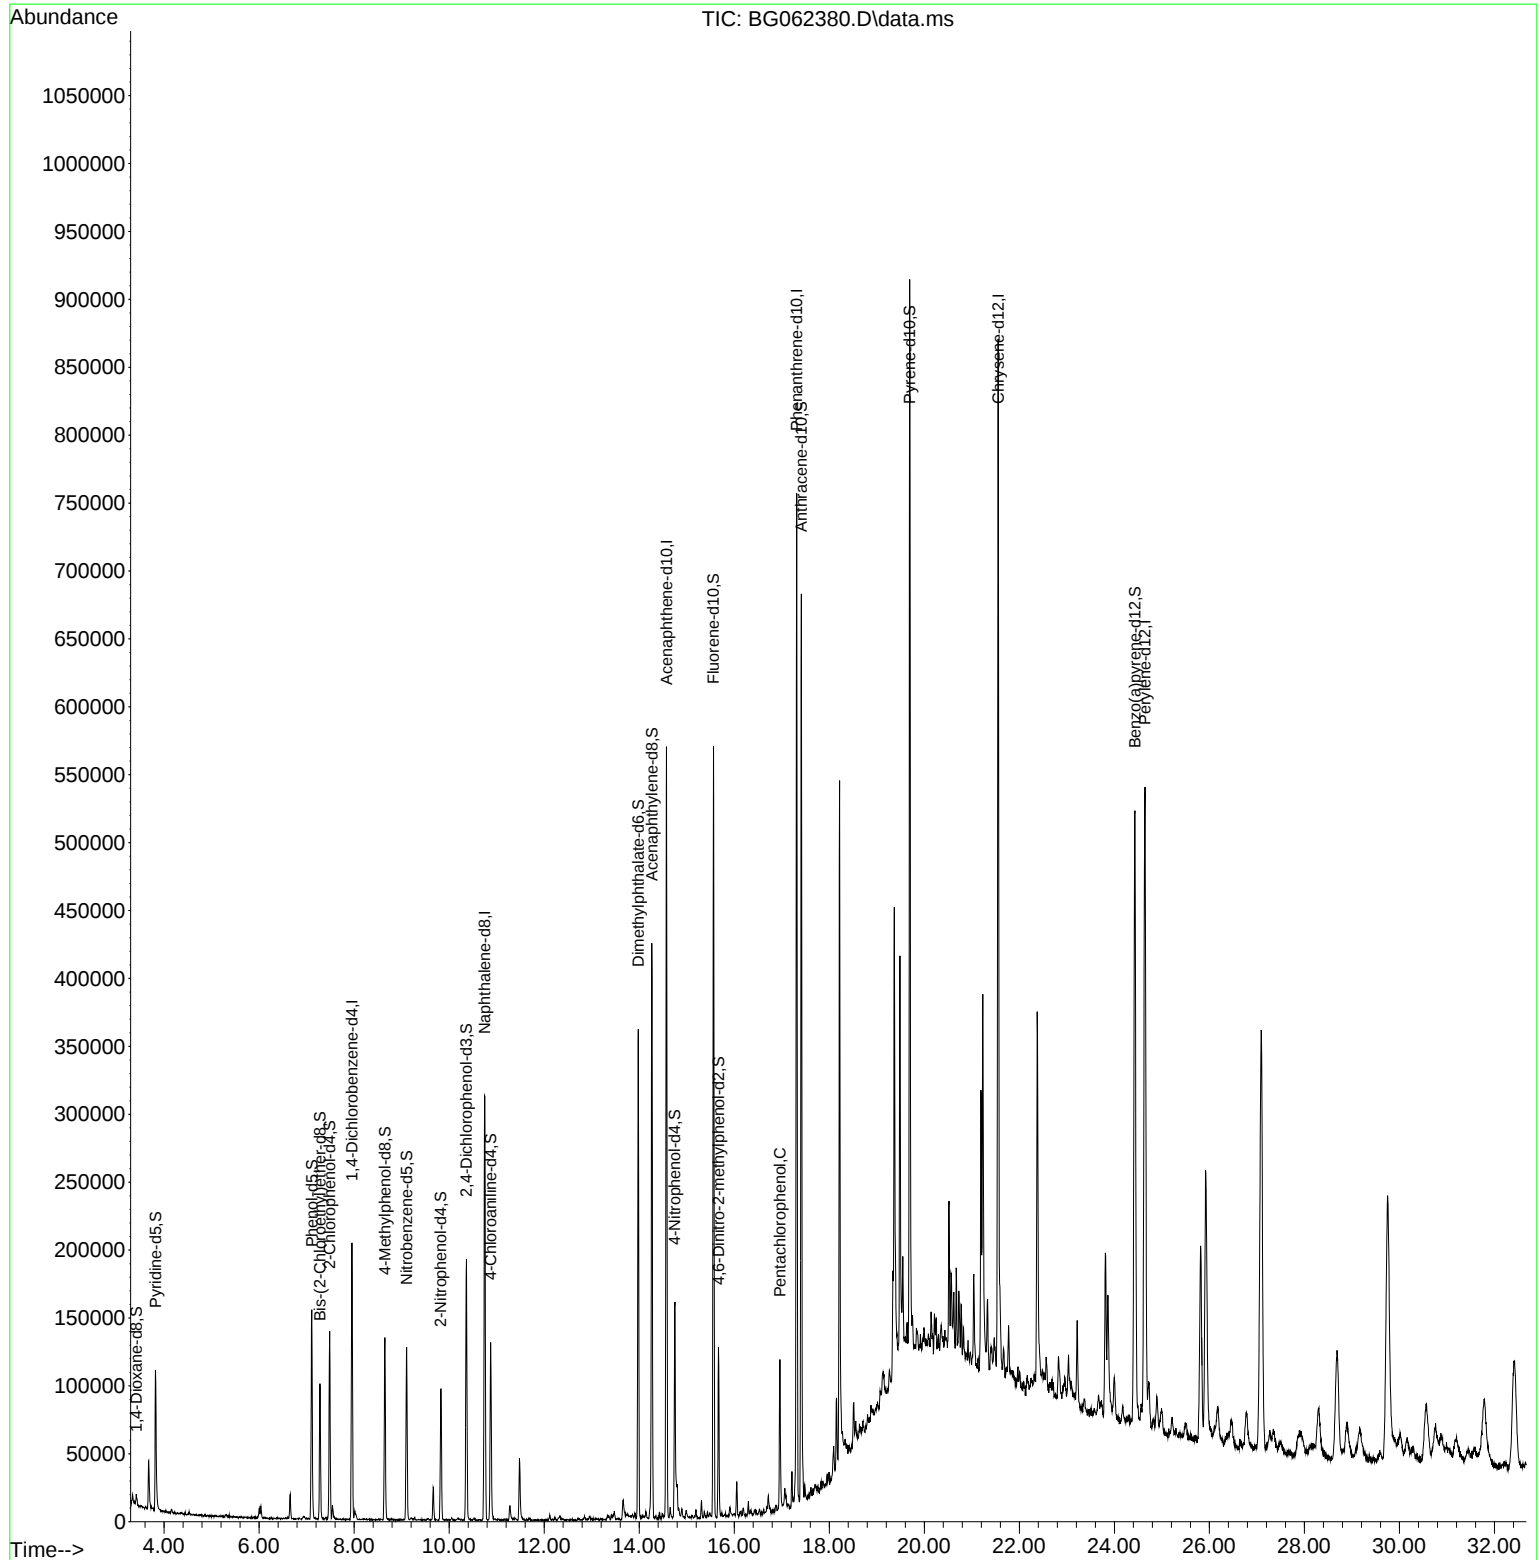

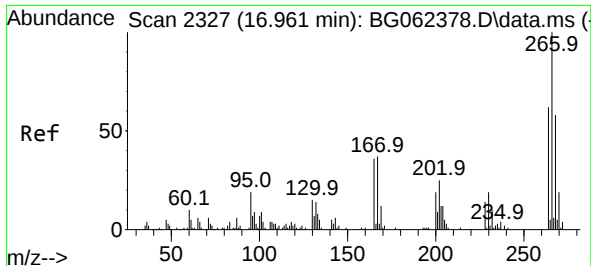

#71
Pentachlorophenol
Concen: 7.217 ng/ul
RT: 16.960 min Scan# 21
Delta R.T. -0.003 min
Lab File: BG062380.D
Acq: 13 Aug 2024 11:27

Instrument :
BNA_G
ClientSampleId :
DCXU0

Tgt Ion:266 Resp: 23274
Ion Ratio Lower Upper
266 100
264 63.1 48.9 73.3
268 61.5 51.2 76.8

