

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
 Data File : BG062381.D
 Acq On : 13 Aug 2024 12:07
 Operator : MA/JU
 Sample : P3502-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCXV1

Quant Time: Aug 13 12:49:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 09 01:00:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.953	152	54023	20.000	ng/ul	0.00
20) Naphthalene-d8	10.744	136	254484	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.568	164	191992	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.311	188	419151	20.000	ng/ul	0.00
79) Chrysene-d12	21.553	240	388309	20.000	ng/ul	0.00
88) Perylene-d12	24.637	264	447038	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.418	96	4466	3.565	ng/uL	0.00
4) Pyridine-d5	3.824	84	26088	6.619	ng/ul	0.00
7) Phenol-d5	7.107	99	120524	23.374	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.278	67	70563	22.231	ng/ul	0.00
11) 2-Chlorophenol-d4	7.483	132	86957	23.538	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	78186	18.204	ng/ul	0.00
21) Nitrobenzene-d5	9.105	128	44679	28.473	ng/ul	0.00
24) 2-Nitrophenol-d4	9.827	143	49328	33.417	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.362	165	107004	24.958	ng/ul	0.00
31) 4-Chloroaniline-d4	10.873	131	52180	8.391	ng/ul	0.00
46) Dimethylphthalate-d6	13.980	166	362667	24.483	ng/ul	0.00
49) Acenaphthylene-d8	14.262	160	417240	24.843	ng/ul	0.00
54) 4-Nitrophenol-d4	14.750	143	42007	20.256	ng/ul	0.00
60) Fluorene-d10	15.561	176	335936	25.266	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.666	200	41401	33.352	ng/ul	0.00
73) Anthracene-d10	17.405	188	495401	24.505	ng/ul	0.00
81) Pyrene-d10	19.690	212	602720	26.114	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.425	264	597904	25.019	ng/ul	0.00
Target Compounds						
71) Pentachlorophenol	16.959	266	16071	5.494	ng/ul	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
Data File : BG062381.D
Acq On : 13 Aug 2024 12:07
Operator : MA/JU
Sample : P3502-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXV1

Quant Time: Aug 13 12:49:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 09 01:00:03 2024
Response via : Initial Calibration

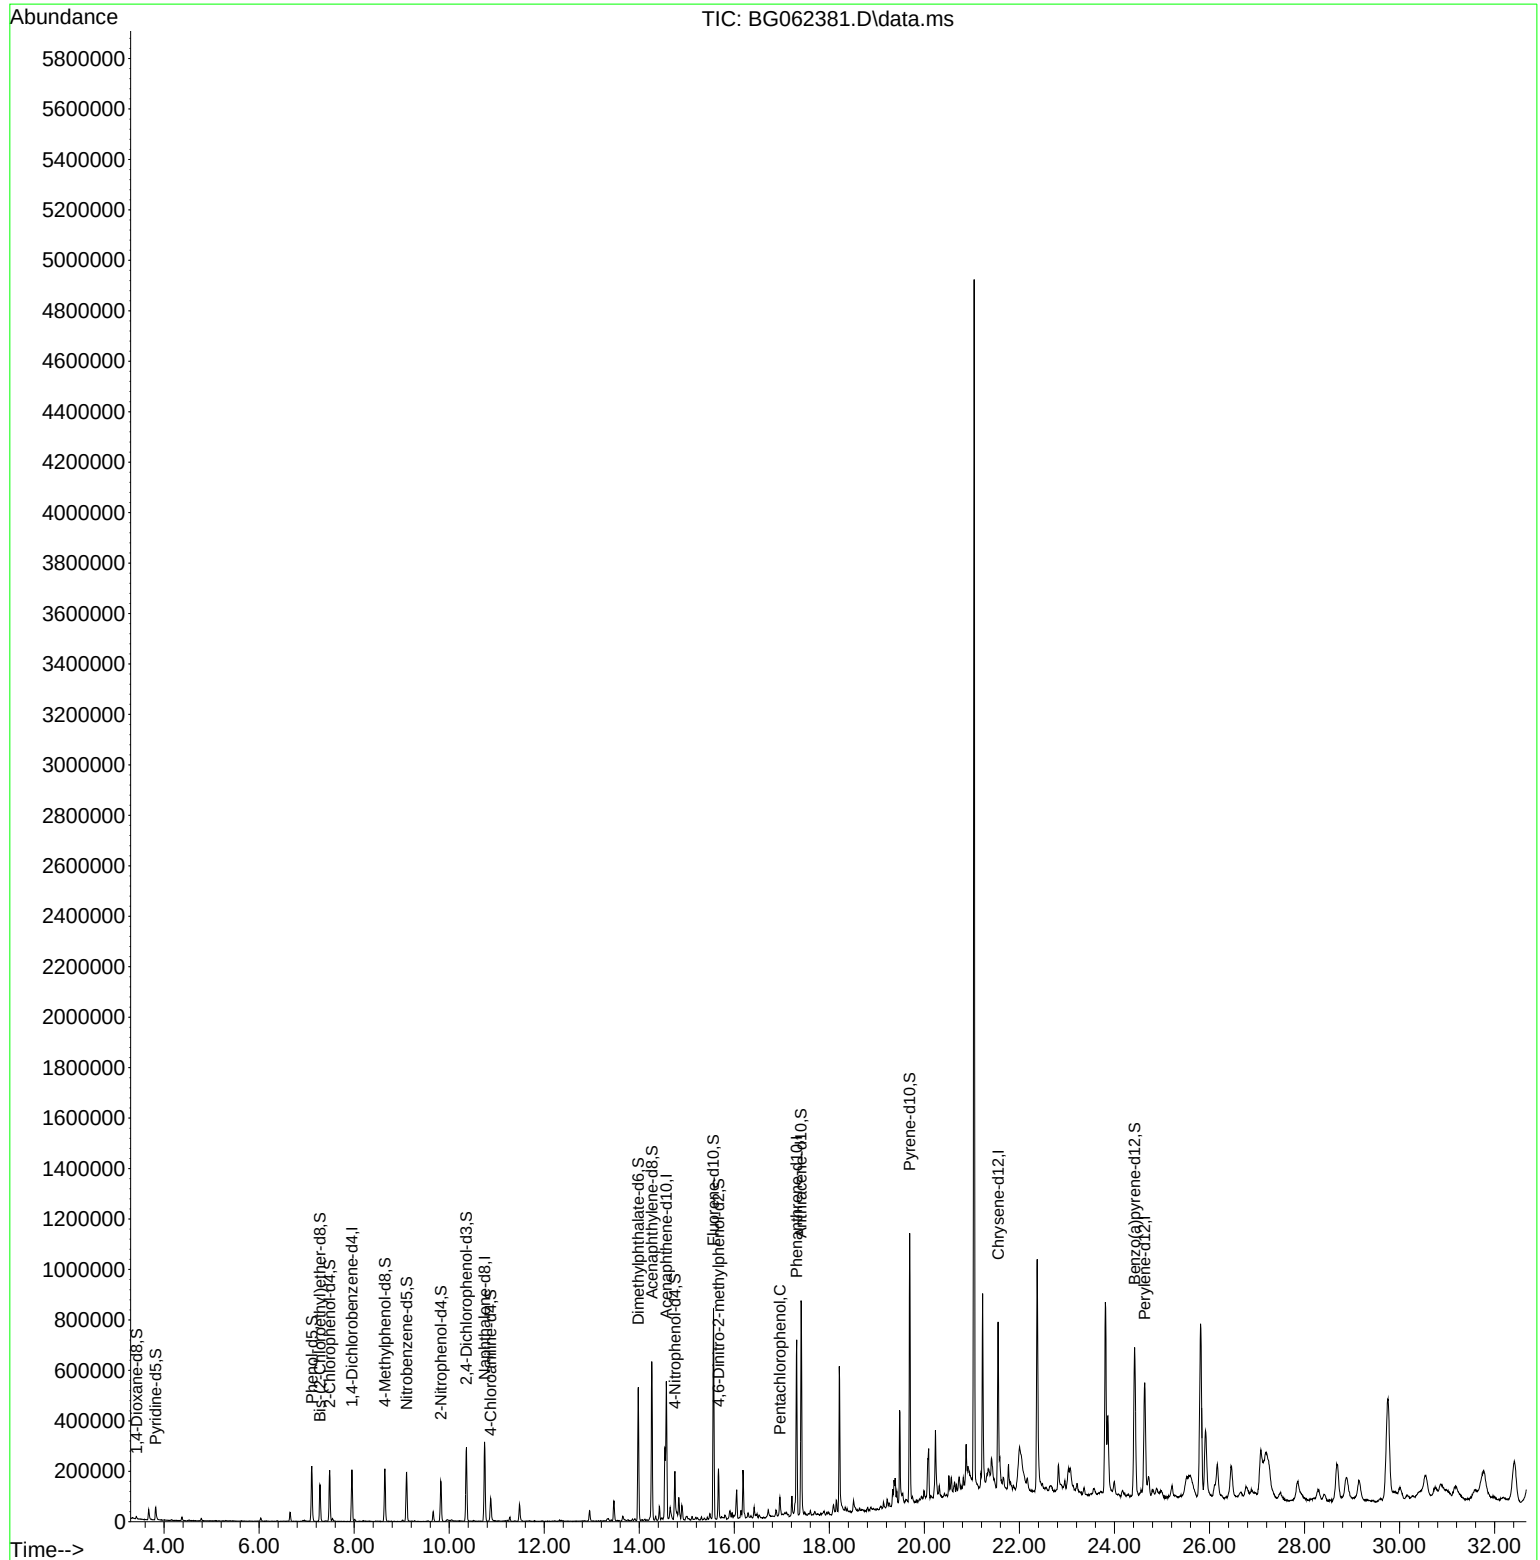

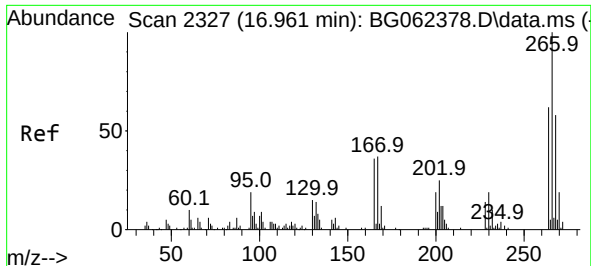

#71
Pentachlorophenol
Concen: 5.494 ng/ul
RT: 16.959 min Scan# 21
Delta R.T. -0.004 min
Lab File: BG062381.D
Acq: 13 Aug 2024 12:07

Instrument :
BNA_G
ClientSampleId :
DCXV1

Tgt Ion	Ratio	Lower	Upper
266	100		
264	52.5	48.9	73.3
268	59.3	51.2	76.8

