

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
 Data File : BG062384.D
 Acq On : 13 Aug 2024 14:10
 Operator : MA/JU
 Sample : P3502-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCXU7

Quant Time: Aug 13 15:28:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 09 01:00:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	54682	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	265025	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.570	164	198684	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.313	188	424890	20.000	ng/u1	0.00
79) Chrysene-d12	21.555	240	395751	20.000	ng/u1	0.00
88) Perylene-d12	24.645	264	446309	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	3646	2.875	ng/uL	0.00
4) Pyridine-d5	3.820	84	57739	14.472	ng/u1	0.00
7) Phenol-d5	7.109	99	101180	19.386	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.280	67	54237	16.881	ng/u1	0.00
11) 2-Chlorophenol-d4	7.485	132	70523	18.859	ng/u1	0.00
15) 4-Methylphenol-d8	8.649	113	75698	17.413	ng/u1	0.00
21) Nitrobenzene-d5	9.107	128	34498	21.110	ng/u1	0.00
24) 2-Nitrophenol-d4	9.823	143	38888	25.296	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.364	165	83734	18.754	ng/u1	0.00
31) 4-Chloroaniline-d4	10.875	131	92334	14.258	ng/u1	0.00
46) Dimethylphthalate-d6	13.977	166	271009	17.679	ng/u1	0.00
49) Acenaphthylene-d8	14.264	160	315223	18.136	ng/u1	0.00
54) 4-Nitrophenol-d4	14.752	143	40407	18.828	ng/u1	0.00
60) Fluorene-d10	15.563	176	253869	18.451	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.668	200	30035	23.869	ng/u1	0.00
73) Anthracene-d10	17.407	188	383683	18.722	ng/u1	0.00
81) Pyrene-d10	19.692	212	463324	19.697	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.427	264	456824	19.147	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.961	266	5431	1.831	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
Data File : BG062384.D
Acq On : 13 Aug 2024 14:10
Operator : MA/JU
Sample : P3502-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXU7


Quant Time: Aug 13 15:28:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 09 01:00:03 2024
Response via : Initial Calibration

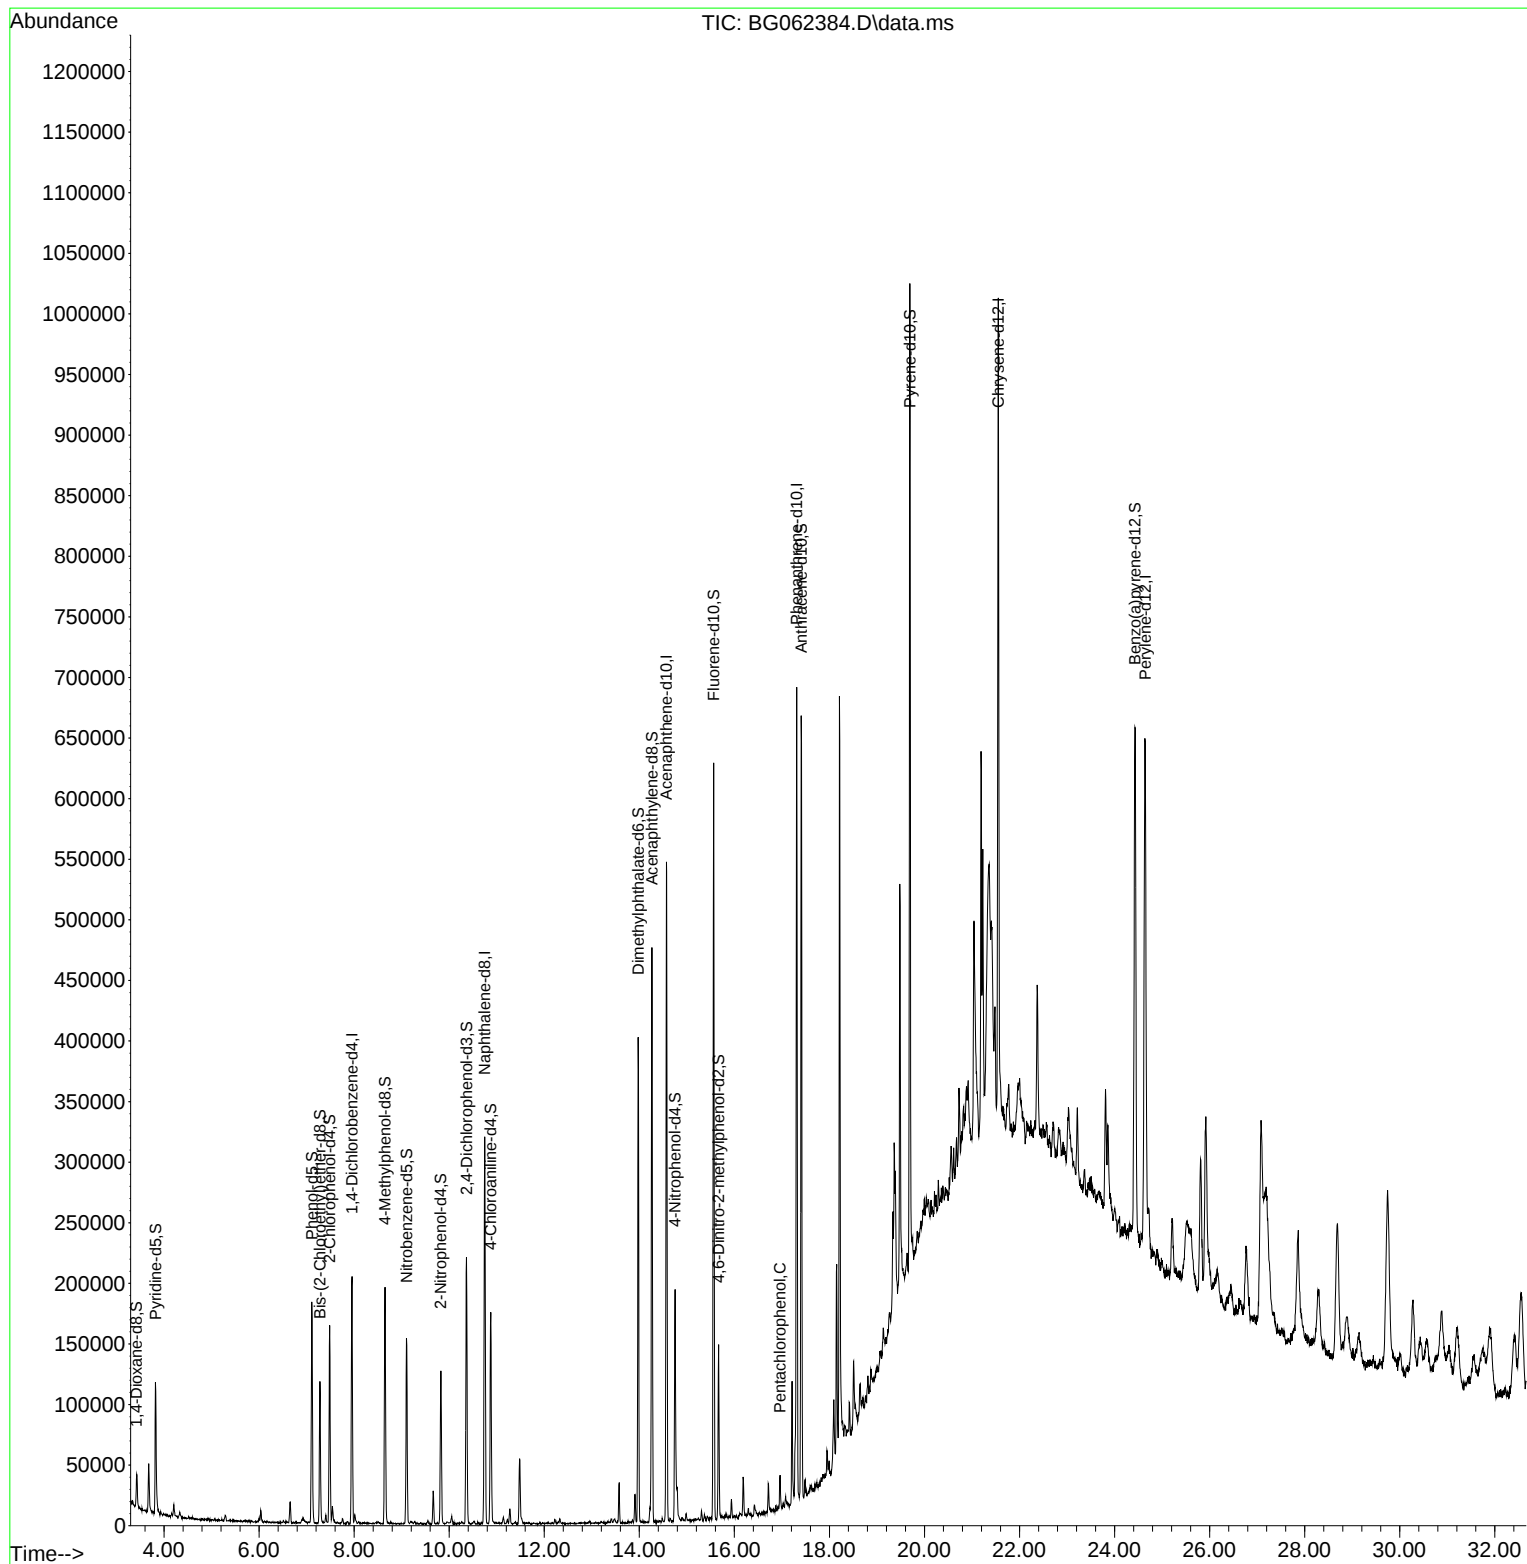

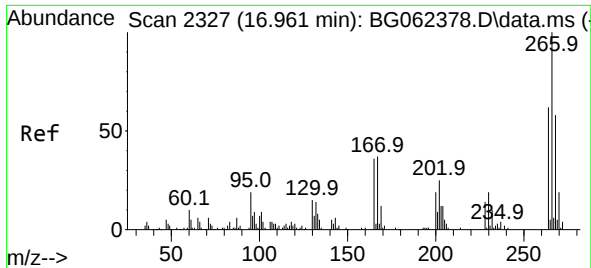

#71
 Pentachlorophenol
 Concen: 1.831 ng/ul
 RT: 16.961 min Scan# 21
 Delta R.T. -0.002 min
 Lab File: BG062384.D
 Acq: 13 Aug 2024 14:10

Instrument :
 BNA_G
 ClientSampleId :
 DCXU7

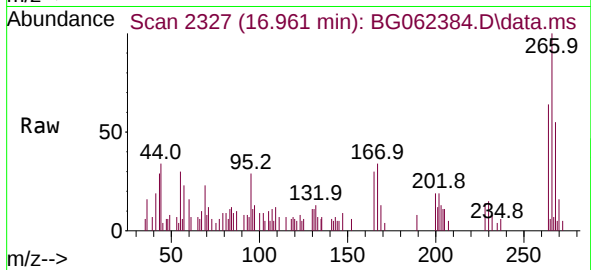

Tgt Ion:266 Resp: 5431
 Ion Ratio Lower Upper
 266 100
 264 63.7 48.9 73.3
 268 54.8 51.2 76.8

