

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
 Data File : BG062379.D
 Acq On : 13 Aug 2024 10:46
 Operator : MA/JU
 Sample : PB162649BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062379.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.414	18	21	27	rVB2	11170	18358	1.06%	0.113%
2	3.767	79	81	83	rBV2	1699	1871	0.11%	0.012%
3	3.820	86	90	103	rVV	164247	265442	15.30%	1.641%
4	4.096	135	137	140	rVB2	1475	1767	0.10%	0.011%
5	4.166	143	149	152	rBV4	2343	4043	0.23%	0.025%
6	7.104	642	649	659	rBV	192779	326245	18.80%	2.016%
7	7.280	671	679	689	rBV	151723	246296	14.19%	1.522%
8	7.480	707	713	722	rVB	169899	290026	16.72%	1.793%
9	7.949	787	793	801	rBV	144954	244065	14.07%	1.509%
10	8.643	904	911	921	rVB	243755	411830	23.74%	2.545%
11	9.101	982	989	998	rBV	175151	311542	17.96%	1.926%
12	9.823	1104	1112	1121	rVB	140443	238835	13.76%	1.476%
13	10.358	1196	1203	1215	rBV	247182	428622	24.70%	2.649%
14	10.746	1261	1269	1278	rVB	236463	407918	23.51%	2.521%
15	10.875	1283	1291	1299	rBV	242219	439223	25.31%	2.715%
16	12.332	1532	1539	1545	rVB3	3705	6099	0.35%	0.038%
17	13.977	1813	1819	1828	rBV	542095	759843	43.79%	4.697%
18	14.264	1861	1868	1877	rVB	588943	906836	52.26%	5.605%
19	14.570	1912	1920	1928	rBV	442187	682673	39.35%	4.220%
20	14.746	1944	1950	1964	rBV	263038	408586	23.55%	2.525%
21	15.563	2081	2089	2099	rVB	834404	1229598	70.87%	7.600%
22	15.668	2101	2107	2118	rBV	191012	282130	16.26%	1.744%
23	15.798	2126	2129	2133	rVB	2889	3301	0.19%	0.020%
24	16.344	2219	2222	2228	rVB3	1999	3085	0.18%	0.019%
25	17.313	2380	2387	2393	rVV	601588	906337	52.24%	5.602%
26	17.407	2396	2403	2415	rVV	964003	1407489	81.12%	8.700%
27	17.683	2447	2450	2454	rVB3	1136	1837	0.11%	0.011%
28	18.224	2537	2542	2544	rBV3	1427	2431	0.14%	0.015%
29	19.258	2715	2718	2722	rVB2	10497	13675	0.79%	0.085%
30	19.328	2725	2730	2734	rBV	10169	13510	0.78%	0.084%
31	19.692	2785	2792	2802	rBV	1178529	1671399	96.33%	10.331%
32	19.839	2816	2817	2821	rBV3	1651	2273	0.13%	0.014%
33	20.074	2852	2857	2860	rVB3	1684	3027	0.17%	0.019%
34	20.250	2885	2887	2889	rVB3	2091	1891	0.11%	0.012%
35	20.427	2914	2917	2918	rBV2	2103	1771	0.10%	0.011%
36	20.456	2918	2922	2923	rBV4	2415	3172	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
 Data File : BG062379.D
 Acq On : 13 Aug 2024 10:46
 Operator : MA/JU
 Sample : PB162649BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	20.673	2956	2959	2962	rBV4	3204	4431	0.26%	0.027%
38	20.738	2966	2970	2973	rBV4	2810	4761	0.27%	0.029%
39	21.126	3033	3036	3038	rBV2	2108	3068	0.18%	0.019%
40	21.196	3047	3048	3051	rVB3	2734	2196	0.13%	0.014%
41	21.243	3051	3056	3058	rBV6	6262	9254	0.53%	0.057%
42	21.402	3081	3083	3085	rBV3	2160	1932	0.11%	0.012%
43	21.549	3101	3108	3117	rBV	631222	995002	57.35%	6.150%
44	21.772	3142	3146	3150	rBV5	13417	24922	1.44%	0.154%
45	22.295	3233	3235	3236	rBV2	3355	3028	0.17%	0.019%
46	22.359	3242	3246	3259	rVB2	24910	53542	3.09%	0.331%
47	22.882	3334	3335	3337	rBV2	2965	1791	0.10%	0.011%
48	23.029	3354	3360	3368	rBV3	20978	42006	2.42%	0.260%
49	23.804	3487	3492	3498	rVB4	20279	39327	2.27%	0.243%
50	24.427	3586	3598	3610	rBV2	656606	1735090	100.00%	10.724%
51	24.633	3622	3633	3642	rBV	413077	1087580	62.68%	6.722%
52	24.715	3644	3647	3659	rVB4	26750	63222	3.64%	0.391%
53	25.291	3743	3745	3747	rBV3	2958	2326	0.13%	0.014%
54	25.808	3826	3833	3839	rVB2	21761	51271	2.95%	0.317%
55	27.106	4046	4054	4065	rVB5	22146	71701	4.13%	0.443%
56	27.546	4127	4129	4131	rBV3	2874	2584	0.15%	0.016%
57	28.674	4313	4321	4322	rBV4	14720	26411	1.52%	0.163%
58	28.903	4358	4360	4362	rBV3	2283	2041	0.12%	0.013%
59	29.491	4458	4460	4461	rBV2	2444	1764	0.10%	0.011%
60	31.335	4772	4774	4777	rBV3	3073	2594	0.15%	0.016%




Sum of corrected areas: 16178890

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
Data File : BG062379.D
Acq On : 13 Aug 2024 10:46
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

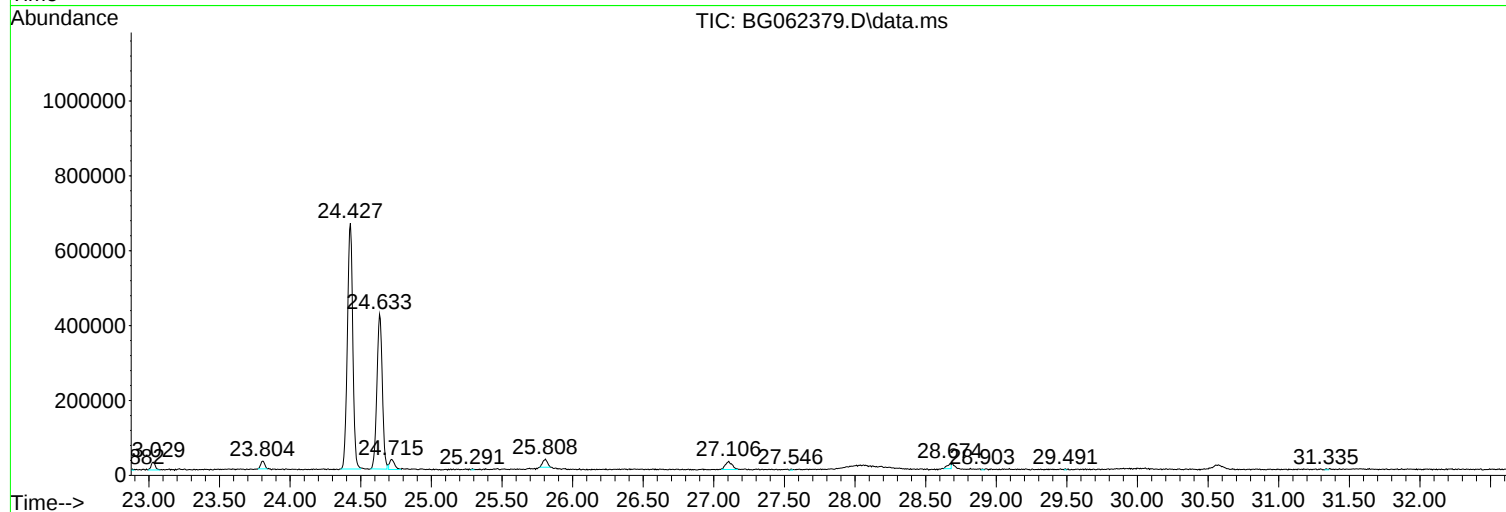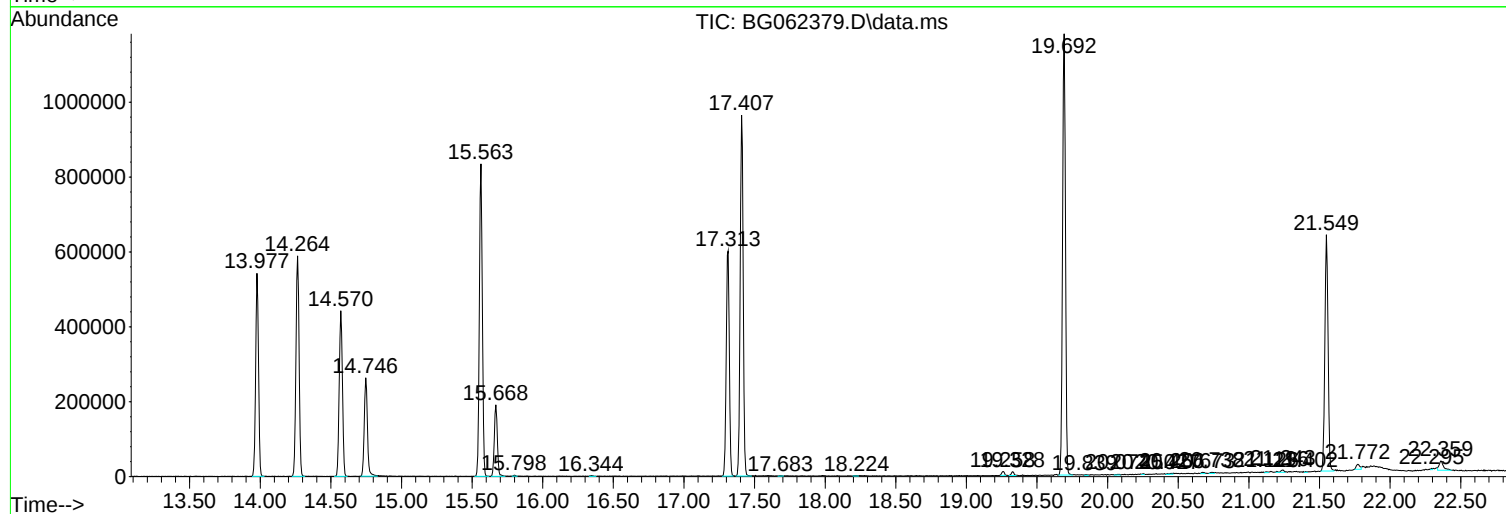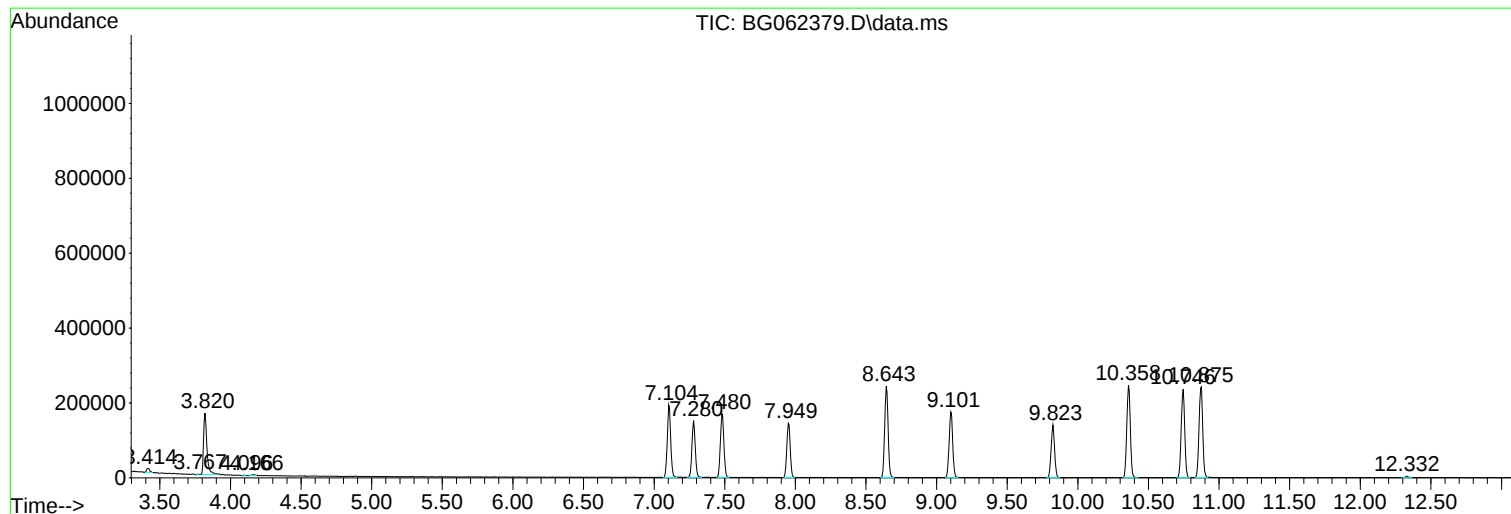

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
Data File : BG062379.D
Acq On : 13 Aug 2024 10:46
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081324\
Data File : BG062379.D
Acq On : 13 Aug 2024 10:46
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc